

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070523\
 Data File : BG058051.D
 Acq On : 6 Jul 2023 15:39
 Operator : CG/JU
 Sample : 03257-19
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EXYW6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG058051.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.361	43	46	50	rBV2	11585	13709	0.54%	0.072%
2	3.772	111	116	125	rBV	77479	130588	5.19%	0.685%
3	4.007	152	156	160	rVB3	5098	7548	0.30%	0.040%
4	4.101	170	172	177	rVB4	3021	4584	0.18%	0.024%
5	7.086	674	680	689	rBV2	48954	85705	3.41%	0.450%
6	7.245	700	707	717	rBV	215335	359146	14.27%	1.884%
7	7.450	733	742	754	rBV	186067	316391	12.57%	1.659%
8	7.920	813	822	830	rBV	181039	305427	12.14%	1.602%
9	8.625	934	942	952	rBV2	147908	265635	10.55%	1.393%
10	9.078	1012	1019	1035	rBV	254778	461803	18.35%	2.422%
11	9.801	1135	1142	1153	rBV	197202	347054	13.79%	1.820%
12	10.341	1226	1234	1246	rBV	266430	489875	19.46%	2.569%
13	10.723	1290	1299	1306	rBV	266616	471549	18.74%	2.473%
14	10.858	1314	1322	1334	rBV	284544	526217	20.91%	2.760%
15	12.315	1564	1570	1577	rVB3	4283	7596	0.30%	0.040%
16	13.443	1757	1762	1767	rBV2	8576	13839	0.55%	0.073%
17	13.960	1843	1850	1861	rBV	671622	996427	39.59%	5.226%
18	14.248	1892	1899	1916	rBV	704311	1137018	45.18%	5.964%
19	14.554	1945	1951	1962	rBV	434342	708600	28.15%	3.717%
20	14.759	1980	1986	1996	rBV2	47405	91891	3.65%	0.482%
21	15.341	2080	2085	2090	rBV2	4582	6685	0.27%	0.035%
22	15.547	2113	2120	2134	rBV	1007461	1546321	61.44%	8.111%
23	15.664	2134	2140	2157	rVV	356957	533129	21.18%	2.796%
24	15.788	2157	2161	2164	rVB3	3728	4774	0.19%	0.025%
25	15.911	2175	2182	2186	rBV	14289	22742	0.90%	0.119%
26	17.298	2412	2418	2428	rBV	613145	951950	37.82%	4.993%
27	17.403	2429	2436	2453	rVB	1177491	1860526	73.92%	9.759%
28	18.155	2559	2564	2565	rBV3	6293	6775	0.27%	0.036%
29	18.185	2565	2569	2576	rVV2	20046	33118	1.32%	0.174%
30	18.255	2579	2581	2585	rVB3	3404	3995	0.16%	0.021%
31	19.037	2710	2714	2716	rBV5	3810	4349	0.17%	0.023%
32	19.084	2716	2722	2739	rVV5	18105	69480	2.76%	0.364%
33	19.254	2746	2751	2756	rVB2	18540	27099	1.08%	0.142%
34	19.325	2758	2763	2768	rBV	16184	24446	0.97%	0.128%
35	19.460	2782	2786	2791	rBV4	5378	10004	0.40%	0.052%
36	19.607	2807	2811	2816	rBV5	3211	4863	0.19%	0.026%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070523\
Data File : BG058051.D
Acq On : 6 Jul 2023 15:39
Operator : CG/JU
Sample : 03257-19
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EXYW6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Title : SVOA CALIBRATION

37	19.689	2819	2825	2840	rVV	1561568	2292134	91.07%	12.022%
38	19.918	2860	2864	2867	rVB5	1882	2897	0.12%	0.015%
39	20.641	2985	2987	2989	rBV3	4245	4369	0.17%	0.023%
40	21.440	3119	3123	3126	rVB2	14117	16624	0.66%	0.087%
41	21.552	3136	3142	3155	rVB	606826	1021279	40.58%	5.357%
42	23.009	3387	3390	3396	rVB5	8954	15769	0.63%	0.083%
43	23.790	3519	3523	3532	rVB4	14778	32451	1.29%	0.170%
44	24.501	3632	3644	3655	rBV2	912716	2516893	100.00%	13.201%
45	24.713	3668	3680	3696	rBV	433637	1217585	48.38%	6.386%
46	25.817	3862	3868	3875	rVB4	16258	41909	1.67%	0.220%
47	27.139	4086	4093	4103	rVB4	16912	52829	2.10%	0.277%




Sum of corrected areas: 19065597

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070523\
Data File : BG058051.D
Acq On : 6 Jul 2023 15:39
Operator : CG/JU
Sample : 03257-19
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EXYW6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

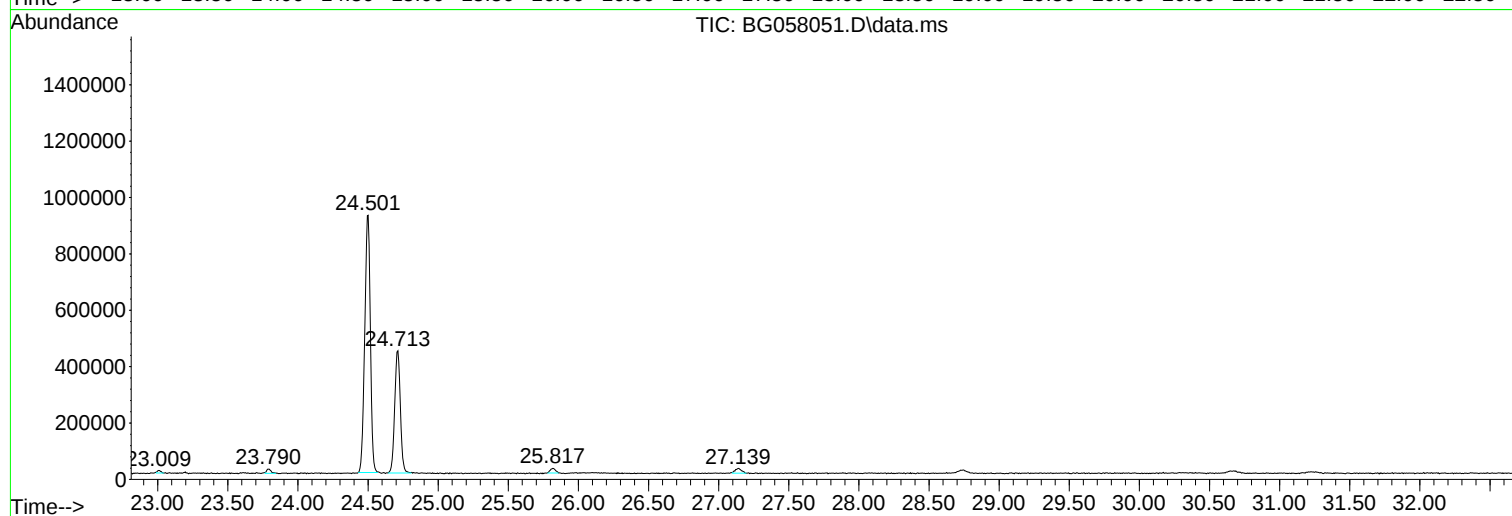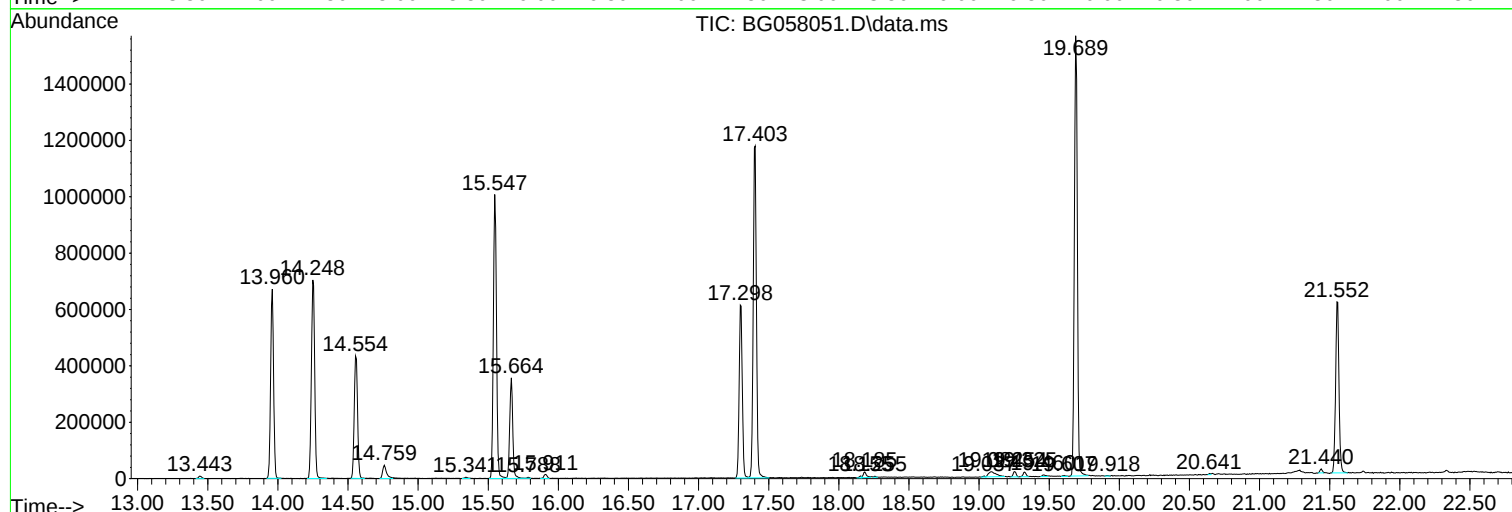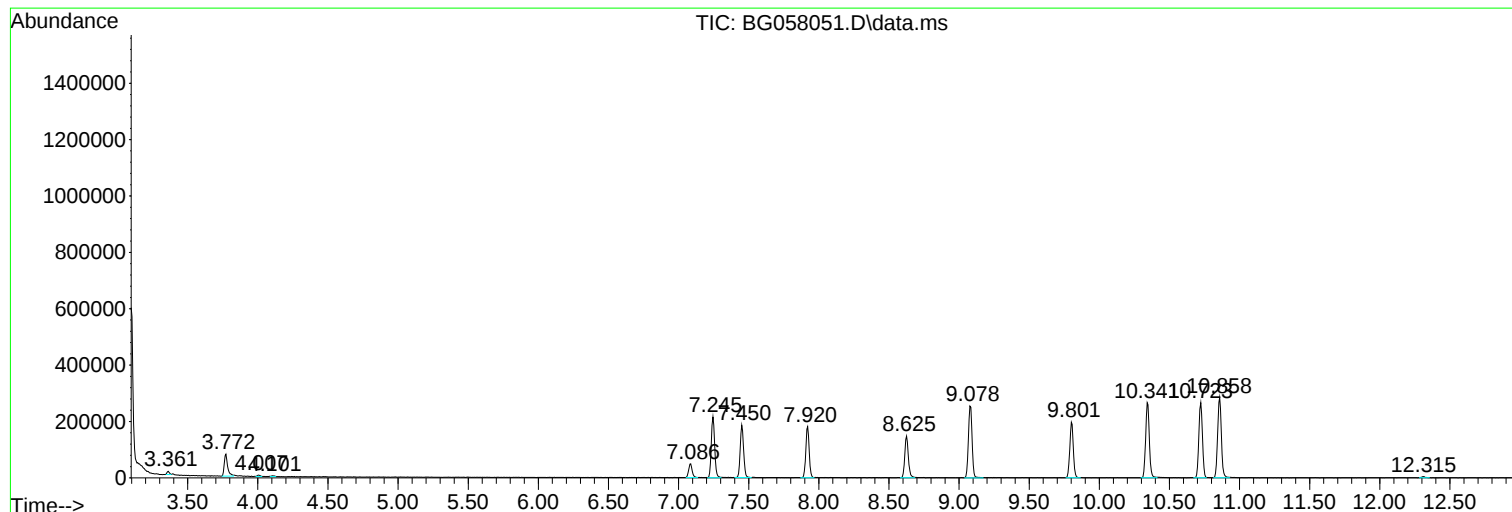

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070523\
Data File : BG058051.D
Acq On : 6 Jul 2023 15:39
Operator : CG/JU
Sample : 03257-19
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EXYW6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070523\
Data File : BG058051.D
Acq On : 6 Jul 2023 15:39
Operator : CG/JU
Sample : 03257-19
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EXYW6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc