

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070523\
 Data File : BG058060.D
 Acq On : 7 Jul 2023 00:09
 Operator : CG/JU
 Sample : PB153639BL
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK639

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG058060.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.164	11	13	17	rVB4	2275	2490	0.15%	0.017%
2	3.357	42	46	55	rVB	13540	22756	1.39%	0.159%
3	3.763	110	115	131	rBV	182243	288616	17.57%	2.019%
4	4.110	170	174	179	rVB6	2159	4004	0.24%	0.028%
5	4.909	308	310	314	rVB3	1677	1708	0.10%	0.012%
6	7.083	673	680	691	rBV	167891	291096	17.72%	2.036%
7	7.241	701	707	716	rBV	143413	233752	14.23%	1.635%
8	7.447	736	742	750	rBV	172600	282712	17.21%	1.978%
9	7.917	814	822	829	rBV	130059	213902	13.02%	1.496%
10	8.622	934	942	958	rBV	212117	377487	22.99%	2.641%
11	9.080	1012	1020	1028	rBV	172361	306727	18.68%	2.146%
12	9.797	1135	1142	1153	rBV	136314	245306	14.94%	1.716%
13	10.343	1227	1235	1247	rBV	203255	363943	22.16%	2.546%
14	10.719	1292	1299	1312	rVB	196899	343339	20.91%	2.402%
15	10.855	1314	1322	1334	rBV	226640	415877	25.32%	2.909%
16	12.306	1565	1569	1578	rBV2	2846	5063	0.31%	0.035%
17	13.440	1757	1762	1768	rBV2	4153	7046	0.43%	0.049%
18	13.957	1843	1850	1859	rBV	475851	692201	42.15%	4.842%
19	14.251	1892	1900	1911	rBV	489344	781972	47.61%	5.470%
20	14.556	1944	1952	1959	rBV	327989	527867	32.14%	3.693%
21	14.756	1980	1986	2001	rBV	173036	334707	20.38%	2.341%
22	15.543	2114	2120	2134	rVV	672775	1038485	63.23%	7.264%
23	15.661	2134	2140	2152	rVB	231037	338162	20.59%	2.366%
24	15.778	2157	2160	2164	rVB5	1941	2822	0.17%	0.020%
25	17.300	2412	2419	2429	rBV	505200	755046	45.97%	5.282%
26	17.400	2429	2436	2449	rVB	815696	1245899	75.86%	8.715%
27	17.682	2480	2484	2487	rVB3	1374	1955	0.12%	0.014%
28	18.358	2594	2599	2604	rVV4	1103	2112	0.13%	0.015%
29	19.251	2747	2751	2755	rVB2	11700	15640	0.95%	0.109%
30	19.321	2759	2763	2772	rVV	9350	14498	0.88%	0.101%
31	19.403	2772	2777	2780	rVV3	875	1819	0.11%	0.013%
32	19.562	2800	2804	2805	rBV2	1506	1890	0.12%	0.013%
33	19.685	2818	2825	2838	rBV	1082885	1548141	94.27%	10.830%
34	20.050	2886	2887	2890	rBV3	2164	1709	0.10%	0.012%
35	20.091	2890	2894	2897	rVV5	1428	2491	0.15%	0.017%
36	20.414	2948	2949	2951	rBV2	1943	1813	0.11%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070523\
 Data File : BG058060.D
 Acq On : 7 Jul 2023 00:09
 Operator : CG/JU
 Sample : PB153639BL
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK639

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Title : SVOA CALIBRATION

37	20.643	2986	2988	2989	rBV	2571	1874	0.11%	0.013%
38	20.702	2996	2998	2999	rBV2	2396	1654	0.10%	0.012%
39	21.554	3136	3143	3155	rBV	494783	830971	50.60%	5.813%
40	21.936	3206	3208	3209	rVB2	3579	1968	0.12%	0.014%
41	21.953	3209	3211	3213	rBV3	3031	3820	0.23%	0.027%
42	22.323	3272	3274	3277	rBV3	4808	6243	0.38%	0.044%
43	23.005	3387	3390	3396	rVB7	10043	16896	1.03%	0.118%
44	23.052	3396	3398	3400	rBV3	2708	2518	0.15%	0.018%
45	23.305	3439	3441	3443	rBV3	2977	2804	0.17%	0.020%
46	23.781	3519	3522	3530	rVB6	11097	21804	1.33%	0.153%
47	24.486	3632	3642	3656	rBV2	586232	1642305	100.00%	11.488%
48	24.703	3669	3679	3697	rVB	336357	978940	59.61%	6.848%
49	25.808	3861	3867	3876	rVB5	13480	35824	2.18%	0.251%
50	28.710	4352	4361	4363	rBV8	11483	23160	1.41%	0.162%
51	30.626	4685	4687	4688	rBV2	4002	3446	0.21%	0.024%
52	32.118	4939	4941	4945	rBV4	2831	4094	0.25%	0.029%
53	32.235	4959	4961	4962	rBV2	2826	2100	0.13%	0.015%




Sum of corrected areas: 14295474

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070523\
Data File : BG058060.D
Acq On : 7 Jul 2023 00:09
Operator : CG/JU
Sample : PB153639BL
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK639

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

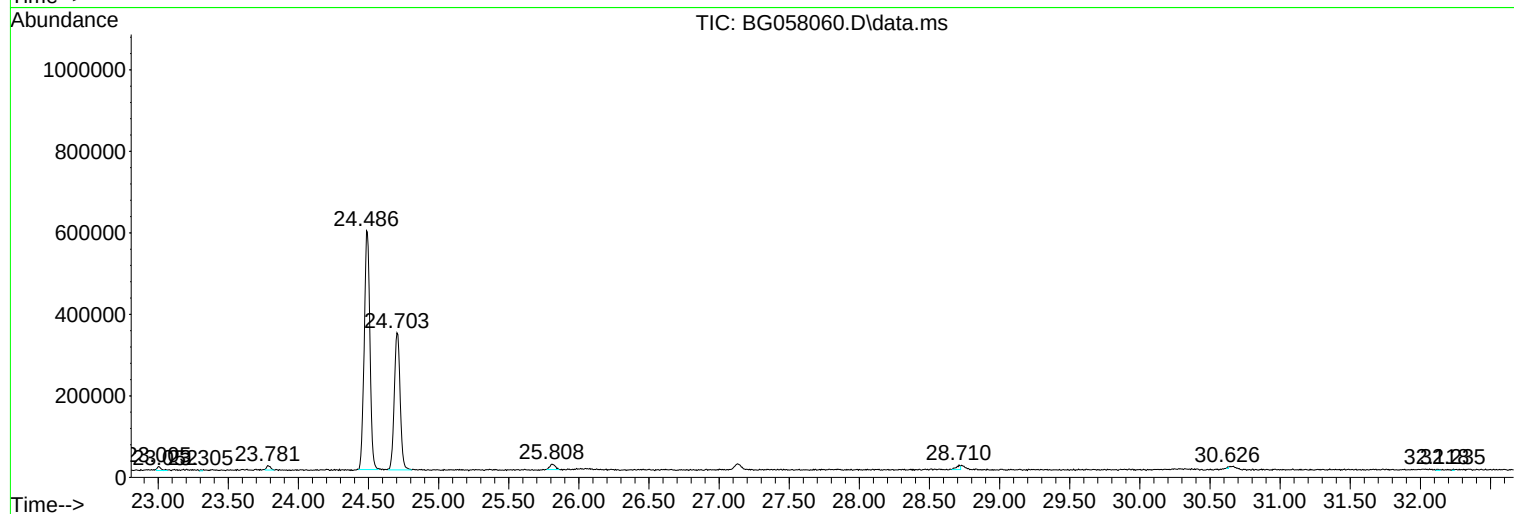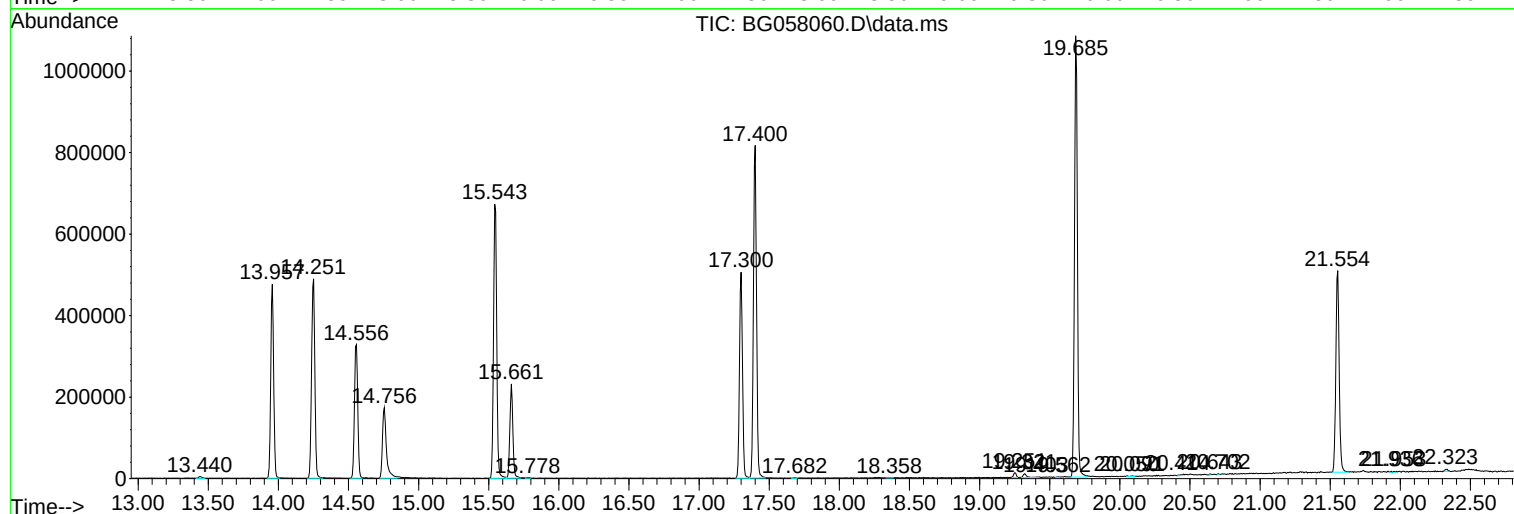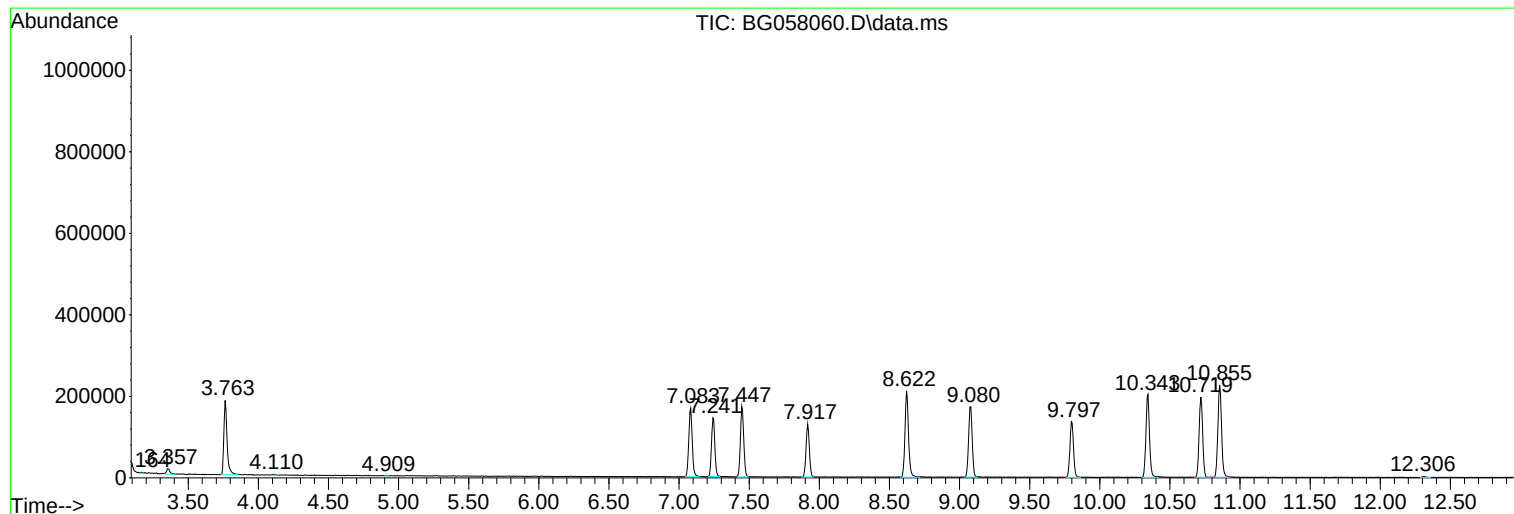

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070523\
Data File : BG058060.D
Acq On : 7 Jul 2023 00:09
Operator : CG/JU
Sample : PB153639BL
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK639

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070523\
Data File : BG058060.D
Acq On : 7 Jul 2023 00:09
Operator : CG/JU
Sample : PB153639BL
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK639

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------