

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070523\
 Data File : BG058075.D
 Acq On : 7 Jul 2023 14:49
 Operator : CG/JU
 Sample : 03284-09
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DCGZ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG058075.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.358	43	46	50	rVB	9605	11711	0.56%	0.077%
2	3.770	112	116	125	rBV	57530	96435	4.58%	0.634%
3	4.011	152	157	162	rVB3	3654	6111	0.29%	0.040%
4	4.105	169	173	174	rBV3	3447	3226	0.15%	0.021%
5	7.083	672	680	690	rBV	47425	81036	3.85%	0.533%
6	7.242	700	707	719	rBV	169073	281518	13.38%	1.851%
7	7.448	736	742	751	rBV	155424	263971	12.55%	1.735%
8	7.918	816	822	831	rVB	118208	199502	9.48%	1.312%
9	8.623	935	942	952	rBV	130088	230248	10.95%	1.514%
10	9.081	1012	1020	1028	rBV	200096	352888	16.78%	2.320%
11	9.804	1132	1143	1151	rBV	150991	275883	13.12%	1.814%
12	10.344	1226	1235	1247	rBV	211353	386547	18.38%	2.541%
13	10.720	1290	1299	1308	rBV	174827	312066	14.84%	2.052%
14	10.856	1315	1322	1337	rBV	215366	392697	18.67%	2.582%
15	12.307	1565	1569	1575	rVB3	3233	5782	0.27%	0.038%
16	13.447	1757	1763	1769	rBV4	2077	4198	0.20%	0.028%
17	13.958	1844	1850	1859	rBV	557025	791480	37.63%	5.203%
18	14.252	1891	1900	1916	rBV	554338	898655	42.72%	5.908%
19	14.557	1945	1952	1959	rBV	297644	463060	22.01%	3.044%
20	14.757	1980	1986	1997	rBV2	42176	87671	4.17%	0.576%
21	14.863	2001	2004	2010	rVB5	3381	6098	0.29%	0.040%
22	15.286	2071	2076	2082	rVB	32084	44819	2.13%	0.295%
23	15.550	2114	2121	2130	rBV	769013	1214470	57.74%	7.984%
24	15.662	2134	2140	2150	rVB	287264	414185	19.69%	2.723%
25	15.785	2157	2161	2167	rVB5	3552	5788	0.28%	0.038%
26	15.908	2176	2182	2187	rBV	27082	38089	1.81%	0.250%
27	16.655	2304	2309	2313	rBV3	1319	2424	0.12%	0.016%
28	16.784	2326	2331	2337	rVB	26684	34362	1.63%	0.226%
29	17.048	2372	2376	2381	rBV4	3321	4449	0.21%	0.029%
30	17.095	2381	2384	2388	rVB4	1679	2177	0.10%	0.014%
31	17.213	2398	2404	2406	rVB4	1675	2242	0.11%	0.015%
32	17.301	2411	2419	2429	rBV	432287	663168	31.53%	4.360%
33	17.401	2429	2436	2455	rVB2	1010891	1549302	73.65%	10.185%
34	17.577	2462	2466	2471	rVB4	2521	3909	0.19%	0.026%
35	17.789	2497	2502	2505	rVB4	3832	5083	0.24%	0.033%
36	17.959	2526	2531	2535	rBV4	4263	5410	0.26%	0.036%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070523\
 Data File : BG058075.D
 Acq On : 7 Jul 2023 14:49
 Operator : CG/JU
 Sample : 03284-09
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DCGZ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Title : SVOA CALIBRATION

37	18.182	2562	2569	2575	rBV5	11300	18746	0.89%	0.123%
38	18.259	2578	2582	2590	rVB	9382	13095	0.62%	0.086%
39	18.476	2614	2619	2624	rBV6	2972	4531	0.22%	0.030%
40	18.682	2651	2654	2660	rBV3	1431	2403	0.11%	0.016%
41	19.111	2722	2727	2731	rBV4	3216	4125	0.20%	0.027%
42	19.146	2731	2733	2737	rVB3	1682	2428	0.12%	0.016%
43	19.187	2737	2740	2743	rBV4	1836	2158	0.10%	0.014%
44	19.257	2746	2752	2758	rBV2	15130	23675	1.13%	0.156%
45	19.322	2758	2763	2772	rBV	14233	24774	1.18%	0.163%
46	19.463	2785	2787	2788	rBV	2971	2200	0.10%	0.014%
47	19.598	2808	2810	2812	rBV3	2890	3460	0.16%	0.023%
48	19.692	2819	2826	2842	rBV	1318344	1981755	94.21%	13.028%
49	20.209	2912	2914	2919	rVB4	3145	4528	0.22%	0.030%
50	20.397	2944	2946	2949	rBV4	2373	2956	0.14%	0.019%
51	20.468	2956	2958	2959	rBV2	2945	2229	0.11%	0.015%
52	20.668	2989	2992	2995	rVB3	5253	5568	0.26%	0.037%
53	20.709	2995	2999	3002	rVB3	4262	6248	0.30%	0.041%
54	20.879	3026	3028	3031	rBV3	1819	2255	0.11%	0.015%
55	21.020	3049	3052	3057	rBV5	4078	4686	0.22%	0.031%
56	21.437	3119	3123	3127	rVB	16327	21758	1.03%	0.143%
57	21.555	3136	3143	3154	rVB	461443	771534	36.68%	5.072%
58	21.743	3171	3175	3179	rVB5	5188	7772	0.37%	0.051%
59	22.095	3234	3235	3237	rBV2	2904	2161	0.10%	0.014%
60	22.330	3272	3275	3279	rVB5	7712	9525	0.45%	0.063%
61	23.006	3386	3390	3397	rVB5	8682	15450	0.73%	0.102%
62	23.100	3403	3406	3412	rVB6	8692	13639	0.65%	0.090%
63	23.194	3417	3422	3425	rVB6	5166	8137	0.39%	0.053%
64	23.793	3519	3524	3530	rVB7	11933	24005	1.14%	0.158%
65	24.498	3632	3644	3659	rBV2	742723	2103484	100.00%	13.829%
66	24.710	3669	3680	3695	rBV	322970	901456	42.86%	5.926%
67	25.814	3860	3868	3880	rVB5	14346	45013	2.14%	0.296%
68	27.131	4082	4092	4093	rBV7	13055	24430	1.16%	0.161%
69	30.039	4585	4587	4590	rBV3	3224	2956	0.14%	0.019%
70	30.626	4685	4687	4688	rBV2	3791	3327	0.16%	0.022%
71	32.042	4925	4928	4929	rBV3	3722	3825	0.18%	0.025%


Sum of corrected areas: 15210952

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070523\
Data File : BG058075.D
Acq On : 7 Jul 2023 14:49
Operator : CG/JU
Sample : 03284-09
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCGZ6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

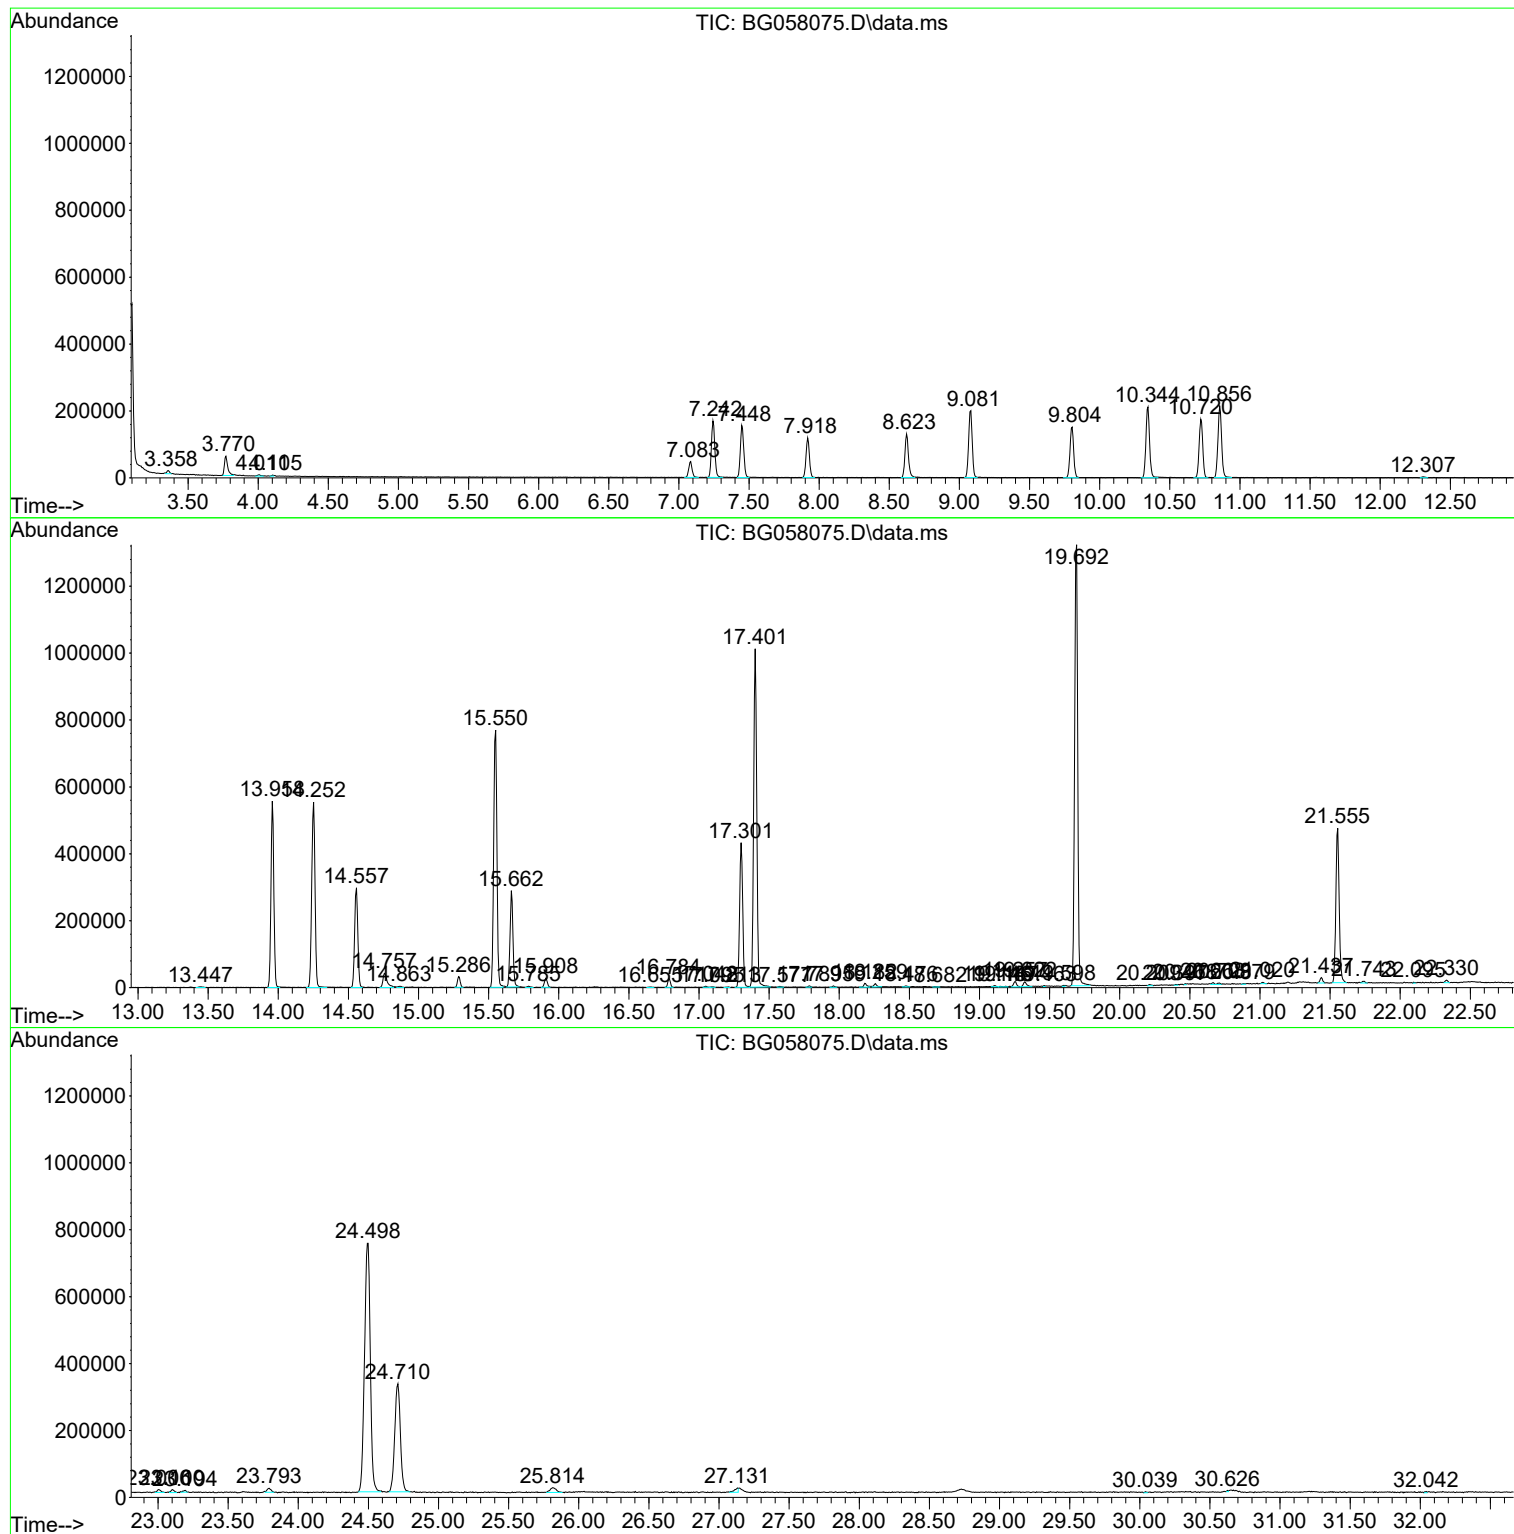

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070523\
Data File : BG058075.D
Acq On : 7 Jul 2023 14:49
Operator : CG/JU
Sample : 03284-09
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCGZ6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070523\
Data File : BG058075.D
Acq On : 7 Jul 2023 14:49
Operator : CG/JU
Sample : 03284-09
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCGZ6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc