

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070523\
 Data File : BG058079.D
 Acq On : 7 Jul 2023 17:37
 Operator : CG/JU
 Sample : 03284-04
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DCGZ1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG058079.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.361	42	46	51	rVB2	11456	17992	0.80%	0.115%
2	3.766	111	115	123	rBV	56407	88971	3.93%	0.568%
3	4.007	154	156	160	rVB2	4490	4587	0.20%	0.029%
4	4.107	169	173	177	rVB5	4296	5481	0.24%	0.035%
5	7.080	673	679	688	rBV	46369	76906	3.40%	0.491%
6	7.244	699	707	716	rBV	162657	268876	11.89%	1.716%
7	7.450	733	742	751	rVB	152684	255479	11.30%	1.630%
8	7.914	815	821	830	rVB	125053	209086	9.24%	1.334%
9	8.619	935	941	954	rBV	124608	224391	9.92%	1.432%
10	9.078	1009	1019	1030	rBV	199672	348756	15.42%	2.225%
11	9.242	1042	1047	1051	rVB4	3979	6153	0.27%	0.039%
12	9.800	1135	1142	1149	rBV	151638	264064	11.68%	1.685%
13	10.341	1225	1234	1249	rBV	206558	372653	16.48%	2.378%
14	10.723	1289	1299	1311	rVB	191411	338811	14.98%	2.162%
15	10.858	1315	1322	1334	rBV	212394	387606	17.14%	2.473%
16	11.516	1430	1434	1438	rBV4	1772	2959	0.13%	0.019%
17	12.309	1563	1569	1575	rVB	2940	4807	0.21%	0.031%
18	13.437	1757	1761	1767	rBV2	2199	4037	0.18%	0.026%
19	13.954	1843	1849	1863	rBV	534431	774744	34.25%	4.943%
20	14.248	1892	1899	1909	rBV	556238	868602	38.40%	5.542%
21	14.554	1941	1951	1959	rBV	334734	508679	22.49%	3.246%
22	14.753	1979	1985	1999	rBV2	42825	90094	3.98%	0.575%
23	15.288	2073	2076	2080	rBV2	2224	3093	0.14%	0.020%
24	15.546	2113	2120	2127	rBV	830424	1213409	53.65%	7.742%
25	15.658	2134	2139	2151	rVB	281084	434473	19.21%	2.772%
26	15.787	2156	2161	2165	rVB4	2972	4253	0.19%	0.027%
27	15.899	2176	2180	2184	rBV3	1666	2287	0.10%	0.015%
28	17.297	2412	2418	2427	rBV	485899	723601	31.99%	4.617%
29	17.397	2427	2435	2445	rBV	1065218	1591655	70.37%	10.156%
30	17.955	2528	2530	2534	rBV3	1748	2348	0.10%	0.015%
31	18.185	2566	2569	2571	rBV3	1992	2542	0.11%	0.016%
32	18.255	2577	2581	2585	rVB	7526	7920	0.35%	0.051%
33	19.148	2729	2733	2737	rBV4	3071	4687	0.21%	0.030%
34	19.254	2745	2751	2756	rBV	15274	22038	0.97%	0.141%
35	19.324	2758	2763	2768	rVV2	12336	19022	0.84%	0.121%
36	19.612	2807	2812	2816	rVB3	3592	6130	0.27%	0.039%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070523\
 Data File : BG058079.D
 Acq On : 7 Jul 2023 17:37
 Operator : CG/JU
 Sample : 03284-04
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DCGZ1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Title : SVOA CALIBRATION

37	19.689	2818	2825	2839	rBV	1421234	2064115	91.26%	13.170%
38	20.212	2911	2914	2918	rBV3	2401	2991	0.13%	0.019%
39	20.593	2972	2979	2982	rBV2	14226	21929	0.97%	0.140%
40	20.705	2996	2998	3000	rVB3	2933	2313	0.10%	0.015%
41	20.911	3031	3033	3039	rBV5	2106	2941	0.13%	0.019%
42	21.022	3050	3052	3056	rVB5	4638	4333	0.19%	0.028%
43	21.434	3119	3122	3127	rVB3	12627	16958	0.75%	0.108%
44	21.551	3136	3142	3155	rBV2	518748	861031	38.07%	5.494%
45	21.733	3170	3173	3177	rVB4	4228	5922	0.26%	0.038%
46	22.327	3271	3274	3282	rVB8	6410	11053	0.49%	0.071%
47	22.985	3378	3386	3396	rBV5	23342	65174	2.88%	0.416%
48	23.590	3485	3489	3490	rBV4	3022	4138	0.18%	0.026%
49	23.784	3517	3522	3531	rVB6	13284	29567	1.31%	0.189%
50	24.495	3631	3643	3662	rBV2	803223	2261727	100.00%	14.431%
51	24.706	3668	3679	3695	rBV	357901	1009774	44.65%	6.443%
52	25.811	3861	3867	3878	rVB5	17757	47186	2.09%	0.301%
53	27.133	4082	4092	4102	rBV5	15944	53175	2.35%	0.339%
54	27.756	4196	4198	4202	rVB4	3108	3149	0.14%	0.020%
55	27.791	4202	4204	4206	rBV2	3270	2539	0.11%	0.016%
56	28.725	4358	4363	4374	rVB9	11493	41320	1.83%	0.264%




Sum of corrected areas: 15672527

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070523\
Data File : BG058079.D
Acq On : 7 Jul 2023 17:37
Operator : CG/JU
Sample : 03284-04
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCGZ1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

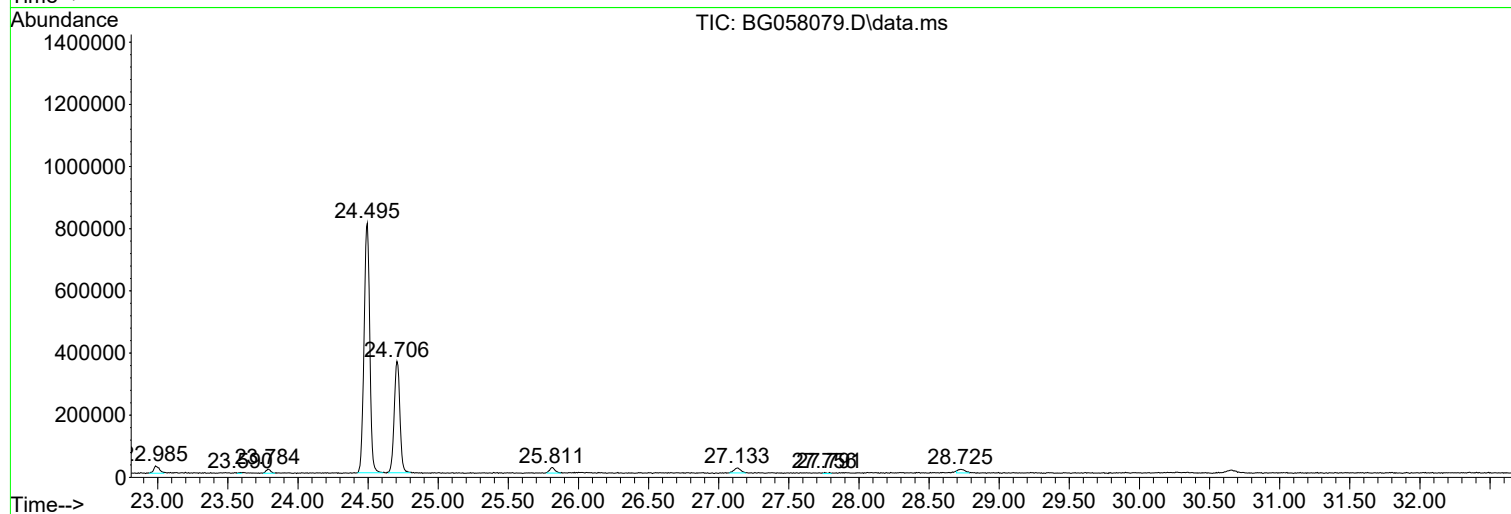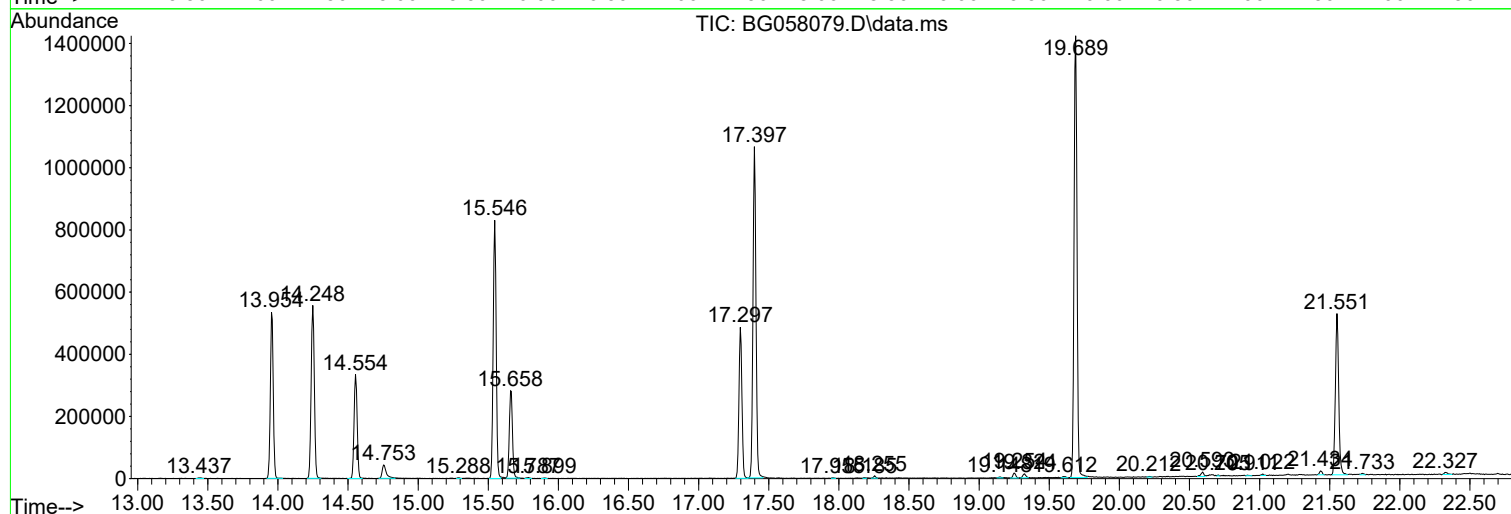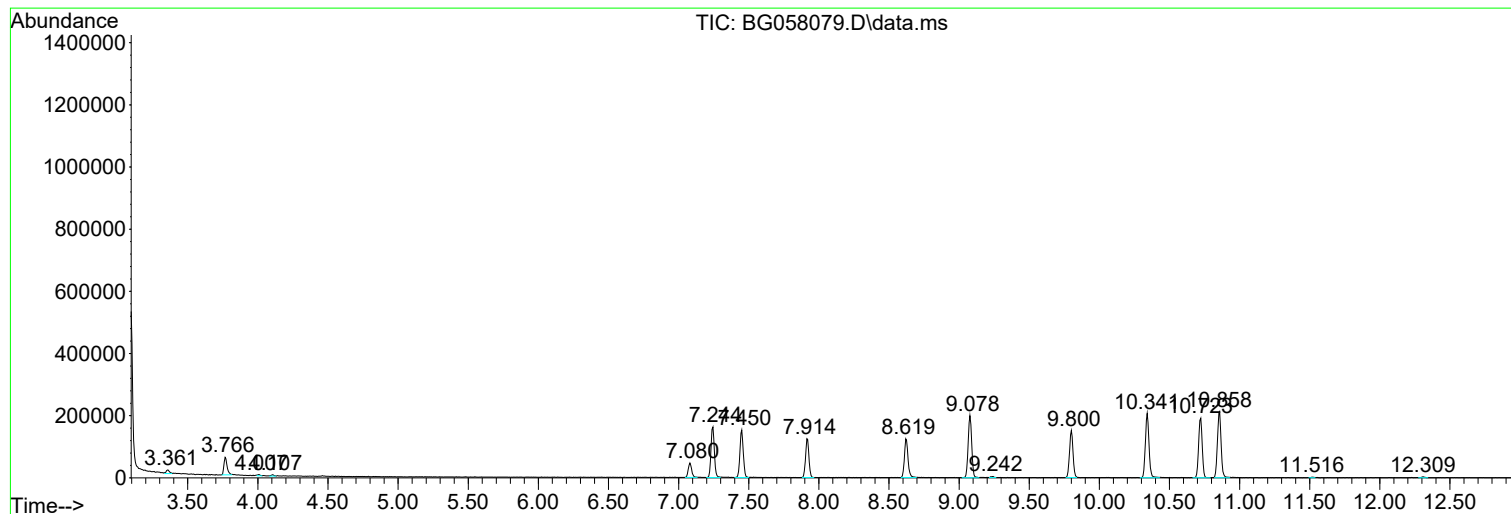

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070523\
Data File : BG058079.D
Acq On : 7 Jul 2023 17:37
Operator : CG/JU
Sample : 03284-04
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCGZ1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070523\
Data File : BG058079.D
Acq On : 7 Jul 2023 17:37
Operator : CG/JU
Sample : 03284-04
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCGZ1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc