
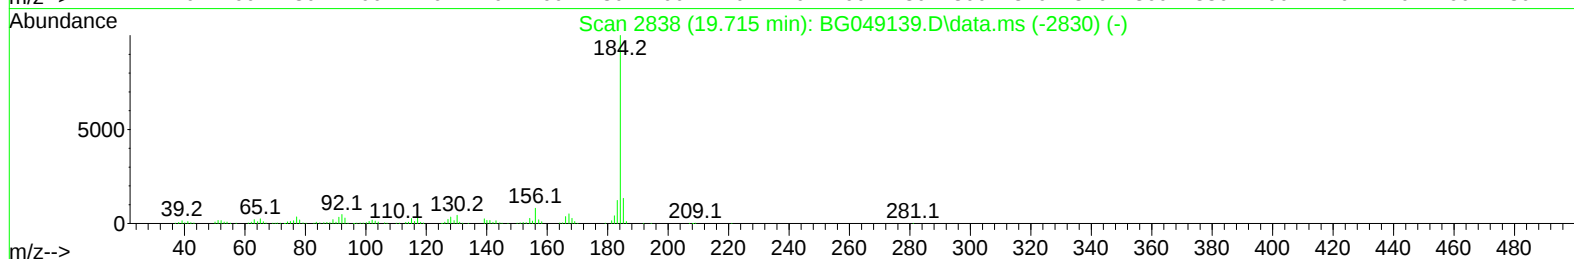
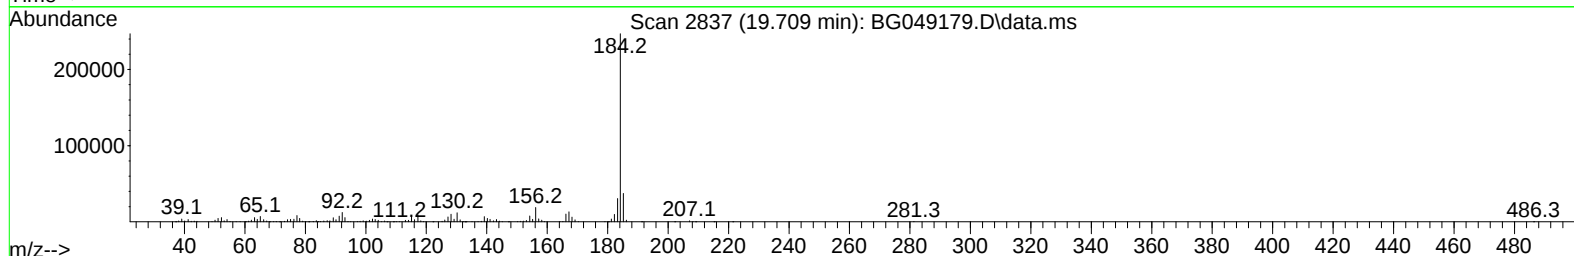


Quant Time: Jul 06 09:35:48 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG063021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 30 15:39:12 2021
Response via : Initial Calibration

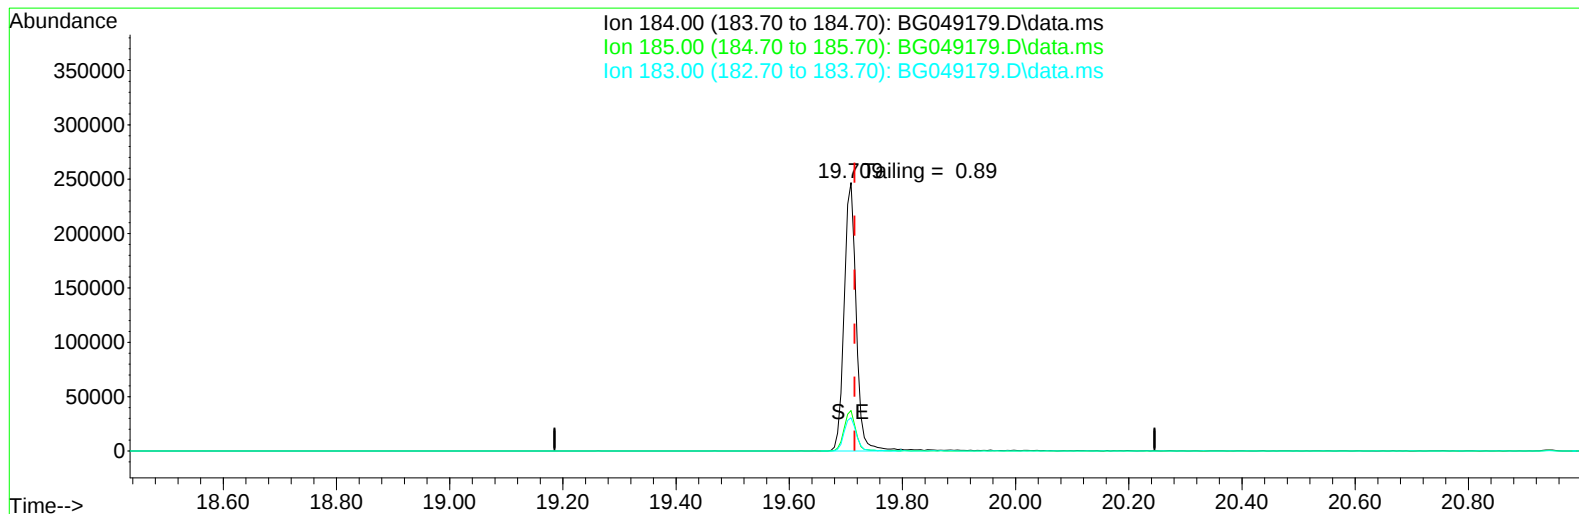

TIC: BG049179.D\data.ms

(77) Benzidine




19.709min (-0.006) 190704.10 ng

response **364568**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	15.10
183.00	11.70	12.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070621\
 Data File : BG049179.D
 Acq On : 6 Jul 2021 8:59
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 06 09:35:48 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG063021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 30 15:39:12 2021
 Response via : Initial Calibration

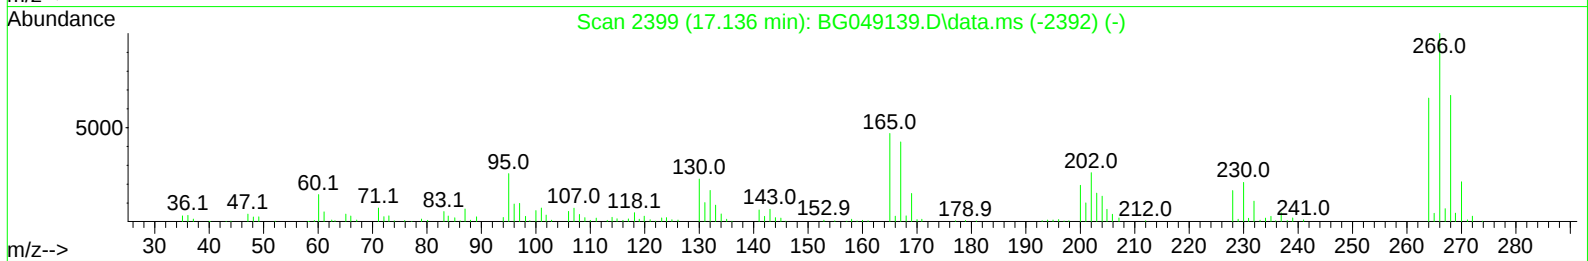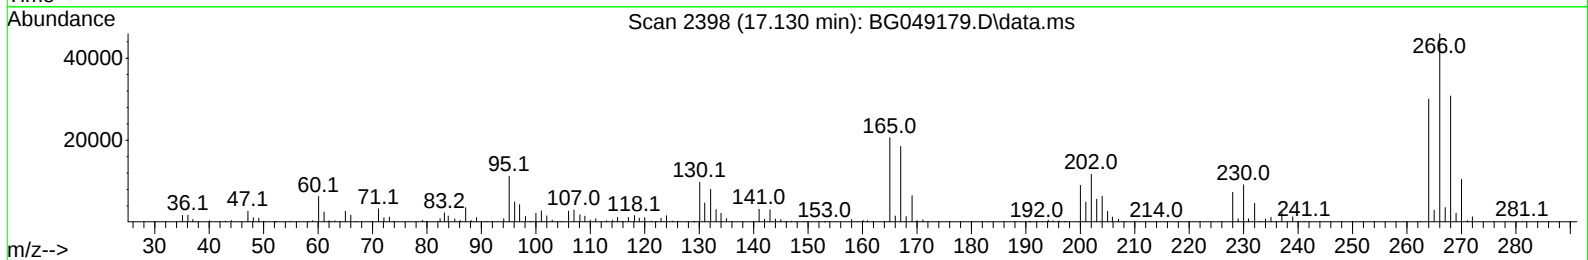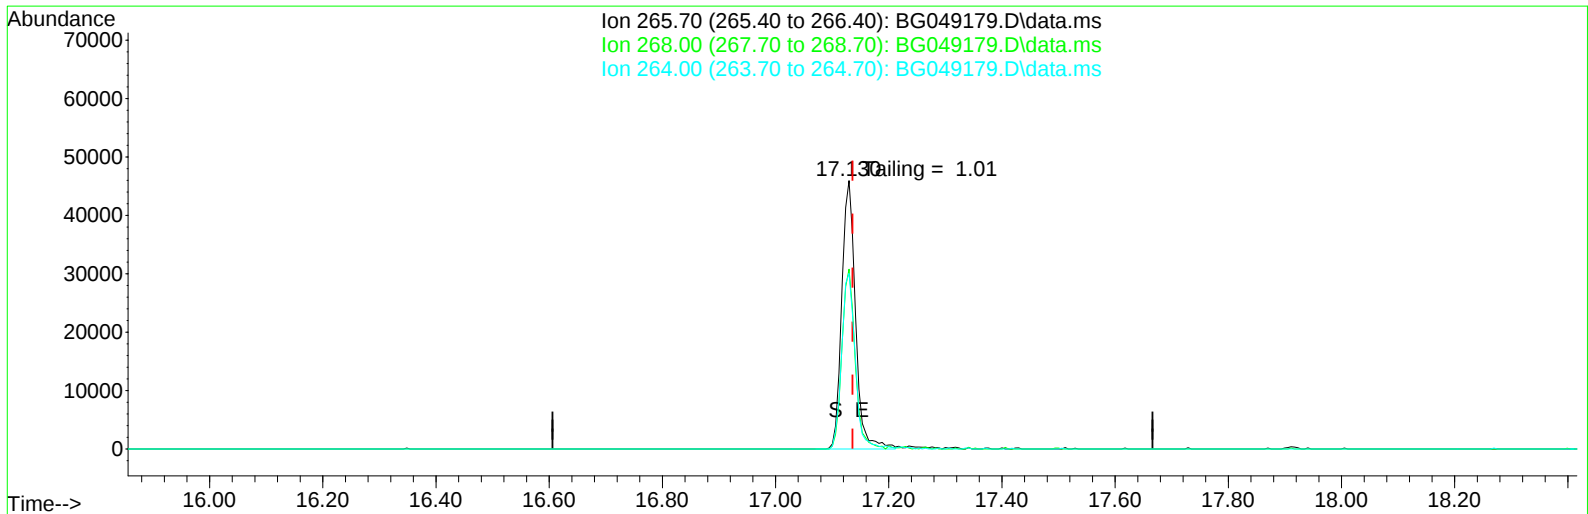

TIC: BG049179.D\data.ms

(70) Pentachlorophenol (C)

17.130min (-0.006) 18731.19 ng

response 77730

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	67.01
264.00	61.30	65.42
0.00	0.00	0.00