
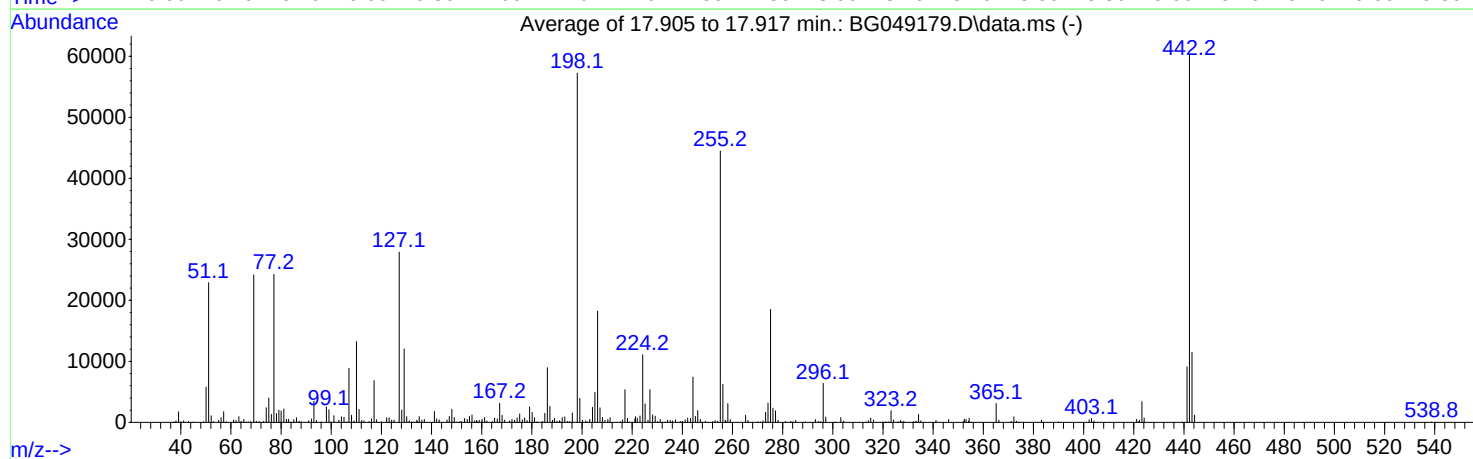


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070621\
 Data File : BG049179.D
 Acq On : 6 Jul 2021 8:59
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG063021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 06 10:59:02 2021

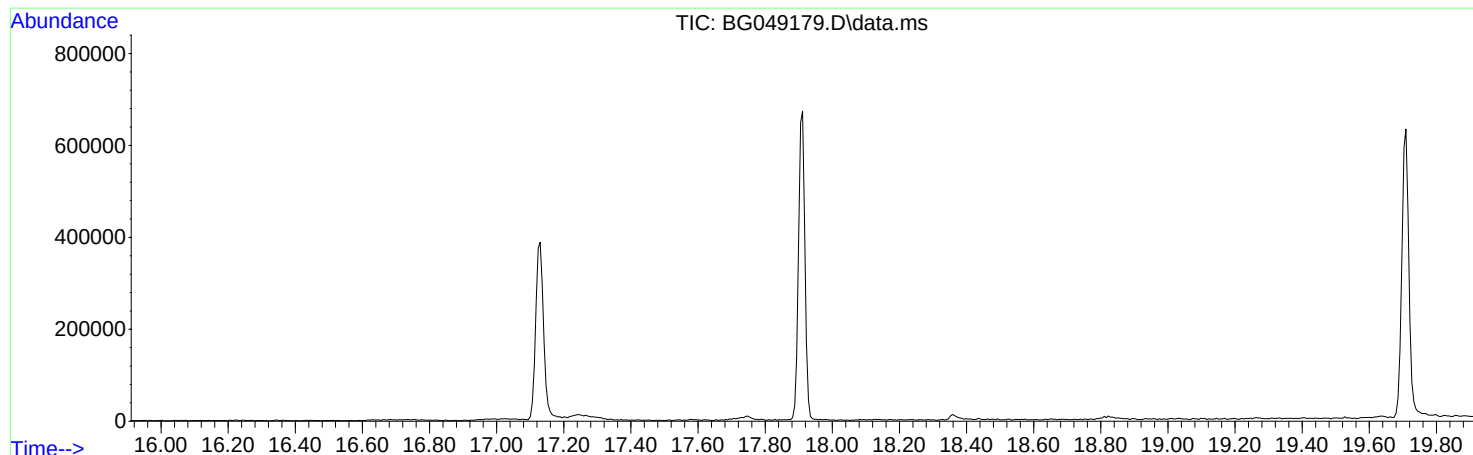




AutoFind: Scans 2530, 2531, 2532; Background Corrected with Scan 2523

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.0	22907	PASS
68	69	0.00	2	0.5	119	PASS
69	198	0.00	100	42.2	24174	PASS
70	69	0.00	2	0.6	156	PASS
127	198	10	80	48.7	27909	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	57259	PASS
199	198	5	9	6.9	3943	PASS
275	198	10	60	32.3	18515	PASS
365	198	1	100	5.4	3085	PASS
441	198	0.01	100	15.9	9096	PASS
442	442	100	100	100.0	60299	PASS
443	442	15	24	19.0	11464	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070621\
Data File : BG049179.D
Acq On : 6 Jul 2021 8:59
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jul 06 09:35:48 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG063021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 30 15:39:12 2021
Response via : Initial Calibration

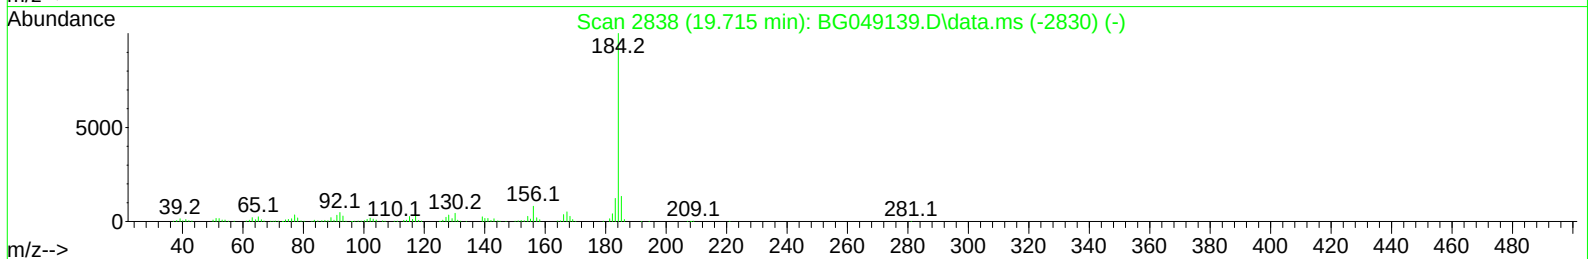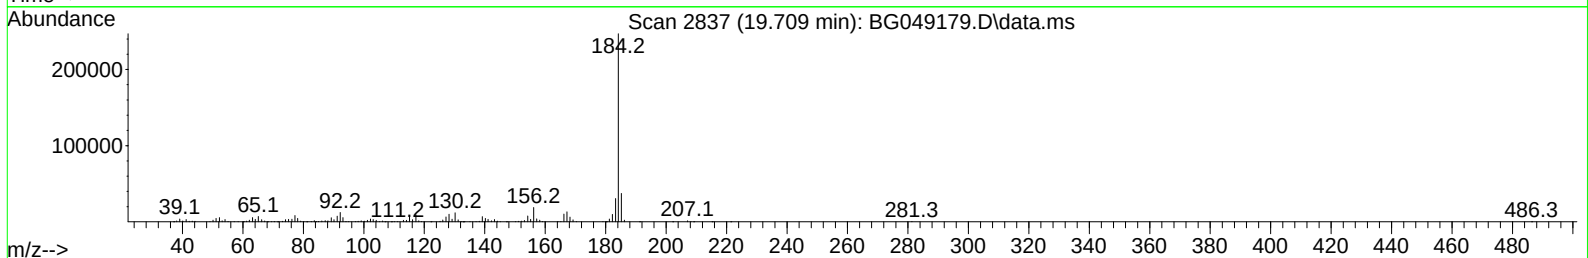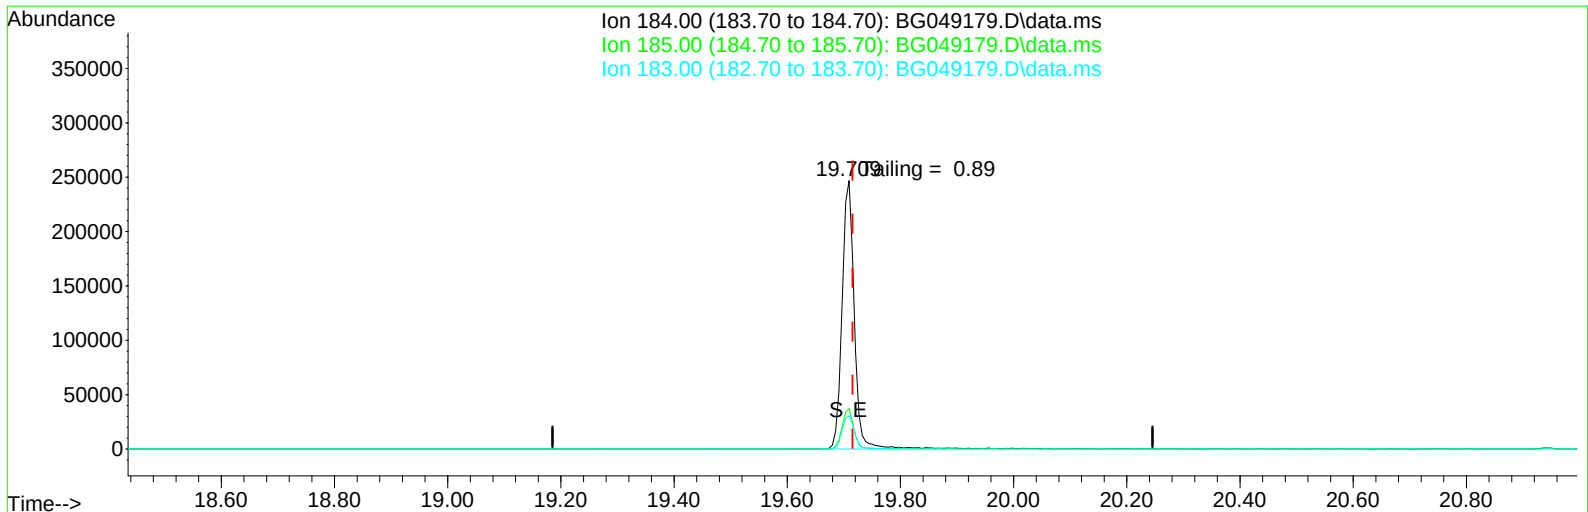

TIC: BG049179.D\data.ms

(77) Benzidine

19.709min (-0.006) 190704.10 ng




response 364568

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	15.10
183.00	11.70	12.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070621\
Data File : BG049179.D
Acq On : 6 Jul 2021 8:59
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jul 06 09:35:48 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG063021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 30 15:39:12 2021
Response via : Initial Calibration

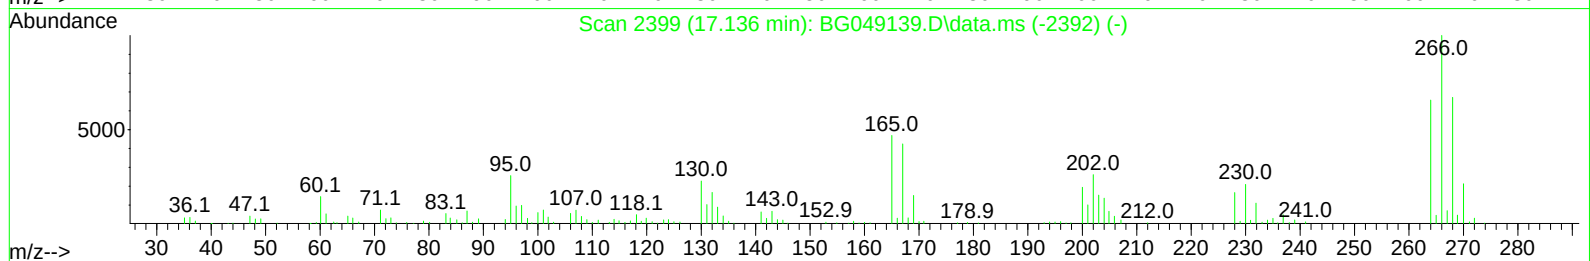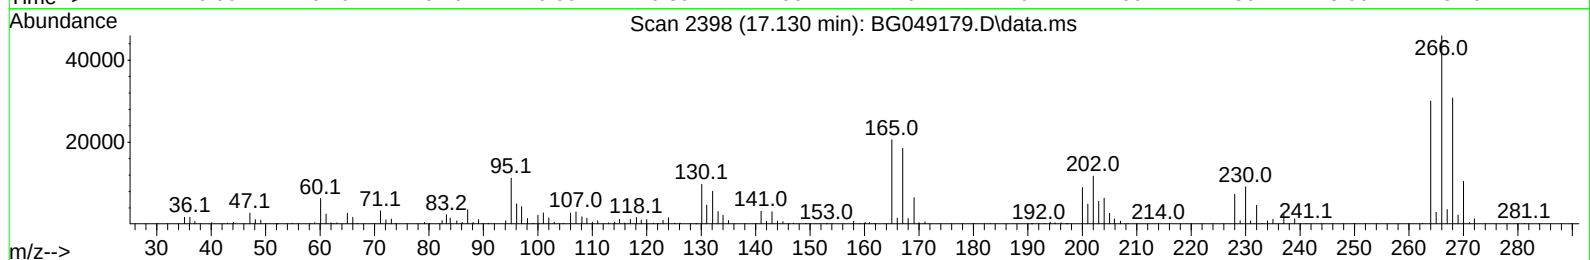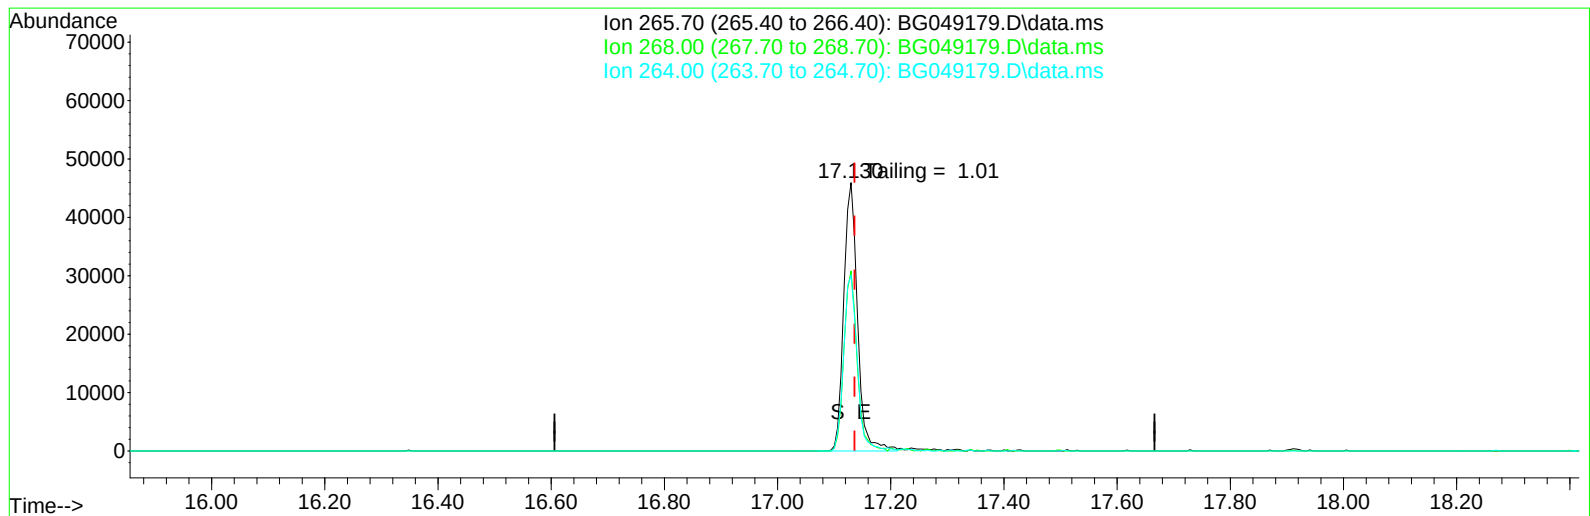

TIC: BG049179.D\data.ms

(70) Pentachlorophenol (C)

17.130min (-0.006) 18731.19 ng

response 77730

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	67.01
264.00	61.30	65.42
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/6/2021	BNA_G	BG049179.D
Compound Name	Response	Retention Time
DDT	192671	20.94
DDD	3975	20.49
DDE	971	19.99
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4946	197617	2.50

Instrument :
BNA_G
ClientSampleId :
DFTPP