

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070722\
 Data File : BG054222.D
 Acq On : 7 Jul 2022 12:39
 Operator : CG/JU
 Sample : PB146067BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB146067BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG054222.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.633	374	382	394	rBV	289140	492764	19.11%	5.863%
2	7.225	646	653	669	rBV	305636	548547	21.28%	6.526%
3	8.059	789	795	804	rVB	67690	121537	4.71%	1.446%
4	9.223	985	993	1003	rBV	182950	346297	13.43%	4.120%
5	10.874	1266	1274	1282	rBV	95581	178173	6.91%	2.120%
6	13.318	1682	1690	1706	rBV	653356	1062313	41.21%	12.639%
7	14.693	1917	1924	1934	rBB	192169	306461	11.89%	3.646%
8	16.179	2170	2177	2193	rBV3	663220	1092626	42.38%	12.999%
9	17.437	2384	2391	2404	rVB	309759	473963	18.39%	5.639%
10	20.045	2829	2835	2847	rVB	1921935	2577958	100.00%	30.671%
11	21.714	3112	3119	3131	rBV2	347186	600404	23.29%	7.143%
12	24.981	3663	3675	3694	rBV2	169880	604129	23.43%	7.188%




Sum of corrected areas: 8405172

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070722\
Data File : BG054222.D
Acq On : 7 Jul 2022 12:39
Operator : CG/JU
Sample : PB146067BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB146067BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

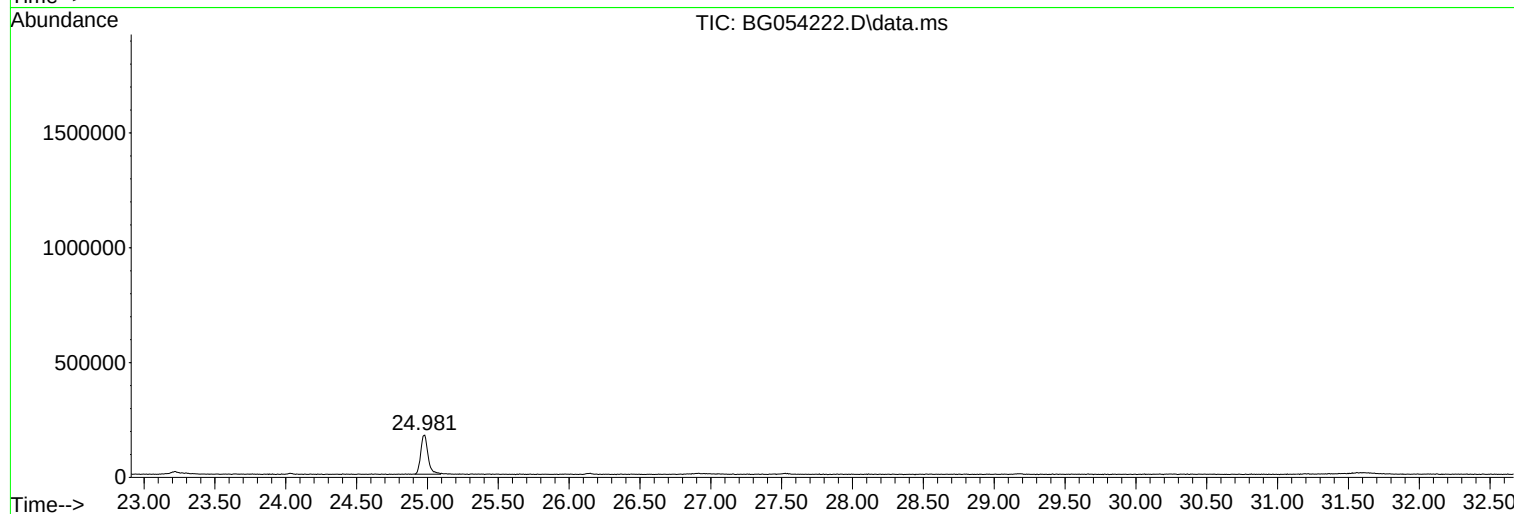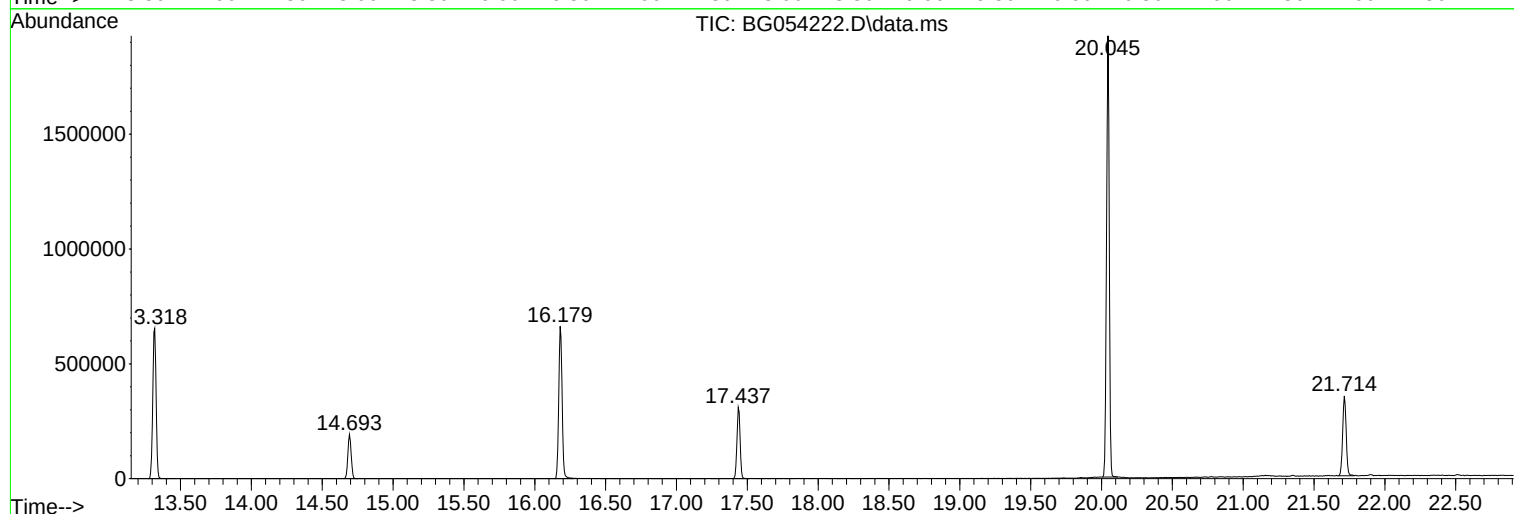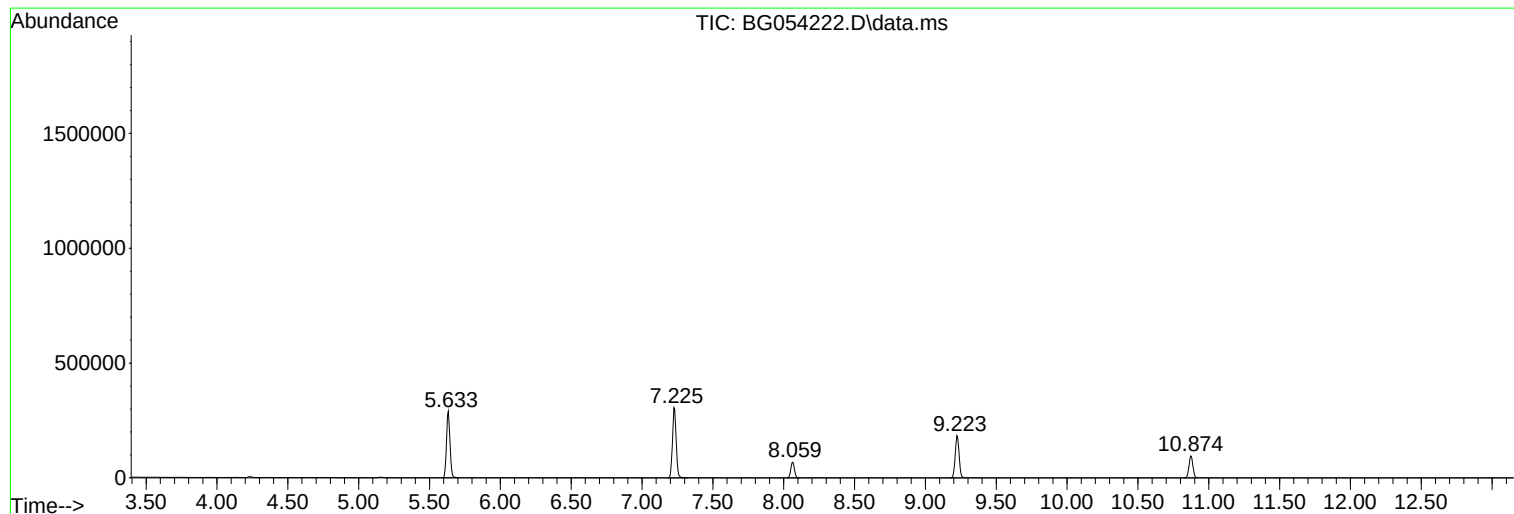

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070722\
Data File : BG054222.D
Acq On : 7 Jul 2022 12:39
Operator : CG/JU
Sample : PB146067BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB146067BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070722\
Data File : BG054222.D
Acq On : 7 Jul 2022 12:39
Operator : CG/JU
Sample : PB146067BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB146067BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------