


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070722\
 Data File : BG054220.D
 Acq On : 7 Jul 2022 10:50
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 08 13:46:14 2022

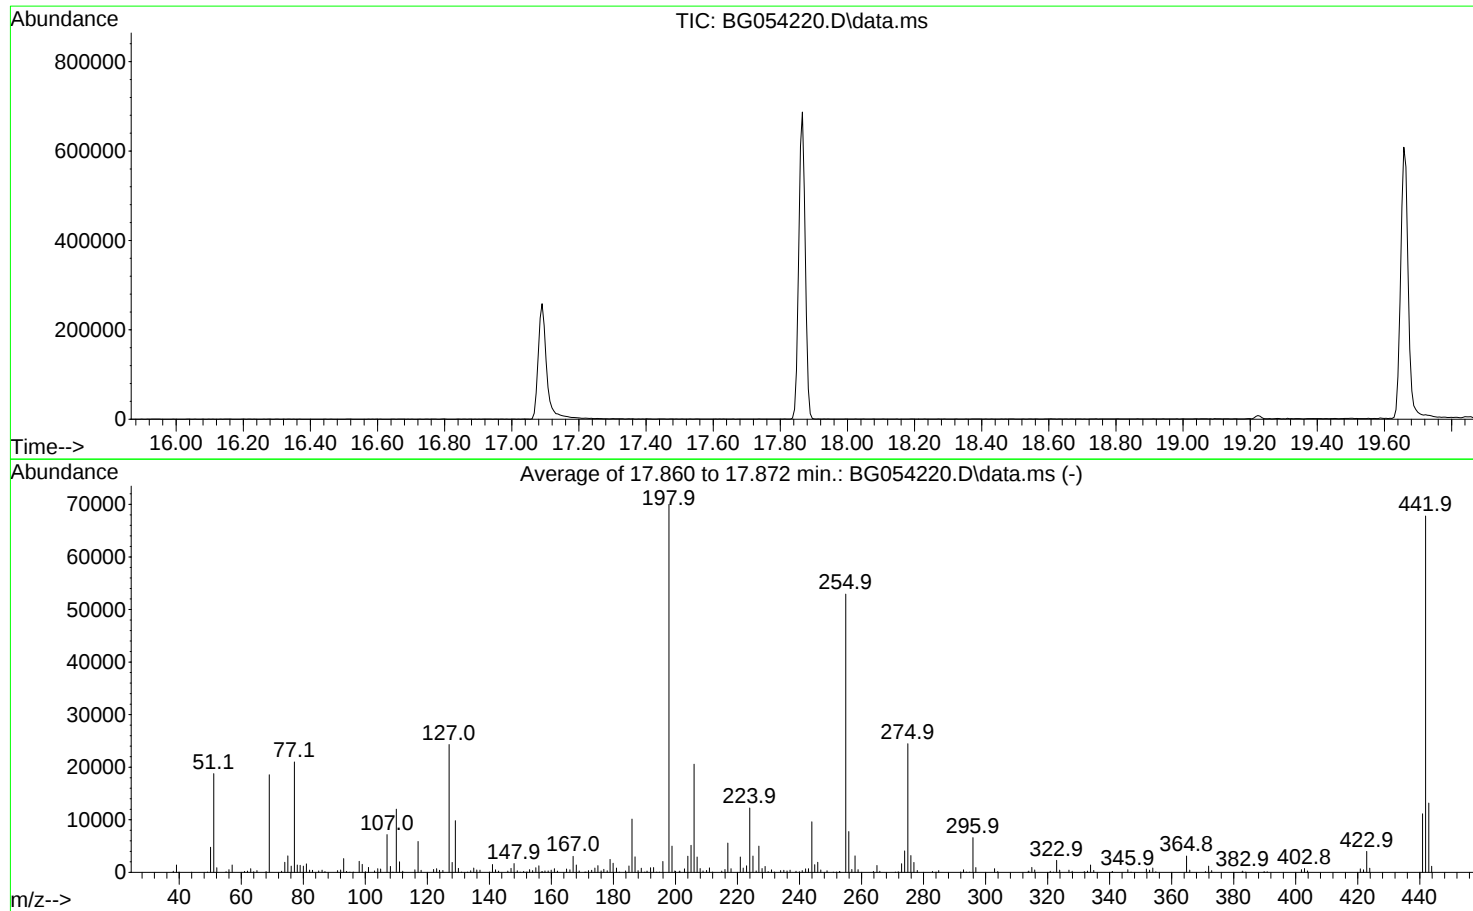




AutoFind: Scans 2463, 2464, 2465; Background Corrected with Scan 2456

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.8	18780	PASS
68	69	0.00	2	0.8	153	PASS
69	198	0.00	100	26.5	18559	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	34.8	24315	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	69971	PASS
199	198	5	9	7.1	4983	PASS
275	198	10	60	35.0	24483	PASS
365	198	1	100	4.5	3115	PASS
441	198	0.01	100	15.9	11147	PASS
442	442	50	100	100.0	67768	PASS
443	442	15	24	19.4	13165	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070722\
Data File : BG054220.D
Acq On : 7 Jul 2022 10:50
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jul 07 13:41:10 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 27 00:27:54 2022
Response via : Initial Calibration

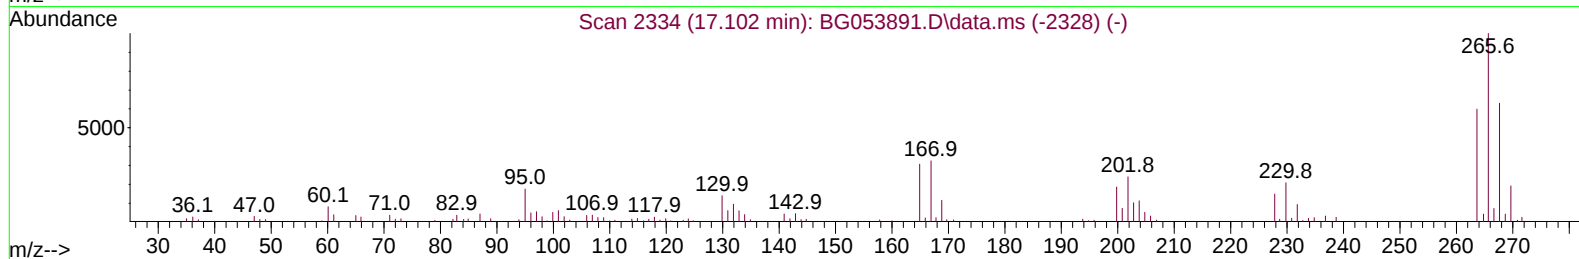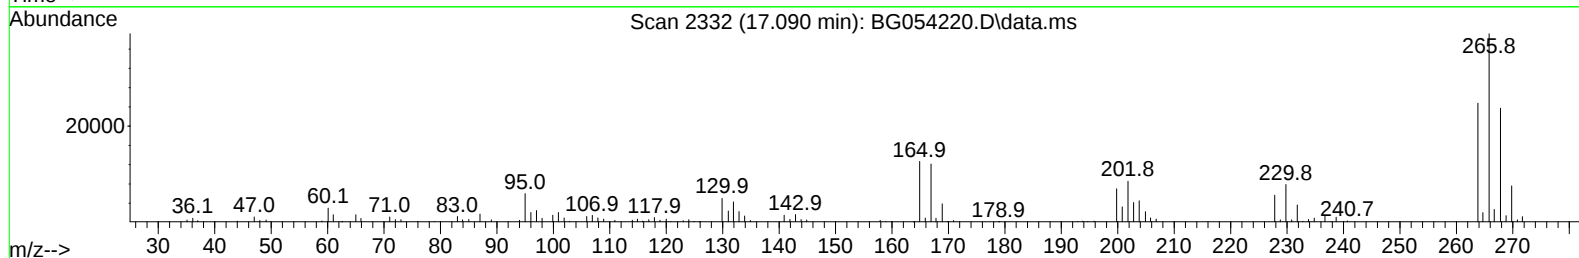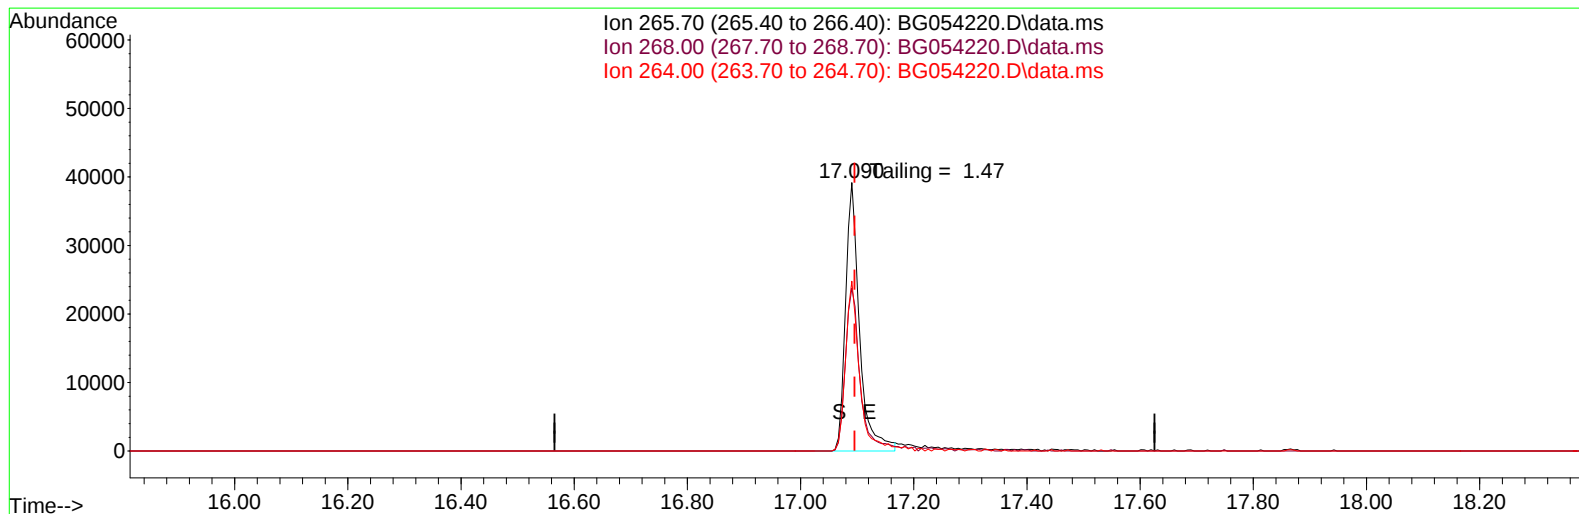

TIC: BG054220.D\data.ms

(70) Pentachlorophenol (C)

17.090min (-0.005) 28483.77 ng




response 69563

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	60.61
264.00	66.20	68.48
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070722\
Data File : BG054220.D
Acq On : 7 Jul 2022 10:50
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jul 07 13:41:10 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 27 00:27:54 2022
Response via : Initial Calibration

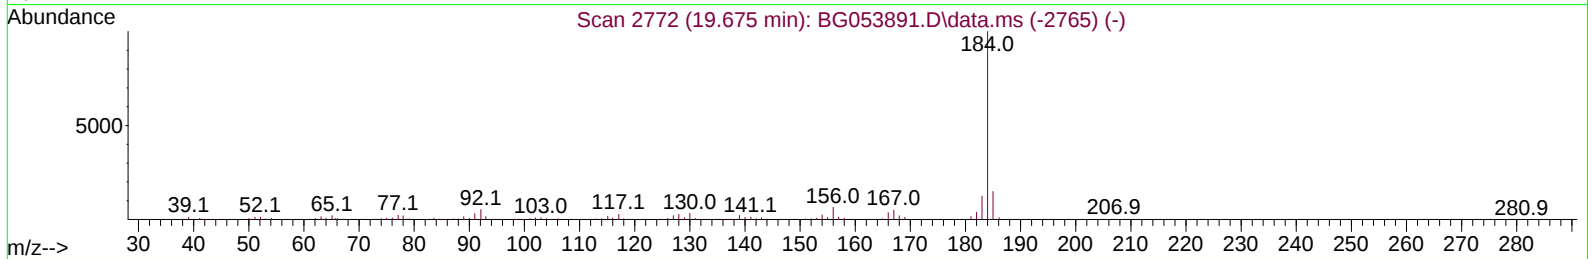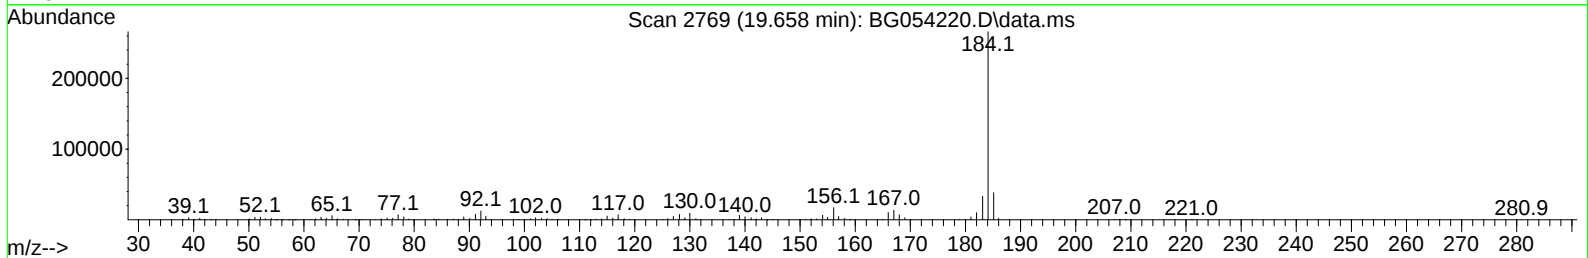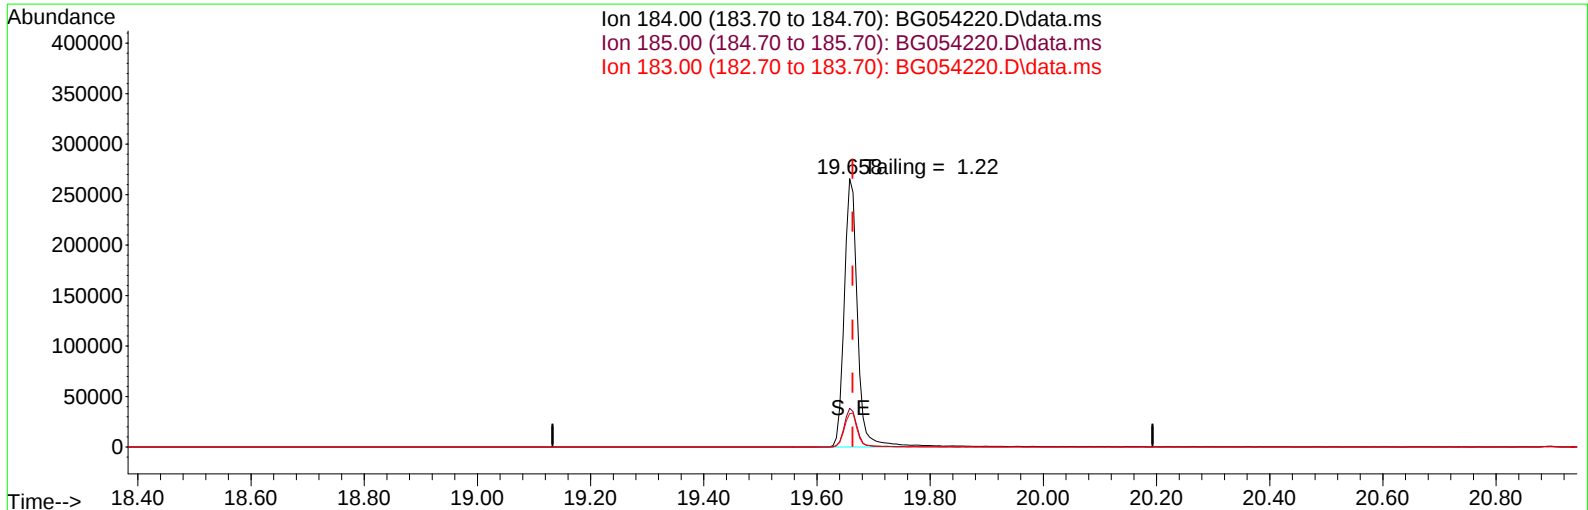

TIC: BG054220.D\data.ms

(77) Benzidine

19.658min (-0.005) 0.00 ng

response 433027

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.43
183.00	11.10	12.47
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/7/2022	BNA_G	<u>BG054220.D</u>
Compound Name	Response	Retention Time
DDT	263231	20.89
DDD	4735	20.45
DDE	1566	19.95
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6301	269532	2.34

Instrument :
BNA_G
ClientSampleId :
DFTPP