
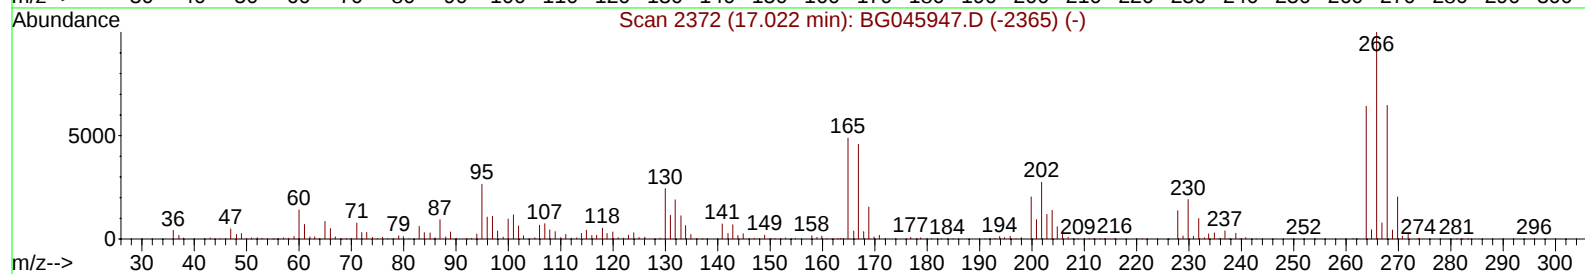
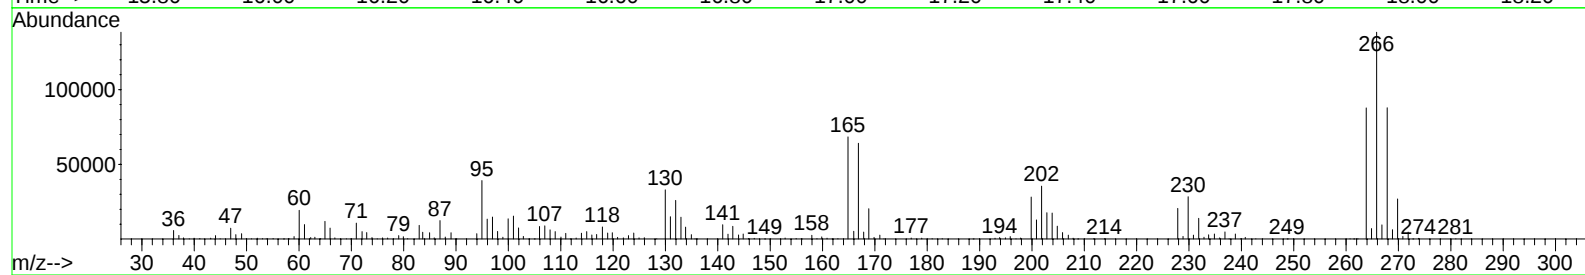


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG070820\
Data File : BG045973.D
Acq On : 8 Jul 2020 8:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 08 17:44:11 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG070620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 07 09:58:42 2020
Response via : Initial Calibration

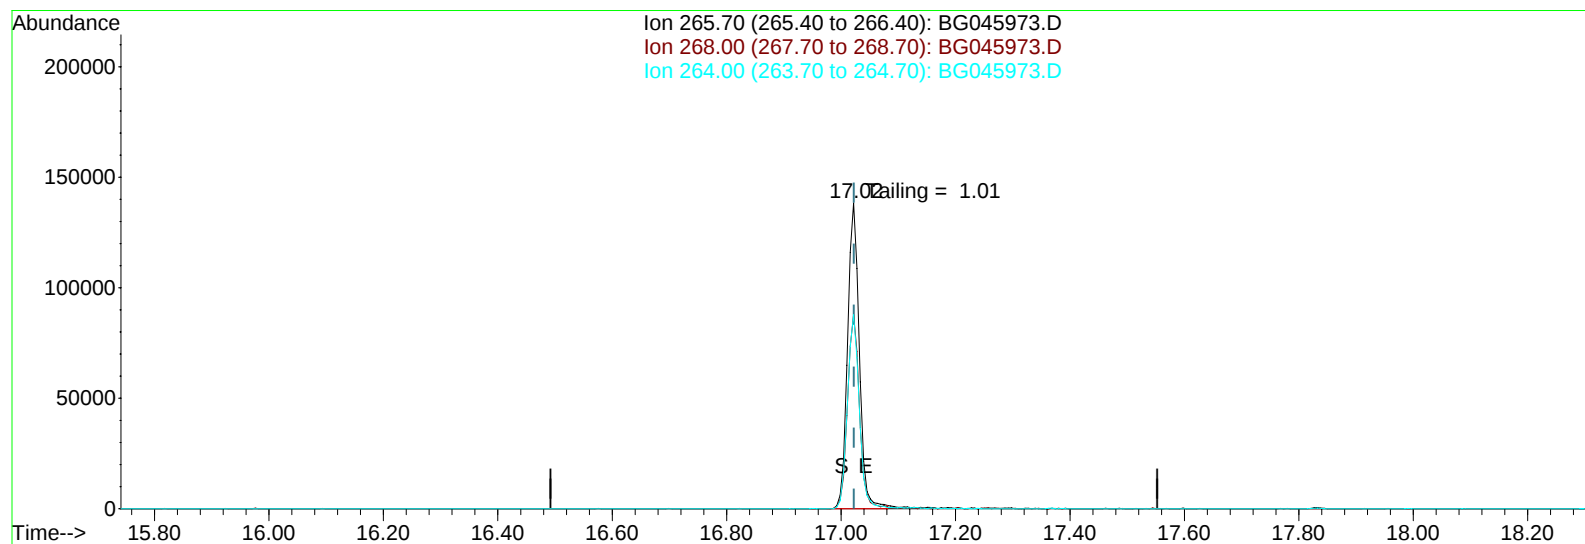

TIC: BG045973.D

(70) Pentachlorophenol (C)




17.022min (-0.001) 530500.45ng

response 198339

Ion	Exp%	Act%
265.70	100	100
268.00	64.80	63.48
264.00	64.20	63.43
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG070820\
 Data File : BG045973.D
 Acq On : 8 Jul 2020 8:10
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 08 17:44:11 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG070620.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 07 09:58:42 2020
 Response via : Initial Calibration

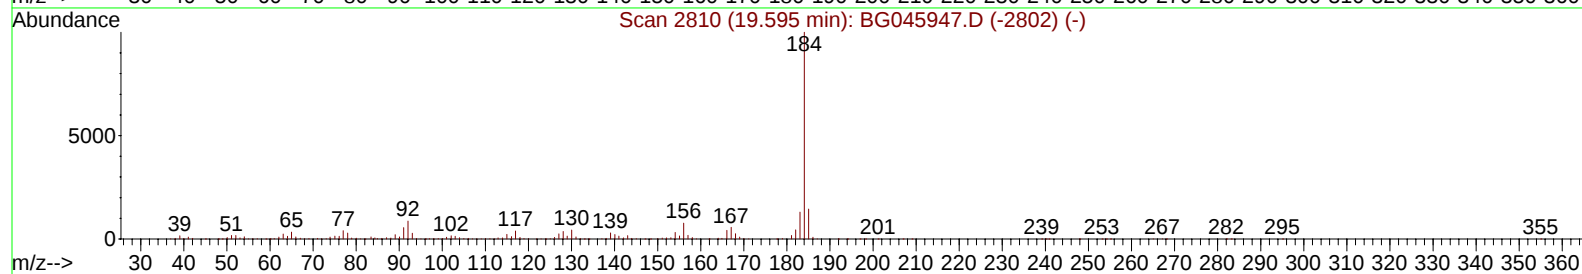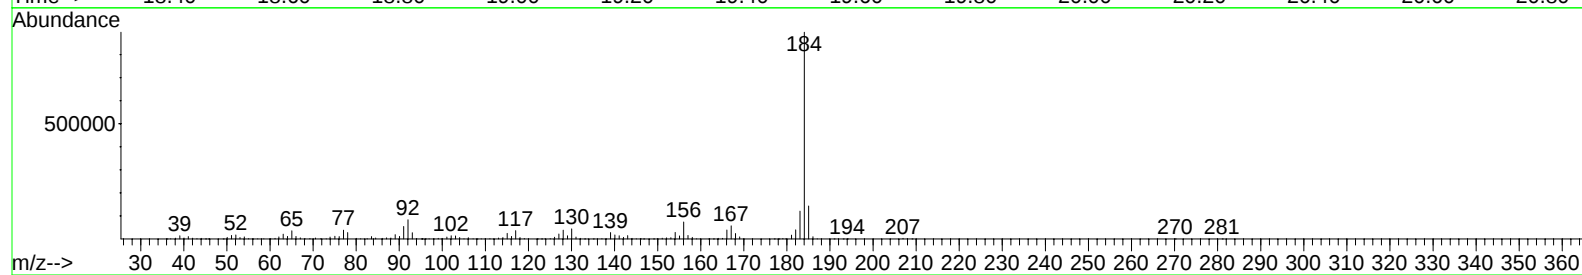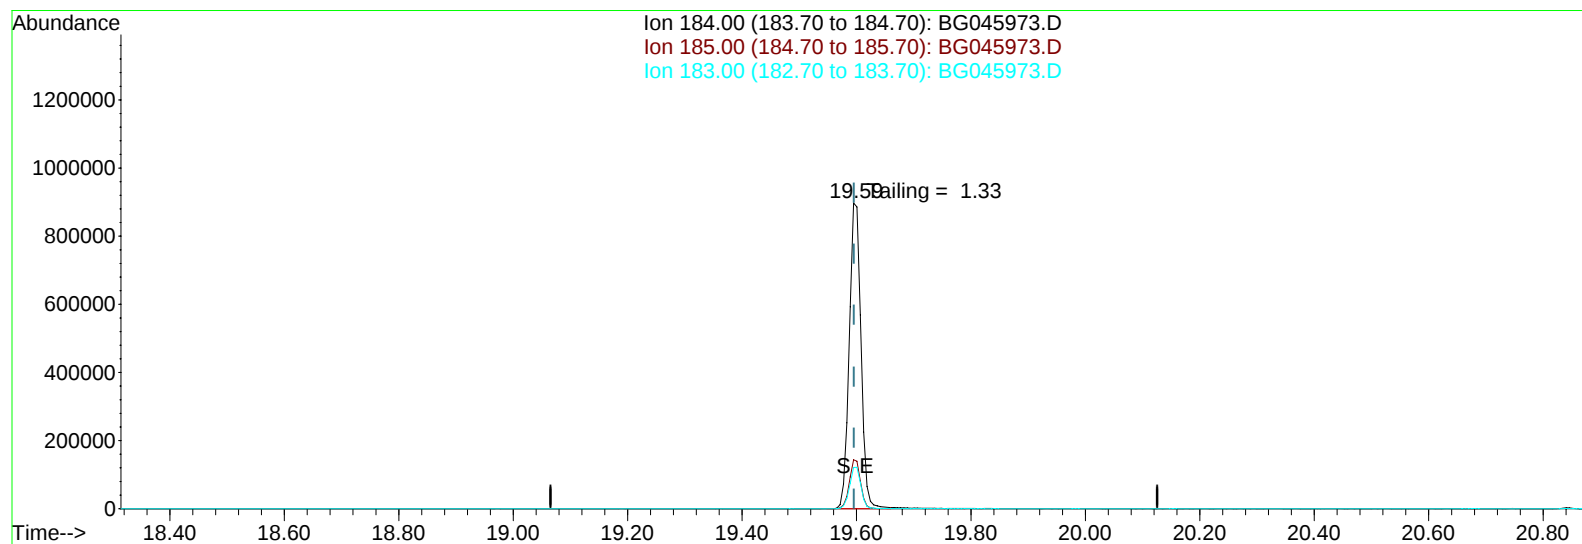

TIC: BG045973.D

(77) Benzidine

19.595min (-0.001) 11755.59ng

response 1289702

Ion	Exp%	Act%
184.00	100	100
185.00	14.50	15.99
183.00	13.00	13.52
0.00	0.00	0.00