


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG070820\
 Data File : BG045973.D
 Acq On : 8 Jul 2020 8:10
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG070620.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 07 09:58:42 2020

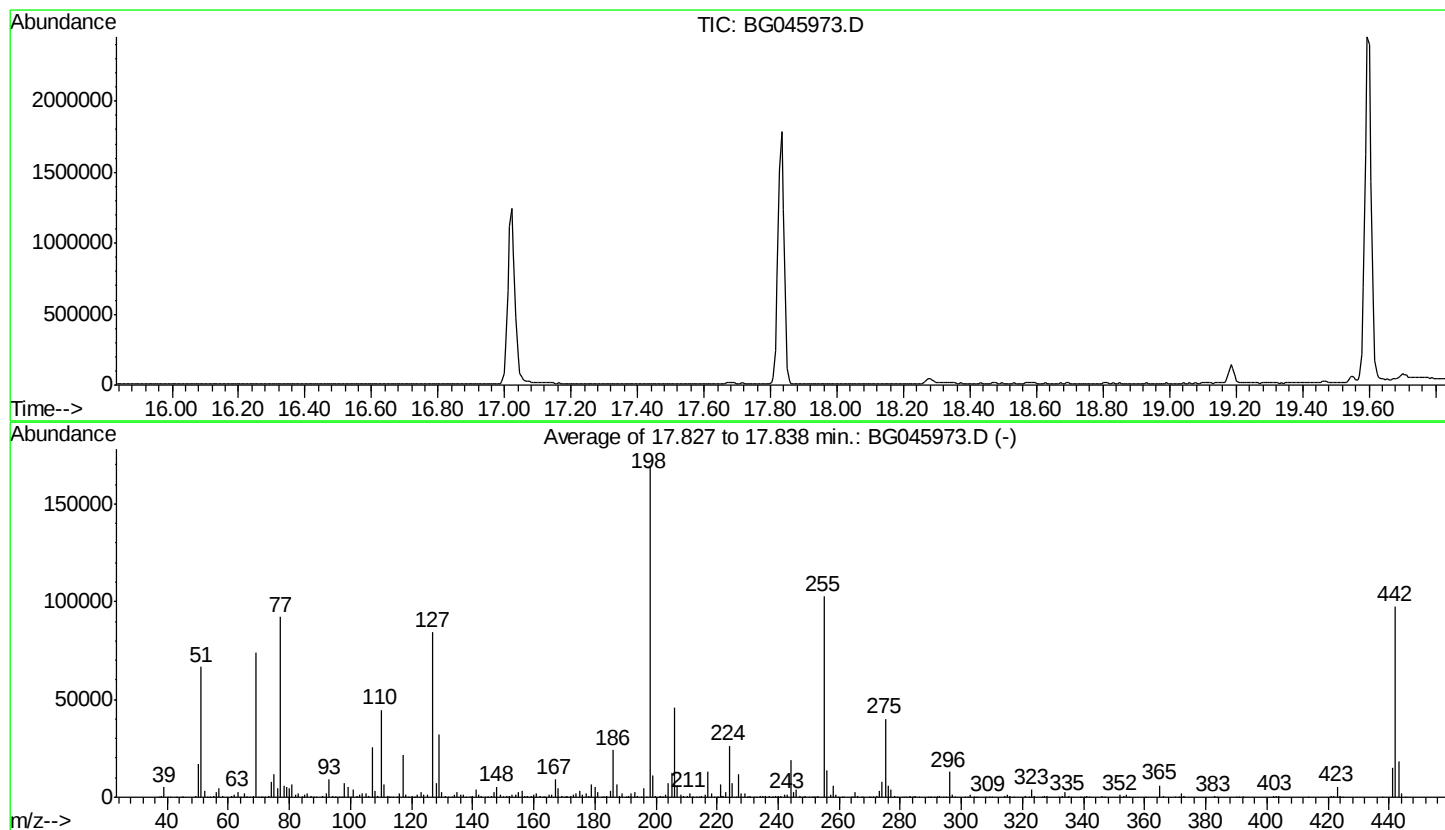

AutoFind: Scans 2509, 2510, 2511; Background Corrected with Scan 2502

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.3	66562	PASS
68	69	0.00	2	1.1	824	PASS
69	198	0.00	100	43.7	74087	PASS
70	69	0.00	2	0.2	165	PASS
127	198	10	80	49.7	84277	PASS
197	198	0.00	2	0.2	332	PASS
198	198	100	100	100.0	169536	PASS
199	198	5	9	6.5	10959	PASS
275	198	10	60	23.6	40002	PASS
365	198	1	100	3.6	6044	PASS
441	198	0.01	100	8.8	15000	PASS
442	198	50	100	57.4	97296	PASS
443	442	15	24	19.1	18600	PASS