

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070823\
 Data File : BG058088.D
 Acq On : 8 Jul 2023 10:54
 Operator : CG/JU
 Sample : 03348-06
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 YBTY3

Quant Time: Jul 09 00:44:07 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 08 10:01:01 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.919	152	33627	20.000	ng/ul	0.00
20) Naphthalene-d8	10.722	136	152244	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.558	164	111589	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.302	188	281079	20.000	ng/ul	0.00
79) Chrysene-d12	21.556	240	253927	20.000	ng/ul	0.00
88) Perylene-d12	24.711	264	309390	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.360	96	6529	6.799	ng/uL	0.00
4) Pyridine-d5	3.765	84	76315	26.176	ng/ul	0.00
7) Phenol-d5	7.085	99	126601	36.865	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.244	67	76267	36.852	ng/ul	0.00
11) 2-Chlorophenol-d4	7.449	132	85752	36.205	ng/ul	0.00
15) 4-Methylphenol-d8	8.624	113	97906	37.783	ng/ul	0.00
21) Nitrobenzene-d5	9.083	128	44836	36.133	ng/ul	0.00
24) 2-Nitrophenol-d4	9.799	143	53377	40.929	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.346	165	95375	38.123	ng/ul	0.00
31) 4-Chloroaniline-d4	10.857	131	121281	31.975	ng/ul	0.00
46) Dimethylphthalate-d6	13.959	166	341189	38.752	ng/ul	0.00
49) Acenaphthylene-d8	14.253	160	376521	39.189	ng/ul	0.00
54) 4-Nitrophenol-d4	14.758	143	51698	33.235	ng/ul	0.00
60) Fluorene-d10	15.551	176	306633	41.008	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.663	200	50142	32.853	ng/ul	0.00
73) Anthracene-d10	17.402	188	531785	40.772	ng/ul	0.00
81) Pyrene-d10	19.688	212	610364	38.166	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.500	264	651405	41.326	ng/ul	0.01


Target Compounds					Qvalue
17) N-Nitroso-di-n-propyla...	8.624	70	2389	1.039 ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070823\
Data File : BG058088.D
Acq On : 8 Jul 2023 10:54
Operator : CG/JU
Sample : 03348-06
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
YBTY3

Quant Time: Jul 09 00:44:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jul 08 10:01:01 2023
Response via : Initial Calibration

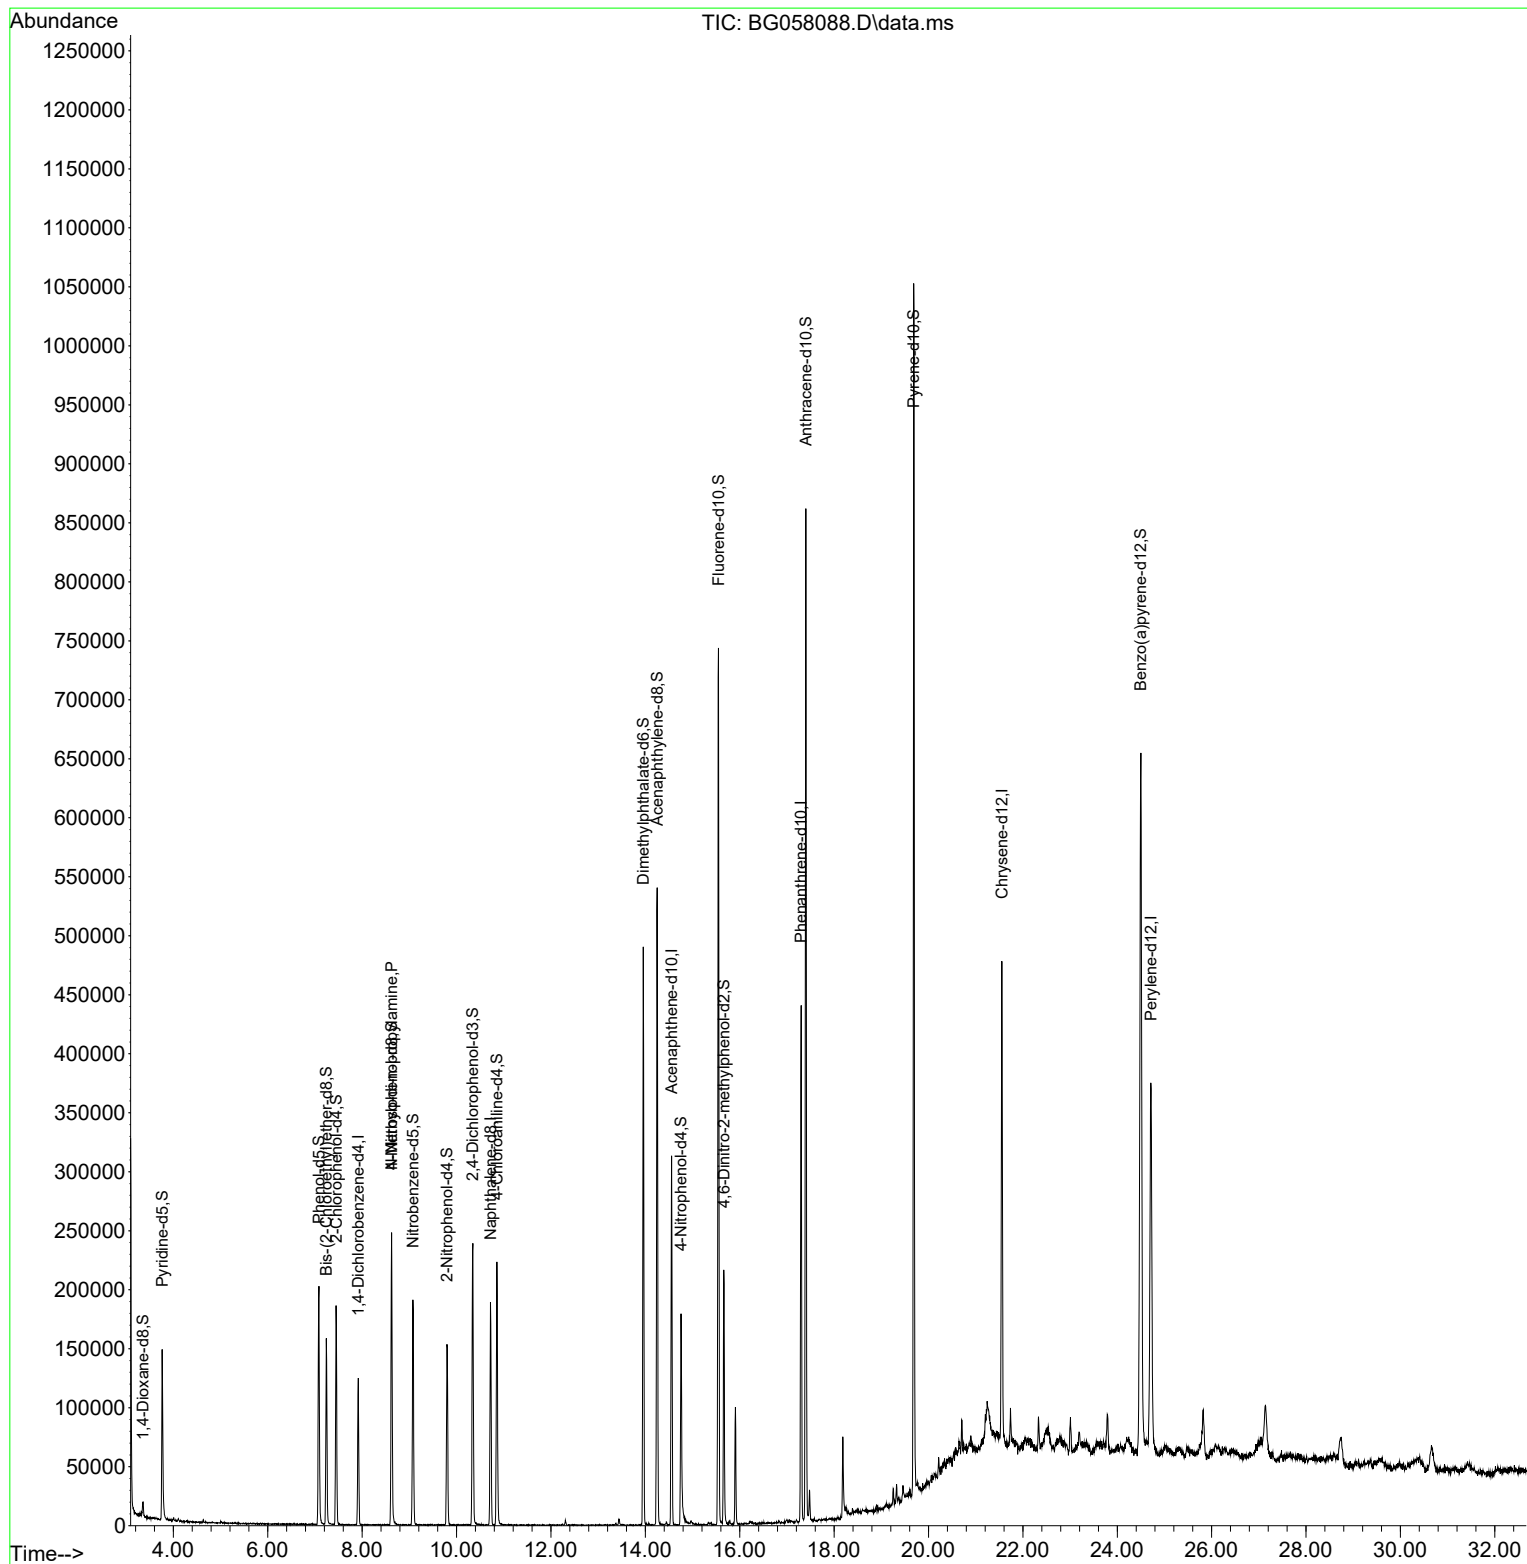

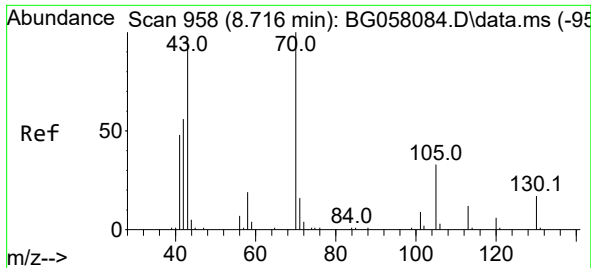

#17
N-Nitroso-di-n-propylamine
Concen: 1.039 ng/ul
RT: 8.624 min Scan# 94
Delta R.T. -0.092 min
Lab File: BG058088.D
Acq: 8 Jul 2023 10:54

Instrument :
BNA_G
ClientSampleId :
YBTY3

Tgt Ion: 70 Resp: 2389
Ion Ratio Lower Upper
70 100
42 370.4 48.0 72.0#
101 0.0 7.4 11.2#
130 0.0 13.4 20.0#

