

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070823\
 Data File : BG058095.D
 Acq On : 8 Jul 2023 15:46
 Operator : CG/JU
 Sample : 03348-12
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 YBW14

Quant Time: Jul 09 00:45:43 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 08 10:01:01 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.917	152	36887	20.000	ng/ul	0.00
20) Naphthalene-d8	10.720	136	173683	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.551	164	131181	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.300	188	339054	20.000	ng/ul	0.00
79) Chrysene-d12	21.548	240	304099	20.000	ng/ul	0.00
88) Perylene-d12	24.703	264	370831	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.358	96	6190	5.876	ng/uL	0.00
4) Pyridine-d5	3.763	84	46511	14.544	ng/ul	0.00
7) Phenol-d5	7.083	99	140062	37.180	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.241	67	84085	37.039	ng/ul	0.00
11) 2-Chlorophenol-d4	7.447	132	93663	36.050	ng/ul	0.00
15) 4-Methylphenol-d8	8.622	113	110402	38.840	ng/ul	0.00
21) Nitrobenzene-d5	9.075	128	53470	37.772	ng/ul	0.00
24) 2-Nitrophenol-d4	9.803	143	60033	40.351	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.344	165	110352	38.665	ng/ul	0.00
31) 4-Chloroaniline-d4	10.855	131	106642	24.645	ng/ul	0.00
46) Dimethylphthalate-d6	13.957	166	401890	38.829	ng/ul	0.00
49) Acenaphthylene-d8	14.251	160	450082	39.849	ng/ul	0.00
54) 4-Nitrophenol-d4	14.756	143	68225	37.309	ng/ul	0.00
60) Fluorene-d10	15.544	176	362884	41.283	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.661	200	63444	34.460	ng/ul	0.00
73) Anthracene-d10	17.394	188	628987	39.979	ng/ul	0.00
81) Pyrene-d10	19.686	212	737505	38.507	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.492	264	777896	41.174	ng/ul	0.00


Target Compounds					Qvalue	
17) N-Nitroso-di-n-propyla...	8.622	70	2788	1.106	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070823\
Data File : BG058095.D
Acq On : 8 Jul 2023 15:46
Operator : CG/JU
Sample : 03348-12
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
YBW14


Quant Time: Jul 09 00:45:43 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jul 08 10:01:01 2023
Response via : Initial Calibration

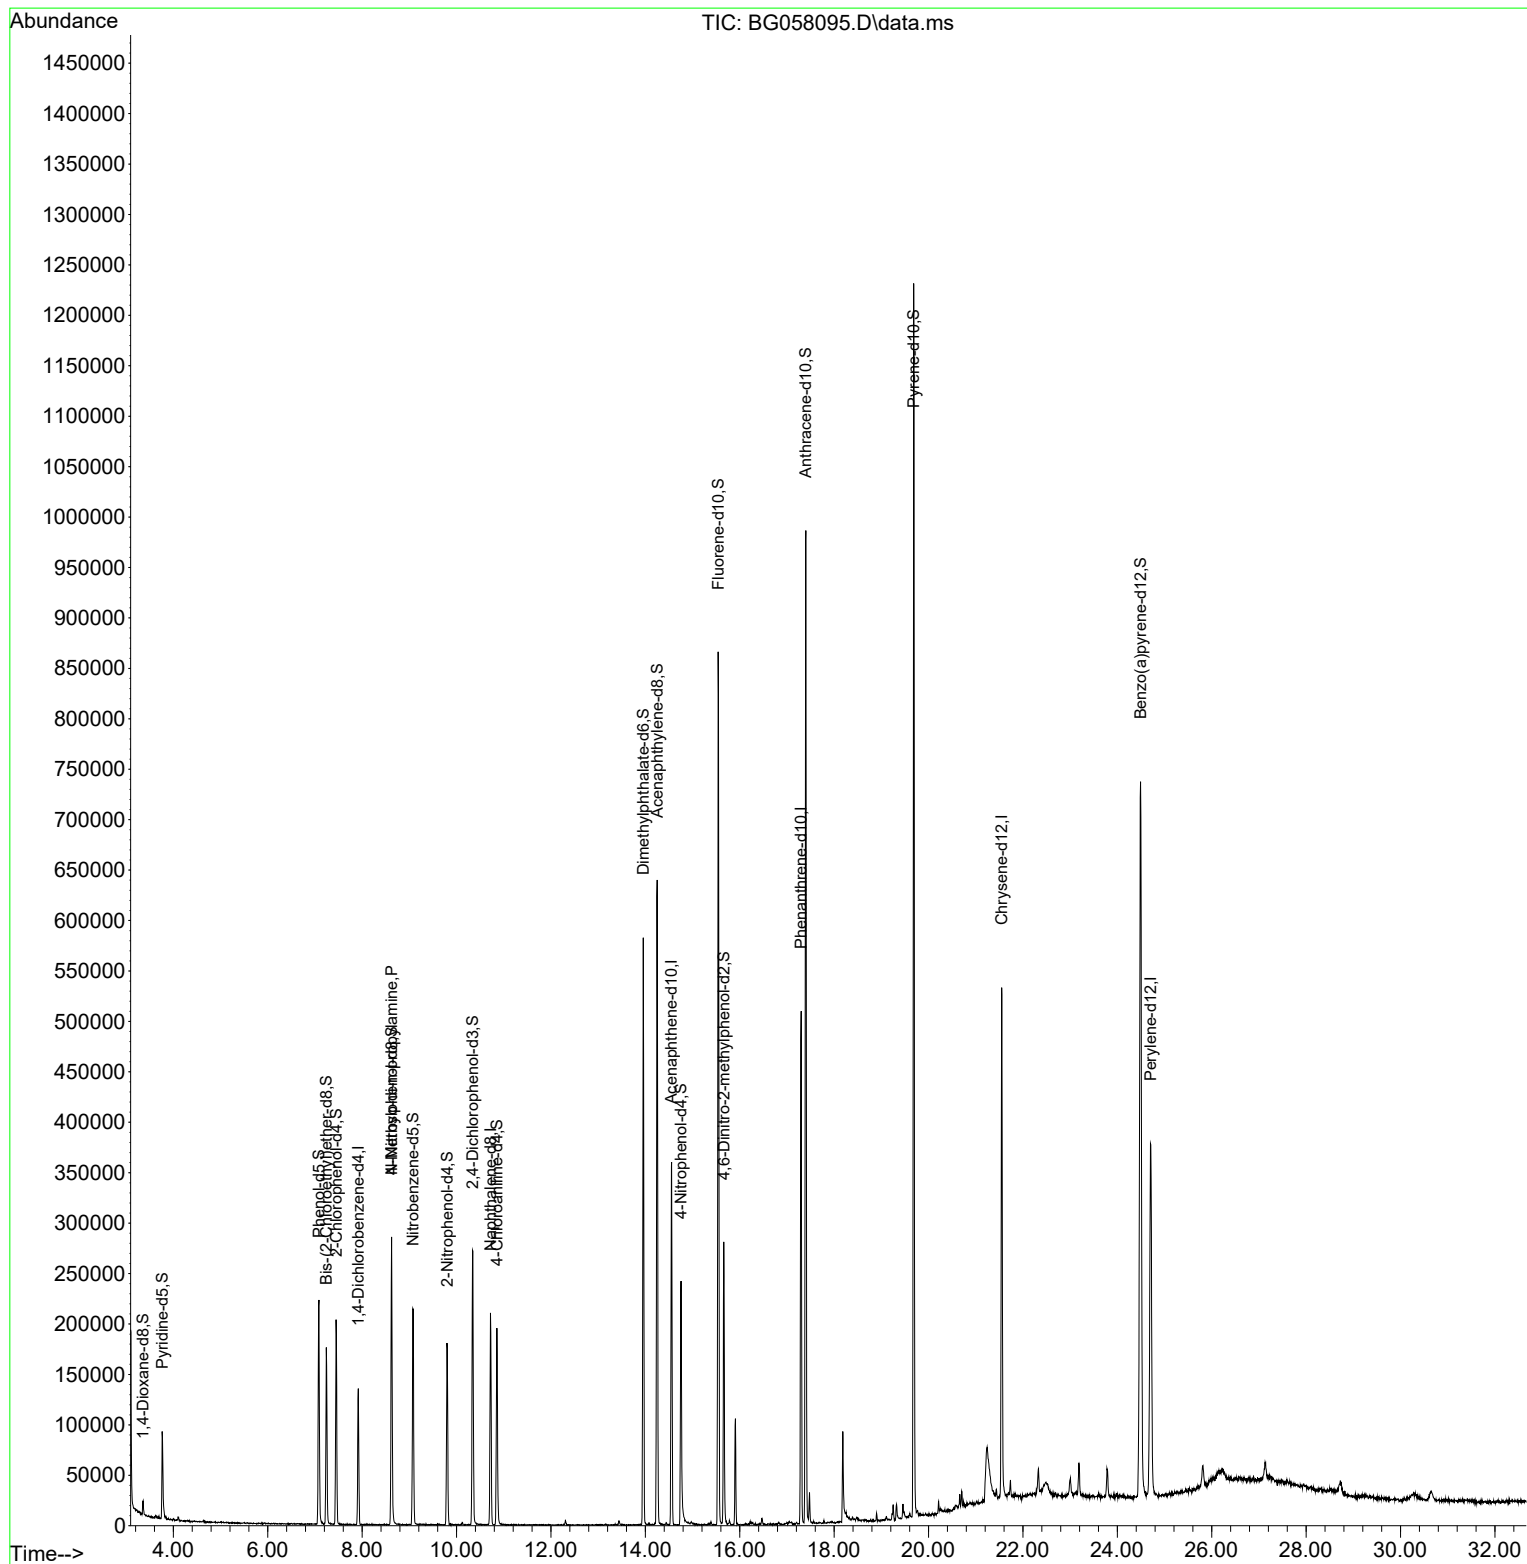

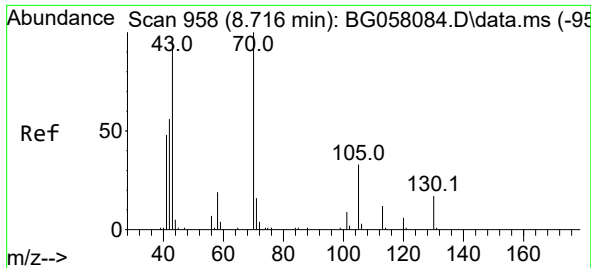

#17
 N-Nitroso-di-n-propylamine
 Concen: 1.106 ng/ul
 RT: 8.622 min Scan# 94
 Delta R.T. -0.094 min
 Lab File: BG058095.D
 Acq: 8 Jul 2023 15:46

Instrument :
 BNA_G
 ClientSampleId :
 YBW14

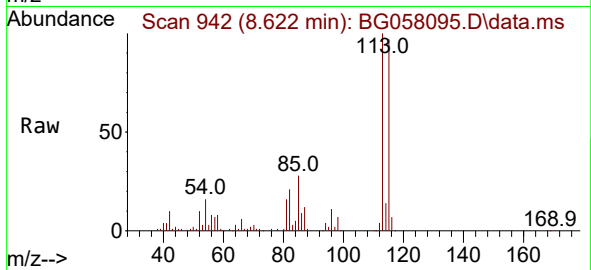

Tgt Ion: 70 Resp: 2788

Ion	Ratio	Lower	Upper
70	100		
42	344.0	48.0	72.0#
101	0.0	7.4	11.2#
130	0.0	13.4	20.0#

