

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070823\
 Data File : BG058097.D
 Acq On : 8 Jul 2023 17:10
 Operator : CG/JU
 Sample : 03348-13
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 YBW15

Quant Time: Jul 09 00:45:57 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 08 10:01:01 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.919	152	44664	20.000	ng/ul	0.00
20) Naphthalene-d8	10.721	136	200799	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.552	164	147360	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.296	188	368449	20.000	ng/ul	0.00
79) Chrysene-d12	21.550	240	334189	20.000	ng/ul	0.00
88) Perylene-d12	24.711	264	402199	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.359	96	5756	4.513	ng/uL	0.00
4) Pyridine-d5	3.771	84	46097	11.904	ng/ul	0.00
7) Phenol-d5	7.078	99	162055	35.528	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.243	67	92148	33.523	ng/ul	0.00
11) 2-Chlorophenol-d4	7.449	132	101478	32.257	ng/ul	0.00
15) 4-Methylphenol-d8	8.624	113	136046	39.528	ng/ul	0.00
21) Nitrobenzene-d5	9.076	128	62851	38.403	ng/ul	0.00
24) 2-Nitrophenol-d4	9.799	143	72803	42.326	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.339	165	136695	41.427	ng/ul	0.00
31) 4-Chloroaniline-d4	10.856	131	110727	22.133	ng/ul	0.00
46) Dimethylphthalate-d6	13.959	166	542173	46.631	ng/ul	0.00
49) Acenaphthylene-d8	14.247	160	593444	46.773	ng/ul	0.00
54) 4-Nitrophenol-d4	14.758	143	89288	43.466	ng/ul	0.00
60) Fluorene-d10	15.545	176	476202	48.226	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.663	200	88951	44.460	ng/ul	0.00
73) Anthracene-d10	17.402	188	819355	47.924	ng/ul	0.00
81) Pyrene-d10	19.687	212	955170	45.382	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.493	264	1021098	49.831	ng/ul	0.00


Target Compounds					Qvalue	
17) N-Nitroso-di-n-propyla...	8.624	70	3197	1.047	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070823\
Data File : BG058097.D
Acq On : 8 Jul 2023 17:10
Operator : CG/JU
Sample : 03348-13
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
YBW15


Quant Time: Jul 09 00:45:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jul 08 10:01:01 2023
Response via : Initial Calibration

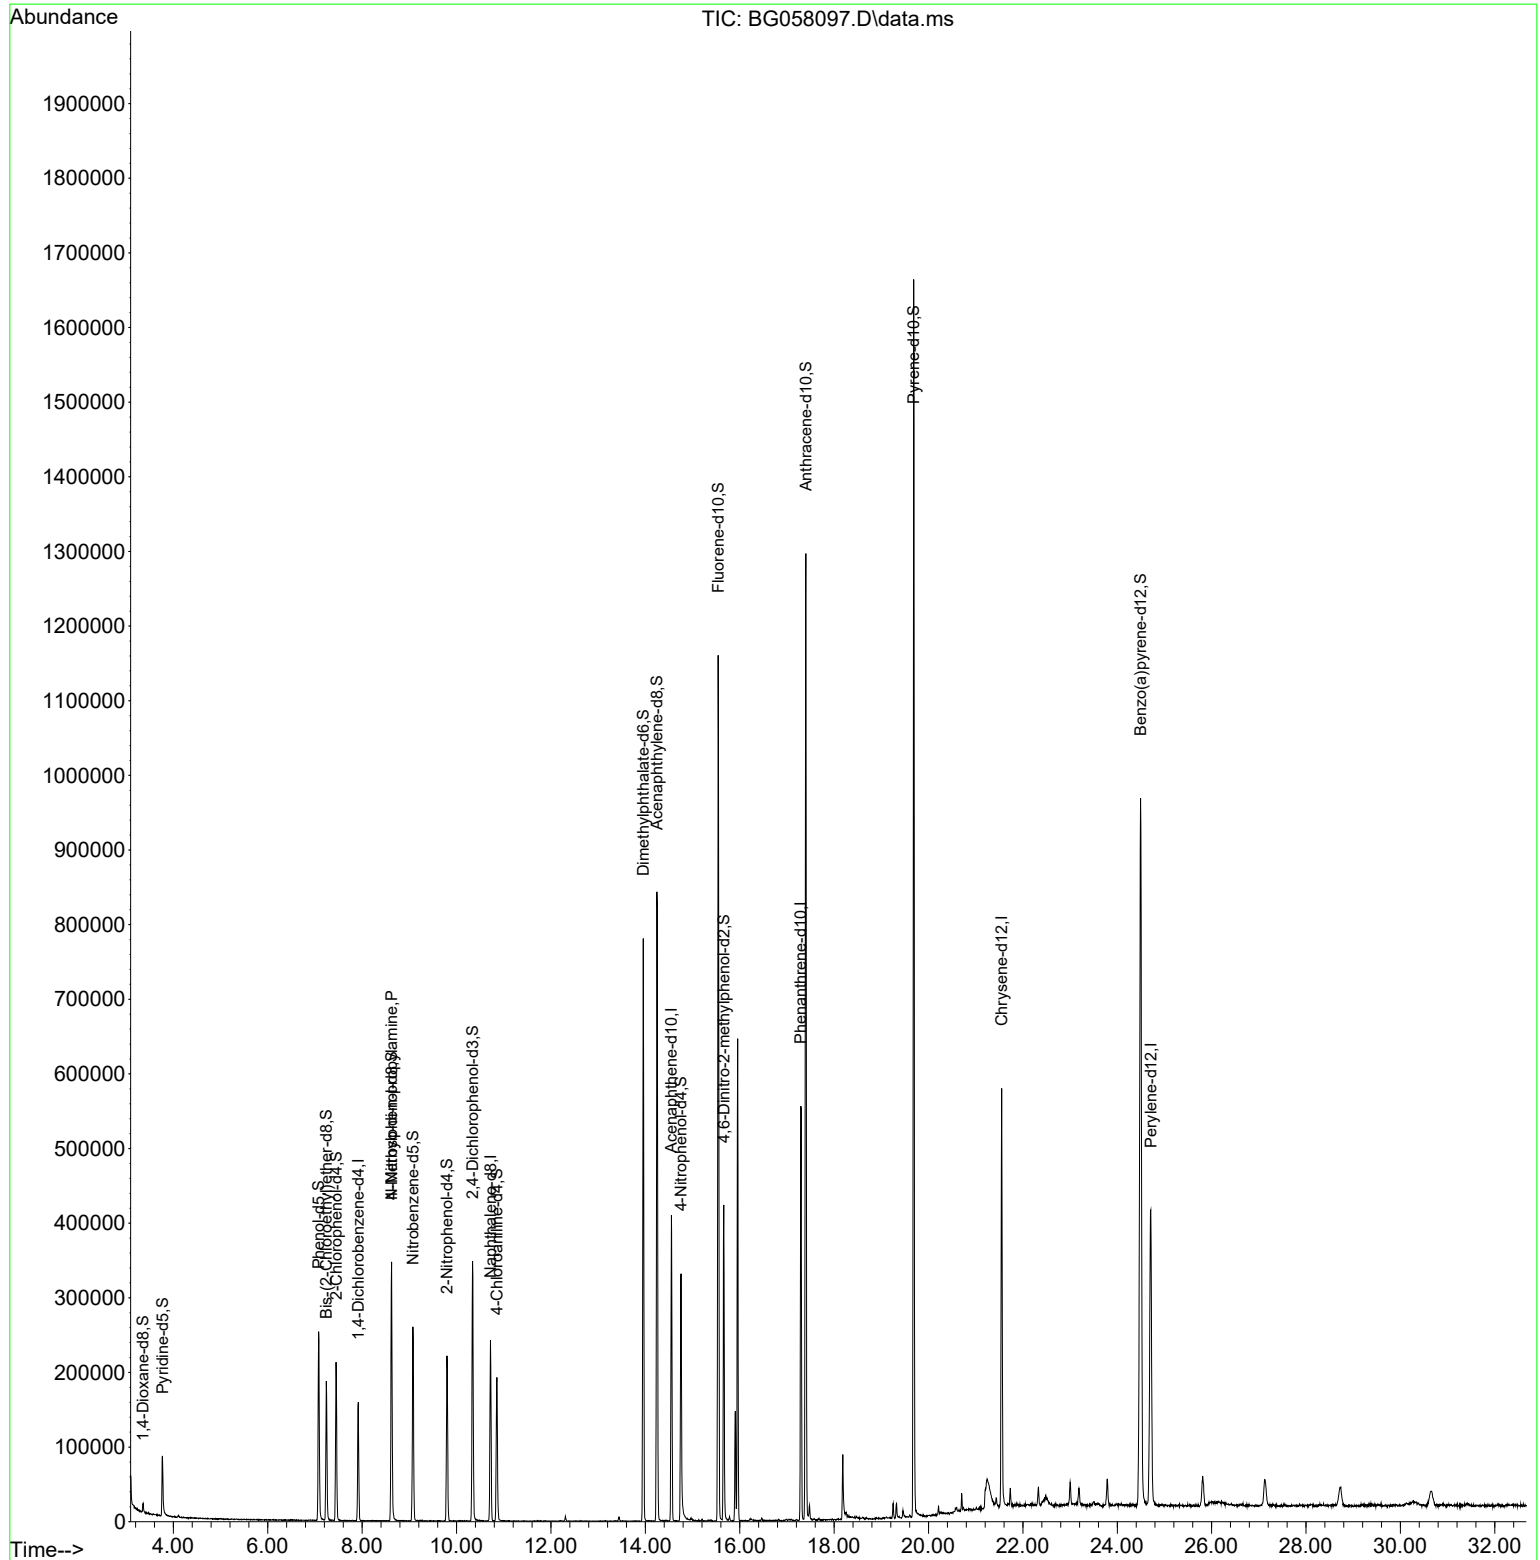

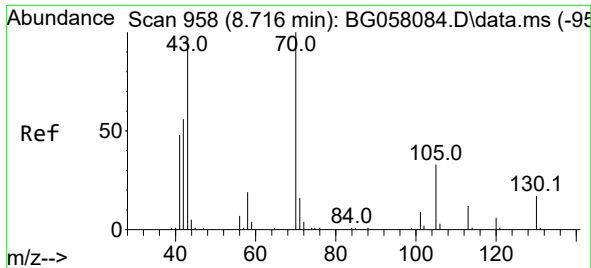

#17
 N-Nitroso-di-n-propylamine
 Concen: 1.047 ng/ul
 RT: 8.624 min Scan# 94
 Delta R.T. -0.093 min
 Lab File: BG058097.D
 Acq: 8 Jul 2023 17:10

Instrument :
 BNA_G
 ClientSampleId :
 YBW15

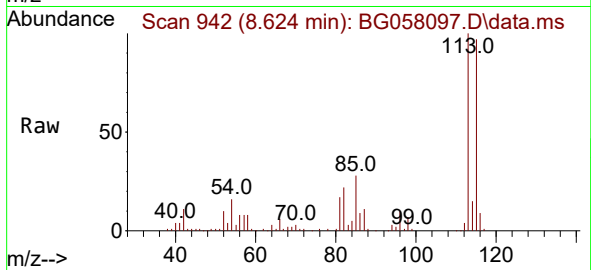

Tgt Ion: 70 Resp: 3197

Ion	Ratio	Lower	Upper
70	100		
42	427.1	48.0	72.0#
101	0.0	7.4	11.2#
130	0.0	13.4	20.0#

