

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070823\
 Data File : BG058117.D
 Acq On : 9 Jul 2023 8:28
 Operator : CG/JU
 Sample : 03349-07MS
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 YBW01MS

Quant Time: Jul 10 00:39:32 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 08 10:01:01 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.915	152	61049	20.000	ng/u1	0.00
20) Naphthalene-d8	10.718	136	281949	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.554	164	208362	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.298	188	513624	20.000	ng/u1	0.00
79) Chrysene-d12	21.552	240	451796	20.000	ng/u1	0.00
88) Perylene-d12	24.707	264	573113	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.356	96	4064	2.331	ng/uL	0.00
4) Pyridine-d5	3.761	84	61879	11.691	ng/u1	0.00
7) Phenol-d5	7.081	99	87705	14.067	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.239	67	52370	13.939	ng/u1	0.00
11) 2-Chlorophenol-d4	7.451	132	58123	13.517	ng/u1	0.00
15) 4-Methylphenol-d8	8.626	113	67376	14.322	ng/u1	0.00
21) Nitrobenzene-d5	9.078	128	32251	14.034	ng/u1	0.00
24) 2-Nitrophenol-d4	9.801	143	36610	15.158	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.342	165	70733	15.267	ng/u1	0.00
31) 4-Chloroaniline-d4	10.859	131	93137	13.259	ng/u1	0.00
46) Dimethylphthalate-d6	13.955	166	237346	14.437	ng/u1	0.00
49) Acenaphthylene-d8	14.249	160	264043	14.718	ng/u1	0.00
54) 4-Nitrophenol-d4	14.754	143	35097	12.083	ng/u1	0.00
60) Fluorene-d10	15.547	176	209965	15.038	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.665	200	36232	12.991	ng/u1	0.00
73) Anthracene-d10	17.398	188	345200	14.484	ng/u1	0.00
81) Pyrene-d10	19.684	212	412341	14.491	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.490	264	433205	14.836	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.391	88	14844	6.892	ng/uL	93
5) Pyridine	3.785	79	100313	18.497	ng/u1	95
6) Benzaldehyde	7.051	77	66988	32.173	ng/u1	95
8) Phenol	7.104	94	134055	21.189	ng/u1	98
10) Bis(2-Chloroethyl)ether	7.333	93	98392	20.141	ng/u1	98
12) 2-Chlorophenol	7.480	128	91983	20.556	ng/u1	98
13) 2-Methylphenol	8.356	108	103898	20.910	ng/u1	97
14) 2,2'-oxybis(1-Chloropr...	8.444	45	156795	20.851	ng/u1	98
16) Acetophenone	8.738	105	166883	21.381	ng/u1	98
17) N-Nitroso-di-n-propyla...	8.720	70	86254	20.672	ng/u1	99
18) 4-Methylphenol	8.685	108	115722	21.539	ng/u1	100
19) Hexachloroethane	8.996	117	34240	19.960	ng/u1	95
22) Nitrobenzene	9.119	77	125114	20.973	ng/u1	99
23) Isophorone	9.636	82	265217	20.835	ng/u1	99
25) 2-Nitrophenol	9.830	139	56704	21.880	ng/u1	99
26) 2,4-Dimethylphenol	9.889	107	114689	19.680	ng/u1	96
27) Bis(2-Chloroethoxy)met...	10.124	93	148197	20.660	ng/u1	98
29) 2,4-Dichlorophenol	10.365	162	97282	21.595	ng/u1	95
30) Naphthalene	10.770	128	328238	20.716	ng/u1	98
32) 4-Chloroaniline	10.876	127	119720	16.668	ng/u1	98
33) Hexachlorobutadiene	11.052	225	66283	20.784	ng/u1	94
34) Caprolactam	11.640	113	38605	21.316	ng/u1	91
35) 4-Chloro-3-methylphenol	12.004	107	125962	22.763	ng/u1	98
36) 2-Methylnaphthalene	12.380	142	227443	21.294	ng/u1	95

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070823\
 Data File : BG058117.D
 Acq On : 9 Jul 2023 8:28
 Operator : CG/JU
 Sample : 03349-07MS
 Misc :
 ALS Vial : 36 Sample Multiplier: 1


Instrument :
 BNA_G
 ClientSampleId :
 YBW01MS


Quant Time: Jul 10 00:39:32 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 08 10:01:01 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.598	142	230461	21.516	ng/ul	98
39) 1,2,4,5-Tetrachloroben...	12.745	216	132971	20.941	ng/ul	96
40) Hexachlorocyclopentadiene	12.721	237	63340	15.837	ng/ul	96
41) 2,4,6-Trichlorophenol	12.985	196	92895	21.585	ng/ul	99
42) 2,4,5-Trichlorophenol	13.062	196	98117	21.081	ng/ul	94
43) 1,1'-Biphenyl	13.385	154	309696	20.625	ng/ul	100
44) 2-Chloronaphthalene	13.432	162	249137	20.674	ng/ul	99
45) 2-Nitroaniline	13.632	65	91400	21.814	ng/ul	96
47) Dimethylphthalate	14.002	163	343975	20.826	ng/ul	100
48) 2,6-Dinitrotoluene	14.131	165	73783	21.763	ng/ul	99
50) Acenaphthylene	14.278	152	410149	21.171	ng/ul	99
51) 3-Nitroaniline	14.460	138	73172	25.539	ng/ul	96
52) Acenaphthene	14.619	153	279543	21.028	ng/ul	98
53) 2,4-Dinitrophenol	14.666	184	37384	21.151	ng/ul	89
55) 4-Nitrophenol	14.772	109	45560	21.174	ng/ul	86
56) Dibenzofuran	14.954	168	401955	21.271	ng/ul	99
57) 2,4-Dinitrotoluene	14.919	165	107719	22.425	ng/ul	99
58) 2,3,4,6-Tetrachlorophenol	15.177	232	89454	21.113	ng/ul	99
59) Diethylphthalate	15.365	149	357189	20.720	ng/ul	99
61) Fluorene	15.600	166	329457	21.248	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.594	204	174872	21.315	ng/ul	96
63) 4-Nitroaniline	15.624	138	76608	29.848	ng/ul	98
66) 4,6-Dinitro-2-methylph...	15.682	198	62233	21.820	ng/ul	100
67) N-Nitrosodiphenylamine	15.806	169	287610	21.041	ng/ul	98
68) 4-Bromophenyl-phenylether	16.487	248	123320	21.873	ng/ul	97
69) Hexachlorobenzene	16.605	284	138411	21.927	ng/ul	99
70) Atrazine	16.752	200	92593	16.565	ng/ul	93
71) Pentachlorophenol	16.946	266	74936	19.774	ng/ul	97
72) Phenanthrene	17.339	178	546325	20.911	ng/ul	99
74) Anthracene	17.433	178	542681	20.526	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.356	216	143300	21.037	ng/uL	96
76) Pentachlorobenzene	14.872	250	350310	48.152	ng/uL	98
77) Carbazole	17.703	167	515787	21.571	ng/ul	98
78) Di-n-butylphthalate	18.256	149	661370	21.713	ng/ul	100
80) Fluoranthene	19.354	202	678357	20.574	ng/ul	98
82) Pyrene	19.719	202	677530	20.414	ng/ul	99
83) Butylbenzylphthalate	20.600	149	288154	21.411	ng/ul	99
84) 3,3'-Dichlorobenzidine	21.452	252	252240	23.062	ng/ul	97
85) Benzo(a)anthracene	21.534	228	682986	21.054	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.434	149	417241	21.634	ng/ul	97
87) Chrysene	21.599	228	653052	21.475	ng/ul	99
89) Di-n-octyl phthalate	22.621	149	738561	20.974	ng/ul	100
90) Benzo(b)fluoranthene	23.702	252	737754	20.790	ng/ul	98
91) Benzo(k)fluoranthene	23.767	252	713642	20.517	ng/ul	98
93) Benzo(a)pyrene	24.554	252	651240	20.734	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	28.291	276	874601	20.970	ng/ul	99
95) Dibenzo(a,h)anthracene	28.356	278	725834	21.104	ng/ul	99
96) Benzo(g,h,i)perylene	29.425	276	712649	20.919	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Jul 10 00:39:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jul 08 10:01:01 2023
Response via : Initial Calibration

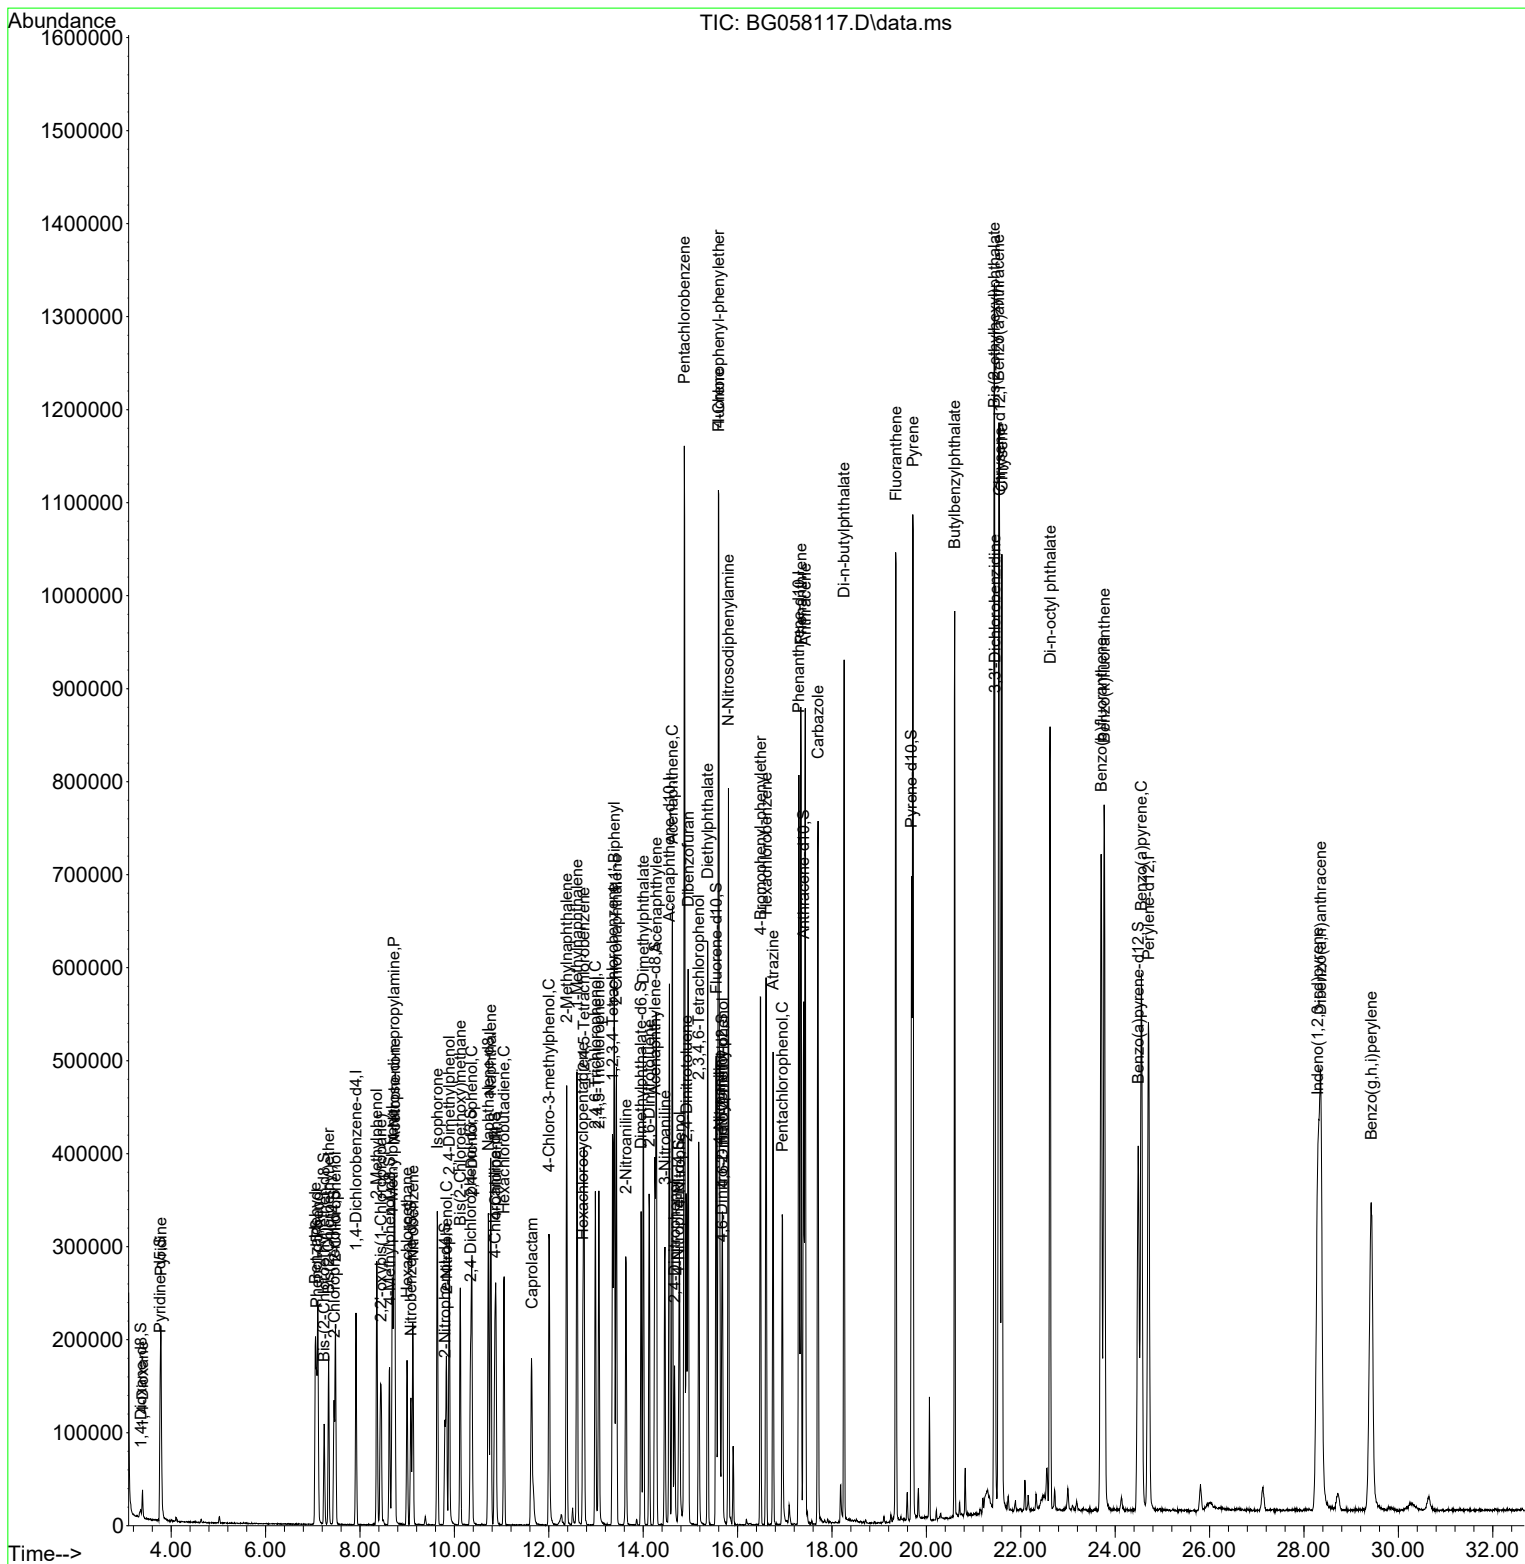



#2
1,4-Dioxane

Concen: 6.892 ng/uL

RT: 3.391 min Scan# 51

Delta R.T. -0.002 min

Lab File: BG058117.D

Acq: 9 Jul 2023 8:28

Instrument :

BNA_G

ClientSampleId :

YBW01MS





Tgt Ion: 88 Resp: 14844

Ion Ratio Lower Upper

88 100

43 29.1 20.6 30.8

58 87.8 65.5 98.3

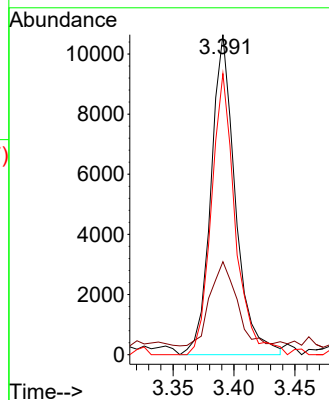

#5

Pyridine

Concen: 18.497 ng/uL

RT: 3.785 min Scan# 118

Delta R.T. -0.002 min

Lab File: BG058117.D

Acq: 9 Jul 2023 8:28




Tgt Ion: 79 Resp: 100313


Ion Ratio Lower Upper

79 100

52 80.8 68.6 102.8

51 38.4 29.4 44.0



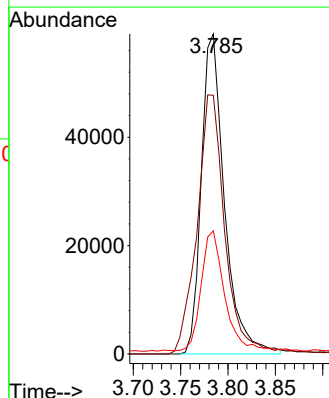





#6
Benzaldehyde
Concen: 32.173 ng/ul
RT: 7.051 min Scan# 611
Delta R.T. -0.008 min
Lab File: BG058117.D
Acq: 9 Jul 2023 8:28




Instrument :
BNA_G
ClientSampleId :
YBW01MS


Tgt Ion: 77 Resp: 66988
Ion Ratio Lower Upper
77 100
105 101.6 74.7 112.1
106 93.5 75.9 113.9

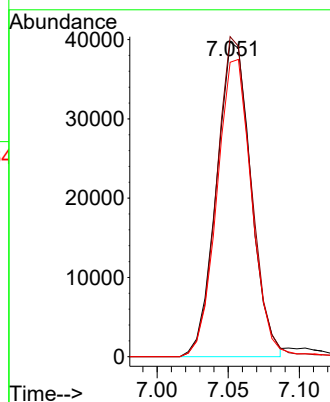

#8
Phenol
Concen: 21.189 ng/ul
RT: 7.104 min Scan# 683
Delta R.T. -0.002 min
Lab File: BG058117.D
Acq: 9 Jul 2023 8:28

Tgt Ion: 94 Resp: 134055
Ion Ratio Lower Upper
94 100
65 29.6 22.2 33.4
66 36.2 28.6 43.0




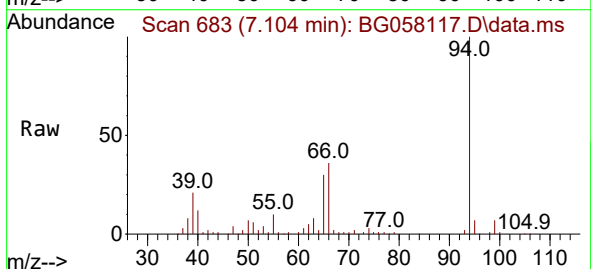




#10
Bis(2-Chloroethyl)ether
Concen: 20.141 ng/ul
RT: 7.333 min Scan# 71
Delta R.T. -0.002 min
Lab File: BG058117.D
Acq: 9 Jul 2023 8:28




Instrument :
BNA_G
ClientSampleId :
YBW01MS


Tgt Ion: 93 Resp: 98392
Ion Ratio Lower Upper
93 100
63 86.2 69.4 104.0
95 31.2 27.0 40.6



#12
2-Chlorophenol
Concen: 20.556 ng/ul
RT: 7.480 min Scan# 747
Delta R.T. -0.002 min
Lab File: BG058117.D
Acq: 9 Jul 2023 8:28

Tgt Ion:128 Resp: 91983
Ion Ratio Lower Upper
128 100
64 56.9 44.3 66.5
130 33.3 27.3 40.9









#13
2-Methylphenol
Concen: 20.910 ng/ul
RT: 8.356 min Scan# 897
Delta R.T. -0.002 min
Lab File: BG058117.D
Acq: 9 Jul 2023 8:28




Instrument :
BNA_G
ClientSampleId :
YBW01MS


Tgt Ion:108 Resp: 103898
Ion Ratio Lower Upper
108 100
107 90.9 75.0 112.4



#14
2,2'-oxybis(1-Chloropropane)
Concen: 20.851 ng/ul
RT: 8.444 min Scan# 911
Delta R.T. 0.004 min
Lab File: BG058117.D
Acq: 9 Jul 2023 8:28

Tgt Ion: 45 Resp: 156795
Ion Ratio Lower Upper
45 100
77 13.2 9.4 14.2
79 10.0 8.3 12.5









#16
Acetophenone
Concen: 21.381 ng/ul
RT: 8.738 min Scan# 961
Delta R.T. -0.002 min
Lab File: BG058117.D
Acq: 9 Jul 2023 8:28




Instrument :
BNA_G
ClientSampleId :
YBW01MS


Tgt Ion:105 Resp: 166883
Ion Ratio Lower Upper
105 100
77 78.4 61.2 91.8
51 29.6 23.5 35.3



#17
N-Nitroso-di-n-propylamine
Concen: 20.672 ng/ul
RT: 8.720 min Scan# 958
Delta R.T. 0.004 min
Lab File: BG058117.D
Acq: 9 Jul 2023 8:28

Tgt Ion: 70 Resp: 86254
Ion Ratio Lower Upper
70 100
42 58.8 48.0 72.0
101 9.2 7.4 11.2
130 16.7 13.4 20.0









#18
4-Methylphenol
Concen: 21.539 ng/ul
RT: 8.685 min Scan# 91
Delta R.T. -0.002 min
Lab File: BG058117.D
Acq: 9 Jul 2023 8:28




Instrument :
BNA_G
ClientSampleId :
YBW01MS


Tgt Ion:108 Resp: 115722
Ion Ratio Lower Upper
108 100
107 114.3 91.1 136.7



#19
Hexachloroethane
Concen: 19.960 ng/ul
RT: 8.996 min Scan# 1005
Delta R.T. -0.002 min
Lab File: BG058117.D
Acq: 9 Jul 2023 8:28

Tgt Ion:117 Resp: 34240
Ion Ratio Lower Upper
117 100
201 111.6 94.0 141.0
199 70.3 59.8 89.6









#22
Nitrobenzene
Concen: 20.973 ng/ul
RT: 9.119 min Scan# 1026
Delta R.T. -0.002 min
Lab File: BG058117.D
Acq: 9 Jul 2023 8:28




Instrument :
BNA_G
ClientSampleId :
YBW01MS


Tgt Ion: 77 Resp: 125114
Ion Ratio Lower Upper
77 100
123 41.3 33.3 49.9
65 13.8 10.4 15.6



#23
Isophorone
Concen: 20.835 ng/ul
RT: 9.636 min Scan# 1114
Delta R.T. -0.002 min
Lab File: BG058117.D
Acq: 9 Jul 2023 8:28

Tgt Ion: 82 Resp: 265217
Ion Ratio Lower Upper
82 100
95 6.0 4.8 7.2
138 14.6 11.4 17.0









#25
2-Nitrophenol
Concen: 21.880 ng/ul
RT: 9.830 min Scan# 1148
Delta R.T. -0.002 min
Lab File: BG058117.D
Acq: 9 Jul 2023 8:28




Instrument :
BNA_G
ClientSampleId :
YBW01MS


Tgt Ion:139 Resp: 56704
Ion Ratio Lower Upper
139 100
65 53.3 42.6 64.0
109 27.6 20.7 31.1



#26
2,4-Dimethylphenol
Concen: 19.680 ng/ul
RT: 9.889 min Scan# 1157
Delta R.T. -0.002 min
Lab File: BG058117.D
Acq: 9 Jul 2023 8:28

Tgt Ion:107 Resp: 114689
Ion Ratio Lower Upper
107 100
121 48.3 40.6 60.8
122 80.3 67.1 100.7





#27

Bis(2-Chloroethoxy)methane

Concen: 20.660 ng/ul

RT: 10.124 min Scan# 1197

Delta R.T. -0.002 min

Lab File: BG058117.D

Acq: 9 Jul 2023 8:28

Instrument :

BNA_G

ClientSampleId :

YBW01MS





Tgt Ion: 93 Resp: 148197

Ion Ratio Lower Upper

93 100

95 32.0 26.4 39.6

123 10.1 7.9 11.9

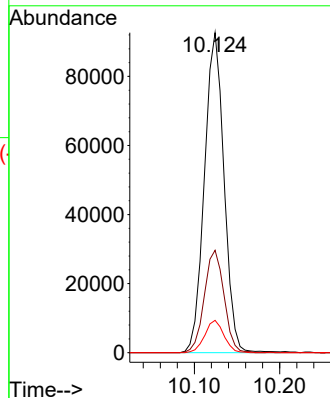

#29

2,4-Dichlorophenol

Concen: 21.595 ng/ul

RT: 10.365 min Scan# 1238

Delta R.T. -0.002 min

Lab File: BG058117.D

Acq: 9 Jul 2023 8:28




Tgt Ion:162 Resp: 97282


Ion Ratio Lower Upper

162 100

164 67.6 51.1 76.7

98 38.6 27.9 41.9



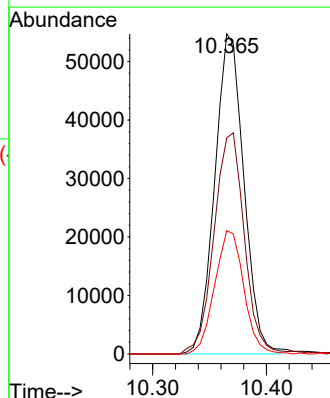





#30
Naphthalene
Concen: 20.716 ng/ul
RT: 10.770 min Scan# 11
Delta R.T. -0.002 min
Lab File: BG058117.D
Acq: 9 Jul 2023 8:28




Instrument :
BNA_G
ClientSampleId :
YBW01MS


Tgt Ion:128 Resp: 328238
Ion Ratio Lower Upper
128 100
129 11.7 8.6 12.8
127 13.6 10.2 15.2



#32
4-Chloroaniline
Concen: 16.668 ng/ul
RT: 10.876 min Scan# 1325
Delta R.T. -0.002 min
Lab File: BG058117.D
Acq: 9 Jul 2023 8:28

Tgt Ion:127 Resp: 119720
Ion Ratio Lower Upper
127 100
129 31.3 26.0 39.0





#33

Hexachlorobutadiene

Concen: 20.784 ng/ul

RT: 11.052 min Scan# 11

Delta R.T. -0.002 min

Lab File: BG058117.D

Acq: 9 Jul 2023 8:28

Instrument :

BNA_G

ClientSampleId :

YBW01MS





Tgt Ion:225 Resp: 66283

Ion Ratio Lower Upper

225 100

223 60.5 53.2 79.8

227 61.3 51.4 77.2

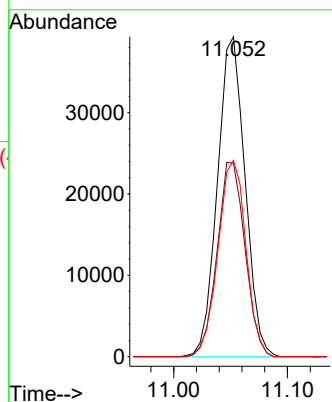

#34

Caprolactam

Concen: 21.316 ng/ul

RT: 11.640 min Scan# 1455

Delta R.T. 0.015 min

Lab File: BG058117.D

Acq: 9 Jul 2023 8:28




Tgt Ion:113 Resp: 38605


Ion Ratio Lower Upper

113 100

55 208.4 183.4 275.2

56 148.4 123.0 184.6









#35
4-Chloro-3-methylphenol
Concen: 22.763 ng/ul
RT: 12.004 min Scan# 11
Delta R.T. -0.002 min
Lab File: BG058117.D
Acq: 9 Jul 2023 8:28




Instrument :
BNA_G
ClientSampleId :
YBW01MS


Tgt Ion:107 Resp: 125962
Ion Ratio Lower Upper
107 100
144 22.4 19.0 28.4
142 71.4 58.4 87.6



#36
2-Methylnaphthalene
Concen: 21.294 ng/ul
RT: 12.380 min Scan# 1581
Delta R.T. 0.004 min
Lab File: BG058117.D
Acq: 9 Jul 2023 8:28

Tgt Ion:142 Resp: 227443
Ion Ratio Lower Upper
142 100
141 91.5 69.4 104.2



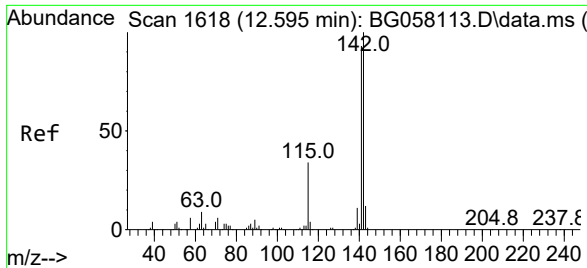

#37

1-Methylnaphthalene

Concen: 21.516 ng/ul

RT: 12.598 min Scan# 1

Delta R.T. -0.002 min

Lab File: BG058117.D

Acq: 9 Jul 2023 8:28

Instrument :

BNA_G

ClientSampleId :

YBW01MS





Tgt Ion:142 Resp: 230461

Ion Ratio Lower Upper

142 100

141 94.7 73.8 110.8

116 3.8 3.0 4.4

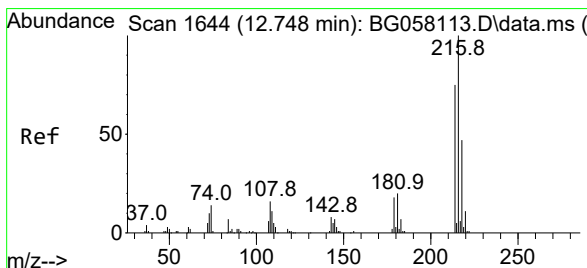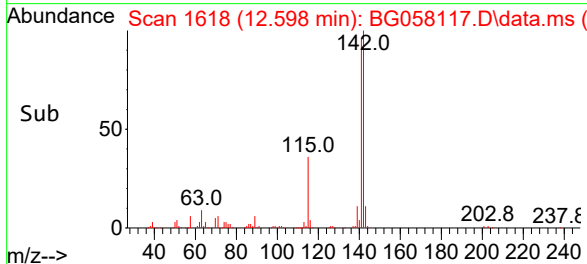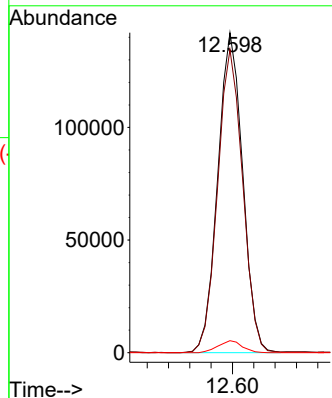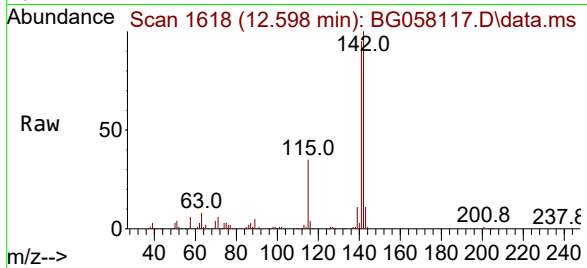

#39

1,2,4,5-Tetrachlorobenzene

Concen: 20.941 ng/ul

RT: 12.745 min Scan# 1643

Delta R.T. -0.002 min

Lab File: BG058117.D

Acq: 9 Jul 2023 8:28

Tgt Ion:216 Resp: 132971




Ion Ratio Lower Upper


216 100

214 75.9 64.1 96.1

179 19.5 16.0 24.0

108 15.2 12.1 18.1

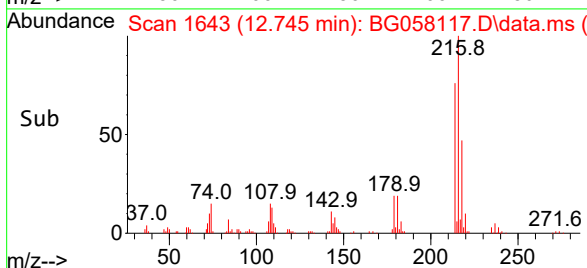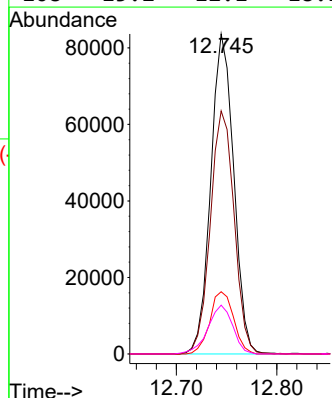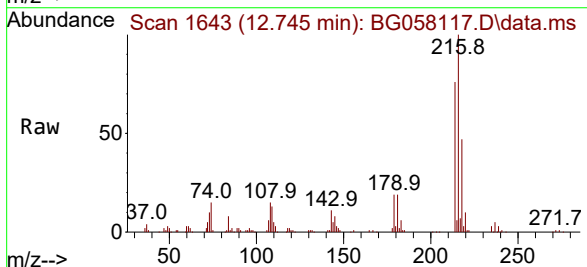



#40

Hexachlorocyclopentadiene

Concen: 15.837 ng/ul

RT: 12.721 min Scan# 1

Delta R.T. -0.002 min

Lab File: BG058117.D

Acq: 9 Jul 2023 8:28

Instrument :

BNA_G

ClientSampleId :

YBW01MS





Tgt Ion:237 Resp: 63340

Ion Ratio Lower Upper

237 100

235 64.8 49.2 73.8

272 13.0 10.4 15.6

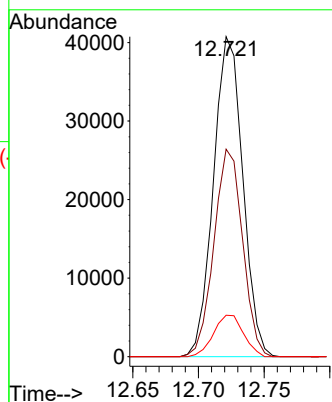

#41

2,4,6-Trichlorophenol

Concen: 21.585 ng/ul

RT: 12.985 min Scan# 1684

Delta R.T. -0.002 min

Lab File: BG058117.D

Acq: 9 Jul 2023 8:28




Tgt Ion:196 Resp: 92895


Ion Ratio Lower Upper

196 100

198 92.5 73.5 110.3

200 30.5 24.8 37.2









#42
2,4,5-Trichlorophenol
Concen: 21.081 ng/ul
RT: 13.062 min Scan# 1
Delta R.T. -0.002 min
Lab File: BG058117.D
Acq: 9 Jul 2023 8:28




Instrument :
BNA_G
ClientSampleId :
YBW01MS


Tgt Ion:196 Resp: 98117
Ion Ratio Lower Upper
196 100
198 89.5 77.2 115.8
200 29.2 23.8 35.6



#43
1,1'-Biphenyl
Concen: 20.625 ng/ul
RT: 13.385 min Scan# 1752
Delta R.T. -0.002 min
Lab File: BG058117.D
Acq: 9 Jul 2023 8:28

Tgt Ion:154 Resp: 309696
Ion Ratio Lower Upper
154 100
153 40.7 32.6 49.0
76 14.7 11.6 17.4









#44
2-Chloronaphthalene
Concen: 20.674 ng/ul
RT: 13.432 min Scan# 1760
Delta R.T. 0.004 min
Lab File: BG058117.D
Acq: 9 Jul 2023 8:28




Instrument :
BNA_G
ClientSampleId :
YBW01MS


Tgt Ion:162 Resp: 249137
Ion Ratio Lower Upper
162 100
164 34.2 27.7 41.5
127 39.3 30.9 46.3



#45
2-Nitroaniline
Concen: 21.814 ng/ul
RT: 13.632 min Scan# 1794
Delta R.T. -0.002 min
Lab File: BG058117.D
Acq: 9 Jul 2023 8:28

Tgt Ion: 65 Resp: 91400
Ion Ratio Lower Upper
65 100
92 63.6 53.2 79.8
138 93.1 71.1 106.7









#47
Dimethylphthalate
Concen: 20.826 ng/ul
RT: 14.002 min Scan# 1857
Delta R.T. -0.002 min
Lab File: BG058117.D
Acq: 9 Jul 2023 8:28




Instrument :
BNA_G
ClientSampleId :
YBW01MS


Tgt Ion:163 Resp: 343975
Ion Ratio Lower Upper
163 100
194 3.7 3.0 4.4
164 10.6 8.6 12.8



#48
2,6-Dinitrotoluene
Concen: 21.763 ng/ul
RT: 14.131 min Scan# 1879
Delta R.T. 0.004 min
Lab File: BG058117.D
Acq: 9 Jul 2023 8:28

Tgt Ion:165 Resp: 73783
Ion Ratio Lower Upper
165 100
89 53.0 42.7 64.1
121 19.1 14.8 22.2









#50
Acenaphthylene
Concen: 21.171 ng/ul
RT: 14.278 min Scan# 1904
Delta R.T. 0.004 min
Lab File: BG058117.D
Acq: 9 Jul 2023 8:28




Instrument :
BNA_G
ClientSampleId :
YBW01MS


Tgt Ion:152 Resp: 410149
Ion Ratio Lower Upper
152 100
151 20.2 15.6 23.4
153 13.1 10.5 15.7



#51
3-Nitroaniline
Concen: 25.539 ng/ul
RT: 14.460 min Scan# 1935
Delta R.T. 0.004 min
Lab File: BG058117.D
Acq: 9 Jul 2023 8:28

Tgt Ion:138 Resp: 73172
Ion Ratio Lower Upper
138 100
108 11.1 8.2 12.2
92 120.9 100.2 150.4









#52
Acenaphthene
Concen: 21.028 ng/ul
RT: 14.619 min Scan# 1962
Delta R.T. 0.004 min
Lab File: BG058117.D
Acq: 9 Jul 2023 8:28




Instrument :
BNA_G
ClientSampleId :
YBW01MS


Tgt Ion:153 Resp: 279543
Ion Ratio Lower Upper
153 100
152 47.7 36.5 54.7
154 86.7 70.5 105.7



#53
2,4-Dinitrophenol
Concen: 21.151 ng/ul
RT: 14.666 min Scan# 1970
Delta R.T. 0.004 min
Lab File: BG058117.D
Acq: 9 Jul 2023 8:28

Tgt Ion:184 Resp: 37384
Ion Ratio Lower Upper
184 100
63 74.4 51.1 76.7
154 59.8 43.3 64.9









#55
4-Nitrophenol
Concen: 21.174 ng/ul
RT: 14.772 min Scan# 1988
Delta R.T. 0.004 min
Lab File: BG058117.D
Acq: 9 Jul 2023 8:28




Instrument :
BNA_G
ClientSampleId :
YBW01MS


Tgt Ion:109 Resp: 45560
Ion Ratio Lower Upper
109 100
139 130.9 119.0 178.4
65 150.5 135.5 203.3

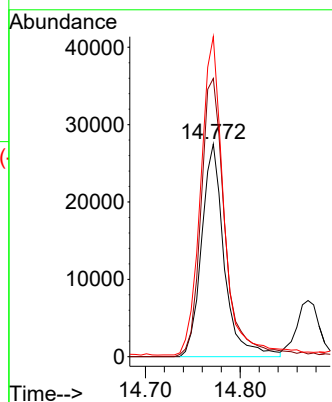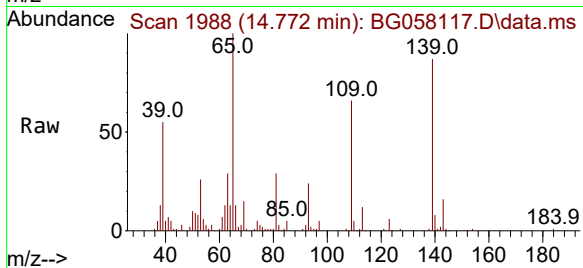

#56
Dibenzofuran
Concen: 21.271 ng/ul
RT: 14.954 min Scan# 2019
Delta R.T. 0.004 min
Lab File: BG058117.D
Acq: 9 Jul 2023 8:28

Tgt Ion:168 Resp: 401955
Ion Ratio Lower Upper
168 100
139 34.8 27.6 41.4




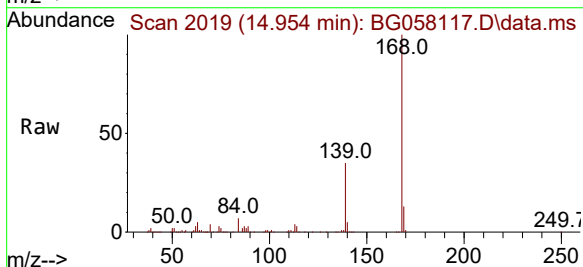




#57
2,4-Dinitrotoluene
Concen: 22.425 ng/ul
RT: 14.919 min Scan# 2013
Delta R.T. 0.004 min
Lab File: BG058117.D
Acq: 9 Jul 2023 8:28




Instrument :
BNA_G
ClientSampleId :
YBW01MS


Tgt Ion:165 Resp: 107719
Ion Ratio Lower Upper
165 100
63 44.0 35.8 53.8
182 1.9 1.6 2.4



#58
2,3,4,6-Tetrachlorophenol
Concen: 21.113 ng/ul
RT: 15.177 min Scan# 2057
Delta R.T. -0.002 min
Lab File: BG058117.D
Acq: 9 Jul 2023 8:28

Tgt Ion:232 Resp: 89454
Ion Ratio Lower Upper
232 100
131 38.4 30.5 45.7
130 2.0 1.4 2.0
166 29.8 22.6 34.0



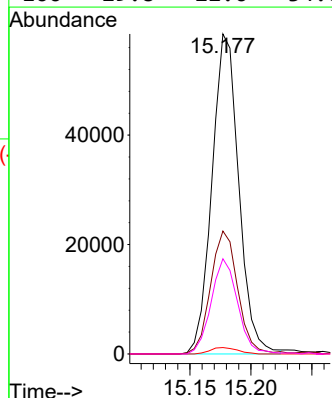





#59
Diethylphthalate
Concen: 20.720 ng/ul
RT: 15.365 min Scan# 2090
Delta R.T. -0.002 min
Lab File: BG058117.D
Acq: 9 Jul 2023 8:28




Instrument :
BNA_G
ClientSampleId :
YBW01MS


Tgt Ion:149 Resp: 357189
Ion Ratio Lower Upper
149 100
177 23.1 17.8 26.8
150 12.9 10.1 15.1

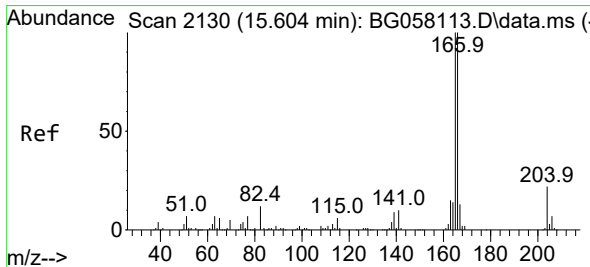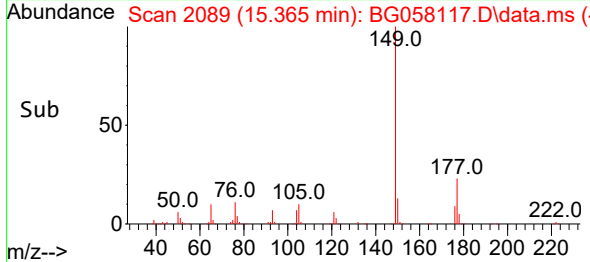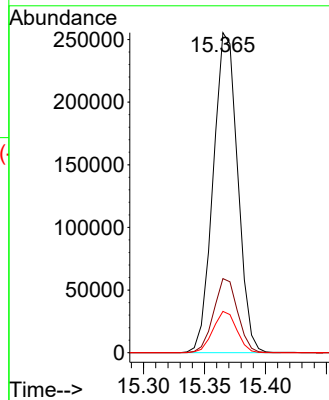

#61
Fluorene
Concen: 21.248 ng/ul
RT: 15.600 min Scan# 2129
Delta R.T. -0.002 min
Lab File: BG058117.D
Acq: 9 Jul 2023 8:28

Tgt Ion:166 Resp: 329457
Ion Ratio Lower Upper
166 100
165 100.1 79.1 118.7
167 13.6 10.7 16.1


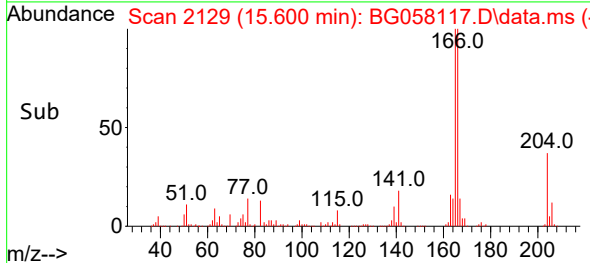
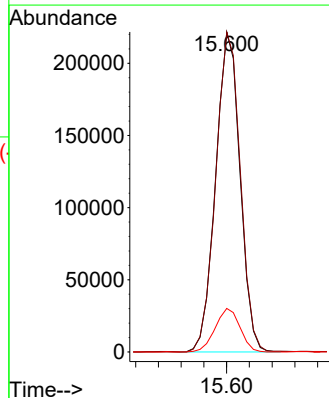
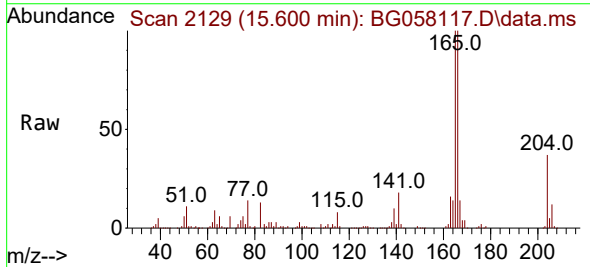




#62
4-Chlorophenyl-phenylether
Concen: 21.315 ng/ul
RT: 15.594 min Scan# 2128
Delta R.T. 0.004 min
Lab File: BG058117.D
Acq: 9 Jul 2023 8:28




Instrument :
BNA_G
ClientSampleId :
YBW01MS


Tgt Ion:204 Resp: 174872
Ion Ratio Lower Upper
204 100
206 33.6 25.8 38.6
141 48.6 41.8 62.6



#63
4-Nitroaniline
Concen: 29.848 ng/ul
RT: 15.624 min Scan# 2133
Delta R.T. 0.010 min
Lab File: BG058117.D
Acq: 9 Jul 2023 8:28

Tgt Ion:138 Resp: 76608
Ion Ratio Lower Upper
138 100
92 54.4 43.8 65.8
108 76.2 58.8 88.2









#66
4,6-Dinitro-2-methylphenol
Concen: 21.820 ng/ul
RT: 15.682 min Scan# 2143
Delta R.T. 0.004 min
Lab File: BG058117.D
Acq: 9 Jul 2023 8:28




Instrument :
BNA_G
ClientSampleId :
YBW01MS


Tgt Ion:198 Resp: 62233
Ion Ratio Lower Upper
198 100
182 3.2 3.1 4.7
77 22.4 17.9 26.9



#67
N-Nitrosodiphenylamine
Concen: 21.041 ng/ul
RT: 15.806 min Scan# 2164
Delta R.T. -0.002 min
Lab File: BG058117.D
Acq: 9 Jul 2023 8:28

Tgt Ion:169 Resp: 287610
Ion Ratio Lower Upper
169 100
168 69.6 54.2 81.2
167 39.3 30.8 46.2









#68
4-Bromophenyl-phenylether
Concen: 21.873 ng/ul
RT: 16.487 min Scan# 21
Delta R.T. -0.002 min
Lab File: BG058117.D
Acq: 9 Jul 2023 8:28




Instrument :
BNA_G
ClientSampleId :
YBW01MS


Tgt Ion:248 Resp: 123320
Ion Ratio Lower Upper
248 100
250 95.5 78.3 117.5
141 59.3 49.1 73.7

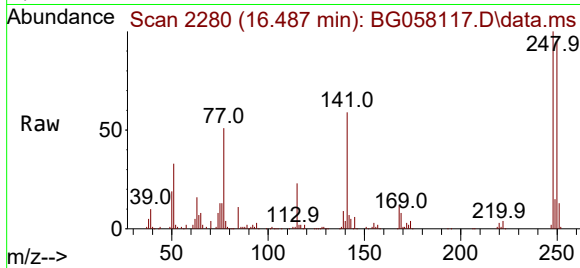

#69
Hexachlorobenzene
Concen: 21.927 ng/ul
RT: 16.605 min Scan# 2300
Delta R.T. 0.004 min
Lab File: BG058117.D
Acq: 9 Jul 2023 8:28

Tgt Ion:284 Resp: 138411
Ion Ratio Lower Upper
284 100
142 27.0 21.9 32.9
249 32.3 25.0 37.6




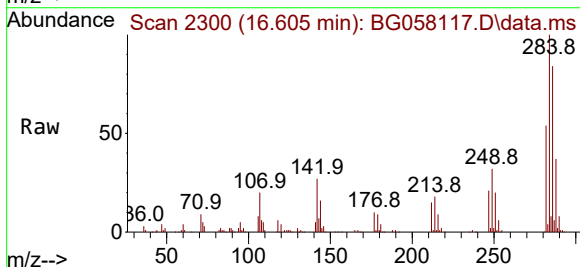




#70
 Atrazine
 Concen: 16.565 ng/ul
 RT: 16.752 min Scan# 21
 Delta R.T. -0.002 min
 Lab File: BG058117.D
 Acq: 9 Jul 2023 8:28




Instrument :
 BNA_G
 ClientSampleId :
 YBW01MS


Tgt Ion:200 Resp: 92593
 Ion Ratio Lower Upper
 200 100
 173 26.5 20.0 30.0
 215 50.4 35.8 53.8



#71
 Pentachlorophenol
 Concen: 19.774 ng/ul
 RT: 16.946 min Scan# 2358
 Delta R.T. -0.002 min
 Lab File: BG058117.D
 Acq: 9 Jul 2023 8:28

Tgt Ion:266 Resp: 74936
 Ion Ratio Lower Upper
 266 100
 264 61.4 51.5 77.3
 268 59.5 49.0 73.4







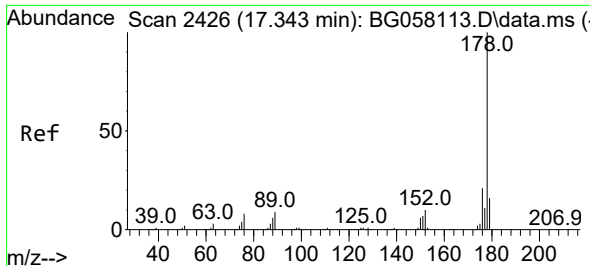

#72
Phenanthrene
Concen: 20.911 ng/ul
RT: 17.339 min Scan# 2425
Delta R.T. -0.002 min
Lab File: BG058117.D
Acq: 9 Jul 2023 8:28




Instrument :
BNA_G
ClientSampleId :
YBW01MS


Tgt Ion:178 Resp: 546325
Ion Ratio Lower Upper
178 100
179 15.5 12.8 19.2
176 20.3 15.7 23.5

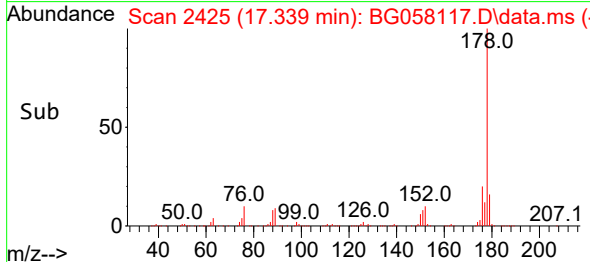

#74
Anthracene
Concen: 20.526 ng/ul
RT: 17.433 min Scan# 2441
Delta R.T. 0.004 min
Lab File: BG058117.D
Acq: 9 Jul 2023 8:28

Tgt Ion:178 Resp: 542681
Ion Ratio Lower Upper
178 100
179 16.2 12.6 18.8
176 19.7 15.4 23.2


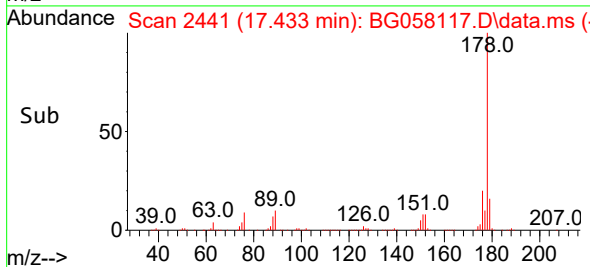

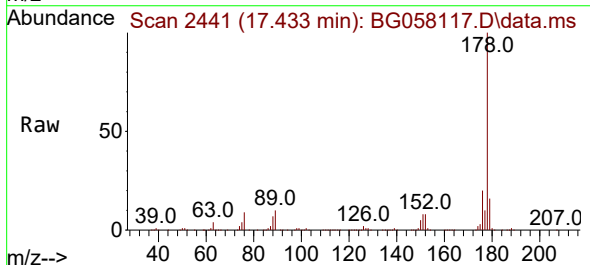




#75
1,2,3,4-Tetrachlorobenzene
Concen: 21.037 ng/uL
RT: 13.356 min Scan# 1
Delta R.T. 0.004 min
Lab File: BG058117.D
Acq: 9 Jul 2023 8:28




Instrument :
BNA_G
ClientSampleId :
YBW01MS


Tgt Ion:216 Resp: 143300
Ion Ratio Lower Upper
216 100
214 76.1 64.8 97.2
218 47.4 39.1 58.7



#76
Pentachlorobenzene
Concen: 48.152 ng/uL
RT: 14.872 min Scan# 2005
Delta R.T. -0.002 min
Lab File: BG058117.D
Acq: 9 Jul 2023 8:28

Tgt Ion:250 Resp: 350310
Ion Ratio Lower Upper
250 100
248 63.9 52.8 79.2
252 63.8 52.4 78.6





#77

Carbazole

Concen: 21.571 ng/ul

RT: 17.703 min Scan# 2487

Delta R.T. 0.004 min

Lab File: BG058117.D

Acq: 9 Jul 2023 8:28

Instrument :

BNA_G

ClientSampleId :

YBW01MS





Tgt Ion:167 Resp: 515787

Ion Ratio Lower Upper

167 100

166 23.0 17.5 26.3

139 12.3 9.5 14.3

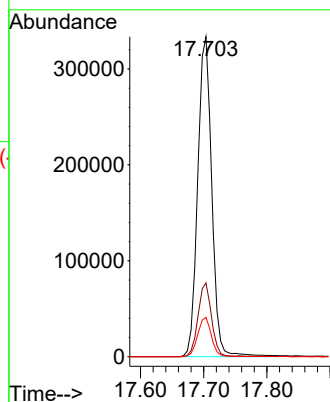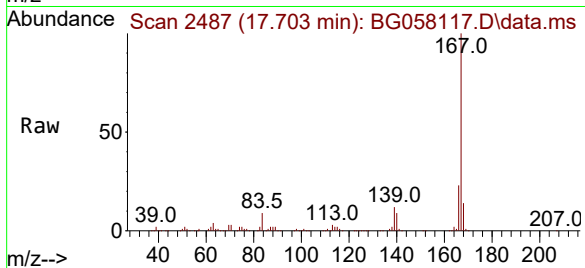

#78

Di-n-butylphthalate

Concen: 21.713 ng/ul

RT: 18.256 min Scan# 2581

Delta R.T. -0.002 min

Lab File: BG058117.D

Acq: 9 Jul 2023 8:28




Tgt Ion:149 Resp: 661370


Ion Ratio Lower Upper

149 100

150 9.2 7.4 11.2

104 4.8 3.9 5.9




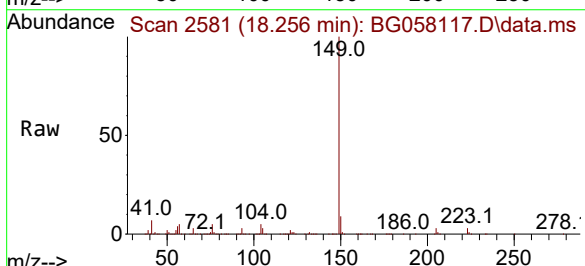


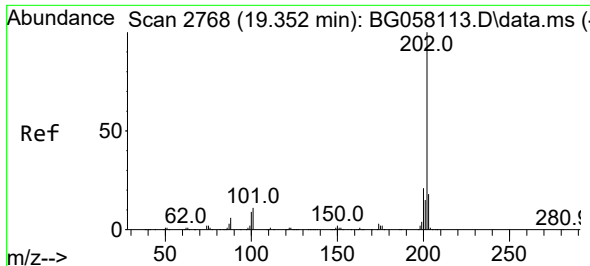

#80
Fluoranthene
Concen: 20.574 ng/ul
RT: 19.354 min Scan# 2768
Delta R.T. 0.004 min
Lab File: BG058117.D
Acq: 9 Jul 2023 8:28




Instrument :
BNA_G
ClientSampleId :
YBW01MS


Tgt Ion:202 Resp: 678357
Ion Ratio Lower Upper
202 100
101 10.6 9.1 13.7
100 8.3 7.1 10.7

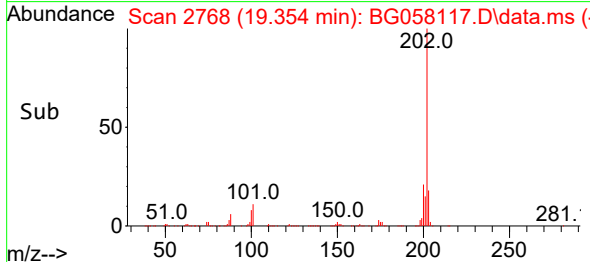

#82
Pyrene
Concen: 20.414 ng/ul
RT: 19.719 min Scan# 2830
Delta R.T. 0.004 min
Lab File: BG058117.D
Acq: 9 Jul 2023 8:28

Tgt Ion:202 Resp: 677530
Ion Ratio Lower Upper
202 100
101 12.6 10.2 15.2
100 10.2 8.9 13.3

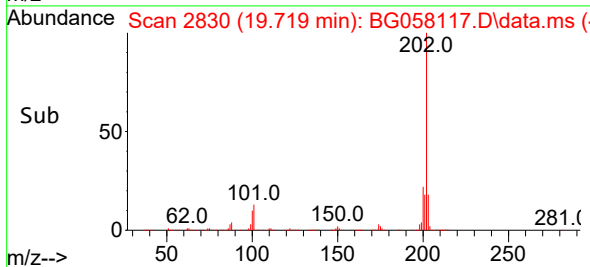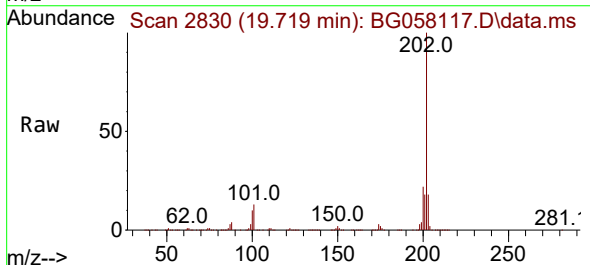



#83

Butylbenzylphthalate

Concen: 21.411 ng/ul

RT: 20.600 min Scan# 2980

Delta R.T. 0.004 min

Lab File: BG058117.D

Acq: 9 Jul 2023 8:28

Instrument :

BNA_G

ClientSampleId :

YBW01MS





Tgt Ion:149 Resp: 288154

Ion Ratio Lower Upper

149 100

91 70.3 56.5 84.7

206 22.3 17.4 26.0



#84

3,3'-Dichlorobenzidine

Concen: 23.062 ng/ul

RT: 21.452 min Scan# 3125

Delta R.T. 0.004 min

Lab File: BG058117.D

Acq: 9 Jul 2023 8:28




Tgt Ion:252 Resp: 252240


Ion Ratio Lower Upper

252 100

254 65.6 50.7 76.1

126 9.7 6.6 10.0







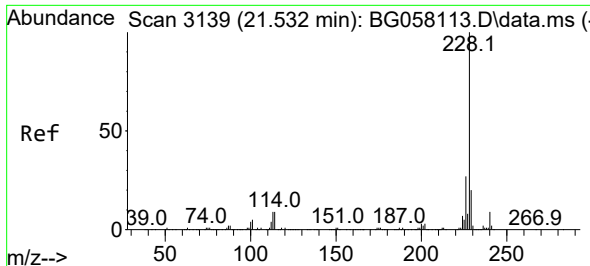

#85
Benzo(a)anthracene
Concen: 21.054 ng/ul
RT: 21.534 min Scan# 3139
Delta R.T. 0.004 min
Lab File: BG058117.D
Acq: 9 Jul 2023 8:28




Instrument :
BNA_G
ClientSampleId :
YBW01MS


Tgt Ion:228 Resp: 682986
Ion Ratio Lower Upper
228 100
229 20.3 16.0 24.0
226 27.9 22.0 33.0

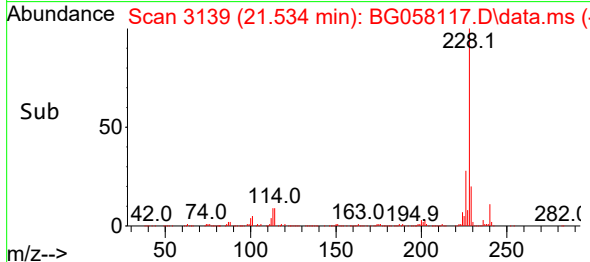

#86
Bis(2-ethylhexyl)phthalate
Concen: 21.634 ng/ul
RT: 21.434 min Scan# 3122
Delta R.T. -0.002 min
Lab File: BG058117.D
Acq: 9 Jul 2023 8:28

Tgt Ion:149 Resp: 417241
Ion Ratio Lower Upper
149 100
167 27.6 20.9 31.3
279 3.9 3.1 4.7

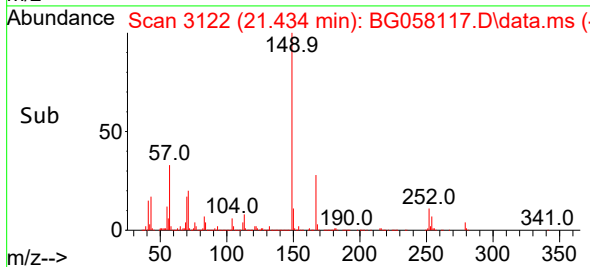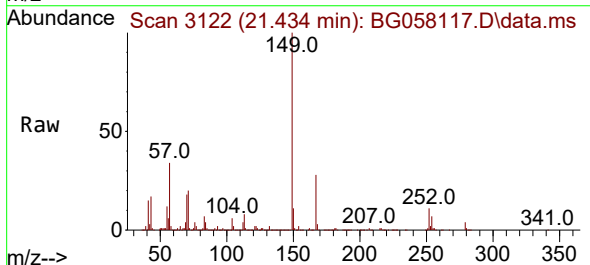



#87

Chrysene

Concen: 21.475 ng/ul

RT: 21.599 min Scan# 3150

Delta R.T. 0.004 min

Lab File: BG058117.D

Acq: 9 Jul 2023 8:28

Instrument :

BNA_G

ClientSampleId :

YBW01MS





Tgt Ion:228 Resp: 653052

Ion Ratio Lower Upper

228 100

226 31.1 24.4 36.6

229 20.4 15.5 23.3

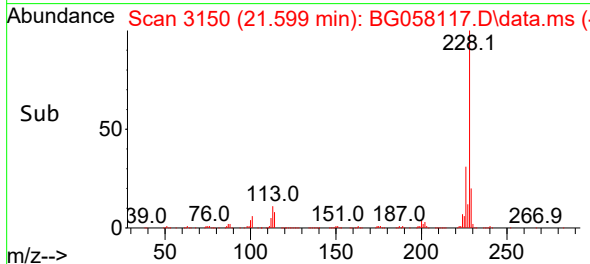

#89

Di-n-octyl phthalate

Concen: 20.974 ng/ul




RT: 22.621 min Scan# 3324


Delta R.T. 0.004 min

Lab File: BG058117.D

Acq: 9 Jul 2023 8:28

Tgt Ion:149 Resp: 738561


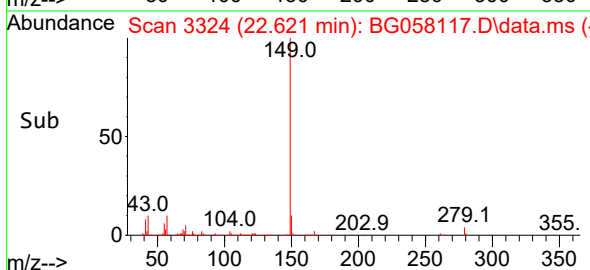

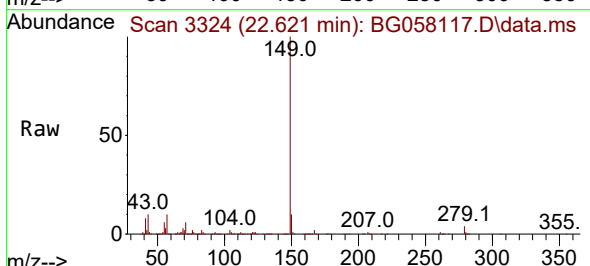




#90
Benzo(b)fluoranthene
Concen: 20.790 ng/ul
RT: 23.702 min Scan# 3508
Delta R.T. 0.004 min
Lab File: BG058117.D
Acq: 9 Jul 2023 8:28




Instrument :
BNA_G
ClientSampleId :
YBW01MS


Tgt Ion:252 Resp: 737754
Ion Ratio Lower Upper
252 100
253 21.6 18.1 27.1
125 8.7 7.5 11.3



#91
Benzo(k)fluoranthene
Concen: 20.517 ng/ul
RT: 23.767 min Scan# 3519
Delta R.T. 0.004 min
Lab File: BG058117.D
Acq: 9 Jul 2023 8:28

Tgt Ion:252 Resp: 713642
Ion Ratio Lower Upper
252 100
253 23.3 17.7 26.5
125 8.9 7.4 11.2









#93
Benzo(a)pyrene
Concen: 20.734 ng/ul
RT: 24.554 min Scan# 3653
Delta R.T. -0.002 min
Lab File: BG058117.D
Acq: 9 Jul 2023 8:28




Instrument :
BNA_G
ClientSampleId :
YBW01MS


Tgt Ion:252 Resp: 651240
Ion Ratio Lower Upper
252 100
253 22.7 17.8 26.6
125 10.9 8.3 12.5



#94
Indeno(1,2,3-cd)pyrene
Concen: 20.970 ng/ul
RT: 28.291 min Scan# 4289
Delta R.T. -0.002 min
Lab File: BG058117.D
Acq: 9 Jul 2023 8:28

Tgt Ion:276 Resp: 874601
Ion Ratio Lower Upper
276 100
138 16.2 14.0 21.0
277 24.2 19.4 29.2

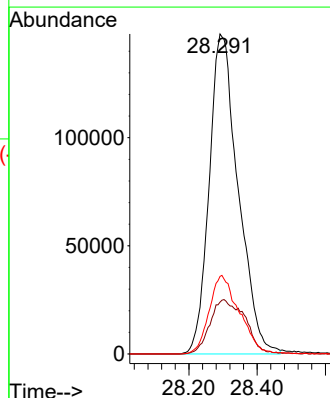



#95

Dibenzo(a,h)anthracene

Concen: 21.104 ng/ul

RT: 28.356 min Scan# 41

Delta R.T. -0.002 min

Lab File: BG058117.D

Acq: 9 Jul 2023 8:28

Instrument :

BNA_G

ClientSampleId :

YBW01MS





Tgt Ion:278 Resp: 725834

Ion Ratio Lower Upper

278 100

139 12.9 11.3 16.9

279 23.9 18.9 28.3

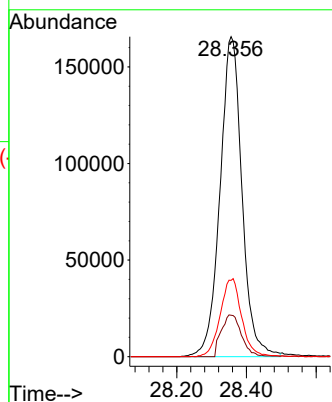

#96

Benzo(g,h,i)perylene

Concen: 20.919 ng/ul

RT: 29.425 min Scan# 4482

Delta R.T. 0.010 min

Lab File: BG058117.D

Acq: 9 Jul 2023 8:28

Tgt Ion:276 Resp: 712649

Ion Ratio Lower Upper

276 100

138 17.5 14.2 21.2

277 24.1 18.6 27.8

