

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070823\
 Data File : BG058118.D
 Acq On : 9 Jul 2023 9:09
 Operator : CG/JU
 Sample : 03349-08MSD
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 YBW01MSD

Quant Time: Jul 10 00:40:03 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 08 10:01:01 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.915	152	65296	20.000	ng/u1	0.00
20) Naphthalene-d8	10.717	136	301963	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.554	164	221412	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.298	188	543210	20.000	ng/u1	0.00
79) Chrysene-d12	21.557	240	471014	20.000	ng/u1	0.00
88) Perylene-d12	24.713	264	596148	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.355	96	4758	2.552	ng/uL	0.00
4) Pyridine-d5	3.761	84	73889	13.052	ng/u1	0.00
7) Phenol-d5	7.080	99	103364	15.501	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.239	67	60231	14.988	ng/u1	0.00
11) 2-Chlorophenol-d4	7.450	132	70432	15.314	ng/u1	0.00
15) 4-Methylphenol-d8	8.626	113	80396	15.978	ng/u1	0.00
21) Nitrobenzene-d5	9.078	128	38615	15.690	ng/u1	0.00
24) 2-Nitrophenol-d4	9.801	143	43378	16.770	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.341	165	82508	16.628	ng/u1	0.00
31) 4-Chloroaniline-d4	10.852	131	109591	14.567	ng/u1	0.00
46) Dimethylphthalate-d6	13.955	166	275987	15.798	ng/u1	0.00
49) Acenaphthylene-d8	14.248	160	305242	16.012	ng/u1	0.00
54) 4-Nitrophenol-d4	14.760	143	42789	13.863	ng/u1	0.00
60) Fluorene-d10	15.547	176	244787	16.499	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.664	200	41828	14.181	ng/u1	0.00
73) Anthracene-d10	17.398	188	395849	15.704	ng/u1	0.00
81) Pyrene-d10	19.683	212	471632	15.899	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.489	264	495907	16.328	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.390	88	16658	7.231	ng/uL	88
5) Pyridine	3.784	79	115915	19.984	ng/u1	97
6) Benzaldehyde	7.057	77	79991	35.919	ng/u1	96
8) Phenol	7.110	94	159050	23.504	ng/u1	99
10) Bis(2-Chloroethyl)ether	7.333	93	115814	22.166	ng/u1	97
12) 2-Chlorophenol	7.480	128	108012	22.569	ng/u1	96
13) 2-Methylphenol	8.361	108	121622	22.885	ng/u1	97
14) 2,2'-oxybis(1-Chloropr...	8.443	45	183034	22.758	ng/u1	98
16) Acetophenone	8.737	105	194471	23.295	ng/u1	100
17) N-Nitroso-di-n-propyla...	8.720	70	101007	22.633	ng/u1	97
18) 4-Methylphenol	8.690	108	137918	24.000	ng/u1	95
19) Hexachloroethane	8.996	117	39438	21.495	ng/u1	95
22) Nitrobenzene	9.119	77	143644	22.483	ng/u1	96
23) Isophorone	9.636	82	309599	22.710	ng/u1	99
25) 2-Nitrophenol	9.830	139	65705	23.673	ng/u1	93
26) 2,4-Dimethylphenol	9.889	107	135428	21.699	ng/u1	95
27) Bis(2-Chloroethoxy)met...	10.124	93	170485	22.192	ng/u1	100
29) 2,4-Dichlorophenol	10.365	162	116043	24.053	ng/u1	96
30) Naphthalene	10.770	128	382238	22.525	ng/u1	99
32) 4-Chloroaniline	10.876	127	139820	18.176	ng/u1	99
33) Hexachlorobutadiene	11.052	225	78113	22.870	ng/u1	97
34) Caprolactam	11.640	113	45870	23.649	ng/u1	94
35) 4-Chloro-3-methylphenol	12.010	107	150194	25.343	ng/u1	99
36) 2-Methylnaphthalene	12.380	142	263210	23.009	ng/u1	93


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070823\
 Data File : BG058118.D
 Acq On : 9 Jul 2023 9:09
 Operator : CG/JU
 Sample : 03349-08MSD
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 YBW01MSD

Quant Time: Jul 10 00:40:03 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 08 10:01:01 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.597	142	267426	23.313	ng/ul	96
39) 1,2,4,5-Tetrachloroben...	12.744	216	155579	23.058	ng/ul	97
40) Hexachlorocyclopentadiene	12.721	237	75713	17.815	ng/ul	97
41) 2,4,6-Trichlorophenol	12.985	196	108371	23.697	ng/ul	96
42) 2,4,5-Trichlorophenol	13.062	196	116303	23.516	ng/ul	99
43) 1,1'-Biphenyl	13.385	154	358451	22.465	ng/ul	100
44) 2-Chloronaphthalene	13.432	162	292145	22.814	ng/ul	99
45) 2-Nitroaniline	13.637	65	109164	24.518	ng/ul	95
47) Dimethylphthalate	14.007	163	395297	22.522	ng/ul	100
48) 2,6-Dinitrotoluene	14.131	165	87378	24.254	ng/ul	99
50) Acenaphthylene	14.278	152	471129	22.886	ng/ul	98
51) 3-Nitroaniline	14.460	138	84735	27.832	ng/ul	99
52) Acenaphthene	14.618	153	323397	22.893	ng/ul	98
53) 2,4-Dinitrophenol	14.666	184	45486	24.218	ng/ul	93
55) 4-Nitrophenol	14.771	109	53320	23.320	ng/ul	87
56) Dibenzofuran	14.953	168	462280	23.021	ng/ul	100
57) 2,4-Dinitrotoluene	14.918	165	125588	24.604	ng/ul	97
58) 2,3,4,6-Tetrachlorophenol	15.177	232	106231	23.595	ng/ul	97
59) Diethylphthalate	15.371	149	415662	22.691	ng/ul	99
61) Fluorene	15.600	166	377218	22.895	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.594	204	203333	23.323	ng/ul	99
63) 4-Nitroaniline	15.623	138	87951	32.248	ng/ul	96
66) 4,6-Dinitro-2-methylph...	15.682	198	73085	24.229	ng/ul	99
67) N-Nitrosodiphenylamine	15.805	169	327630	22.663	ng/ul	99
68) 4-Bromophenyl-phenylether	16.487	248	141557	23.740	ng/ul	98
69) Hexachlorobenzene	16.604	284	160664	24.066	ng/ul	99
70) Atrazine	16.751	200	105223	17.799	ng/ul	97
71) Pentachlorophenol	16.951	266	88507	22.083	ng/ul	93
72) Phenanthrene	17.345	178	623715	22.573	ng/ul	99
74) Anthracene	17.433	178	620274	22.183	ng/ul	98
75) 1,2,3,4-Tetrachloroben...	13.355	216	165640	22.992	ng/ul	98
76) Pentachlorobenzene	14.871	250	402845	52.357	ng/ul	97
77) Carbazole	17.703	167	576851	22.811	ng/ul	99
78) Di-n-butylphthalate	18.255	149	750385	23.294	ng/ul	99
80) Fluoranthene	19.354	202	762968	22.196	ng/ul	99
82) Pyrene	19.718	202	763573	22.068	ng/ul	99
83) Butylbenzylphthalate	20.600	149	326085	23.241	ng/ul	99
84) 3,3'-Dichlorobenzidine	21.452	252	284854	24.981	ng/ul	99
85) Benzo(a)anthracene	21.534	228	771715	22.819	ng/ul	100
86) Bis(2-ethylhexyl)phtha...	21.434	149	472995	23.524	ng/ul	98
87) Chrysene	21.599	228	739282	23.319	ng/ul	98
89) Di-n-octyl phthalate	22.621	149	836195	22.829	ng/ul	100
90) Benzo(b)fluoranthene	23.708	252	828426	22.443	ng/ul	98
91) Benzo(k)fluoranthene	23.772	252	808823	22.355	ng/ul	100
93) Benzo(a)pyrene	24.560	252	737641	22.578	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	28.297	276	988679	22.789	ng/ul	98
95) Dibenzo(a,h)anthracene	28.361	278	823860	23.029	ng/ul	98
96) Benzo(g,h,i)perylene	29.431	276	802631	22.650	ng/ul	98





(#) = qualifier out of range (m) = manual integration (+) = signals summed



#2
1,4-Dioxane
Concen: 7.231 ng/uL
RT: 3.390 min Scan# 51
Delta R.T. -0.003 min
Lab File: BG058118.D
Acq: 9 Jul 2023 9:09




Instrument :
BNA_G
ClientSampleId :
YBW01MSD


Tgt Ion:	88	Resp:	16658
Ion	Ratio	Lower	Upper
88	100		
43	29.8	20.6	30.8
58	94.1	65.5	98.3



#5
Pyridine
Concen: 19.984 ng/uL
RT: 3.784 min Scan# 118
Delta R.T. -0.003 min
Lab File: BG058118.D
Acq: 9 Jul 2023 9:09

Tgt Ion:	79	Resp:	115915
Ion	Ratio	Lower	Upper
79	100		
52	82.9	68.6	102.8
51	38.6	29.4	44.0





#6

Benzaldehyde

Concen: 35.919 ng/ul

RT: 7.057 min Scan# 61

Delta R.T. -0.003 min

Lab File: BG058118.D

Acq: 9 Jul 2023 9:09

Instrument :

BNA_G

ClientSampleId :

YBW01MSD





Tgt Ion: 77 Resp: 79991

Ion Ratio Lower Upper

77 100

105 100.4 74.7 112.1

106 95.0 75.9 113.9

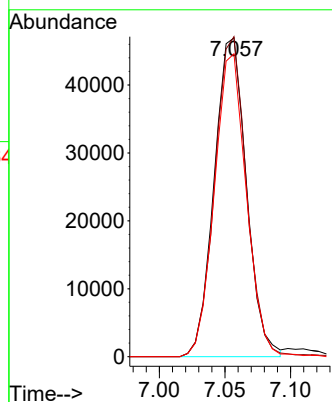

#8

Phenol

Concen: 23.504 ng/ul

RT: 7.110 min Scan# 684

Delta R.T. 0.003 min

Lab File: BG058118.D

Acq: 9 Jul 2023 9:09




Tgt Ion: 94 Resp: 159050


Ion Ratio Lower Upper

94 100

65 29.1 22.2 33.4

66 36.0 28.6 43.0









#10
Bis(2-Chloroethyl)ether
Concen: 22.166 ng/ul
RT: 7.333 min Scan# 71
Delta R.T. -0.003 min
Lab File: BG058118.D
Acq: 9 Jul 2023 9:09




Instrument :
BNA_G
ClientSampleId :
YBW01MSD


Tgt Ion: 93 Resp: 115814
Ion Ratio Lower Upper
93 100
63 83.7 69.4 104.0
95 32.1 27.0 40.6

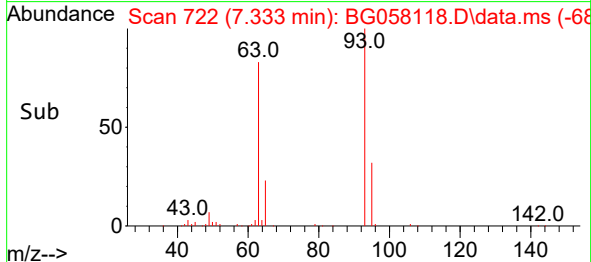

#12
2-Chlorophenol
Concen: 22.569 ng/ul
RT: 7.480 min Scan# 747
Delta R.T. -0.003 min
Lab File: BG058118.D
Acq: 9 Jul 2023 9:09

Tgt Ion:128 Resp: 108012
Ion Ratio Lower Upper
128 100
64 59.1 44.3 66.5
130 33.2 27.3 40.9


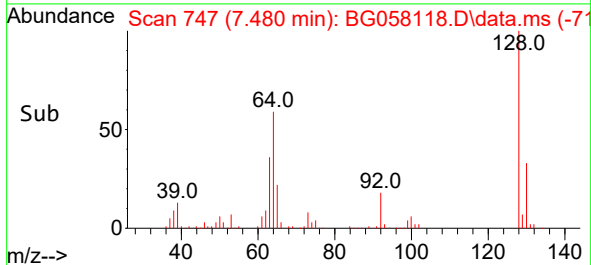






#13
2-Methylphenol
Concen: 22.885 ng/ul
RT: 8.361 min Scan# 897
Delta R.T. 0.003 min
Lab File: BG058118.D
Acq: 9 Jul 2023 9:09




Instrument :
BNA_G
ClientSampleId :
YBW01MSD


Tgt Ion:108 Resp: 121622
Ion Ratio Lower Upper
108 100
107 90.4 75.0 112.4

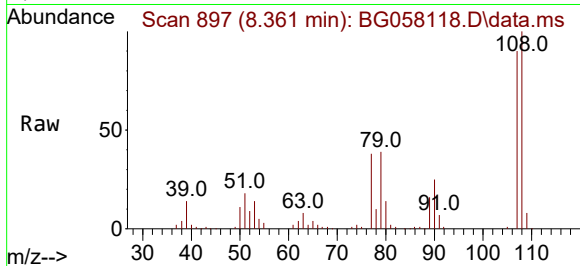

#14
2,2'-oxybis(1-Chloropropane)
Concen: 22.758 ng/ul
RT: 8.443 min Scan# 911
Delta R.T. 0.003 min
Lab File: BG058118.D
Acq: 9 Jul 2023 9:09

Tgt Ion: 45 Resp: 183034
Ion Ratio Lower Upper
45 100
77 12.6 9.4 14.2
79 9.9 8.3 12.5




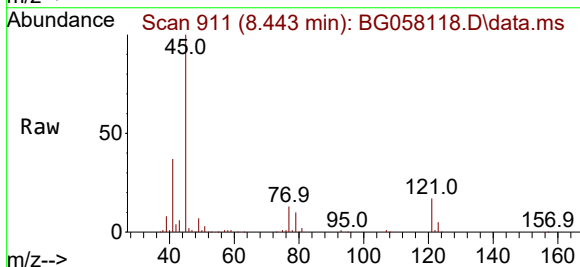




#16
Acetophenone
Concen: 23.295 ng/ul
RT: 8.737 min Scan# 961
Delta R.T. -0.003 min
Lab File: BG058118.D
Acq: 9 Jul 2023 9:09




Instrument :
BNA_G
ClientSampleId :
YBW01MSD


Tgt Ion:105 Resp: 194471
Ion Ratio Lower Upper
105 100
77 76.8 61.2 91.8
51 29.2 23.5 35.3

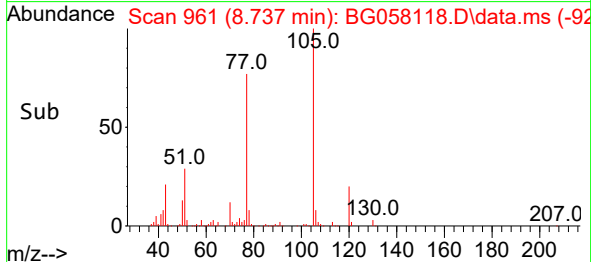

#17
N-Nitroso-di-n-propylamine
Concen: 22.633 ng/ul
RT: 8.720 min Scan# 958
Delta R.T. 0.003 min
Lab File: BG058118.D
Acq: 9 Jul 2023 9:09

Tgt Ion: 70 Resp: 101007
Ion Ratio Lower Upper
70 100
42 57.7 48.0 72.0
101 9.0 7.4 11.2
130 19.0 13.4 20.0









#18
4-Methylphenol
Concen: 24.000 ng/ul
RT: 8.690 min Scan# 91
Delta R.T. 0.003 min
Lab File: BG058118.D
Acq: 9 Jul 2023 9:09




Instrument :
BNA_G
ClientSampleId :
YBW01MSD


Tgt Ion:108 Resp: 137918
Ion Ratio Lower Upper
108 100
107 108.3 91.1 136.7

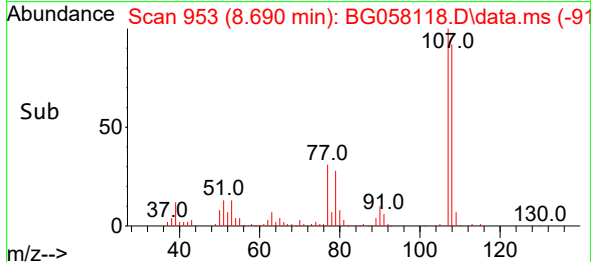

#19
Hexachloroethane
Concen: 21.495 ng/ul
RT: 8.996 min Scan# 1005
Delta R.T. -0.003 min
Lab File: BG058118.D
Acq: 9 Jul 2023 9:09

Tgt Ion:117 Resp: 39438
Ion Ratio Lower Upper
117 100
201 124.1 94.0 141.0
199 77.8 59.8 89.6

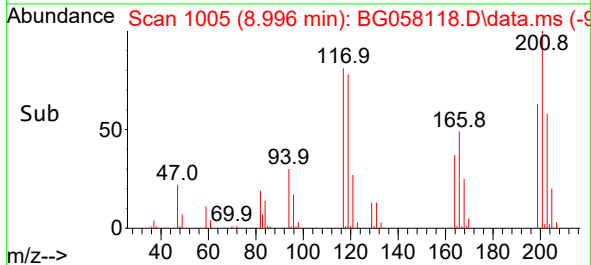



#22

Nitrobenzene

Concen: 22.483 ng/ul

RT: 9.119 min Scan# 1026

Delta R.T. -0.003 min

Lab File: BG058118.D

Acq: 9 Jul 2023 9:09

Instrument :

BNA_G

ClientSampleId :

YBW01MSD





Tgt Ion: 77 Resp: 143644

Ion Ratio Lower Upper

77 100

123 43.8 33.3 49.9

65 15.2 10.4 15.6



#23

Isophorone

Concen: 22.710 ng/ul

RT: 9.636 min Scan# 1114

Delta R.T. -0.003 min

Lab File: BG058118.D

Acq: 9 Jul 2023 9:09




Tgt Ion: 82 Resp: 309599


Ion Ratio Lower Upper

82 100

95 6.3 4.8 7.2

138 14.6 11.4 17.0









#25
2-Nitrophenol
Concen: 23.673 ng/ul
RT: 9.830 min Scan# 1148
Delta R.T. -0.003 min
Lab File: BG058118.D
Acq: 9 Jul 2023 9:09




Instrument :
BNA_G
ClientSampleId :
YBW01MSD


Tgt Ion:139 Resp: 65705
Ion Ratio Lower Upper
139 100
65 57.8 42.6 64.0
109 30.3 20.7 31.1



#26
2,4-Dimethylphenol
Concen: 21.699 ng/ul
RT: 9.889 min Scan# 1157
Delta R.T. -0.003 min
Lab File: BG058118.D
Acq: 9 Jul 2023 9:09

Tgt Ion:107 Resp: 135428
Ion Ratio Lower Upper
107 100
121 47.2 40.6 60.8
122 78.9 67.1 100.7

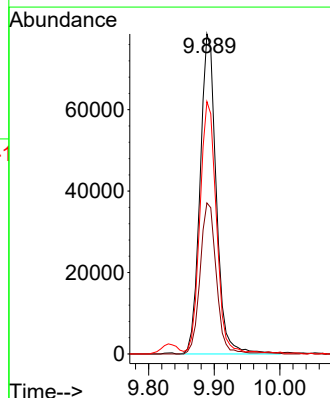







#27
 Bis(2-Chloroethoxy)methane
 Concen: 22.192 ng/ul
 RT: 10.124 min Scan# 1197
 Delta R.T. -0.003 min
 Lab File: BG058118.D
 Acq: 9 Jul 2023 9:09

Instrument :
 BNA_G
 ClientSampleId :
 YBW01MSD

Tgt Ion: 93 Resp: 170485




Ion	Ratio	Lower	Upper
93	100		
95	32.8	26.4	39.6
123	10.0	7.9	11.9




#29
 2,4-Dichlorophenol
 Concen: 24.053 ng/ul
 RT: 10.365 min Scan# 1238
 Delta R.T. -0.003 min
 Lab File: BG058118.D
 Acq: 9 Jul 2023 9:09

Tgt Ion: 162 Resp: 116043


Ion	Ratio	Lower	Upper
162	100		
164	67.2	51.1	76.7
98	37.3	27.9	41.9








#30
Naphthalene
Concen: 22.525 ng/ul
RT: 10.770 min Scan# 11
Delta R.T. -0.003 min
Lab File: BG058118.D
Acq: 9 Jul 2023 9:09

Instrument :
BNA_G
ClientSampleId :
YBW01MSD







Tgt Ion:128 Resp: 382238
Ion Ratio Lower Upper
128 100
129 11.3 8.6 12.8
127 13.2 10.2 15.2

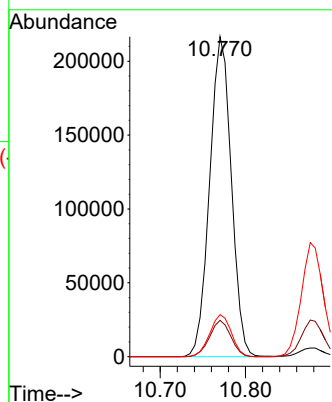

#32
4-Chloroaniline
Concen: 18.176 ng/ul
RT: 10.876 min Scan# 1325
Delta R.T. -0.003 min
Lab File: BG058118.D
Acq: 9 Jul 2023 9:09

Tgt Ion:127 Resp: 139820
Ion Ratio Lower Upper
127 100
129 32.2 26.0 39.0









#33
Hexachlorobutadiene
Concen: 22.870 ng/ul
RT: 11.052 min Scan# 11
Delta R.T. -0.003 min
Lab File: BG058118.D
Acq: 9 Jul 2023 9:09




Instrument :
BNA_G
ClientSampleId :
YBW01MSD


Tgt Ion:225 Resp: 78113
Ion Ratio Lower Upper
225 100
223 62.9 53.2 79.8
227 62.8 51.4 77.2

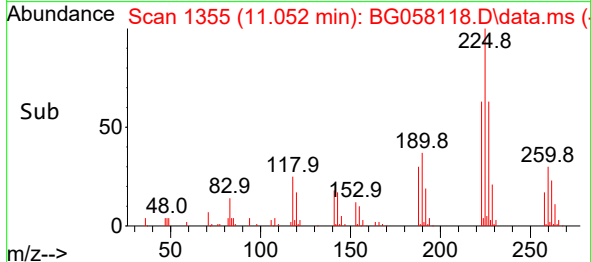

#34
Caprolactam
Concen: 23.649 ng/ul
RT: 11.640 min Scan# 1455
Delta R.T. 0.015 min
Lab File: BG058118.D
Acq: 9 Jul 2023 9:09

Tgt Ion:113 Resp: 45870
Ion Ratio Lower Upper
113 100
55 228.6 183.4 275.2
56 172.4 123.0 184.6




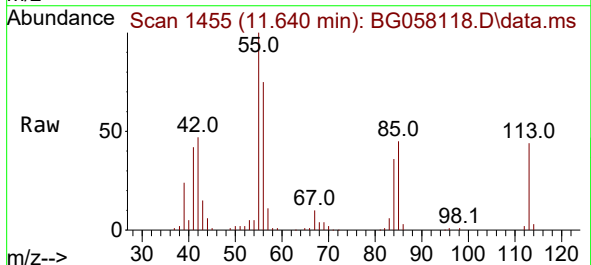




#35
 4-Chloro-3-methylphenol
 Concen: 25.343 ng/ul
 RT: 12.010 min Scan# 1518
 Delta R.T. 0.003 min
 Lab File: BG058118.D
 Acq: 9 Jul 2023 9:09




Instrument :
 BNA_G
 ClientSampleId :
 YBW01MSD


Tgt Ion:107 Resp: 150194
 Ion Ratio Lower Upper
 107 100
 144 23.2 19.0 28.4
 142 74.1 58.4 87.6

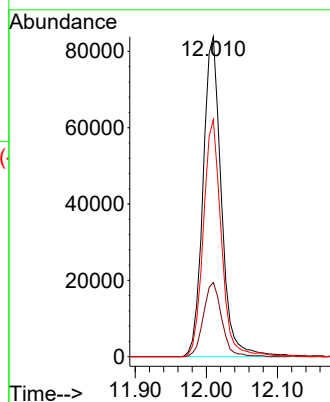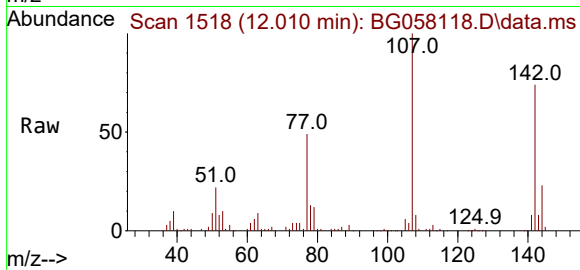

#36
 2-Methylnaphthalene
 Concen: 23.009 ng/ul
 RT: 12.380 min Scan# 1581
 Delta R.T. 0.003 min
 Lab File: BG058118.D
 Acq: 9 Jul 2023 9:09

Tgt Ion:142 Resp: 263210
 Ion Ratio Lower Upper
 142 100
 141 93.0 69.4 104.2



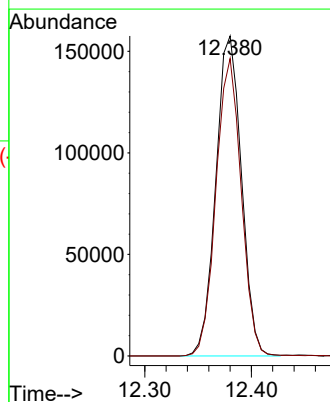
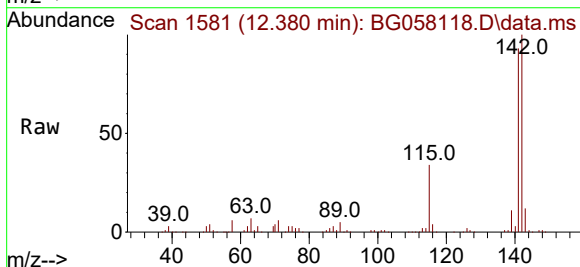


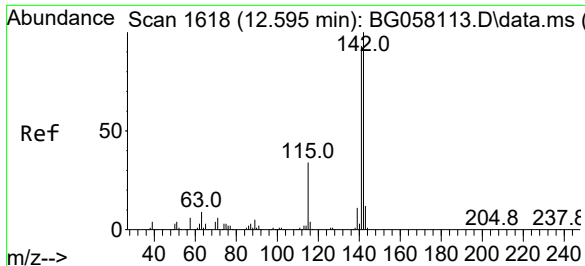

#37
1-Methylnaphthalene
Concen: 23.313 ng/ul
RT: 12.597 min Scan# 1618
Delta R.T. -0.003 min
Lab File: BG058118.D
Acq: 9 Jul 2023 9:09




Instrument :
BNA_G
ClientSampleId :
YBW01MSD


Tgt Ion:142 Resp: 267426
Ion Ratio Lower Upper
142 100
141 96.5 73.8 110.8
116 3.8 3.0 4.4

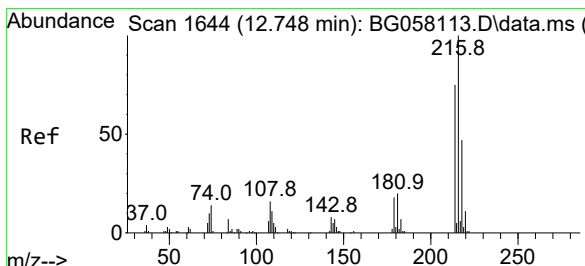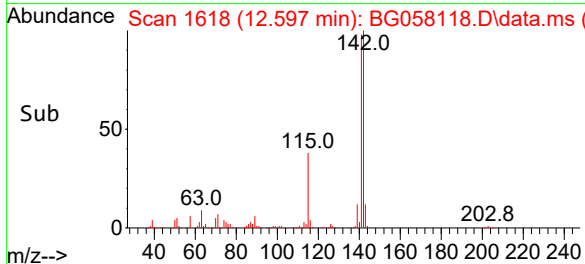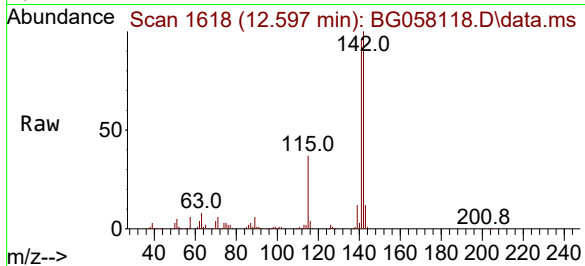

#39
1,2,4,5-Tetrachlorobenzene
Concen: 23.058 ng/ul
RT: 12.744 min Scan# 1643
Delta R.T. -0.003 min
Lab File: BG058118.D
Acq: 9 Jul 2023 9:09


Tgt Ion:216 Resp: 155579
Ion Ratio Lower Upper
216 100
214 76.2 64.1 96.1
179 19.8 16.0 24.0
108 14.9 12.1 18.1

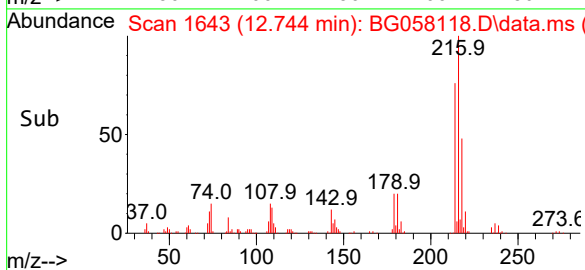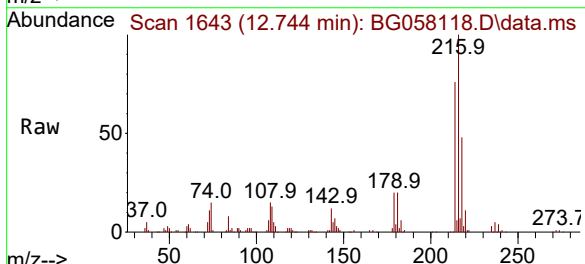






#40
Hexachlorocyclopentadiene
Concen: 17.815 ng/ul
RT: 12.721 min Scan# 1639
Delta R.T. -0.003 min
Lab File: BG058118.D
Acq: 9 Jul 2023 9:09

Instrument :
BNA_G
ClientSampleId :
YBW01MSD







Tgt Ion:237 Resp: 75713
Ion Ratio Lower Upper
237 100
235 64.2 49.2 73.8
272 14.1 10.4 15.6



#41
2,4,6-Trichlorophenol
Concen: 23.697 ng/ul
RT: 12.985 min Scan# 1684
Delta R.T. -0.003 min
Lab File: BG058118.D
Acq: 9 Jul 2023 9:09

Tgt Ion:196 Resp: 108371
Ion Ratio Lower Upper
196 100
198 96.5 73.5 110.3
200 31.1 24.8 37.2









#42
2,4,5-Trichlorophenol
Concen: 23.516 ng/ul
RT: 13.062 min Scan# 1
Delta R.T. -0.003 min
Lab File: BG058118.D
Acq: 9 Jul 2023 9:09




Instrument :
BNA_G
ClientSampleId :
YBW01MSD


Tgt Ion:196 Resp: 116303
Ion Ratio Lower Upper
196 100
198 97.3 77.2 115.8
200 31.3 23.8 35.6



#43
1,1'-Biphenyl
Concen: 22.465 ng/ul
RT: 13.385 min Scan# 1752
Delta R.T. -0.003 min
Lab File: BG058118.D
Acq: 9 Jul 2023 9:09

Tgt Ion:154 Resp: 358451
Ion Ratio Lower Upper
154 100
153 40.8 32.6 49.0
76 14.6 11.6 17.4









#44
2-Chloronaphthalene
Concen: 22.814 ng/ul
RT: 13.432 min Scan# 1760
Delta R.T. 0.003 min
Lab File: BG058118.D
Acq: 9 Jul 2023 9:09




Instrument :
BNA_G
ClientSampleId :
YBW01MSD


Tgt Ion:162 Resp: 292145
Ion Ratio Lower Upper
162 100
164 34.8 27.7 41.5
127 38.2 30.9 46.3

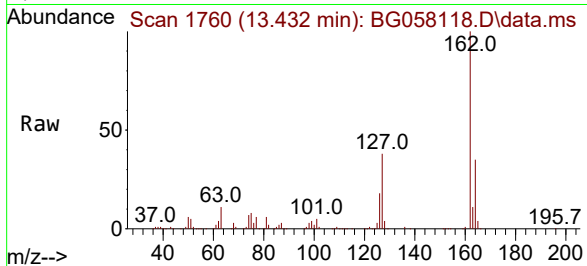

#45
2-Nitroaniline
Concen: 24.518 ng/ul
RT: 13.637 min Scan# 1795
Delta R.T. 0.003 min
Lab File: BG058118.D
Acq: 9 Jul 2023 9:09

Tgt Ion: 65 Resp: 109164
Ion Ratio Lower Upper
65 100
92 65.5 53.2 79.8
138 96.0 71.1 106.7




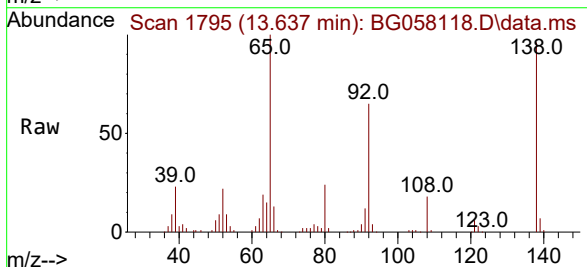


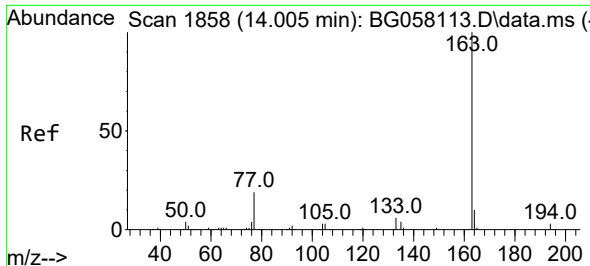

#47
Dimethylphthalate
Concen: 22.522 ng/ul
RT: 14.007 min Scan# 1858
Delta R.T. 0.003 min
Lab File: BG058118.D
Acq: 9 Jul 2023 9:09




Instrument :
BNA_G
ClientSampleId :
YBW01MSD


Tgt Ion:163 Resp: 395297
Ion Ratio Lower Upper
163 100
194 3.6 3.0 4.4
164 10.7 8.6 12.8

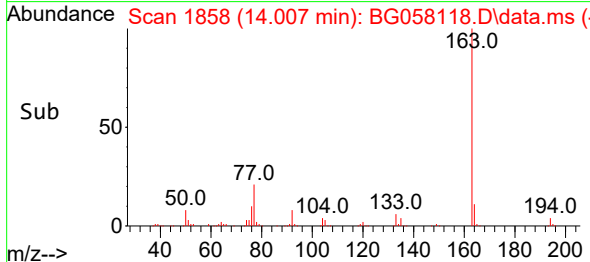

#48
2,6-Dinitrotoluene
Concen: 24.254 ng/ul
RT: 14.131 min Scan# 1879
Delta R.T. 0.003 min
Lab File: BG058118.D
Acq: 9 Jul 2023 9:09

Tgt Ion:165 Resp: 87378
Ion Ratio Lower Upper
165 100
89 54.1 42.7 64.1
121 18.8 14.8 22.2


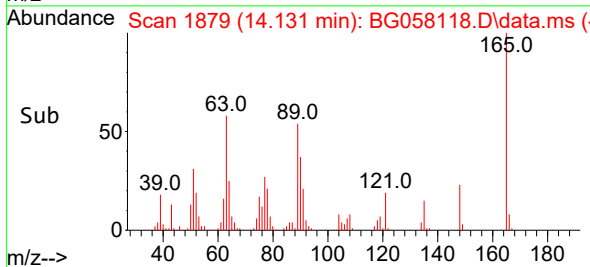

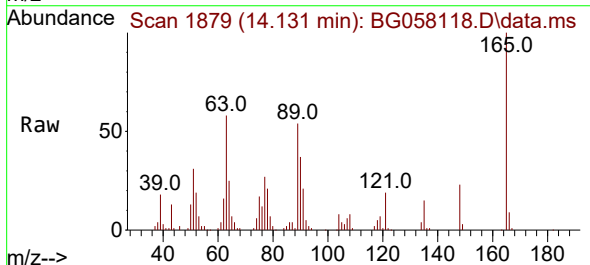




#50
Acenaphthylene
Concen: 22.886 ng/ul
RT: 14.278 min Scan# 1904
Delta R.T. 0.003 min
Lab File: BG058118.D
Acq: 9 Jul 2023 9:09




Instrument :
BNA_G
ClientSampleId :
YBW01MSD


Tgt Ion:152 Resp: 471129
Ion Ratio Lower Upper
152 100
151 20.6 15.6 23.4
153 13.3 10.5 15.7

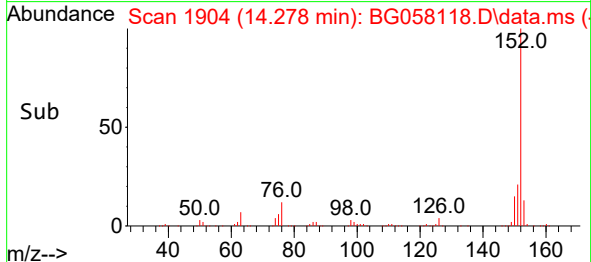

#51
3-Nitroaniline
Concen: 27.832 ng/ul
RT: 14.460 min Scan# 1935
Delta R.T. 0.003 min
Lab File: BG058118.D
Acq: 9 Jul 2023 9:09

Tgt Ion:138 Resp: 84735
Ion Ratio Lower Upper
138 100
108 10.3 8.2 12.2
92 126.4 100.2 150.4


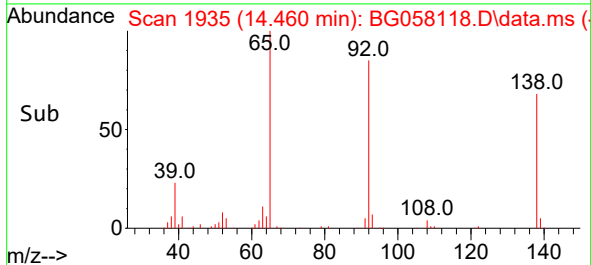






#52
Acenaphthene
Concen: 22.893 ng/ul
RT: 14.618 min Scan# 1962
Delta R.T. 0.003 min
Lab File: BG058118.D
Acq: 9 Jul 2023 9:09




Instrument :
BNA_G
ClientSampleId :
YBW01MSD


Tgt Ion:153 Resp: 323397
Ion Ratio Lower Upper
153 100
152 48.9 36.5 54.7
154 87.3 70.5 105.7



#53
2,4-Dinitrophenol
Concen: 24.218 ng/ul
RT: 14.666 min Scan# 1970
Delta R.T. 0.003 min
Lab File: BG058118.D
Acq: 9 Jul 2023 9:09

Tgt Ion:184 Resp: 45486
Ion Ratio Lower Upper
184 100
63 68.8 51.1 76.7
154 59.1 43.3 64.9









#55
4-Nitrophenol
Concen: 23.320 ng/ul
RT: 14.771 min Scan# 1988
Delta R.T. 0.003 min
Lab File: BG058118.D
Acq: 9 Jul 2023 9:09




Instrument :
BNA_G
ClientSampleId :
YBW01MSD


Tgt Ion:109 Resp: 53320
Ion Ratio Lower Upper
109 100
139 135.2 119.0 178.4
65 148.1 135.5 203.3

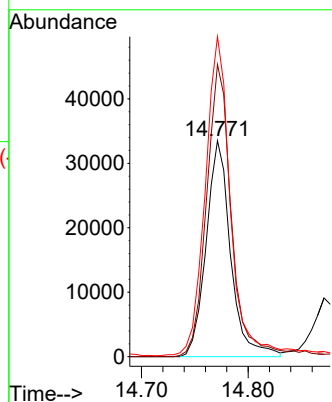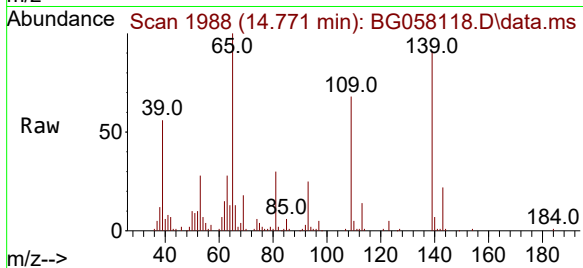

#56
Dibenzofuran
Concen: 23.021 ng/ul
RT: 14.953 min Scan# 2019
Delta R.T. 0.003 min
Lab File: BG058118.D
Acq: 9 Jul 2023 9:09

Tgt Ion:168 Resp: 462280
Ion Ratio Lower Upper
168 100
139 34.7 27.6 41.4



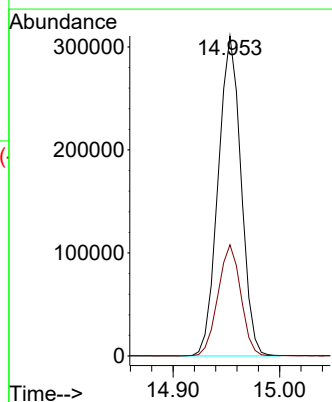
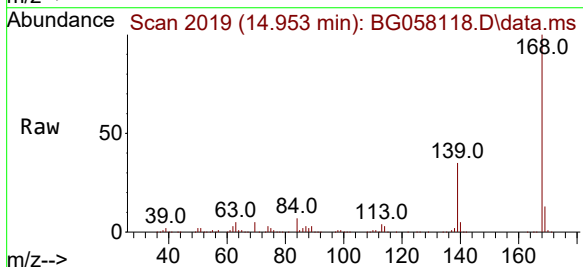




#57
2,4-Dinitrotoluene
Concen: 24.604 ng/ul
RT: 14.918 min Scan# 2013
Delta R.T. 0.003 min
Lab File: BG058118.D
Acq: 9 Jul 2023 9:09




Instrument :
BNA_G
ClientSampleId :
YBW01MSD


Tgt Ion:165 Resp: 125588
Ion Ratio Lower Upper
165 100
63 42.7 35.8 53.8
182 2.0 1.6 2.4

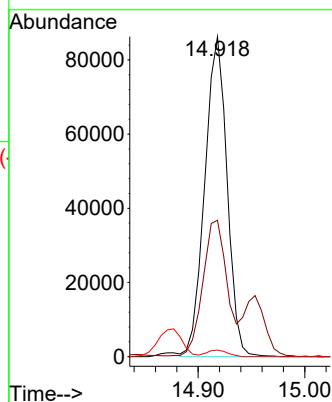

#58
2,3,4,6-Tetrachlorophenol
Concen: 23.595 ng/ul
RT: 15.177 min Scan# 2057
Delta R.T. -0.003 min
Lab File: BG058118.D
Acq: 9 Jul 2023 9:09

Tgt Ion:232 Resp: 106231
Ion Ratio Lower Upper
232 100
131 40.3 30.5 45.7
130 1.9 1.4 2.0
166 29.1 22.6 34.0









#59
Diethylphthalate
Concen: 22.691 ng/ul
RT: 15.371 min Scan# 2090
Delta R.T. 0.003 min
Lab File: BG058118.D
Acq: 9 Jul 2023 9:09




Instrument :
BNA_G
ClientSampleId :
YBW01MSD


Tgt Ion:149 Resp: 415662
Ion Ratio Lower Upper
149 100
177 22.0 17.8 26.8
150 12.1 10.1 15.1

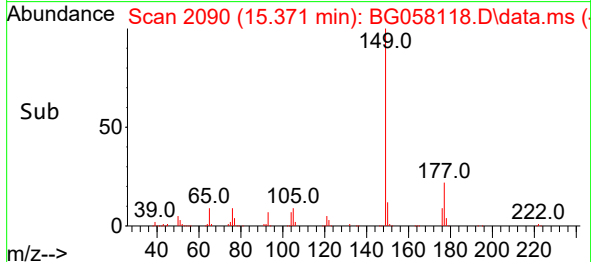

#61
Fluorene
Concen: 22.895 ng/ul
RT: 15.600 min Scan# 2129
Delta R.T. -0.003 min
Lab File: BG058118.D
Acq: 9 Jul 2023 9:09

Tgt Ion:166 Resp: 377218
Ion Ratio Lower Upper
166 100
165 99.9 79.1 118.7
167 13.2 10.7 16.1

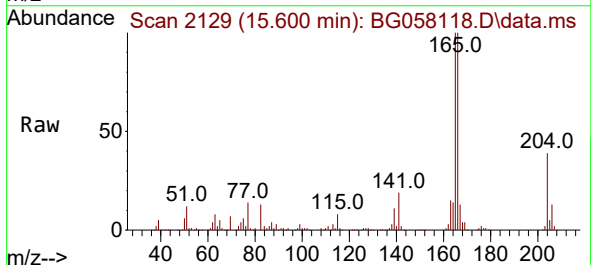



#62

4-Chlorophenyl-phenylether

Concen: 23.323 ng/ul

RT: 15.594 min Scan# 2128

Delta R.T. 0.003 min

Lab File: BG058118.D

Acq: 9 Jul 2023 9:09

Instrument :

BNA_G

ClientSampleId :

YBW01MSD





Tgt Ion:204 Resp: 203333

Ion Ratio Lower Upper

204 100

206 32.1 25.8 38.6

141 51.0 41.8 62.6



#63

4-Nitroaniline

Concen: 32.248 ng/ul

RT: 15.623 min Scan# 2133

Delta R.T. 0.009 min

Lab File: BG058118.D

Acq: 9 Jul 2023 9:09




Tgt Ion:138 Resp: 87951


Ion Ratio Lower Upper

138 100

92 55.9 43.8 65.8

108 78.8 58.8 88.2









#66
4,6-Dinitro-2-methylphenol
Concen: 24.229 ng/ul
RT: 15.682 min Scan# 2143
Delta R.T. 0.003 min
Lab File: BG058118.D
Acq: 9 Jul 2023 9:09




Instrument :
BNA_G
ClientSampleId :
YBW01MSD


Tgt Ion:198 Resp: 73085
Ion Ratio Lower Upper
198 100
182 3.7 3.1 4.7
77 22.1 17.9 26.9



#67
N-Nitrosodiphenylamine
Concen: 22.663 ng/ul
RT: 15.805 min Scan# 2164
Delta R.T. -0.003 min
Lab File: BG058118.D
Acq: 9 Jul 2023 9:09

Tgt Ion:169 Resp: 327630
Ion Ratio Lower Upper
169 100
168 69.2 54.2 81.2
167 38.9 30.8 46.2




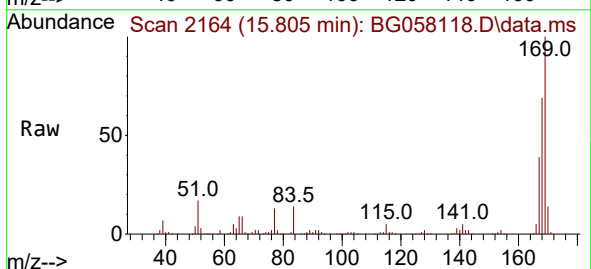




#68
4-Bromophenyl-phenylether
Concen: 23.740 ng/ul
RT: 16.487 min Scan# 21
Delta R.T. -0.003 min
Lab File: BG058118.D
Acq: 9 Jul 2023 9:09




Instrument :
BNA_G
ClientSampleId :
YBW01MSD


Tgt Ion:248 Resp: 141557
Ion Ratio Lower Upper
248 100
250 96.9 78.3 117.5
141 59.0 49.1 73.7

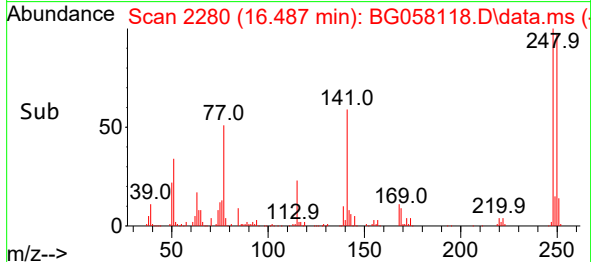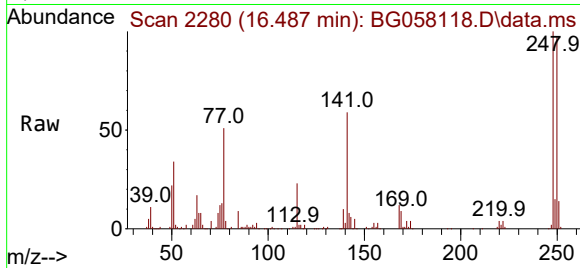

#69
Hexachlorobenzene
Concen: 24.066 ng/ul
RT: 16.604 min Scan# 2300
Delta R.T. 0.003 min
Lab File: BG058118.D
Acq: 9 Jul 2023 9:09

Tgt Ion:284 Resp: 160664
Ion Ratio Lower Upper
284 100
142 26.4 21.9 32.9
249 31.7 25.0 37.6

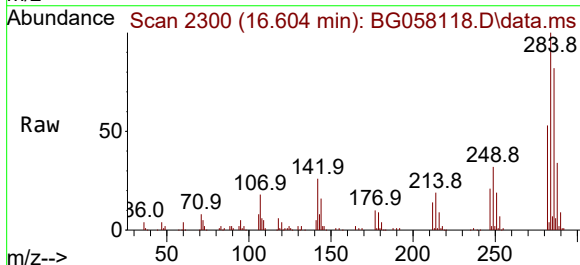



#70

Atrazine

Concen: 17.799 ng/ul

RT: 16.751 min Scan# 21

Delta R.T. -0.003 min

Lab File: BG058118.D

Acq: 9 Jul 2023 9:09

Instrument :

BNA_G

ClientSampleId :

YBW01MSD





Tgt Ion:200 Resp: 105223

Ion Ratio Lower Upper

200 100

173 25.6 20.0 30.0

215 47.7 35.8 53.8



#71

Pentachlorophenol

Concen: 22.083 ng/ul

RT: 16.951 min Scan# 2359

Delta R.T. 0.003 min

Lab File: BG058118.D

Acq: 9 Jul 2023 9:09




Tgt Ion:266 Resp: 88507


Ion Ratio Lower Upper

266 100

264 64.0 51.5 77.3

268 71.7 49.0 73.4





#72

Phenanthrene

Concen: 22.573 ng/ul

RT: 17.345 min Scan# 2426

Delta R.T. 0.003 min

Lab File: BG058118.D

Acq: 9 Jul 2023 9:09

Instrument :

BNA_G

ClientSampleId :

YBW01MSD





Tgt Ion:178 Resp: 623715

Ion Ratio Lower Upper

178 100

179 16.3 12.8 19.2

176 20.2 15.7 23.5

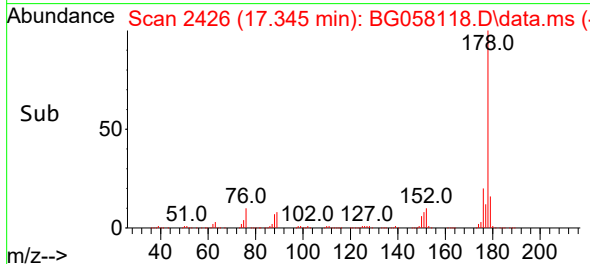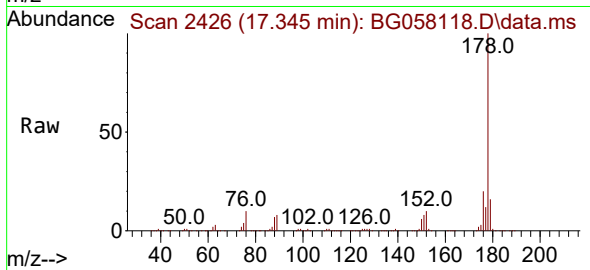

#74

Anthracene

Concen: 22.183 ng/ul

RT: 17.433 min Scan# 2441

Delta R.T. 0.003 min

Lab File: BG058118.D

Acq: 9 Jul 2023 9:09




Tgt Ion:178 Resp: 620274


Ion Ratio Lower Upper

178 100

179 17.0 12.6 18.8

176 19.7 15.4 23.2


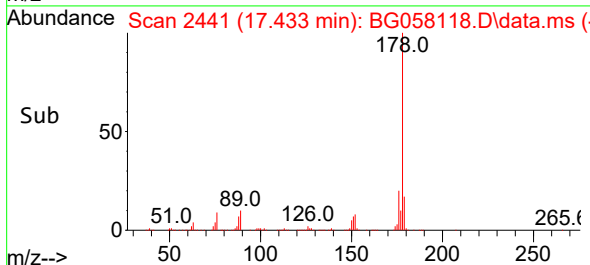
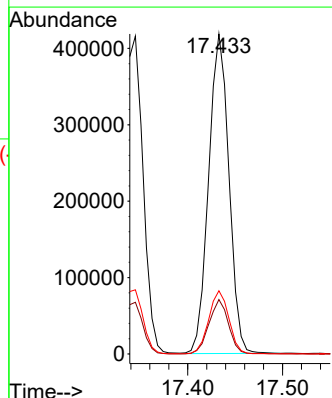
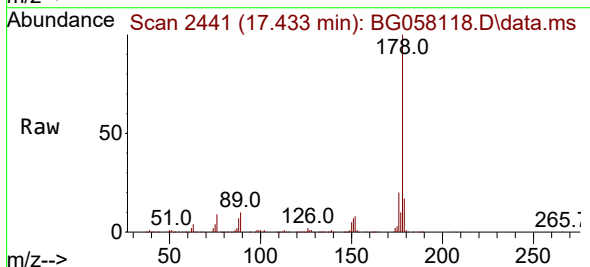




#75
1,2,3,4-Tetrachlorobenzene
Concen: 22.992 ng/uL
RT: 13.355 min Scan# 1
Delta R.T. 0.003 min
Lab File: BG058118.D
Acq: 9 Jul 2023 9:09




Instrument :
BNA_G
ClientSampleId :
YBW01MSD


Tgt Ion:216 Resp: 165640
Ion Ratio Lower Upper
216 100
214 78.4 64.8 97.2
218 47.7 39.1 58.7

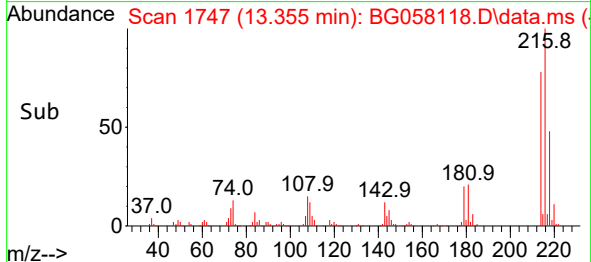

#76
Pentachlorobenzene
Concen: 52.357 ng/uL
RT: 14.871 min Scan# 2005
Delta R.T. -0.003 min
Lab File: BG058118.D
Acq: 9 Jul 2023 9:09

Tgt Ion:250 Resp: 402845
Ion Ratio Lower Upper
250 100
248 63.4 52.8 79.2
252 63.4 52.4 78.6

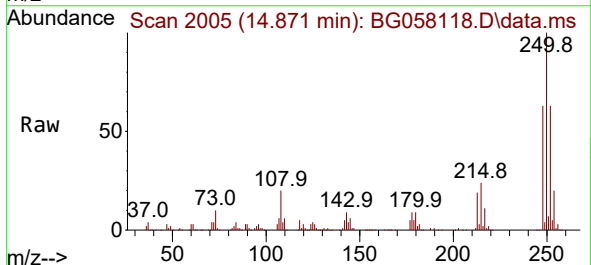



#77

Carbazole

Concen: 22.811 ng/ul

RT: 17.703 min Scan# 2487

Delta R.T. 0.003 min

Lab File: BG058118.D

Acq: 9 Jul 2023 9:09

Instrument :

BNA_G

ClientSampleId :

YBW01MSD





Tgt Ion:167 Resp: 576851

Ion Ratio Lower Upper

167 100

166 22.9 17.5 26.3

139 12.0 9.5 14.3

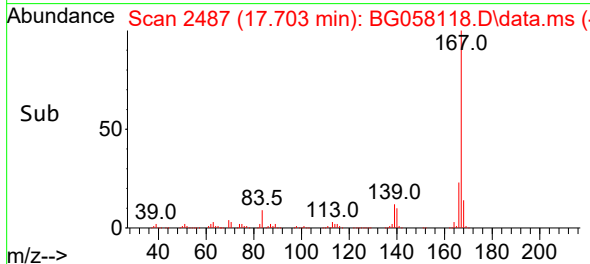

#78

Di-n-butylphthalate

Concen: 23.294 ng/ul

RT: 18.255 min Scan# 2581

Delta R.T. -0.003 min

Lab File: BG058118.D

Acq: 9 Jul 2023 9:09




Tgt Ion:149 Resp: 750385


Ion Ratio Lower Upper

149 100

150 9.8 7.4 11.2

104 5.2 3.9 5.9


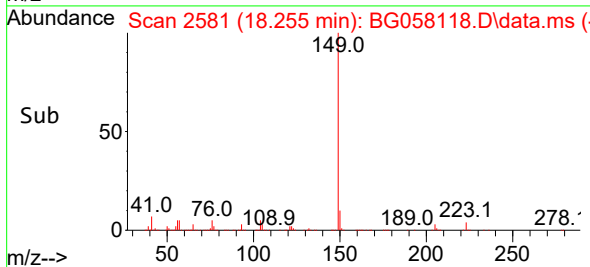

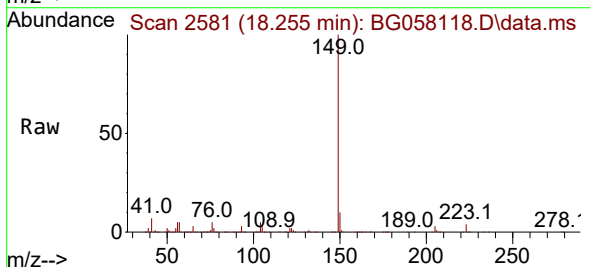




#80
Fluoranthene
Concen: 22.196 ng/ul
RT: 19.354 min Scan# 2768
Delta R.T. 0.003 min
Lab File: BG058118.D
Acq: 9 Jul 2023 9:09




Instrument :
BNA_G
ClientSampleId :
YBW01MSD


Tgt Ion:202 Resp: 762968
Ion Ratio Lower Upper
202 100
101 10.9 9.1 13.7
100 8.8 7.1 10.7

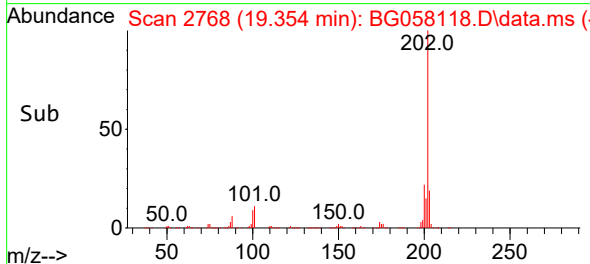

#82
Pyrene
Concen: 22.068 ng/ul
RT: 19.718 min Scan# 2830
Delta R.T. 0.003 min
Lab File: BG058118.D
Acq: 9 Jul 2023 9:09

Tgt Ion:202 Resp: 763573
Ion Ratio Lower Upper
202 100
101 13.0 10.2 15.2
100 10.9 8.9 13.3

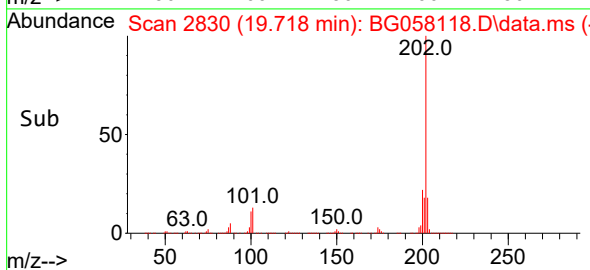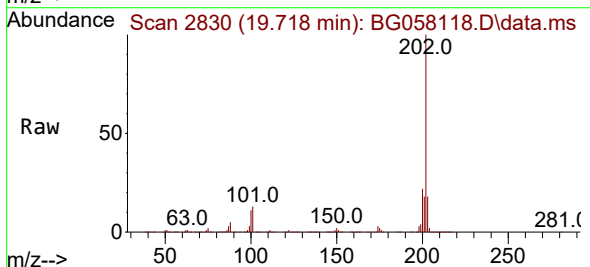



#83

Butylbenzylphthalate

Concen: 23.241 ng/ul

RT: 20.600 min Scan# 2980

Delta R.T. 0.003 min

Lab File: BG058118.D

Acq: 9 Jul 2023 9:09

Instrument :

BNA_G

ClientSampleId :

YBW01MSD





Tgt Ion:149 Resp: 326085

Ion Ratio Lower Upper

149 100

91 71.1 56.5 84.7

206 22.9 17.4 26.0



#84

3,3'-Dichlorobenzidine

Concen: 24.981 ng/ul

RT: 21.452 min Scan# 3125

Delta R.T. 0.003 min

Lab File: BG058118.D

Acq: 9 Jul 2023 9:09




Tgt Ion:252 Resp: 284854


Ion Ratio Lower Upper

252 100

254 64.5 50.7 76.1

126 8.6 6.6 10.0

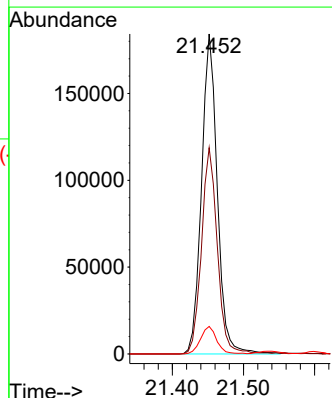



#85

Benzo(a)anthracene

Concen: 22.819 ng/ul

RT: 21.534 min Scan# 3139

Delta R.T. 0.003 min

Lab File: BG058118.D

Acq: 9 Jul 2023 9:09

Instrument :

BNA_G

ClientSampleId :

YBW01MSD





Tgt Ion:228 Resp: 771715

Ion Ratio Lower Upper

228 100

229 20.1 16.0 24.0

226 27.6 22.0 33.0

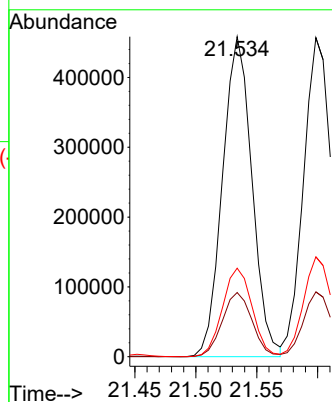

#86

Bis(2-ethylhexyl)phthalate

Concen: 23.524 ng/ul

RT: 21.434 min Scan# 3122

Delta R.T. -0.003 min

Lab File: BG058118.D

Acq: 9 Jul 2023 9:09




Tgt Ion:149 Resp: 472995


Ion Ratio Lower Upper

149 100

167 27.1 20.9 31.3

279 3.6 3.1 4.7





#87

Chrysene

Concen: 23.319 ng/ul

RT: 21.599 min Scan# 3150

Delta R.T. 0.003 min

Lab File: BG058118.D

Acq: 9 Jul 2023 9:09

Instrument :

BNA_G

ClientSampleId :

YBW01MSD





Tgt Ion:228 Resp: 739282

Ion Ratio Lower Upper

228 100

226 31.3 24.4 36.6

229 20.3 15.5 23.3



#89

Di-n-octyl phthalate

Concen: 22.829 ng/ul




RT: 22.621 min Scan# 3324


Delta R.T. 0.003 min

Lab File: BG058118.D

Acq: 9 Jul 2023 9:09

Tgt Ion:149 Resp: 836195









#90
Benzo(b)fluoranthene
Concen: 22.443 ng/ul
RT: 23.708 min Scan# 31
Delta R.T. 0.009 min
Lab File: BG058118.D
Acq: 9 Jul 2023 9:09




Instrument :
BNA_G
ClientSampleId :
YBW01MSD


Tgt Ion:252 Resp: 828426
Ion Ratio Lower Upper
252 100
253 21.9 18.1 27.1
125 8.3 7.5 11.3



#91
Benzo(k)fluoranthene
Concen: 22.355 ng/ul
RT: 23.772 min Scan# 3520
Delta R.T. 0.009 min
Lab File: BG058118.D
Acq: 9 Jul 2023 9:09

Tgt Ion:252 Resp: 808823
Ion Ratio Lower Upper
252 100
253 22.2 17.7 26.5
125 9.1 7.4 11.2





#93

Benzo(a)pyrene

Concen: 22.578 ng/ul

RT: 24.560 min Scan# 3

Delta R.T. 0.003 min

Lab File: BG058118.D

Acq: 9 Jul 2023 9:09

Instrument :

BNA_G

ClientSampleId :

YBW01MSD





Tgt Ion:252 Resp: 737641

Ion Ratio Lower Upper

252 100

253 21.6 17.8 26.6

125 10.0 8.3 12.5



#94

Indeno(1,2,3-cd)pyrene

Concen: 22.789 ng/ul

RT: 28.297 min Scan# 4290

Delta R.T. 0.003 min

Lab File: BG058118.D

Acq: 9 Jul 2023 9:09




Tgt Ion:276 Resp: 988679


Ion Ratio Lower Upper

276 100

138 15.8 14.0 21.0

277 23.6 19.4 29.2









#95
 Dibenzo(a,h)anthracene
 Concen: 23.029 ng/ul
 RT: 28.361 min Scan# 41
 Delta R.T. 0.003 min
 Lab File: BG058118.D
 Acq: 9 Jul 2023 9:09

Instrument :
 BNA_G
 ClientSampleId :
 YBW01MSD

Tgt Ion:278 Resp: 823860
 Ion Ratio Lower Upper
 278 100
 139 12.7 11.3 16.9
 279 24.4 18.9 28.3

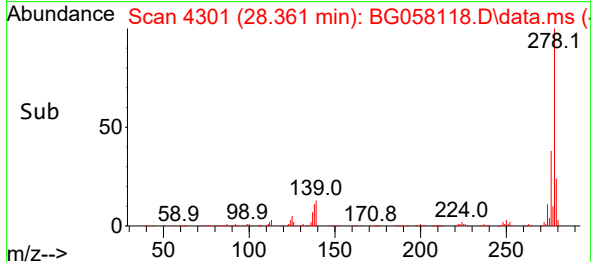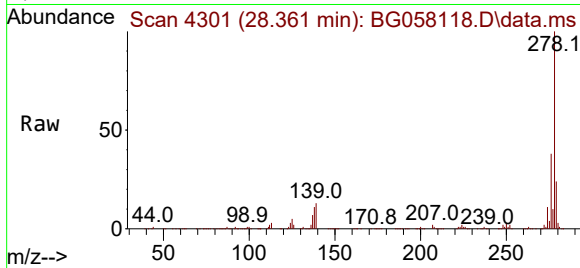

#96
 Benzo(g,h,i)perylene
 Concen: 22.650 ng/ul
 RT: 29.431 min Scan# 4483
 Delta R.T. 0.015 min
 Lab File: BG058118.D
 Acq: 9 Jul 2023 9:09

Tgt Ion:276 Resp: 802631
 Ion Ratio Lower Upper
 276 100
 138 16.9 14.2 21.2
 277 24.2 18.6 27.8

