




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070823\
 Data File : BG058094.D
 Acq On : 8 Jul 2023 15:05
 Operator : CG/JU
 Sample : 03348-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 YBTX8

Manual IntegrationsAPPROVED

Quant Time: Jul 09 00:45:36 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 08 10:01:01 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/09/2023
 Supervised By :mohammad ahmed 07/09/2023

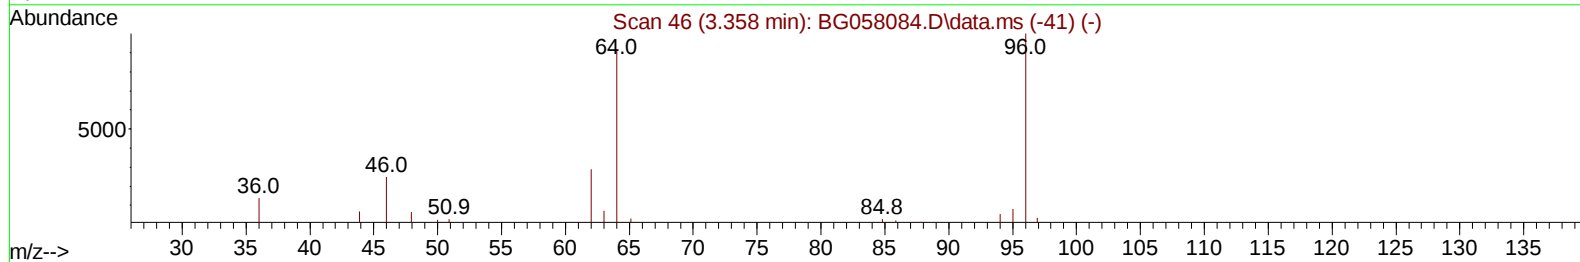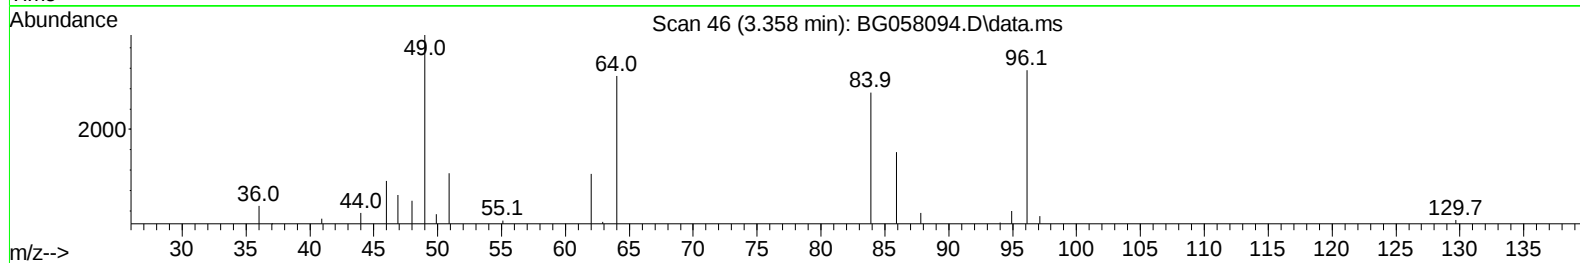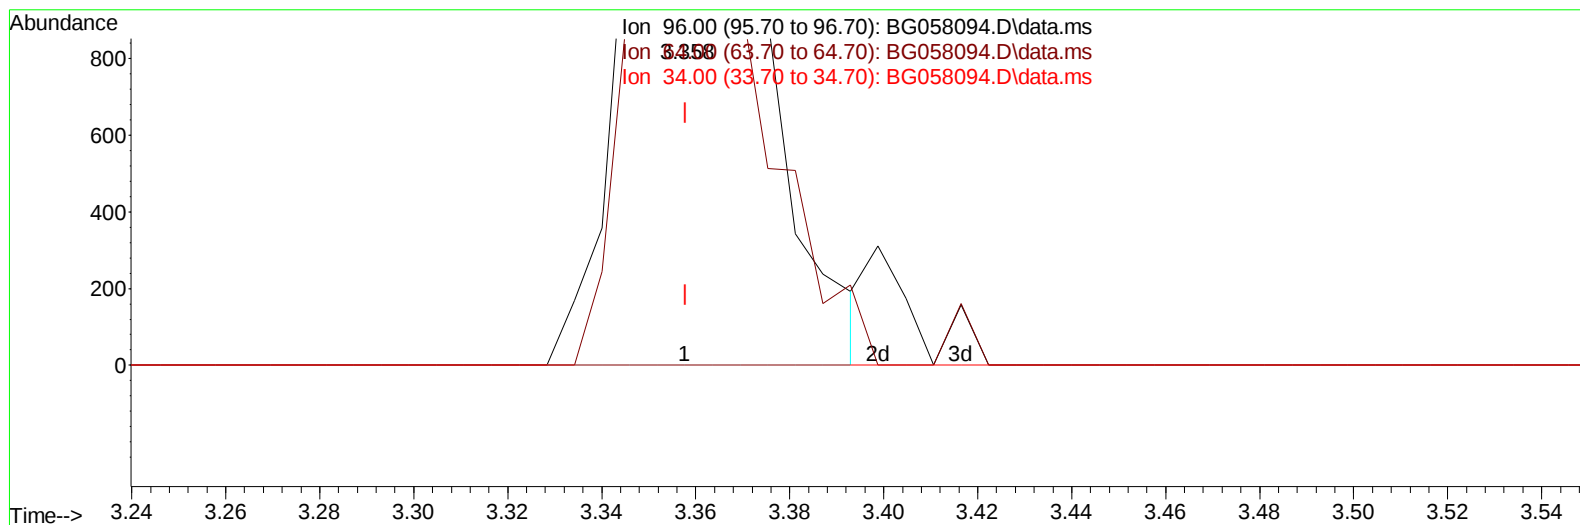

TIC: BG058094.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.358min (-0.000) 4.00 ng/uL

response 4736

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	79.90	96.17#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070823\
 Data File : BG058094.D
 Acq On : 8 Jul 2023 15:05
 Operator : CG/JU
 Sample : 03348-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 YBTX8

Manual IntegrationsAPPROVED

Quant Time: Jul 09 00:45:36 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 08 10:01:01 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/09/2023
 Supervised By :mohammad ahmed 07/09/2023

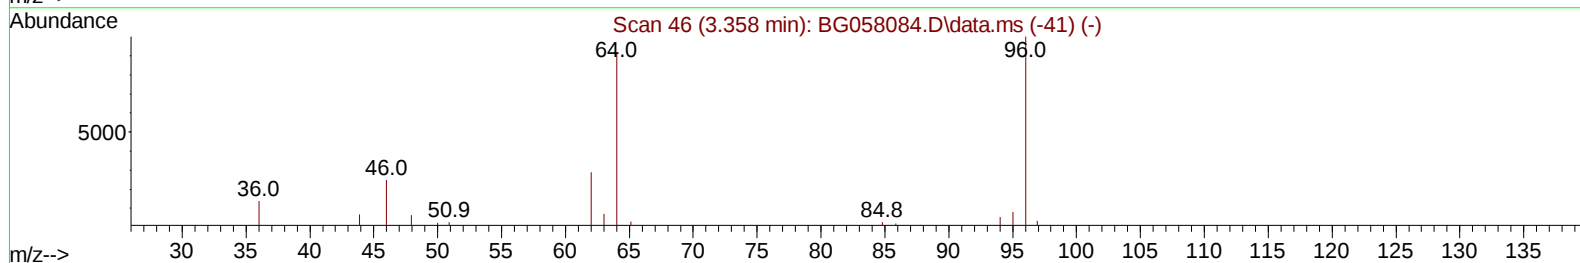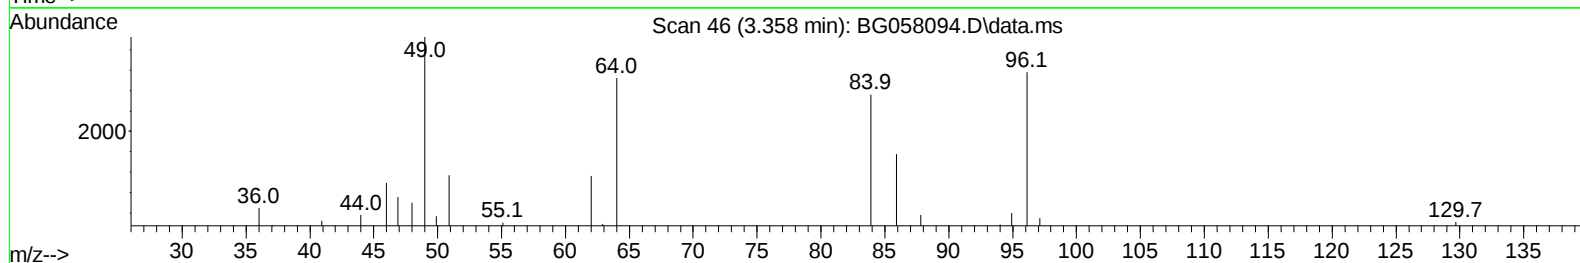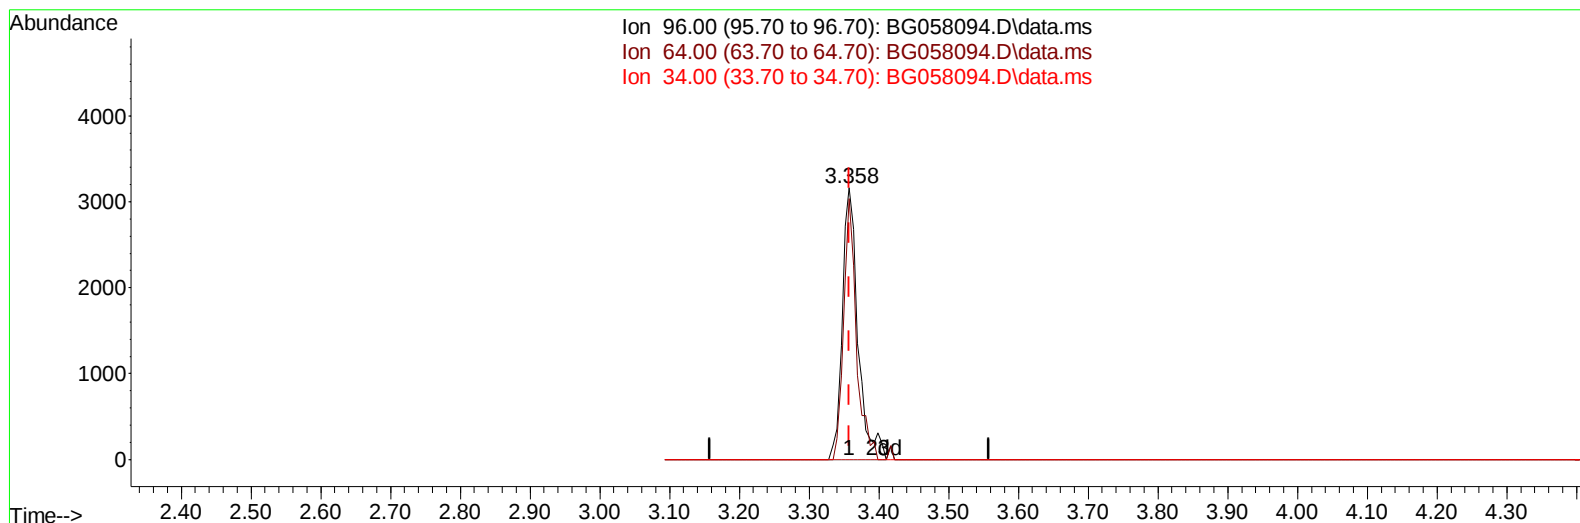

TIC: BG058094.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.358min (-0.000) 4.15 ng/uL m

response 4907

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	79.90	96.17#
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070823\
 Data File : BG058094.D
 Acq On : 8 Jul 2023 15:05
 Operator : CG/JU
 Sample : 03348-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 YBTX8

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/09/2023
 Supervised By :mohammad ahmed 07/09/2023

Quant Time: Jul 09 01:12:19 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 08 10:01:01 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.917	152	41422	20.000	ng/ul	0.00
20) Naphthalene-d8	10.720	136	186667	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.556	164	135842	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.300	188	347043	20.000	ng/ul	0.00
79) Chrysene-d12	21.548	240	314961	20.000	ng/ul	0.00
88) Perylene-d12	24.709	264	388022	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.358	96	4907m	4.148	ng/uL	0.00
4) Pyridine-d5	3.769	84	46443	12.932	ng/ul	0.00
7) Phenol-d5	7.083	99	97117	22.958	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.241	67	65004	25.499	ng/ul	0.00
11) 2-Chlorophenol-d4	7.447	132	72823	24.960	ng/ul	0.00
15) 4-Methylphenol-d8	8.622	113	76066	23.831	ng/ul	0.00
21) Nitrobenzene-d5	9.075	128	39198	25.764	ng/ul	0.00
24) 2-Nitrophenol-d4	9.803	143	43012	26.899	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.344	165	78136	25.473	ng/ul	0.00
31) 4-Chloroaniline-d4	10.855	131	103180	22.186	ng/ul	0.00
46) Dimethylphthalate-d6	13.957	166	288680	26.934	ng/ul	0.00
49) Acenaphthylene-d8	14.251	160	332709	28.446	ng/ul	0.00
54) 4-Nitrophenol-d4	14.756	143	43925	23.196	ng/ul	0.00
60) Fluorene-d10	15.543	176	265637	29.183	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.661	200	38984	20.687	ng/ul	0.00
73) Anthracene-d10	17.394	188	456145	28.326	ng/ul	0.00
81) Pyrene-d10	19.686	212	553468	27.902	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.486	264	574847	29.078	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070823\
Data File : BG058094.D
Acq On : 8 Jul 2023 15:05
Operator : CG/JU
Sample : 03348-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
YBTX8

Manual IntegrationsAPPROVED

Quant Time: Jul 09 01:12:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jul 08 10:01:01 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/09/2023
Supervised By :mohammad ahmed 07/09/2023

