




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070823\
 Data File : BG058100.D
 Acq On : 8 Jul 2023 19:57
 Operator : CG/JU
 Sample : 03348-05
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 YBTY2

Manual IntegrationsAPPROVED

Quant Time: Jul 09 00:46:41 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 08 10:01:01 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/09/2023
 Supervised By :mohammad ahmed 07/09/2023

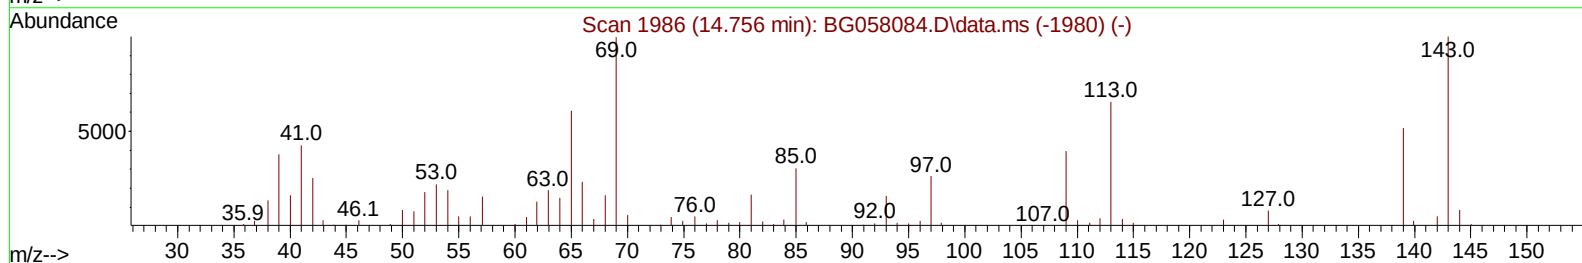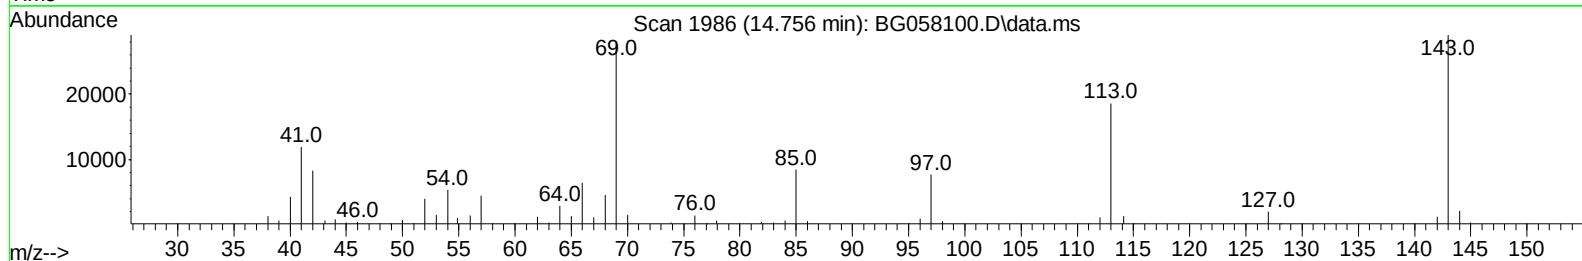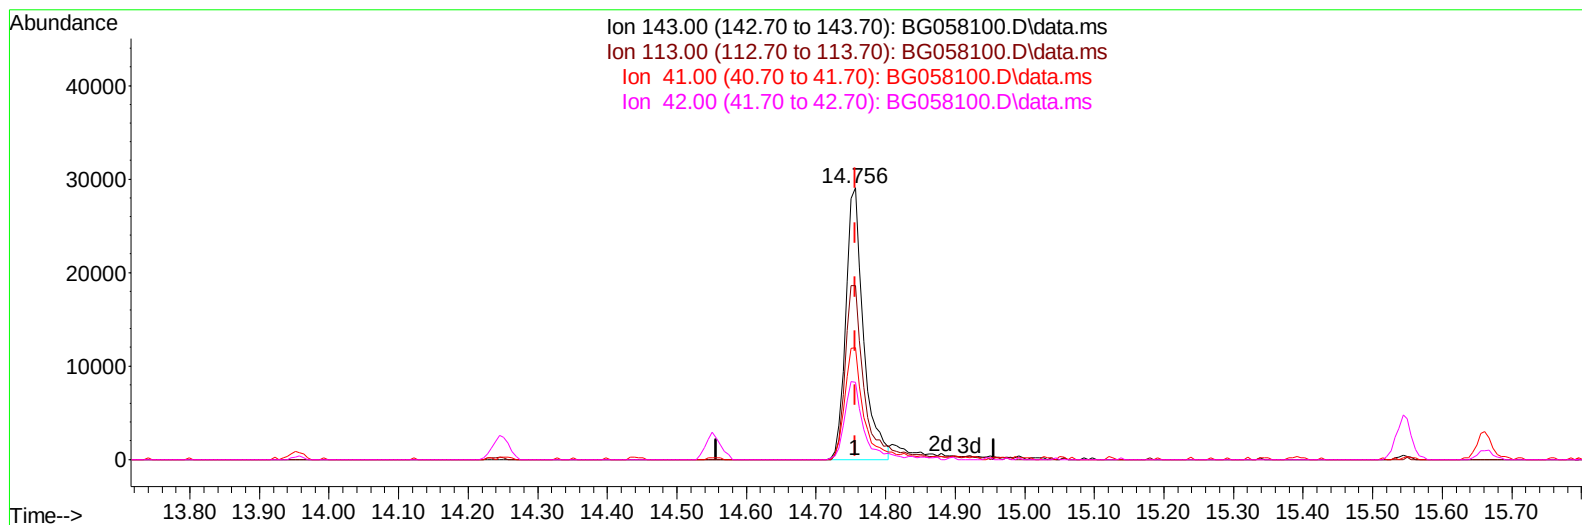

TIC: BG058100.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.756min (+ 0.000) 24.47 ng/ul

response 51120

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	66.40	63.93
41.00	40.50	41.04
42.00	27.50	28.41




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070823\
 Data File : BG058100.D
 Acq On : 8 Jul 2023 19:57
 Operator : CG/JU
 Sample : 03348-05
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 YBTY2

Manual IntegrationsAPPROVED

Quant Time: Jul 09 00:46:41 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 08 10:01:01 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/09/2023
 Supervised By :mohammad ahmed 07/09/2023

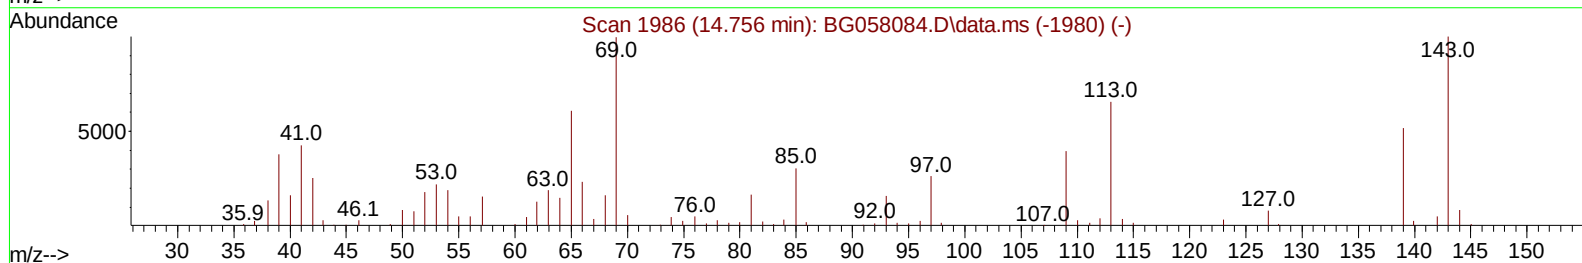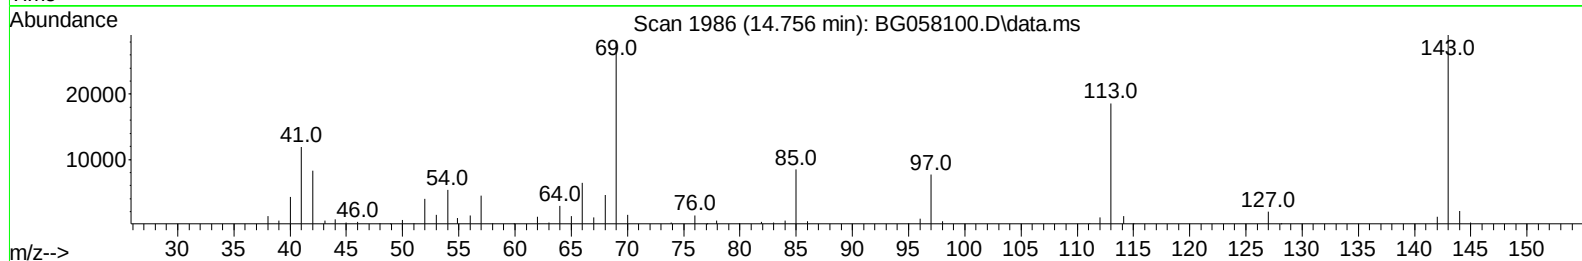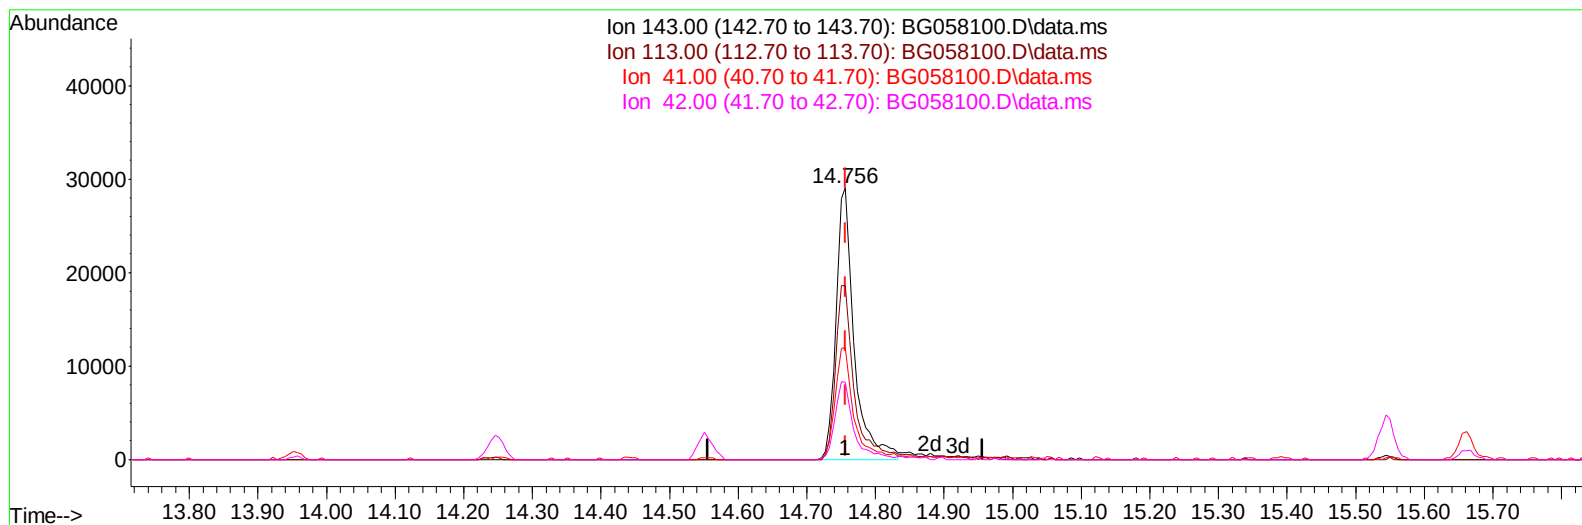

TIC: BG058100.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.756min (+ 0.000) 25.52 ng/ul m

response 53305

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	66.40	63.93
41.00	40.50	41.04
42.00	27.50	28.41

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070823\
 Data File : BG058100.D
 Acq On : 8 Jul 2023 19:57
 Operator : CG/JU
 Sample : 03348-05
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 YBTY2

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/09/2023
 Supervised By :mohammad ahmed 07/09/2023

Quant Time: Jul 09 01:20:25 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 08 10:01:01 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.917	152	44648	20.000	ng/ul	0.00
20) Naphthalene-d8	10.720	136	200575	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.551	164	149856	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.295	188	390842	20.000	ng/ul	0.00
79) Chrysene-d12	21.548	240	355306	20.000	ng/ul	0.00
88) Perylene-d12	24.704	264	435025	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.358	96	6469	5.074	ng/uL	0.00
4) Pyridine-d5	3.763	84	60931	15.741	ng/ul	0.00
7) Phenol-d5	7.083	99	122930	26.960	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.242	67	70263	25.571	ng/ul	0.00
11) 2-Chlorophenol-d4	7.447	132	81551	25.932	ng/ul	0.00
15) 4-Methylphenol-d8	8.622	113	93518	27.181	ng/ul	0.00
21) Nitrobenzene-d5	9.075	128	41992	25.687	ng/ul	0.00
24) 2-Nitrophenol-d4	9.803	143	49047	28.547	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.338	165	90552	27.474	ng/ul	0.00
31) 4-Chloroaniline-d4	10.855	131	96094	19.230	ng/ul	0.00
46) Dimethylphthalate-d6	13.957	166	344787	29.160	ng/ul	0.00
49) Acenaphthylene-d8	14.245	160	356849	27.657	ng/ul	0.00
54) 4-Nitrophenol-d4	14.756	143	53305m	25.517	ng/ul	0.00
60) Fluorene-d10	15.544	176	307926	30.665	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.661	200	49602	23.372	ng/ul	0.00
73) Anthracene-d10	17.395	188	559786	30.866	ng/ul	0.00
81) Pyrene-d10	19.686	212	670383	29.958	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.492	264	700840	31.621	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070823\
Data File : BG058100.D
Acq On : 8 Jul 2023 19:57
Operator : CG/JU
Sample : 03348-05
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
YBTY2

Manual IntegrationsAPPROVED

Quant Time: Jul 09 01:20:25 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jul 08 10:01:01 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/09/2023
Supervised By :mohammad ahmed 07/09/2023

