




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070823\
Data File : BG058103.D
Acq On : 8 Jul 2023 22:01
Operator : CG/JU
Sample : 03348-10
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
YBTY5

Manual IntegrationsAPPROVED

Quant Time: Jul 09 06:59:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jul 08 10:01:01 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/09/2023
Supervised By :mohammad ahmed 07/09/2023

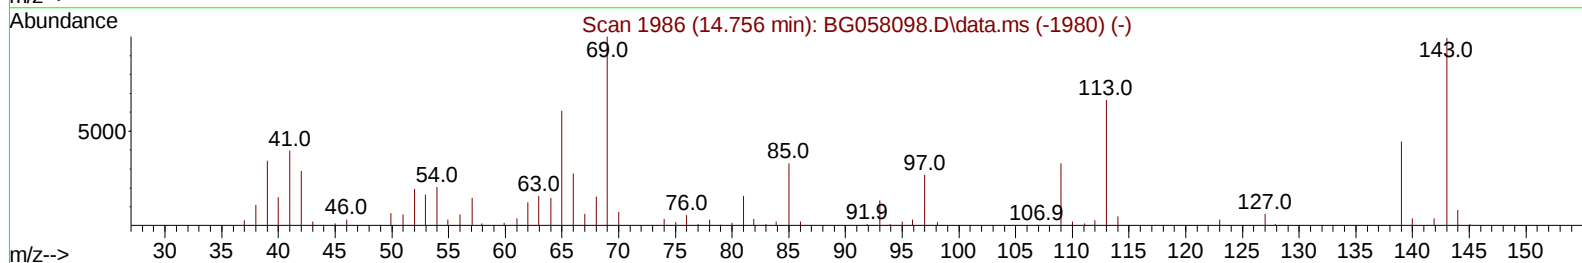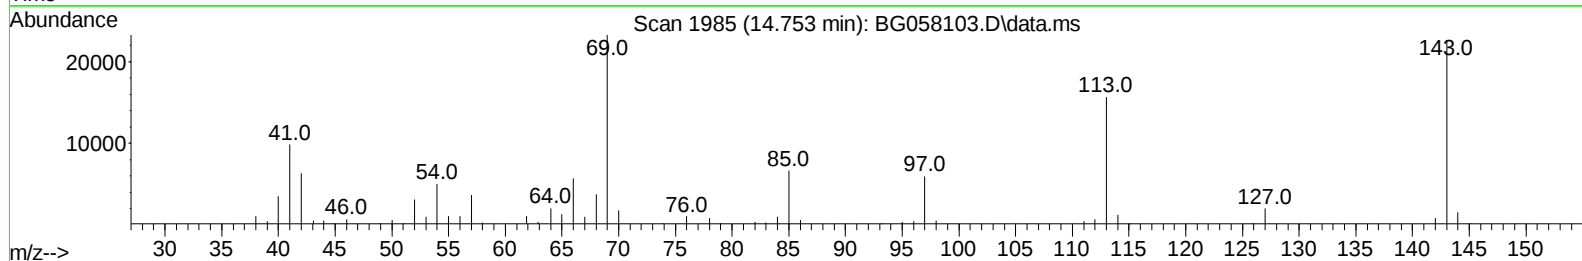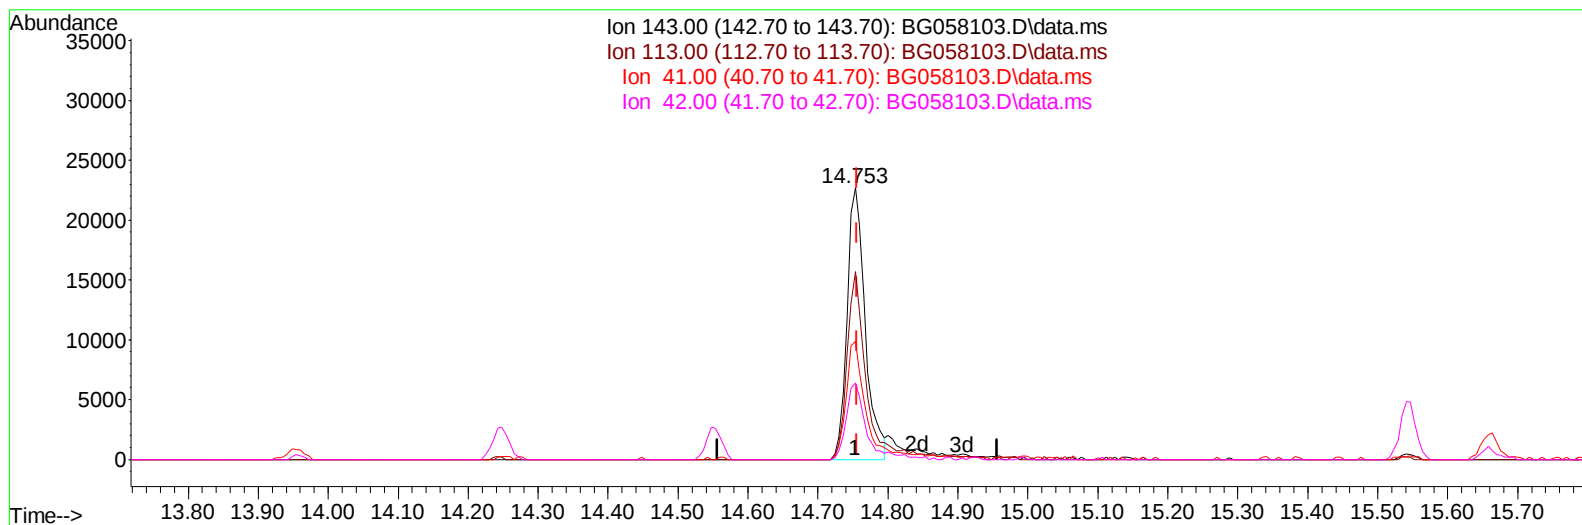

TIC: BG058103.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.753min (-0.003) 20.74 ng/u1

response 40747

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	66.40	69.21
41.00	40.50	43.44
42.00	27.50	28.12




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070823\
Data File : BG058103.D
Acq On : 8 Jul 2023 22:01
Operator : CG/JU
Sample : 03348-10
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
YBTY5

Manual IntegrationsAPPROVED

Quant Time: Jul 09 01:24:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jul 08 10:01:01 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/09/2023
Supervised By :mohammad ahmed 07/09/2023

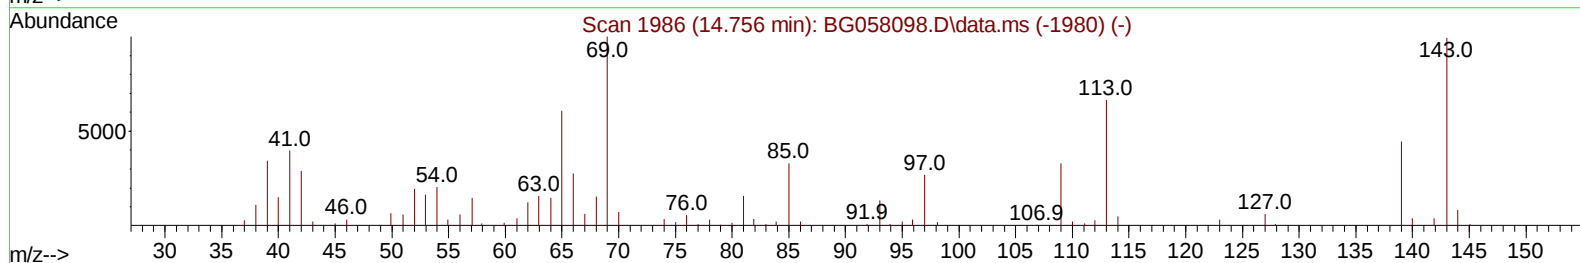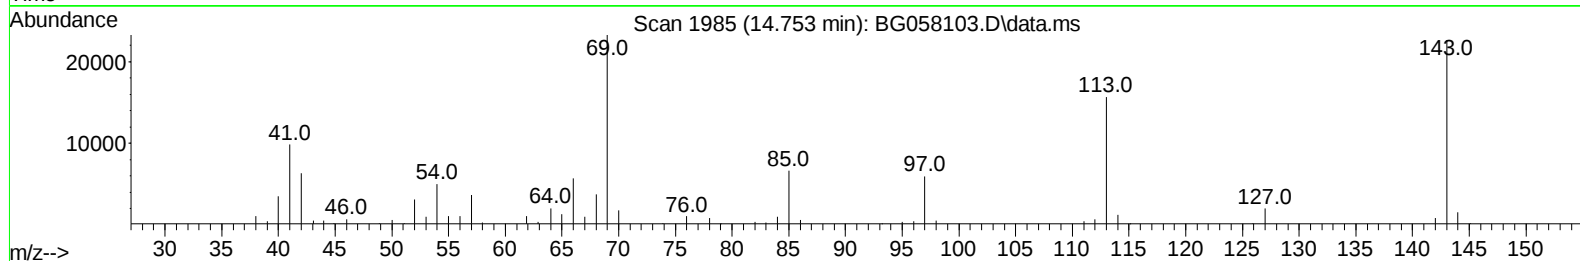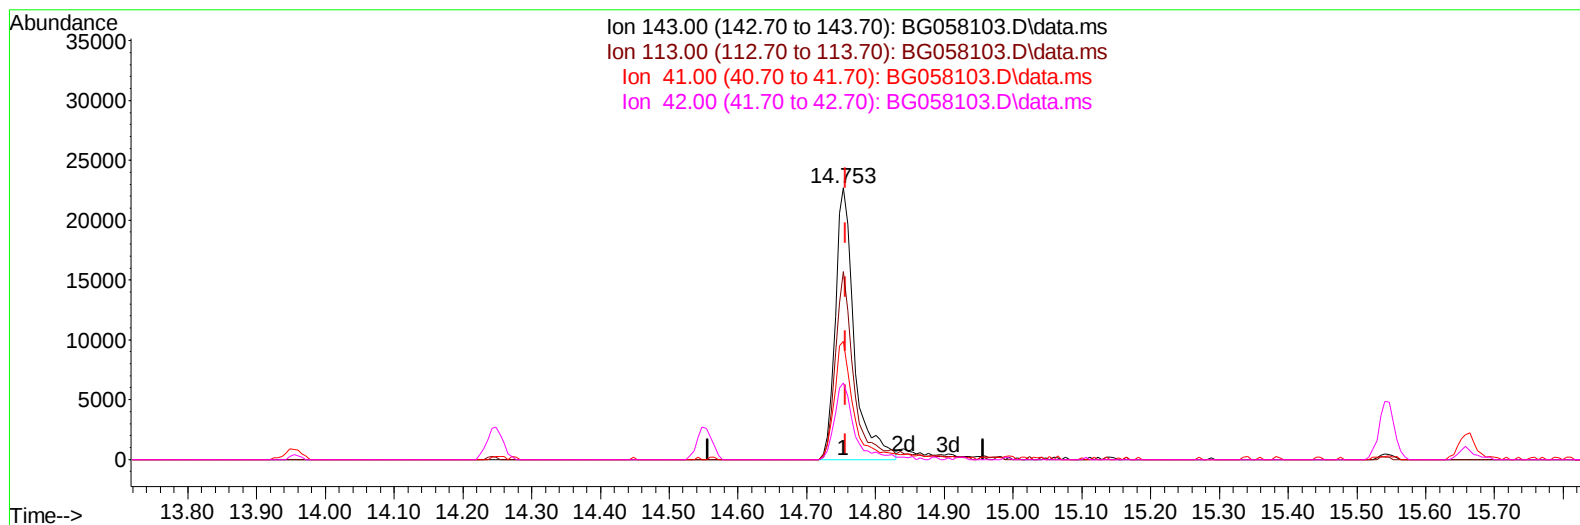

TIC: BG058103.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.753min (-0.003) 22.06 ng/ul m

response 43330

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	66.40	69.21
41.00	40.50	43.44
42.00	27.50	28.12

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070823\
 Data File : BG058103.D
 Acq On : 8 Jul 2023 22:01
 Operator : CG/JU
 Sample : 03348-10
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 YBTY5

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/09/2023
 Supervised By :mohammad ahmed 07/09/2023

Quant Time: Jul 09 01:24:40 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 08 10:01:01 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.914	152	41638	20.000	ng/ul	0.00
20) Naphthalene-d8	10.717	136	190274	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.554	164	140922	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.297	188	368505	20.000	ng/ul	0.00
79) Chrysene-d12	21.551	240	325507	20.000	ng/ul	0.00
88) Perylene-d12	24.701	264	396268	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.355	96	6382	5.367	ng/uL	0.00
4) Pyridine-d5	3.766	84	67305	18.644	ng/ul	0.00
7) Phenol-d5	7.080	99	123843	29.124	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.239	67	74434	29.047	ng/ul	0.00
11) 2-Chlorophenol-d4	7.450	132	83898	28.607	ng/ul	0.00
15) 4-Methylphenol-d8	8.619	113	97234	30.304	ng/ul	0.00
21) Nitrobenzene-d5	9.078	128	47463	30.605	ng/ul	0.00
24) 2-Nitrophenol-d4	9.800	143	53393	32.759	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.341	165	96953	31.008	ng/ul	0.00
31) 4-Chloroaniline-d4	10.852	131	97828	20.637	ng/ul	0.00
46) Dimethylphthalate-d6	13.954	166	360832	32.452	ng/ul	0.00
49) Acenaphthylene-d8	14.248	160	399960	32.964	ng/ul	0.00
54) 4-Nitrophenol-d4	14.753	143	43330m	22.057	ng/ul	0.00
60) Fluorene-d10	15.547	176	328994	34.840	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.664	200	39884	19.932	ng/ul	0.00
73) Anthracene-d10	17.397	188	569046	33.278	ng/ul	0.00
81) Pyrene-d10	19.683	212	664121	32.395	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.483	264	691622	34.258	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070823\
Data File : BG058103.D
Acq On : 8 Jul 2023 22:01
Operator : CG/JU
Sample : 03348-10
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
YBTY5

Manual IntegrationsAPPROVED

Quant Time: Jul 09 01:24:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jul 08 10:01:01 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/09/2023
Supervised By :mohammad ahmed 07/09/2023

