

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070823\
 Data File : BG058114.D
 Acq On : 9 Jul 2023 6:24
 Operator : CG/JU
 Sample : PB153885BL
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK885

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG058114.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.353	41	45	54	rVB	14504	21515	1.33%	0.143%
2	3.764	110	115	130	rBV	193158	314617	19.51%	2.092%
3	4.099	168	172	178	rVB5	3260	6318	0.39%	0.042%
4	7.078	672	679	690	rBV	198881	330640	20.50%	2.198%
5	7.243	700	707	715	rBV	154995	253416	15.71%	1.685%
6	7.448	735	742	751	rBV	181530	305480	18.94%	2.031%
7	7.912	815	821	829	rVB	152378	254190	15.76%	1.690%
8	8.617	935	941	956	rBV	223793	395617	24.53%	2.630%
9	9.076	1010	1019	1032	rBV	185153	322168	19.98%	2.142%
10	9.798	1132	1142	1150	rBV	148194	261572	16.22%	1.739%
11	10.339	1227	1234	1247	rBV	226983	399386	24.76%	2.655%
12	10.721	1291	1299	1309	rVB	236633	406977	25.23%	2.706%
13	10.850	1314	1321	1331	rBV	227968	427993	26.54%	2.845%
14	12.237	1552	1557	1563	rBV2	4338	6264	0.39%	0.042%
15	12.307	1563	1569	1575	rVB2	3083	5477	0.34%	0.036%
16	13.447	1755	1763	1769	rBV3	4767	8900	0.55%	0.059%
17	13.952	1843	1849	1859	rBV	448527	653297	40.51%	4.343%
18	14.246	1891	1899	1910	rBV	518693	815270	50.55%	5.420%
19	14.552	1944	1951	1963	rBV	424343	640694	39.73%	4.259%
20	14.751	1978	1985	2002	rBV	170667	328160	20.35%	2.182%
21	14.857	2002	2003	2011	rVB6	3073	4219	0.26%	0.028%
22	15.545	2113	2120	2134	rBV	706186	1053517	65.32%	7.004%
23	15.662	2134	2140	2155	rVV	211358	314720	19.51%	2.092%
24	15.786	2155	2161	2163	rVB3	2512	3444	0.21%	0.023%
25	17.296	2412	2418	2428	rBV	581934	899522	55.78%	5.980%
26	17.395	2428	2435	2452	rVB	827197	1247275	77.34%	8.292%
27	19.252	2745	2751	2755	rBV2	9987	14083	0.87%	0.094%
28	19.323	2757	2763	2769	rBV	8766	12095	0.75%	0.080%
29	19.599	2807	2810	2812	rBV4	2274	2115	0.13%	0.014%
30	19.687	2818	2825	2835	rBV	1060679	1487259	92.22%	9.888%
31	20.180	2907	2909	2912	rBV4	1273	1773	0.11%	0.012%
32	20.210	2912	2914	2918	rVB4	1911	2087	0.13%	0.014%
33	20.838	3019	3021	3022	rVB	3238	1722	0.11%	0.011%
34	21.056	3055	3058	3060	rBV3	2105	3403	0.21%	0.023%
35	21.103	3064	3066	3069	rBV4	2061	2342	0.15%	0.016%
36	21.549	3135	3142	3155	rBV2	591202	985751	61.12%	6.553%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070823\
 Data File : BG058114.D
 Acq On : 9 Jul 2023 6:24
 Operator : CG/JU
 Sample : PB153885BL
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK885

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Title : SVOA CALIBRATION

37	22.319	3271	3273	3278	rVB5	4884	7280	0.45%	0.048%
38	22.783	3350	3352	3355	rBV3	2238	2144	0.13%	0.014%
39	22.995	3384	3388	3398	rVB8	11343	23531	1.46%	0.156%
40	23.788	3518	3523	3530	rVB6	10111	20692	1.28%	0.138%
41	23.976	3554	3555	3559	rBV4	3023	4327	0.27%	0.029%
42	24.123	3578	3580	3585	rVB6	2491	2743	0.17%	0.018%
43	24.487	3628	3642	3660	rBV2	587222	1612754	100.00%	10.722%
44	24.704	3668	3679	3696	rVB2	394034	1116685	69.24%	7.424%
45	25.098	3744	3746	3749	rVB4	2750	2104	0.13%	0.014%
46	25.210	3763	3765	3768	rBV3	2536	2274	0.14%	0.015%
47	25.609	3831	3833	3834	rBV2	2654	2273	0.14%	0.015%
48	25.803	3862	3866	3875	rVB6	14274	37221	2.31%	0.247%
49	26.303	3950	3951	3953	rBV2	3764	3165	0.20%	0.021%
50	26.450	3974	3976	3978	rBV2	2649	2310	0.14%	0.015%
51	27.401	4136	4138	4139	rVB	3183	1904	0.12%	0.013%
52	31.044	4756	4758	4759	rBV	4947	3140	0.19%	0.021%
53	32.525	5008	5010	5013	rBV4	3016	3927	0.24%	0.026%


Sum of corrected areas: 15041752

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070823\
Data File : BG058114.D
Acq On : 9 Jul 2023 6:24
Operator : CG/JU
Sample : PB153885BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK885

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

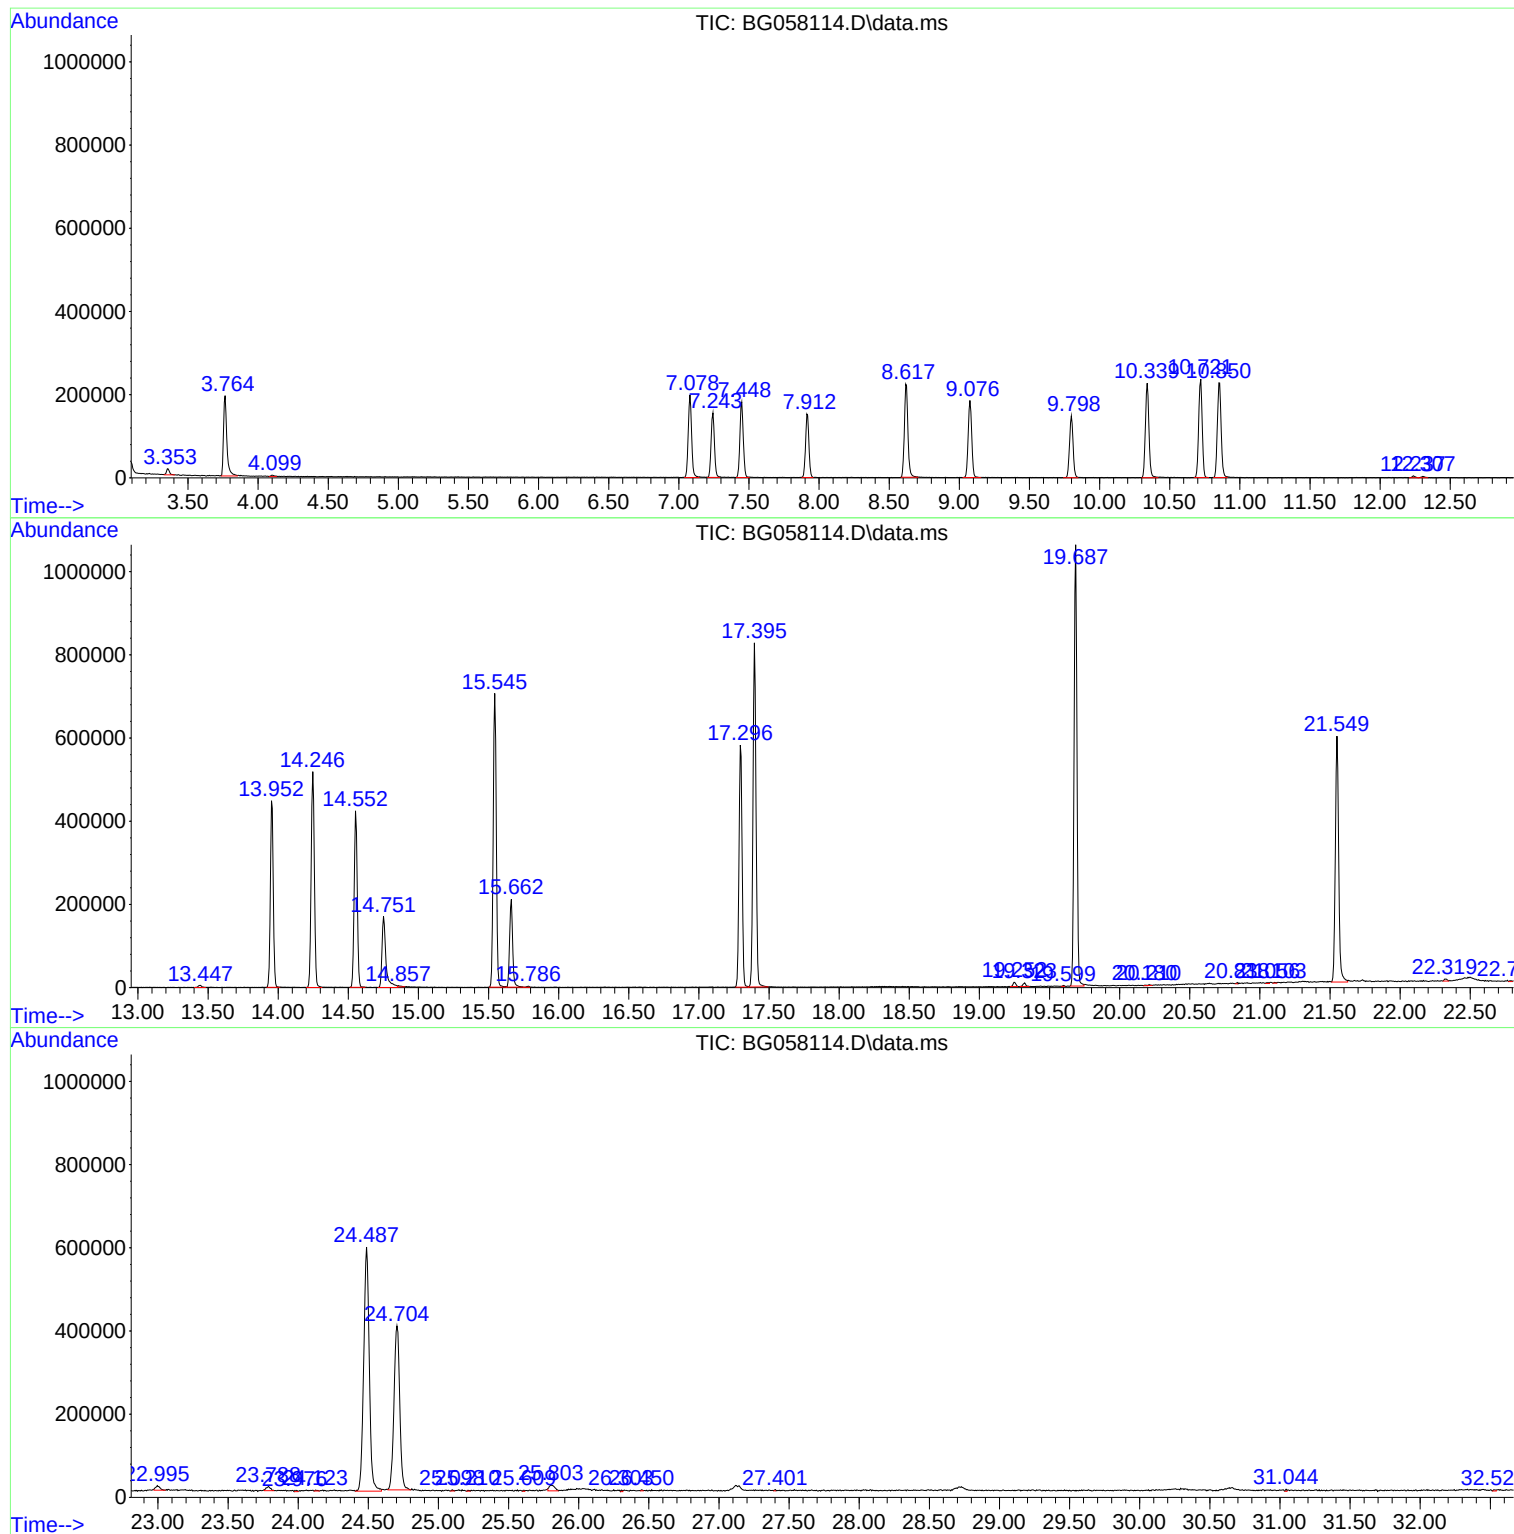

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070823\
Data File : BG058114.D
Acq On : 9 Jul 2023 6:24
Operator : CG/JU
Sample : PB153885BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK885

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070823\
Data File : BG058114.D
Acq On : 9 Jul 2023 6:24
Operator : CG/JU
Sample : PB153885BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK885

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc