

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070823\
 Data File : BG058120.D
 Acq On : 9 Jul 2023 10:33
 Operator : CG/JU
 Sample : 03349-10
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 YBW03

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG058120.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	27	29	31	rVB2	2659	2189	0.15%	0.014%
2	3.358	40	46	50	rVB	11938	18009	1.26%	0.111%
3	3.628	90	92	96	rVB2	1843	2141	0.15%	0.013%
4	3.764	110	115	129	rBV	161885	253613	17.73%	1.564%
5	4.004	153	156	159	rVB2	1332	1628	0.11%	0.010%
6	4.104	169	173	178	rVB3	4220	6088	0.43%	0.038%
7	7.077	672	679	688	rBV	176298	302426	21.14%	1.865%
8	7.142	688	690	692	rVB2	1880	1464	0.10%	0.009%
9	7.242	700	707	719	rBV	139655	229354	16.03%	1.415%
10	7.365	725	728	733	rBV3	1086	2025	0.14%	0.012%
11	7.447	736	742	750	rVV	163394	272634	19.06%	1.681%
12	7.917	813	822	830	rBV	202817	338879	23.69%	2.090%
13	8.623	935	942	958	rBV	214502	380454	26.60%	2.346%
14	9.075	1011	1019	1032	rBV	168476	294945	20.62%	1.819%
15	9.480	1084	1088	1093	rVB3	996	1805	0.13%	0.011%
16	9.798	1135	1142	1153	rVB	137696	236884	16.56%	1.461%
17	10.338	1226	1234	1245	rBV	211730	375775	26.27%	2.318%
18	10.720	1290	1299	1307	rBV	304763	537213	37.56%	3.313%
19	10.855	1315	1322	1333	rBV	219699	395258	27.63%	2.438%
20	12.242	1553	1558	1561	rBV2	1274	1573	0.11%	0.010%
21	12.306	1565	1569	1575	rBV2	3765	5737	0.40%	0.035%
22	13.370	1745	1750	1753	rBV3	2307	2881	0.20%	0.018%
23	13.435	1756	1761	1768	rVB2	3379	6118	0.43%	0.038%
24	13.952	1842	1849	1857	rBV	415235	612514	42.82%	3.778%
25	14.022	1859	1861	1866	rVV2	1064	1766	0.12%	0.011%
26	14.075	1866	1870	1874	rVV2	1311	1550	0.11%	0.010%
27	14.140	1876	1881	1886	rVV2	985	1689	0.12%	0.010%
28	14.245	1892	1899	1907	rBV2	471911	753914	52.71%	4.650%
29	14.439	1930	1932	1936	rVB2	2029	2424	0.17%	0.015%
30	14.551	1945	1951	1963	rBV	505748	815304	57.00%	5.028%
31	14.751	1979	1985	2001	rBV	147475	282751	19.77%	1.744%
32	14.962	2018	2021	2024	rBV3	1311	1718	0.12%	0.011%
33	15.338	2080	2085	2087	rBV2	1148	1721	0.12%	0.011%
34	15.397	2091	2095	2097	rVB2	1884	2356	0.16%	0.015%
35	15.544	2113	2120	2129	rBV	685178	998674	69.82%	6.159%
36	15.661	2134	2140	2149	rBV	171164	247985	17.34%	1.529%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070823\
 Data File : BG058120.D
 Acq On : 9 Jul 2023 10:33
 Operator : CG/JU
 Sample : 03349-10
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 YBW03

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Title : SVOA CALIBRATION

37	15.779	2157	2160	2164	rBV2	1909	2551	0.18%	0.016%
38	15.908	2175	2182	2192	rVV	122703	180703	12.63%	1.114%
39	16.255	2237	2241	2242	rVV3	1726	2075	0.15%	0.013%
40	16.278	2242	2245	2247	rVB3	2397	2391	0.17%	0.015%
41	16.472	2273	2278	2285	rVB	17113	22923	1.60%	0.141%
42	16.601	2296	2300	2305	rBV3	1762	2725	0.19%	0.017%
43	16.772	2328	2329	2333	rVB2	1280	1523	0.11%	0.009%
44	16.825	2333	2338	2346	rBV4	2075	3415	0.24%	0.021%
45	16.995	2364	2367	2372	rVB4	2227	3118	0.22%	0.019%
46	17.042	2372	2375	2379	rBV3	2119	2800	0.20%	0.017%
47	17.089	2379	2383	2386	rBV3	1530	2394	0.17%	0.015%
48	17.201	2400	2402	2408	rVB2	2011	2865	0.20%	0.018%
49	17.295	2412	2418	2428	rBV	724177	1113091	77.82%	6.865%
50	17.395	2428	2435	2445	rVV2	767851	1151549	80.51%	7.102%
51	17.477	2445	2449	2456	rVB2	24284	33526	2.34%	0.207%
52	17.653	2476	2479	2481	rBV2	1439	1653	0.12%	0.010%
53	17.712	2486	2489	2491	rVB3	1561	1590	0.11%	0.010%
54	18.064	2546	2549	2550	rBV3	1646	1669	0.12%	0.010%
55	18.182	2564	2569	2579	rBV2	47042	90444	6.32%	0.558%
56	18.288	2585	2587	2591	rVB4	3067	3438	0.24%	0.021%
57	18.388	2600	2604	2607	rVB6	2003	2572	0.18%	0.016%
58	18.476	2616	2619	2625	rVB6	1840	2575	0.18%	0.016%
59	18.899	2687	2691	2696	rVV3	7443	8347	0.58%	0.051%
60	18.969	2698	2703	2705	rVB5	1394	2148	0.15%	0.013%
61	19.104	2722	2726	2730	rBV3	3931	5300	0.37%	0.033%
62	19.151	2730	2734	2736	rVV3	1243	1791	0.13%	0.011%
63	19.222	2742	2746	2748	rBV4	9491	11239	0.79%	0.069%
64	19.251	2748	2751	2755	rVB3	10398	13816	0.97%	0.085%
65	19.322	2758	2763	2767	rBV	10334	15770	1.10%	0.097%
66	19.463	2784	2787	2792	rBV5	4479	6226	0.44%	0.038%
67	19.592	2807	2809	2813	rBV3	2190	3077	0.22%	0.019%
68	19.686	2818	2825	2835	rBV	967324	1372197	95.93%	8.463%
69	19.921	2863	2865	2867	rBV2	1979	1936	0.14%	0.012%
70	19.950	2867	2870	2872	rVB4	3098	3409	0.24%	0.021%
71	20.215	2910	2915	2917	rBV3	9403	11529	0.81%	0.071%
72	20.274	2920	2925	2927	rBV5	2569	4577	0.32%	0.028%
73	20.650	2987	2989	2990	rVB2	2664	1549	0.11%	0.010%
74	20.703	2995	2998	3002	rVB3	11110	13199	0.92%	0.081%
75	21.143	3071	3073	3074	rBV2	2447	1603	0.11%	0.010%
76	21.173	3076	3078	3079	rBV2	2213	1641	0.11%	0.010%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070823\
 Data File : BG058120.D
 Acq On : 9 Jul 2023 10:33
 Operator : CG/JU
 Sample : 03349-10
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 YBW03

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Title : SVOA CALIBRATION

77	21.231	3079	3088	3090	rBV7	36594	88980	6.22%	0.549%
78	21.437	3119	3123	3127	rVB3	10831	16200	1.13%	0.100%
79	21.549	3135	3142	3156	rBV2	714498	1202000	84.03%	7.413%
80	21.690	3164	3166	3169	rBV3	3200	3660	0.26%	0.023%
81	21.731	3169	3173	3179	rVB	16203	24390	1.71%	0.150%
82	22.324	3268	3274	3279	rBV2	17800	27911	1.95%	0.172%
83	22.694	3331	3337	3339	rBV7	6070	10742	0.75%	0.066%
84	23.000	3383	3389	3397	rVB	25367	49107	3.43%	0.303%
85	23.188	3415	3421	3429	rVB	47138	90628	6.34%	0.559%
86	23.722	3511	3512	3515	rBV3	2951	2775	0.19%	0.017%
87	23.787	3517	3523	3530	rVB2	31751	64522	4.51%	0.398%
88	24.486	3631	3642	3654	rBV2	518463	1430390	100.00%	8.822%
89	24.704	3668	3679	3692	rBV2	492861	1422622	99.46%	8.774%
90	25.650	3838	3840	3841	rBV2	2953	2202	0.15%	0.014%
91	25.808	3858	3867	3876	rBV5	35925	104019	7.27%	0.642%
92	26.613	4003	4004	4007	rVB3	4951	2409	0.17%	0.015%
93	27.136	4083	4093	4102	rVB3	28843	102676	7.18%	0.633%
94	27.982	4235	4237	4238	rBV2	3481	1905	0.13%	0.012%
95	28.717	4353	4362	4364	rBV5	17640	44593	3.12%	0.275%
96	28.869	4386	4388	4389	rBV2	3190	2070	0.14%	0.013%
97	30.620	4681	4686	4687	rBV5	8794	13172	0.92%	0.081%
98	31.314	4802	4804	4807	rBV4	2678	2549	0.18%	0.016%


Sum of corrected areas: 16213925

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070823\
Data File : BG058120.D
Acq On : 9 Jul 2023 10:33
Operator : CG/JU
Sample : 03349-10
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
YBW03

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

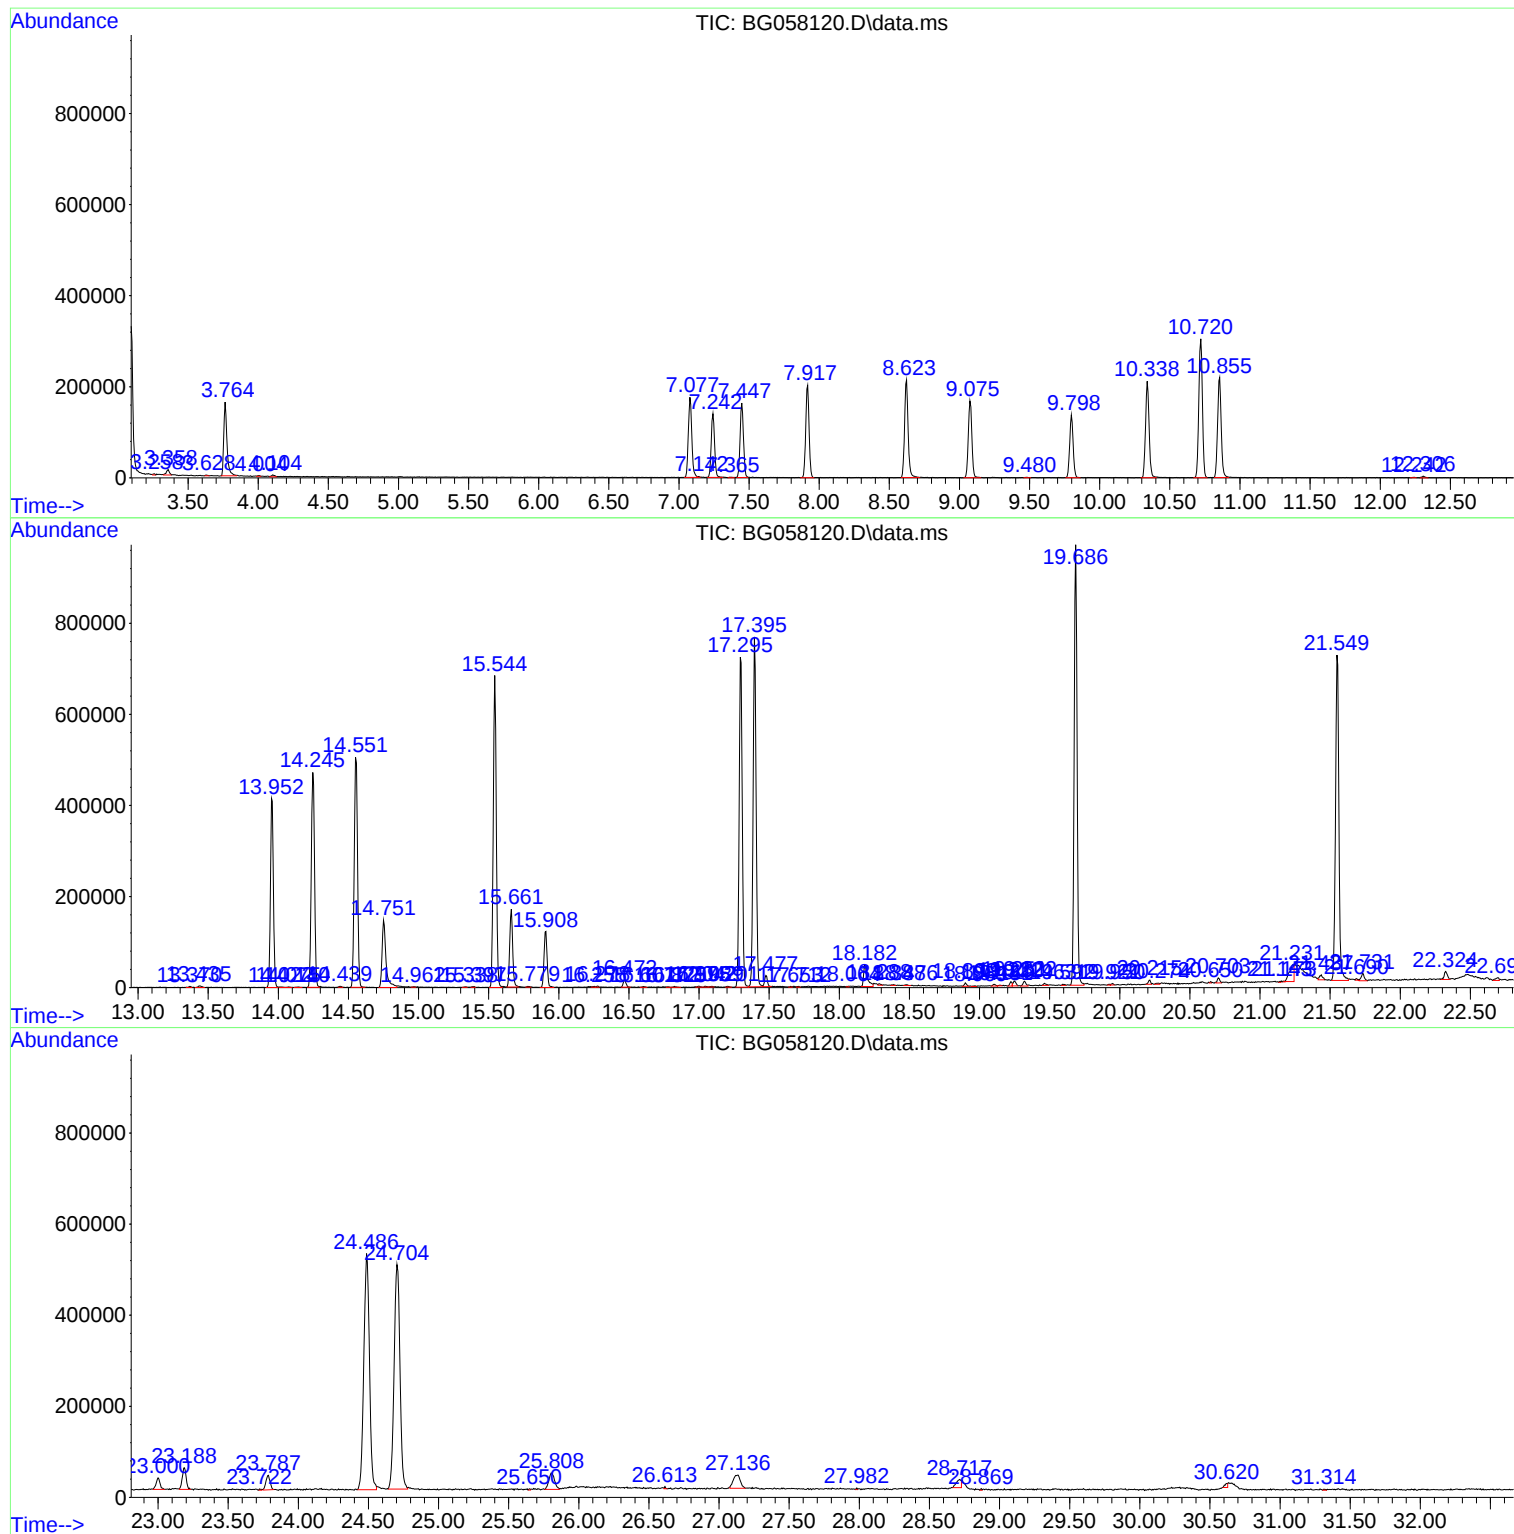

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070823\
Data File : BG058120.D
Acq On : 9 Jul 2023 10:33
Operator : CG/JU
Sample : 03349-10
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
YBW03










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzophenone Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.908	4.43 ng/ul	180703	Acenaphthene-d10	14.551

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzophenone	182	C13H10O	000119-61-9	96
2			Benzophenone	182	C13H10O	000119-61-9	95
3			Benzophenone	182	C13H10O	000119-61-9	94
4			Benzophenone	182	C13H10O	000119-61-9	90
5			Benzophenone	182	C13H10O	000119-61-9	90

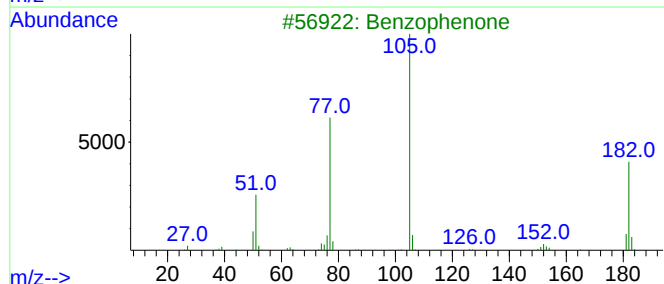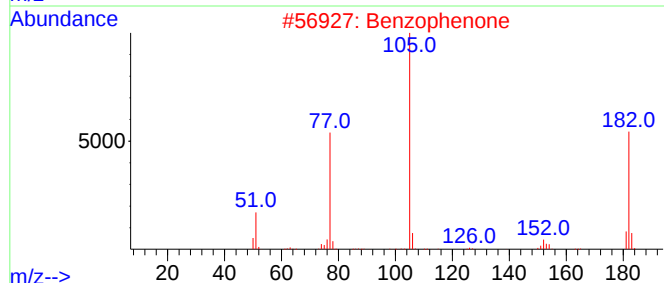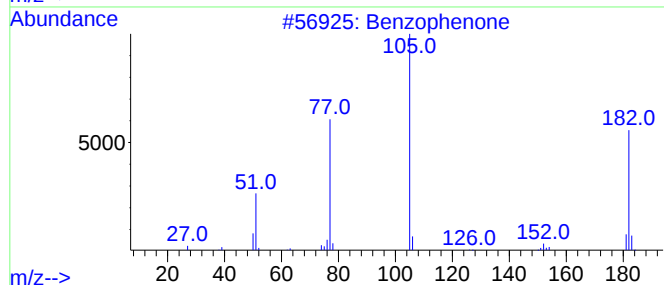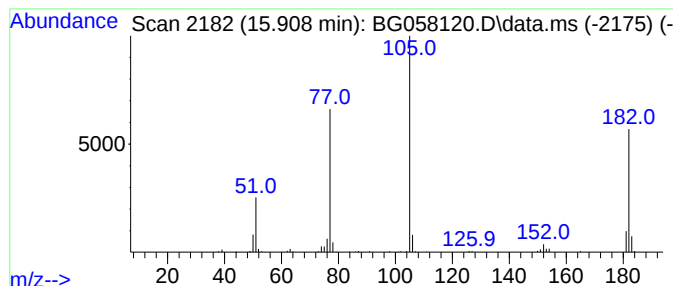

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070823\
Data File : BG058120.D
Acq On : 9 Jul 2023 10:33
Operator : CG/JU
Sample : 03349-10
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
YBW03

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzophenone	15.908	4.4	ng/u1	180703	3	14.551	815304	20.0