


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG070921\
Data File : BG049251.D
Acq On : 10 Jul 2021 00:10
Operator : CG/JU
Sample : M2878-13
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGE04

Manual Integrations
APPROVED

mohammad
7/12/2021 12:33:48 PM

Quant Time: Jul 10 01:06:05 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG070921.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 09 22:53:59 2021
Response via : Initial Calibration

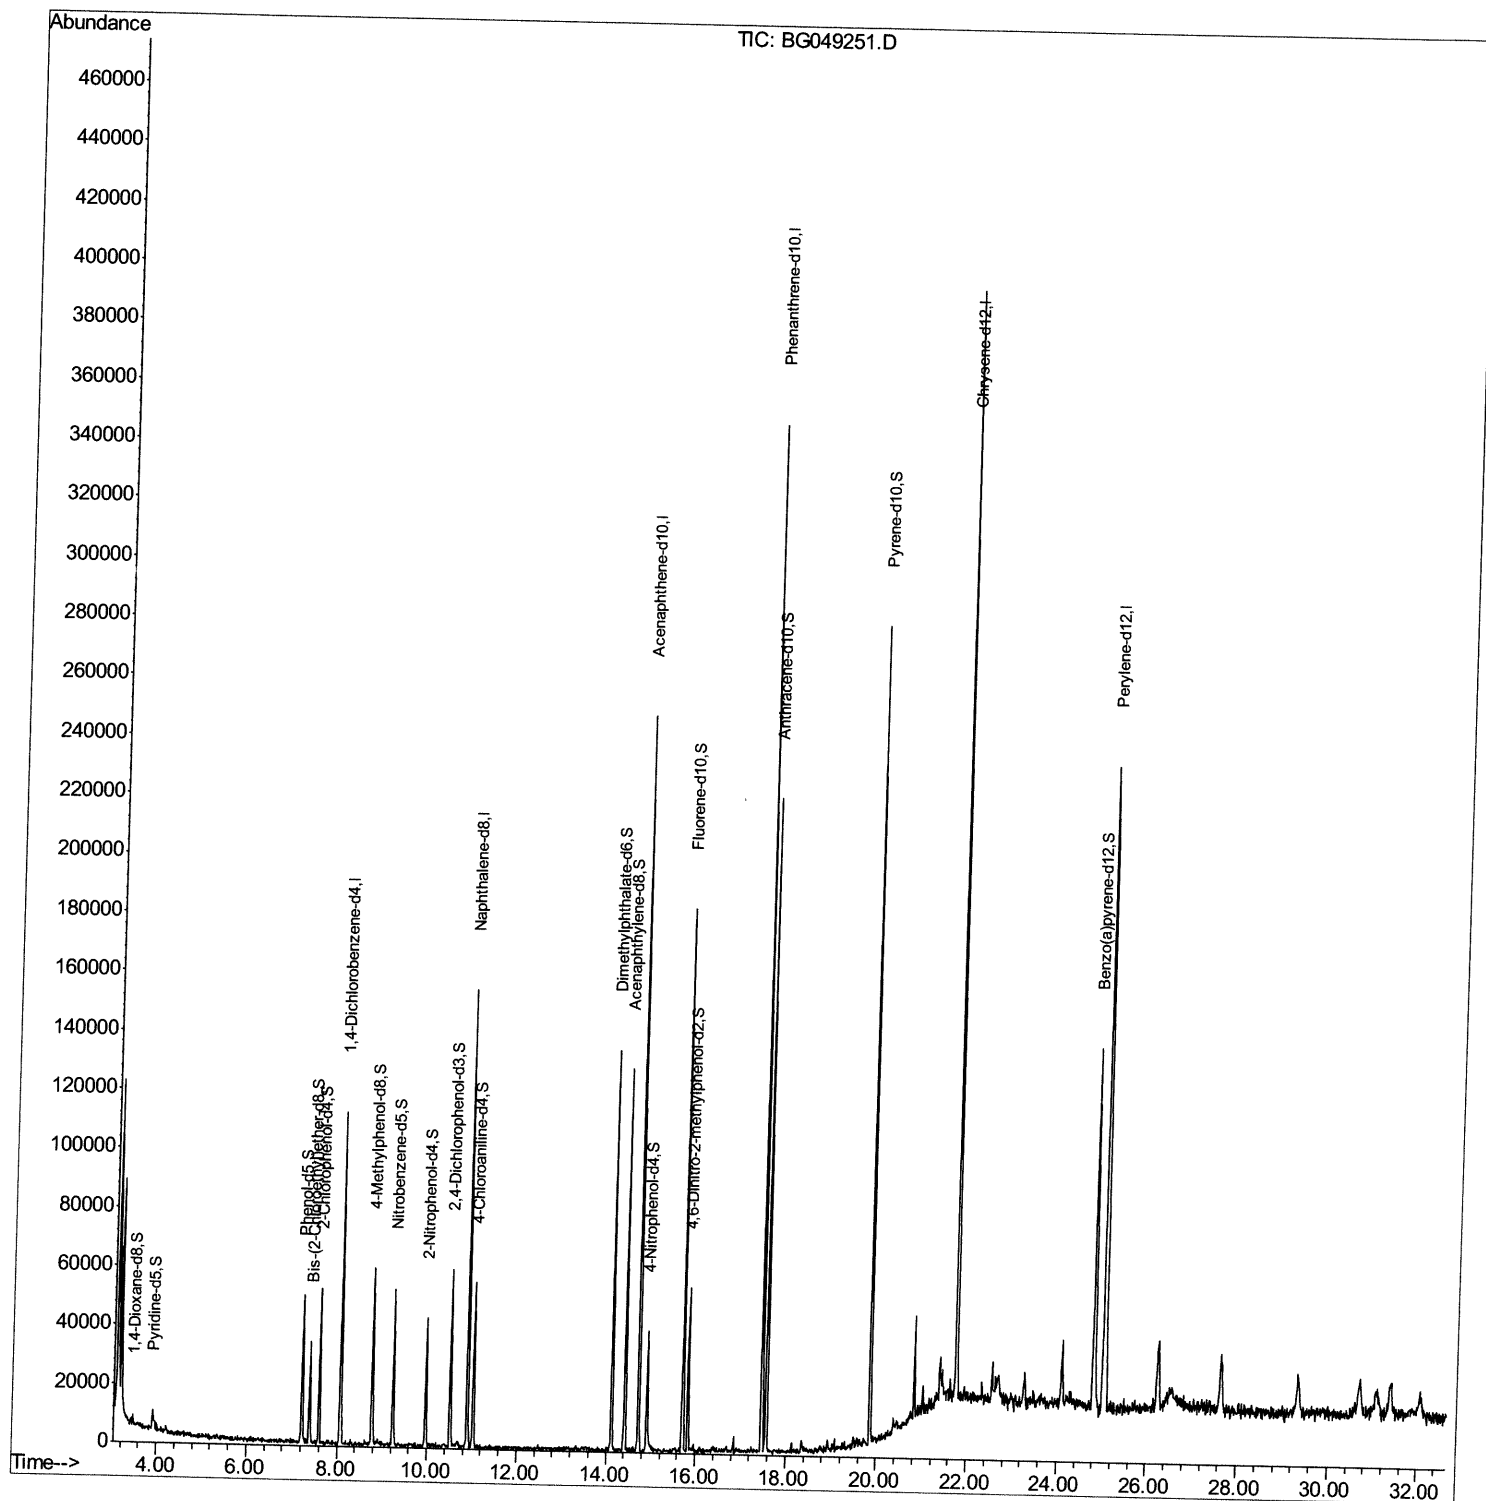

Quantitation Report (Qedit)


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG070921\
 Data File : BG049251.D
 Acq On : 10 Jul 2021 00:10
 Operator : CG/JU
 Sample : M2878-13
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGE04

Manual Integrations
 APPROVED

mohammad
 7/12/2021 12:33:48 PM

Quant Time: Jul 10 01:01:58 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG070921.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 09 22:53:59 2021
 Response via : Initial Calibration

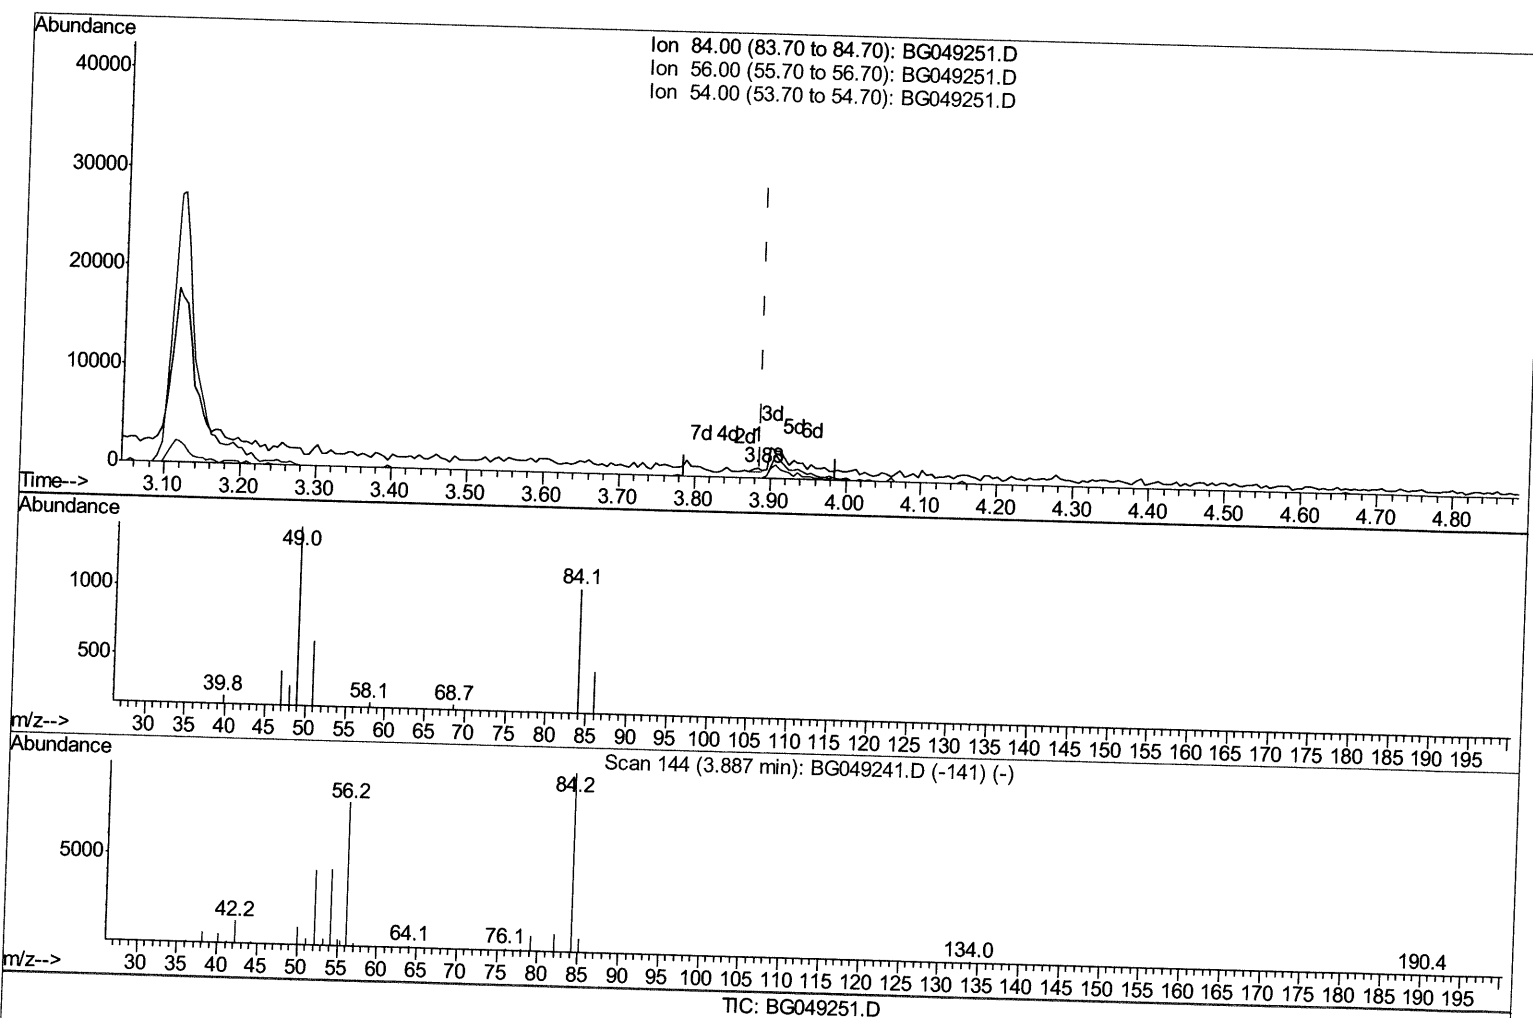

(4) Pyridine-d5 (S)

3.884min (-0.003) 0.14ng/ul

response 263

Ion	Exp%	Act%
84.00	100	100
56.00	76.20	0.00#
54.00	42.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG070921\
 Data File : BG049251.D
 Acq On : 10 Jul 2021 00:10
 Operator : CG/JU
 Sample : M2878-13
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGE04

Manual Integrations
 APPROVED

mohammad
 7/12/2021 12:33:48 PM

Quant Time: Jul 10 01:01:58 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG070921.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 09 22:53:59 2021
 Response via : Initial Calibration

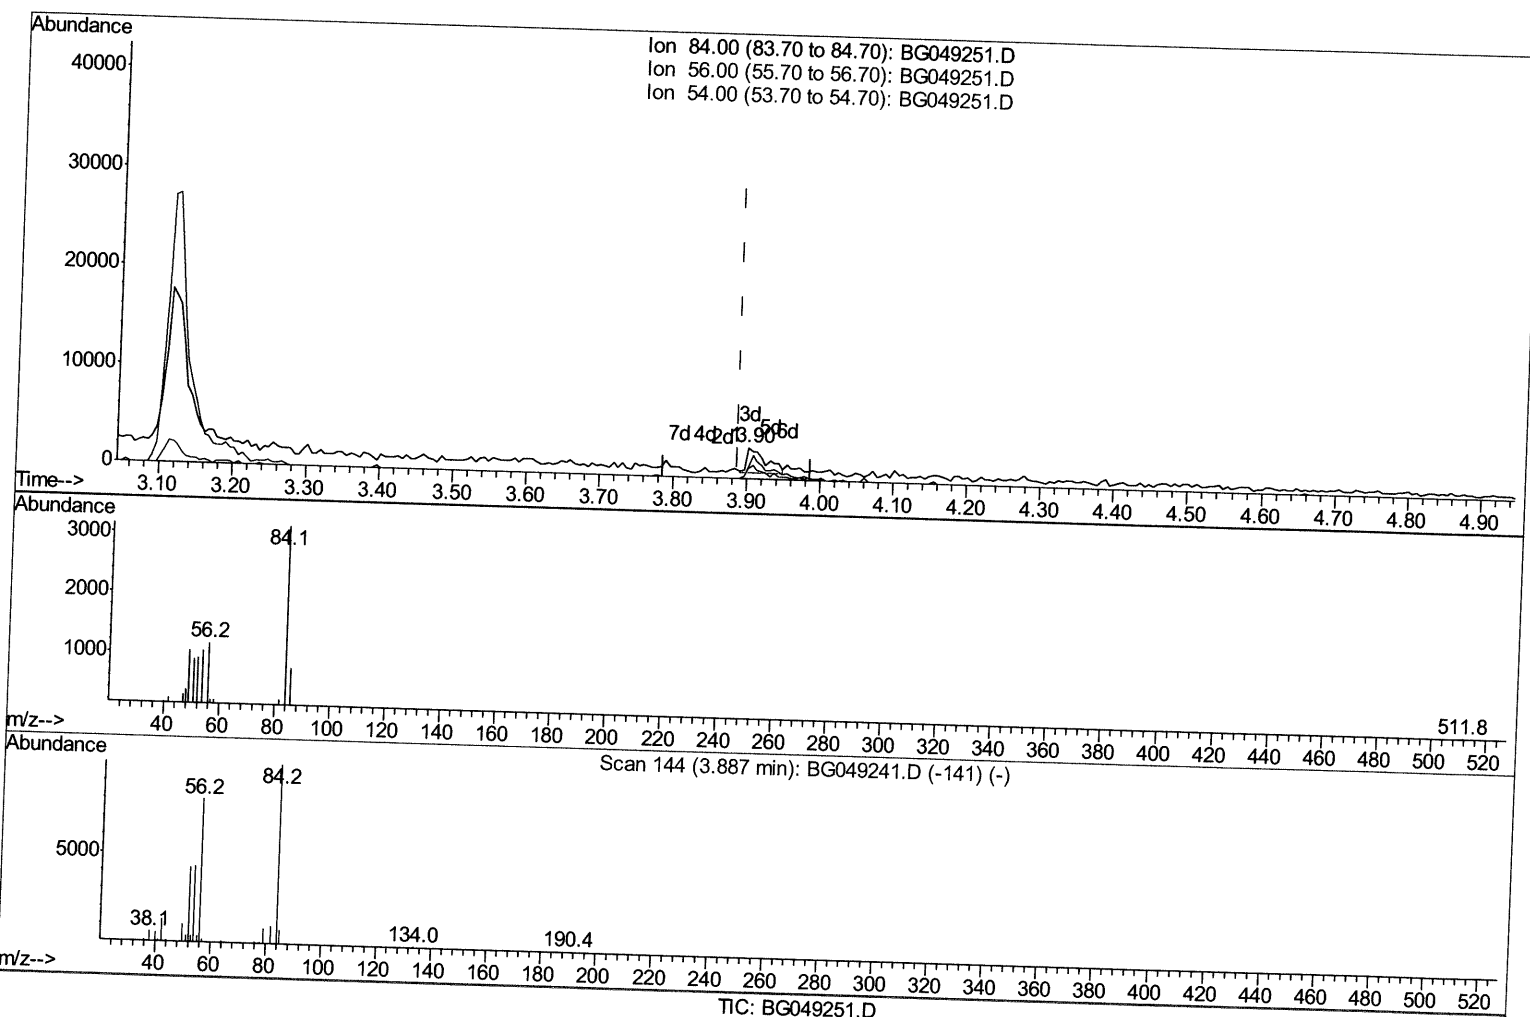

(4) Pyridine-d5 (S)

3.901min (+0.015) 2.42ng/ul m 07/13/21 JU

response 4442

Ion	Exp%	Act%
84.00	100	100
56.00	76.20	37.05#
54.00	42.60	32.95#
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG070921\
 Data File : BG049251.D
 Acq On : 10 Jul 2021 00:10
 Operator : CG/JU
 Sample : M2878-13
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGE04

Manual Integrations
 APPROVED

mohammad
 7/12/2021 12:33:48 PM

Quant Time: Jul 10 01:06:05 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG070921.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 09 22:53:59 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.07	152	29320	20.00	ng/ul	0.00
20) Naphthalene-d8	10.89	136	125445	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.72	164	91144	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.47	188	223023	20.00	ng/ul	0.00
79) Chrysene-d12	21.75	240	240630	20.00	ng/ul	0.00
88) Perylene-d12	25.05	264	245504	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.47	96	1146	1.84	ng/uL	0.00
4) Pyridine-d5	3.90	84	4442m >	2.42	ng/ul >	0.01
7) Phenol-d5	7.22	99	25773	10.11	ng/ul	0.00
9) Bis-(2-Chloroethyl)ether-d	7.39	67	17429	11.78	ng/ul	0.00
11) 2-Chlorophenol-d4	7.60	132	21486	11.40	ng/ul	0.00
15) 4-Methylphenol-d8	8.78	113	22129	10.83	ng/ul	0.00
21) Nitrobenzene-d5	9.24	128	10819	11.24	ng/ul	0.00
24) 2-Nitrophenol-d4	9.96	143	13329	12.06	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.51	165	23051	10.69	ng/ul	0.00
31) 4-Chloroaniline-d4	11.02	131	28230	10.05	ng/ul	0.00
46) Dimethylphthalate-d6	14.12	166	89010	12.70	ng/ul	0.00
49) Acenaphthylene-d8	14.41	160	94546	11.50	ng/ul	0.00
54) 4-Nitrophenol-d4	14.91	143	10641	9.17	ng/ul	0.00
60) Fluorene-d10	15.71	176	75270	12.68	ng/ul	0.00
65) 4,6-Dinitro-2-methylphenol	15.82	200	13313	9.39	ng/ul	0.00
73) Anthracene-d10	17.57	188	129910	12.79	ng/ul	0.00
81) Pyrene-d10	19.85	212	151355	12.27	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.82	264	141016	11.05	ng/ul	0.00

Target Compounds

Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed