

(QT Reviewed)


```
Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG070921\  
Data File : BG049294.D  
Acq On    : 11 Jul 2021 10:48  
Operator  : CG/JU  
Sample    : M2958-01  
Misc      :  
ALS Vial  : 65      Sample Multiplier: 1
```

Instrument :
BNA_G
ClientSampleId :
DBK23

Manual Integrations

mohammad
7/13/2021 8:08:01 AM

Quant Time: Jul 12 01:41:07 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG070921.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 09 03:15:38 2021
Response via : Initial Calibration

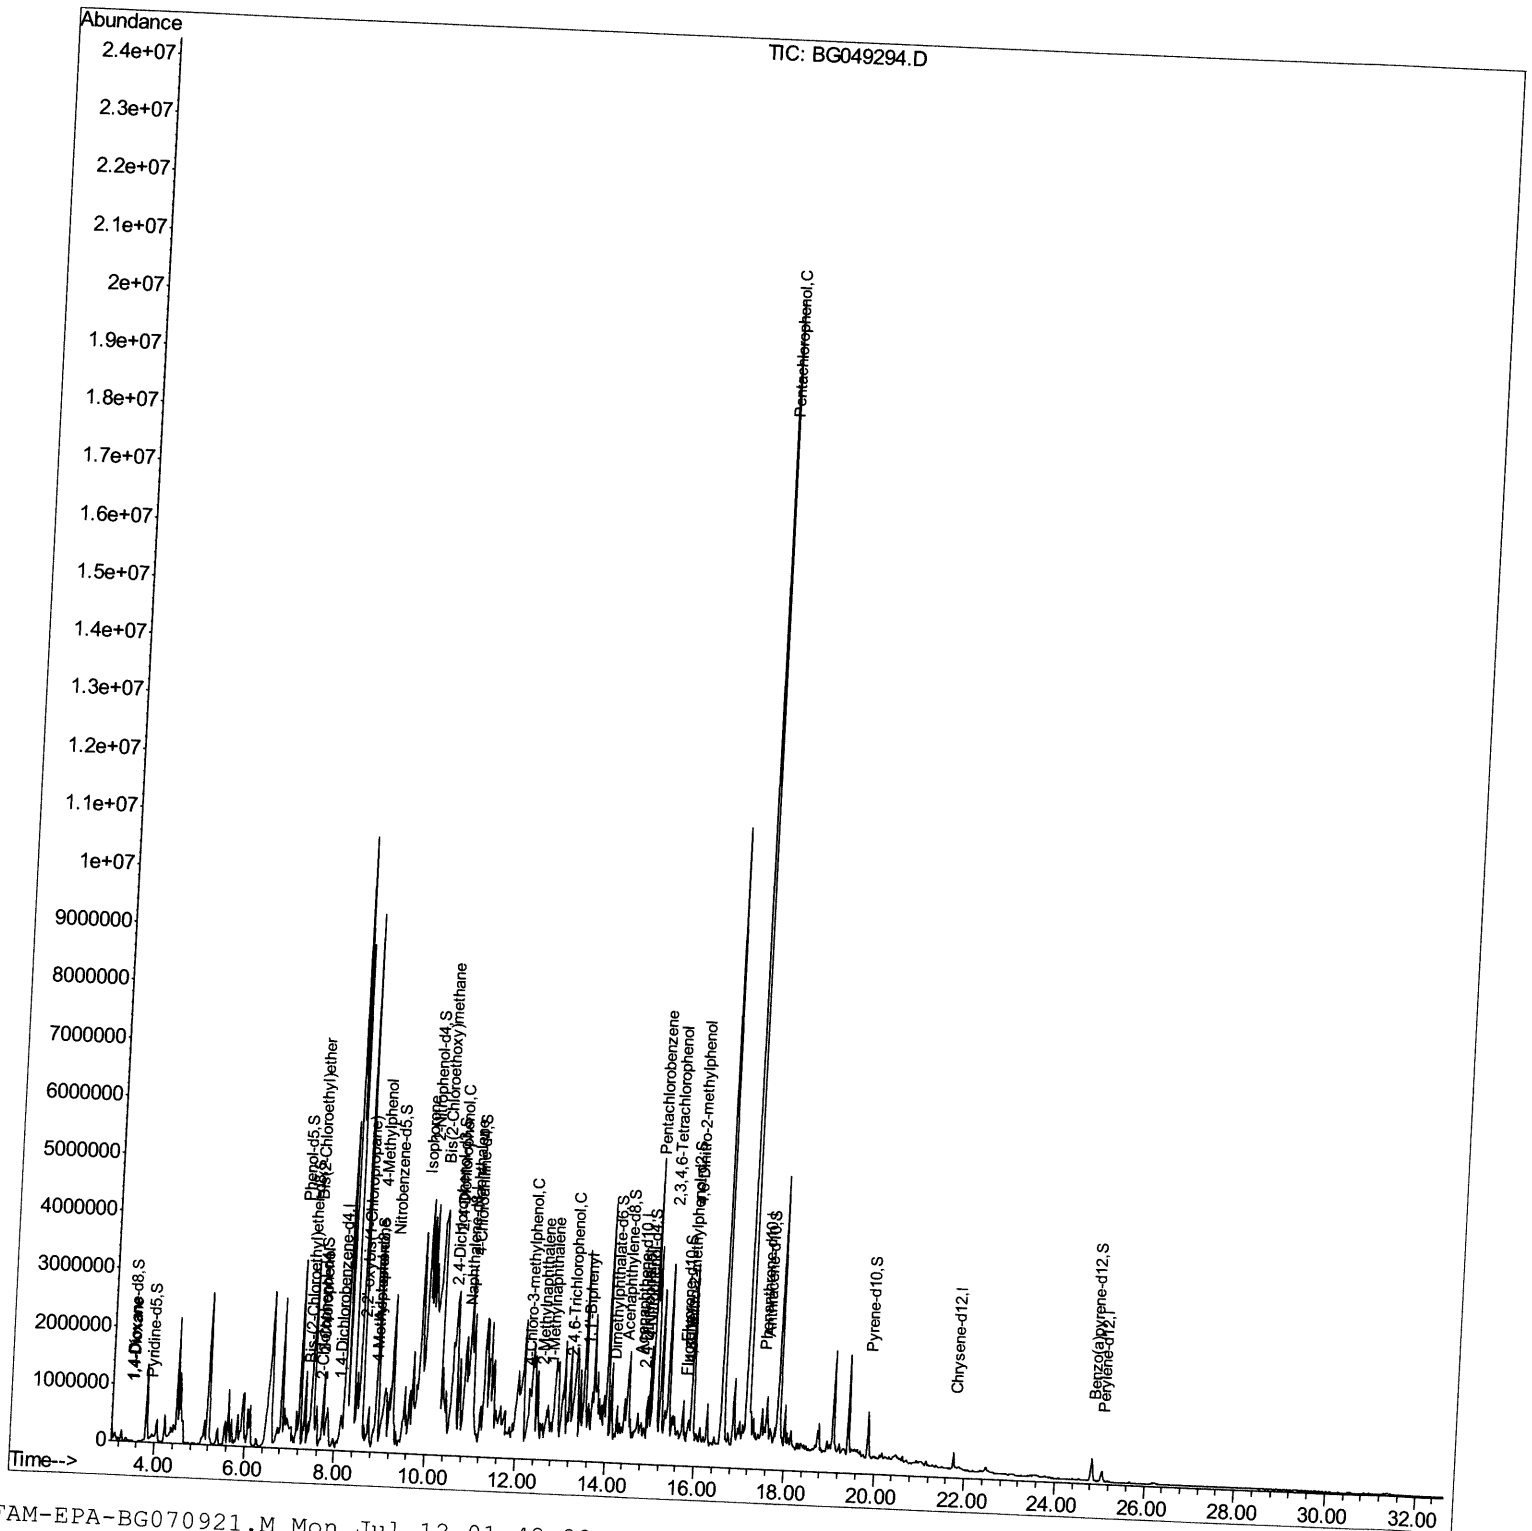

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG070921\
 Data File : BG049294.D
 Acq On : 11 Jul 2021 10:48
 Operator : CG/JU
 Sample : M2958-01
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBK23

Manual Integrations
 APPROVED

mohammad
 7/13/2021 8:08:01 AM

Quant Time: Jul 12 01:04:14 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG070921.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 09 03:15:38 2021
 Response via : Initial Calibration

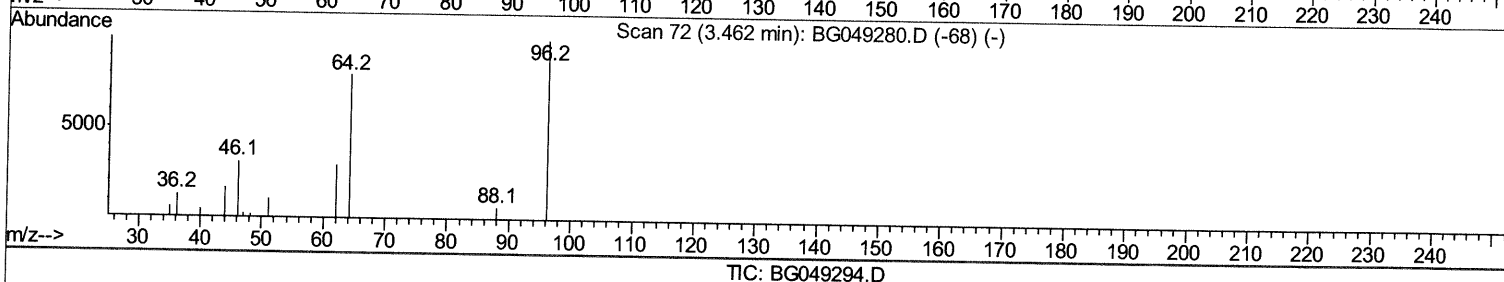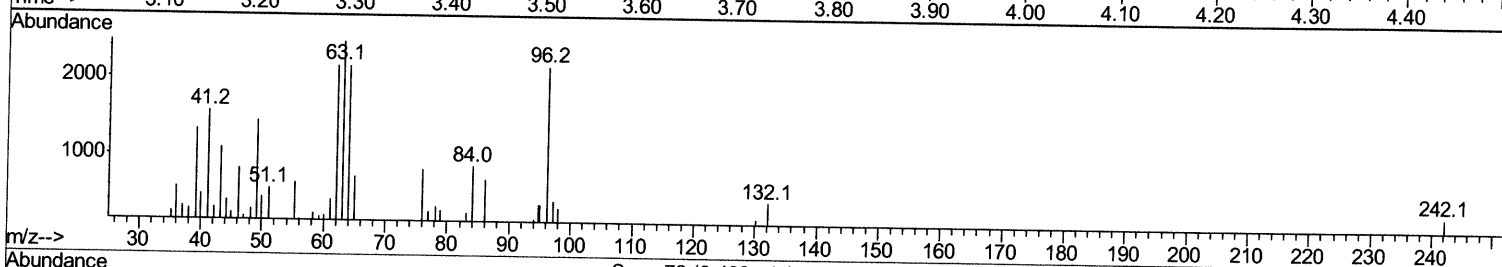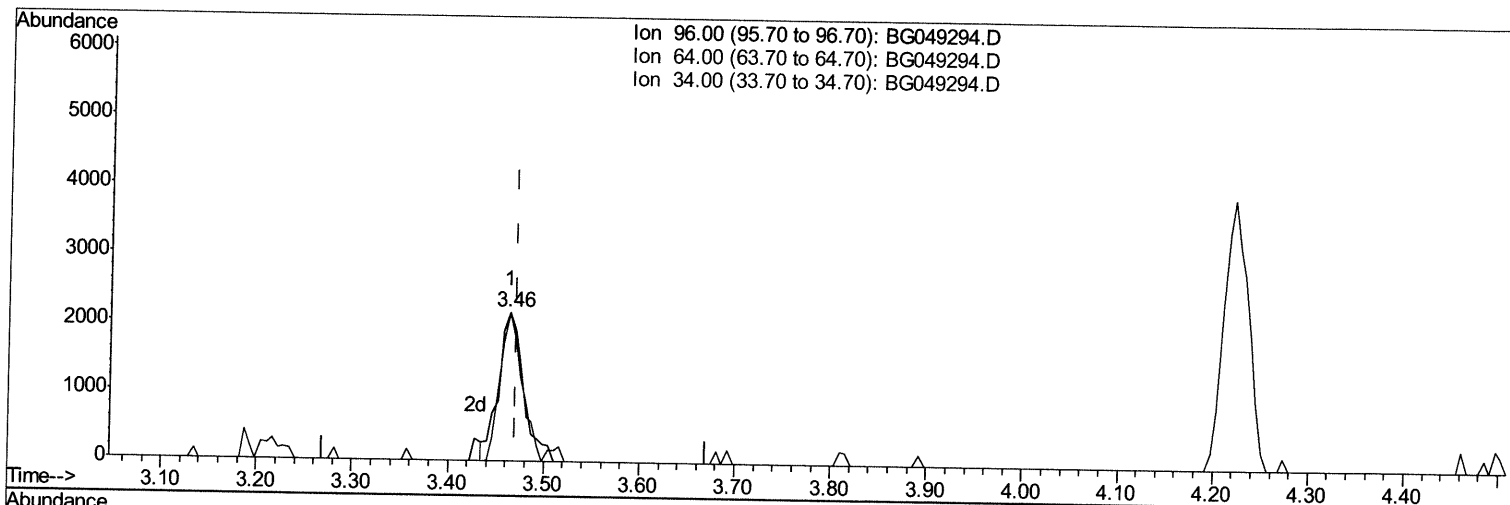

(3) 1,4-Dioxane-d8 (S)

3.463min (-0.007) 6.67ng/uL

response 3836

Ion	Exp%	Act%
96.00	100	100
64.00	62.20	99.91#
34.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG070921\
Data File : BG049294.D
Acq On : 11 Jul 2021 10:48
Operator : CG/JU
Sample : M2958-01
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBK23

Manual Integrations
APPROVED

mohammad
7/13/2021 8:08:01 AM

Quant Time: Jul 12 01:04:14 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG070921.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 09 03:15:38 2021
Response via : Initial Calibration

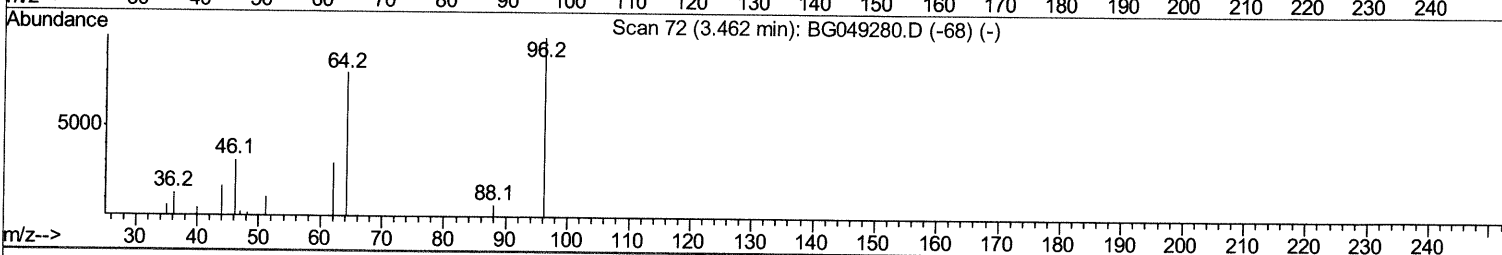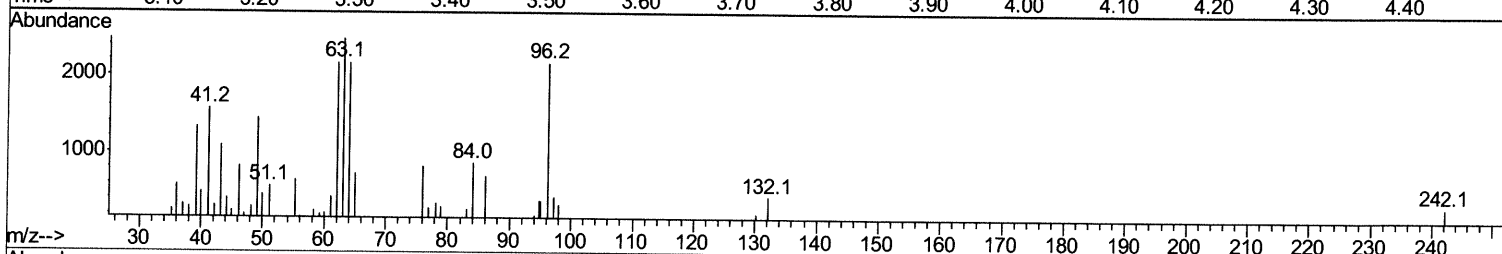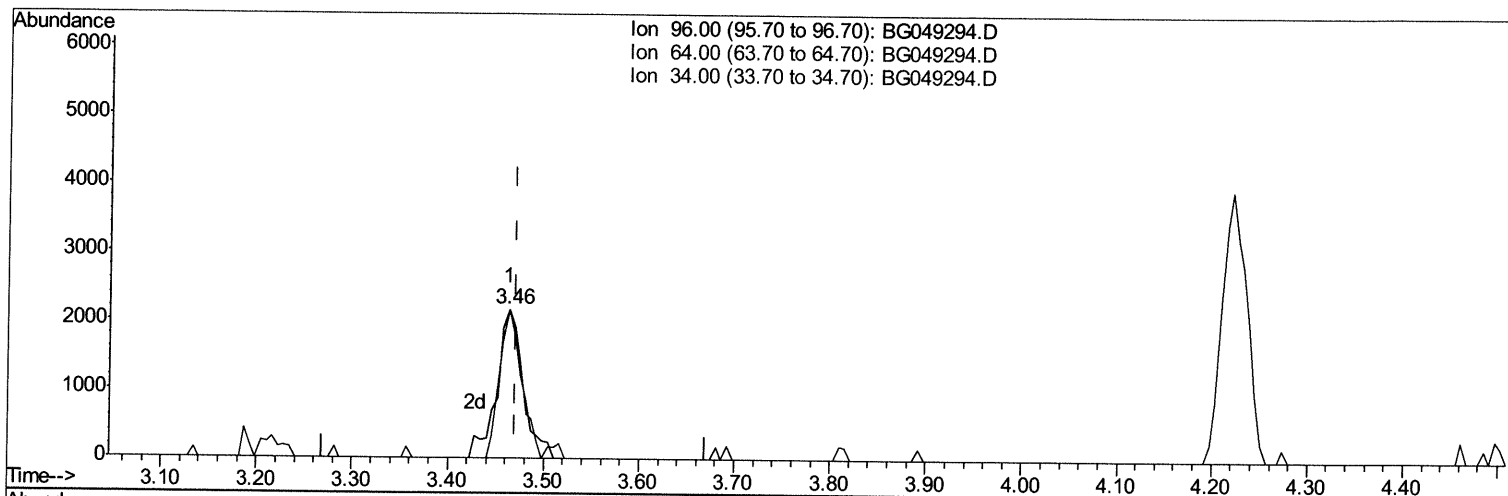

TIC: BG049294.D

(3) 1,4-Dioxane-d8 (S)

3.463min (-0.007) 7.03ng/uL m 0 7/13/21 JU

response 4045

Ion	Exp%	Act%
96.00	100	100
64.00	62.20	99.91#
34.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG070921\
 Data File : BG049294.D
 Acq On : 11 Jul 2021 10:48
 Operator : CG/JU
 Sample : M2958-01
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_G
ClientSampleId :
 DBK23

Manual Integrations
APPROVED

mohammad
 7/13/2021 8:08:01 AM

Quant Time: Jul 12 01:27:40 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG070921.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 09 03:15:38 2021
 Response via : Initial Calibration

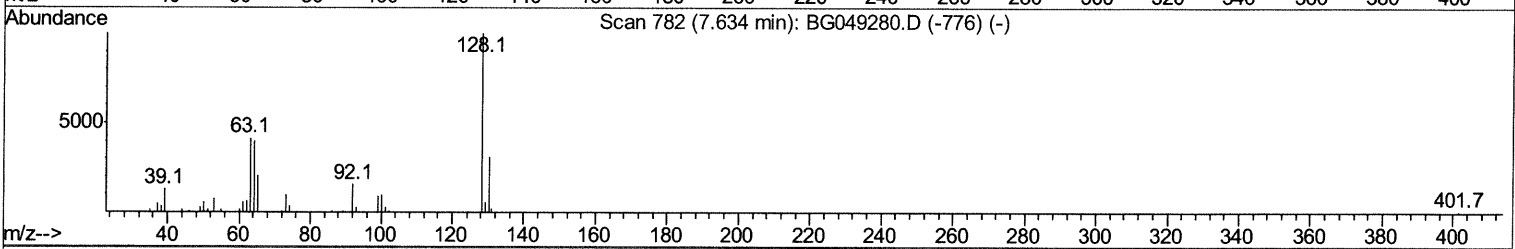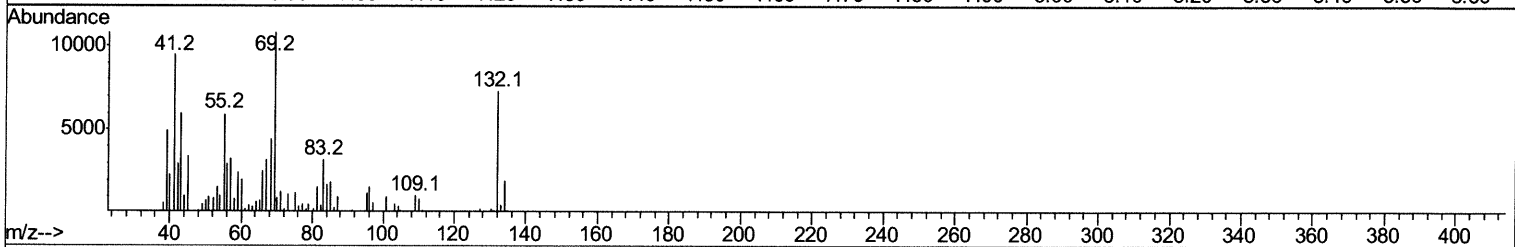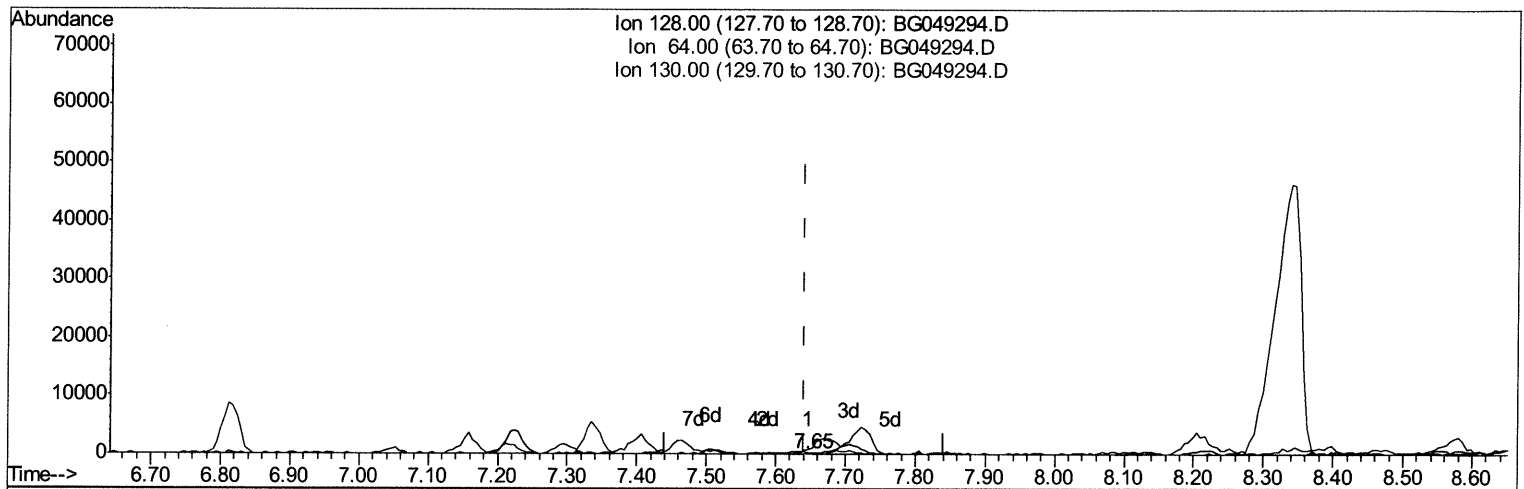

TIC: BG049294.D

(12) 2-Chlorophenol

7.646min (+0.005) 0.03ng/ul

response 59

Ion	Exp%	Act%
128.00	100	100
64.00	57.50	450.00#
130.00	33.40	176.19#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG070921\
 Data File : BG049294.D
 Acq On : 11 Jul 2021 10:48
 Operator : CG/JU
 Sample : M2958-01
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBK23

Manual Integrations
 APPROVED

mohammad
 7/13/2021 8:08:01 AM

Quant Time: Jul 12 01:27:40 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG070921.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 09 03:15:38 2021
 Response via : Initial Calibration

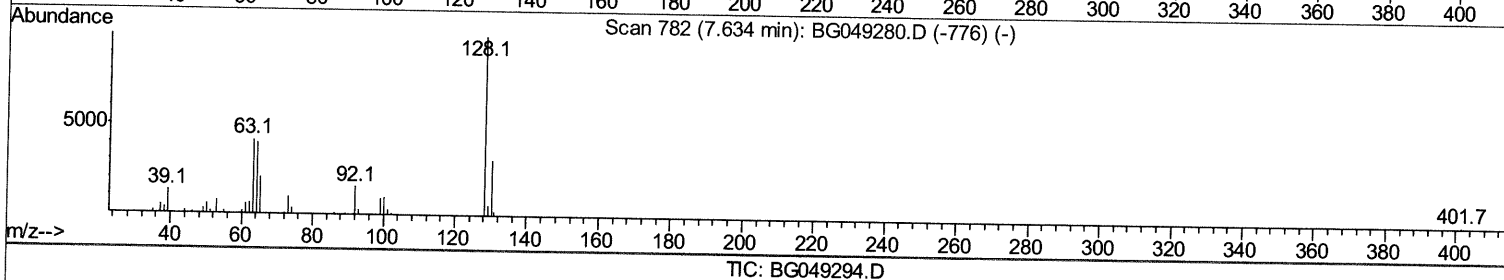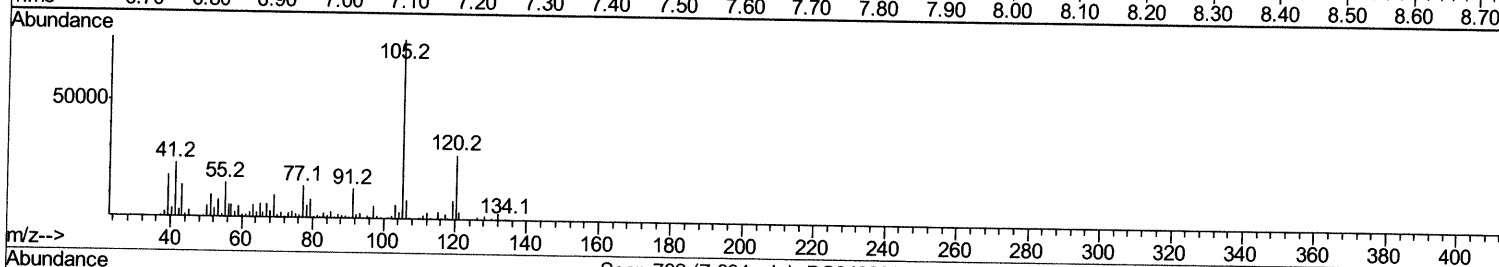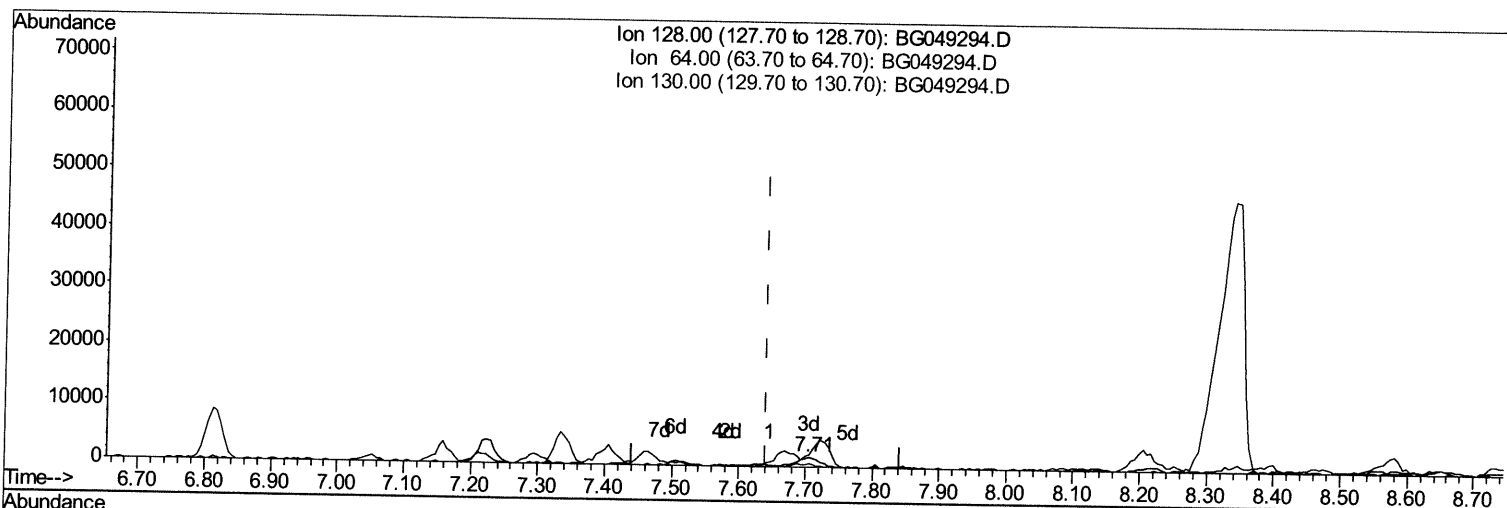

(12) 2-Chlorophenol

7.705min (+0.064) 2.35ng/ul m 07/13/21JU

response 4127

Ion	Exp%	Act%
128.00	100	100
64.00	57.50	127.58#
130.00	33.40	39.18
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG070921\
Data File : BG049294.D
Acq On : 11 Jul 2021 10:48
Operator : CG/JU
Sample : M2958-01
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBK23

Manual Integrations
APPROVED

mohammad
7/13/2021 8:08:01 AM

Quant Time: Jul 12 01:28:32 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG070921.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 09 03:15:38 2021
Response via : Initial Calibration

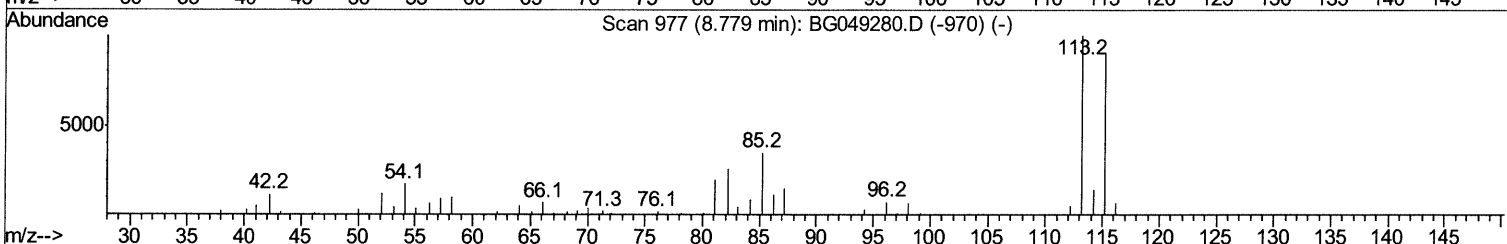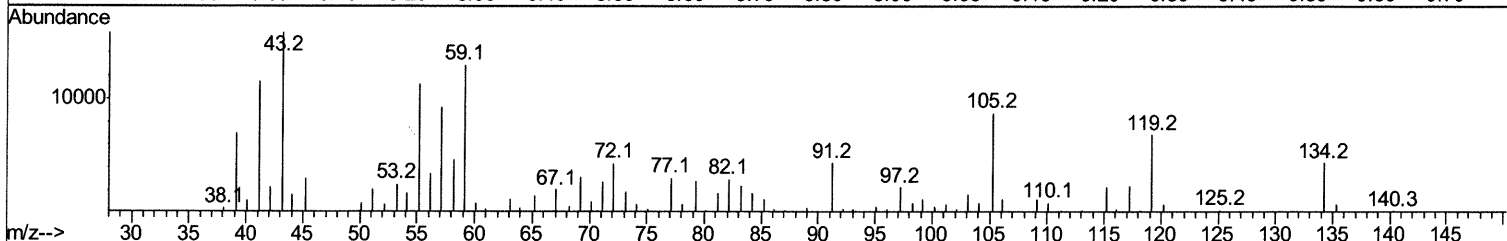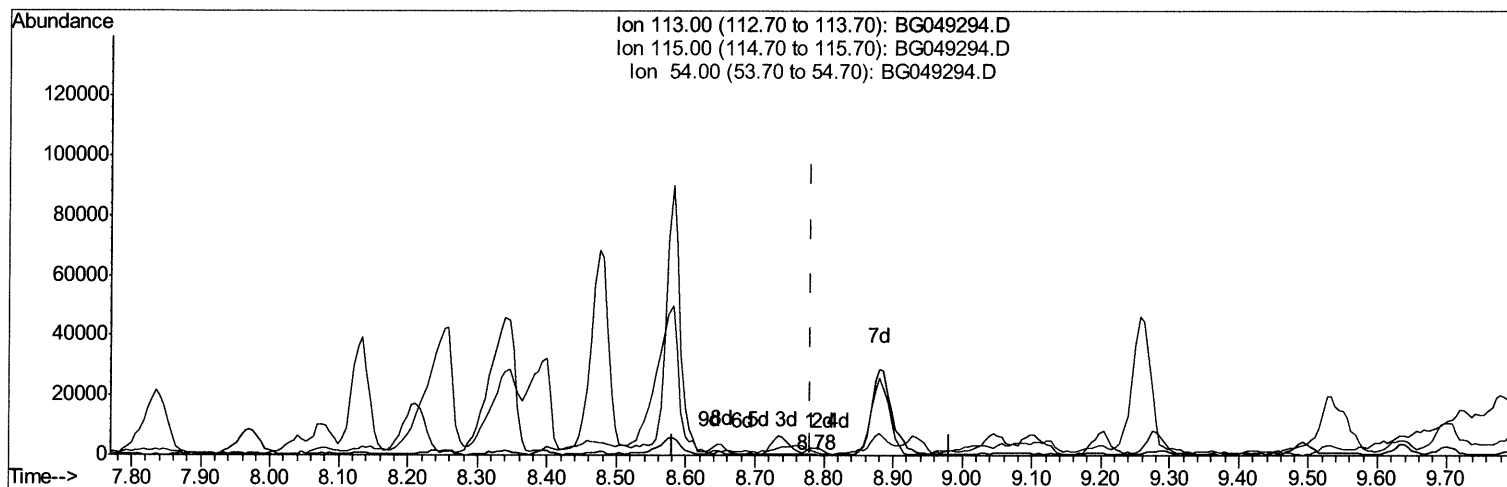

TIC: BG049294.D

(15) 4-Methylphenol-d8 (S)

8.780min (-0.001) 0.06ng/ul

response 120

Ion	Exp%	Act%
113.00	100	100
115.00	99.50	691.29#
54.00	19.50	544.74#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG070921\
Data File : BG049294.D
Acq On : 11 Jul 2021 10:48
Operator : CG/JU
Sample : M2958-01
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampled :
DBK23

Manual Integrations
APPROVED

mohammad
7/13/2021 8:08:01 AM

Quant Time: Jul 12 01:28:32 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG070921.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 09 03:15:38 2021
Response via : Initial Calibration

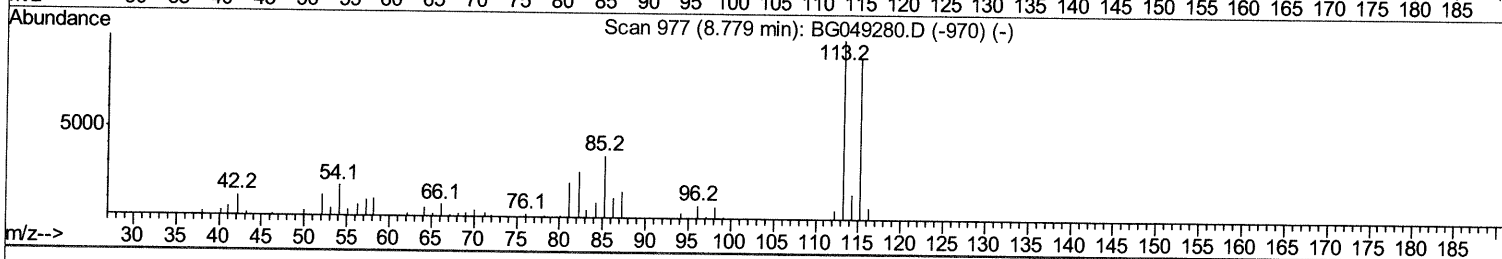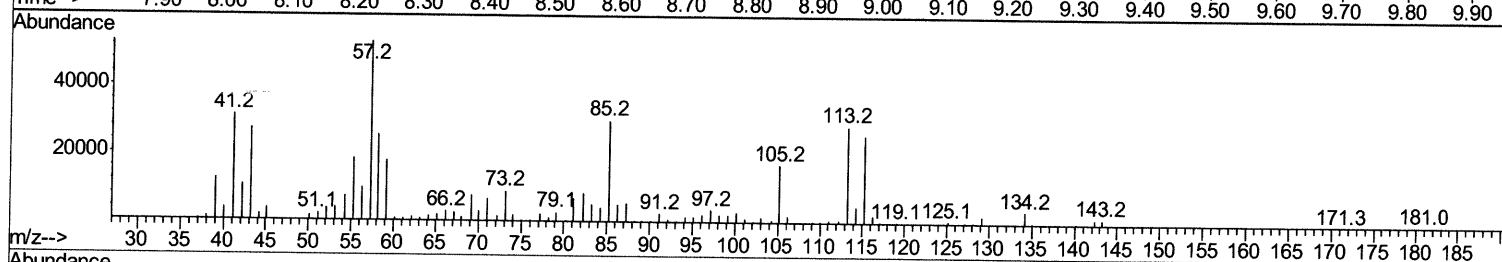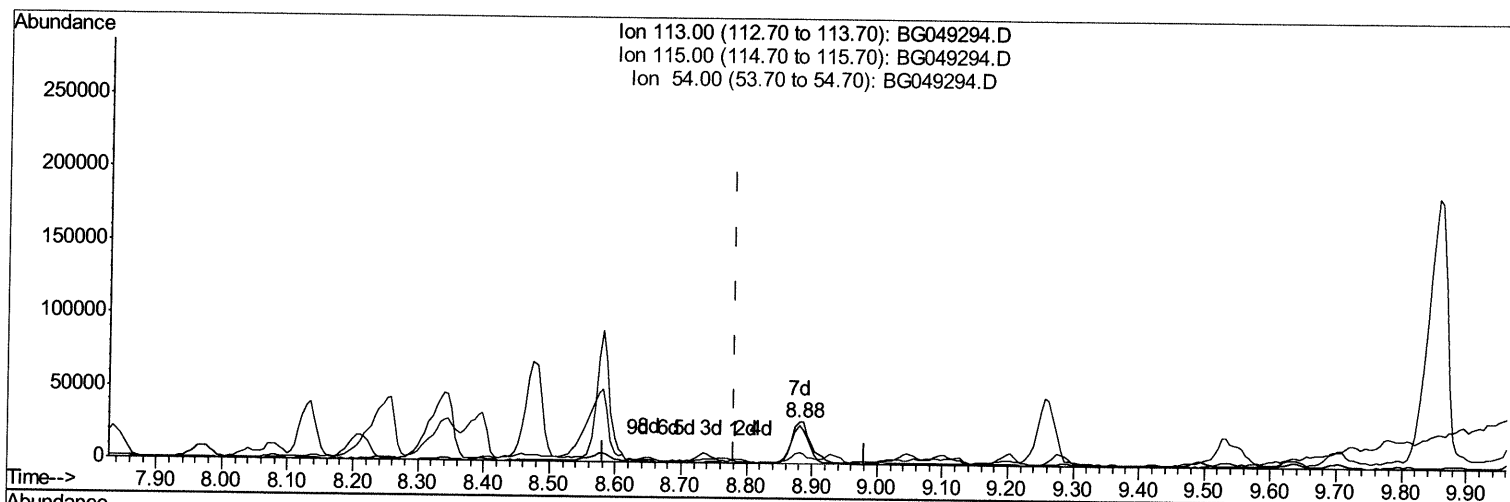

TIC: BG049294.D

(15) 4-Methylphenol-d8 (S)

8.880min (+0.099) 32.02ng/ul m 07/13/2021

response 60404

Ion	Exp%	Act%
113.00	100	100
115.00	99.50	90.83
54.00	19.50	26.02#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG070921\
Data File : BG049294.D
Acq On : 11 Jul 2021 10:48
Operator : CG/JU
Sample : M2958-01
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBK23

Manual Integrations
APPROVED

mohammad
7/13/2021 8:08:01 AM

Quant Time: Jul 12 01:31:20 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG070921.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 09 03:15:38 2021
Response via : Initial Calibration

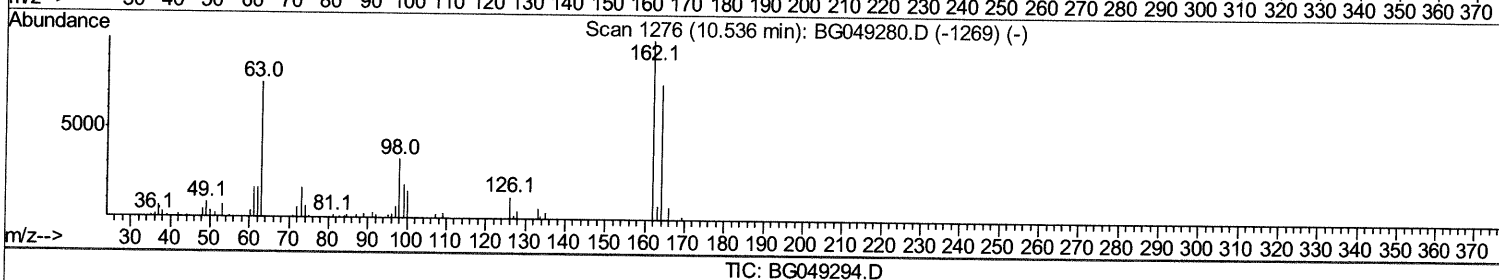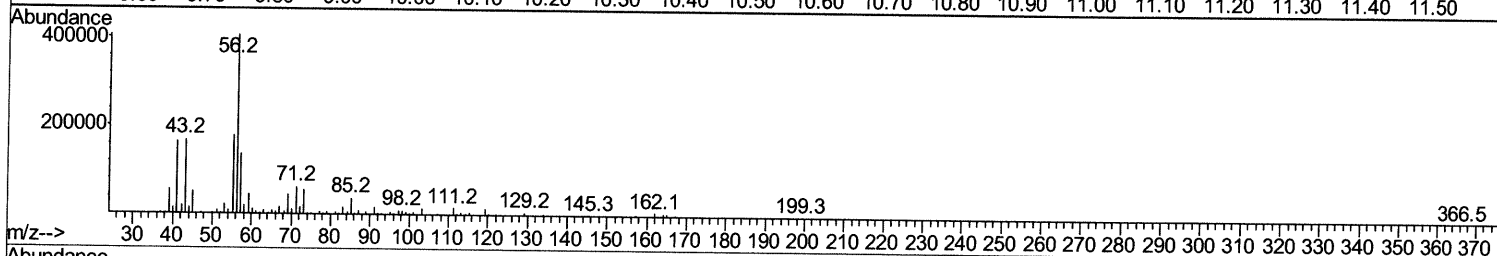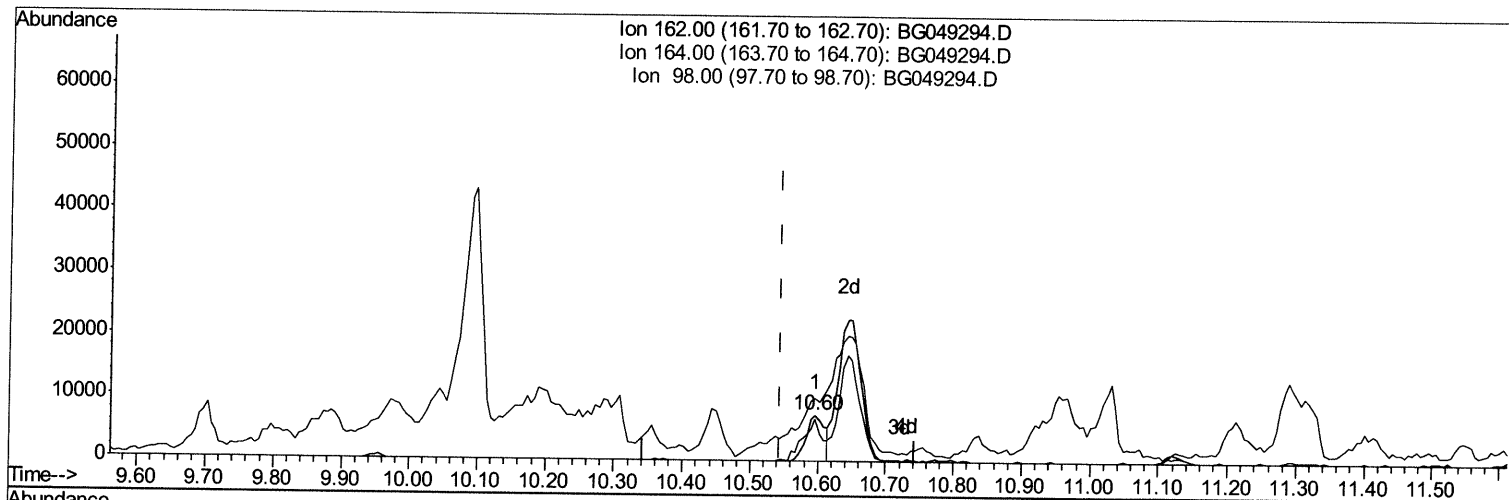

(29) 2,4-Dichlorophenol (C)

10.596min (+0.052) 7.61ng/ul

response 14064

Ion	Exp%	Act%
162.00	100	100
164.00	66.80	92.58#
98.00	32.30	135.60#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG070921\
Data File : BG049294.D
Acq On : 11 Jul 2021 10:48
Operator : CG/JU
Sample : M2958-01
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBK23

Manual Integrations
APPROVED

mohammad
7/13/2021 8:08:01 AM

Quant Time: Jul 12 01:31:20 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG070921.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 09 03:15:38 2021
Response via : Initial Calibration

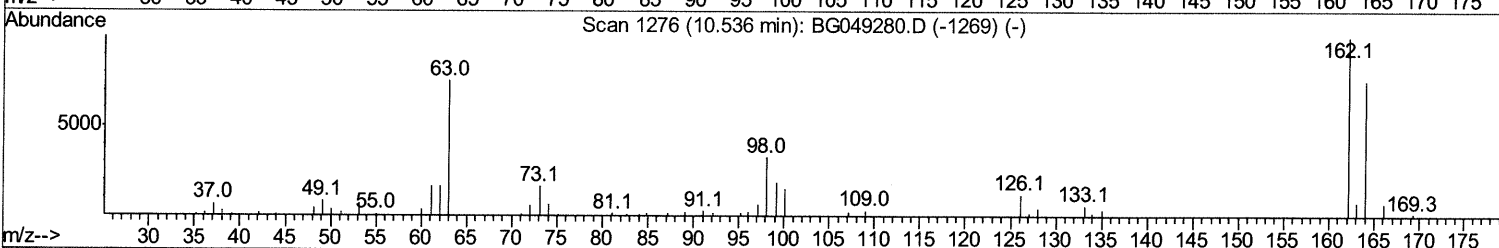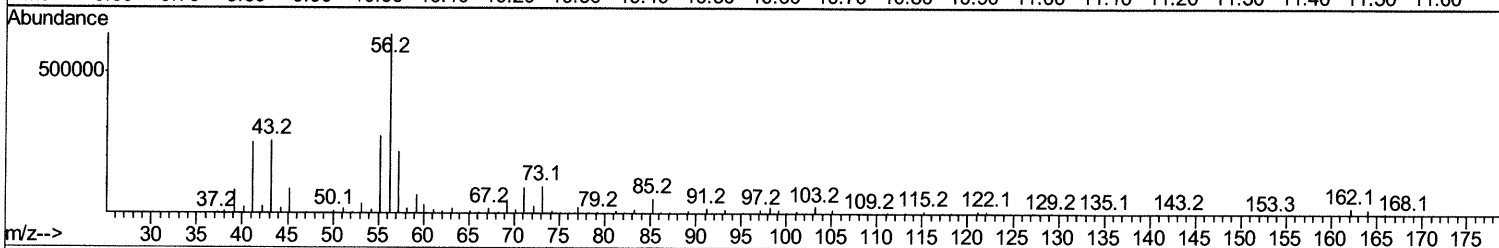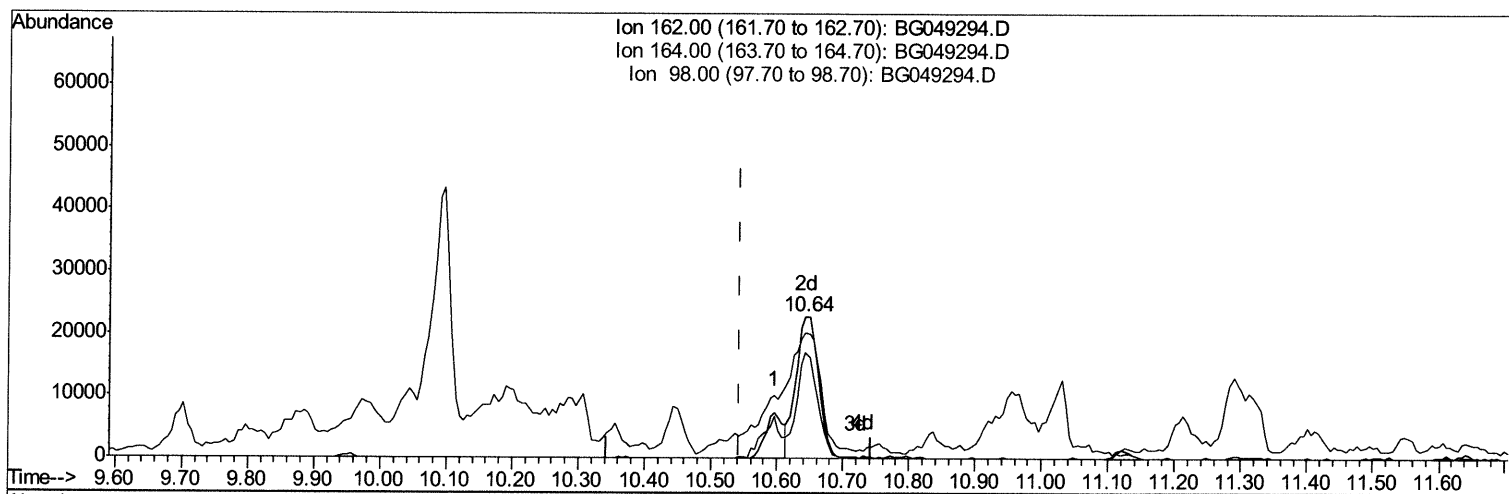

TIC: BG049294.D

(29) 2,4-Dichlorophenol (C)

10.643min (+0.099) 28.87ng/ul m 07/13/21 JU

response 53375

Ion	Exp%	Act%
162.00	100	100
164.00	66.80	74.68
98.00	32.30	88.13#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG070921\
 Data File : BG049294.D
 Acq On : 11 Jul 2021 10:48
 Operator : CG/JU
 Sample : M2958-01
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_G
ClientSampleId :
 DBK23

Manual Integrations
APPROVED

mohammad
 7/13/2021 8:08:01 AM

Quant Time: Jul 12 01:33:01 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG070921.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 09 03:15:38 2021
 Response via : Initial Calibration

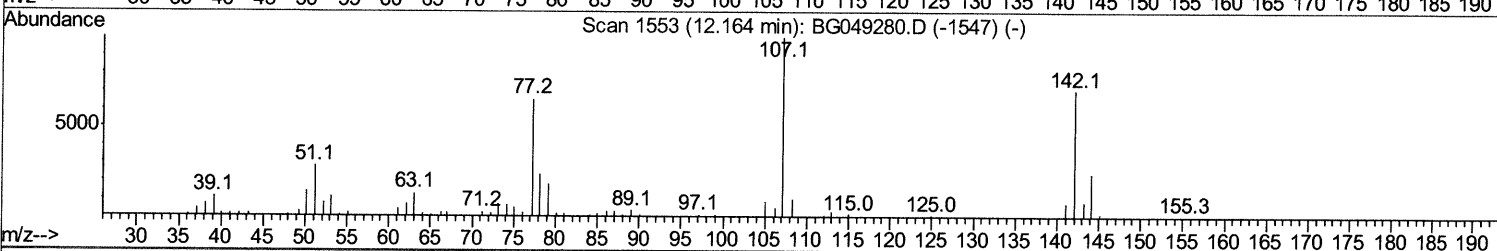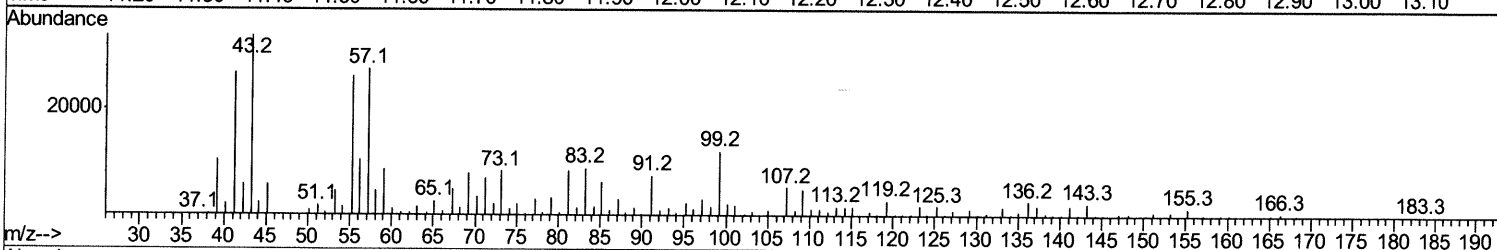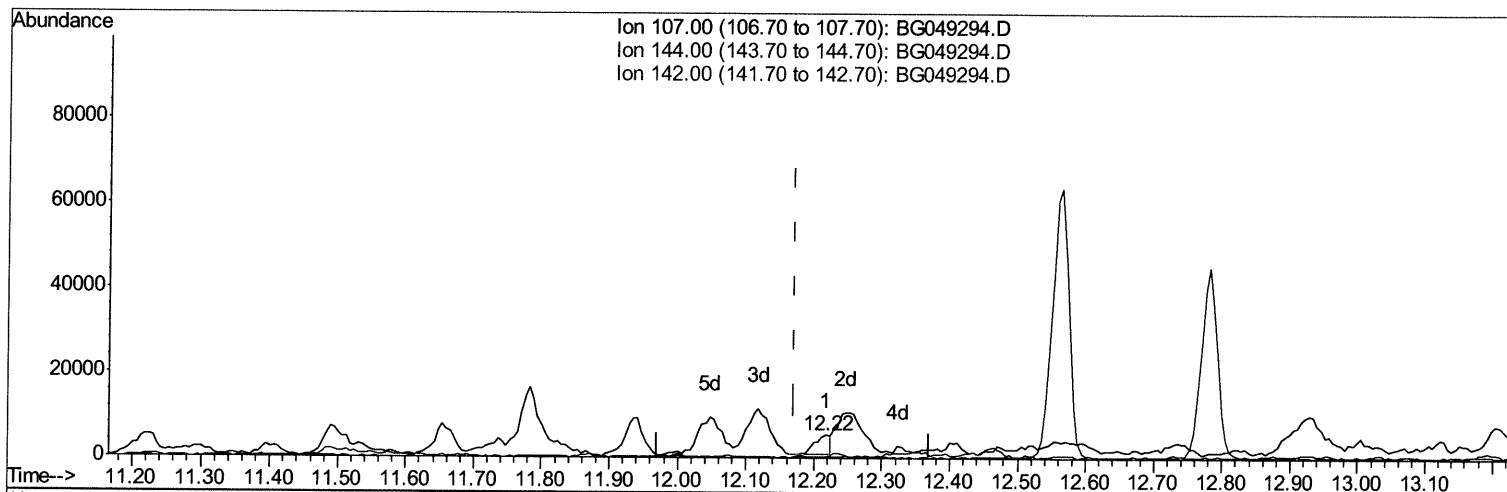

TIC: BG049294.D

(35) 4-Chloro-3-methylphenol (C)

12.218min (+0.046) 3.58ng/ul

response 7393

Ion	Exp%	Act%
107.00	100	100
144.00	27.90	5.60#
142.00	80.90	7.47#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG070921\
 Data File : BG049294.D
 Acq On : 11 Jul 2021 10:48
 Operator : CG/JU
 Sample : M2958-01
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBK23

Manual Integrations
 APPROVED

mohammad
 7/13/2021 8:08:01 AM

Quant Time: Jul 12 01:33:01 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG070921.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 09 03:15:38 2021
 Response via : Initial Calibration

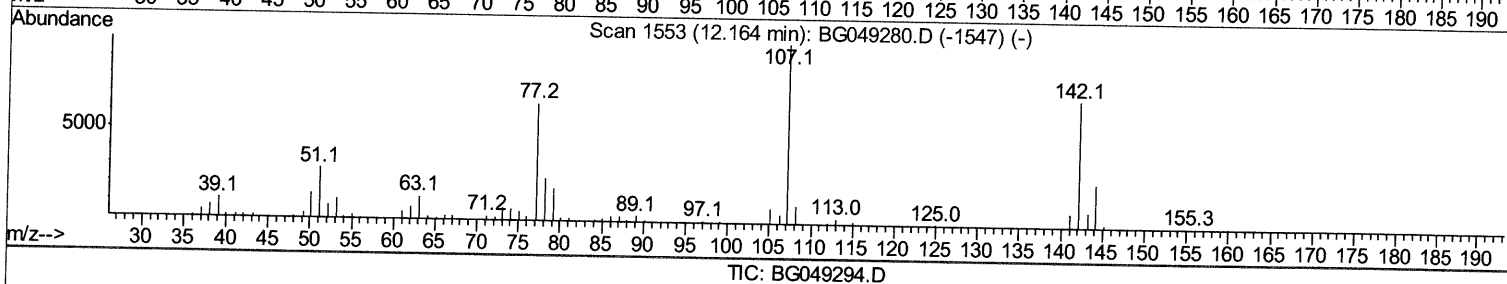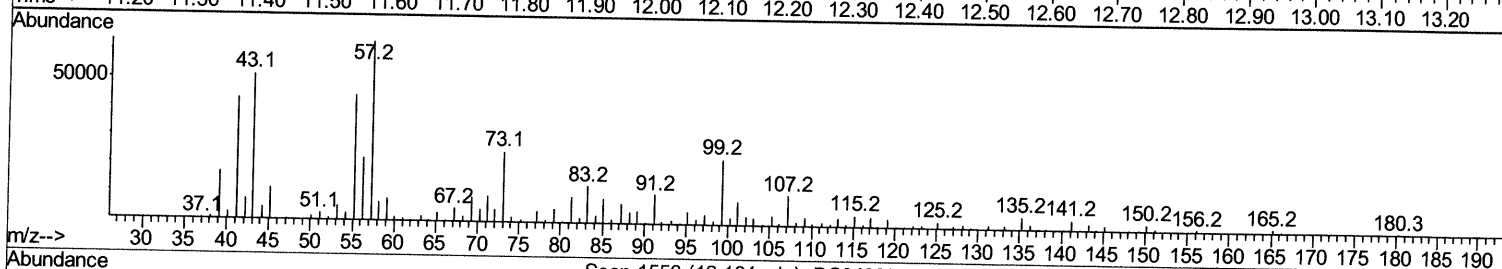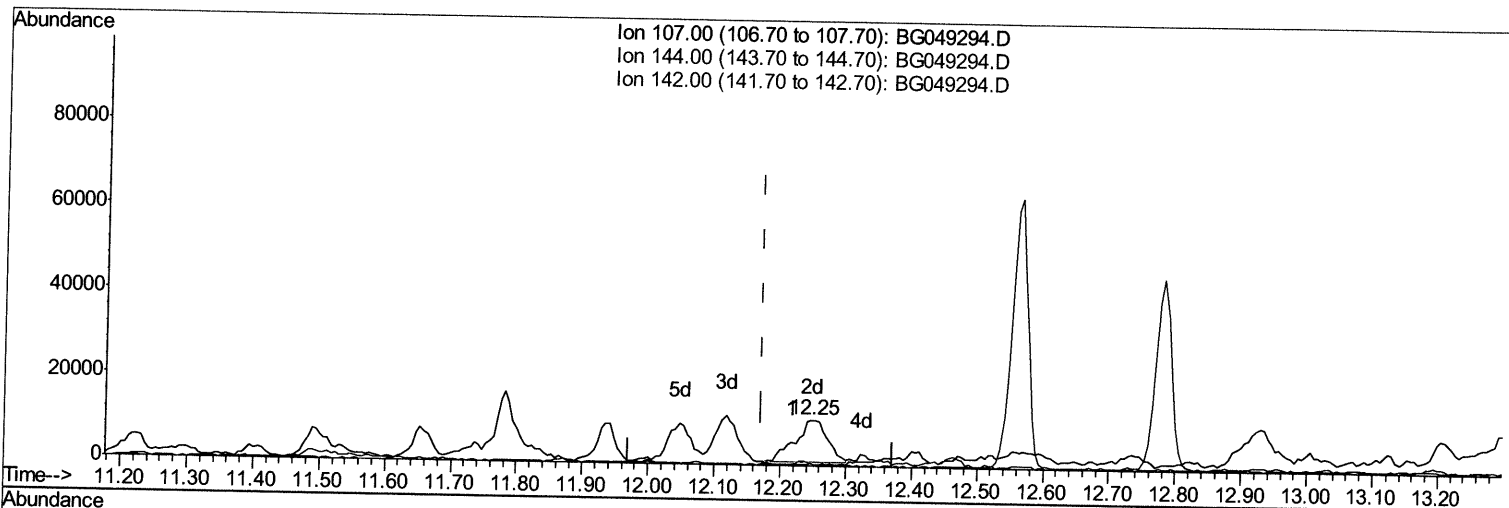

TIC: BG049294.D

(35) 4-Chloro-3-methylphenol (C)

12.247min (+0.076) 16.96ng/ul m 07/13/21 JU

response 35021

Ion	Exp%	Act%
107.00	100	100
144.00	27.90	4.13#
142.00	80.90	5.68#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG070921\
 Data File : BG049294.D
 Acq On : 11 Jul 2021 10:48
 Operator : CG/JU
 Sample : M2958-01
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampled :
 DBK23

Manual Integrations
 APPROVED

mohammad
 7/13/2021 8:08:01 AM

Quant Time: Jul 12 01:33:41 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG070921.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 09 03:15:38 2021
 Response via : Initial Calibration

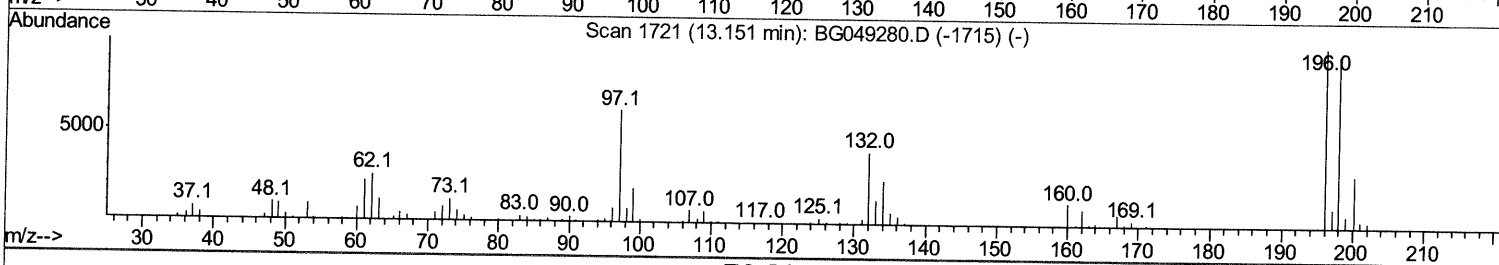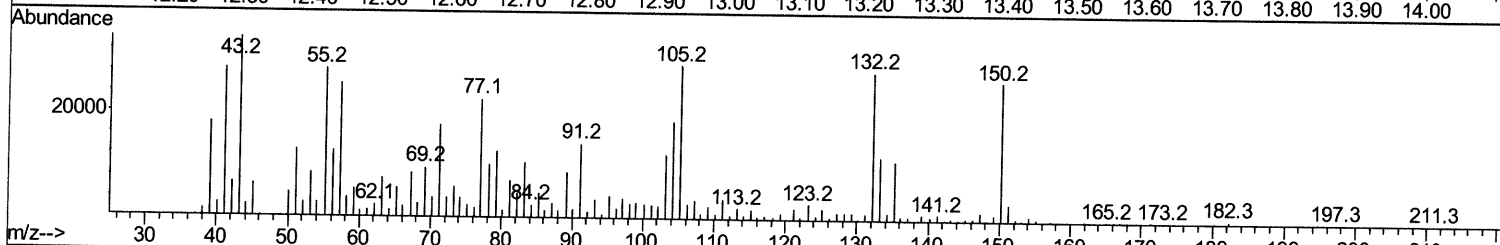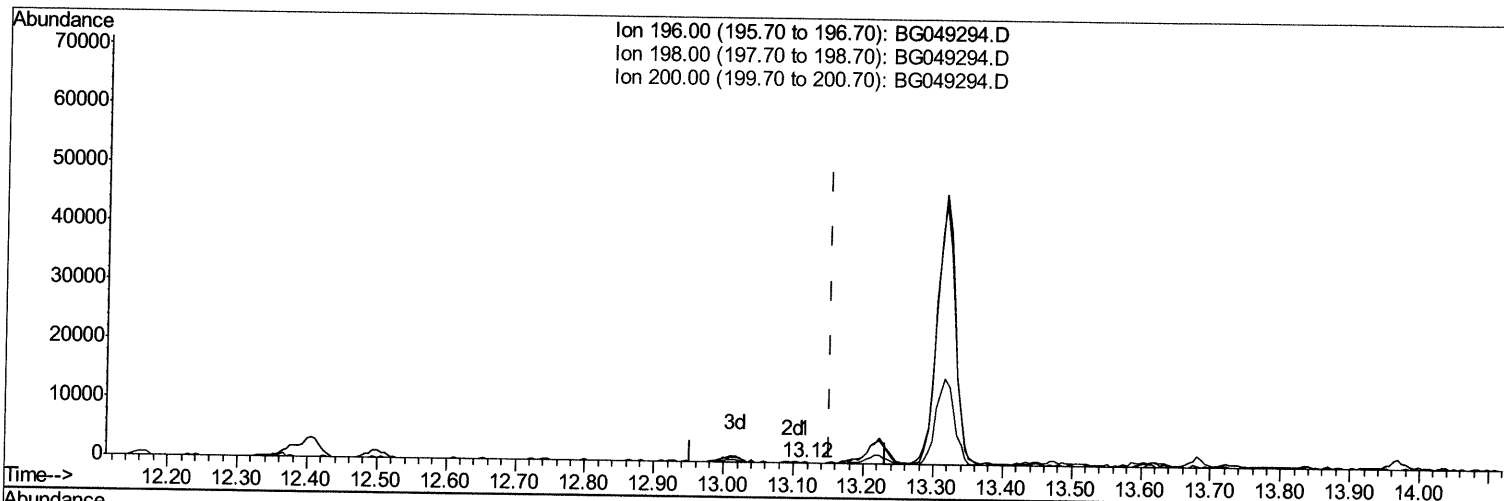

TIC: BG049294.D

(41) 2,4,6-Trichlorophenol (C)

13.117min (-0.036) 0.04ng/ul

response 67

Ion	Exp%	Act%
196.00	100	100
198.00	86.00	0.00#
200.00	28.00	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG070921\
Data File : BG049294.D
Acq On : 11 Jul 2021 10:48
Operator : CG/JU
Sample : M2958-01
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBK23

Manual Integrations
APPROVED

mohammad
7/13/2021 8:08:01 AM

Quant Time: Jul 12 01:33:41 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG070921.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 09 03:15:38 2021
Response via : Initial Calibration

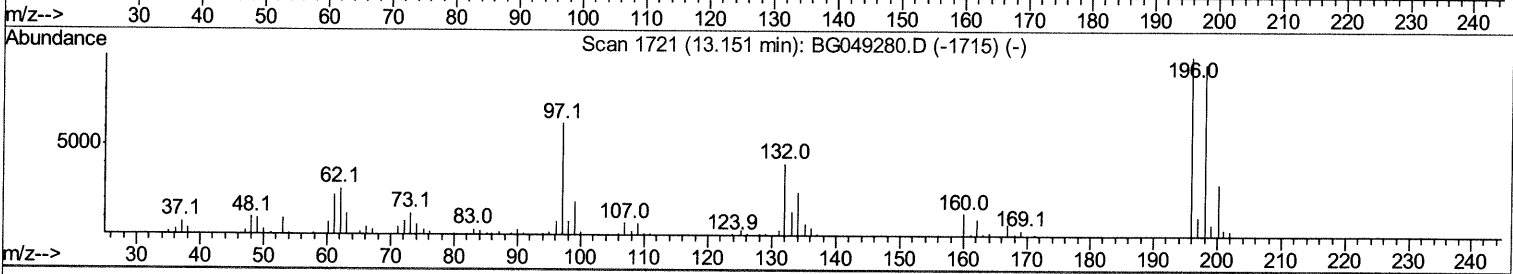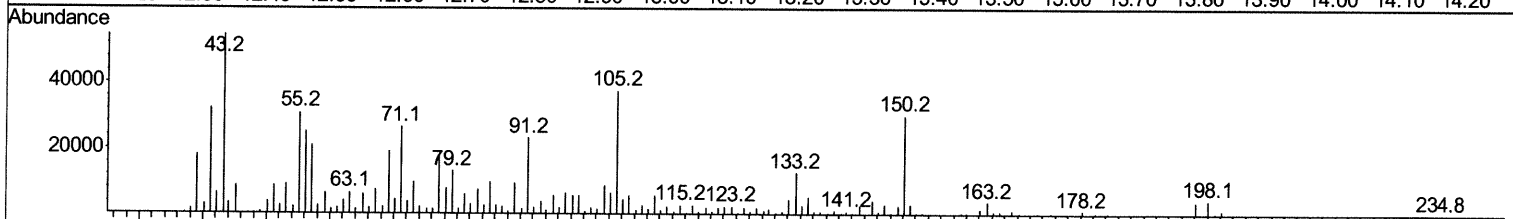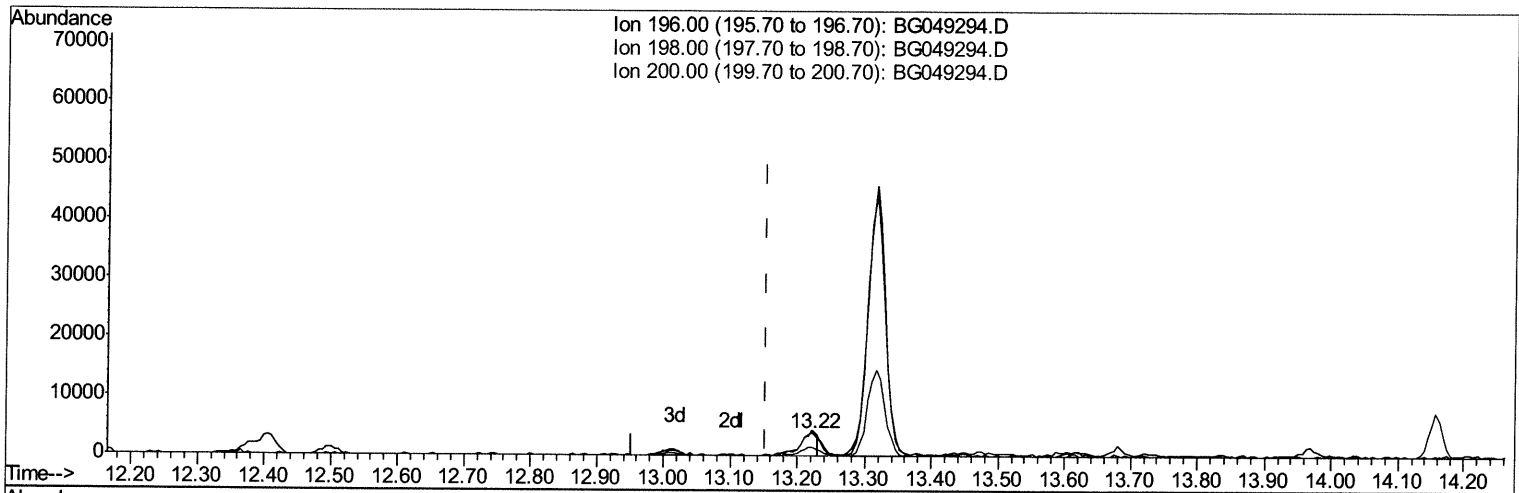

TIC: BG049294.D

(41) 2,4,6-Trichlorophenol (C)

13.222min (+0.070) 5.26ng/ul m 07/13/21JU

response 8795

Ion	Exp%	Act%
196.00	100	100
198.00	86.00	110.98#
200.00	28.00	36.88#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG070921\
Data File : BG049294.D
Acq On : 11 Jul 2021 10:48
Operator : CG/JU
Sample : M2958-01
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBK23

Manual Integrations
APPROVED

mohammad
7/13/2021 8:08:01 AM

Quant Time: Jul 12 01:36:11 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG070921.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 09 03:15:38 2021
Response via : Initial Calibration

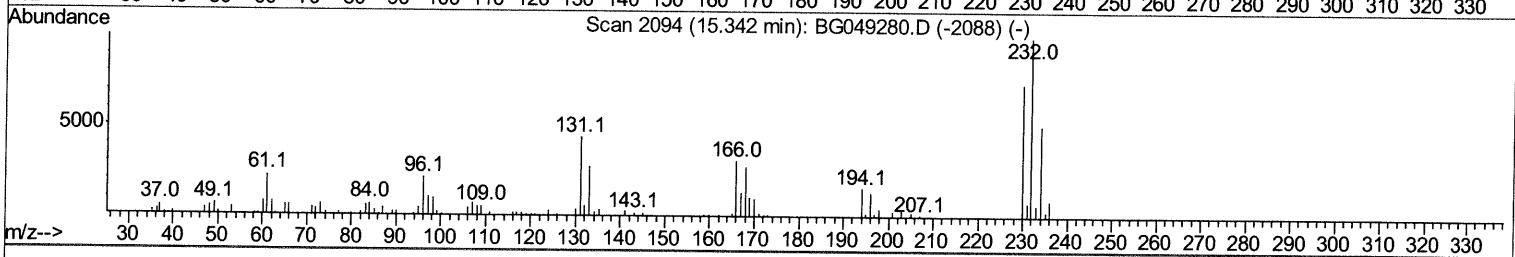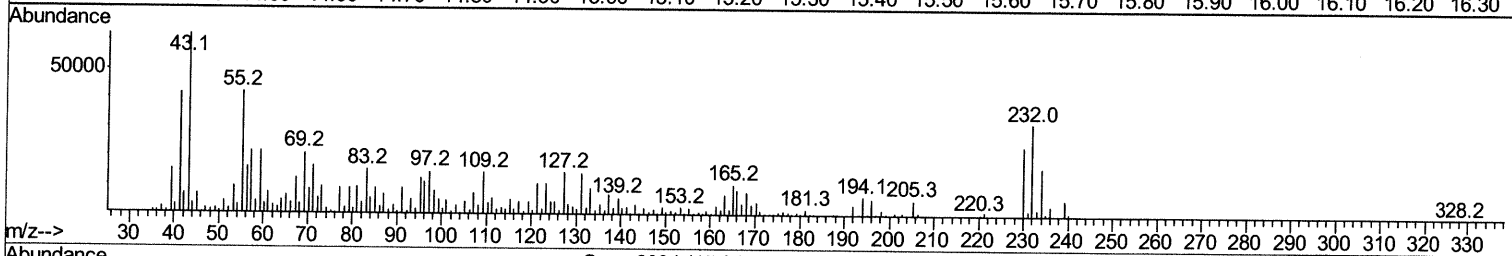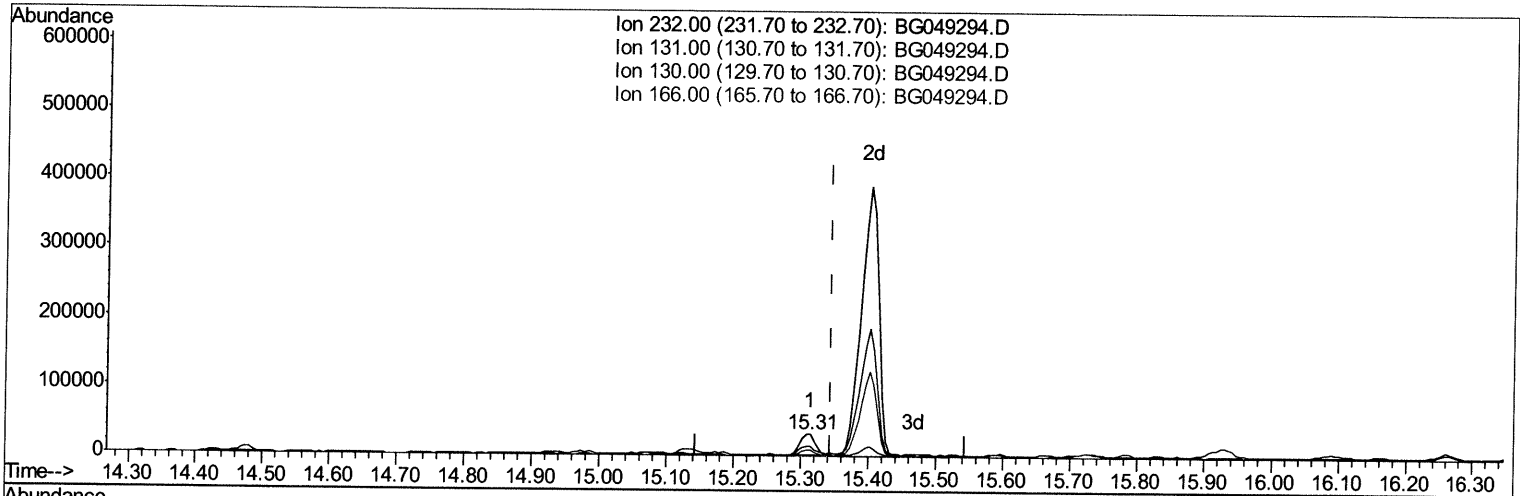

TIC: BG049294.D

(58) 2,3,4,6-Tetrachlorophenol

15.314min (-0.030) 32.42ng/ul

response 54091

Ion	Exp%	Act%
232.00	100	100
131.00	38.20	44.90
130.00	2.90	5.31#
166.00	27.30	27.58

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG070921\
 Data File : BG049294.D
 Acq On : 11 Jul 2021 10:48
 Operator : CG/JU
 Sample : M2958-01
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBK23

Manual Integrations
 APPROVED

mohammad
 7/13/2021 8:08:01 AM

Quant Time: Jul 12 01:36:11 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG070921.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 09 03:15:38 2021
 Response via : Initial Calibration

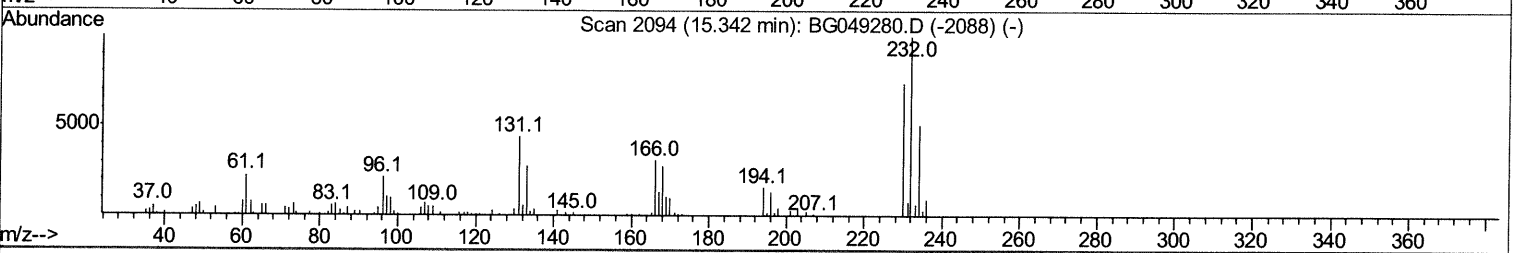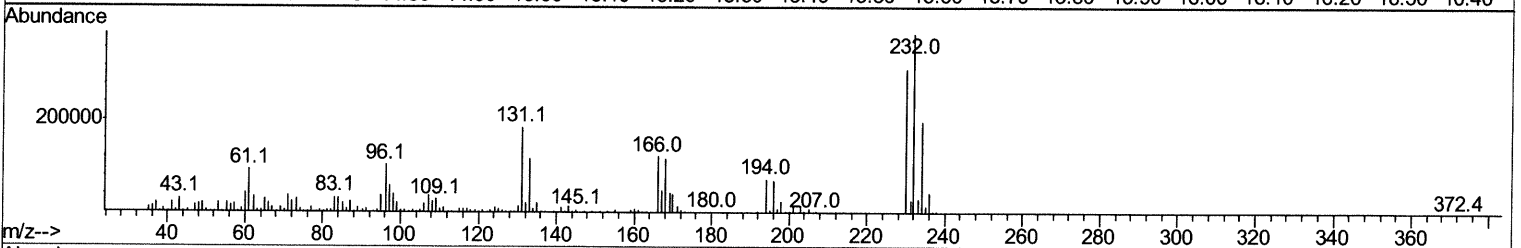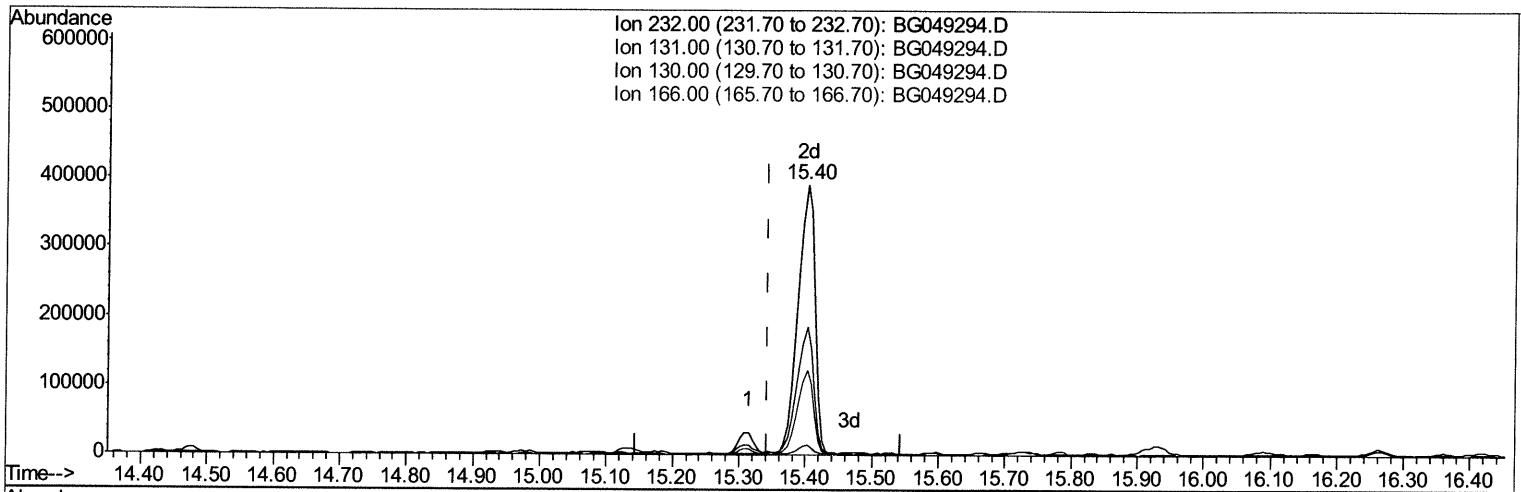

TIC: BG049294.D

(58) 2,3,4,6-Tetrachlorophenol

15.402min (+0.058) 422.45ng/ul m 07/13/21 JU

response 704933

Ion	Exp%	Act%
232.00	100	100
131.00	38.20	47.29#
130.00	2.90	3.49#
166.00	27.30	31.49

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG070921\
Data File : BG049294.D
Acq On : 11 Jul 2021 10:48
Operator : CG/JU
Sample : M2958-01
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBK23

Manual Integrations
APPROVED

mohammad
7/13/2021 8:08:01 AM

Quant Time: Jul 12 01:38:05 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG070921.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 09 03:15:38 2021
Response via : Initial Calibration

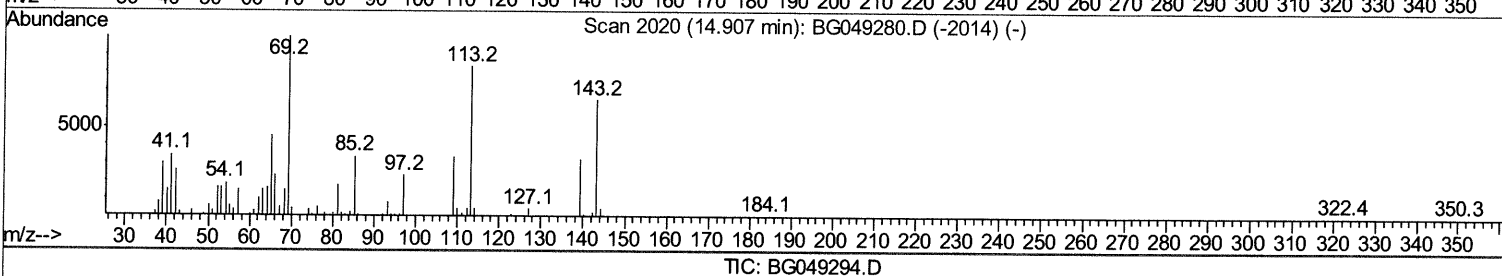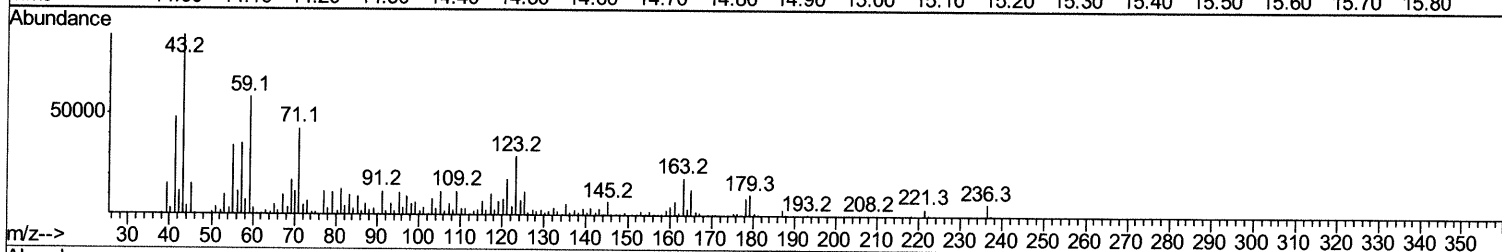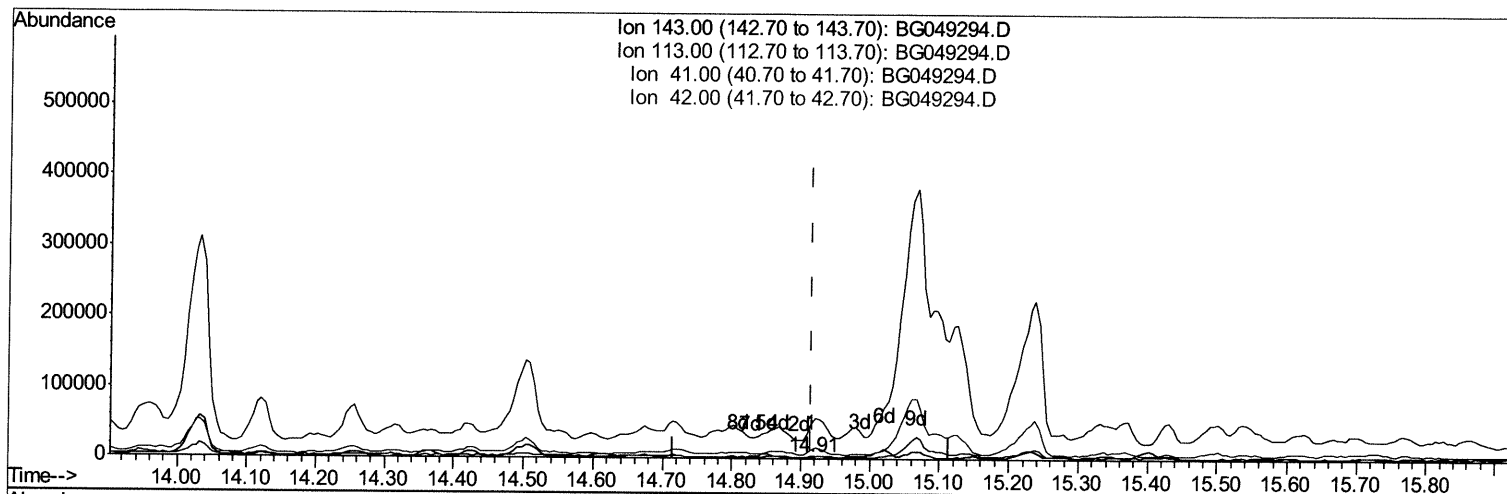

TIC: BG049294.D

(54) 4-Nitrophenol-d4 (S)

14.914min (-0.001) 0.71ng/ul

response 745

Ion	Exp%	Act%
143.00	100	100
113.00	103.00	70.65#
41.00	53.60	1583.49#
42.00	38.30	386.73#

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG070921\
Data File : BG049294.D
Acq On : 11 Jul 2021 10:48
Operator : CG/JU
Sample : M2958-01
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBK23

Manual Integrations
APPROVED

mohammad
7/13/2021 8:08:01 AM

Quant Time: Jul 12 01:38:05 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG070921.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 09 03:15:38 2021
Response via : Initial Calibration

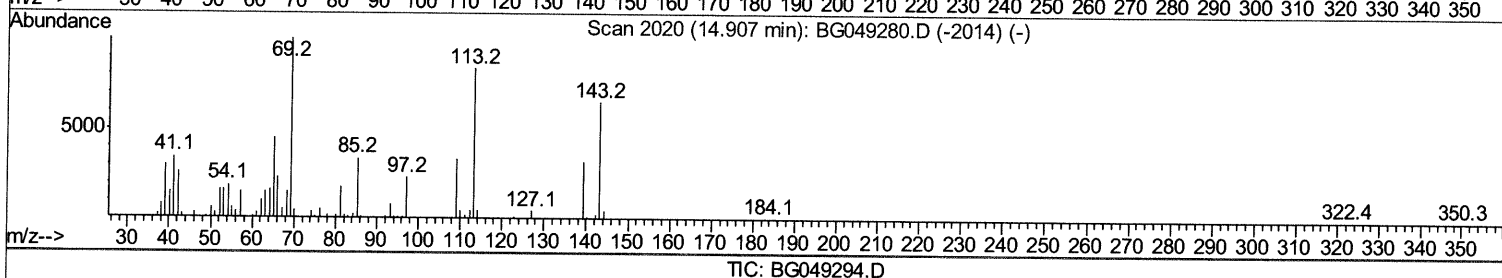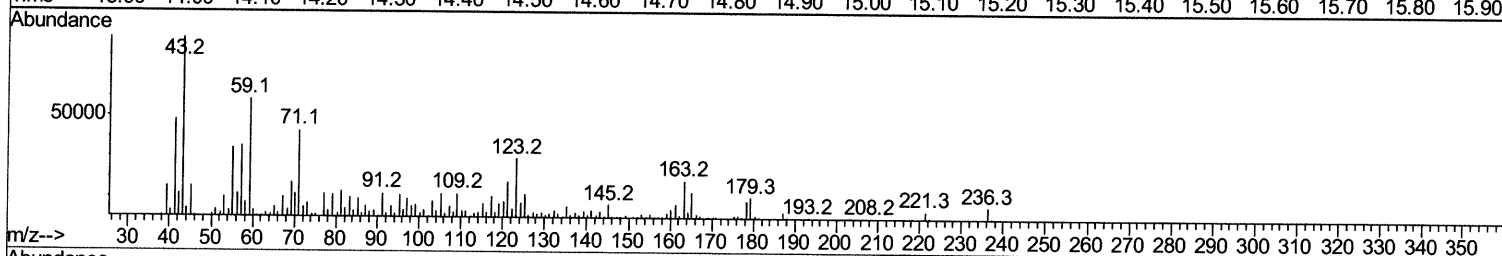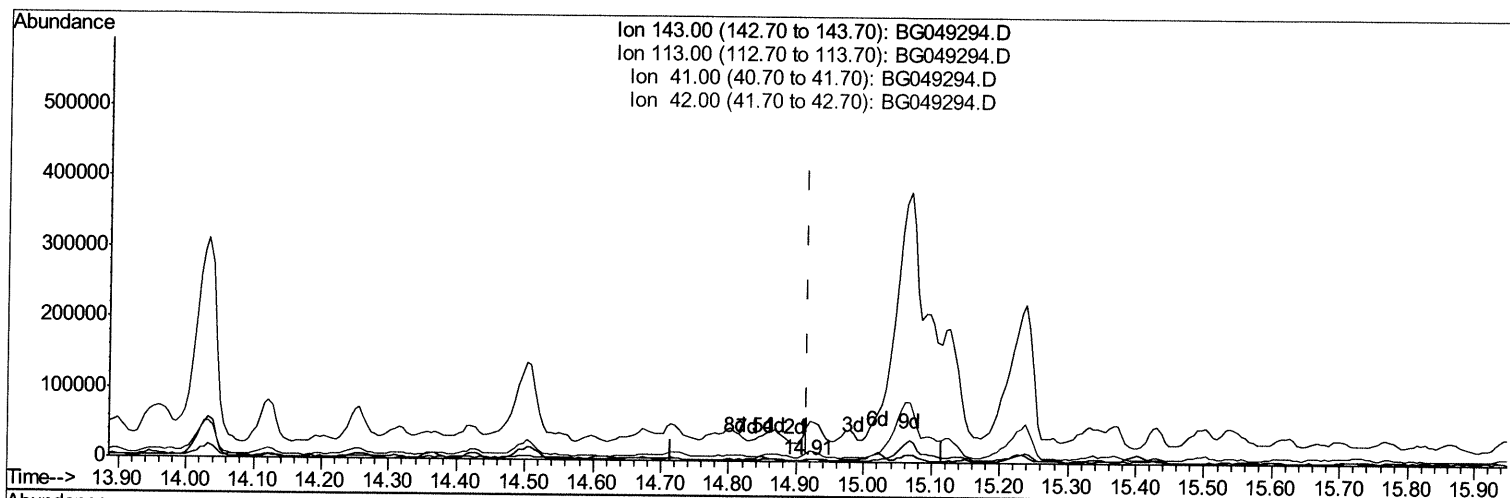

TIC: BG049294.D

(54) 4-Nitrophenol-d4 (S)

14.914min (-0.001) 5.43ng/ul m 07/13/2021

response 5692

Ion	Exp%	Act%
143.00	100	100
113.00	103.00	70.65#
41.00	53.60	1583.49#
42.00	38.30	386.73#

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG070921\
 Data File : BG049294.D
 Acq On : 11 Jul 2021 10:48
 Operator : CG/JU
 Sample : M2958-01
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBK23

Manual Integrations
 APPROVED

mohammad
 7/13/2021 8:08:01 AM

Quant Time: Jul 12 01:41:07 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG070921.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 09 03:15:38 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.08	152	27071	20.00	ng/ul	0.00
20) Naphthalene-d8	10.91	136	117700	20.00	ng/ul	0.02
38) Acenaphthene-d10	14.73	164	82347	20.00	ng/ul	0.01
64) Phenanthrene-d10	17.49	188	171125	20.00	ng/ul	0.02
79) Chrysene-d12	21.75	240	177542	20.00	ng/ul	0.00
88) Perylene-d12	25.05	264	185450	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.46	96	4045m >	7.03	ng/uL >	0.00	07/13/2021
4) Pyridine-d5	3.90	84	22348	13.21	ng/ul	0.01	
7) Phenol-d5	7.22	99	31138	13.22	ng/ul	0.00	
9) Bis-(2-Chloroethyl)ether-d	7.40	67	64855	47.49	ng/ul	0.00	
11) 2-Chlorophenol-d4	7.67	132	63041	36.22	ng/ul	0.06	
15) 4-Methylphenol-d8	8.88	113	60404m >	32.02	ng/ul >	0.10	07/13/2021
21) Nitrobenzene-d5	9.26	128	44499	49.27	ng/ul	0.02	
24) 2-Nitrophenol-d4	9.99	143	47655	45.96	ng/ul	0.02	
28) 2,4-Dichlorophenol-d3	10.57	165	83061	41.06	ng/ul	0.05	
31) 4-Chloroaniline-d4	11.02	131	12868	4.88	ng/ul	0.00	
46) Dimethylphthalate-d6	14.16	166	267109	42.18	ng/ul	0.04	
49) Acenaphthylene-d8	14.43	160	332807	44.79	ng/ul	0.01	
54) 4-Nitrophenol-d4	14.91	143	5692m >	5.43	ng/ul >	0.00	07/13/2021
60) Fluorene-d10	15.73	176	232272	43.32	ng/ul	0.01	
65) 4,6-Dinitro-2-methylphenol	15.84	200	33931	31.20	ng/ul	0.02	
73) Anthracene-d10	17.59	188	354931	45.56	ng/ul	0.02	
81) Pyrene-d10	19.86	212	399137	43.86	ng/ul	0.00	
92) Benzo(a)pyrene-d12	24.83	264	441662	45.81	ng/ul	0.00	

Target Compounds

					Ovalue	
2) 1,4-Dioxane	3.50	88	1748	2.494	ng/uL#	1
10) Bis(2-Chloroethyl)ether	7.51	93	6440	3.678	ng/ul#	1
12) 2-Chlorophenol	7.71	128	4127m >	2.349	ng/ul >	07/13/2021
14) 2,2'-oxybis(1-Chloropropan	8.61	45	21300	7.563	ng/ul#	91
16) Acetophenone	8.90	105	107756	34.817	ng/ul#	37
18) 4-Methylphenol	8.94	108	13255	7.103	ng/ul	93
23) Isophorone	9.86	82	1692592	384.692	ng/ul#	94
27) Bis(2-Chloroethoxy)methane	10.27	93	72115	30.743	ng/ul#	59
29) 2,4-Dichlorophenol	10.64	162	53375m >	28.874	ng/ul >	07/13/2021
30) Naphthalene	10.96	128	1265242	215.606	ng/ul#	85
35) 4-Chloro-3-methylphenol	12.25	107	35021m >	16.960	ng/ul >	07/13/2021
36) 2-Methylnaphthalene	12.56	142	108056	24.236	ng/ul	92
37) 1-Methylnaphthalene	12.78	142	75257	16.973	ng/ul#	96
41) 2,4,6-Trichlorophenol	13.22	196	8795m >	5.257	ng/ul >	07/13/2021
42) 2,4,5-Trichlorophenol	13.22	196	8795	4.942	ng/ul	95
43) 1,1'-Biphenyl	13.56	154	13904	2.499	ng/ul#	81
53) 2,4-Dinitrophenol	14.85	184	1398	1.743	ng/ul#	27
58) 2,3,4,6-Tetrachlorophenol	15.40	232	704933m >	422.446	ng/ul >	07/13/2021
61) Fluorene	15.78	166	8244	1.432	ng/ul#	64
66) 4,6-Dinitro-2-methylphenol	15.93	198	1038959	1003.752	ng/ul#	51
71) Pentachlorophenol	17.21	266	5985179	4639.284	ng/ul#	81
76) Pentachlorobenzene	15.05	250	5140	2.075	ng/uL	93

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG070921\
Data File : BG049294.D
Acq On : 11 Jul 2021 10:48
Operator : CG/JU
Sample : M2958-01
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBK23

Manual Integrations
APPROVED

mohammad
7/13/2021 8:08:01 AM

Quant Time: Jul 12 01:41:07 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG070921.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 09 03:15:38 2021
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
--------------------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed