

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070921\
 Data File : BG049235.D
 Acq On : 9 Jul 2021 13:12
 Operator : CG/JU
 Sample : M2877-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGDY9

Quant Time: Jul 09 13:56:52 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG070921.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 09 03:15:38 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.073	152	29761	20.000	ng/ul	0.00
20) Naphthalene-d8	10.900	136	116168	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.719	164	86649	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.468	188	205862	20.000	ng/ul	0.00
79) Chrysene-d12	21.757	240	222975	20.000	ng/ul	0.00
88) Perylene-d12	25.054	264	231130	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.473	96	1004	1.587	ng/uL	0.00
4) Pyridine-d5	3.896	84	9691	5.209	ng/ul	0.00
7) Phenol-d5	7.227	99	26316	10.165	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.392	67	16967	11.300	ng/ul	0.00
11) 2-Chlorophenol-d4	7.609	132	20993	10.972	ng/ul	0.00
15) 4-Methylphenol-d8	8.773	113	20572	9.918	ng/ul	0.00
21) Nitrobenzene-d5	9.243	128	10909	12.238	ng/ul	0.00
24) 2-Nitrophenol-d4	9.965	143	12429	12.146	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.512	165	21102	10.568	ng/ul	0.00
31) 4-Chloroaniline-d4	11.029	131	28033	10.773	ng/ul	0.00
46) Dimethylphthalate-d6	14.119	166	80226	12.039	ng/ul	0.00
49) Acenaphthylene-d8	14.413	160	93373	11.942	ng/ul	0.00
54) 4-Nitrophenol-d4	14.918	143	9276	8.410	ng/ul	0.00
60) Fluorene-d10	15.712	176	69026	12.234	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.823	200	12770	9.759	ng/ul	0.00
73) Anthracene-d10	17.568	188	118537	12.647	ng/ul	0.00
81) Pyrene-d10	19.854	212	143200	12.530	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.824	264	123965	10.318	ng/ul	0.00
Target Compounds						
					Qvalue	
47) Dimethylphthalate	14.166	163	18553	3.000	ng/ul#	94
80) Fluoranthene	19.519	202	14384	1.082	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070921\
Data File : BG049235.D
Acq On : 9 Jul 2021 13:12
Operator : CG/JU
Sample : M2877-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGDY9

Quant Time: Jul 09 13:56:52 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG070921.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 09 03:15:38 2021
Response via : Initial Calibration




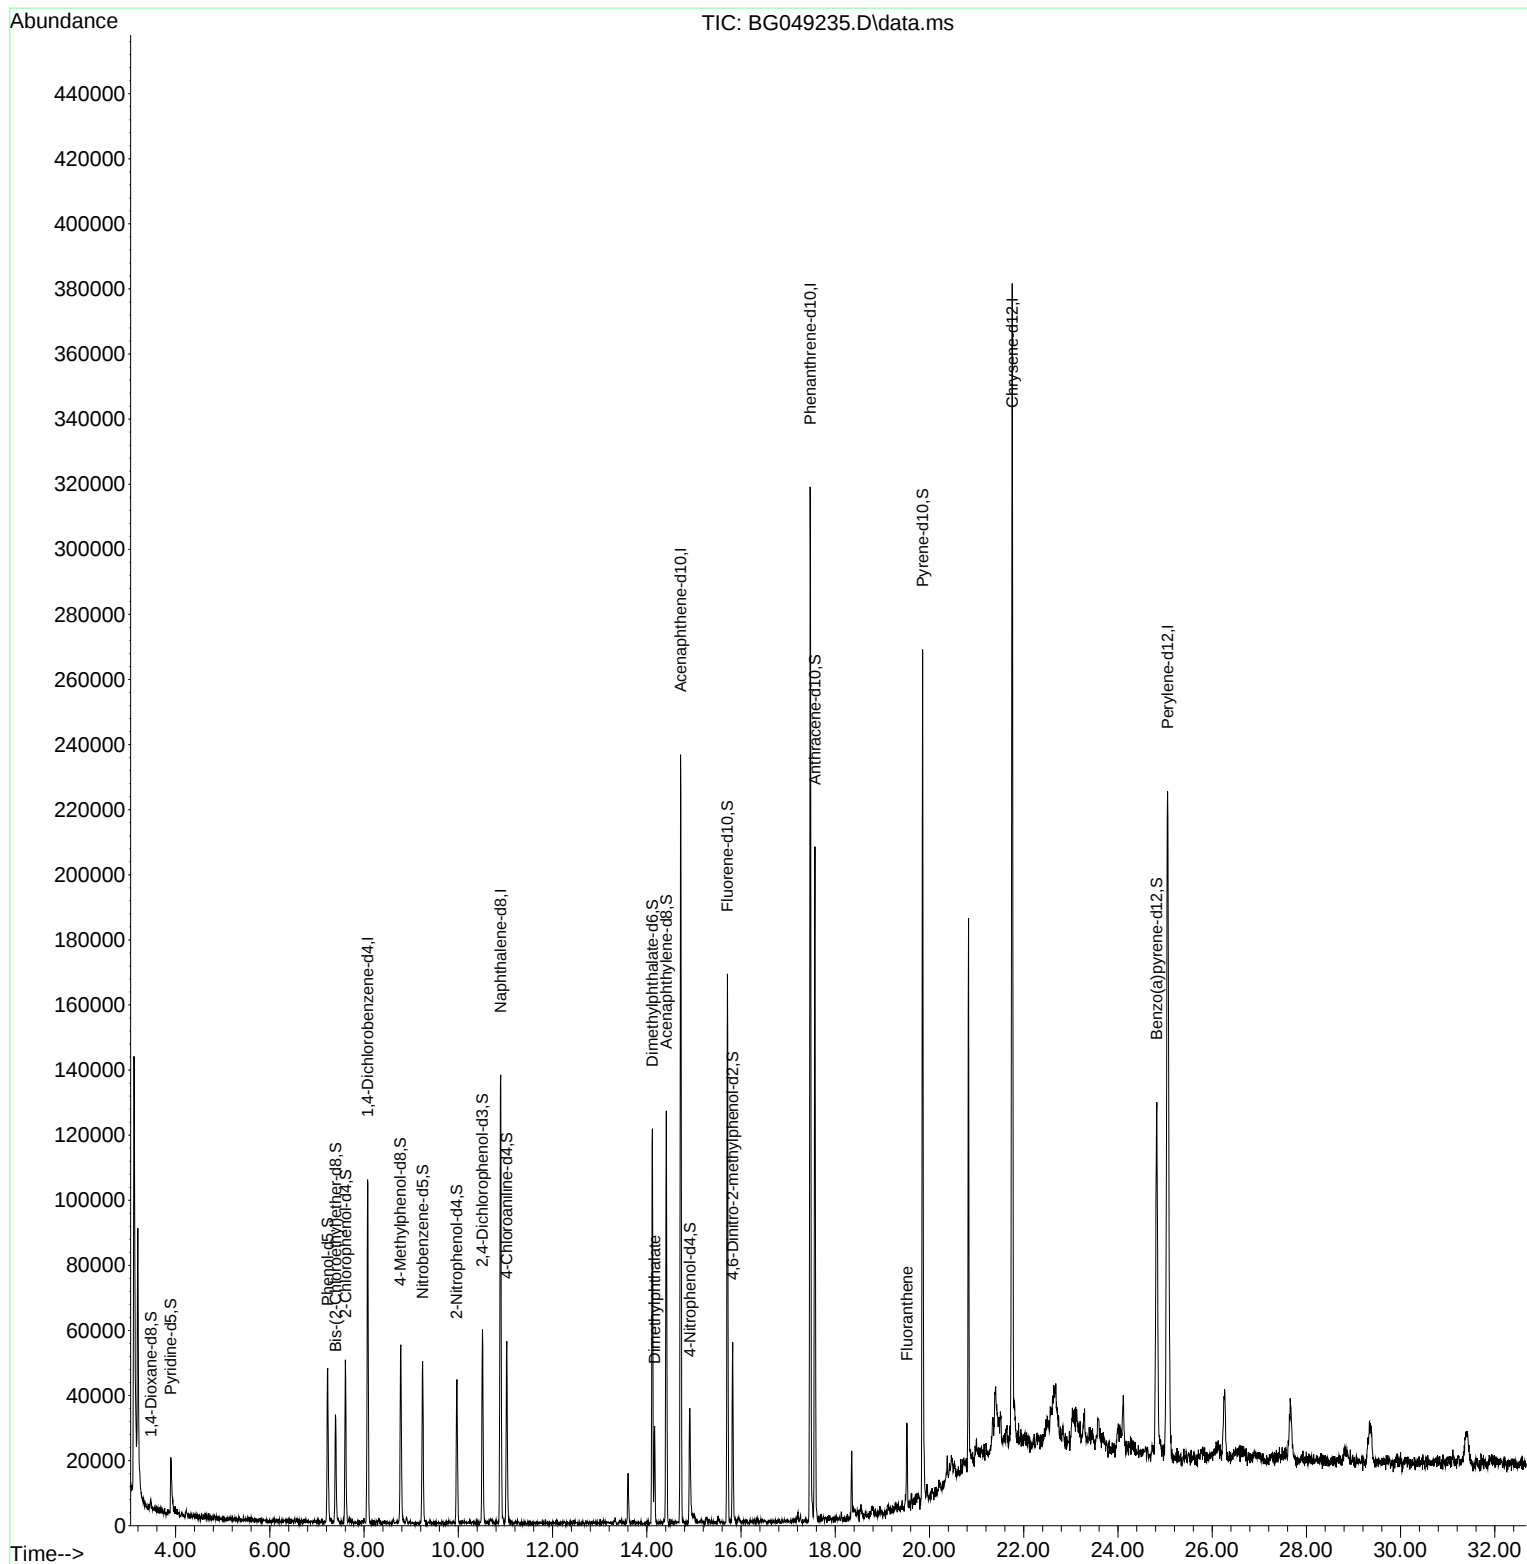


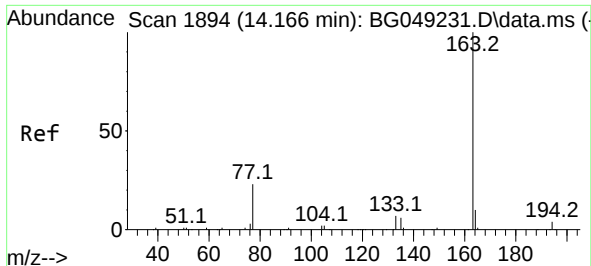

#47
Dimethylphthalate
Concen: 3.000 ng/ul
RT: 14.166 min Scan# 1894
Delta R.T. -0.003 min
Lab File: BG049235.D
Acq: 9 Jul 2021 13:12

Instrument :
BNA_G
ClientSampleId :
BGDY9

Tgt Ion:163 Resp: 18553
Ion Ratio Lower Upper
163 100
194 2.4 2.4 3.6#
164 7.7 8.4 12.6#

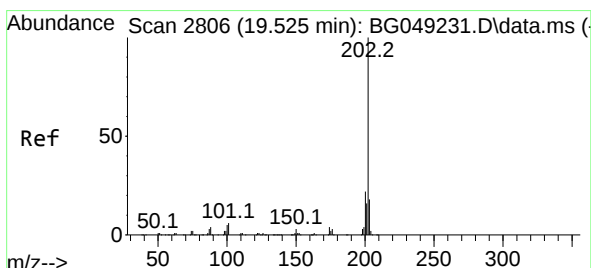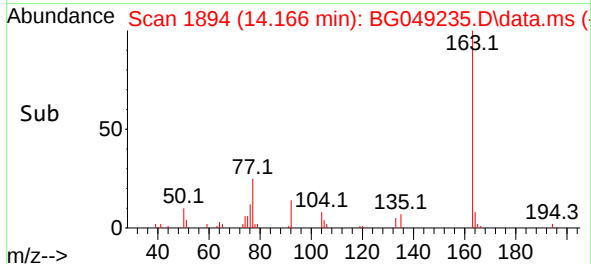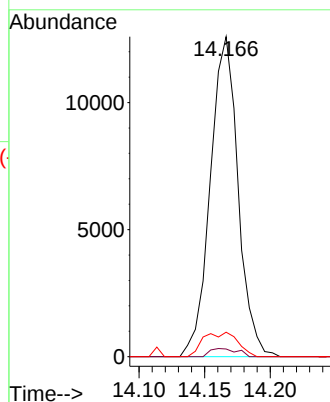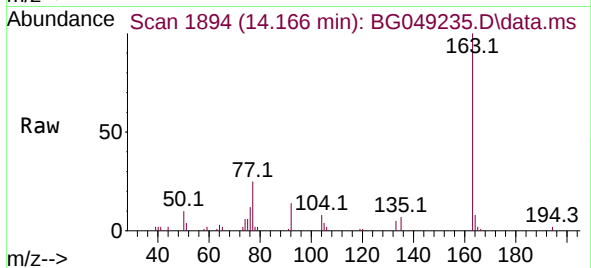

#80
Fluoranthene
Concen: 1.082 ng/ul
RT: 19.519 min Scan# 2805
Delta R.T. -0.003 min
Lab File: BG049235.D
Acq: 9 Jul 2021 13:12

Tgt Ion:202 Resp: 14384
Ion Ratio Lower Upper
202 100
101 4.7 4.6 6.8
100 4.8 4.0 6.0

