

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070921\
 Data File : BG049284.D
 Acq On : 11 Jul 2021 4:00
 Operator : CG/JU
 Sample : M2910-02
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AX0

Quant Time: Jul 11 05:14:17 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG070921.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jul 11 04:28:44 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.070	152	32188	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.890	136	130202	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.715	164	98196	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.465	188	231046	20.000	ng/ul	0.00
79) Chrysene-d12	21.748	240	225321	20.000	ng/ul	0.00
88) Perylene-d12	25.044	264	229983	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.464	96	3096	4.524	ng/uL	0.00
4) Pyridine-d5	3.893	84	16654	8.277	ng/ul	0.00
7) Phenol-d5	7.224	99	19493	6.962	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.394	67	51516	31.723	ng/ul	0.00
11) 2-Chlorophenol-d4	7.600	132	53947	26.070	ng/ul	0.00
15) 4-Methylphenol-d8	8.775	113	37804	16.852	ng/ul	0.00
21) Nitrobenzene-d5	9.239	128	35130	35.161	ng/ul	0.00
24) 2-Nitrophenol-d4	9.968	143	39819	34.718	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.508	165	75755	33.850	ng/ul	0.00
31) 4-Chloroaniline-d4	11.025	131	88026	30.183	ng/ul	0.00
46) Dimethylphthalate-d6	14.116	166	268886	35.605	ng/ul	0.00
49) Acenaphthylene-d8	14.410	160	311429	35.147	ng/ul	0.00
54) 4-Nitrophenol-d4	14.909	143	8175	6.540	ng/ul	0.00
60) Fluorene-d10	15.708	176	233005	36.442	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.820	200	39353	26.797	ng/ul	0.00
73) Anthracene-d10	17.565	188	419873	39.915	ng/ul	0.00
81) Pyrene-d10	19.850	212	483640	41.879	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.821	264	494342	41.349	ng/ul	0.00
Target Compounds						
35) 4-Chloro-3-methylphenol	12.171	107	3029	1.326	ng/ul#	Qvalue 56


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070921\
Data File : BG049284.D
Acq On : 11 Jul 2021 4:00
Operator : CG/JU
Sample : M2910-02
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AX0

Quant Time: Jul 11 05:14:17 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG070921.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Jul 11 04:28:44 2021
Response via : Initial Calibration

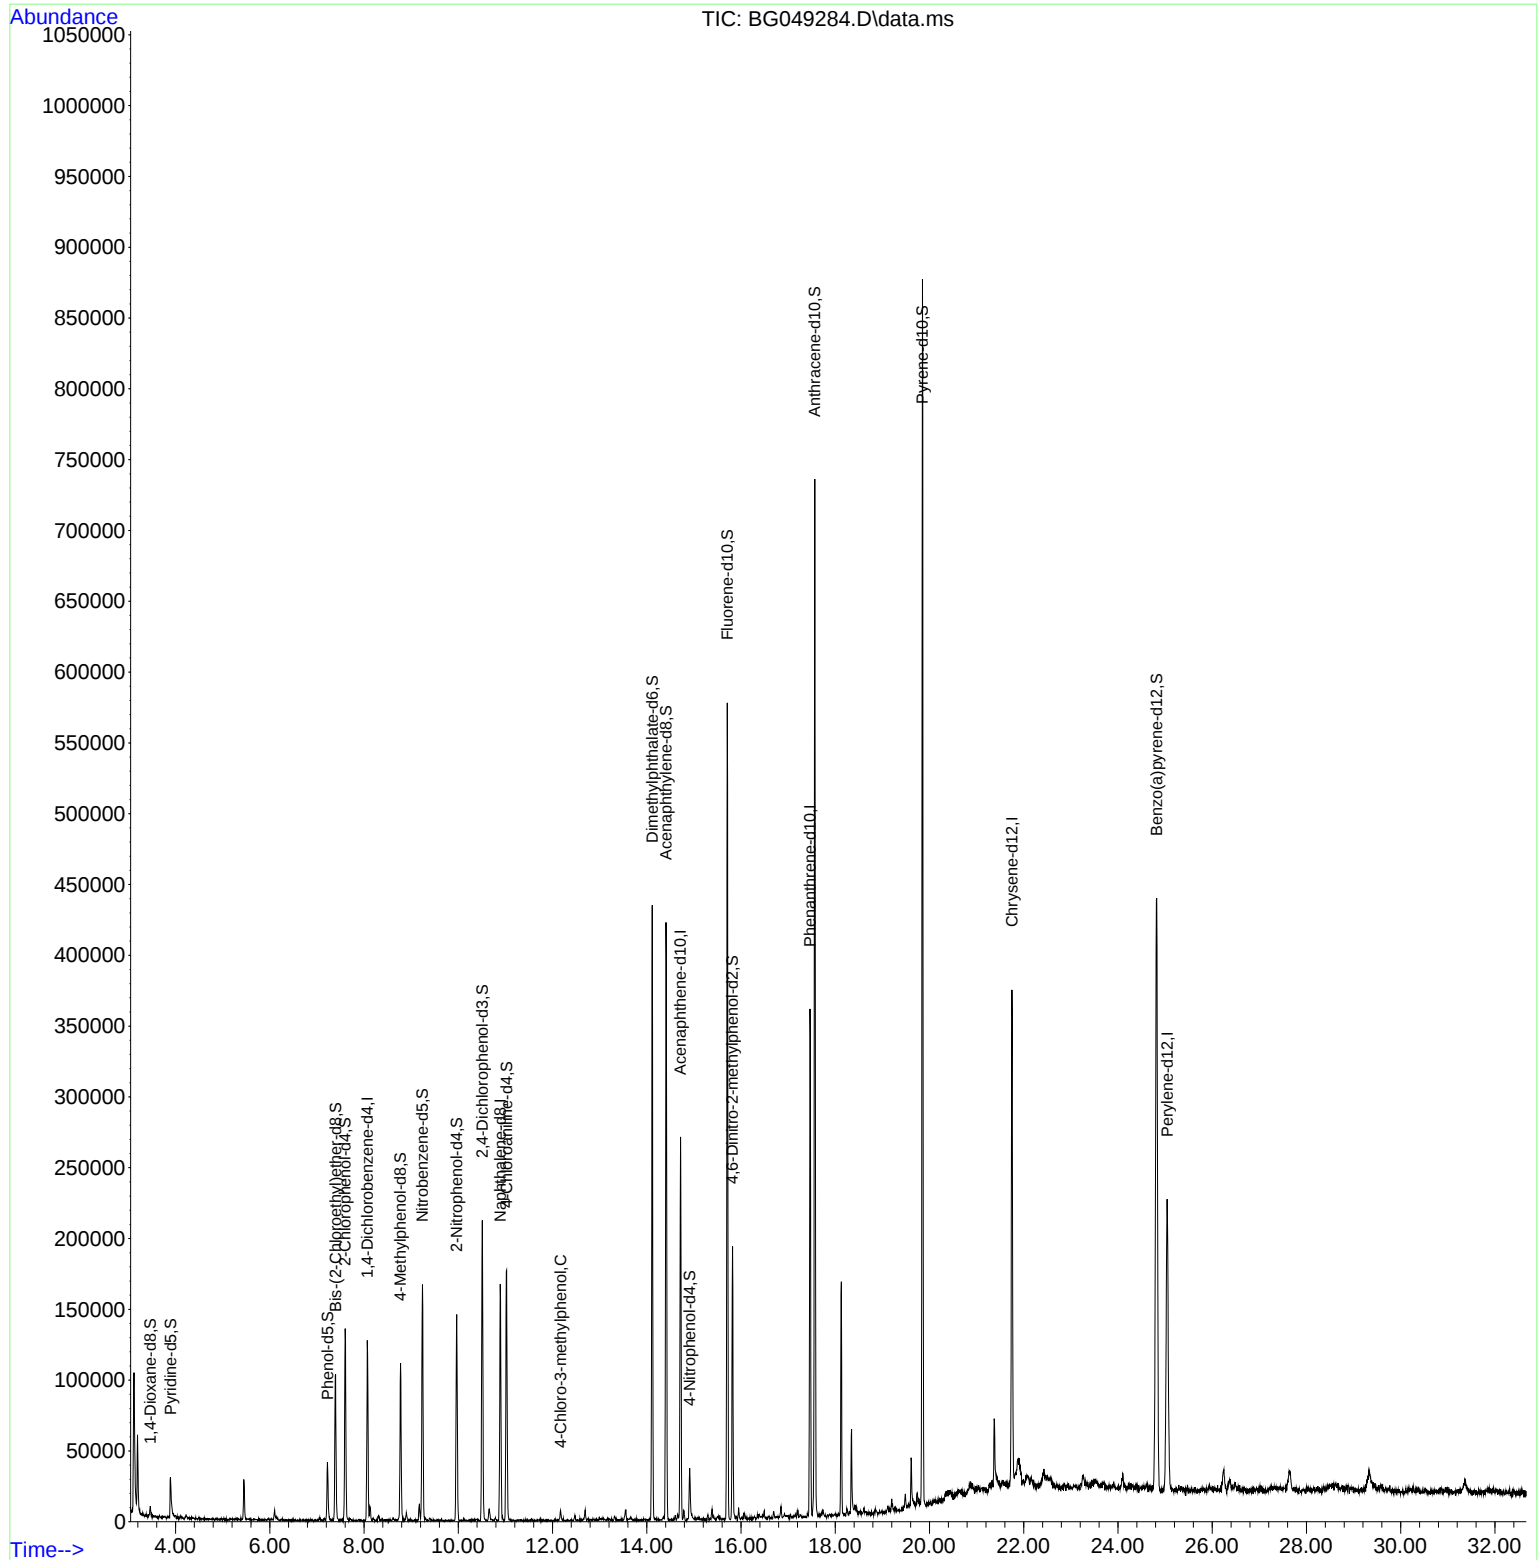

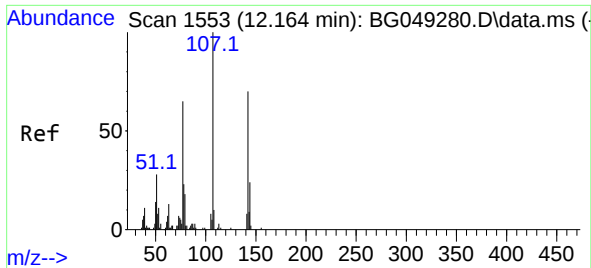

#35
4-Chloro-3-methylphenol
Concen: 1.326 ng/ul
RT: 12.171 min Scan# 1554
Delta R.T. -0.000 min
Lab File: BG049284.D
Acq: 11 Jul 2021 4:00

Instrument :
BNA_G
ClientSampleId :
C0AX0

Tgt Ion:107 Resp: 3029
Ion Ratio Lower Upper
107 100
144 18.7 22.3 33.5#
142 33.8 64.7 97.1#

