

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071023\
 Data File : BG058137.D
 Acq On : 10 Jul 2023 11:24
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SSTD020506

Quant Time: Jul 11 00:44:07 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 10 16:52:40 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.970	152	39335	20.000	ng/u1	0.00
20) Naphthalene-d8	10.778	136	180105	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.603	164	128590	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.341	188	309674	20.000	ng/u1	0.00
79) Chrysene-d12	21.601	240	278774	20.000	ng/u1	0.00
88) Perylene-d12	24.785	264	333517	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.399	96	8718	7.761	ng/uL	0.00
4) Pyridine-d5	3.810	84	65376	19.170	ng/u1	0.00
7) Phenol-d5	7.130	99	77081	19.188	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.294	67	46782	19.325	ng/u1	0.00
11) 2-Chlorophenol-d4	7.506	132	52069	18.794	ng/u1	0.00
15) 4-Methylphenol-d8	8.675	113	58254	19.219	ng/u1	0.00
21) Nitrobenzene-d5	9.133	128	28475	19.398	ng/u1	0.00
24) 2-Nitrophenol-d4	9.856	143	31194	20.219	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.396	165	59738	20.185	ng/u1	0.00
31) 4-Chloroaniline-d4	10.913	131	88433	19.708	ng/u1	0.00
46) Dimethylphthalate-d6	14.004	166	195815	19.300	ng/u1	0.00
49) Acenaphthylene-d8	14.298	160	223448	20.182	ng/u1	0.00
54) 4-Nitrophenol-d4	14.797	143	31620	17.640	ng/u1	0.00
60) Fluorene-d10	15.590	176	173231	20.104	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.708	200	32826	19.521	ng/u1	0.00
73) Anthracene-d10	17.441	188	287248	19.990	ng/u1	0.00
81) Pyrene-d10	19.727	212	327449	18.650	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.568	264	330390	19.444	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.440	88	9933	7.158	ng/uL	97
5) Pyridine	3.833	79	68712	19.665	ng/u1	95
6) Benzaldehyde	7.112	77	22245	16.582	ng/u1	98
8) Phenol	7.159	94	78785	19.327	ng/u1	98
10) Bis(2-Chloroethyl)ether	7.388	93	60093	19.092	ng/u1	98
12) 2-Chlorophenol	7.535	128	55915	19.394	ng/u1	98
13) 2-Methylphenol	8.410	108	60952	19.039	ng/u1	96
14) 2,2'-oxybis(1-Chloropr...	8.499	45	94161	19.434	ng/u1	97
16) Acetophenone	8.792	105	100527	19.990	ng/u1	99
17) N-Nitroso-di-n-propyla...	8.769	70	53265	19.813	ng/u1#	95
18) 4-Methylphenol	8.739	108	68795	19.873	ng/u1	99
19) Hexachloroethane	9.057	117	21410	19.371	ng/u1	98
22) Nitrobenzene	9.174	77	73745	19.352	ng/u1	100
23) Isophorone	9.691	82	157809	19.407	ng/u1	99
25) 2-Nitrophenol	9.891	139	33093	19.990	ng/u1	97
26) 2,4-Dimethylphenol	9.944	107	73937	19.862	ng/u1	98
27) Bis(2-Chloroethoxy)met...	10.173	93	88909	19.404	ng/u1	98
29) 2,4-Dichlorophenol	10.426	162	58632	20.376	ng/u1	97
30) Naphthalene	10.825	128	198784	19.640	ng/u1	99
32) 4-Chloroaniline	10.937	127	92135	20.081	ng/u1	100
33) Hexachlorobutadiene	11.107	225	39834	19.553	ng/u1	96
34) Caprolactam	11.683	113	22026	19.039	ng/u1	96
35) 4-Chloro-3-methylphenol	12.053	107	72543	20.523	ng/u1	98
36) 2-Methylnaphthalene	12.429	142	135187	19.814	ng/u1	95

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071023\
 Data File : BG058137.D
 Acq On : 10 Jul 2023 11:24
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SSTD020506

Quant Time: Jul 11 00:44:07 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 10 16:52:40 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.652	142	136393	19.935	ng/ul	95
39) 1,2,4,5-Tetrachloroben...	12.799	216	77656	19.817	ng/ul	98
40) Hexachlorocyclopentadiene	12.776	237	56432	22.863	ng/ul	99
41) 2,4,6-Trichlorophenol	13.034	196	54161	20.392	ng/ul	99
42) 2,4,5-Trichlorophenol	13.111	196	57265	19.937	ng/ul	100
43) 1,1'-Biphenyl	13.434	154	185672	20.036	ng/ul	99
44) 2-Chloronaphthalene	13.481	162	146757	19.733	ng/ul	100
45) 2-Nitroaniline	13.681	65	51636	19.969	ng/ul	98
47) Dimethylphthalate	14.051	163	200579	19.677	ng/ul	99
48) 2,6-Dinitrotoluene	14.174	165	40702	19.453	ng/ul#	95
50) Acenaphthylene	14.327	152	239457	20.028	ng/ul	100
51) 3-Nitroaniline	14.503	138	29652	16.770	ng/ul#	91
52) Acenaphthene	14.662	153	165982	20.232	ng/ul	97
53) 2,4-Dinitrophenol	14.715	184	19824	18.174	ng/ul	94
55) 4-Nitrophenol	14.815	109	23771	17.901	ng/ul	92
56) Dibenzofuran	14.997	168	236607	20.288	ng/ul	98
57) 2,4-Dinitrotoluene	14.962	165	58889	19.865	ng/ul	99
58) 2,3,4,6-Tetrachlorophenol	15.226	232	51335	19.632	ng/ul#	99
59) Diethylphthalate	15.408	149	205525	19.318	ng/ul	99
61) Fluorene	15.649	166	194187	20.293	ng/ul	96
62) 4-Chlorophenyl-phenyle...	15.637	204	103719	20.485	ng/ul	99
63) 4-Nitroaniline	15.661	138	19839	12.525	ng/ul	97
66) 4,6-Dinitro-2-methylph...	15.719	198	33452	19.453	ng/ul	94
67) N-Nitrosodiphenylamine	15.849	169	164148	19.917	ng/ul	99
68) 4-Bromophenyl-phenylether	16.530	248	69152	20.343	ng/ul	99
69) Hexachlorobenzene	16.648	284	77973	20.488	ng/ul	98
70) Atrazine	16.795	200	64662	19.187	ng/ul	98
71) Pentachlorophenol	16.994	266	41043	17.963	ng/ul	94
72) Phenanthrene	17.382	178	316909	20.118	ng/ul	100
74) Anthracene	17.476	178	317181	19.898	ng/ul	100
75) 1,2,3,4-Tetrachloroben...	13.399	216	83641	20.366	ng/uL	95
76) Pentachlorobenzene	14.920	250	88823	20.250	ng/uL	97
77) Carbazole	17.747	167	287432	19.938	ng/ul	99
78) Di-n-butylphthalate	18.299	149	362298	19.728	ng/ul	99
80) Fluoranthene	19.392	202	377224	18.542	ng/ul	100
82) Pyrene	19.756	202	385738	18.836	ng/ul	99
83) Butylbenzylphthalate	20.637	149	158134	19.043	ng/ul	97
84) 3,3'-Dichlorobenzidine	21.495	252	128091	18.980	ng/ul	100
85) Benzo(a)anthracene	21.577	228	381093	19.039	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.477	149	231257	19.433	ng/ul	99
87) Chrysene	21.648	228	372861	19.871	ng/ul	99
89) Di-n-octyl phthalate	22.676	149	405428	19.785	ng/ul	100
90) Benzo(b)fluoranthene	23.769	252	391724	18.969	ng/ul	97
91) Benzo(k)fluoranthene	23.839	252	400612	19.792	ng/ul	99
93) Benzo(a)pyrene	24.638	252	355232	19.435	ng/ul	100
94) Indeno(1,2,3-cd)pyrene	28.422	276	472575	19.470	ng/ul	100
95) Dibenzo(a,h)anthracene	28.487	278	393036	19.638	ng/ul	98
96) Benzo(g,h,i)perylene	29.562	276	376818	19.008	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071023\
 Data File : BG058137.D
 Acq On : 10 Jul 2023 11:24
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SSTD020506

Quant Time: Jul 11 00:44:07 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 10 16:52:40 2023
 Response via : Initial Calibration




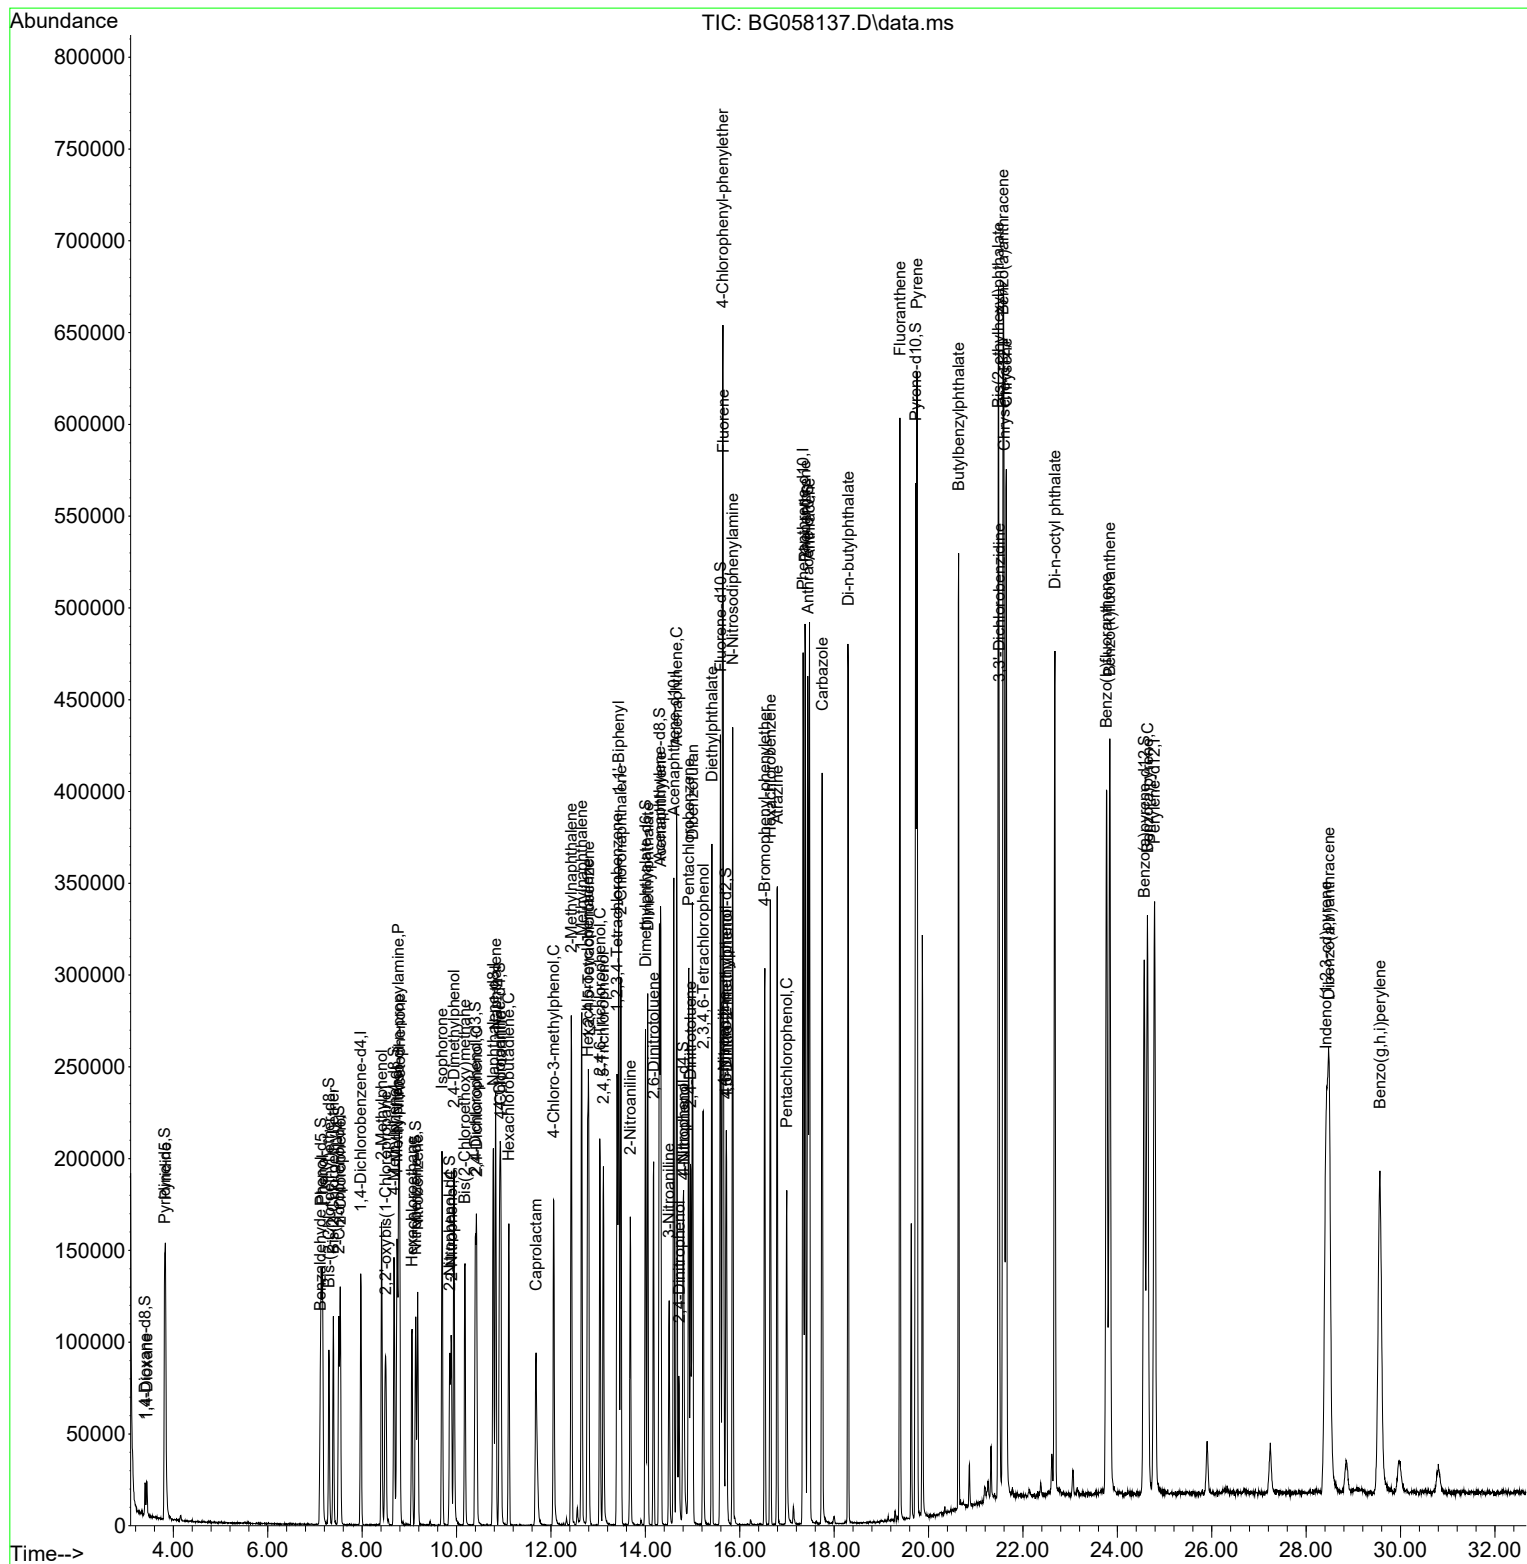




#2
1,4-Dioxane
Concen: 7.158 ng/uL
RT: 3.440 min Scan# 60
Delta R.T. 0.000 min
Lab File: BG058137.D
Acq: 10 Jul 2023 11:24




Instrument :
BNA_G
ClientSampleId :
SSTD020506


Tgt Ion:	88	Resp:	9933
Ion	Ratio	Lower	Upper
88	100		
43	24.6	20.6	30.8
58	84.6	65.5	98.3



#5
Pyridine
Concen: 19.665 ng/uL
RT: 3.833 min Scan# 127
Delta R.T. 0.000 min
Lab File: BG058137.D
Acq: 10 Jul 2023 11:24

Tgt Ion:	79	Resp:	68712
Ion	Ratio	Lower	Upper
79	100		
52	81.0	68.6	102.8
51	40.4	29.4	44.0



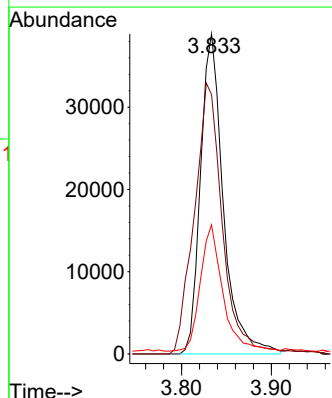





#6
Benzaldehyde
Concen: 16.582 ng/ul
RT: 7.112 min Scan# 685
Delta R.T. 0.000 min
Lab File: BG058137.D
Acq: 10 Jul 2023 11:24




Instrument :
BNA_G
ClientSampleId :
SSTD020506


Tgt Ion: 77 Resp: 22245
Ion Ratio Lower Upper
77 100
105 95.1 74.7 112.1
106 97.7 75.9 113.9



#8
Phenol
Concen: 19.327 ng/ul
RT: 7.159 min Scan# 693
Delta R.T. 0.000 min
Lab File: BG058137.D
Acq: 10 Jul 2023 11:24

Tgt Ion: 94 Resp: 78785
Ion Ratio Lower Upper
94 100
65 29.1 22.2 33.4
66 35.2 28.6 43.0

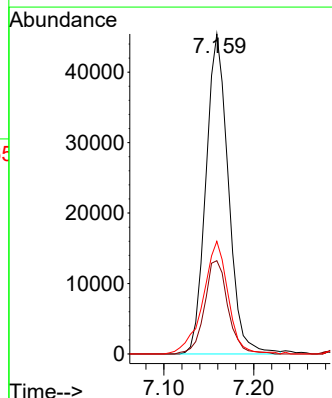



#10

Bis(2-Chloroethyl)ether

Concen: 19.092 ng/ul

RT: 7.388 min Scan# 732

Delta R.T. 0.000 min

Lab File: BG058137.D

Acq: 10 Jul 2023 11:24

Instrument :

BNA_G

ClientSampleId :

SSTD020506





Tgt Ion: 93 Resp: 60093

Ion Ratio Lower Upper

93 100

63 88.1 69.4 104.0

95 31.9 27.0 40.6



#12

2-Chlorophenol

Concen: 19.394 ng/ul

RT: 7.535 min Scan# 757

Delta R.T. 0.000 min

Lab File: BG058137.D

Acq: 10 Jul 2023 11:24




Tgt Ion:128 Resp: 55915


Ion Ratio Lower Upper

128 100

64 54.4 44.3 66.5

130 32.2 27.3 40.9





#13

2-Methylphenol

Concen: 19.039 ng/ul

RT: 8.410 min Scan# 906

Delta R.T. 0.000 min

Lab File: BG058137.D

Acq: 10 Jul 2023 11:24

Instrument :

BNA_G

ClientSampleId :





SSTD020506

Tgt Ion:108 Resp: 60952

Ion Ratio Lower Upper

108 100

107 89.9 75.0 112.4



#14

2,2'-oxybis(1-Chloropropane)

Concen: 19.434 ng/ul

RT: 8.499 min Scan# 921

Delta R.T. 0.000 min

Lab File: BG058137.D

Acq: 10 Jul 2023 11:24




Tgt Ion: 45 Resp: 94161


Ion Ratio Lower Upper

45 100

77 13.6 9.4 14.2

79 10.8 8.3 12.5









#16
Acetophenone
Concen: 19.990 ng/ul
RT: 8.792 min Scan# 971
Delta R.T. 0.000 min
Lab File: BG058137.D
Acq: 10 Jul 2023 11:24




Instrument :
BNA_G
ClientSampleId :
SSTD020506


Tgt Ion:105 Resp: 100527
Ion Ratio Lower Upper
105 100
77 76.2 61.2 91.8
51 28.6 23.5 35.3

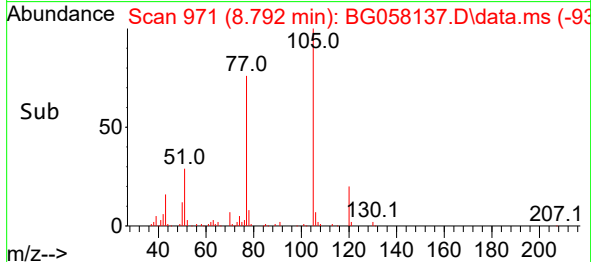

#17
N-Nitroso-di-n-propylamine
Concen: 19.813 ng/ul
RT: 8.769 min Scan# 967
Delta R.T. 0.000 min
Lab File: BG058137.D
Acq: 10 Jul 2023 11:24

Tgt Ion: 70 Resp: 53265
Ion Ratio Lower Upper
70 100
42 56.1 48.0 72.0
101 7.3 7.4 11.2#
130 18.7 13.4 20.0









#18
4-Methylphenol
Concen: 19.873 ng/ul
RT: 8.739 min Scan# 962
Delta R.T. 0.000 min
Lab File: BG058137.D
Acq: 10 Jul 2023 11:24




Instrument :
BNA_G
ClientSampleId :
SSTD020506


Tgt Ion:108 Resp: 68795
Ion Ratio Lower Upper
108 100
107 112.9 91.1 136.7



#19
Hexachloroethane
Concen: 19.371 ng/ul
RT: 9.057 min Scan# 1016
Delta R.T. 0.000 min
Lab File: BG058137.D
Acq: 10 Jul 2023 11:24

Tgt Ion:117 Resp: 21410
Ion Ratio Lower Upper
117 100
201 119.4 94.0 141.0
199 71.8 59.8 89.6





#22

Nitrobenzene

Concen: 19.352 ng/ul

RT: 9.174 min Scan# 1036

Delta R.T. 0.000 min

Lab File: BG058137.D

Acq: 10 Jul 2023 11:24

Instrument :

BNA_G

ClientSampleId :

SSTD020506





Tgt Ion: 77 Resp: 73745

Ion Ratio Lower Upper

77 100

123 41.9 33.3 49.9

65 12.9 10.4 15.6

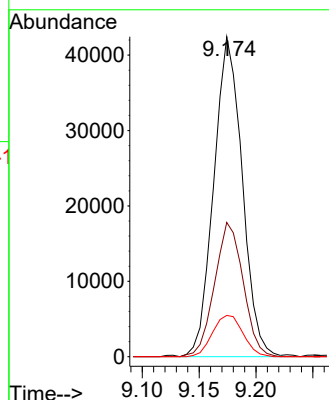

#23

Isophorone

Concen: 19.407 ng/ul

RT: 9.691 min Scan# 1124

Delta R.T. 0.000 min

Lab File: BG058137.D

Acq: 10 Jul 2023 11:24




Tgt Ion: 82 Resp: 157809


Ion Ratio Lower Upper

82 100

95 6.7 4.8 7.2

138 14.3 11.4 17.0



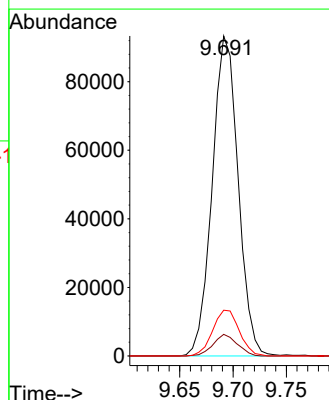
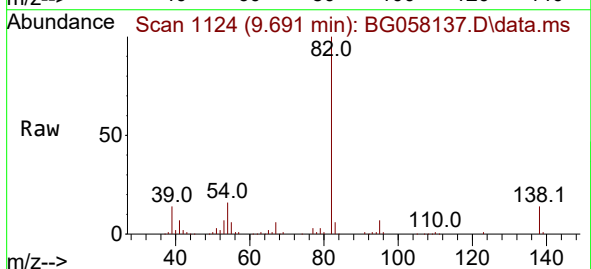




#25
2-Nitrophenol
Concen: 19.990 ng/ul
RT: 9.891 min Scan# 1158
Delta R.T. 0.000 min
Lab File: BG058137.D
Acq: 10 Jul 2023 11:24




Instrument :
BNA_G
ClientSampleId :
SSTD020506


Tgt Ion:139 Resp: 33093
Ion Ratio Lower Upper
139 100
65 54.9 42.6 64.0
109 27.7 20.7 31.1



#26
2,4-Dimethylphenol
Concen: 19.862 ng/ul
RT: 9.944 min Scan# 1167
Delta R.T. 0.000 min
Lab File: BG058137.D
Acq: 10 Jul 2023 11:24

Tgt Ion:107 Resp: 73937
Ion Ratio Lower Upper
107 100
121 50.3 40.6 60.8
122 81.9 67.1 100.7





#27

Bis(2-Chloroethoxy)methane

Concen: 19.404 ng/ul

RT: 10.173 min Scan# 1206

Delta R.T. 0.000 min

Lab File: BG058137.D

Acq: 10 Jul 2023 11:24

Instrument :

BNA_G

ClientSampleId :

SSTD020506





Tgt Ion: 93 Resp: 88909

Ion Ratio Lower Upper

93 100

95 32.0 26.4 39.6

123 10.2 7.9 11.9



#29

2,4-Dichlorophenol

Concen: 20.376 ng/ul

RT: 10.426 min Scan# 1249

Delta R.T. 0.000 min

Lab File: BG058137.D

Acq: 10 Jul 2023 11:24




Tgt Ion:162 Resp: 58632


Ion Ratio Lower Upper

162 100

164 66.2 51.1 76.7


98 37.2 27.9 41.9

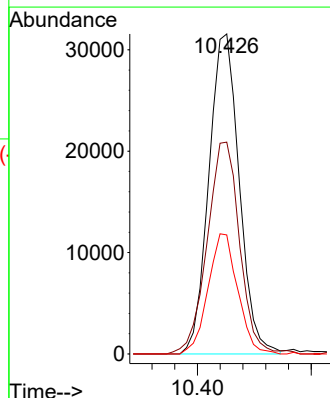






#30
Naphthalene
Concen: 19.640 ng/ul
RT: 10.825 min Scan# 11
Delta R.T. 0.000 min
Lab File: BG058137.D
Acq: 10 Jul 2023 11:24

Instrument :
BNA_G
ClientSampleId :
SSTD020506







Tgt Ion:128 Resp: 198784
Ion Ratio Lower Upper
128 100
129 11.7 8.6 12.8
127 12.7 10.2 15.2

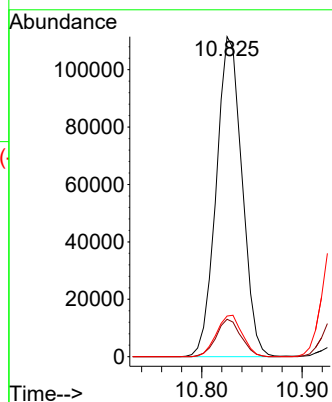

#32
4-Chloroaniline
Concen: 20.081 ng/ul
RT: 10.937 min Scan# 1336
Delta R.T. 0.000 min
Lab File: BG058137.D
Acq: 10 Jul 2023 11:24

Tgt Ion:127 Resp: 92135
Ion Ratio Lower Upper
127 100
129 32.7 26.0 39.0









#33
Hexachlorobutadiene
Concen: 19.553 ng/ul
RT: 11.107 min Scan# 1365
Delta R.T. 0.000 min
Lab File: BG058137.D
Acq: 10 Jul 2023 11:24




Instrument :
BNA_G
ClientSampleId :
SSTD020506


Tgt Ion:225 Resp: 39834
Ion Ratio Lower Upper
225 100
223 62.1 53.2 79.8
227 67.0 51.4 77.2

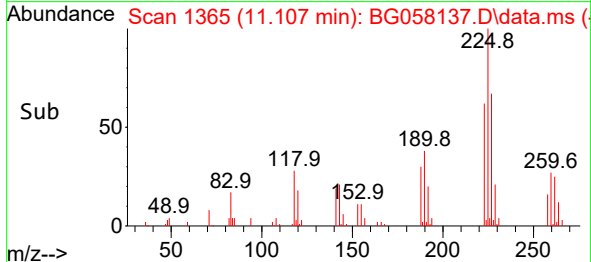

#34
Caprolactam
Concen: 19.039 ng/ul
RT: 11.683 min Scan# 1463
Delta R.T. 0.000 min
Lab File: BG058137.D
Acq: 10 Jul 2023 11:24

Tgt Ion:113 Resp: 22026
Ion Ratio Lower Upper
113 100
55 229.9 183.4 275.2
56 165.3 123.0 184.6



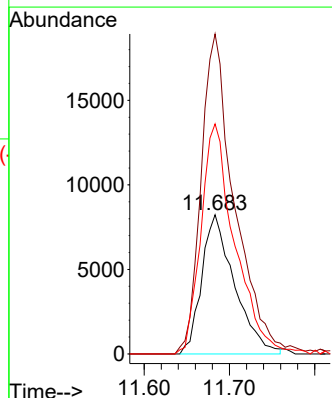





#35
 4-Chloro-3-methylphenol
 Concen: 20.523 ng/ul
 RT: 12.053 min Scan# 1526
 Delta R.T. 0.000 min
 Lab File: BG058137.D
 Acq: 10 Jul 2023 11:24




Instrument :
 BNA_G
 ClientSampleId :
 SSTD020506


Tgt Ion:107 Resp: 72543
 Ion Ratio Lower Upper
 107 100
 144 24.6 19.0 28.4
 142 71.5 58.4 87.6

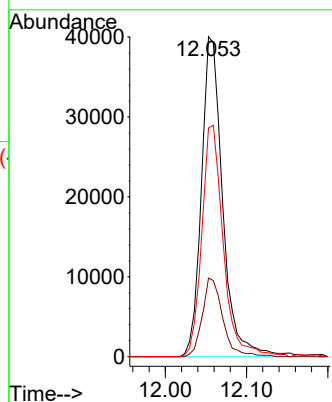

#36
 2-Methylnaphthalene
 Concen: 19.814 ng/ul
 RT: 12.429 min Scan# 1590
 Delta R.T. 0.000 min
 Lab File: BG058137.D
 Acq: 10 Jul 2023 11:24

Tgt Ion:142 Resp: 135187
 Ion Ratio Lower Upper
 142 100
 141 91.3 69.4 104.2









#37
1-Methylnaphthalene
Concen: 19.935 ng/ul
RT: 12.652 min Scan# 1628
Delta R.T. 0.000 min
Lab File: BG058137.D
Acq: 10 Jul 2023 11:24




Instrument :
BNA_G
ClientSampleId :
SSTD020506


Tgt Ion:142 Resp: 136393
Ion Ratio Lower Upper
142 100
141 96.8 73.8 110.8
116 4.2 3.0 4.4



#39
1,2,4,5-Tetrachlorobenzene
Concen: 19.817 ng/ul
RT: 12.799 min Scan# 1653
Delta R.T. 0.000 min
Lab File: BG058137.D
Acq: 10 Jul 2023 11:24

Tgt Ion:216 Resp: 77656
Ion Ratio Lower Upper
216 100
214 78.7 64.1 96.1
179 19.0 16.0 24.0
108 15.5 12.1 18.1









#40
Hexachlorocyclopentadiene
Concen: 22.863 ng/ul
RT: 12.776 min Scan# 1649
Delta R.T. 0.000 min
Lab File: BG058137.D
Acq: 10 Jul 2023 11:24




Instrument :
BNA_G
ClientSampleId :
SSTD020506


Tgt Ion:237 Resp: 56432
Ion Ratio Lower Upper
237 100
235 62.0 49.2 73.8
272 13.0 10.4 15.6

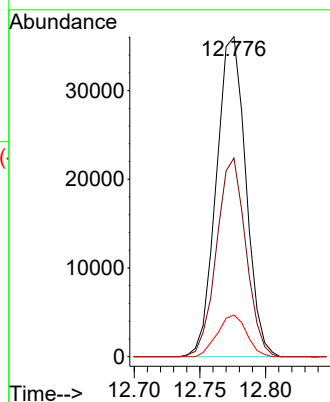

#41
2,4,6-Trichlorophenol
Concen: 20.392 ng/ul
RT: 13.034 min Scan# 1693
Delta R.T. 0.000 min
Lab File: BG058137.D
Acq: 10 Jul 2023 11:24

Tgt Ion:196 Resp: 54161
Ion Ratio Lower Upper
196 100
198 93.1 73.5 110.3
200 29.8 24.8 37.2




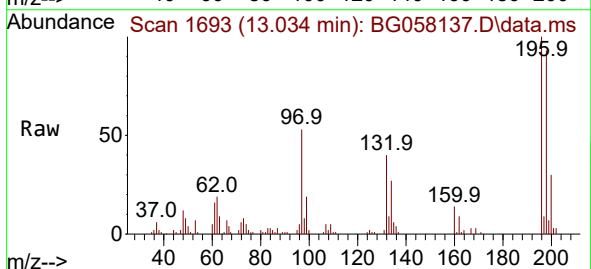




#42
2,4,5-Trichlorophenol
Concen: 19.937 ng/ul
RT: 13.111 min Scan# 1706
Delta R.T. 0.000 min
Lab File: BG058137.D
Acq: 10 Jul 2023 11:24




Instrument :
BNA_G
ClientSampleId :
SSTD020506


Tgt Ion:196 Resp: 57265
Ion Ratio Lower Upper
196 100
198 96.8 77.2 115.8
200 29.0 23.8 35.6



#43
1,1'-Biphenyl
Concen: 20.036 ng/ul
RT: 13.434 min Scan# 1761
Delta R.T. 0.000 min
Lab File: BG058137.D
Acq: 10 Jul 2023 11:24

Tgt Ion:154 Resp: 185672
Ion Ratio Lower Upper
154 100
153 40.3 32.6 49.0
76 14.2 11.6 17.4




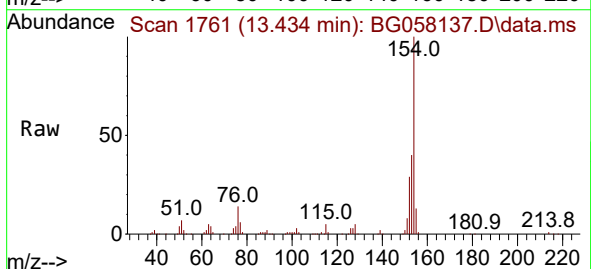




#44
2-Chloronaphthalene
Concen: 19.733 ng/ul
RT: 13.481 min Scan# 1769
Delta R.T. 0.000 min
Lab File: BG058137.D
Acq: 10 Jul 2023 11:24




Instrument :
BNA_G
ClientSampleId :
SSTD020506


Tgt Ion:162 Resp: 146757
Ion Ratio Lower Upper
162 100
164 35.0 27.7 41.5
127 38.5 30.9 46.3



#45
2-Nitroaniline
Concen: 19.969 ng/ul
RT: 13.681 min Scan# 1803
Delta R.T. 0.000 min
Lab File: BG058137.D
Acq: 10 Jul 2023 11:24

Tgt Ion: 65 Resp: 51636
Ion Ratio Lower Upper
65 100
92 64.6 53.2 79.8
138 88.1 71.1 106.7









#47
Dimethylphthalate
Concen: 19.677 ng/ul
RT: 14.051 min Scan# 1866
Delta R.T. 0.000 min
Lab File: BG058137.D
Acq: 10 Jul 2023 11:24




Instrument :
BNA_G
ClientSampleId :
SSTD020506


Tgt Ion:163 Resp: 200579
Ion Ratio Lower Upper
163 100
194 3.9 3.0 4.4
164 10.2 8.6 12.8

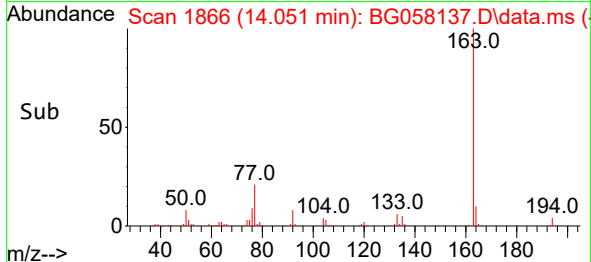

#48
2,6-Dinitrotoluene
Concen: 19.453 ng/ul
RT: 14.174 min Scan# 1887
Delta R.T. 0.000 min
Lab File: BG058137.D
Acq: 10 Jul 2023 11:24


Tgt Ion:165 Resp: 40702
Ion Ratio Lower Upper
165 100
89 55.9 42.7 64.1
121 22.4 14.8 22.2#








#50
Acenaphthylene
Concen: 20.028 ng/ul
RT: 14.327 min Scan# 1913
Delta R.T. 0.000 min
Lab File: BG058137.D
Acq: 10 Jul 2023 11:24

Instrument :
BNA_G
ClientSampleId :
SSTD020506







Tgt Ion:152 Resp: 239457
Ion Ratio Lower Upper
152 100
151 19.5 15.6 23.4
153 13.1 10.5 15.7



#51
3-Nitroaniline
Concen: 16.770 ng/ul
RT: 14.503 min Scan# 1943
Delta R.T. 0.000 min
Lab File: BG058137.D
Acq: 10 Jul 2023 11:24

Tgt Ion:138 Resp: 29652
Ion Ratio Lower Upper
138 100
108 12.4 8.2 12.2#
92 136.3 100.2 150.4









#52
Acenaphthene
Concen: 20.232 ng/ul
RT: 14.662 min Scan# 1970
Delta R.T. 0.000 min
Lab File: BG058137.D
Acq: 10 Jul 2023 11:24




Instrument :
BNA_G
ClientSampleId :
SSTD020506


Tgt Ion:153 Resp: 165982
Ion Ratio Lower Upper
153 100
152 47.5 36.5 54.7
154 84.9 70.5 105.7

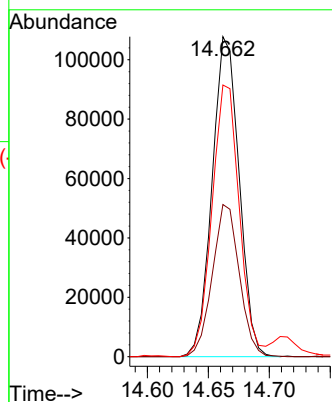

#53
2,4-Dinitrophenol
Concen: 18.174 ng/ul
RT: 14.715 min Scan# 1979
Delta R.T. 0.000 min
Lab File: BG058137.D
Acq: 10 Jul 2023 11:24

Tgt Ion:184 Resp: 19824
Ion Ratio Lower Upper
184 100
63 57.8 51.1 76.7
154 56.4 43.3 64.9









#55
4-Nitrophenol
Concen: 17.901 ng/ul
RT: 14.815 min Scan# 1996
Delta R.T. 0.000 min
Lab File: BG058137.D
Acq: 10 Jul 2023 11:24




Instrument :
BNA_G
ClientSampleId :
SSTD020506


Tgt Ion:109 Resp: 23771
Ion Ratio Lower Upper
109 100
139 139.4 119.0 178.4
65 158.3 135.5 203.3



#56
Dibenzofuran
Concen: 20.288 ng/ul
RT: 14.997 min Scan# 2027
Delta R.T. 0.000 min
Lab File: BG058137.D
Acq: 10 Jul 2023 11:24

Tgt Ion:168 Resp: 236607
Ion Ratio Lower Upper
168 100
139 33.1 27.6 41.4





#57

2,4-Dinitrotoluene

Concen: 19.865 ng/ul

RT: 14.962 min Scan# 2021

Delta R.T. 0.000 min

Lab File: BG058137.D

Acq: 10 Jul 2023 11:24

Instrument :

BNA_G

ClientSampleId :

SSTD020506





Tgt Ion:165 Resp: 58889

Ion Ratio Lower Upper

165 100

63 45.3 35.8 53.8

182 2.1 1.6 2.4



#58

2,3,4,6-Tetrachlorophenol

Concen: 19.632 ng/ul

RT: 15.226 min Scan# 2066

Delta R.T. 0.000 min

Lab File: BG058137.D

Acq: 10 Jul 2023 11:24

Tgt Ion:232 Resp: 51335




Ion Ratio Lower Upper


232 100

131 37.9 30.5 45.7

130 2.1 1.4 2.0#

166 27.7 22.6 34.0



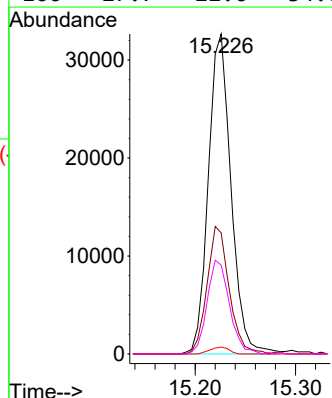





#59
Diethylphthalate
Concen: 19.318 ng/ul
RT: 15.408 min Scan# 2097
Delta R.T. 0.000 min
Lab File: BG058137.D
Acq: 10 Jul 2023 11:24




Instrument :
BNA_G
ClientSampleId :
SSTD020506


Tgt Ion:149 Resp: 205525
Ion Ratio Lower Upper
149 100
177 22.1 17.8 26.8
150 12.2 10.1 15.1



#61
Fluorene
Concen: 20.293 ng/ul
RT: 15.649 min Scan# 2138
Delta R.T. 0.000 min
Lab File: BG058137.D
Acq: 10 Jul 2023 11:24

Tgt Ion:166 Resp: 194187
Ion Ratio Lower Upper
166 100
165 102.6 79.1 118.7
167 14.3 10.7 16.1









#62
4-Chlorophenyl-phenylether
Concen: 20.485 ng/ul
RT: 15.637 min Scan# 2136
Delta R.T. 0.000 min
Lab File: BG058137.D
Acq: 10 Jul 2023 11:24




Instrument :
BNA_G
ClientSampleId :
SSTD020506


Tgt Ion:204 Resp: 103719
Ion Ratio Lower Upper
204 100
206 32.6 25.8 38.6
141 51.0 41.8 62.6

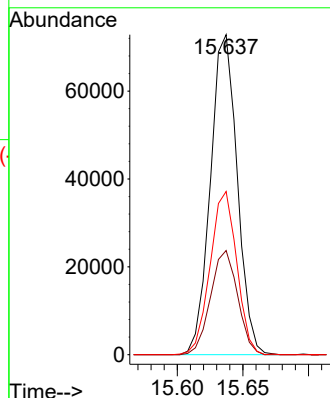

#63
4-Nitroaniline
Concen: 12.525 ng/ul
RT: 15.661 min Scan# 2140
Delta R.T. 0.000 min
Lab File: BG058137.D
Acq: 10 Jul 2023 11:24

Tgt Ion:138 Resp: 19839
Ion Ratio Lower Upper
138 100
92 50.4 43.8 65.8
108 73.8 58.8 88.2









#66
 4,6-Dinitro-2-methylphenol
 Concen: 19.453 ng/ul
 RT: 15.719 min Scan# 2150
 Delta R.T. 0.000 min
 Lab File: BG058137.D
 Acq: 10 Jul 2023 11:24




Instrument :
 BNA_G
 ClientSampleId :
 SSTD020506


Tgt Ion:198 Resp: 33452
 Ion Ratio Lower Upper
 198 100
 182 4.4 3.1 4.7
 77 25.7 17.9 26.9

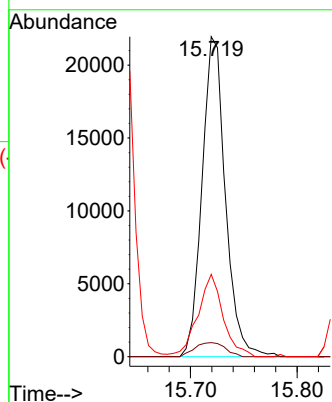

#67
 N-Nitrosodiphenylamine
 Concen: 19.917 ng/ul
 RT: 15.849 min Scan# 2172
 Delta R.T. 0.000 min
 Lab File: BG058137.D
 Acq: 10 Jul 2023 11:24

Tgt Ion:169 Resp: 164148
 Ion Ratio Lower Upper
 169 100
 168 67.5 54.2 81.2
 167 39.2 30.8 46.2



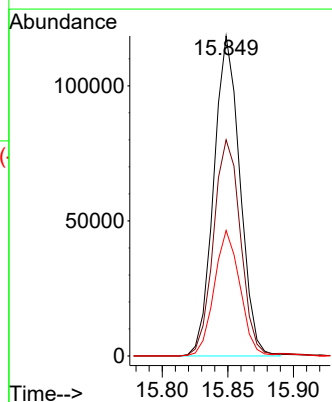
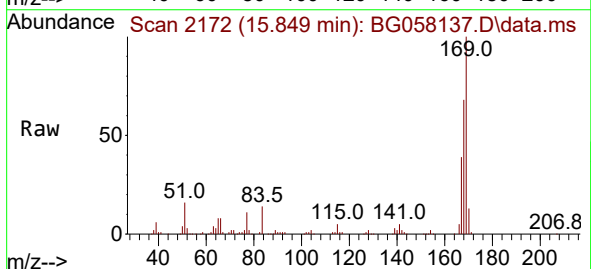




#68
4-Bromophenyl-phenylether
Concen: 20.343 ng/ul
RT: 16.530 min Scan# 21
Delta R.T. 0.000 min
Lab File: BG058137.D
Acq: 10 Jul 2023 11:24




Instrument :
BNA_G
ClientSampleId :
SSTD020506


Tgt Ion:248 Resp: 69152
Ion Ratio Lower Upper
248 100
250 96.9 78.3 117.5
141 60.7 49.1 73.7

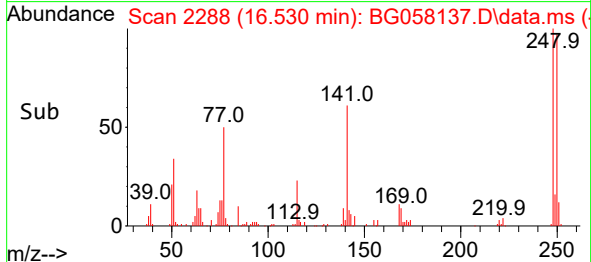

#69
Hexachlorobenzene
Concen: 20.488 ng/ul
RT: 16.648 min Scan# 2308
Delta R.T. 0.000 min
Lab File: BG058137.D
Acq: 10 Jul 2023 11:24

Tgt Ion:284 Resp: 77973
Ion Ratio Lower Upper
284 100
142 27.0 21.9 32.9
249 33.4 25.0 37.6





#70

Atrazine

Concen: 19.187 ng/ul

RT: 16.795 min Scan# 21

Delta R.T. 0.000 min

Lab File: BG058137.D

Acq: 10 Jul 2023 11:24

Instrument :

BNA_G

ClientSampleId :

SSTD020506





Tgt Ion:200 Resp: 64662

Ion Ratio Lower Upper

200 100

173 25.6 20.0 30.0

215 46.8 35.8 53.8

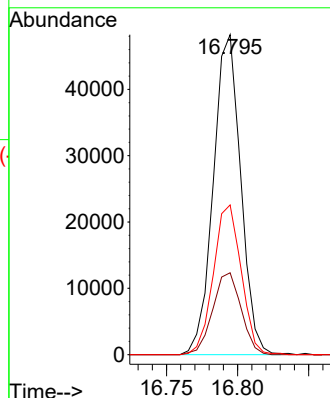

#71

Pentachlorophenol

Concen: 17.963 ng/ul

RT: 16.994 min Scan# 2367

Delta R.T. 0.000 min

Lab File: BG058137.D

Acq: 10 Jul 2023 11:24




Tgt Ion:266 Resp: 41043


Ion Ratio Lower Upper

266 100

264 62.5 51.5 77.3

268 68.3 49.0 73.4









#72
Phenanthrene
Concen: 20.118 ng/ul
RT: 17.382 min Scan# 2433
Delta R.T. 0.000 min
Lab File: BG058137.D
Acq: 10 Jul 2023 11:24




Instrument :
BNA_G
ClientSampleId :
SSTD020506


Tgt Ion:178 Resp: 316909
Ion Ratio Lower Upper
178 100
179 16.2 12.8 19.2
176 19.6 15.7 23.5

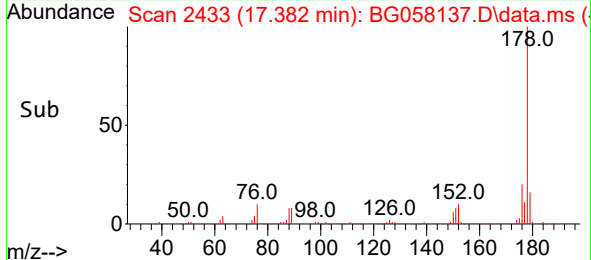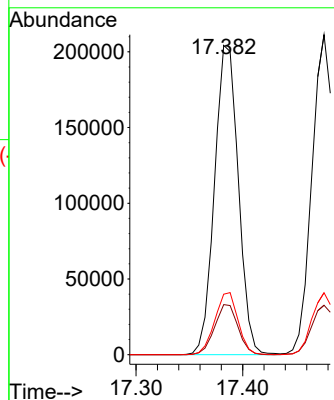

#74
Anthracene
Concen: 19.898 ng/ul
RT: 17.476 min Scan# 2449
Delta R.T. 0.000 min
Lab File: BG058137.D
Acq: 10 Jul 2023 11:24

Tgt Ion:178 Resp: 317181
Ion Ratio Lower Upper
178 100
179 15.5 12.6 18.8
176 19.3 15.4 23.2



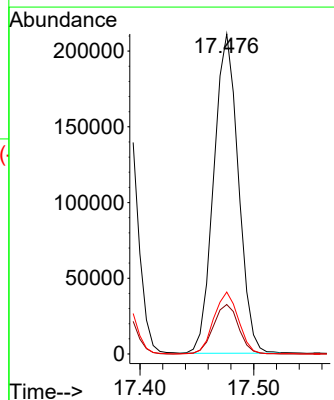





#75
1,2,3,4-Tetrachlorobenzene
Concen: 20.366 ng/uL
RT: 13.399 min Scan# 1755
Delta R.T. 0.000 min
Lab File: BG058137.D
Acq: 10 Jul 2023 11:24




Instrument :
BNA_G
ClientSampleId :
SSTD020506


Tgt Ion:216 Resp: 83641
Ion Ratio Lower Upper
216 100
214 75.9 64.8 97.2
218 46.3 39.1 58.7



#76
Pentachlorobenzene
Concen: 20.250 ng/uL
RT: 14.920 min Scan# 2014
Delta R.T. 0.000 min
Lab File: BG058137.D
Acq: 10 Jul 2023 11:24

Tgt Ion:250 Resp: 88823
Ion Ratio Lower Upper
250 100
248 62.8 52.8 79.2
252 64.2 52.4 78.6









#77
 Carbazole
 Concen: 19.938 ng/ul
 RT: 17.747 min Scan# 2495
 Delta R.T. 0.000 min
 Lab File: BG058137.D
 Acq: 10 Jul 2023 11:24




Instrument :
 BNA_G
 ClientSampleId :
 SSTD020506


Tgt Ion:167 Resp: 287432
 Ion Ratio Lower Upper
 167 100
 166 22.4 17.5 26.3
 139 11.8 9.5 14.3



#78
 Di-n-butylphthalate
 Concen: 19.728 ng/ul
 RT: 18.299 min Scan# 2589
 Delta R.T. 0.000 min
 Lab File: BG058137.D
 Acq: 10 Jul 2023 11:24

Tgt Ion:149 Resp: 362298
 Ion Ratio Lower Upper
 149 100
 150 8.8 7.4 11.2
 104 4.9 3.9 5.9









#80
Fluoranthene
Concen: 18.542 ng/ul
RT: 19.392 min Scan# 2775
Delta R.T. 0.000 min
Lab File: BG058137.D
Acq: 10 Jul 2023 11:24




Instrument :
BNA_G
ClientSampleId :
SSTD020506


Tgt Ion:202 Resp: 377224
Ion Ratio Lower Upper
202 100
101 11.4 9.1 13.7
100 8.7 7.1 10.7

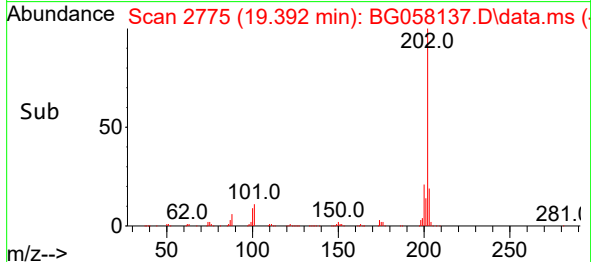

#82
Pyrene
Concen: 18.836 ng/ul
RT: 19.756 min Scan# 2837
Delta R.T. 0.000 min
Lab File: BG058137.D
Acq: 10 Jul 2023 11:24

Tgt Ion:202 Resp: 385738
Ion Ratio Lower Upper
202 100
101 12.9 10.2 15.2
100 10.6 8.9 13.3









#83
Butylbenzylphthalate
Concen: 19.043 ng/ul
RT: 20.637 min Scan# 2987
Delta R.T. 0.000 min
Lab File: BG058137.D
Acq: 10 Jul 2023 11:24




Instrument :
BNA_G
ClientSampleId :
SSTD020506


Tgt Ion:149 Resp: 158134
Ion Ratio Lower Upper
149 100
91 68.0 56.5 84.7
206 22.4 17.4 26.0



#84
3,3'-Dichlorobenzidine
Concen: 18.980 ng/ul
RT: 21.495 min Scan# 3133
Delta R.T. 0.000 min
Lab File: BG058137.D
Acq: 10 Jul 2023 11:24

Tgt Ion:252 Resp: 128091
Ion Ratio Lower Upper
252 100
254 63.1 50.7 76.1
126 8.9 6.6 10.0









#85
Benzo(a)anthracene
Concen: 19.039 ng/ul
RT: 21.577 min Scan# 3147
Delta R.T. 0.000 min
Lab File: BG058137.D
Acq: 10 Jul 2023 11:24




Instrument :
BNA_G
ClientSampleId :
SSTD020506


Tgt Ion:228 Resp: 381093
Ion Ratio Lower Upper
228 100
229 20.8 16.0 24.0
226 27.6 22.0 33.0



#86
Bis(2-ethylhexyl)phthalate
Concen: 19.433 ng/ul
RT: 21.477 min Scan# 3130
Delta R.T. 0.000 min
Lab File: BG058137.D
Acq: 10 Jul 2023 11:24

Tgt Ion:149 Resp: 231257
Ion Ratio Lower Upper
149 100
167 26.8 20.9 31.3
279 3.7 3.1 4.7






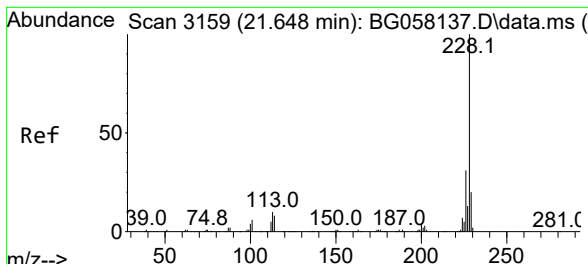


#87
 Chrysene
 Concen: 19.871 ng/ul
 RT: 21.648 min Scan# 3159
 Delta R.T. 0.000 min
 Lab File: BG058137.D
 Acq: 10 Jul 2023 11:24

Instrument :
 BNA_G
 ClientSampleId :
 SSTD020506




Tgt Ion:228 Resp: 372861


Ion	Ratio	Lower	Upper
228	100		
226	30.6	24.4	36.6
229	20.0	15.5	23.3

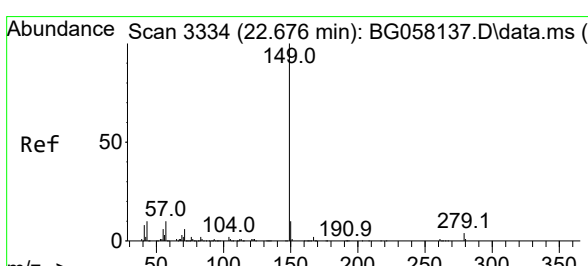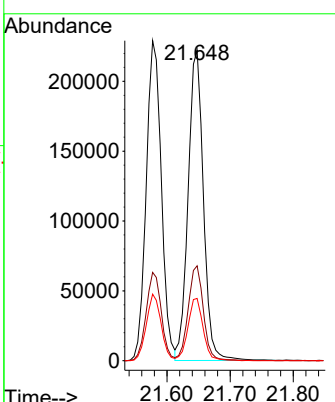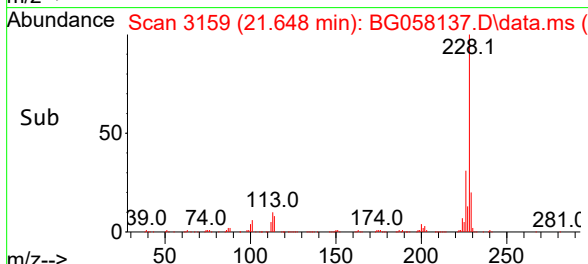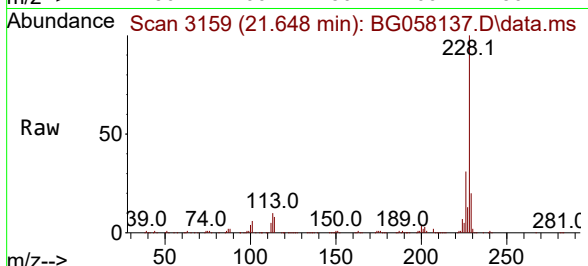

#89
 Di-n-octyl phthalate
 Concen: 19.785 ng/ul
 RT: 22.676 min Scan# 3334
 Delta R.T. 0.000 min
 Lab File: BG058137.D
 Acq: 10 Jul 2023 11:24

Tgt Ion:149 Resp: 405428


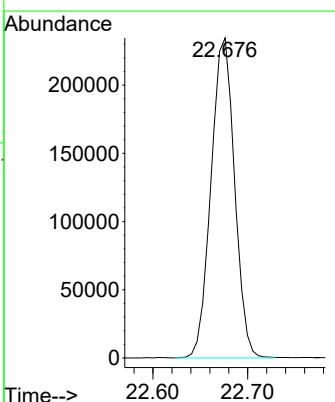
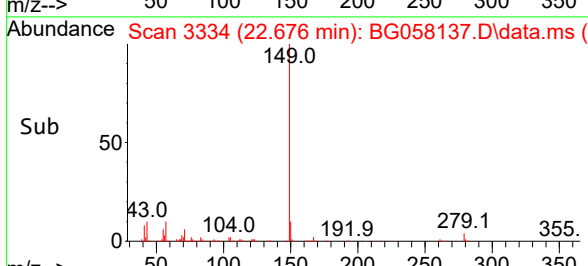
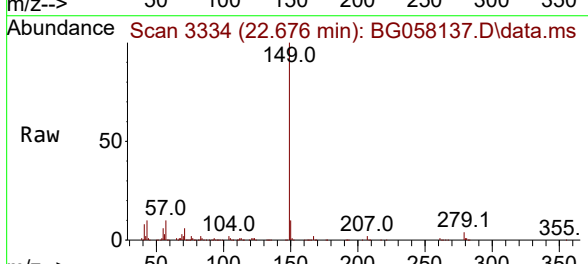




#90
Benzo(b)fluoranthene
Concen: 18.969 ng/ul
RT: 23.769 min Scan# 3520
Delta R.T. 0.000 min
Lab File: BG058137.D
Acq: 10 Jul 2023 11:24




Instrument :
BNA_G
ClientSampleId :
SSTD020506


Tgt Ion:252 Resp: 391724
Ion Ratio Lower Upper
252 100
253 21.5 18.1 27.1
125 8.2 7.5 11.3

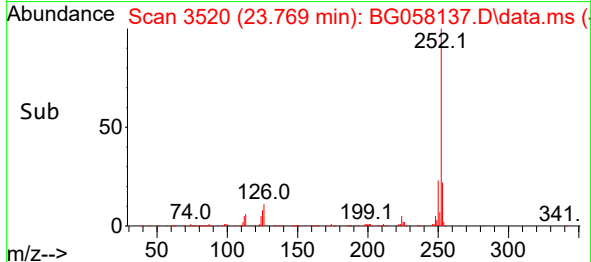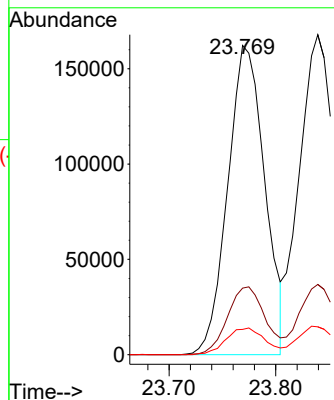

#91
Benzo(k)fluoranthene
Concen: 19.792 ng/ul
RT: 23.839 min Scan# 3532
Delta R.T. 0.000 min
Lab File: BG058137.D
Acq: 10 Jul 2023 11:24

Tgt Ion:252 Resp: 400612
Ion Ratio Lower Upper
252 100
253 21.9 17.7 26.5
125 8.7 7.4 11.2



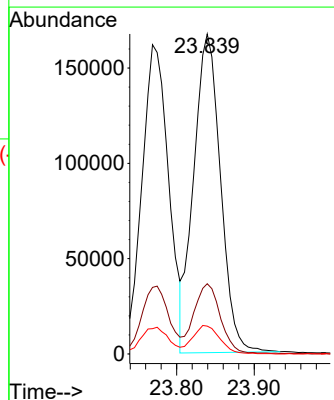





#93
Benzo(a)pyrene
Concen: 19.435 ng/ul
RT: 24.638 min Scan# 3668
Delta R.T. 0.000 min
Lab File: BG058137.D
Acq: 10 Jul 2023 11:24




Instrument :
BNA_G
ClientSampleId :
SSTD020506


Tgt Ion:252 Resp: 355232
Ion Ratio Lower Upper
252 100
253 22.1 17.8 26.6
125 10.3 8.3 12.5



#94
Indeno(1,2,3-cd)pyrene
Concen: 19.470 ng/ul
RT: 28.422 min Scan# 4312
Delta R.T. 0.000 min
Lab File: BG058137.D
Acq: 10 Jul 2023 11:24

Tgt Ion:276 Resp: 472575
Ion Ratio Lower Upper
276 100
138 17.3 14.0 21.0
277 24.2 19.4 29.2





#95

Dibenzo(a,h)anthracene

Concen: 19.638 ng/ul

RT: 28.487 min Scan# 41

Delta R.T. 0.000 min

Lab File: BG058137.D

Acq: 10 Jul 2023 11:24

Instrument :

BNA_G

ClientSampleId :

SSTD020506





Tgt Ion:278 Resp: 393036

Ion Ratio Lower Upper

278 100

139 13.1 11.3 16.9

279 22.9 18.9 28.3

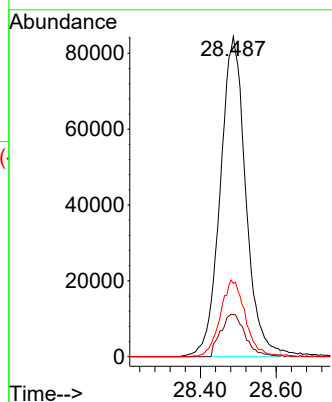

#96

Benzo(g,h,i)perylene

Concen: 19.008 ng/ul

RT: 29.562 min Scan# 4506

Delta R.T. 0.000 min

Lab File: BG058137.D

Acq: 10 Jul 2023 11:24

Tgt Ion:276 Resp: 376818

Ion Ratio Lower Upper

276 100

138 20.2 14.2 21.2

277 23.9 18.6 27.8

