




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071023\
 Data File : BP016169.D
 Acq On : 10 Jul 2023 22:39
 Operator : MA/JU
 Sample : 03404-10
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTDCCC020

Manual IntegrationsAPPROVED

Quant Time: Jul 10 23:23:53 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 10 23:19:51 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/11/2023
 Supervised By :mohammad ahmed 07/11/2023

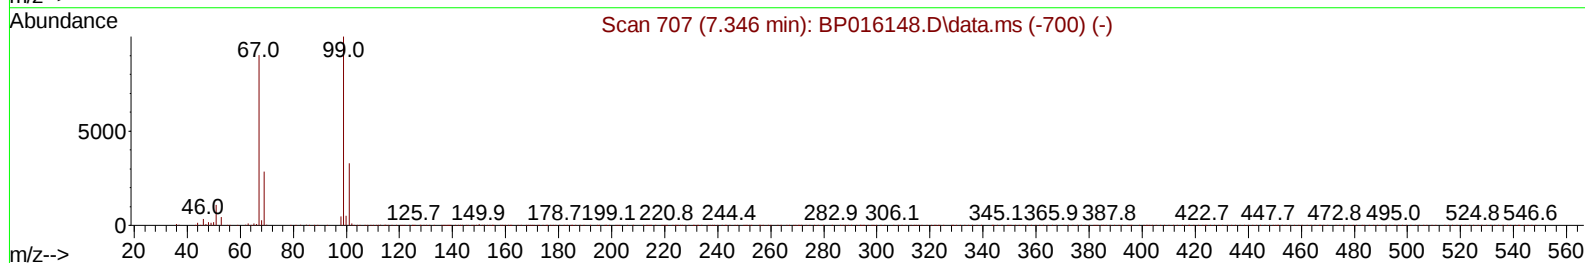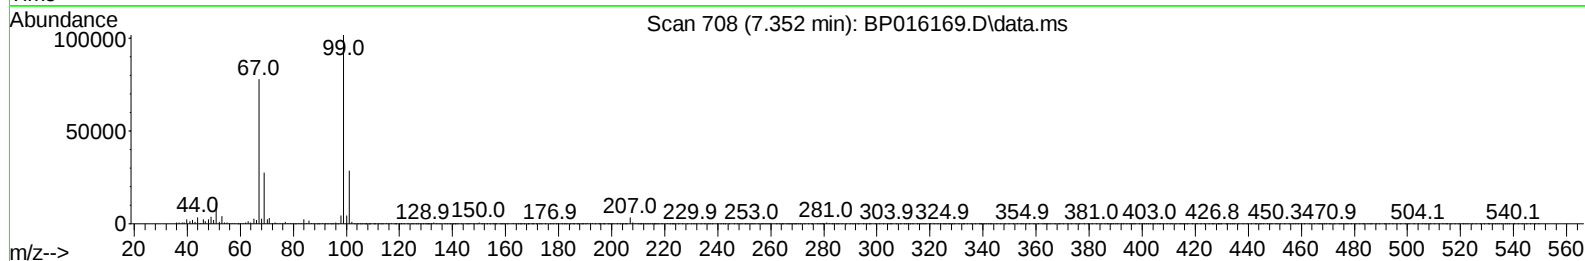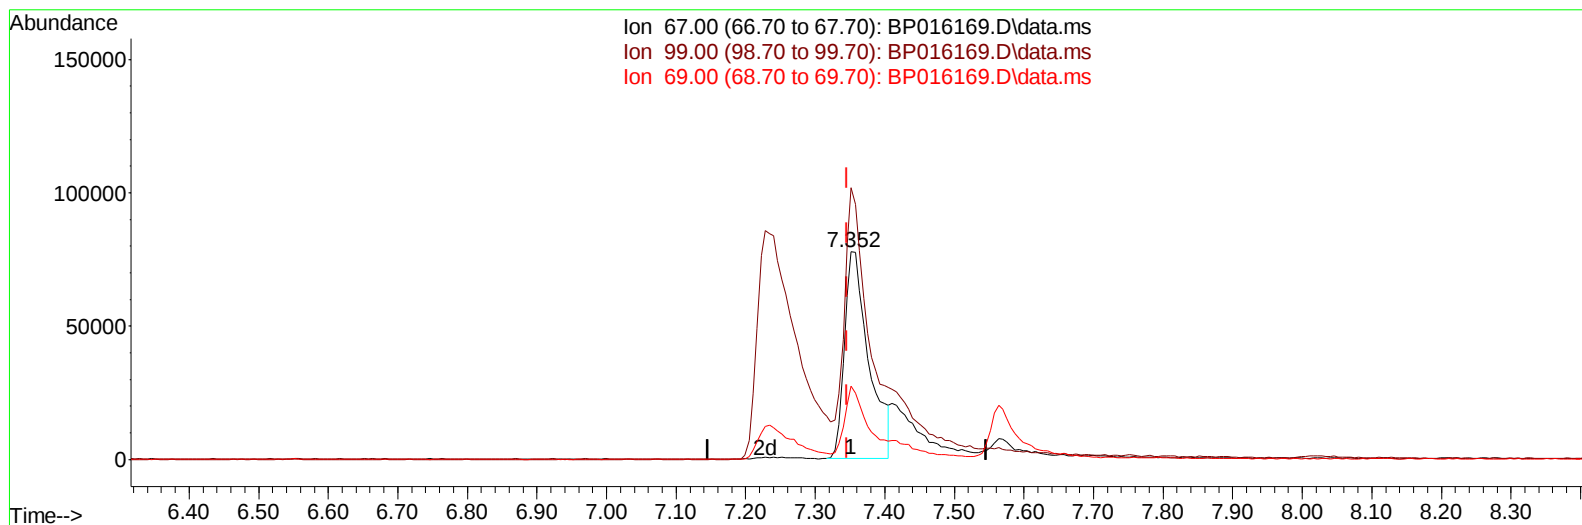

TIC: BP016169.D\data.ms

(9) Bis-(2-Chloroethyl)ether-d8 (S)

7.352min (+ 0.006) 22.38 ng/u1

response 188728

Ion	Exp%	Act%
67.00	100.00	100.00
99.00	117.80	130.57
69.00	32.10	35.41
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071023\
 Data File : BP016169.D
 Acq On : 10 Jul 2023 22:39
 Operator : MA/JU
 Sample : 03404-10
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTDCCC020

Manual IntegrationsAPPROVED

Quant Time: Jul 10 23:23:53 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 10 23:19:51 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/11/2023
 Supervised By :mohammad ahmed 07/11/2023

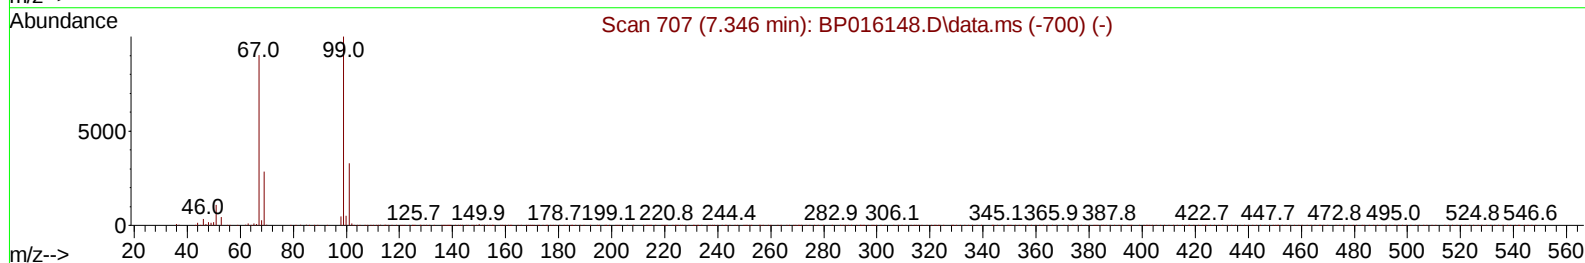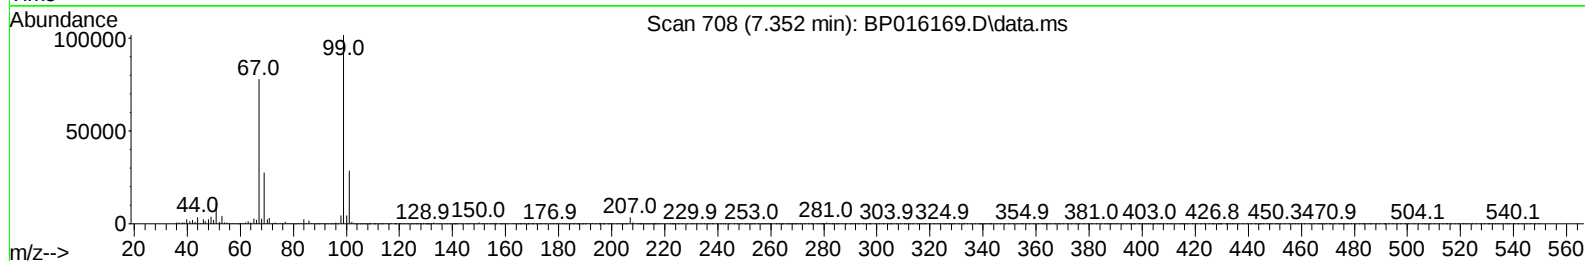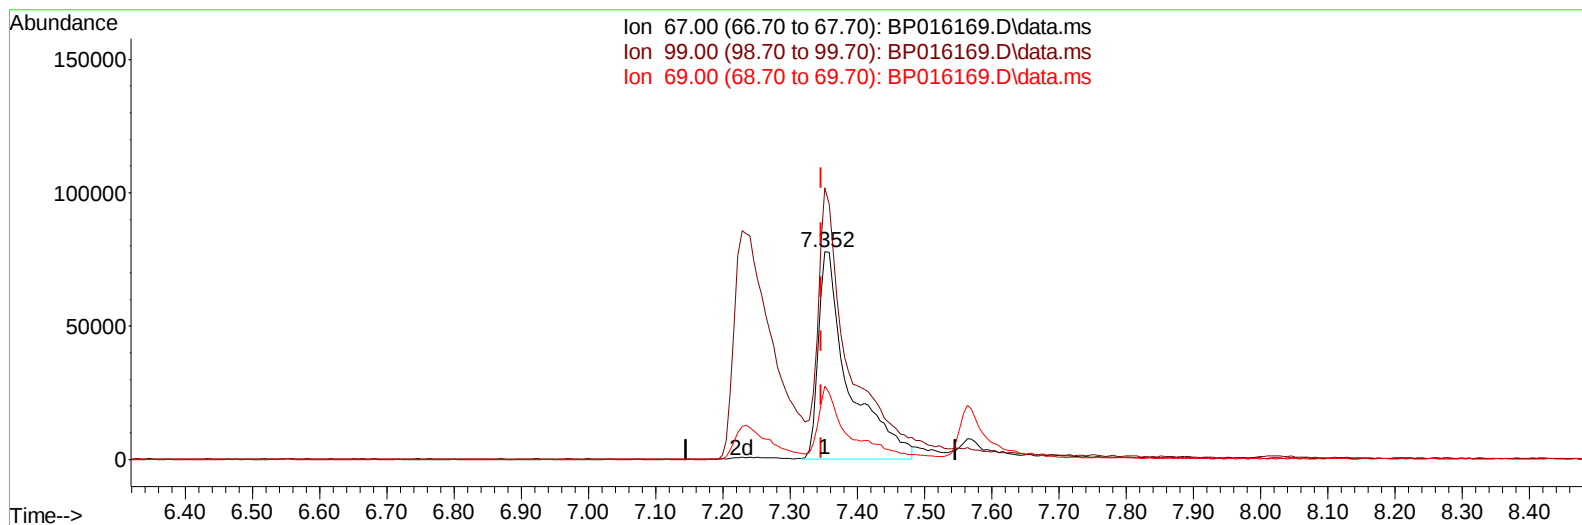

TIC: BP016169.D\data.ms

(9) Bis-(2-Chloroethyl)ether-d8 (S)

7.352min (+ 0.006) 29.04 ng/ul m

response 244879

Ion	Exp%	Act%
67.00	100.00	100.00
99.00	117.80	130.57
69.00	32.10	35.41
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071023\
Data File : BP016169.D
Acq On : 10 Jul 2023 22:39
Operator : MA/JU
Sample : 03404-10
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
LabSampleId :
SSTDCCC020

Manual IntegrationsAPPROVED

Quant Time: Jul 11 00:33:42 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 10 23:19:51 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/11/2023
Supervised By :mohammad ahmed 07/11/2023

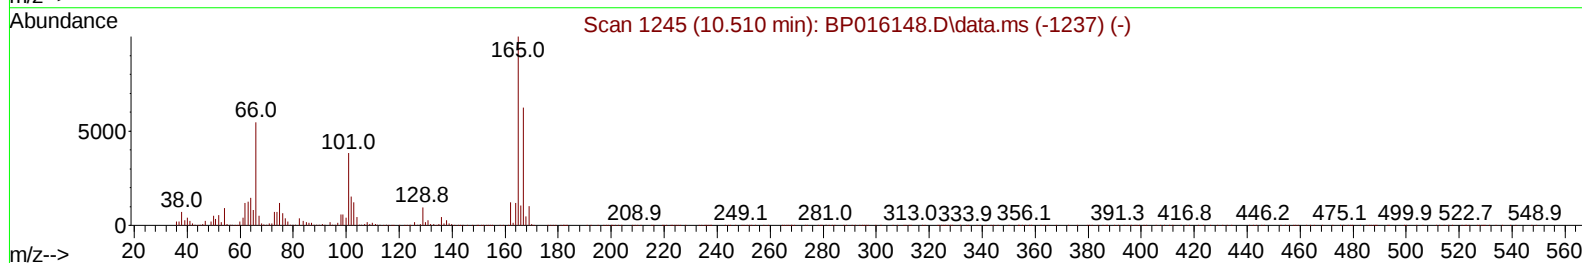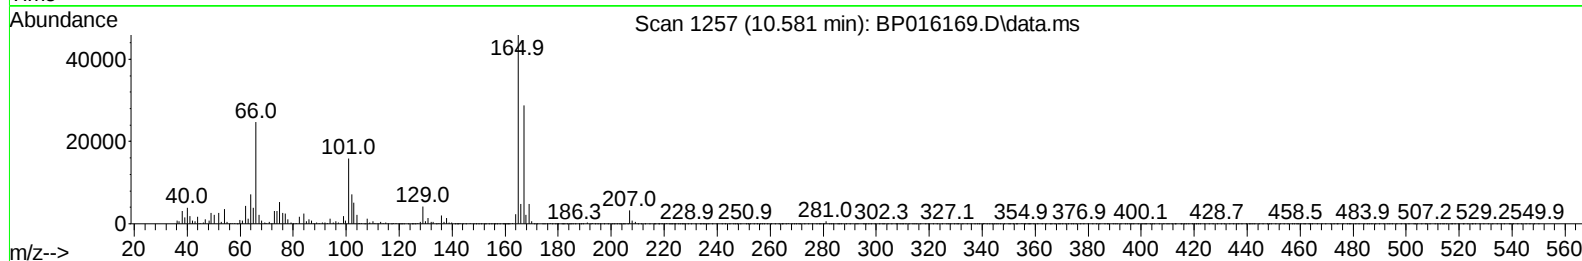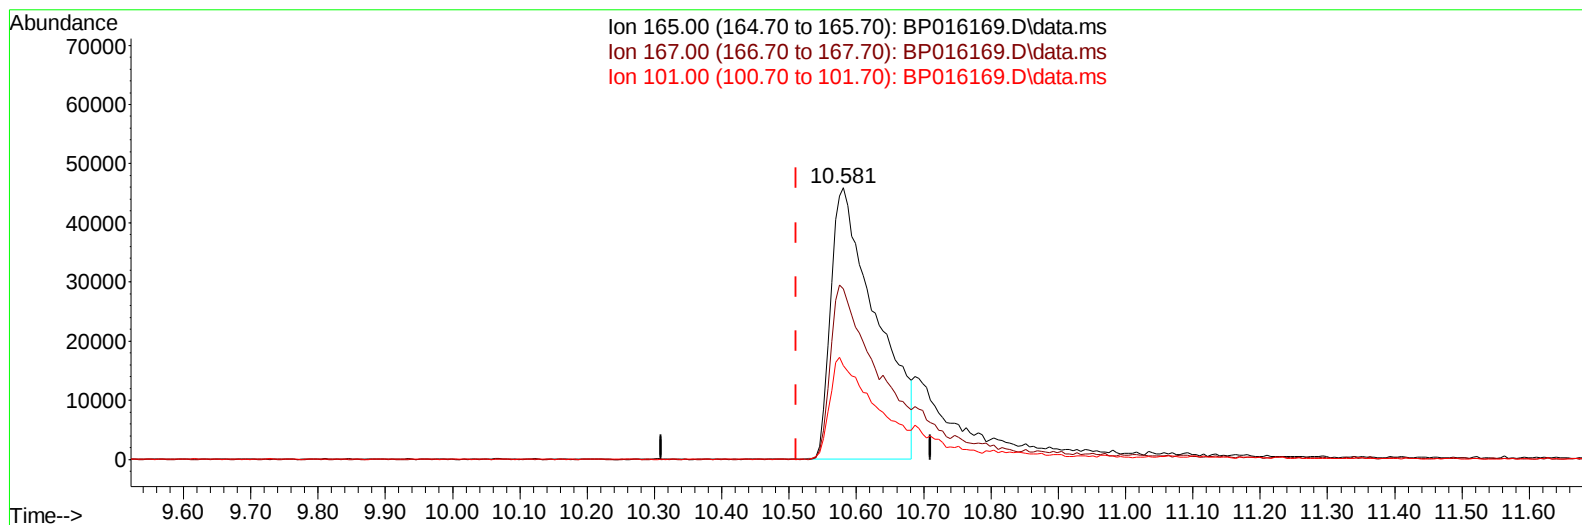

TIC: BP016169.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.581min (+ 0.071) 18.12 ng/u1

response 215661

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	66.20	62.73
101.00	37.30	34.45
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071023\
 Data File : BP016169.D
 Acq On : 10 Jul 2023 22:39
 Operator : MA/JU
 Sample : 03404-10
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTDCCC020

Manual IntegrationsAPPROVED

Quant Time: Jul 11 00:33:42 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 10 23:19:51 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/11/2023
 Supervised By :mohammad ahmed 07/11/2023

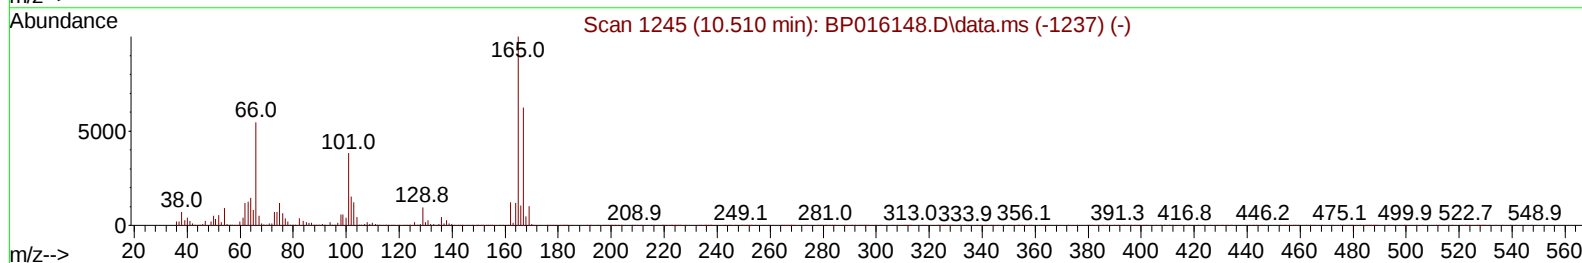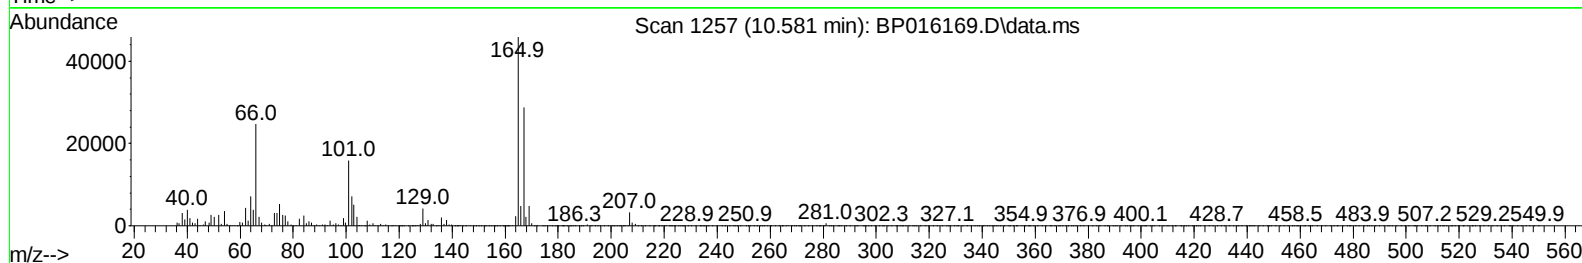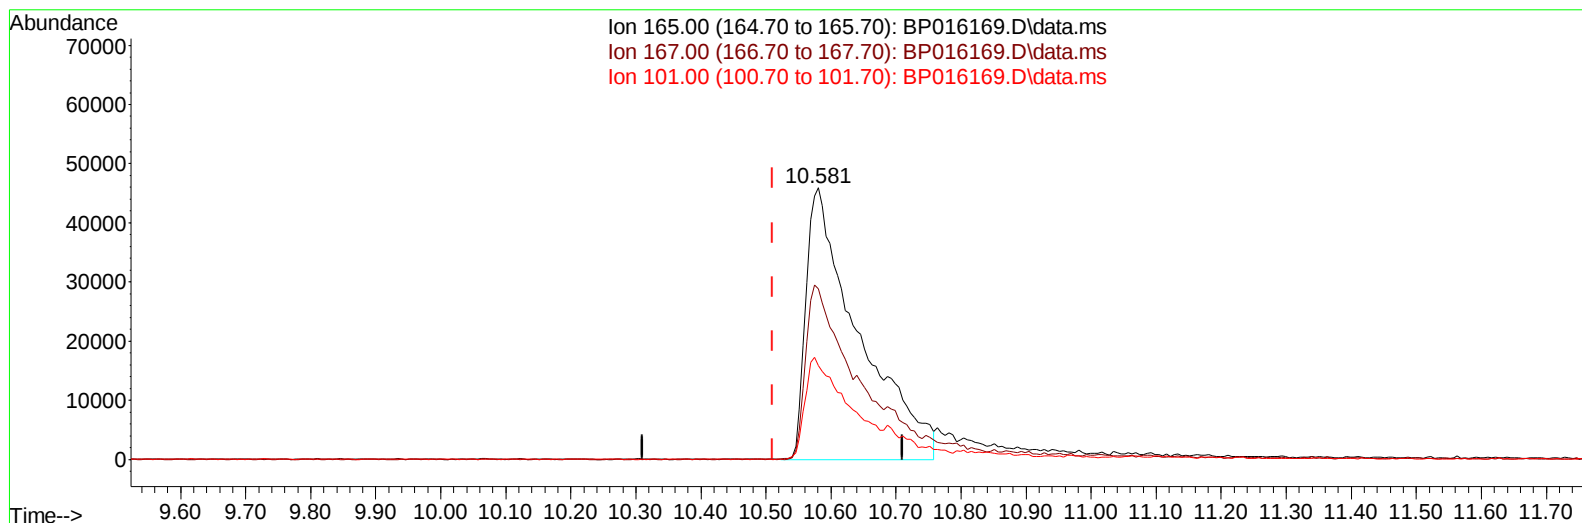

TIC: BP016169.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.581min (+ 0.071) 21.58 ng/ul m

response 256812

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	66.20	62.73
101.00	37.30	34.45
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071023\
 Data File : BP016169.D
 Acq On : 10 Jul 2023 22:39
 Operator : MA/JU
 Sample : 03404-10
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTDCCC020

Manual IntegrationsAPPROVED

Quant Time: Jul 11 00:33:42 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 10 23:19:51 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/11/2023
 Supervised By :mohammad ahmed 07/11/2023

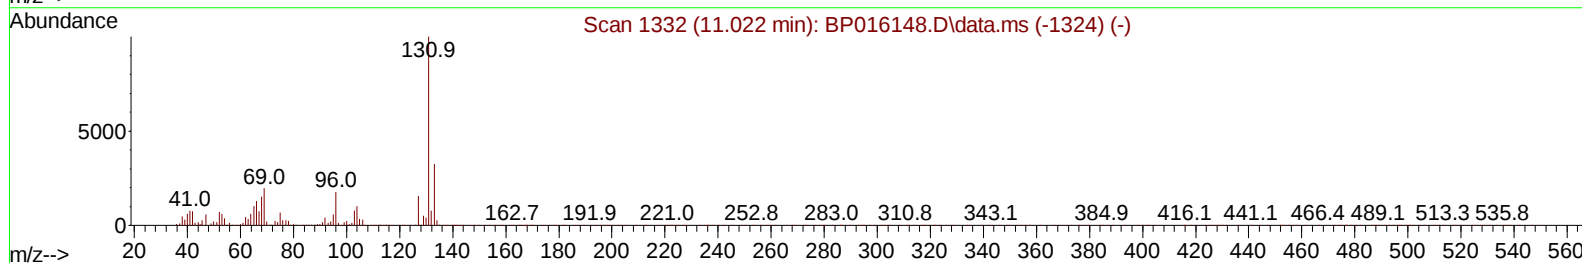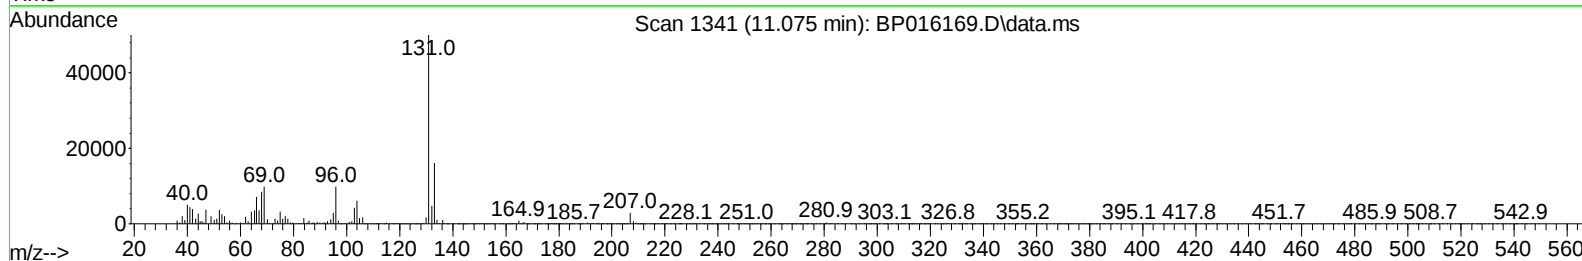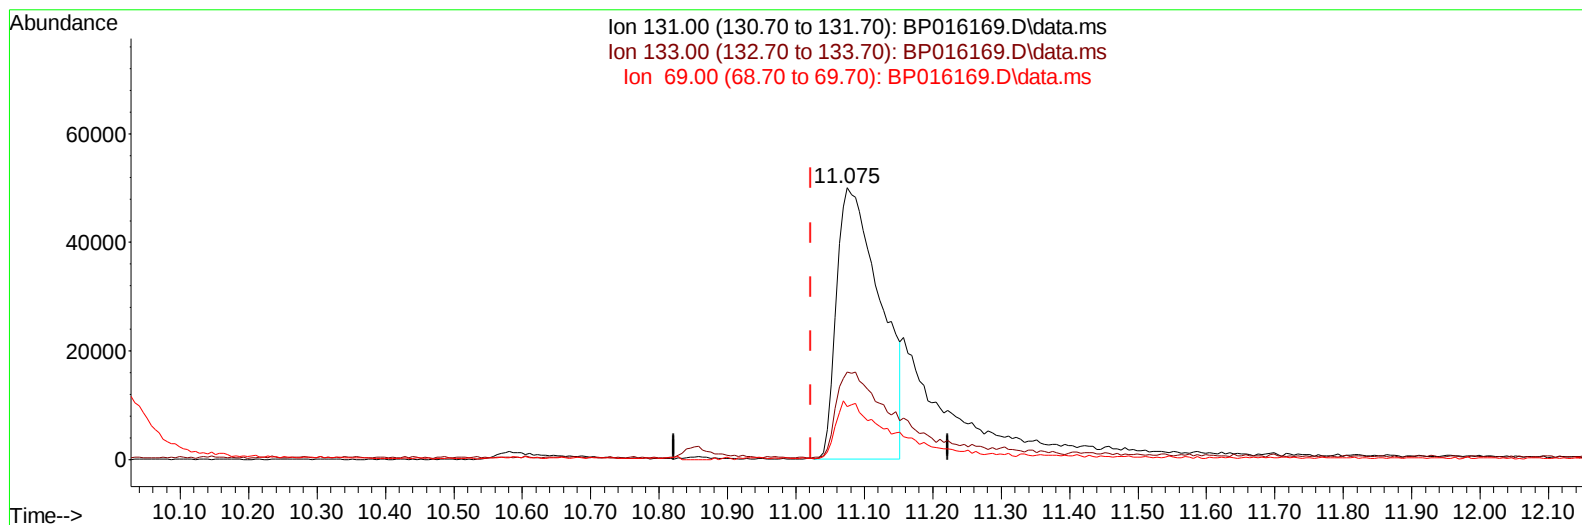

TIC: BP016169.D\data.ms

(31) 4-Chloroaniline-d4 (S)

11.075min (+ 0.053) 14.47 ng/ul

response 221112

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	34.50	32.18
69.00	22.20	19.51
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071023\
 Data File : BP016169.D
 Acq On : 10 Jul 2023 22:39
 Operator : MA/JU
 Sample : 03404-10
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTDCCC020

Manual IntegrationsAPPROVED

Quant Time: Jul 11 00:33:42 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 10 23:19:51 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/11/2023
 Supervised By :mohammad ahmed 07/11/2023

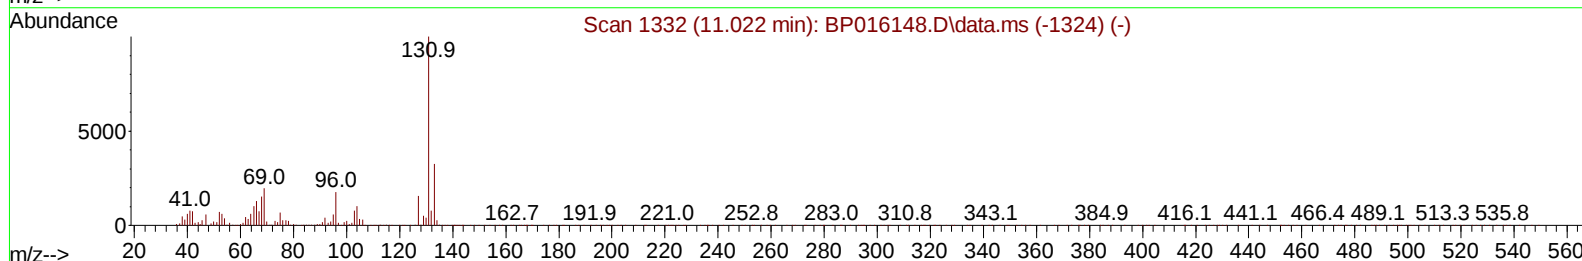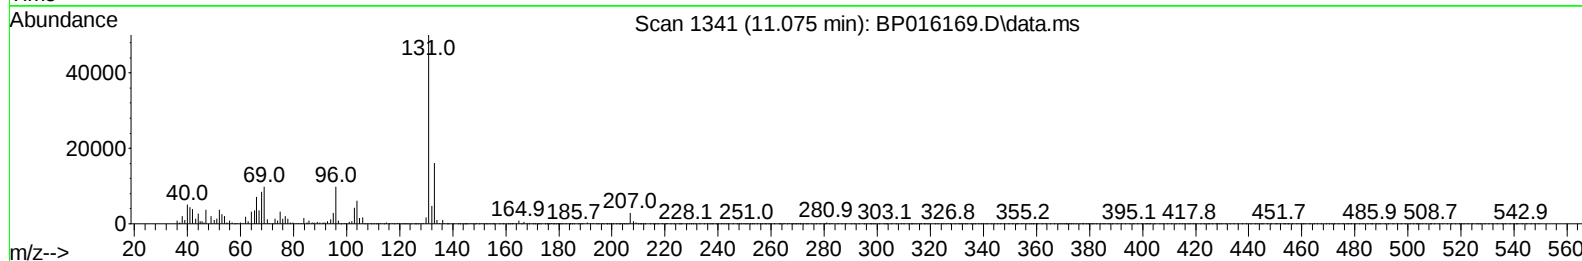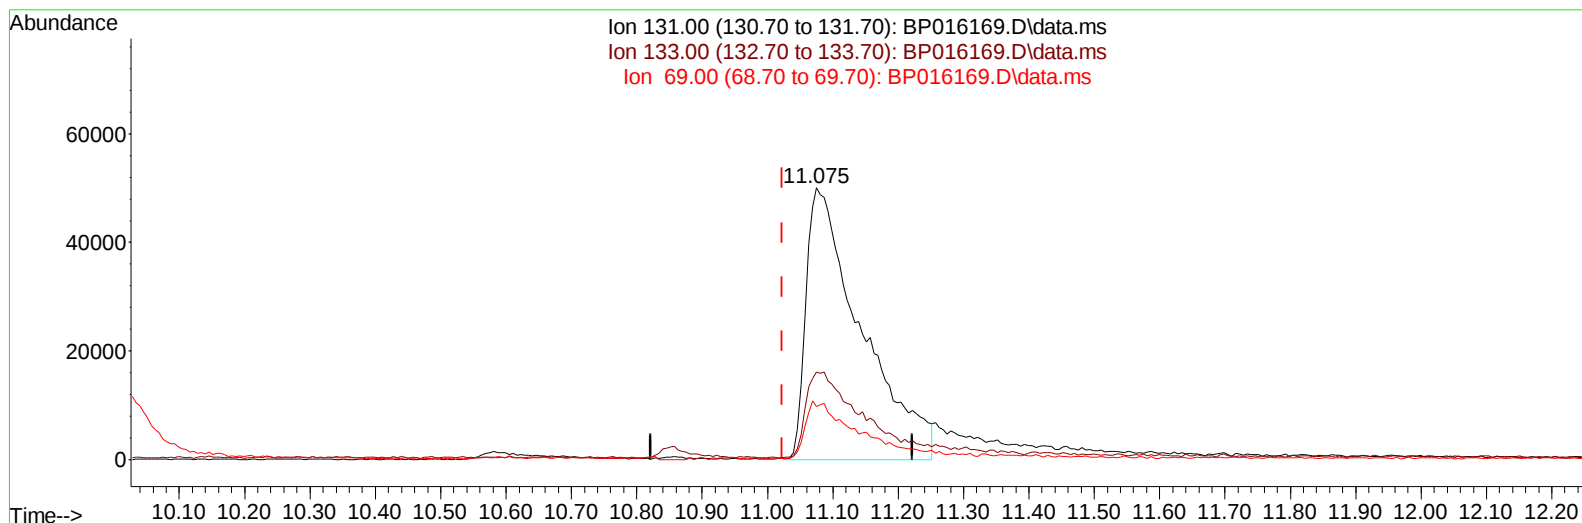

TIC: BP016169.D\data.ms

(31) 4-Chloroaniline-d4 (S)

11.075min (+ 0.053) 19.14 ng/ul m

response 292643

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	34.50	32.18
69.00	22.20	19.51
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071023\
Data File : BP016169.D
Acq On : 10 Jul 2023 22:39
Operator : MA/JU
Sample : 03404-10
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :

BNA_G




LabSampleId :

SSTDCCC020

Manual IntegrationsAPPROVED

Quant Time: Jul 11 00:33:42 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 10 23:19:51 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/11/2023
Supervised By :mohammad ahmed 07/11/2023

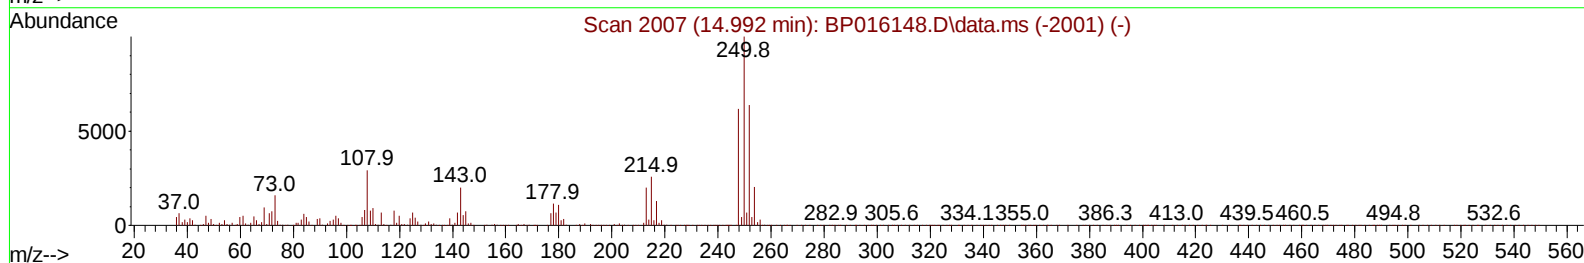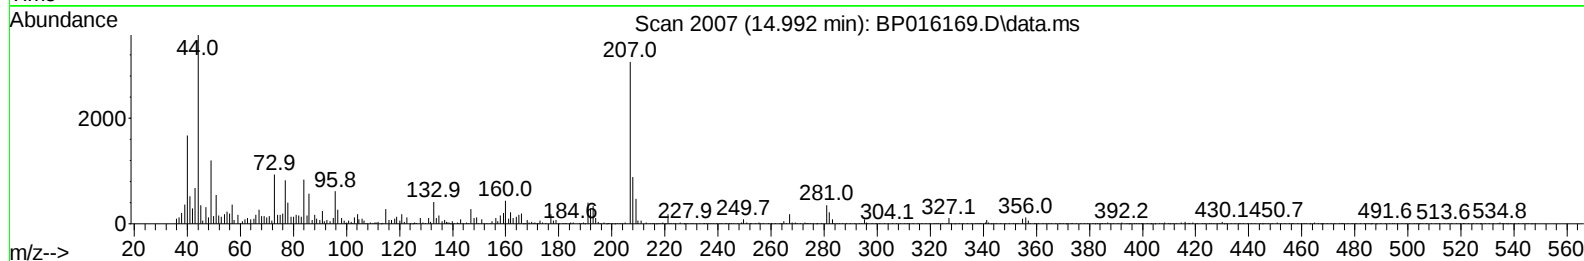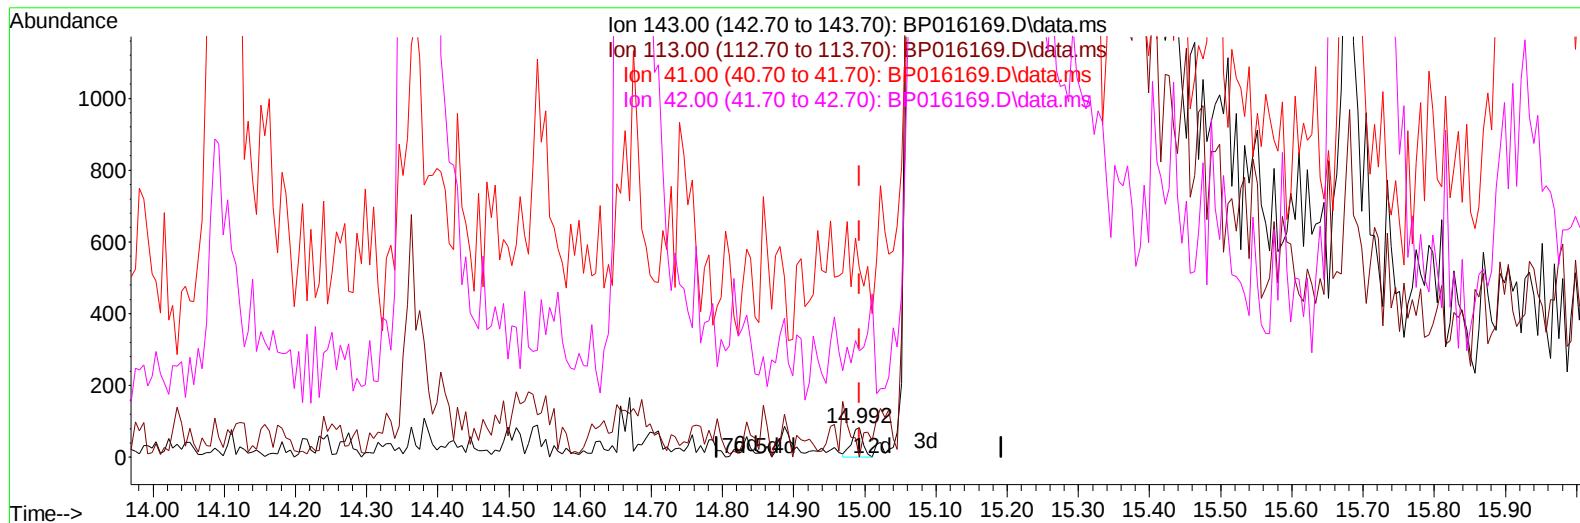

TIC: BP016169.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.992min (+ 0.000) 0.02 ng/u1

response 92

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	94.00	9.64#
41.00	45.70	634.94#
42.00	31.20	357.83#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071023\
 Data File : BP016169.D
 Acq On : 10 Jul 2023 22:39
 Operator : MA/JU
 Sample : 03404-10
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTDCCC020

Manual IntegrationsAPPROVED

Quant Time: Jul 11 00:34:26 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 10 23:19:51 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/11/2023
 Supervised By :mohammad ahmed 07/11/2023

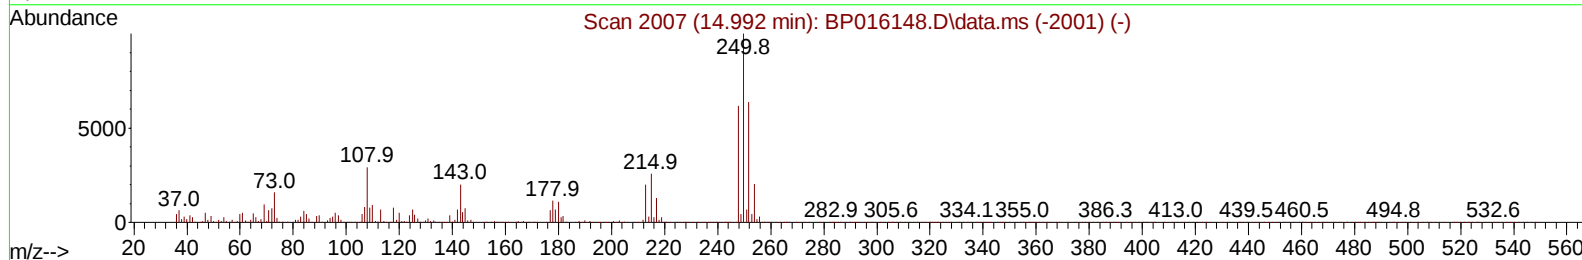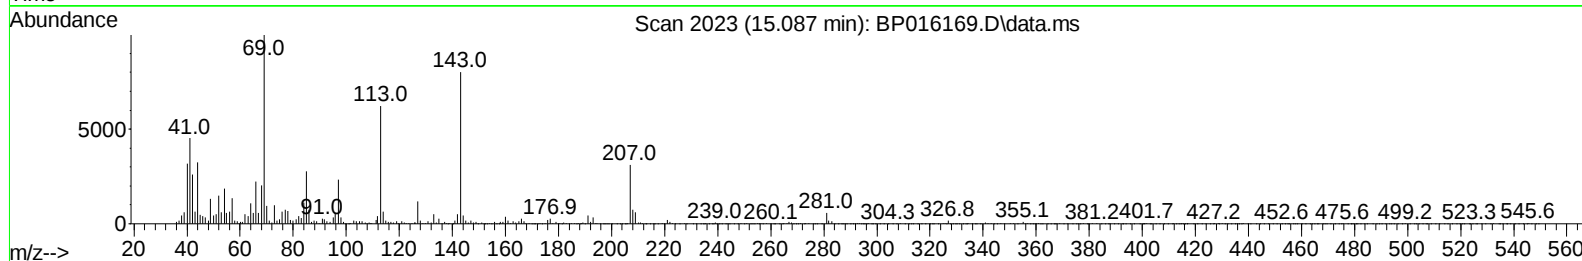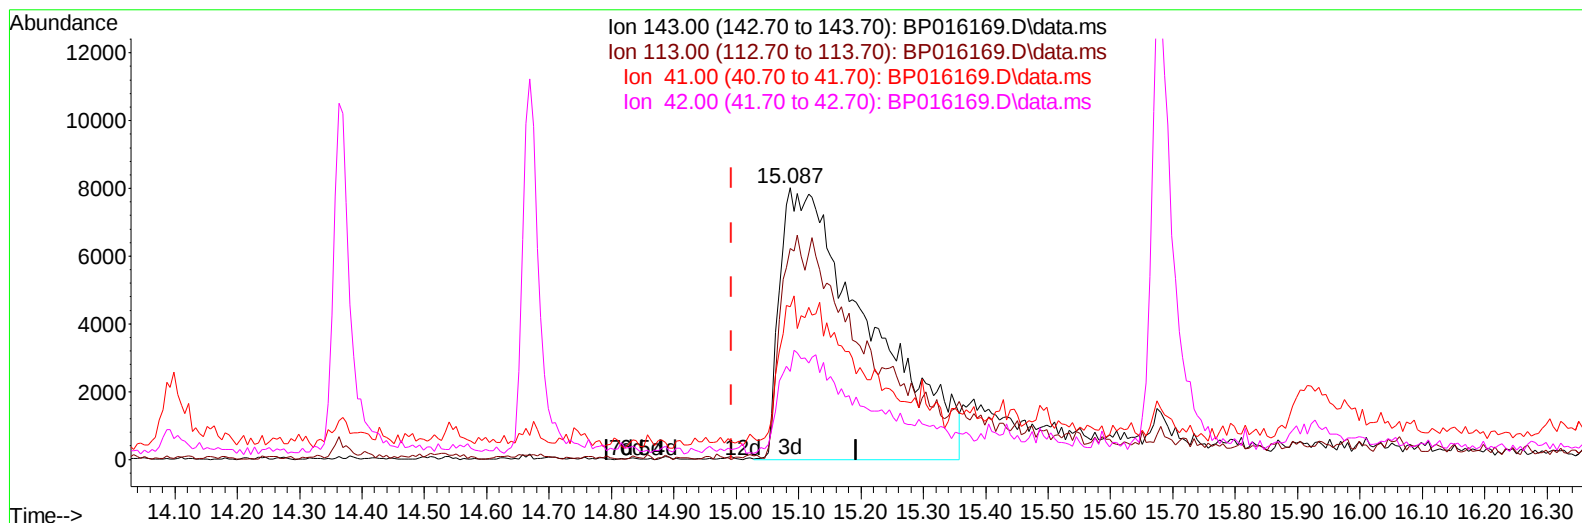

TIC: BP016169.D\data.ms

(54) 4-Nitrophenol-d4 (S)

15.087min (+ 0.094) 15.77 ng/ul m

response 78812

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	94.00	77.65
41.00	45.70	56.36#
42.00	31.20	32.51




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071023\
Data File : BP016169.D
Acq On : 10 Jul 2023 22:39
Operator : MA/JU
Sample : 03404-10
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
LabSampleId :
SSTDCCC020

Manual IntegrationsAPPROVED

Quant Time: Jul 11 00:34:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 10 23:19:51 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/11/2023
Supervised By :mohammad ahmed 07/11/2023

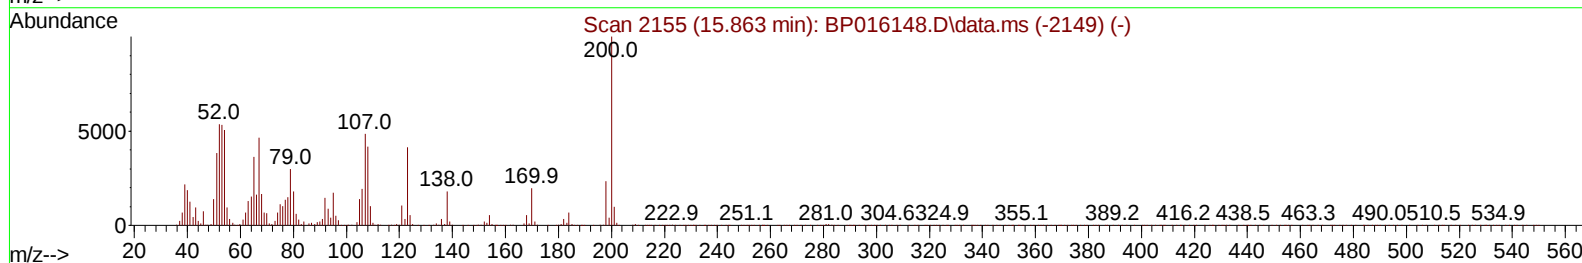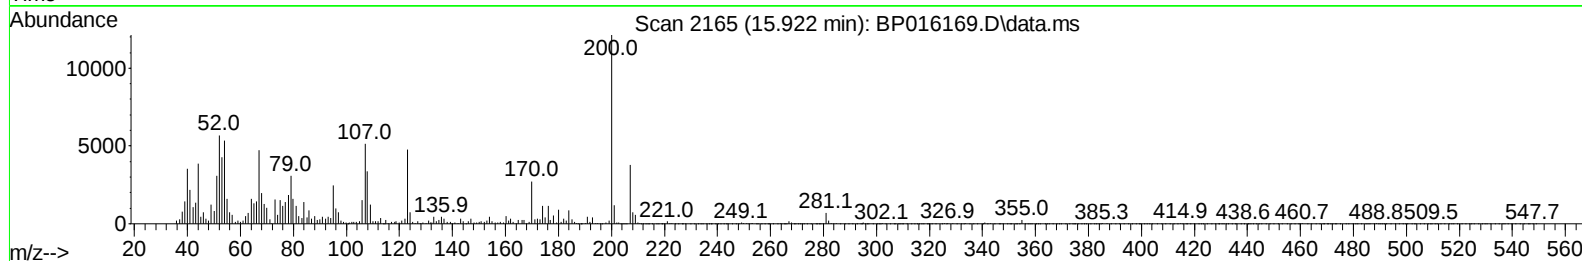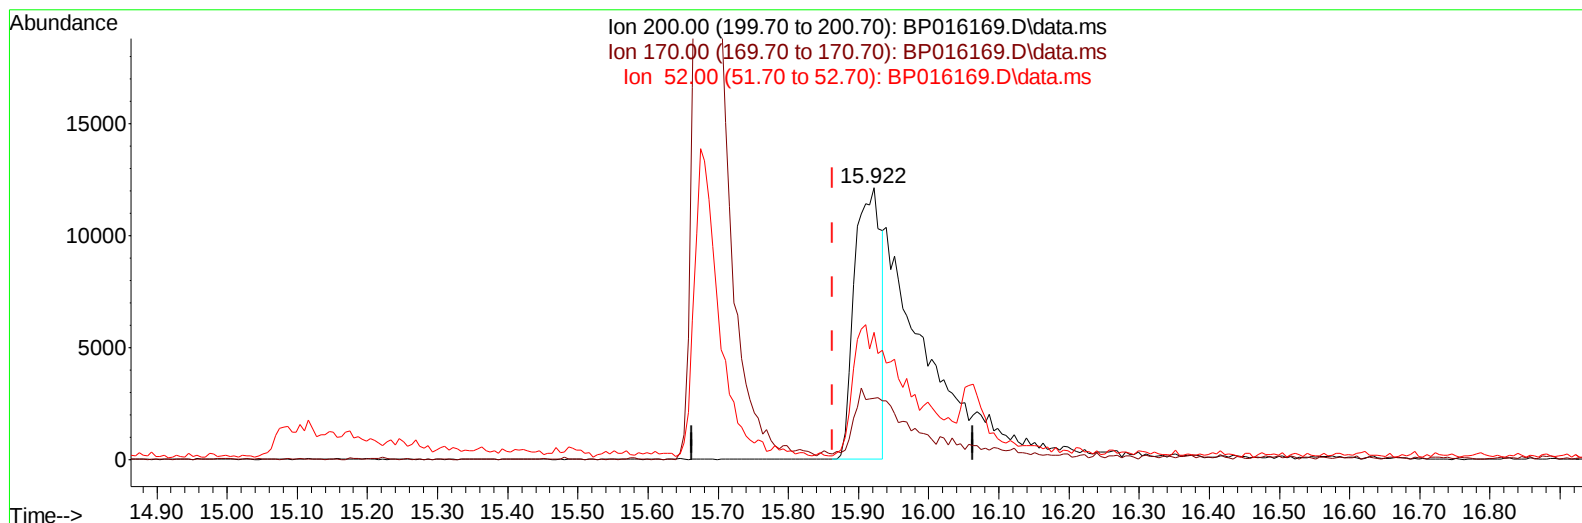

TIC: BP016169.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.922min (+ 0.059) 4.74 ng/u1

response 31724

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	24.30	22.42
52.00	52.20	46.90
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071023\
Data File : BP016169.D
Acq On : 10 Jul 2023 22:39
Operator : MA/JU
Sample : 03404-10
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
LabSampleId :
SSTDCCC020

Manual IntegrationsAPPROVED

Quant Time: Jul 11 00:34:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 10 23:19:51 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/11/2023
Supervised By :mohammad ahmed 07/11/2023

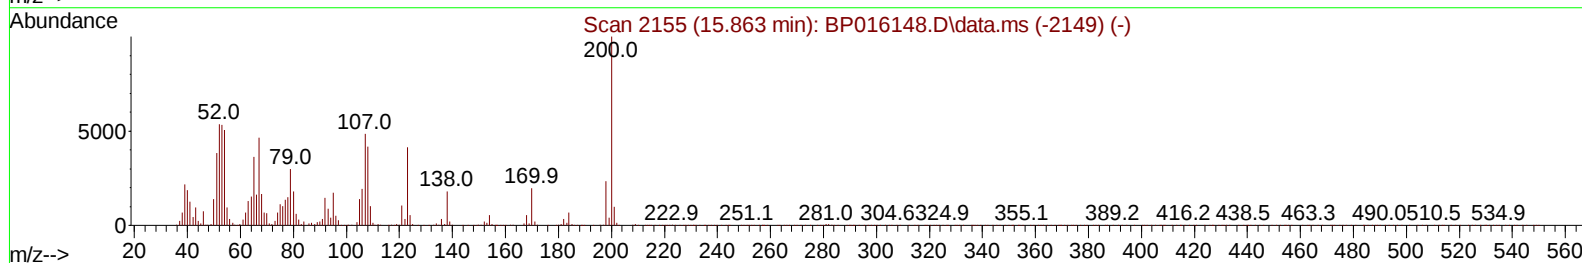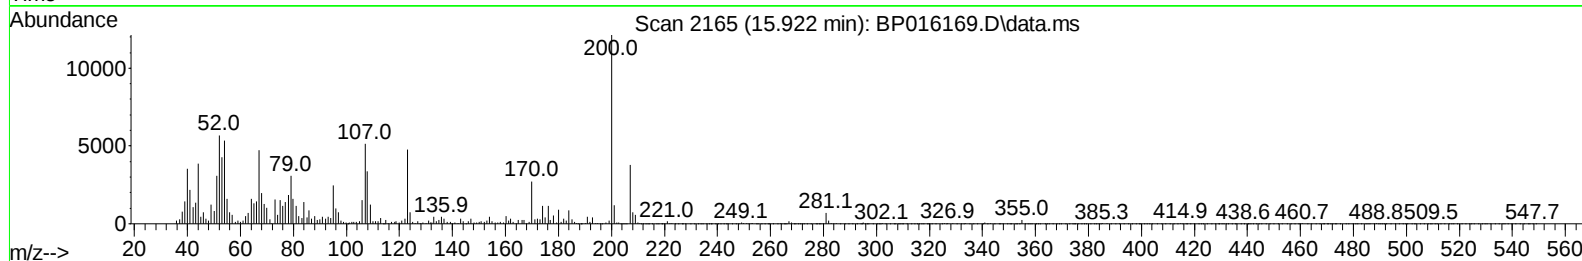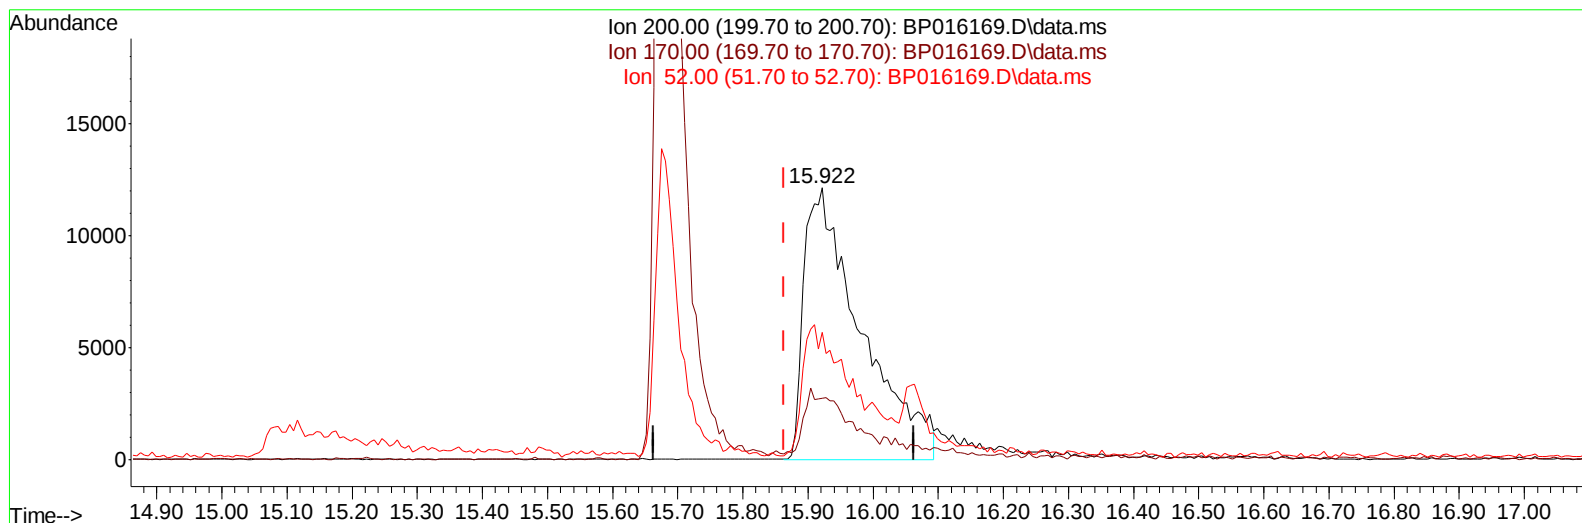

TIC: BP016169.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.922min (+ 0.059) 10.98 ng/ul m

response 73427

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	24.30	22.42
52.00	52.20	46.90
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071023\
 Data File : BG058137.D
 Acq On : 10 Jul 2023 11:24
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTDCCC020

Manual IntegrationsAPPROVED

Quant Time: Jul 11 00:44:07 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 10 16:52:40 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/11/2023
 Supervised By :mohammad ahmed 07/11/2023

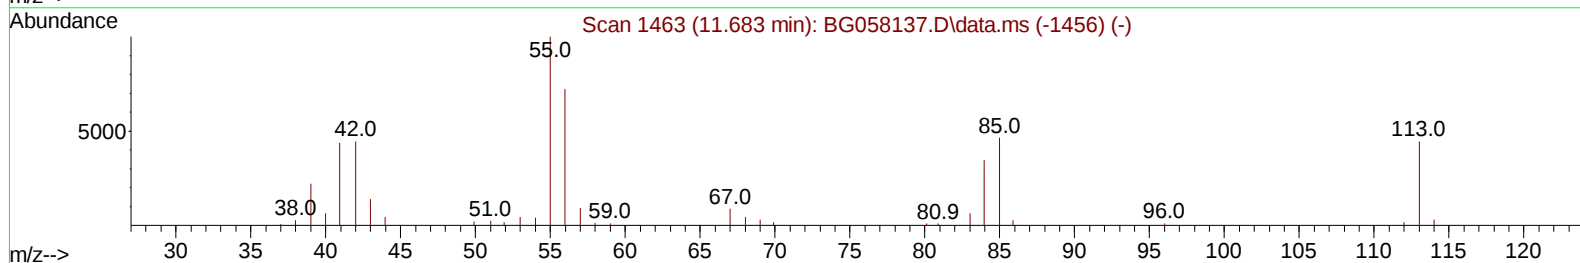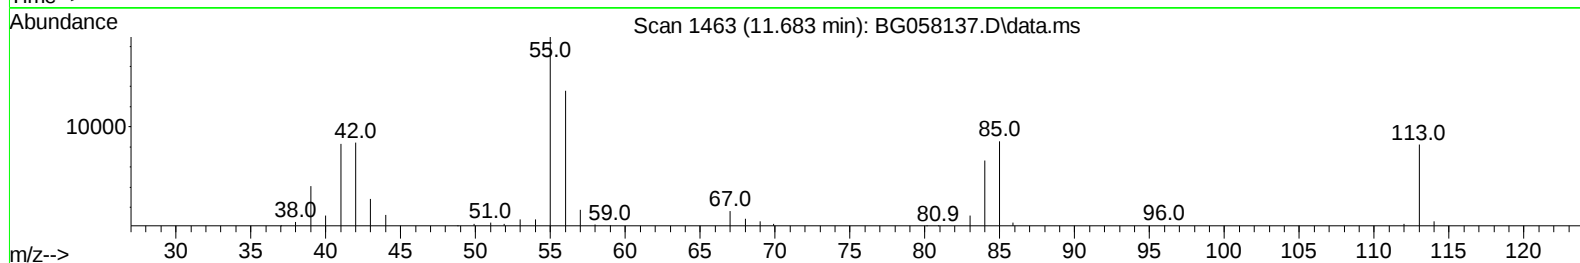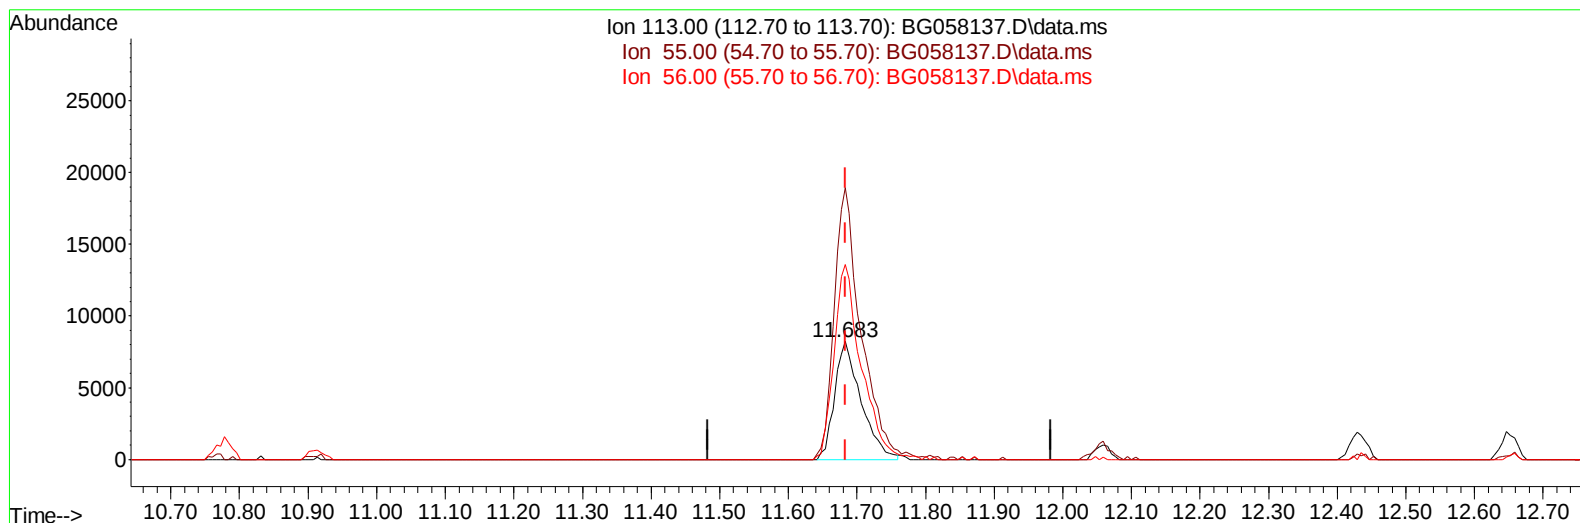

TIC: BG058137.D\data.ms

(34) Caprolactam

11.683min (0.000) 19.04 ng/ul

response 22026

Ion	Exp%	Act%
113.00	100.00	100.00
55.00	229.30	229.90
56.00	153.80	165.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071023\
 Data File : BG058137.D
 Acq On : 10 Jul 2023 11:24
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :

BNA_G




LabSampleId :

SSTDCCC020

Manual IntegrationsAPPROVED

Quant Time: Jul 11 00:44:07 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 10 16:52:40 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/11/2023
 Supervised By :mohammad ahmed 07/11/2023

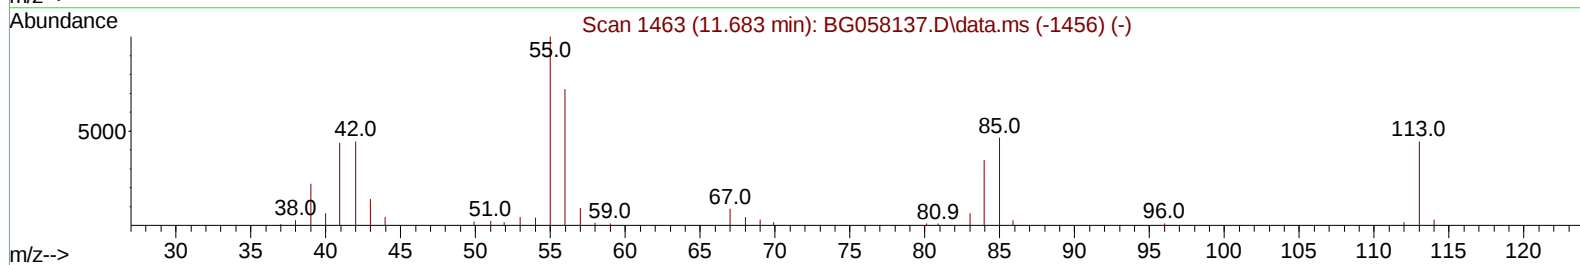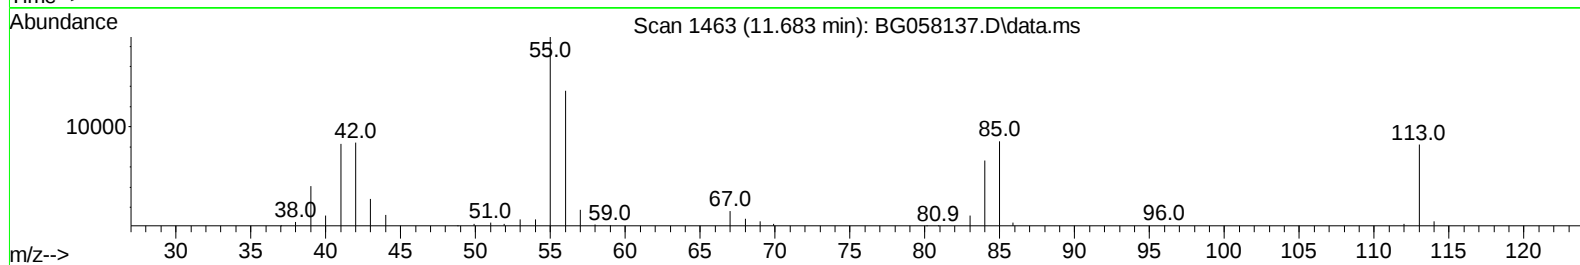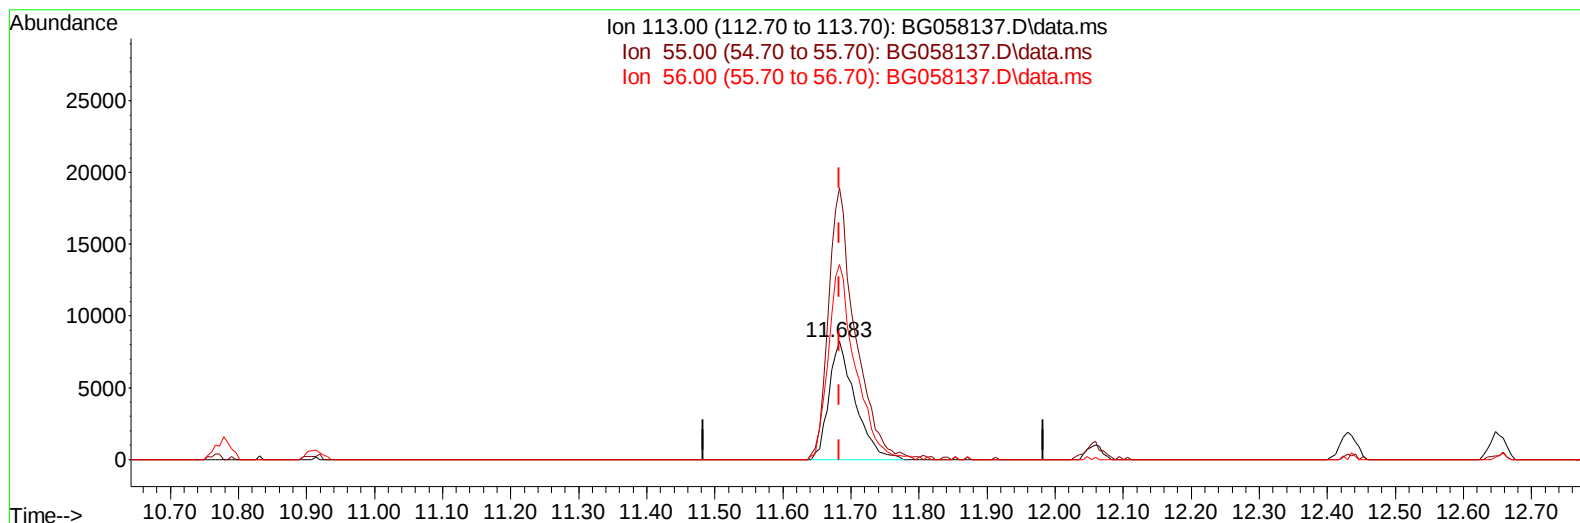

TIC: BG058137.D\data.ms

(34) Caprolactam

11.683min (0.000) 19.18 ng/ul m

response 22189

Ion	Exp%	Act%
113.00	100.00	100.00
55.00	229.30	229.90
56.00	153.80	165.32
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071023\
 Data File : BG058137.D
 Acq On : 10 Jul 2023 11:24
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTDCCC020

Manual IntegrationsAPPROVED

Quant Time: Jul 11 00:49:19 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 10 16:52:40 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/11/2023
 Supervised By :mohammad ahmed 07/11/2023

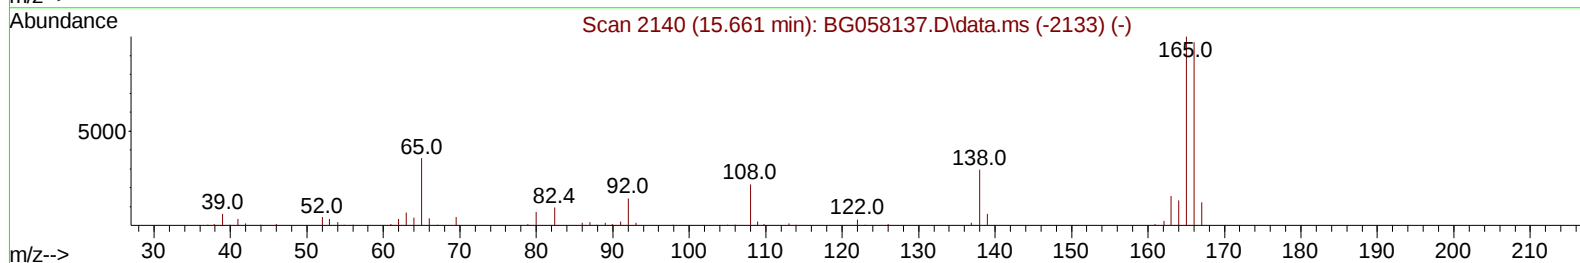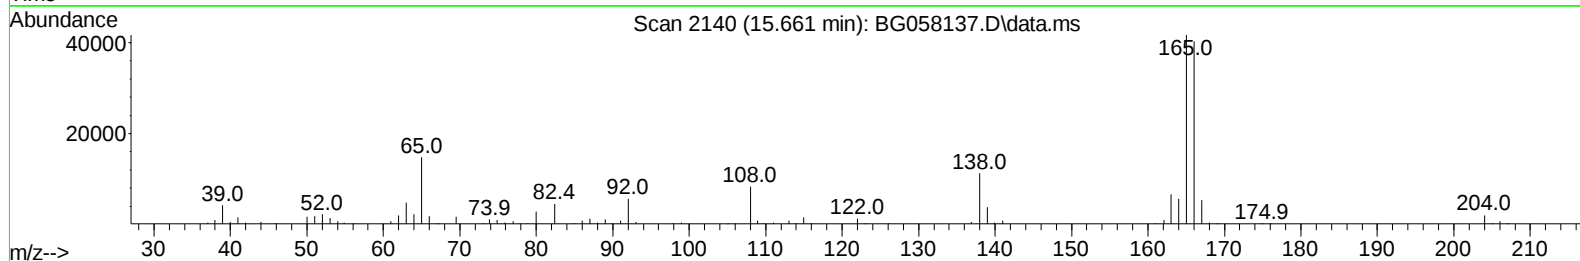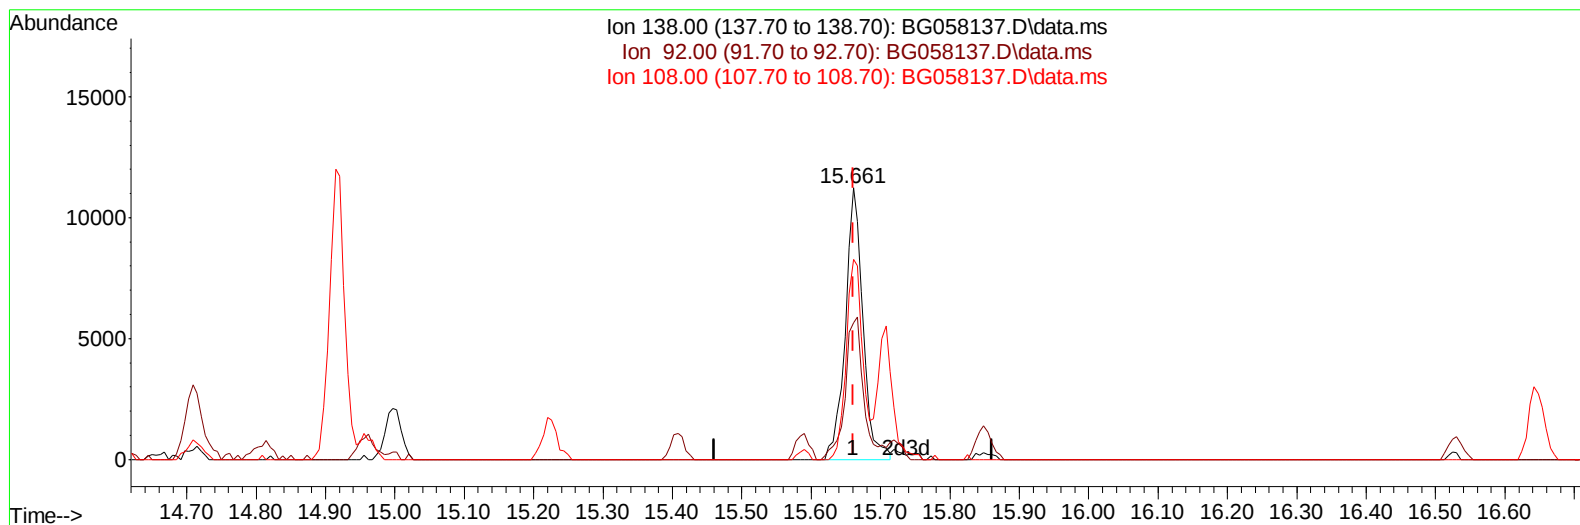

TIC: BG058137.D\data.ms

(63) 4-Nitroaniline

15.661min (0.000) 12.52 ng/ul

response 19839

Ion	Exp%	Act%
138.00	100.00	100.00
92.00	54.80	50.36
108.00	73.50	73.79
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071023\
 Data File : BG058137.D
 Acq On : 10 Jul 2023 11:24
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTDCCC020

Manual IntegrationsAPPROVED

Quant Time: Jul 11 00:49:19 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 10 16:52:40 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/11/2023
 Supervised By :mohammad ahmed 07/11/2023

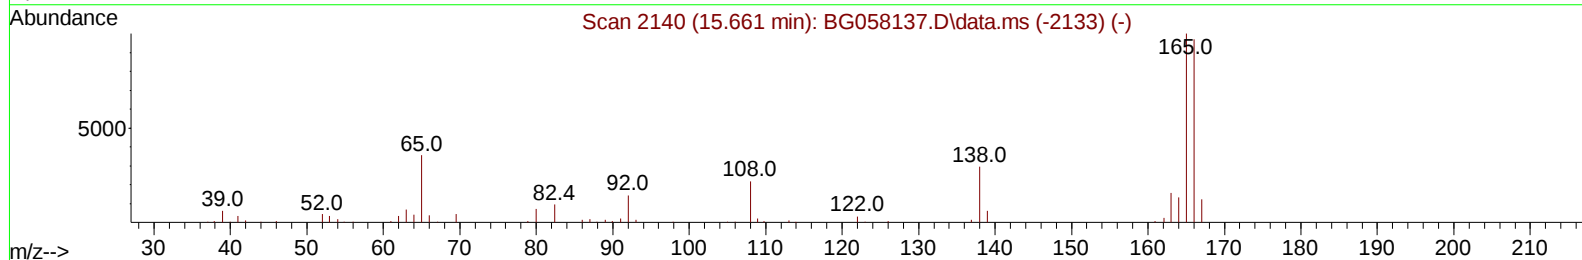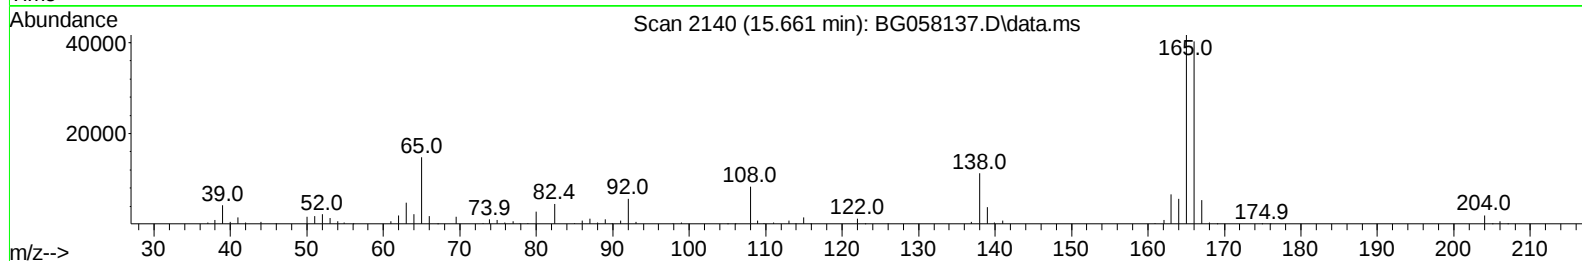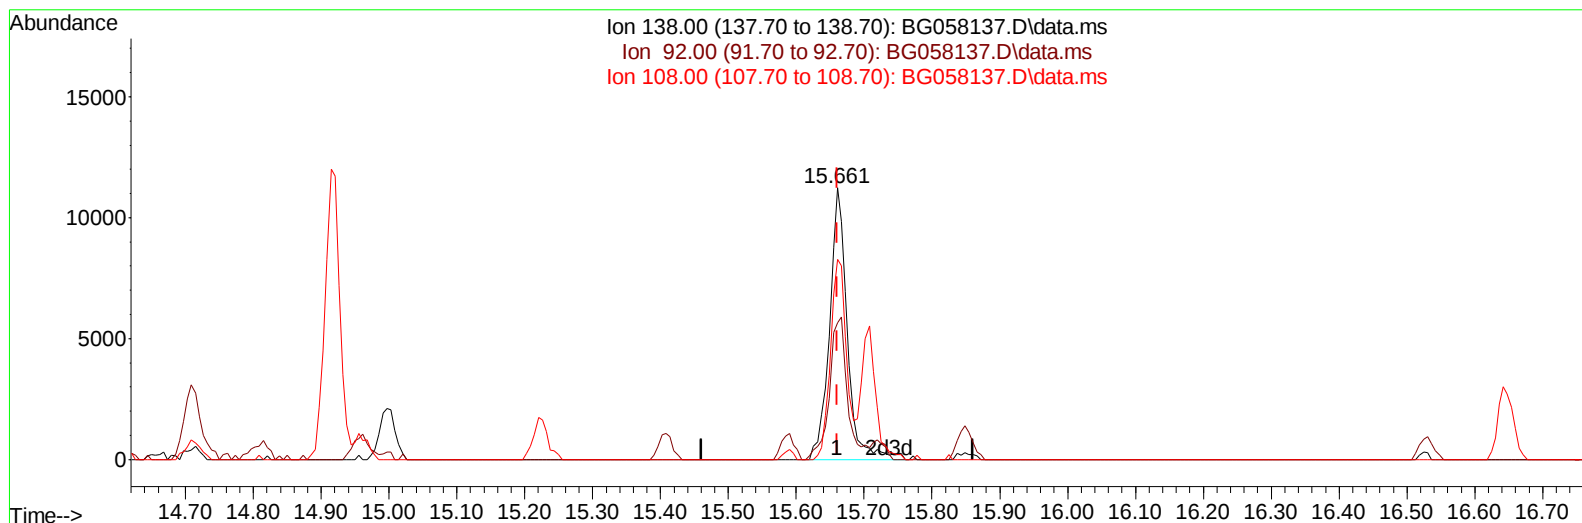

TIC: BG058137.D\data.ms

(63) 4-Nitroaniline

15.661min (0.000) 12.93 ng/ul m

response 20481

Ion	Exp%	Act%
138.00	100.00	100.00
92.00	54.80	50.36
108.00	73.50	73.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071023\
 Data File : BG058137.D
 Acq On : 10 Jul 2023 11:24
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTDCCC020

Manual IntegrationsAPPROVED

Quant Time: Jul 11 00:49:56 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 10 16:52:40 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/11/2023
 Supervised By :mohammad ahmed 07/11/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.970	152	39335	20.000	ng/ul	0.00
20) Naphthalene-d8	10.778	136	180105	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.603	164	128590	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.341	188	309674	20.000	ng/ul	0.00
79) Chrysene-d12	21.601	240	278774	20.000	ng/ul	0.00
88) Perylene-d12	24.785	264	333517	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.399	96	8718	7.761	ng/uL	0.00
4) Pyridine-d5	3.810	84	65376	19.170	ng/ul	0.00
7) Phenol-d5	7.130	99	77081	19.188	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.294	67	46782	19.325	ng/ul	0.00
11) 2-Chlorophenol-d4	7.506	132	52069	18.794	ng/ul	0.00
15) 4-Methylphenol-d8	8.675	113	58254	19.219	ng/ul	0.00
21) Nitrobenzene-d5	9.133	128	28475	19.398	ng/ul	0.00
24) 2-Nitrophenol-d4	9.856	143	31194	20.219	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.396	165	59738	20.185	ng/ul	0.00
31) 4-Chloroaniline-d4	10.913	131	88433	19.708	ng/ul	0.00
46) Dimethylphthalate-d6	14.004	166	195815	19.300	ng/ul	0.00
49) Acenaphthylene-d8	14.298	160	223448	20.182	ng/ul	0.00
54) 4-Nitrophenol-d4	14.797	143	31620	17.640	ng/ul	0.00
60) Fluorene-d10	15.590	176	173231	20.104	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.708	200	32826	19.521	ng/ul	0.00
73) Anthracene-d10	17.441	188	287248	19.990	ng/ul	0.00
81) Pyrene-d10	19.727	212	327449	18.650	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.568	264	330390	19.444	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.440	88	9933	7.158	ng/uL	97
5) Pyridine	3.833	79	68712	19.665	ng/ul	95
6) Benzaldehyde	7.112	77	22245	16.582	ng/ul	98
8) Phenol	7.159	94	78785	19.327	ng/ul	98
10) Bis(2-Chloroethyl)ether	7.388	93	60093	19.092	ng/ul	98
12) 2-Chlorophenol	7.535	128	55915	19.394	ng/ul	98
13) 2-Methylphenol	8.410	108	60952	19.039	ng/ul	96
14) 2,2'-oxybis(1-Chloropr...	8.499	45	94161	19.434	ng/ul	97
16) Acetophenone	8.792	105	100527	19.990	ng/ul	99
17) N-Nitroso-di-n-propyla...	8.769	70	53265	19.813	ng/ul#	95
18) 4-Methylphenol	8.739	108	68795	19.873	ng/ul	99
19) Hexachloroethane	9.057	117	21410	19.371	ng/ul	98
22) Nitrobenzene	9.174	77	73745	19.352	ng/ul	100
23) Isophorone	9.691	82	157809	19.407	ng/ul	99
25) 2-Nitrophenol	9.891	139	33093	19.990	ng/ul	97
26) 2,4-Dimethylphenol	9.944	107	73937	19.862	ng/ul	98
27) Bis(2-Chloroethoxy)met...	10.173	93	88909	19.404	ng/ul	98
29) 2,4-Dichlorophenol	10.426	162	58632	20.376	ng/ul	97
30) Naphthalene	10.825	128	198784	19.640	ng/ul	99
32) 4-Chloroaniline	10.937	127	92135	20.081	ng/ul	100
33) Hexachlorobutadiene	11.107	225	39834	19.553	ng/ul	96
34) Caprolactam	11.683	113	22189m	19.180	ng/ul	
35) 4-Chloro-3-methylphenol	12.053	107	72543	20.523	ng/ul	98

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071023\
 Data File : BG058137.D
 Acq On : 10 Jul 2023 11:24
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTDCCC020

Manual IntegrationsAPPROVED

Quant Time: Jul 11 00:49:56 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 10 16:52:40 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/11/2023
 Supervised By :mohammad ahmed 07/11/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
36) 2-Methylnaphthalene	12.429	142	135187	19.814	ng/ul	95
37) 1-Methylnaphthalene	12.652	142	136393	19.935	ng/ul	95
39) 1,2,4,5-Tetrachloroben...	12.799	216	77656	19.817	ng/ul	98
40) Hexachlorocyclopentadiene	12.776	237	56432	22.863	ng/ul	99
41) 2,4,6-Trichlorophenol	13.034	196	54161	20.392	ng/ul	99
42) 2,4,5-Trichlorophenol	13.111	196	57265	19.937	ng/ul	100
43) 1,1'-Biphenyl	13.434	154	185672	20.036	ng/ul	99
44) 2-Chloronaphthalene	13.481	162	146757	19.733	ng/ul	100
45) 2-Nitroaniline	13.681	65	51636	19.969	ng/ul	98
47) Dimethylphthalate	14.051	163	200579	19.677	ng/ul	99
48) 2,6-Dinitrotoluene	14.174	165	40702	19.453	ng/ul#	95
50) Acenaphthylene	14.327	152	239457	20.028	ng/ul	100
51) 3-Nitroaniline	14.503	138	29652	16.770	ng/ul#	91
52) Acenaphthene	14.662	153	165982	20.232	ng/ul	97
53) 2,4-Dinitrophenol	14.715	184	19824	18.174	ng/ul	94
55) 4-Nitrophenol	14.815	109	23771	17.901	ng/ul	92
56) Dibenzofuran	14.997	168	236607	20.288	ng/ul	98
57) 2,4-Dinitrotoluene	14.962	165	58889	19.865	ng/ul	99
58) 2,3,4,6-Tetrachlorophenol	15.226	232	51335	19.632	ng/ul#	99
59) Diethylphthalate	15.408	149	205525	19.318	ng/ul	99
61) Fluorene	15.649	166	194187	20.293	ng/ul	96
62) 4-Chlorophenyl-phenyle...	15.637	204	103719	20.485	ng/ul	99
63) 4-Nitroaniline	15.661	138	20481m	12.930	ng/ul	
66) 4,6-Dinitro-2-methylph...	15.719	198	33452	19.453	ng/ul	94
67) N-Nitrosodiphenylamine	15.849	169	164148	19.917	ng/ul	99
68) 4-Bromophenyl-phenylether	16.530	248	69152	20.343	ng/ul	99
69) Hexachlorobenzene	16.648	284	77973	20.488	ng/ul	98
70) Atrazine	16.795	200	64662	19.187	ng/ul	98
71) Pentachlorophenol	16.994	266	41043	17.963	ng/ul	94
72) Phenanthrene	17.382	178	316909	20.118	ng/ul	100
74) Anthracene	17.476	178	317181	19.898	ng/ul	100
75) 1,2,3,4-Tetrachloroben...	13.399	216	83641	20.366	ng/uL	95
76) Pentachlorobenzene	14.920	250	88823	20.250	ng/uL	97
77) Carbazole	17.747	167	287432	19.938	ng/ul	99
78) Di-n-butylphthalate	18.299	149	362298	19.728	ng/ul	99
80) Fluoranthene	19.392	202	377224	18.542	ng/ul	100
82) Pyrene	19.756	202	385738	18.836	ng/ul	99
83) Butylbenzylphthalate	20.637	149	158134	19.043	ng/ul	97
84) 3,3'-Dichlorobenzidine	21.495	252	128091	18.980	ng/ul	100
85) Benzo(a)anthracene	21.577	228	381093	19.039	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.477	149	231257	19.433	ng/ul	99
87) Chrysene	21.648	228	372861	19.871	ng/ul	99
89) Di-n-octyl phthalate	22.676	149	405428	19.785	ng/ul	100
90) Benzo(b)fluoranthene	23.769	252	391724	18.969	ng/ul	97
91) Benzo(k)fluoranthene	23.839	252	400612	19.792	ng/ul	99
93) Benzo(a)pyrene	24.638	252	355232	19.435	ng/ul	100
94) Indeno(1,2,3-cd)pyrene	28.422	276	472575	19.470	ng/ul	100
95) Dibenzo(a,h)anthracene	28.487	278	393036	19.638	ng/ul	98
96) Benzo(g,h,i)perylene	29.562	276	376818	19.008	ng/ul	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Instrument :

BNA_G

LabSampleId :

SSTDCCC020

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/11/2023

Supervised By :mohammad ahmed 07/11/2023

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071023\
 Data File : BG058137.D
 Acq On : 10 Jul 2023 11:24
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTDCCC020

Manual IntegrationsAPPROVED

Quant Time: Jul 11 00:49:56 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 10 16:52:40 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/11/2023
 Supervised By :mohammad ahmed 07/11/2023

