


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG071119\
 Data File : BG041623.D
 Acq On : 11 Jul 2019 17:35
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 12 05:39:06 2019

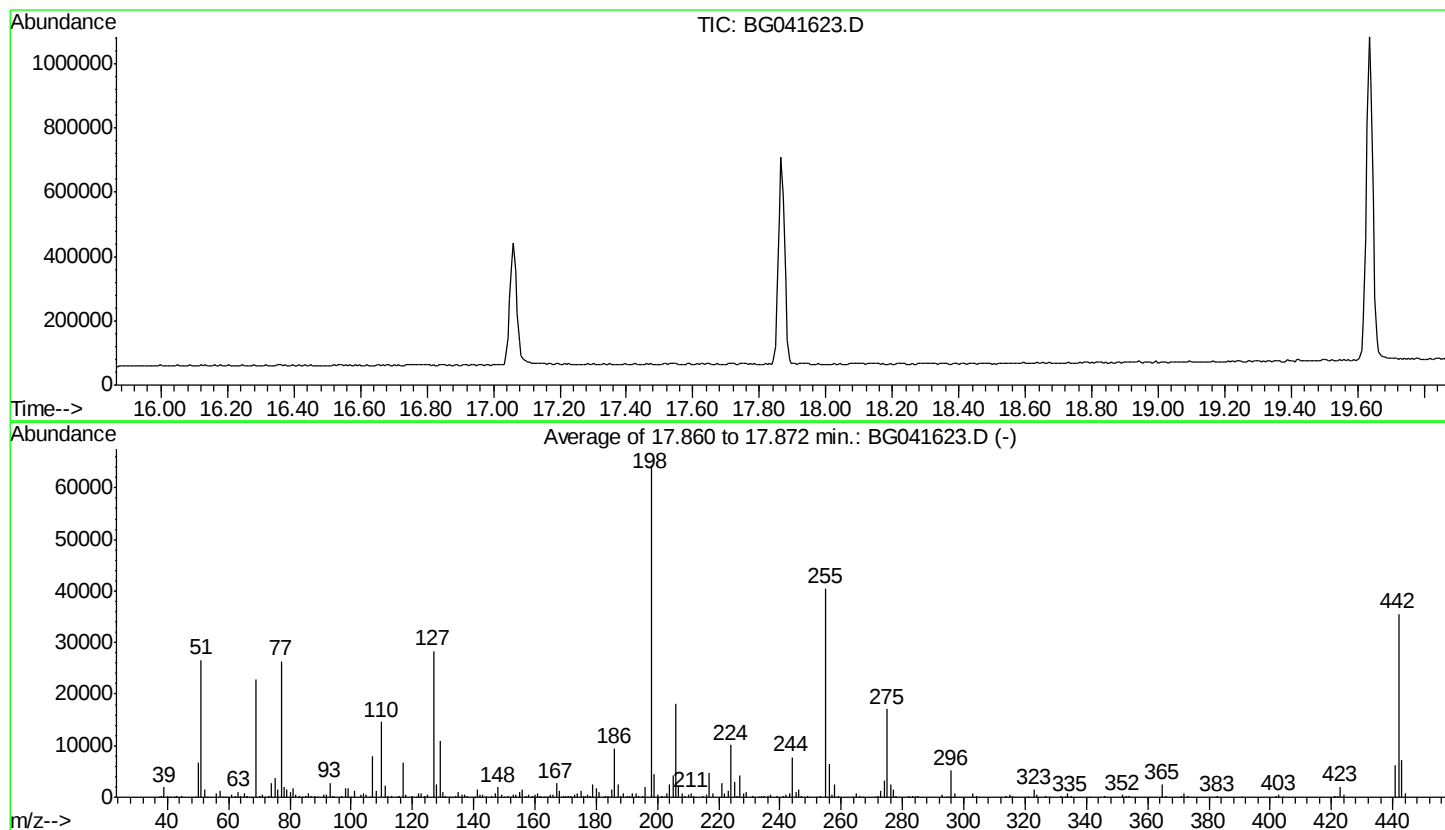

AutoFind: Scans 2514, 2515, 2516; Background Corrected with Scan 2507

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.4	26655	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.4	22783	PASS
70	69	0.00	2	1.3	301	PASS
127	198	10	80	44.1	28382	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	64312	PASS
199	198	5	9	6.8	4385	PASS
275	198	10	60	26.6	17128	PASS
365	198	1	100	3.8	2446	PASS
441	198	0.01	100	9.7	6224	PASS
442	198	50	100	55.2	35525	PASS
443	442	15	24	20.2	7168	PASS