

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071123\
 Data File : BG058193.D
 Acq On : 12 Jul 2023 19:23
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SSTD020512

Quant Time: Jul 12 22:08:19 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 10 16:52:40 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.970	152	52827	20.000	ng/u1	0.00
20) Naphthalene-d8	10.778	136	237053	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.598	164	160280	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.341	188	369202	20.000	ng/u1	0.00
79) Chrysene-d12	21.595	240	323832	20.000	ng/u1	0.00
88) Perylene-d12	24.786	264	389049	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.405	96	10499	6.959	ng/uL	0.00
4) Pyridine-d5	3.816	84	81412	17.775	ng/u1	0.00
7) Phenol-d5	7.130	99	102510	19.001	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.294	67	61572	18.938	ng/u1	0.00
11) 2-Chlorophenol-d4	7.506	132	70313	18.897	ng/u1	0.00
15) 4-Methylphenol-d8	8.675	113	76266	18.735	ng/u1	0.00
21) Nitrobenzene-d5	9.133	128	36558	18.922	ng/u1	0.00
24) 2-Nitrophenol-d4	9.856	143	40693	20.040	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.397	165	75412	19.359	ng/u1	0.00
31) 4-Chloroaniline-d4	10.914	131	107667	18.230	ng/u1	0.00
46) Dimethylphthalate-d6	13.998	166	225794	17.855	ng/u1	0.00
49) Acenaphthylene-d8	14.292	160	266909	19.341	ng/u1	0.00
54) 4-Nitrophenol-d4	14.797	143	35711	15.983	ng/u1	0.00
60) Fluorene-d10	15.591	176	202039	18.812	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.708	200	35110	17.513	ng/u1	0.00
73) Anthracene-d10	17.441	188	324105	18.918	ng/u1	0.00
81) Pyrene-d10	19.727	212	369730	18.128	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.568	264	378900	19.116	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.440	88	12090	6.487	ng/uL#	84
5) Pyridine	3.834	79	86767	18.490	ng/u1	95
6) Benzaldehyde	7.112	77	18218	10.112	ng/u1	96
8) Phenol	7.159	94	105205	19.217	ng/u1	99
10) Bis(2-Chloroethyl)ether	7.388	93	79983	18.921	ng/u1	98
12) 2-Chlorophenol	7.535	128	71902	18.570	ng/u1	97
13) 2-Methylphenol	8.411	108	80495	18.721	ng/u1	98
14) 2,2'-oxybis(1-Chloropr...	8.493	45	124400	19.118	ng/u1	97
16) Acetophenone	8.793	105	128516	19.028	ng/u1	98
17) N-Nitroso-di-n-propyla...	8.769	70	65659	18.185	ng/u1	98
18) 4-Methylphenol	8.740	108	88671	19.073	ng/u1	99
19) Hexachloroethane	9.051	117	28284	19.055	ng/u1	99
22) Nitrobenzene	9.175	77	96068	19.154	ng/u1	96
23) Isophorone	9.692	82	193441	18.074	ng/u1	100
25) 2-Nitrophenol	9.885	139	43938	20.165	ng/u1	95
26) 2,4-Dimethylphenol	9.944	107	94278	19.242	ng/u1	95
27) Bis(2-Chloroethoxy)met...	10.173	93	109684	18.187	ng/u1	98
29) 2,4-Dichlorophenol	10.420	162	75325	19.888	ng/u1	91
30) Naphthalene	10.826	128	256735	19.272	ng/u1	99
32) 4-Chloroaniline	10.937	127	111146	18.405	ng/u1	98
33) Hexachlorobutadiene	11.108	225	51094	19.055	ng/u1	95
34) Caprolactam	11.683	113	25126	16.501	ng/u1	92
35) 4-Chloro-3-methylphenol	12.053	107	89938	19.331	ng/u1	97
36) 2-Methylnaphthalene	12.430	142	170640	19.002	ng/u1	97


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071123\
 Data File : BG058193.D
 Acq On : 12 Jul 2023 19:23
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SSTD020512

Quant Time: Jul 12 22:08:19 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 10 16:52:40 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.647	142	170900	18.978	ng/ul	95
39) 1,2,4,5-Tetrachloroben...	12.794	216	101282	20.736	ng/ul	96
40) Hexachlorocyclopentadiene	12.776	237	34512	11.218	ng/ul	99
41) 2,4,6-Trichlorophenol	13.035	196	66562	20.106	ng/ul	99
42) 2,4,5-Trichlorophenol	13.111	196	68467	19.124	ng/ul	98
43) 1,1'-Biphenyl	13.434	154	228068	19.745	ng/ul	99
44) 2-Chloronaphthalene	13.481	162	182509	19.688	ng/ul	100
45) 2-Nitroaniline	13.681	65	61549	19.097	ng/ul	94
47) Dimethylphthalate	14.045	163	231398	18.213	ng/ul	99
48) 2,6-Dinitrotoluene	14.169	165	47979	18.397	ng/ul	94
50) Acenaphthylene	14.321	152	290002	19.460	ng/ul	98
51) 3-Nitroaniline	14.504	138	36661	16.634	ng/ul	95
52) Acenaphthene	14.662	153	197836	19.346	ng/ul	97
53) 2,4-Dinitrophenol	14.709	184	19677	14.472	ng/ul	89
55) 4-Nitrophenol	14.809	109	26913	16.260	ng/ul	91
56) Dibenzofuran	14.997	168	280538	19.299	ng/ul	99
57) 2,4-Dinitrotoluene	14.956	165	69596	18.835	ng/ul	100
58) 2,3,4,6-Tetrachlorophenol	15.220	232	59710	18.320	ng/ul	96
59) Diethylphthalate	15.408	149	231318	17.444	ng/ul	99
61) Fluorene	15.643	166	228866	19.189	ng/ul	100
62) 4-Chlorophenyl-phenyle...	15.632	204	120334	19.067	ng/ul	99
63) 4-Nitroaniline	15.661	138	20252	10.258	ng/ul	97
66) 4,6-Dinitro-2-methylph...	15.720	198	36822	17.960	ng/ul#	99
67) N-Nitrosodiphenylamine	15.849	169	189684	19.305	ng/ul	98
68) 4-Bromophenyl-phenylether	16.525	248	80342	19.824	ng/ul	99
69) Hexachlorobenzene	16.648	284	88845	19.581	ng/ul	99
70) Atrazine	16.789	200	73437	18.277	ng/ul	98
71) Pentachlorophenol	16.989	266	40496	14.866	ng/ul	93
72) Phenanthrene	17.383	178	357667	19.045	ng/ul	99
74) Anthracene	17.477	178	361969	19.046	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.399	216	104368	21.315	ng/uL	98
76) Pentachlorobenzene	14.915	250	108509	20.750	ng/uL	96
77) Carbazole	17.741	167	327266	19.041	ng/ul	100
78) Di-n-butylphthalate	18.293	149	401860	18.354	ng/ul	99
80) Fluoranthene	19.392	202	426845	18.062	ng/ul	99
82) Pyrene	19.756	202	433138	18.208	ng/ul	99
83) Butylbenzylphthalate	20.632	149	179555	18.614	ng/ul	99
84) 3,3'-Dichlorobenzidine	21.495	252	159036	20.286	ng/ul	96
85) Benzo(a)anthracene	21.578	228	439122	18.886	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.472	149	259270	18.756	ng/ul	99
87) Chrysene	21.642	228	407062	18.675	ng/ul	99
89) Di-n-octyl phthalate	22.670	149	455984	19.076	ng/ul	100
90) Benzo(b)fluoranthene	23.769	252	455573	18.912	ng/ul	98
91) Benzo(k)fluoranthene	23.834	252	447261	18.943	ng/ul	99
93) Benzo(a)pyrene	24.639	252	400549	18.786	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	28.423	276	478549	16.902	ng/ul	99
95) Dibenzo(a,h)anthracene	28.481	278	181403	7.770	ng/ul	98
96) Benzo(g,h,i)perylene	29.562	276	336446	14.549	ng/ul	98





(#) = qualifier out of range (m) = manual integration (+) = signals summed



#2
1,4-Dioxane
Concen: 6.487 ng/uL
RT: 3.440 min Scan# 60
Delta R.T. 0.000 min
Lab File: BG058193.D
Acq: 12 Jul 2023 19:23




Instrument :
BNA_G
ClientSampleId :
SSTD020512


Tgt Ion: 88 Resp: 12090
Ion Ratio Lower Upper
88 100
43 34.3 20.6 30.8#
58 95.5 65.5 98.3



#5
Pyridine
Concen: 18.490 ng/uL
RT: 3.834 min Scan# 127
Delta R.T. 0.000 min
Lab File: BG058193.D
Acq: 12 Jul 2023 19:23

Tgt Ion: 79 Resp: 86767
Ion Ratio Lower Upper
79 100
52 88.3 68.6 102.8
51 43.0 29.4 44.0




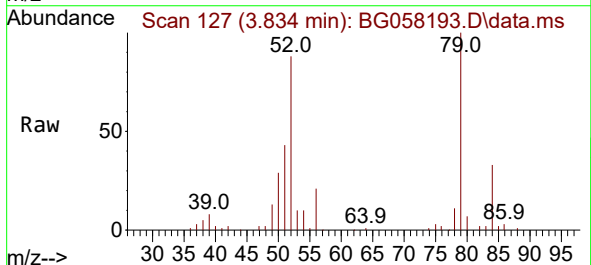




#6
Benzaldehyde
Concen: 10.112 ng/ul
RT: 7.112 min Scan# 685
Delta R.T. 0.000 min
Lab File: BG058193.D
Acq: 12 Jul 2023 19:23




Instrument :
BNA_G
ClientSampleId :
SSTD020512


Tgt Ion: 77 Resp: 18218
Ion Ratio Lower Upper
77 100
105 100.3 74.7 112.1
106 93.9 75.9 113.9

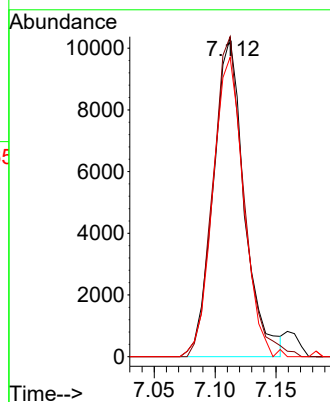

#8
Phenol
Concen: 19.217 ng/ul
RT: 7.159 min Scan# 693
Delta R.T. 0.000 min
Lab File: BG058193.D
Acq: 12 Jul 2023 19:23

Tgt Ion: 94 Resp: 105205
Ion Ratio Lower Upper
94 100
65 28.9 22.2 33.4
66 35.5 28.6 43.0




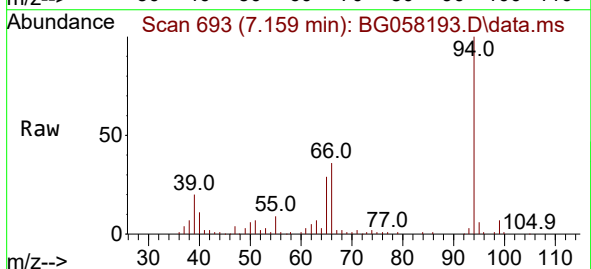




#10
Bis(2-Chloroethyl)ether
Concen: 18.921 ng/ul
RT: 7.388 min Scan# 732
Delta R.T. 0.000 min
Lab File: BG058193.D
Acq: 12 Jul 2023 19:23




Instrument :
BNA_G
ClientSampleId :
SSTD020512


Tgt Ion: 93	Resp: 79983
Ion Ratio	Lower Upper
93	100
63	87.1 69.4 104.0
95	30.4 27.0 40.6



#12
2-Chlorophenol
Concen: 18.570 ng/ul
RT: 7.535 min Scan# 757
Delta R.T. 0.000 min
Lab File: BG058193.D
Acq: 12 Jul 2023 19:23

Tgt Ion: 128	Resp: 71902
Ion Ratio	Lower Upper
128	100
64	58.0 44.3 66.5
130	32.5 27.3 40.9



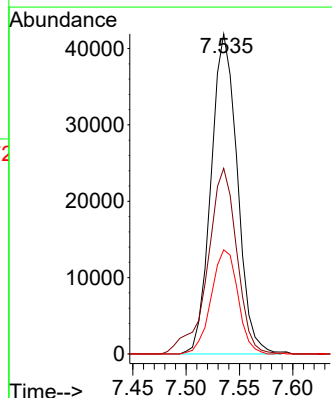





#13
2-Methylphenol
Concen: 18.721 ng/ul
RT: 8.411 min Scan# 90
Delta R.T. 0.000 min
Lab File: BG058193.D
Acq: 12 Jul 2023 19:23




Instrument :
BNA_G
ClientSampleId :
SSTD020512


Tgt Ion:108 Resp: 80495
Ion Ratio Lower Upper
108 100
107 91.3 75.0 112.4

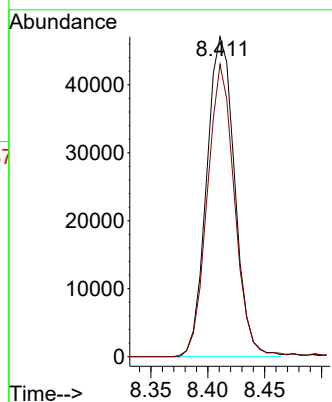

#14
2,2'-oxybis(1-Chloropropane)
Concen: 19.118 ng/ul
RT: 8.493 min Scan# 920
Delta R.T. -0.006 min
Lab File: BG058193.D
Acq: 12 Jul 2023 19:23

Tgt Ion: 45 Resp: 124400
Ion Ratio Lower Upper
45 100
77 13.1 9.4 14.2
79 9.6 8.3 12.5









#16
Acetophenone
Concen: 19.028 ng/ul
RT: 8.793 min Scan# 971
Delta R.T. 0.000 min
Lab File: BG058193.D
Acq: 12 Jul 2023 19:23




Instrument :
BNA_G
ClientSampleId :
SSTD020512


Tgt Ion:105 Resp: 128516
Ion Ratio Lower Upper
105 100
77 74.0 61.2 91.8
51 29.8 23.5 35.3

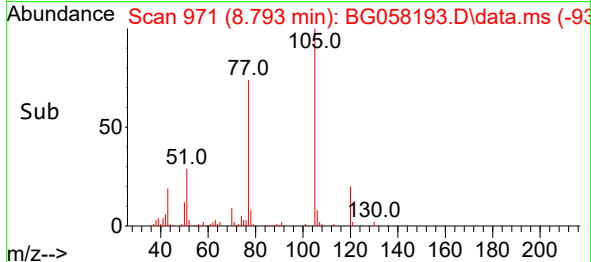

#17
N-Nitroso-di-n-propylamine
Concen: 18.185 ng/ul
RT: 8.769 min Scan# 967
Delta R.T. 0.000 min
Lab File: BG058193.D
Acq: 12 Jul 2023 19:23

Tgt Ion: 70 Resp: 65659
Ion Ratio Lower Upper
70 100
42 58.8 48.0 72.0
101 8.0 7.4 11.2
130 16.9 13.4 20.0


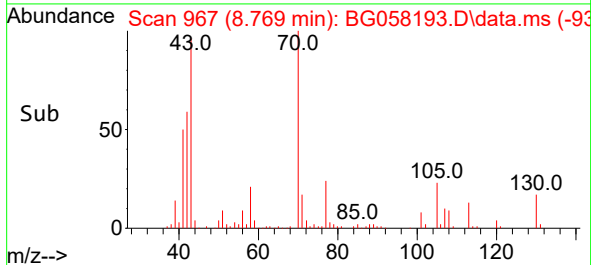






#18
4-Methylphenol
Concen: 19.073 ng/ul
RT: 8.740 min Scan# 90
Delta R.T. 0.000 min
Lab File: BG058193.D
Acq: 12 Jul 2023 19:23




Instrument :
BNA_G
ClientSampleId :
SSTD020512


Tgt Ion:108 Resp: 88671
Ion Ratio Lower Upper
108 100
107 112.9 91.1 136.7

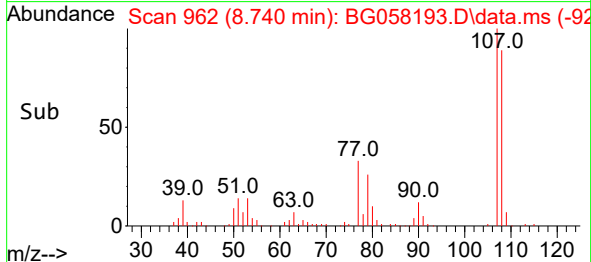

#19
Hexachloroethane
Concen: 19.055 ng/ul
RT: 9.051 min Scan# 1015
Delta R.T. -0.006 min
Lab File: BG058193.D
Acq: 12 Jul 2023 19:23

Tgt Ion:117 Resp: 28284
Ion Ratio Lower Upper
117 100
201 115.6 94.0 141.0
199 75.0 59.8 89.6

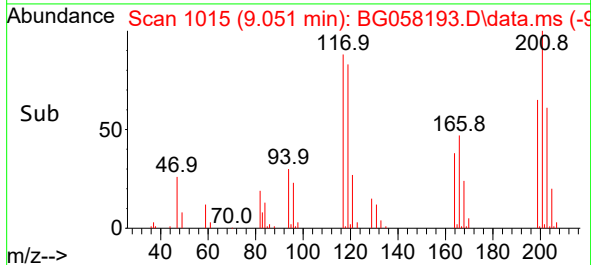



#22

Nitrobenzene

Concen: 19.154 ng/ul

RT: 9.175 min Scan# 11036

Delta R.T. 0.000 min

Lab File: BG058193.D

Acq: 12 Jul 2023 19:23

Instrument :

BNA_G

ClientSampleId :

SSTD020512





Tgt Ion: 77 Resp: 96068

Ion Ratio Lower Upper

77 100

123 43.8 33.3 49.9

65 14.6 10.4 15.6



#23

Isophorone

Concen: 18.074 ng/ul

RT: 9.692 min Scan# 1124

Delta R.T. 0.000 min

Lab File: BG058193.D

Acq: 12 Jul 2023 19:23




Tgt Ion: 82 Resp: 193441


Ion Ratio Lower Upper

82 100

95 6.0 4.8 7.2

138 14.2 11.4 17.0




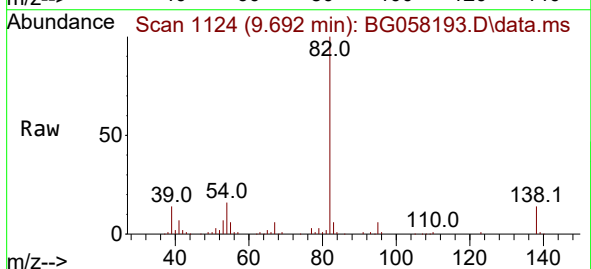




#25
2-Nitrophenol
Concen: 20.165 ng/ul
RT: 9.885 min Scan# 1157
Delta R.T. -0.006 min
Lab File: BG058193.D
Acq: 12 Jul 2023 19:23




Instrument :
BNA_G
ClientSampleId :
SSTD020512


Tgt Ion:139 Resp: 43938
Ion Ratio Lower Upper
139 100
65 56.8 42.6 64.0
109 27.9 20.7 31.1



#26
2,4-Dimethylphenol
Concen: 19.242 ng/ul
RT: 9.944 min Scan# 1167
Delta R.T. 0.000 min
Lab File: BG058193.D
Acq: 12 Jul 2023 19:23

Tgt Ion:107 Resp: 94278
Ion Ratio Lower Upper
107 100
121 46.4 40.6 60.8
122 80.2 67.1 100.7









#27
 Bis(2-Chloroethoxy)methane
 Concen: 18.187 ng/ul
 RT: 10.173 min Scan# 1206
 Delta R.T. 0.000 min
 Lab File: BG058193.D
 Acq: 12 Jul 2023 19:23




Instrument :
 BNA_G
 ClientSampleId :
 SSTD020512


Tgt Ion: 93 Resp: 109684
 Ion Ratio Lower Upper
 93 100
 95 31.9 26.4 39.6
 123 10.9 7.9 11.9



#29
 2,4-Dichlorophenol
 Concen: 19.888 ng/ul
 RT: 10.420 min Scan# 1248
 Delta R.T. -0.006 min
 Lab File: BG058193.D
 Acq: 12 Jul 2023 19:23

Tgt Ion: 162 Resp: 75325
 Ion Ratio Lower Upper
 162 100
 164 72.2 51.1 76.7
 98 38.4 27.9 41.9









#30
Naphthalene
Concen: 19.272 ng/ul
RT: 10.826 min Scan# 11
Delta R.T. 0.000 min
Lab File: BG058193.D
Acq: 12 Jul 2023 19:23




Instrument :
BNA_G
ClientSampleId :
SSTD020512


Tgt Ion:128 Resp: 256735
Ion Ratio Lower Upper
128 100
129 10.9 8.6 12.8
127 13.2 10.2 15.2

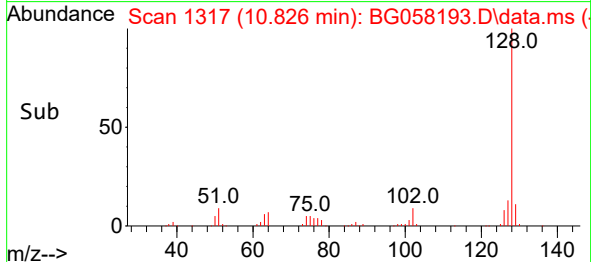

#32
4-Chloroaniline
Concen: 18.405 ng/ul
RT: 10.937 min Scan# 1336
Delta R.T. 0.000 min
Lab File: BG058193.D
Acq: 12 Jul 2023 19:23

Tgt Ion:127 Resp: 111146
Ion Ratio Lower Upper
127 100
129 31.2 26.0 39.0




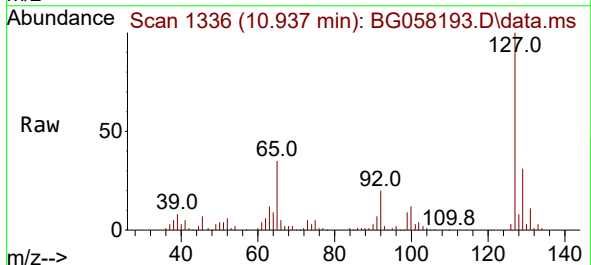




#33
Hexachlorobutadiene
Concen: 19.055 ng/ul
RT: 11.108 min Scan# 11
Delta R.T. 0.000 min
Lab File: BG058193.D
Acq: 12 Jul 2023 19:23




Instrument :
BNA_G
ClientSampleId :
SSTD020512


Tgt Ion:225 Resp: 51094
Ion Ratio Lower Upper
225 100
223 60.0 53.2 79.8
227 63.6 51.4 77.2

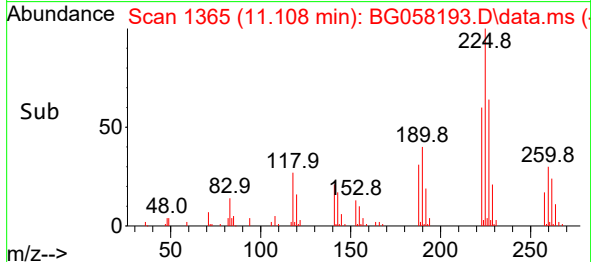

#34
Caprolactam
Concen: 16.501 ng/ul
RT: 11.683 min Scan# 1463
Delta R.T. 0.000 min
Lab File: BG058193.D
Acq: 12 Jul 2023 19:23

Tgt Ion:113 Resp: 25126
Ion Ratio Lower Upper
113 100
55 218.6 183.4 275.2
56 166.9 123.0 184.6




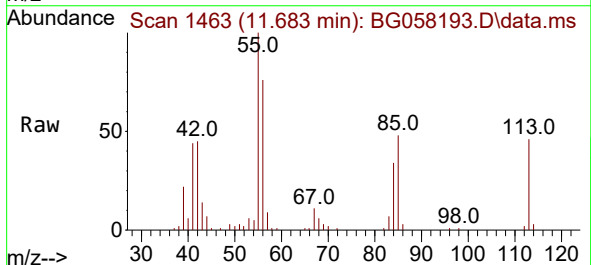




#35
 4-Chloro-3-methylphenol
 Concen: 19.331 ng/ul
 RT: 12.053 min Scan# 1526
 Delta R.T. 0.000 min
 Lab File: BG058193.D
 Acq: 12 Jul 2023 19:23




Instrument :
 BNA_G
 ClientSampleId :
 SSTD020512


Tgt Ion:	107	Resp:	89938
Ion	Ratio	Lower	Upper
107	100		
144	23.9	19.0	28.4
142	75.7	58.4	87.6

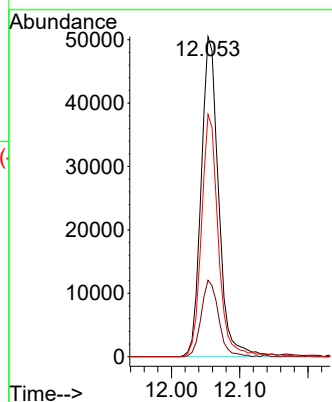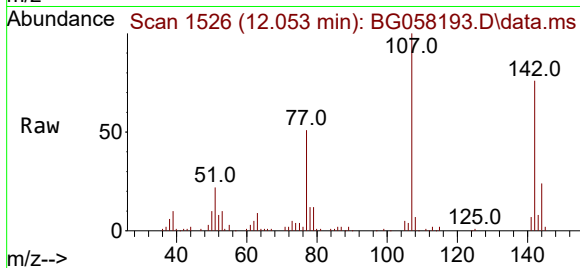

#36
 2-Methylnaphthalene
 Concen: 19.002 ng/ul
 RT: 12.430 min Scan# 1590
 Delta R.T. 0.000 min
 Lab File: BG058193.D
 Acq: 12 Jul 2023 19:23

Tgt Ion:	142	Resp:	170640
Ion	Ratio	Lower	Upper
142	100		
141	89.5	69.4	104.2



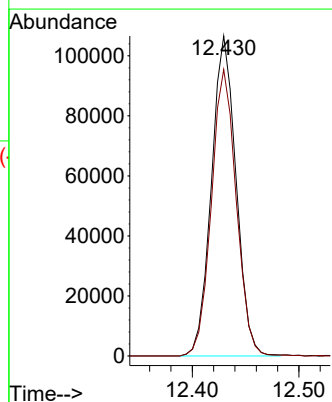
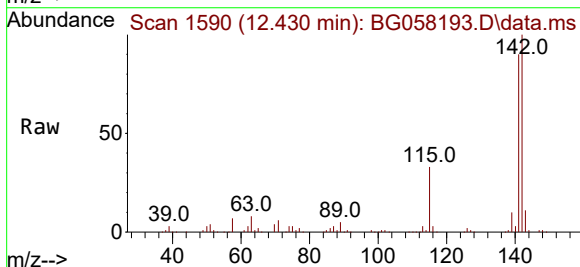


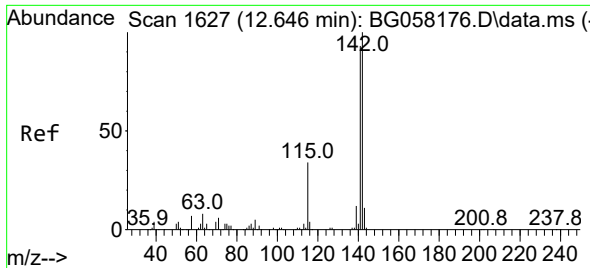

#37
1-Methylnaphthalene
Concen: 18.978 ng/ul
RT: 12.647 min Scan# 1
Delta R.T. -0.006 min
Lab File: BG058193.D
Acq: 12 Jul 2023 19:23




Instrument :
BNA_G
ClientSampleId :
SSTD020512


Tgt Ion:142 Resp: 170900
Ion Ratio Lower Upper
142 100
141 97.3 73.8 110.8
116 4.2 3.0 4.4

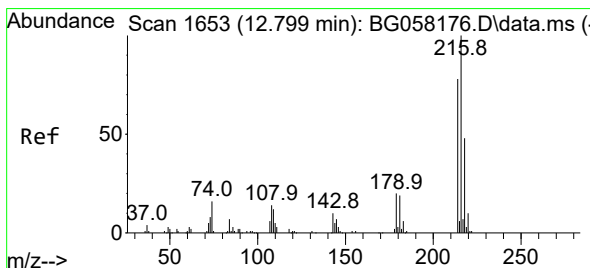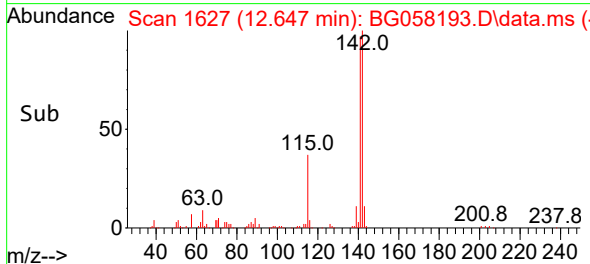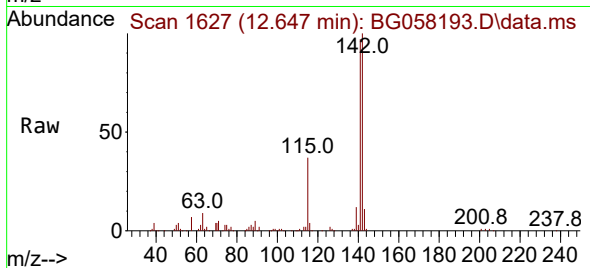

#39
1,2,4,5-Tetrachlorobenzene
Concen: 20.736 ng/ul
RT: 12.794 min Scan# 1652
Delta R.T. -0.006 min
Lab File: BG058193.D
Acq: 12 Jul 2023 19:23

Tgt Ion:216 Resp: 101282
Ion Ratio Lower Upper
216 100
214 75.8 64.1 96.1
179 19.7 16.0 24.0
108 15.6 12.1 18.1


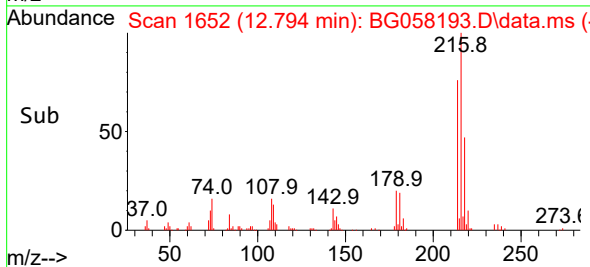

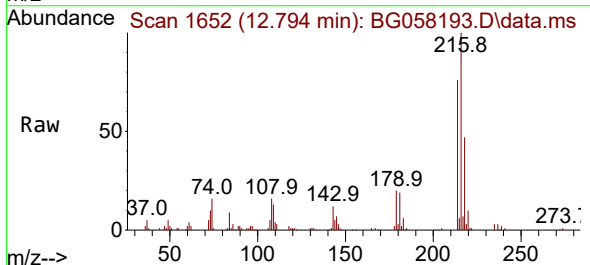




#40
Hexachlorocyclopentadiene
Concen: 11.218 ng/ul
RT: 12.776 min Scan# 1648
Delta R.T. 0.000 min
Lab File: BG058193.D
Acq: 12 Jul 2023 19:23




Instrument :
BNA_G
ClientSampleId :
SSTD020512


Tgt Ion:237 Resp: 34512
Ion Ratio Lower Upper
237 100
235 60.5 49.2 73.8
272 12.1 10.4 15.6

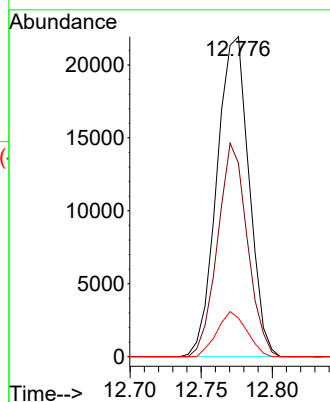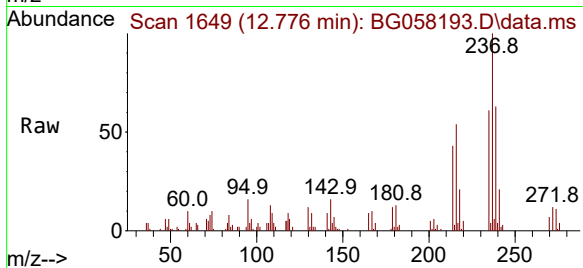

#41
2,4,6-Trichlorophenol
Concen: 20.106 ng/ul
RT: 13.035 min Scan# 1693
Delta R.T. 0.000 min
Lab File: BG058193.D
Acq: 12 Jul 2023 19:23

Tgt Ion:196 Resp: 66562
Ion Ratio Lower Upper
196 100
198 93.1 73.5 110.3
200 31.7 24.8 37.2



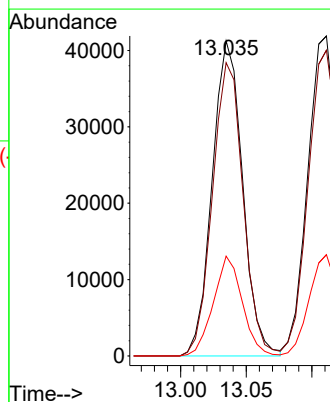
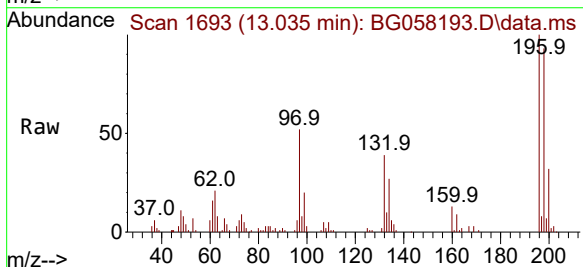




#42
2,4,5-Trichlorophenol
Concen: 19.124 ng/ul
RT: 13.111 min Scan# 1706
Delta R.T. 0.000 min
Lab File: BG058193.D
Acq: 12 Jul 2023 19:23




Instrument :
BNA_G
ClientSampleId :
SSTD020512


Tgt Ion:196 Resp: 68467
Ion Ratio Lower Upper
196 100
198 95.6 77.2 115.8
200 31.6 23.8 35.6



#43
1,1'-Biphenyl
Concen: 19.745 ng/ul
RT: 13.434 min Scan# 1761
Delta R.T. 0.000 min
Lab File: BG058193.D
Acq: 12 Jul 2023 19:23

Tgt Ion:154 Resp: 228068
Ion Ratio Lower Upper
154 100
153 40.0 32.6 49.0
76 14.9 11.6 17.4


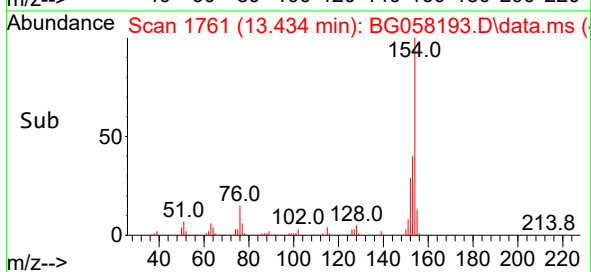






#44
2-Chloronaphthalene
Concen: 19.688 ng/ul
RT: 13.481 min Scan# 1769
Delta R.T. 0.000 min
Lab File: BG058193.D
Acq: 12 Jul 2023 19:23




Instrument :
BNA_G
ClientSampleId :
SSTD020512


Tgt Ion:162 Resp: 182509
Ion Ratio Lower Upper
162 100
164 34.6 27.7 41.5
127 38.6 30.9 46.3



#45
2-Nitroaniline
Concen: 19.097 ng/ul
RT: 13.681 min Scan# 1803
Delta R.T. 0.000 min
Lab File: BG058193.D
Acq: 12 Jul 2023 19:23

Tgt Ion: 65 Resp: 61549
Ion Ratio Lower Upper
65 100
92 68.9 53.2 79.8
138 95.8 71.1 106.7









#47
Dimethylphthalate
Concen: 18.213 ng/ul
RT: 14.045 min Scan# 1865
Delta R.T. -0.006 min
Lab File: BG058193.D
Acq: 12 Jul 2023 19:23




Instrument :
BNA_G
ClientSampleId :
SSTD020512


Tgt Ion:163 Resp: 231398
Ion Ratio Lower Upper
163 100
194 3.8 3.0 4.4
164 10.1 8.6 12.8



#48
2,6-Dinitrotoluene
Concen: 18.397 ng/ul
RT: 14.169 min Scan# 1886
Delta R.T. -0.006 min
Lab File: BG058193.D
Acq: 12 Jul 2023 19:23

Tgt Ion:165 Resp: 47979
Ion Ratio Lower Upper
165 100
89 57.4 42.7 64.1
121 21.9 14.8 22.2









#50
Acenaphthylene
Concen: 19.460 ng/ul
RT: 14.321 min Scan# 1912
Delta R.T. -0.006 min
Lab File: BG058193.D
Acq: 12 Jul 2023 19:23




Instrument :
BNA_G
ClientSampleId :
SSTD020512


Tgt Ion:152 Resp: 290002
Ion Ratio Lower Upper
152 100
151 20.8 15.6 23.4
153 13.2 10.5 15.7



#51
3-Nitroaniline
Concen: 16.634 ng/ul
RT: 14.504 min Scan# 1943
Delta R.T. 0.000 min
Lab File: BG058193.D
Acq: 12 Jul 2023 19:23

Tgt Ion:138 Resp: 36661
Ion Ratio Lower Upper
138 100
108 11.4 8.2 12.2
92 119.0 100.2 150.4



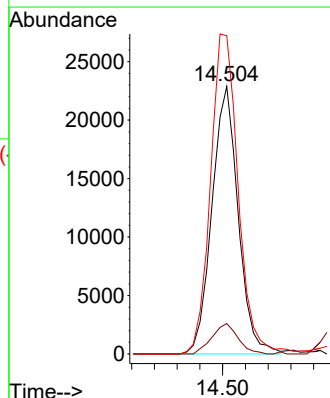





#52
Acenaphthene
Concen: 19.346 ng/ul
RT: 14.662 min Scan# 1970
Delta R.T. 0.000 min
Lab File: BG058193.D
Acq: 12 Jul 2023 19:23




Instrument :
BNA_G
ClientSampleId :
SSTD020512


Tgt Ion:153 Resp: 197836
Ion Ratio Lower Upper
153 100
152 47.1 36.5 54.7
154 85.6 70.5 105.7



#53
2,4-Dinitrophenol
Concen: 14.472 ng/ul
RT: 14.709 min Scan# 1978
Delta R.T. -0.006 min
Lab File: BG058193.D
Acq: 12 Jul 2023 19:23

Tgt Ion:184 Resp: 19677
Ion Ratio Lower Upper
184 100
63 75.1 51.1 76.7
154 59.6 43.3 64.9









#55
4-Nitrophenol
Concen: 16.260 ng/ul
RT: 14.809 min Scan# 1995
Delta R.T. -0.006 min
Lab File: BG058193.D
Acq: 12 Jul 2023 19:23




Instrument :
BNA_G
ClientSampleId :
SSTD020512


Tgt Ion:109 Resp: 26913
Ion Ratio Lower Upper
109 100
139 141.4 119.0 178.4
65 153.3 135.5 203.3

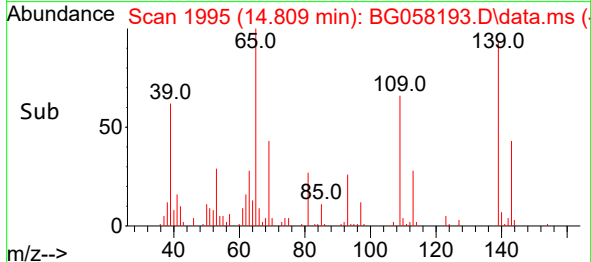

#56
Dibenzofuran
Concen: 19.299 ng/ul
RT: 14.997 min Scan# 2027
Delta R.T. 0.000 min
Lab File: BG058193.D
Acq: 12 Jul 2023 19:23

Tgt Ion:168 Resp: 280538
Ion Ratio Lower Upper
168 100
139 34.2 27.6 41.4

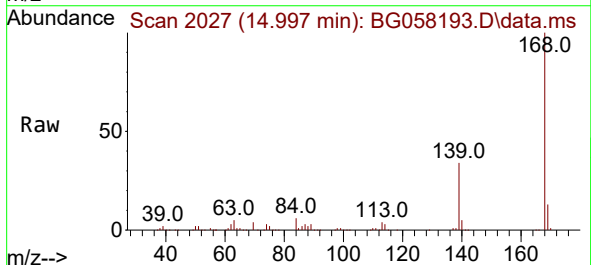



#57

2,4-Dinitrotoluene

Concen: 18.835 ng/ul

RT: 14.956 min Scan# 20

Delta R.T. -0.006 min

Lab File: BG058193.D

Acq: 12 Jul 2023 19:23

Instrument :

BNA_G

ClientSampleId :

SSTD020512





Tgt Ion:165 Resp: 69596

Ion Ratio Lower Upper

165 100

63 45.1 35.8 53.8

182 1.9 1.6 2.4



#58

2,3,4,6-Tetrachlorophenol

Concen: 18.320 ng/ul

RT: 15.220 min Scan# 2065

Delta R.T. -0.006 min

Lab File: BG058193.D

Acq: 12 Jul 2023 19:23

Tgt Ion:232 Resp: 59710




Ion Ratio Lower Upper


232 100

131 39.9 30.5 45.7

130 1.9 1.4 2.0

166 30.8 22.6 34.0



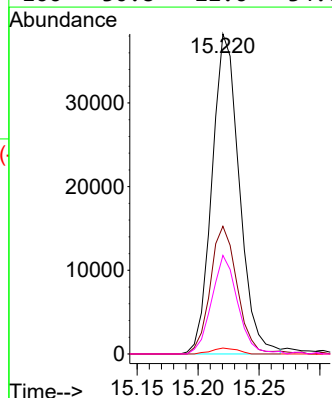





#59
Diethylphthalate
Concen: 17.444 ng/ul
RT: 15.408 min Scan# 2097
Delta R.T. 0.000 min
Lab File: BG058193.D
Acq: 12 Jul 2023 19:23




Instrument :
BNA_G
ClientSampleId :
SSTD020512


Tgt Ion:149 Resp: 231318
Ion Ratio Lower Upper
149 100
177 22.3 17.8 26.8
150 11.8 10.1 15.1



#61
Fluorene
Concen: 19.189 ng/ul
RT: 15.643 min Scan# 2137
Delta R.T. -0.006 min
Lab File: BG058193.D
Acq: 12 Jul 2023 19:23

Tgt Ion:166 Resp: 228866
Ion Ratio Lower Upper
166 100
165 98.9 79.1 118.7
167 13.0 10.7 16.1





#62

4-Chlorophenyl-phenylether

Concen: 19.067 ng/ul

RT: 15.632 min Scan# 2135

Delta R.T. -0.006 min

Lab File: BG058193.D

Acq: 12 Jul 2023 19:23

Instrument :

BNA_G

ClientSampleId :

SSTD020512





Tgt Ion:204 Resp: 120334

Ion Ratio Lower Upper

204 100

206 32.8 25.8 38.6

141 51.9 41.8 62.6

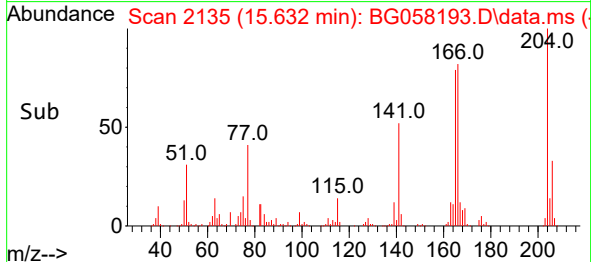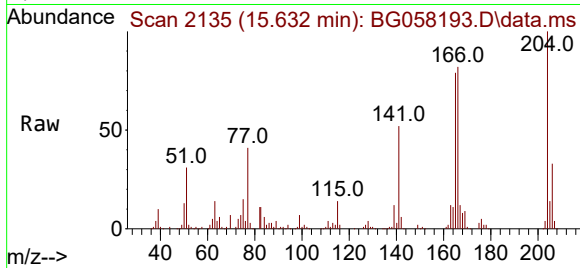

#63

4-Nitroaniline

Concen: 10.258 ng/ul

RT: 15.661 min Scan# 2140

Delta R.T. 0.000 min

Lab File: BG058193.D

Acq: 12 Jul 2023 19:23




Tgt Ion:138 Resp: 20252


Ion Ratio Lower Upper

138 100

92 50.7 43.8 65.8

108 74.3 58.8 88.2




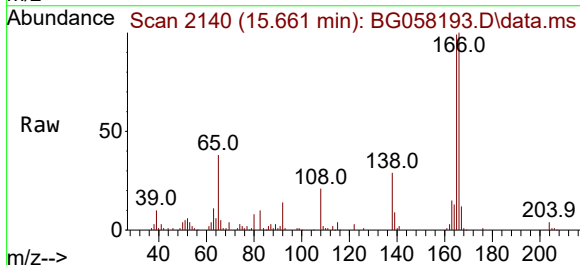




#66
4,6-Dinitro-2-methylphenol
Concen: 17.960 ng/ul
RT: 15.720 min Scan# 2151
Delta R.T. 0.000 min
Lab File: BG058193.D
Acq: 12 Jul 2023 19:23




Instrument :
BNA_G
ClientSampleId :
SSTD020512


Tgt Ion:198 Resp: 36822
Ion Ratio Lower Upper
198 100
182 4.7 3.1 4.7#
77 22.9 17.9 26.9



#67
N-Nitrosodiphenylamine
Concen: 19.305 ng/ul
RT: 15.849 min Scan# 2172
Delta R.T. 0.000 min
Lab File: BG058193.D
Acq: 12 Jul 2023 19:23

Tgt Ion:169 Resp: 189684
Ion Ratio Lower Upper
169 100
168 69.8 54.2 81.2
167 39.2 30.8 46.2









#68
4-Bromophenyl-phenylether
Concen: 19.824 ng/ul
RT: 16.525 min Scan# 21
Delta R.T. -0.006 min
Lab File: BG058193.D
Acq: 12 Jul 2023 19:23




Instrument :
BNA_G
ClientSampleId :
SSTD020512


Tgt Ion:248 Resp: 80342
Ion Ratio Lower Upper
248 100
250 98.3 78.3 117.5
141 62.4 49.1 73.7

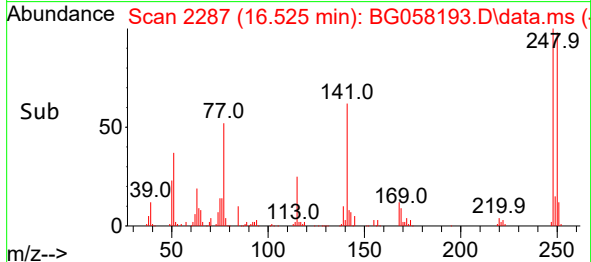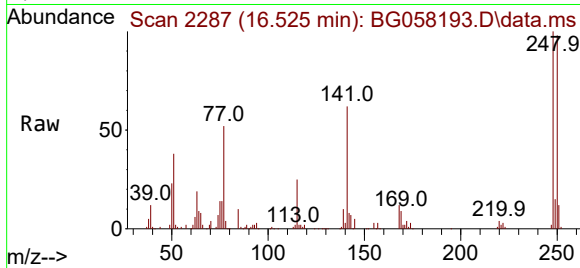

#69
Hexachlorobenzene
Concen: 19.581 ng/ul
RT: 16.648 min Scan# 2308
Delta R.T. 0.000 min
Lab File: BG058193.D
Acq: 12 Jul 2023 19:23

Tgt Ion:284 Resp: 88845
Ion Ratio Lower Upper
284 100
142 26.4 21.9 32.9
249 31.5 25.0 37.6

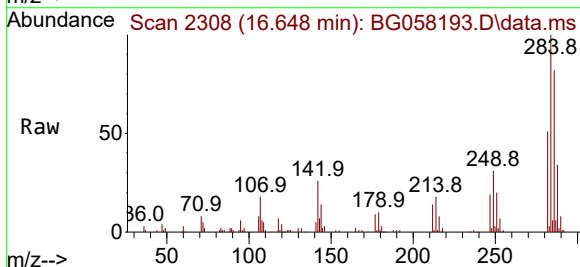



#70

Atrazine

Concen: 18.277 ng/ul

RT: 16.789 min Scan# 21

Delta R.T. -0.006 min

Lab File: BG058193.D

Acq: 12 Jul 2023 19:23

Instrument :

BNA_G

ClientSampleId :

SSTD020512





Tgt Ion:200 Resp: 73437

Ion Ratio Lower Upper

200 100

173 24.8 20.0 30.0

215 46.7 35.8 53.8



#71

Pentachlorophenol

Concen: 14.866 ng/ul

RT: 16.989 min Scan# 2366

Delta R.T. -0.006 min

Lab File: BG058193.D

Acq: 12 Jul 2023 19:23




Tgt Ion:266 Resp: 40496


Ion Ratio Lower Upper

266 100

264 66.1 51.5 77.3

268 70.6 49.0 73.4







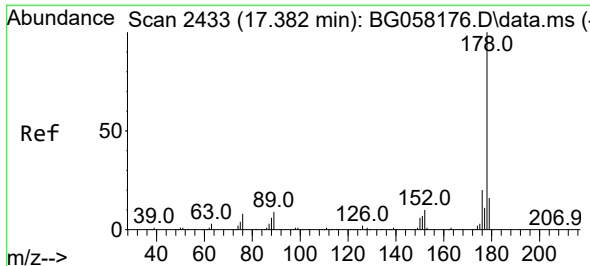

#72
Phenanthrene
Concen: 19.045 ng/ul
RT: 17.383 min Scan# 2433
Delta R.T. 0.000 min
Lab File: BG058193.D
Acq: 12 Jul 2023 19:23




Instrument :
BNA_G
ClientSampleId :
SSTD020512


Tgt Ion:178 Resp: 357667
Ion Ratio Lower Upper
178 100
179 16.5 12.8 19.2
176 19.9 15.7 23.5

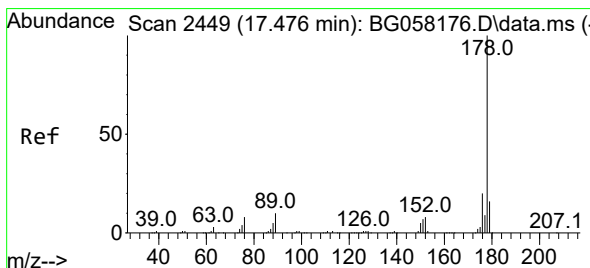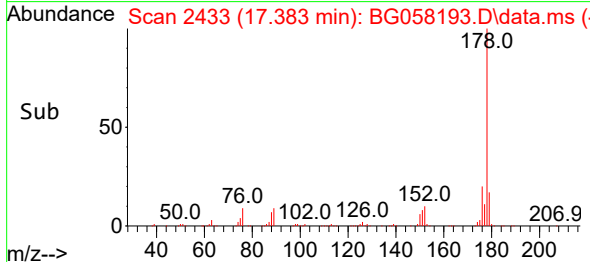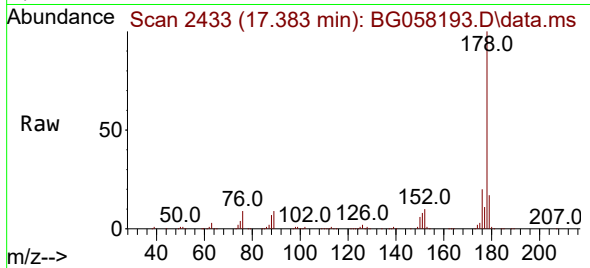

#74
Anthracene
Concen: 19.046 ng/ul
RT: 17.477 min Scan# 2449
Delta R.T. 0.000 min
Lab File: BG058193.D
Acq: 12 Jul 2023 19:23

Tgt Ion:178 Resp: 361969
Ion Ratio Lower Upper
178 100
179 15.3 12.6 18.8
176 19.2 15.4 23.2


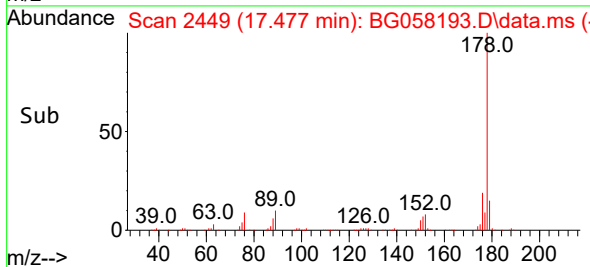

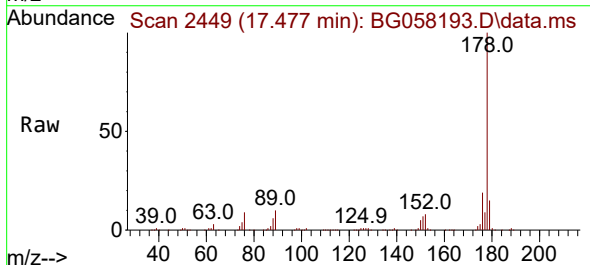




#75
1,2,3,4-Tetrachlorobenzene
Concen: 21.315 ng/uL
RT: 13.399 min Scan# 1
Delta R.T. 0.000 min
Lab File: BG058193.D
Acq: 12 Jul 2023 19:23




Instrument :
BNA_G
ClientSampleId :
SSTD020512


Tgt Ion:216 Resp: 104368
Ion Ratio Lower Upper
216 100
214 78.3 64.8 97.2
218 48.7 39.1 58.7

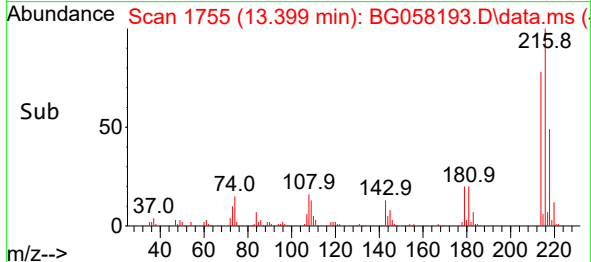

#76
Pentachlorobenzene
Concen: 20.750 ng/uL
RT: 14.915 min Scan# 2013
Delta R.T. -0.006 min
Lab File: BG058193.D
Acq: 12 Jul 2023 19:23

Tgt Ion:250 Resp: 108509
Ion Ratio Lower Upper
250 100
248 62.7 52.8 79.2
252 62.9 52.4 78.6




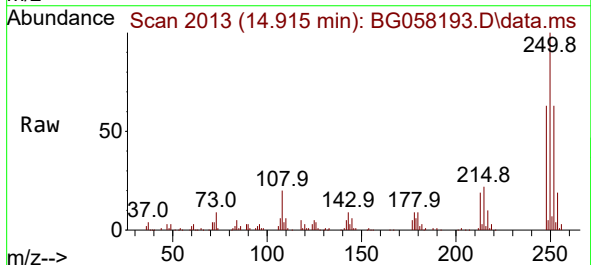


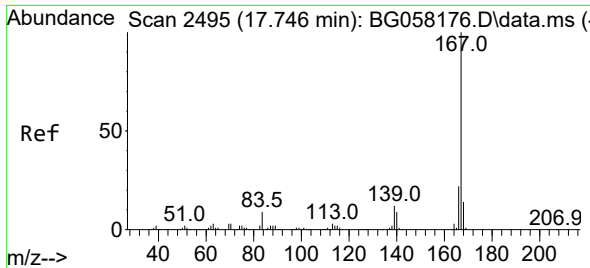

#77
 Carbazole
 Concen: 19.041 ng/ul
 RT: 17.741 min Scan# 2494
 Delta R.T. -0.006 min
 Lab File: BG058193.D
 Acq: 12 Jul 2023 19:23




Instrument :
 BNA_G
 ClientSampleId :
 SSTD020512


Tgt Ion:167 Resp: 327266
 Ion Ratio Lower Upper
 167 100
 166 21.9 17.5 26.3
 139 11.5 9.5 14.3

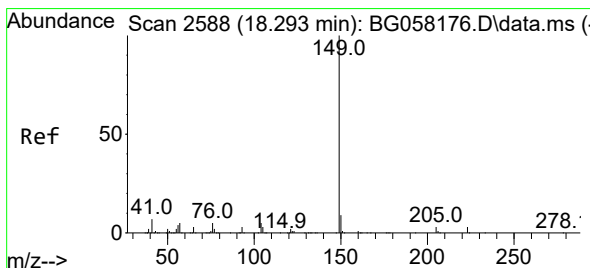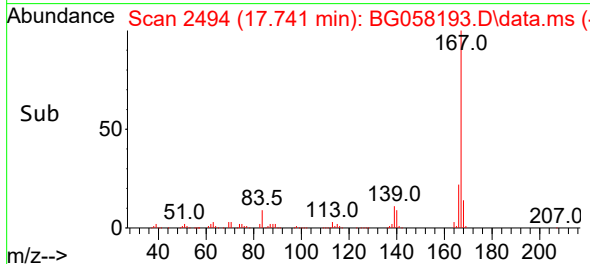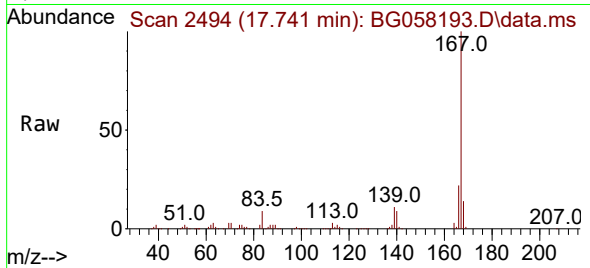

#78
 Di-n-butylphthalate
 Concen: 18.354 ng/ul
 RT: 18.293 min Scan# 2588
 Delta R.T. -0.006 min
 Lab File: BG058193.D
 Acq: 12 Jul 2023 19:23

Tgt Ion:149 Resp: 401860
 Ion Ratio Lower Upper
 149 100
 150 9.1 7.4 11.2
 104 4.8 3.9 5.9


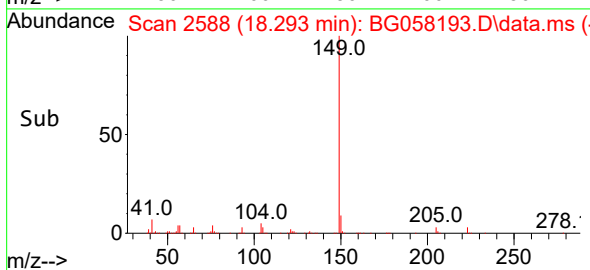

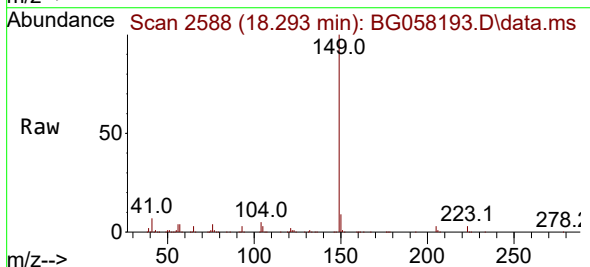




#80
Fluoranthene
Concen: 18.062 ng/ul
RT: 19.392 min Scan# 21
Delta R.T. 0.000 min
Lab File: BG058193.D
Acq: 12 Jul 2023 19:23




Instrument :
BNA_G
ClientSampleId :
SSTD020512


Tgt Ion:202 Resp: 426845
Ion Ratio Lower Upper
202 100
101 10.9 9.1 13.7
100 8.4 7.1 10.7

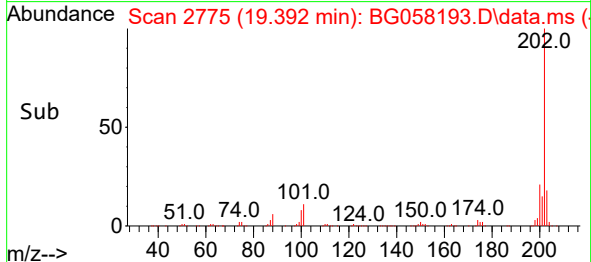

#82
Pyrene
Concen: 18.208 ng/ul
RT: 19.756 min Scan# 2837
Delta R.T. 0.000 min
Lab File: BG058193.D
Acq: 12 Jul 2023 19:23

Tgt Ion:202 Resp: 433138
Ion Ratio Lower Upper
202 100
101 13.2 10.2 15.2
100 11.1 8.9 13.3




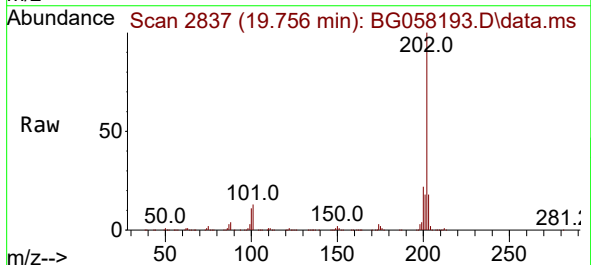




#83
Butylbenzylphthalate
Concen: 18.614 ng/ul
RT: 20.632 min Scan# 2986
Delta R.T. -0.006 min
Lab File: BG058193.D
Acq: 12 Jul 2023 19:23




Instrument :
BNA_G
ClientSampleId :
SSTD020512


Tgt Ion:149 Resp: 179555
Ion Ratio Lower Upper
149 100
91 70.0 56.5 84.7
206 21.9 17.4 26.0



#84
3,3'-Dichlorobenzidine
Concen: 20.286 ng/ul
RT: 21.495 min Scan# 3133
Delta R.T. 0.000 min
Lab File: BG058193.D
Acq: 12 Jul 2023 19:23

Tgt Ion:252 Resp: 159036
Ion Ratio Lower Upper
252 100
254 66.2 50.7 76.1
126 9.6 6.6 10.0





#85

Benzo(a)anthracene

Concen: 18.886 ng/ul

RT: 21.578 min Scan# 3147

Delta R.T. 0.000 min

Lab File: BG058193.D

Acq: 12 Jul 2023 19:23

Instrument :

BNA_G

ClientSampleId :

SSTD020512





Tgt Ion:228 Resp: 439122

Ion Ratio Lower Upper

228 100

229 20.3 16.0 24.0

226 28.4 22.0 33.0

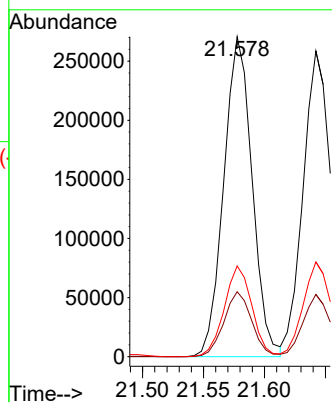

#86

Bis(2-ethylhexyl)phthalate

Concen: 18.756 ng/ul

RT: 21.472 min Scan# 3129

Delta R.T. -0.006 min

Lab File: BG058193.D

Acq: 12 Jul 2023 19:23




Tgt Ion:149 Resp: 259270


Ion Ratio Lower Upper

149 100

167 26.9 20.9 31.3

279 3.6 3.1 4.7





#87

Chrysene

Concen: 18.675 ng/ul

RT: 21.642 min Scan# 3159

Delta R.T. -0.006 min

Lab File: BG058193.D

Acq: 12 Jul 2023 19:23

Instrument :

BNA_G

ClientSampleId :

SSTD020512





Tgt Ion:228 Resp: 407062

Ion Ratio Lower Upper

228 100

226 31.0 24.4 36.6

229 20.4 15.5 23.3



#89

Di-n-octyl phthalate

Concen: 19.076 ng/ul




RT: 22.670 min Scan# 3333


Delta R.T. -0.006 min

Lab File: BG058193.D

Acq: 12 Jul 2023 19:23

Tgt Ion:149 Resp: 455984









#90
Benzo(b)fluoranthene
Concen: 18.912 ng/ul
RT: 23.769 min Scan# 3520
Delta R.T. 0.000 min
Lab File: BG058193.D
Acq: 12 Jul 2023 19:23




Instrument :
BNA_G
ClientSampleId :
SSTD020512


Tgt Ion:252 Resp: 455573
Ion Ratio Lower Upper
252 100
253 21.7 18.1 27.1
125 9.2 7.5 11.3



#91
Benzo(k)fluoranthene
Concen: 18.943 ng/ul
RT: 23.834 min Scan# 3531
Delta R.T. -0.006 min
Lab File: BG058193.D
Acq: 12 Jul 2023 19:23

Tgt Ion:252 Resp: 447261
Ion Ratio Lower Upper
252 100
253 22.6 17.7 26.5
125 8.6 7.4 11.2









#93
Benzo(a)pyrene
Concen: 18.786 ng/ul
RT: 24.639 min Scan# 3668
Delta R.T. 0.000 min
Lab File: BG058193.D
Acq: 12 Jul 2023 19:23




Instrument :
BNA_G
ClientSampleId :
SSTD020512


Tgt Ion:252 Resp: 400549
Ion Ratio Lower Upper
252 100
253 21.4 17.8 26.6
125 10.3 8.3 12.5

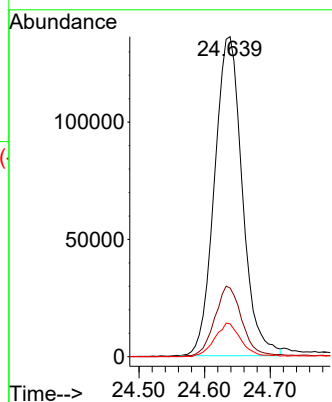

#94
Indeno(1,2,3-cd)pyrene
Concen: 16.902 ng/ul
RT: 28.423 min Scan# 4312
Delta R.T. 0.000 min
Lab File: BG058193.D
Acq: 12 Jul 2023 19:23

Tgt Ion:276 Resp: 478549
Ion Ratio Lower Upper
276 100
138 16.9 14.0 21.0
277 25.0 19.4 29.2





#95

Dibenzo(a,h)anthracene

Concen: 7.770 ng/ul

RT: 28.481 min Scan# 41

Delta R.T. -0.006 min

Lab File: BG058193.D

Acq: 12 Jul 2023 19:23

Instrument :

BNA_G

ClientSampleId :

SSTD020512





Tgt Ion:278 Resp: 181403

Ion Ratio Lower Upper

278 100

139 13.1 11.3 16.9

279 24.5 18.9 28.3

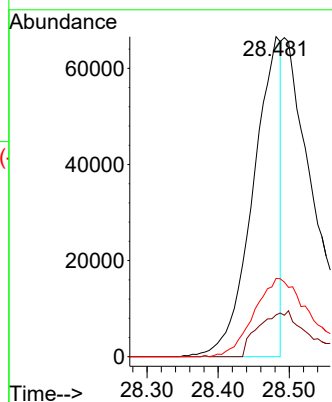

#96

Benzo(g,h,i)perylene

Concen: 14.549 ng/ul

RT: 29.562 min Scan# 4506

Delta R.T. 0.000 min

Lab File: BG058193.D

Acq: 12 Jul 2023 19:23

Tgt Ion:276 Resp: 336446

Ion Ratio Lower Upper

276 100

138 18.7 14.2 21.2

277 24.2 18.6 27.8

