




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071123\
 Data File : BG058166.D
 Acq On : 11 Jul 2023 19:46
 Operator : CG/JU
 Sample : 03385-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EX7X9

Manual IntegrationsAPPROVED

Quant Time: Jul 11 22:58:00 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 10 16:52:40 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/12/2023
 Supervised By :mohammad ahmed 07/12/2023

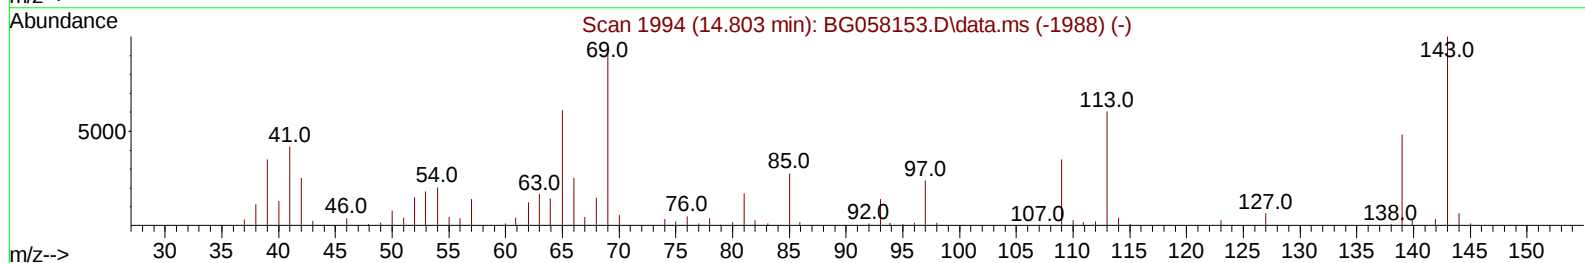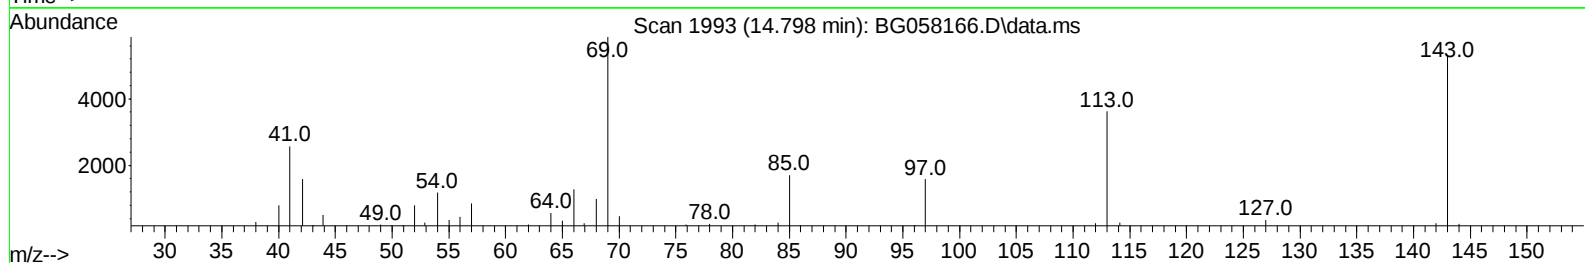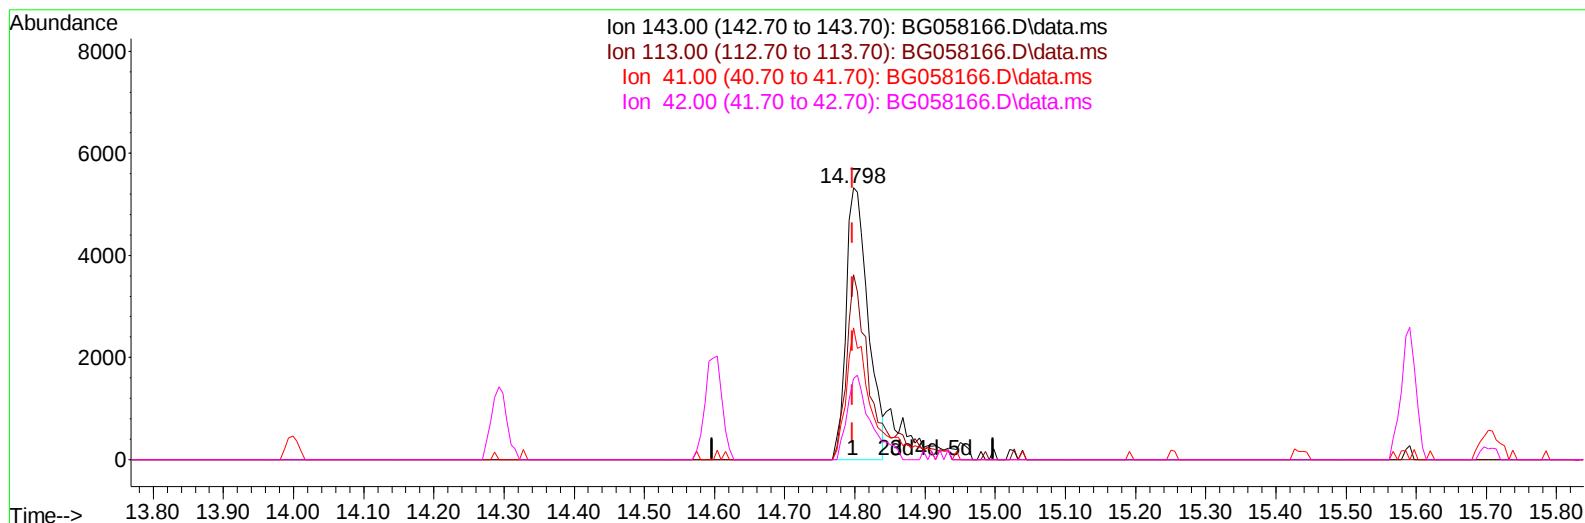

TIC: BG058166.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.798min (+ 0.001) 6.71 ng/u1

response 11608

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	66.40	68.06
41.00	40.50	48.37
42.00	27.50	29.91




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071123\
Data File : BG058166.D
Acq On : 11 Jul 2023 19:46
Operator : CG/JU
Sample : 03385-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EX7X9

Manual IntegrationsAPPROVED

Quant Time: Jul 11 22:58:00 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 10 16:52:40 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/12/2023
Supervised By :mohammad ahmed 07/12/2023

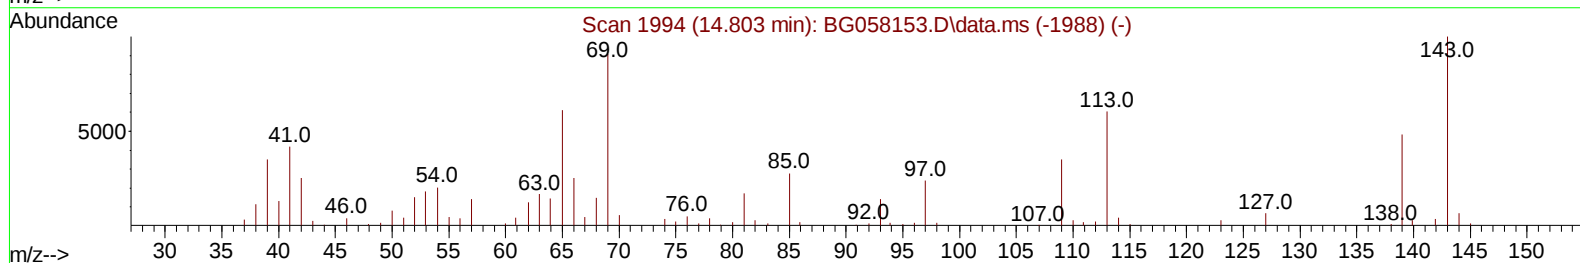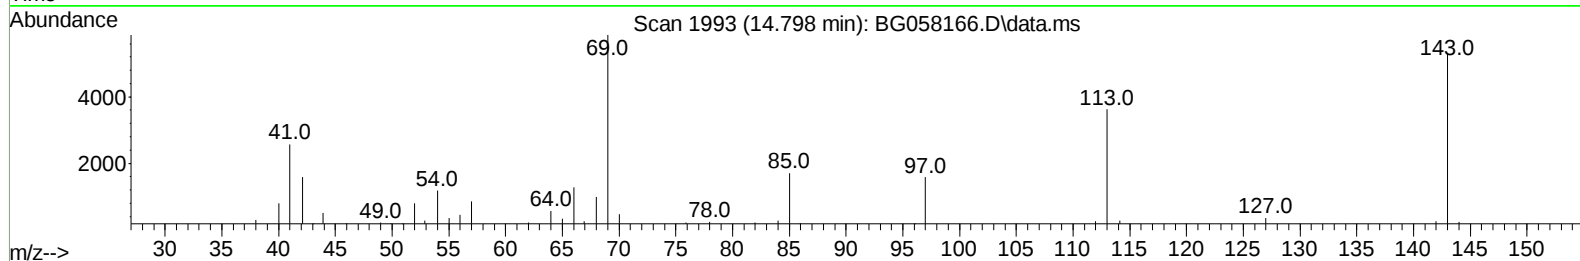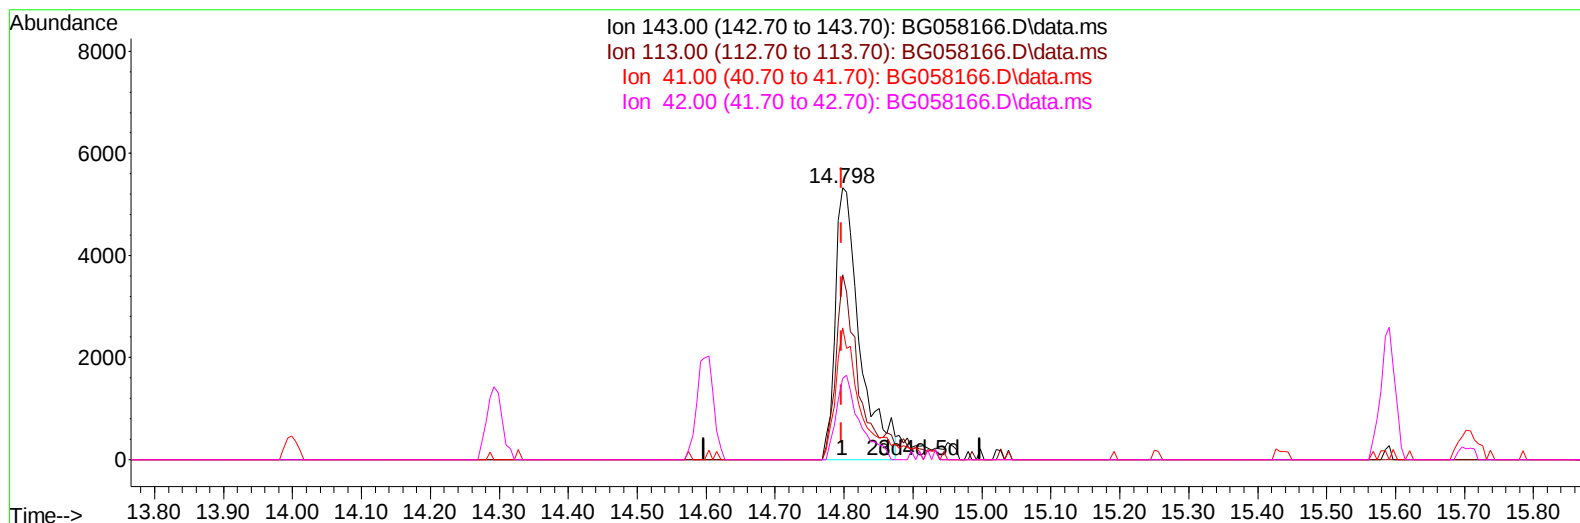

TIC: BG058166.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.798min (+ 0.001) 7.58 ng/ul m

response 13122

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	66.40	68.06
41.00	40.50	48.37
42.00	27.50	29.91

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071123\
 Data File : BG058166.D
 Acq On : 11 Jul 2023 19:46
 Operator : CG/JU
 Sample : 03385-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EX7X9

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/12/2023
 Supervised By :mohammad ahmed 07/12/2023

Quant Time: Jul 11 23:36:55 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 10 16:52:40 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.976	152	36853	20.000	ng/ul	0.00
20) Naphthalene-d8	10.779	136	173857	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.598	164	124114	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.342	188	283512	20.000	ng/ul	0.00
79) Chrysene-d12	21.601	240	244236	20.000	ng/ul	0.00
88) Perylene-d12	24.792	264	297451	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.405	96	1994	1.895	ng/uL	0.00
4) Pyridine-d5	3.816	84	22687	7.101	ng/ul	0.00
7) Phenol-d5	7.130	99	63991	17.003	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.295	67	38821	17.116	ng/ul	0.00
11) 2-Chlorophenol-d4	7.506	132	45320	17.459	ng/ul	0.00
15) 4-Methylphenol-d8	8.675	113	51158	18.014	ng/ul	0.00
21) Nitrobenzene-d5	9.134	128	24876	17.555	ng/ul	0.00
24) 2-Nitrophenol-d4	9.856	143	27532	18.487	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.397	165	52030	18.212	ng/ul	0.00
31) 4-Chloroaniline-d4	10.908	131	75045	17.325	ng/ul	0.00
46) Dimethylphthalate-d6	13.999	166	176711	18.045	ng/ul	0.00
49) Acenaphthylene-d8	14.292	160	205439	19.225	ng/ul	0.00
54) 4-Nitrophenol-d4	14.798	143	13122m	7.584	ng/ul	0.00
60) Fluorene-d10	15.591	176	161457	19.414	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.708	200	9933	6.452	ng/ul	0.00
73) Anthracene-d10	17.442	188	254262	19.327	ng/ul	0.00
81) Pyrene-d10	19.727	212	292172	18.994	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.569	264	302124	19.936	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071123\
Data File : BG058166.D
Acq On : 11 Jul 2023 19:46
Operator : CG/JU
Sample : 03385-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EX7X9

Manual IntegrationsAPPROVED

Quant Time: Jul 11 23:36:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 10 16:52:40 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/12/2023
Supervised By :mohammad ahmed 07/12/2023

