




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071123\
 Data File : BG058177.D
 Acq On : 12 Jul 2023 6:49
 Operator : CG/JU
 Sample : PB153956BL
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK956

Manual IntegrationsAPPROVED

Quant Time: Jul 12 07:32:13 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 10 16:52:40 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/12/2023
 Supervised By :mohammad ahmed 07/13/2023

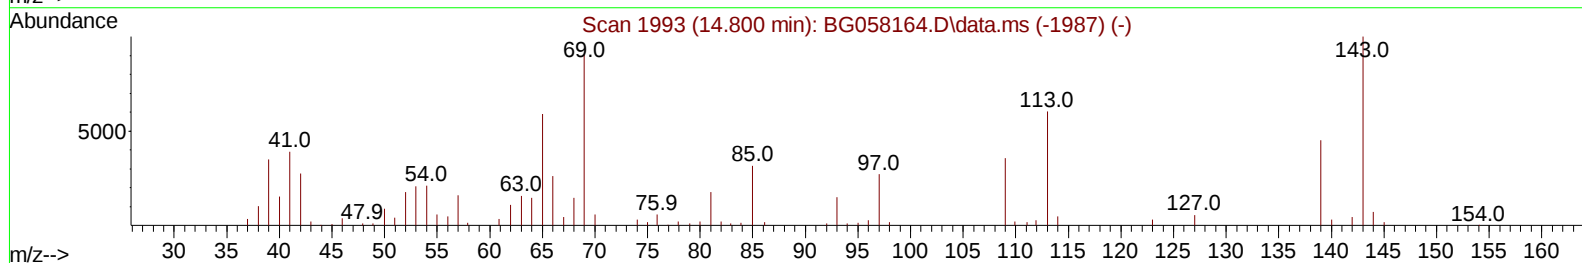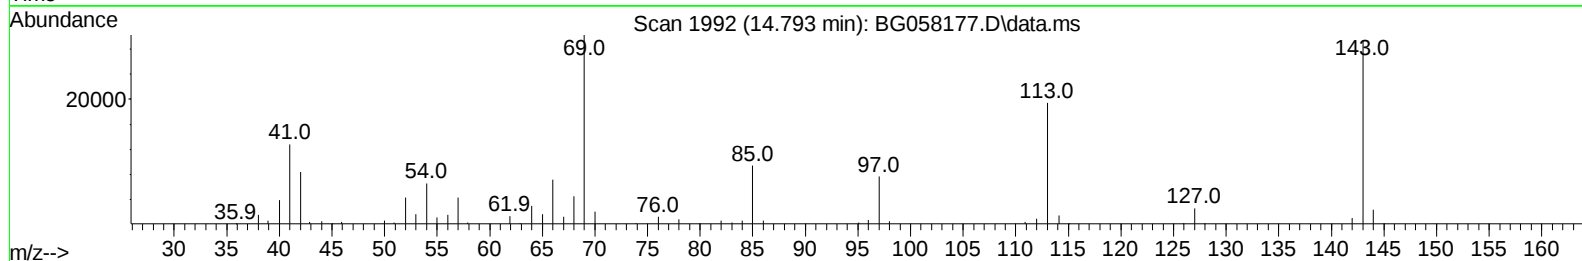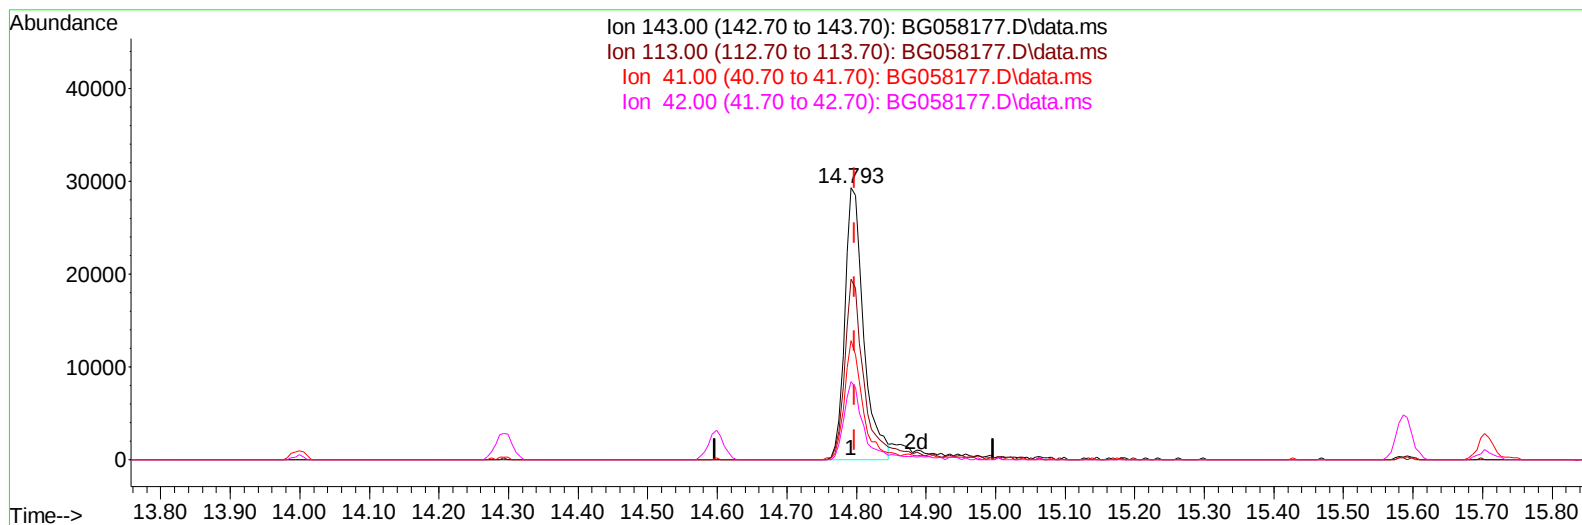

TIC: BG058177.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.793min (-0.004) 21.87 ng/u1

response 54773

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	66.40	66.41
41.00	40.50	43.78
42.00	27.50	28.66




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071123\
 Data File : BG058177.D
 Acq On : 12 Jul 2023 6:49
 Operator : CG/JU
 Sample : PB153956BL
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK956

Manual IntegrationsAPPROVED

Quant Time: Jul 12 07:32:13 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 10 16:52:40 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/12/2023
 Supervised By :mohammad ahmed 07/13/2023

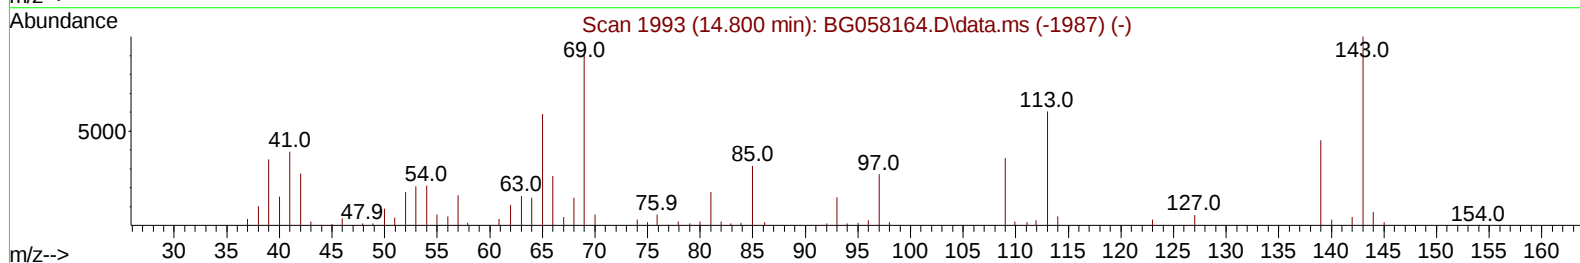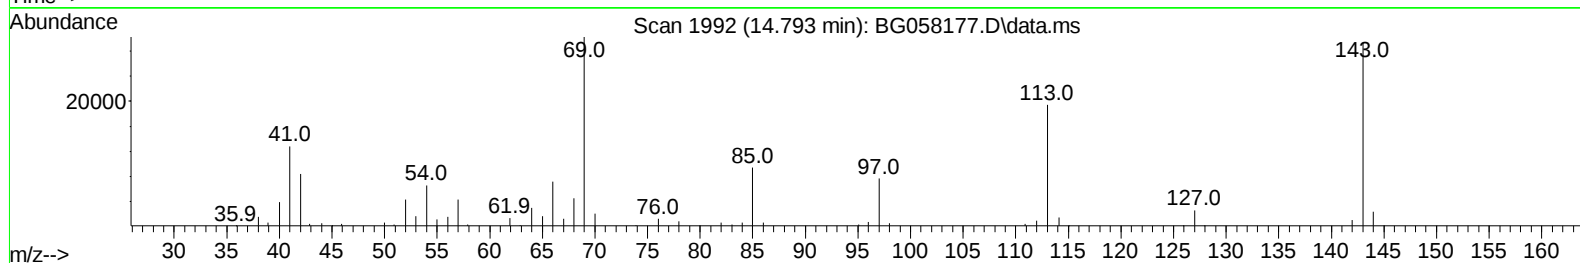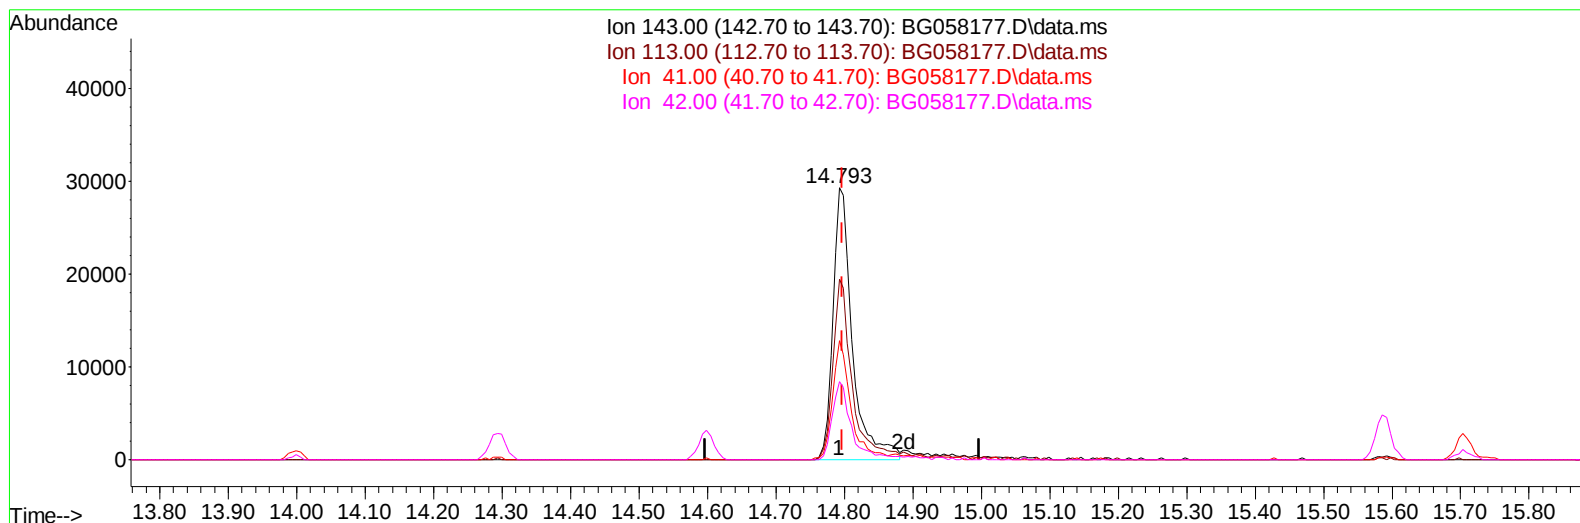

TIC: BG058177.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.793min (-0.004) 23.05 ng/ul m

response 57708

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	66.40	66.41
41.00	40.50	43.78
42.00	27.50	28.66

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071123\
 Data File : BG058177.D
 Acq On : 12 Jul 2023 6:49
 Operator : CG/JU
 Sample : PB153956BL
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK956

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/12/2023
 Supervised By :mohammad ahmed 07/13/2023

Quant Time: Jul 12 07:34:44 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 10 16:52:40 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.971	152	52103	20.000	ng/ul	0.00
20) Naphthalene-d8	10.774	136	245691	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.599	164	179625	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.343	188	420321	20.000	ng/ul	0.00
79) Chrysene-d12	21.596	240	373070	20.000	ng/ul	0.00
88) Perylene-d12	24.787	264	441829	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.400	96	7743	5.204	ng/uL	0.00
4) Pyridine-d5	3.811	84	114731	25.398	ng/ul	0.00
7) Phenol-d5	7.131	99	149785	28.150	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.295	67	88646	27.645	ng/ul	0.00
11) 2-Chlorophenol-d4	7.501	132	104019	28.344	ng/ul	0.00
15) 4-Methylphenol-d8	8.670	113	114306	28.470	ng/ul	0.00
21) Nitrobenzene-d5	9.134	128	56090	28.010	ng/ul	0.00
24) 2-Nitrophenol-d4	9.857	143	64296	30.550	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.392	165	111495	27.616	ng/ul	0.00
31) 4-Chloroaniline-d4	10.909	131	163946	26.783	ng/ul	0.00
46) Dimethylphthalate-d6	13.999	166	369493	26.071	ng/ul	0.00
49) Acenaphthylene-d8	14.293	160	431230	27.883	ng/ul	0.00
54) 4-Nitrophenol-d4	14.793	143	57708m	23.047	ng/ul	0.00
60) Fluorene-d10	15.586	176	338652	28.136	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.703	200	48879	21.416	ng/ul	0.00
73) Anthracene-d10	17.442	188	551736	28.288	ng/ul	0.00
81) Pyrene-d10	19.728	212	639768	27.229	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.575	264	661194	29.373	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071123\
Data File : BG058177.D
Acq On : 12 Jul 2023 6:49
Operator : CG/JU
Sample : PB153956BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK956

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/12/2023
Supervised By :mohammad ahmed 07/13/2023

Quant Time: Jul 12 07:34:44 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 10 16:52:40 2023
Response via : Initial Calibration

