

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071123\
 Data File : BG058192.D
 Acq On : 12 Jul 2023 18:41
 Operator : CG/JU
 Sample : 03477-02DL 5X
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 HOA42DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG058192.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.141	5	9	19	rVB	183633	251589	17.43%	3.137%
2	3.382	45	50	55	rBV	53527	81155	5.62%	1.012%
3	3.440	56	60	70	rVB	36456	53919	3.74%	0.672%
4	3.822	121	125	134	rVB3	13995	24274	1.68%	0.303%
5	4.686	265	272	286	rBV	920925	1443259	100.00%	17.998%
6	5.039	329	332	337	rVB4	1129	2143	0.15%	0.027%
7	7.001	663	666	670	rBV3	856	1550	0.11%	0.019%
8	7.136	683	689	694	rBV2	7039	12569	0.87%	0.157%
9	7.295	711	716	727	rVB	32481	53916	3.74%	0.672%
10	7.500	746	751	758	rBV	26757	46499	3.22%	0.580%
11	7.577	760	764	769	rVB5	979	1462	0.10%	0.018%
12	7.970	824	831	839	rBV	153402	255422	17.70%	3.185%
13	8.675	945	951	957	rBV2	19828	34926	2.42%	0.436%
14	9.134	1023	1029	1039	rBV	37804	70792	4.91%	0.883%
15	9.856	1146	1152	1159	rVB2	27133	50095	3.47%	0.625%
16	10.397	1238	1244	1254	rBV3	41871	77505	5.37%	0.966%
17	10.773	1300	1308	1321	rVB	239693	431834	29.92%	5.385%
18	10.908	1326	1331	1338	rBV	44039	80482	5.58%	1.004%
19	13.482	1765	1769	1774	rBV4	4370	6955	0.48%	0.087%
20	13.846	1824	1831	1837	rBV3	6096	9710	0.67%	0.121%
21	13.999	1851	1857	1863	rBV	101103	148737	10.31%	1.855%
22	14.292	1901	1907	1913	rBV	115869	178591	12.37%	2.227%
23	14.598	1952	1959	1973	rBV	407708	638116	44.21%	7.957%
24	14.815	1992	1996	2001	rBV6	1506	3180	0.22%	0.040%
25	15.585	2121	2127	2137	rBV	154300	237727	16.47%	2.964%
26	15.703	2143	2147	2156	rVB2	22474	35615	2.47%	0.444%
27	15.949	2184	2189	2197	rVB2	9429	14755	1.02%	0.184%
28	17.342	2419	2426	2435	rBV	529923	780872	54.10%	9.738%
29	17.436	2435	2442	2452	rVB	159633	250993	17.39%	3.130%
30	18.217	2573	2575	2581	rBV4	2368	3731	0.26%	0.047%
31	18.305	2584	2590	2597	rVV3	16121	22296	1.54%	0.278%
32	19.298	2755	2759	2761	rVV4	2485	2951	0.20%	0.037%
33	19.328	2761	2764	2766	rVB2	1529	1542	0.11%	0.019%
34	19.363	2766	2770	2773	rBV2	3123	4234	0.29%	0.053%
35	19.498	2789	2793	2796	rBV4	1354	1650	0.11%	0.021%
36	19.627	2812	2815	2821	rVV6	2526	3665	0.25%	0.046%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071123\
 Data File : BG058192.D
 Acq On : 12 Jul 2023 18:41
 Operator : CG/JU
 Sample : 03477-02DL 5X
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 HOA42DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Title : SVOA CALIBRATION

37	19.721	2826	2831	2840	rBV	214111	316994	21.96%	3.953%
38	19.810	2845	2846	2852	rVB5	1764	2634	0.18%	0.033%
39	20.379	2940	2943	2945	rBV4	1087	1480	0.10%	0.018%
40	20.473	2955	2959	2961	rBV4	1866	2619	0.18%	0.033%
41	20.679	2989	2994	2996	rBV4	2527	4086	0.28%	0.051%
42	20.826	3016	3019	3020	rBV3	2419	2597	0.18%	0.032%
43	20.855	3023	3024	3027	rVV3	2344	1745	0.12%	0.022%
44	21.055	3056	3058	3061	rVB4	3040	2213	0.15%	0.028%
45	21.349	3106	3108	3110	rBV2	3176	3063	0.21%	0.038%
46	21.596	3143	3150	3160	rBV	495806	814173	56.41%	10.153%
47	21.860	3193	3195	3196	rBV2	2618	1919	0.13%	0.024%
48	22.042	3222	3226	3227	rBV4	1963	2160	0.15%	0.027%
49	22.189	3250	3251	3252	rBV	2709	1810	0.13%	0.023%
50	22.371	3278	3282	3288	rBV6	5688	9701	0.67%	0.121%
51	22.518	3305	3307	3310	rVV4	2230	2266	0.16%	0.028%
52	22.835	3359	3361	3362	rBV2	1884	1528	0.11%	0.019%
53	23.053	3391	3398	3405	rVB4	10748	26514	1.84%	0.331%
54	23.846	3528	3533	3539	rVB2	16124	30306	2.10%	0.378%
55	23.934	3546	3548	3552	rVB6	3326	3090	0.21%	0.039%
56	24.128	3579	3581	3583	rBV3	2179	1525	0.11%	0.019%
57	24.563	3646	3655	3670	rBV	104287	302112	20.93%	3.767%
58	24.792	3682	3694	3709	rBV2	297995	944546	65.45%	11.779%
59	25.896	3872	3882	3892	rBV3	23637	69590	4.82%	0.868%
60	26.948	4060	4061	4064	rBV2	2214	2116	0.15%	0.026%
61	27.130	4090	4092	4093	rBV2	2246	1570	0.11%	0.020%
62	27.230	4101	4109	4121	rVB3	21146	74840	5.19%	0.933%
63	27.665	4181	4183	4184	rVB2	2699	1506	0.10%	0.019%
64	28.423	4309	4312	4313	rBV2	2356	2116	0.15%	0.026%
65	28.840	4374	4383	4395	rVB7	17361	63843	4.42%	0.796%
66	30.679	4694	4696	4697	rBV2	2502	1570	0.11%	0.020%
67	31.226	4786	4789	4790	rBV2	2413	2275	0.16%	0.028%
68	32.336	4977	4978	4980	rBV2	2382	1965	0.14%	0.025%




Sum of corrected areas: 8019183

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071123\
Data File : BG058192.D
Acq On : 12 Jul 2023 18:41
Operator : CG/JU
Sample : 03477-02DL 5X
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
HOA42DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

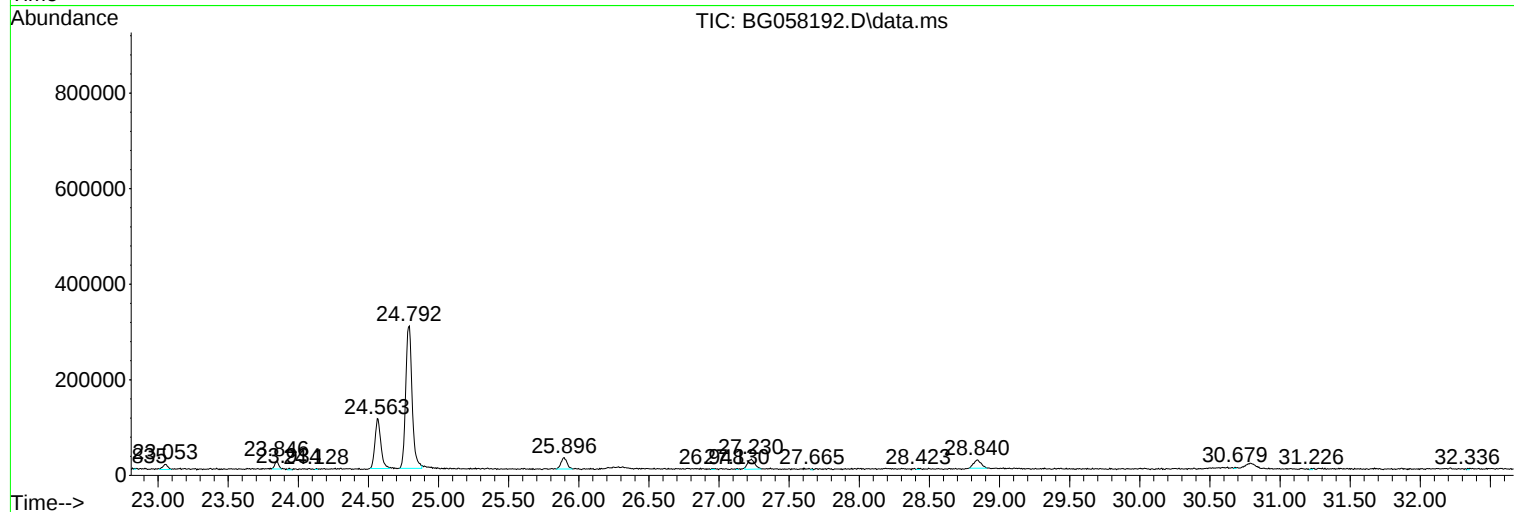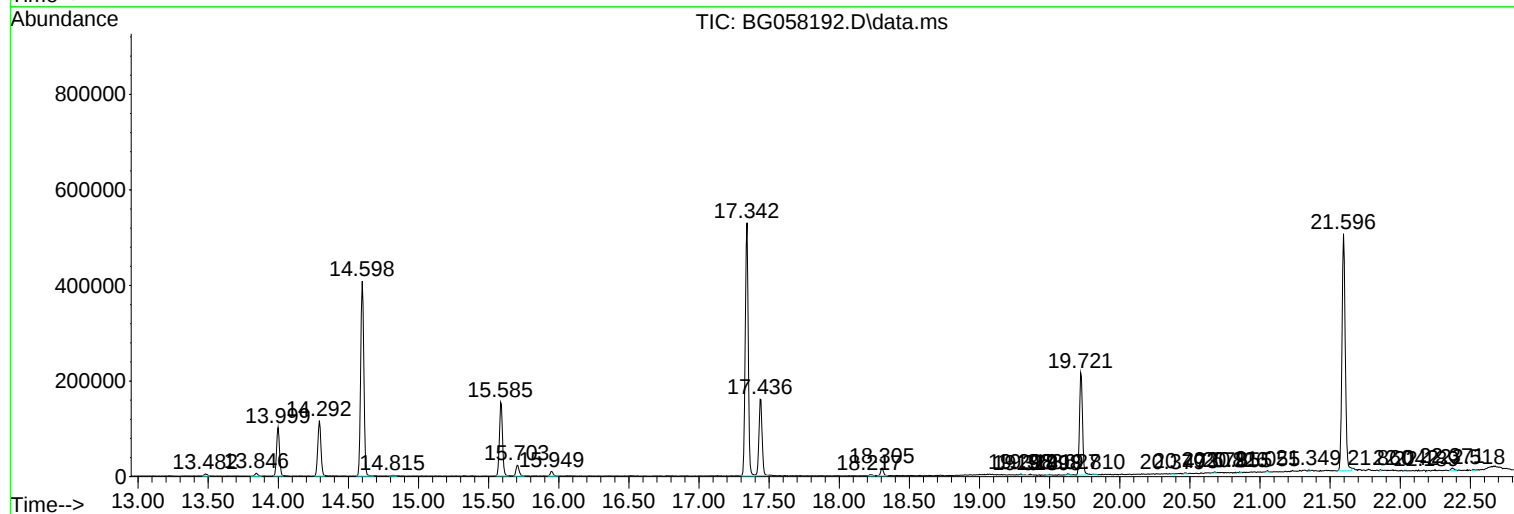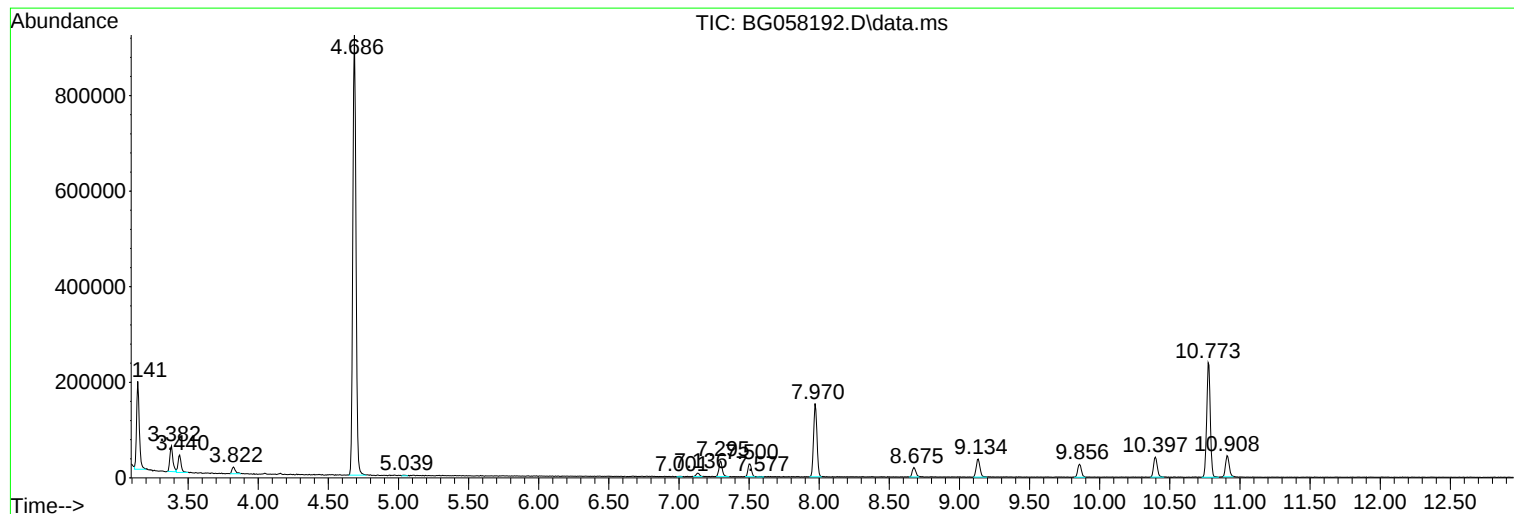

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071123\
Data File : BG058192.D
Acq On : 12 Jul 2023 18:41
Operator : CG/JU
Sample : 03477-02DL 5X
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
HOA42DL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.141	19.70 ng/ul	251589	1,4-Dichlorobenzene-d4	7.970

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	72
3			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	39
4			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	39
5			Acetamide, N-ethyl-	87	C4H9NO	000625-50-3	27

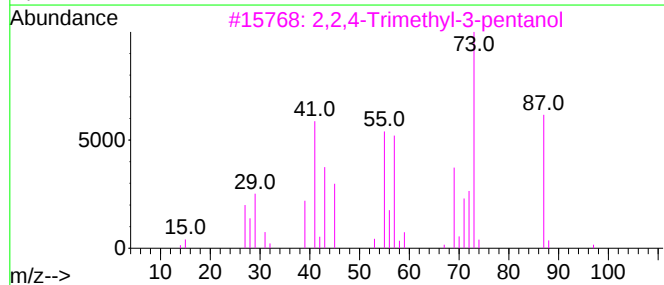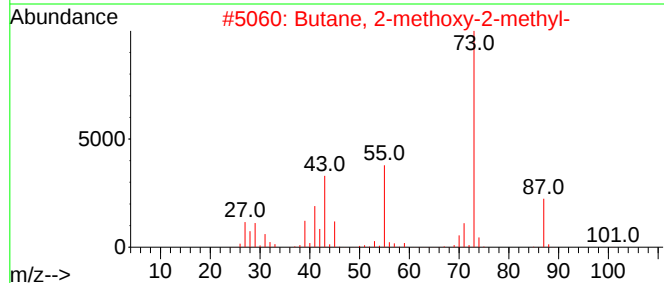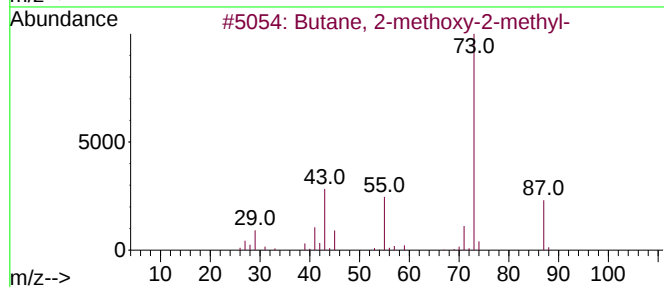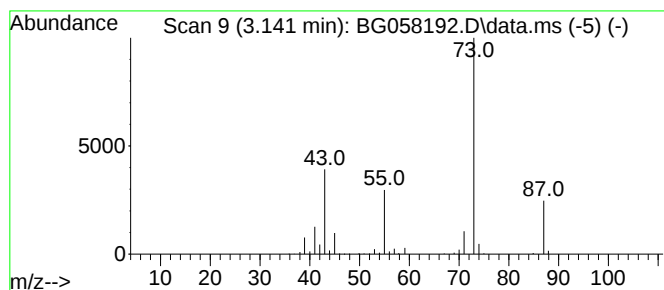

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071123\
Data File : BG058192.D
Acq On : 12 Jul 2023 18:41
Operator : CG/JU
Sample : 03477-02DL 5X
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
HOA42DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.141	19.7	ng/ul	251589	1	7.970	255422	20.0