
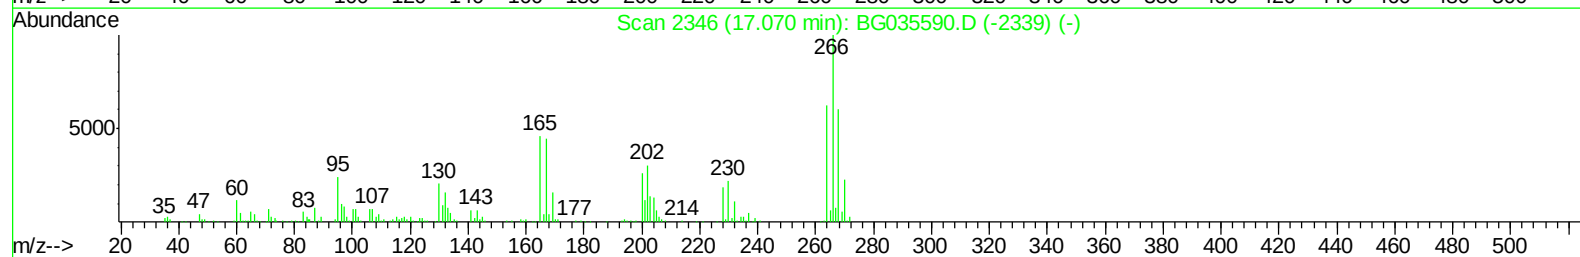
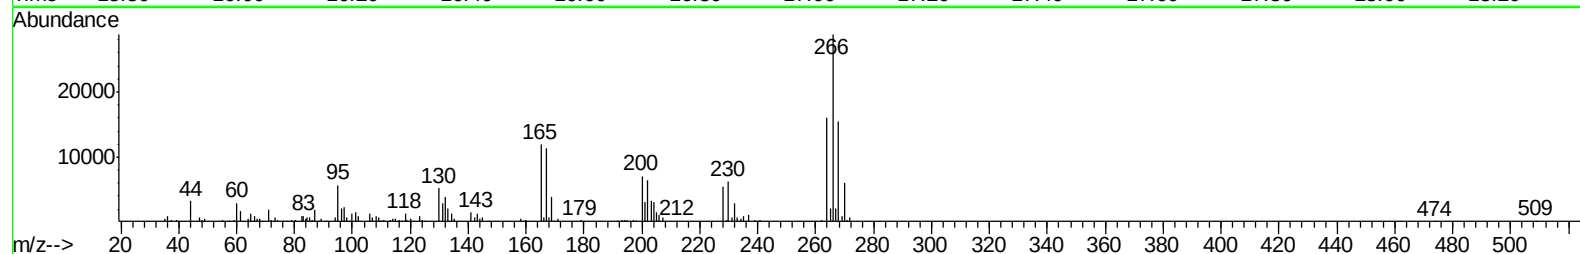


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG071218\
Data File : BG035586.D
Acq On : 12 Jul 2018 9:26
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 13 05:18:55 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 12 14:43:32 2018
Response via : Initial Calibration

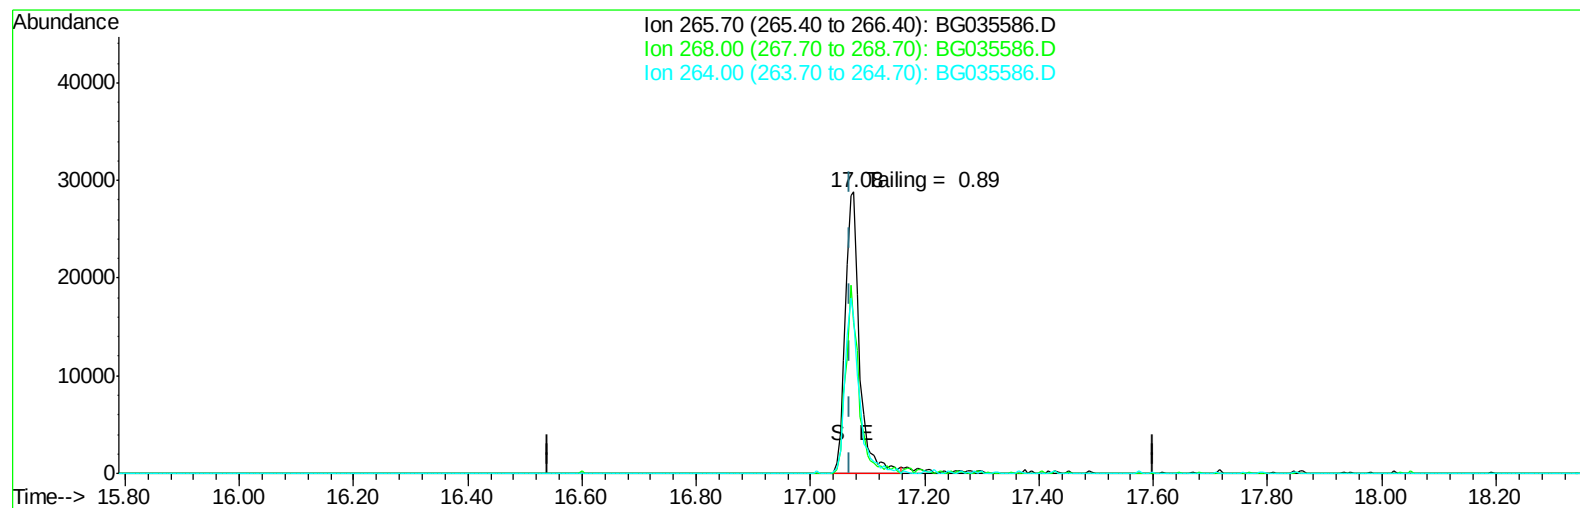

TIC: BG035586.D

(69) Pentachlorophenol (C)

17.076min (+0.006) 110582.03ng

response 49893

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	53.83
264.00	62.00	55.44
0.00	0.00	0.00

