
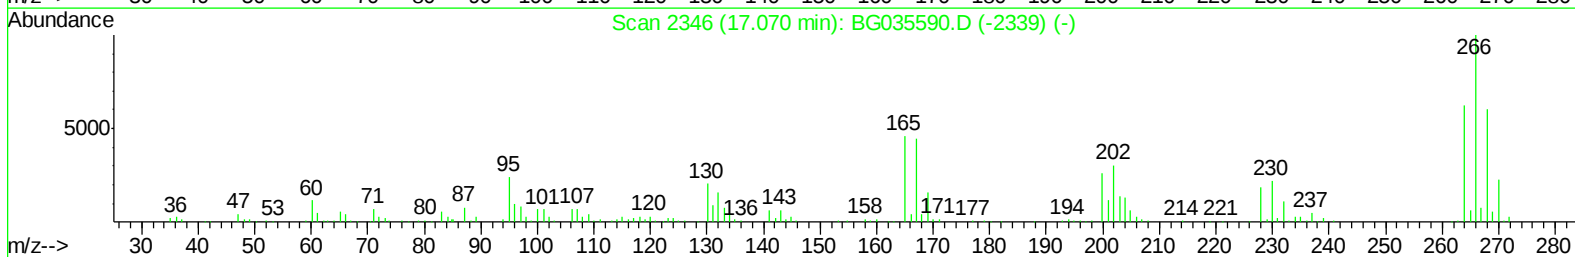
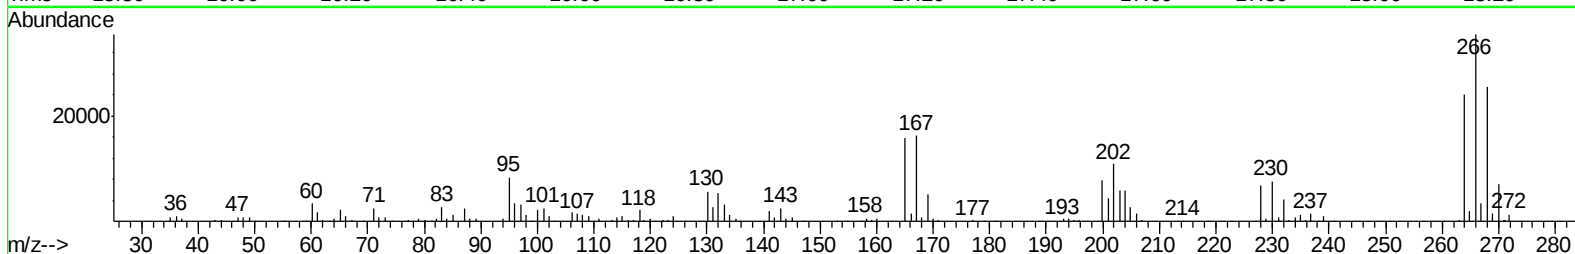


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG071218\
Data File : BG035614.D
Acq On : 13 Jul 2018 4:19
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 13 05:23:25 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 12 14:43:32 2018
Response via : Initial Calibration

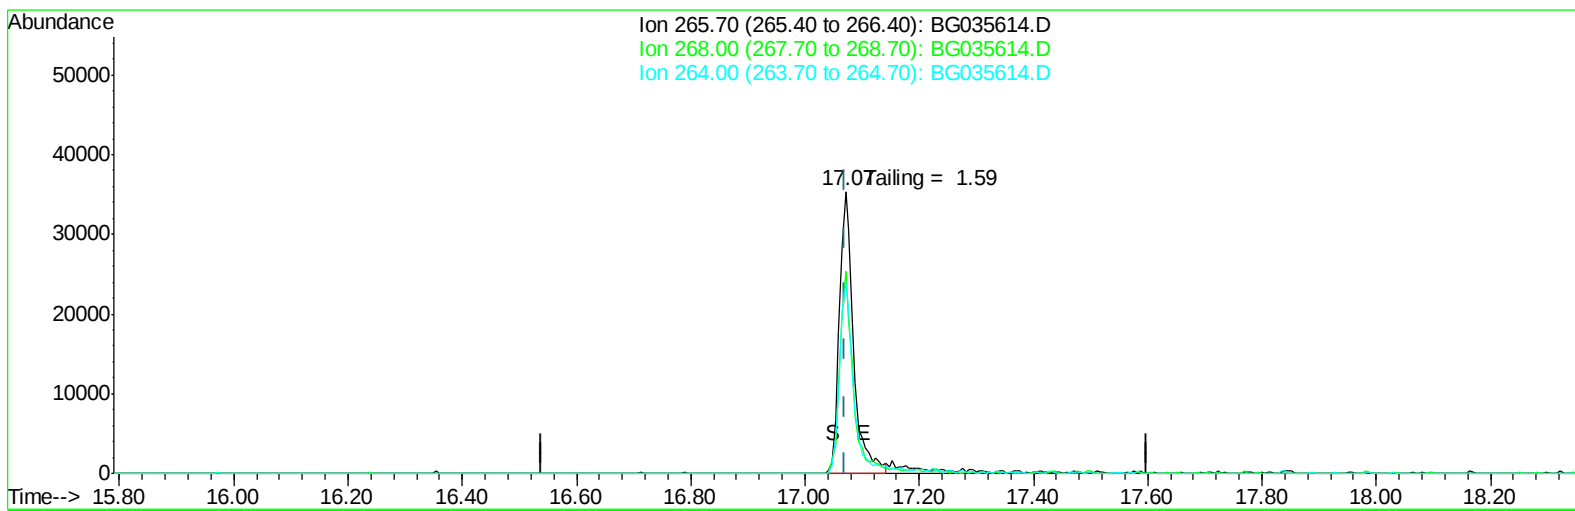

TIC: BG035614.D

(69) Pentachlorophenol (C)




17.071min (+0.001) 60030.93ng

response 60723

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	72.00
264.00	62.00	67.81
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG071218\
 Data File : BG035614.D
 Acq On : 13 Jul 2018 4:19
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 13 05:23:25 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 12 14:43:32 2018
 Response via : Initial Calibration

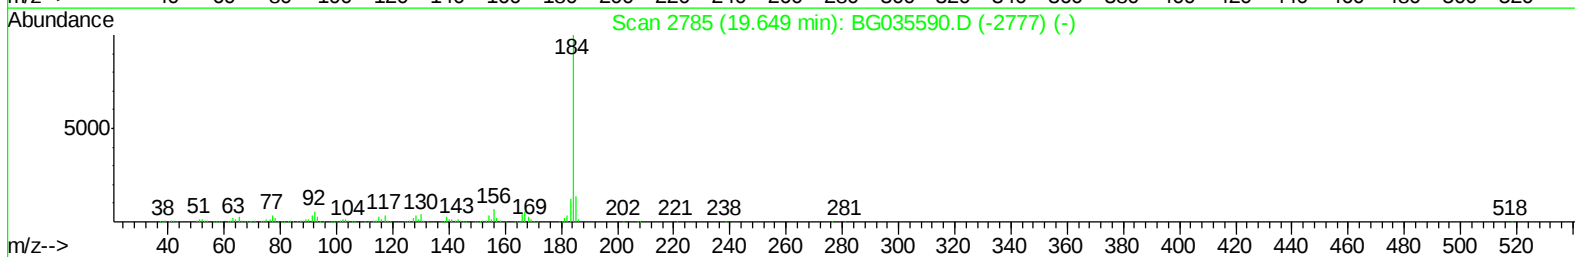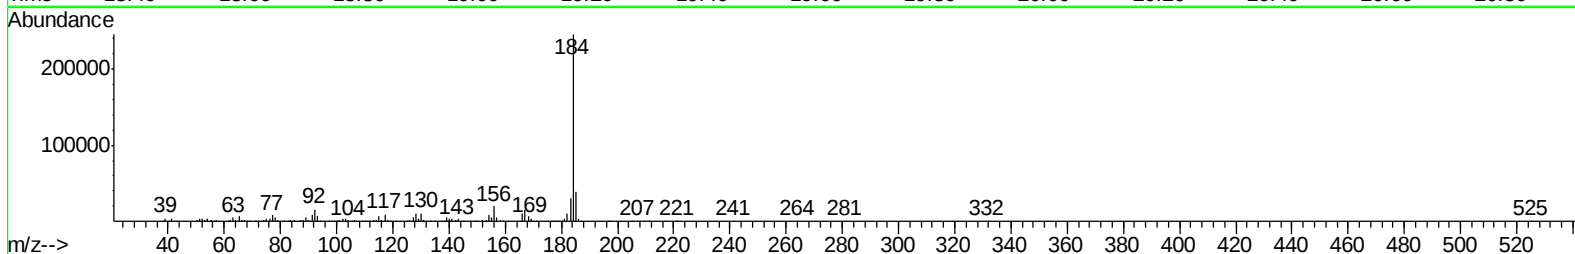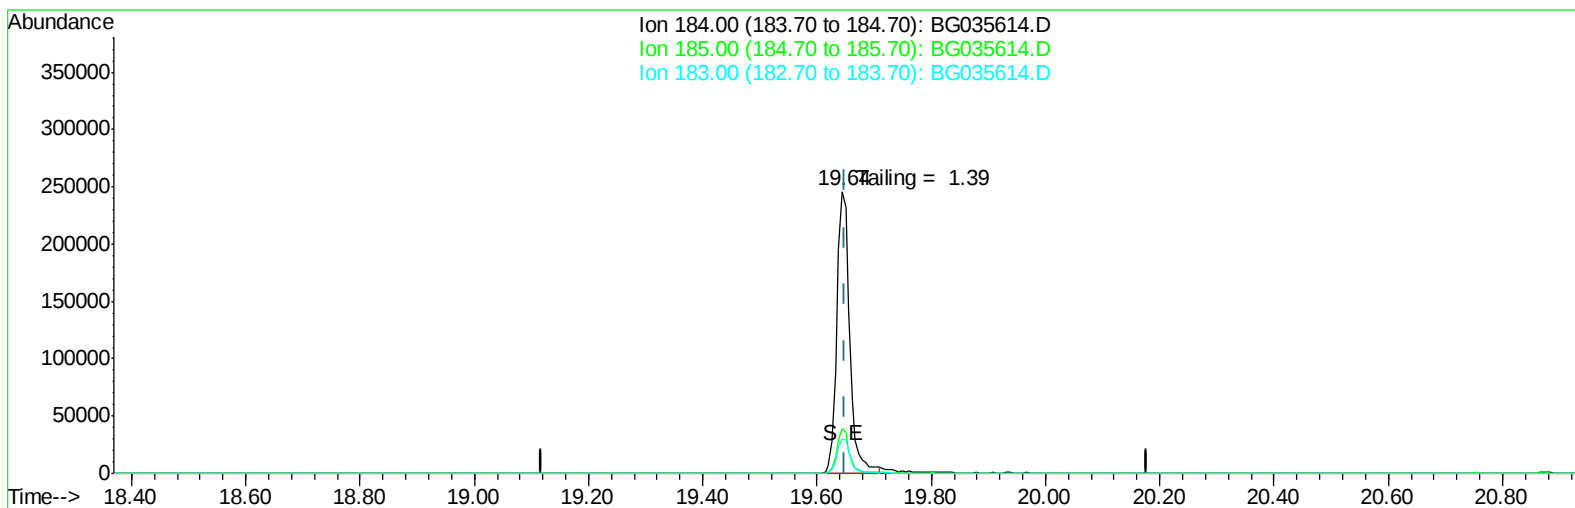

TIC: BG035614.D

(76) Benzidine

19.644min (-0.005) 28949.75ng

response 395009

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	15.76
183.00	13.30	12.22
0.00	0.00	0.00