

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG071218\
 Data File : BG035605.D
 Acq On : 12 Jul 2018 21:49
 Operator : JU/SJ
 Sample : PB110987BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB110987BL

Quant Time: Jul 13 01:56:33 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 12 14:43:32 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.06	152	52312	20.00	ng	0.00
21) Naphthalene-d8	10.86	136	198605	20.00	ng	0.00
38) Acenaphthene-d10	14.68	164	144591	20.00	ng	0.00
63) Phenanthrene-d10	17.42	188	417881	20.00	ng	0.00
75) Chrysene-d12	21.69	240	473152	20.00	ng	0.00
86) Perylene-d12	24.91	264	432698	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.64	112	400949	127.25	ng	0.00
7) Phenol-d6	7.22	99	595439	126.66	ng	0.00
23) Nitrobenzene-d5	9.22	82	374721	78.82	ng	0.00
41) 2,4,6-Tribromophenol	16.16	330	258797	135.79	ng	0.00
44) 2-Fluorobiphenyl	13.30	172	873994	80.98	ng	0.00
78) Terphenyl-d14	20.02	244	1700565	79.23	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG071218\
Data File : BG035605.D
Acq On : 12 Jul 2018 21:49
Operator : JU/SJ
Sample : PB110987BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB110987BL

Quant Time: Jul 13 01:56:33 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 12 14:43:32 2018
Response via : Initial Calibration

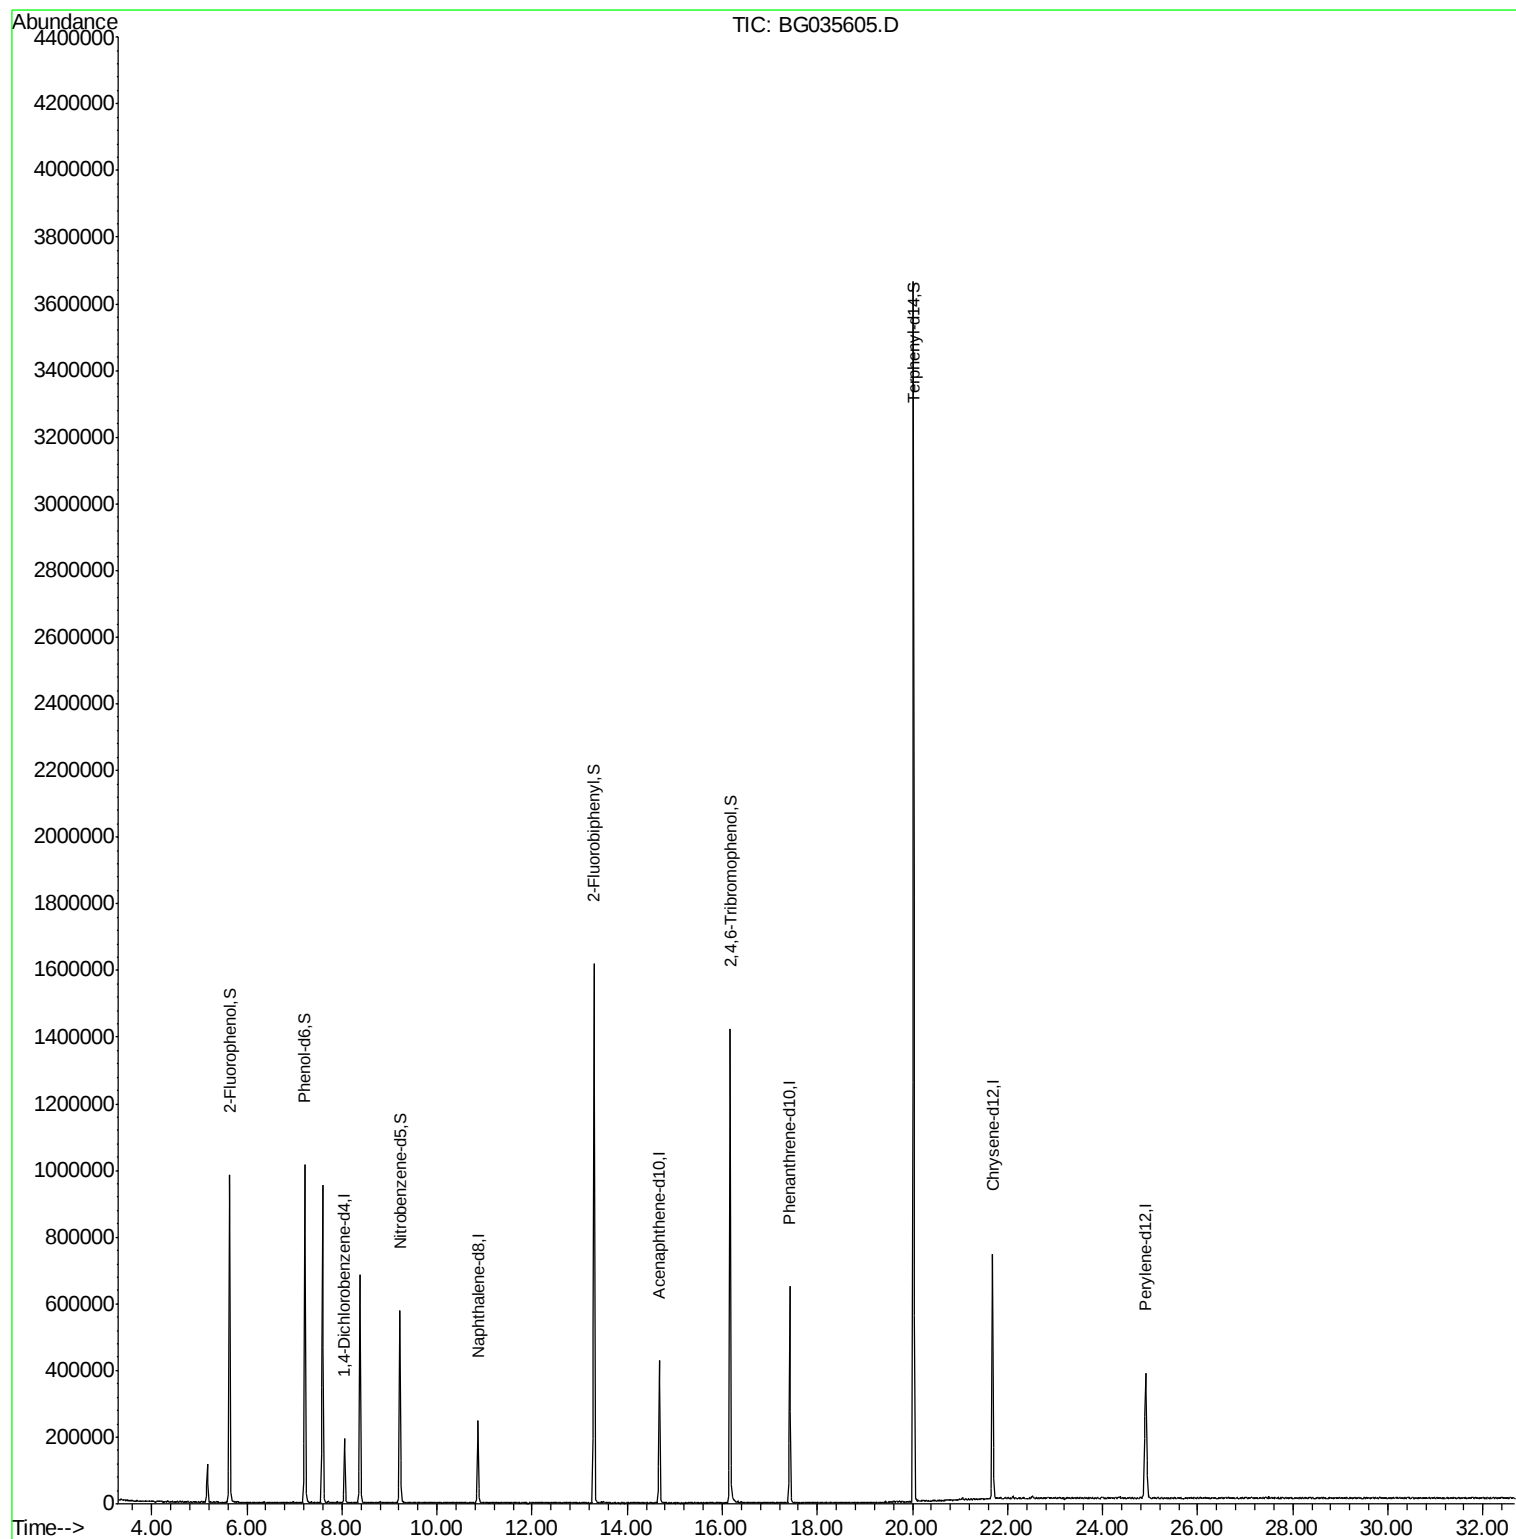

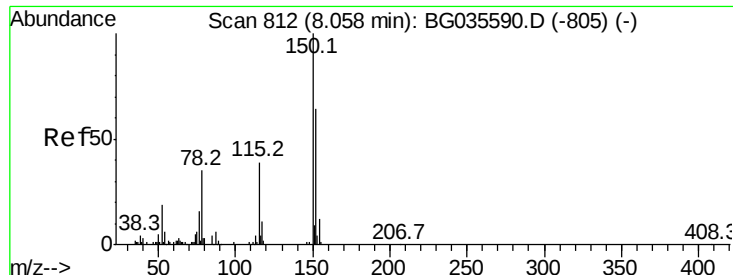

#1

1,4-Dichlorobenzene-d4

Concen: 20.000 ng

RT: 8.06 min Scan# 812

Delta R.T. -0.00 min

Lab File: BG035605.D

Acq: 12 Jul 2018 21:49

Instrument :

BNA_G

ClientSampleId :

PB110987BL


Tot Ion:152 Resp: 52312

Ion Ratio Lower Upper

152 100

150 135.7 126.6 189.8




115 61.4 53.0 79.4

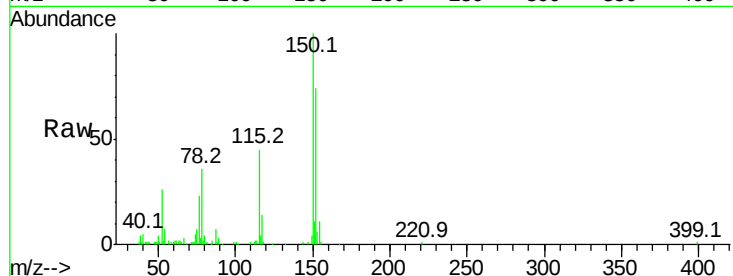

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

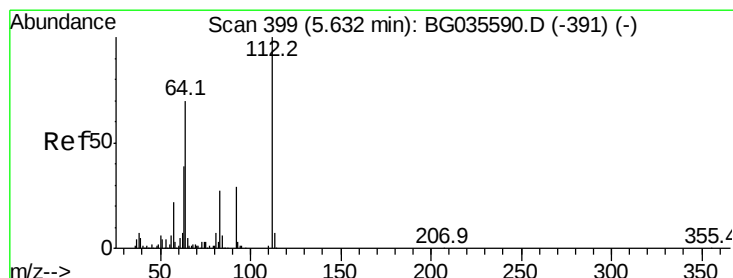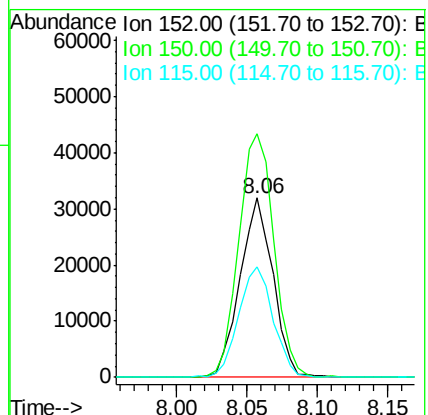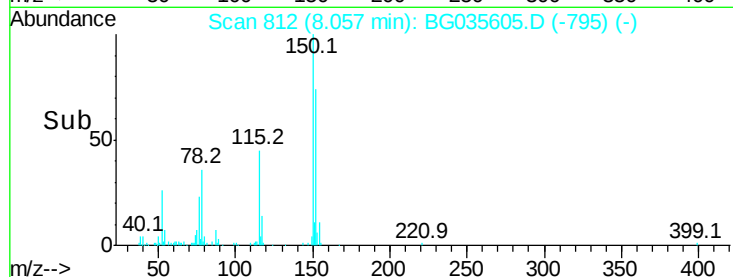

#5

2-Fluorophenol

Concen: 127.250 ng

RT: 5.64 min Scan# 400

Delta R.T. 0.00 min

Lab File: BG035605.D

Acq: 12 Jul 2018 21:49


Tgt Ion:112 Resp: 400949

Ion Ratio Lower Upper

112 100

64 68.0 56.3 84.5



63 37.5 30.1 45.1

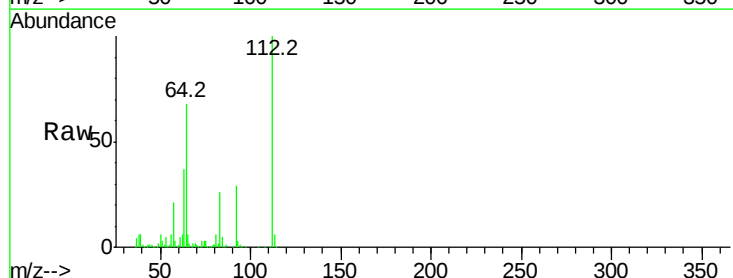

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

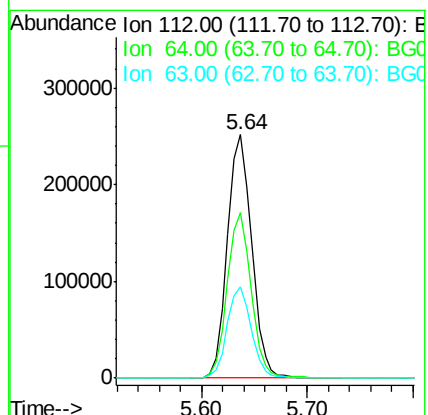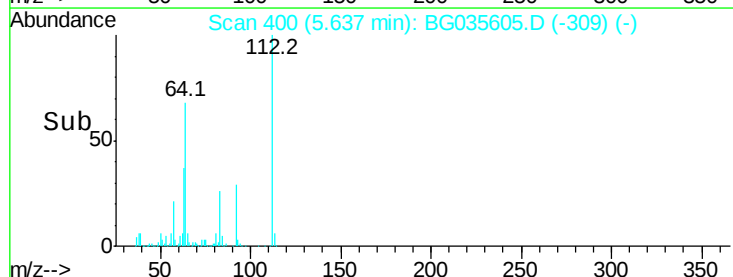



#7

Phenol-d6

Concen: 126.660 ng

RT: 7.22 min Scan# 670

Delta R.T. 0.00 min

Lab File: BG035605.D

Acq: 12 Jul 2018 21:49

Instrument :

BNA_G

ClientSampleId :

PB110987BL


Tot Ion: 99 Resp: 595439

Ion Ratio Lower Upper




99 100

42 17.7 14.1 21.1

71 42.9 26.1 39.1#

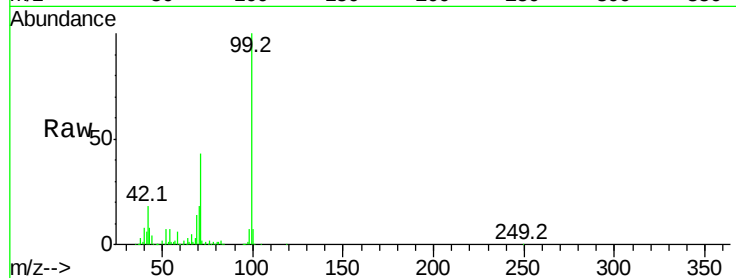

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

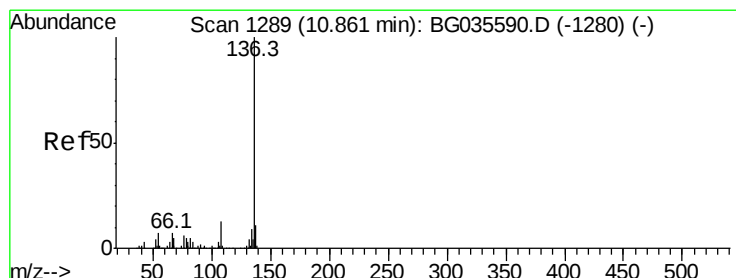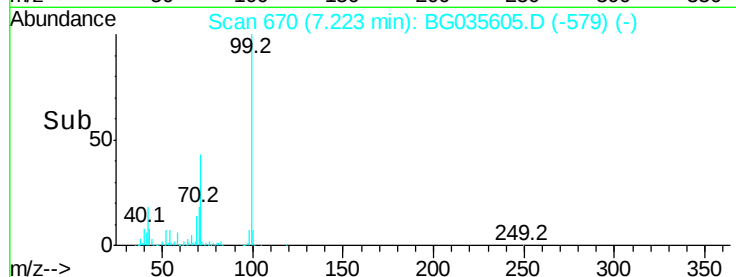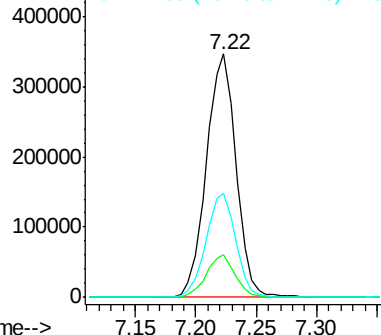

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.86 min Scan# 1289

Delta R.T. -0.00 min

Lab File: BG035605.D

Acq: 12 Jul 2018 21:49

Tgt Ion:136 Resp: 198605


Ion Ratio Lower Upper

136 100



137 11.1 9.2 13.8


54 8.1 10.3 15.5#

68 7.7 4.5 6.7#

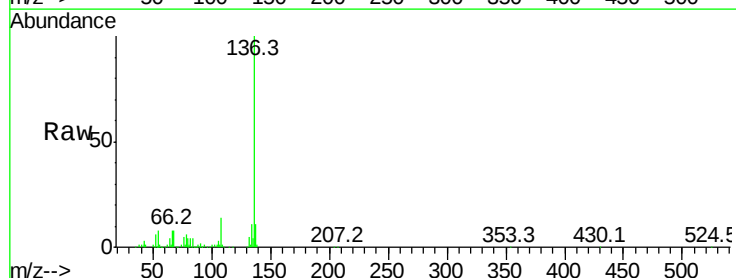

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC


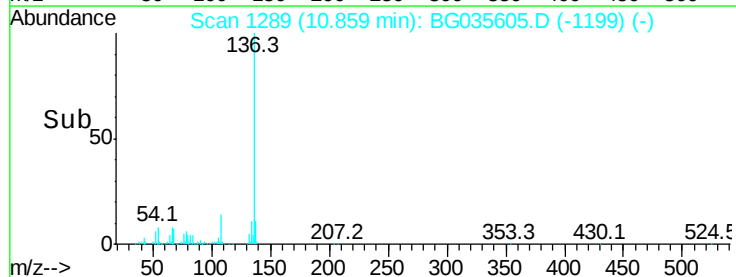
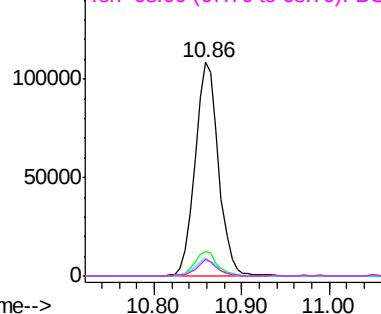


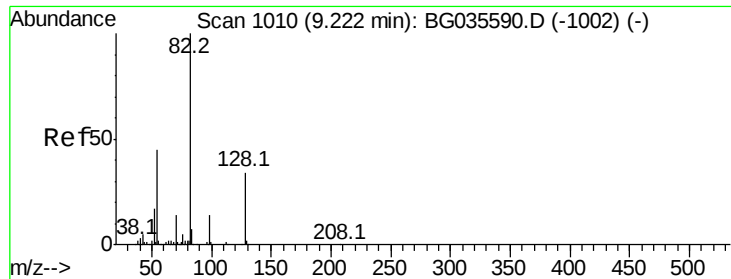

#23
Nitrobenzene-d5
Concen: 78.819 ng
RT: 9.22 min Scan# 1010
Delta R.T. -0.00 min
Lab File: BG035605.D
Acq: 12 Jul 2018 21:49




Instrument :
BNA_G
ClientSampleId :
PB110987BL

Tot Ion	Ratio	Lower	Upper
82	100		
128	34.2	29.7	44.5
54	44.0	43.1	64.7

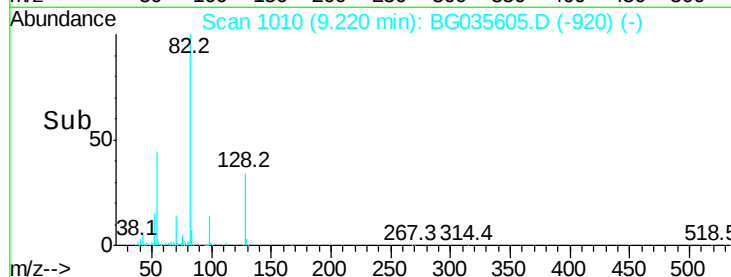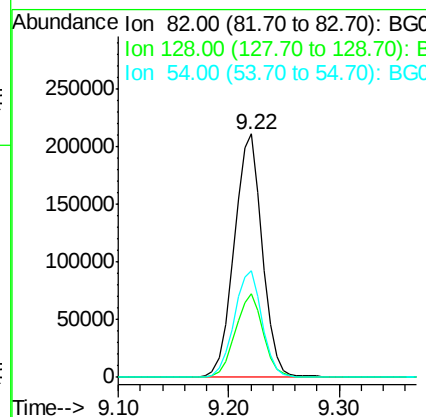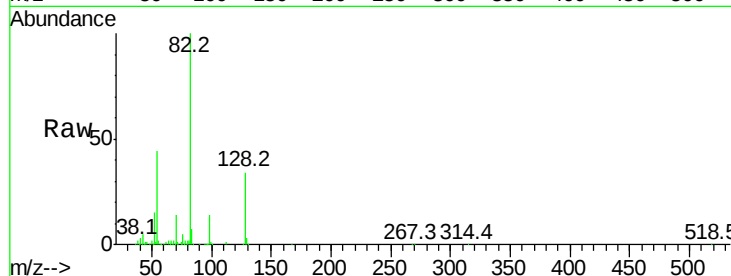

#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.68 min Scan# 1939
Delta R.T. -0.00 min
Lab File: BG035605.D
Acq: 12 Jul 2018 21:49

Tgt Ion	Ratio	Lower	Upper
164	100		
162	104.3	78.8	118.2
160	47.5	35.4	53.0


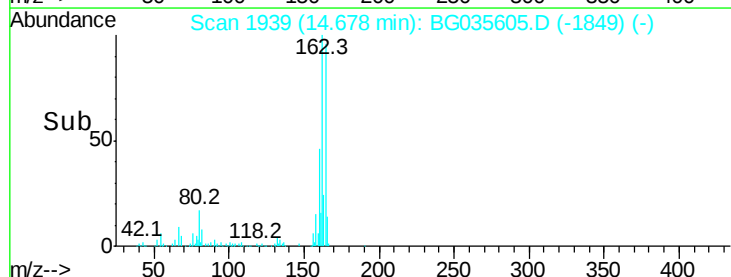
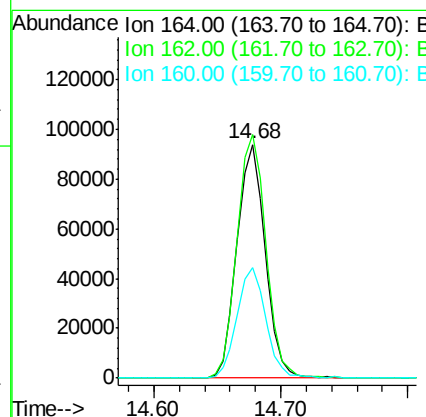
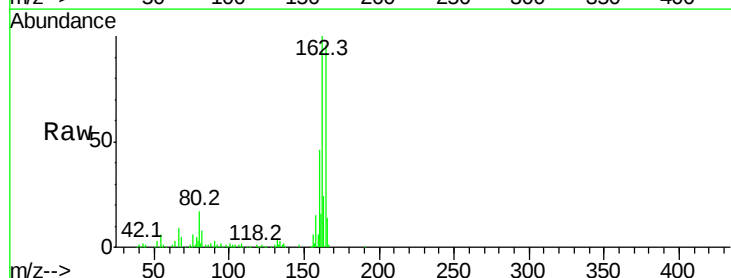




#41
 2,4,6-Tribromophenol
 Concen: 135.794 ng
 RT: 16.16 min Scan# 2192
 Delta R.T. -0.00 min
 Lab File: BG035605.D
 Acq: 12 Jul 2018 21:49




Instrument :
 BNA_G
 ClientSampleId :
 PB110987BL

Tot Ion	Ratio	Lower	Upper
330	100		
332	94.8	77.0	115.6
141	38.7	25.2	37.8#

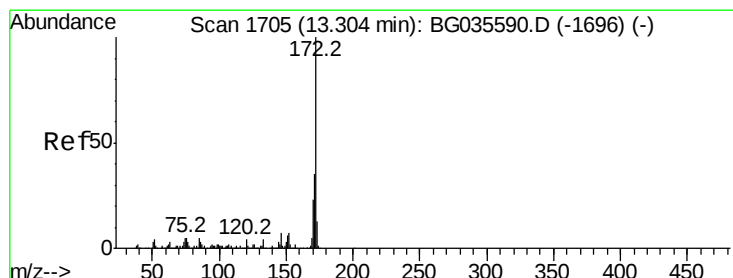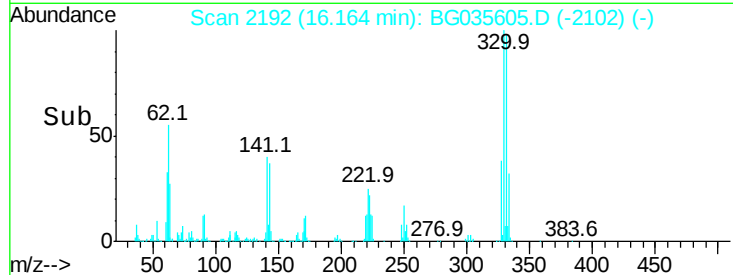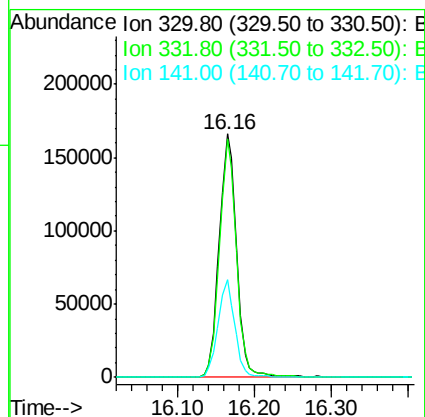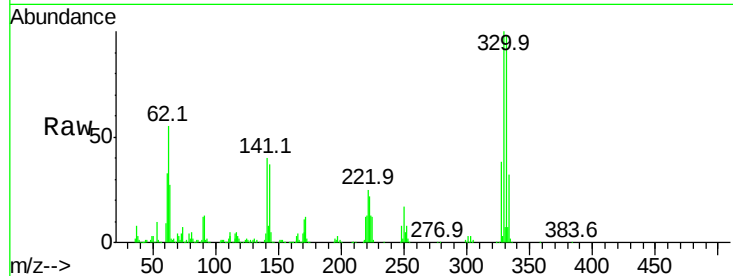

#44
 2-Fluorobiphenyl
 Concen: 80.982 ng
 RT: 13.30 min Scan# 1705
 Delta R.T. -0.00 min
 Lab File: BG035605.D
 Acq: 12 Jul 2018 21:49

Tgt Ion	Ratio	Lower	Upper
172	100		
171	34.3	30.0	45.0
170	22.5	19.5	29.3

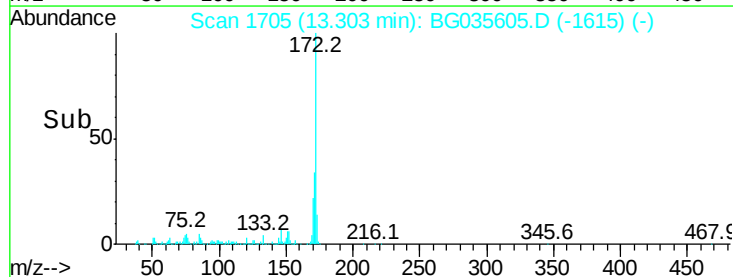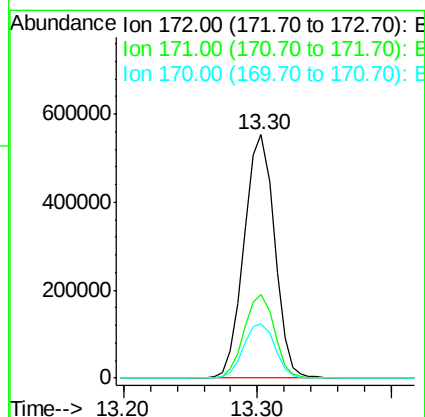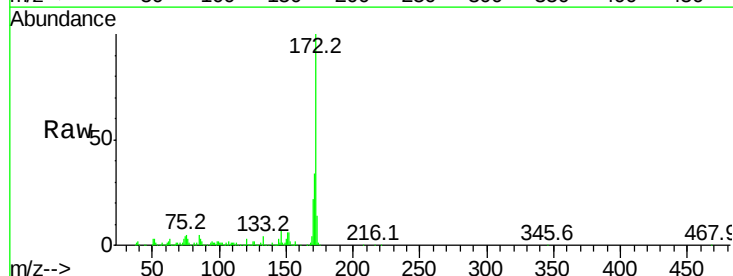



#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.42 min Scan# 2406

Delta R.T. -0.00 min

Lab File: BG035605.D

Acq: 12 Jul 2018 21:49

Instrument :

BNA_G

ClientSampleId :

PB110987BL


Tot Ion:188 Resp: 417881

Ion Ratio Lower Upper

188 100

94 6.1 6.9 10.3#



80 8.4 7.7 11.5

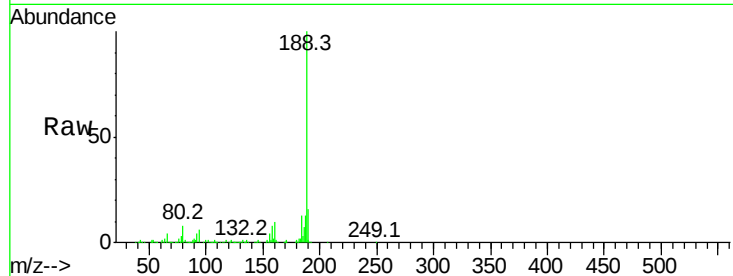

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

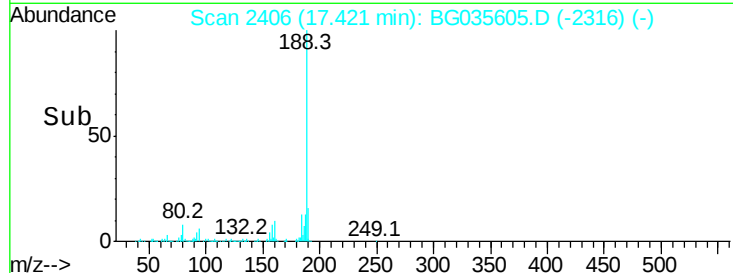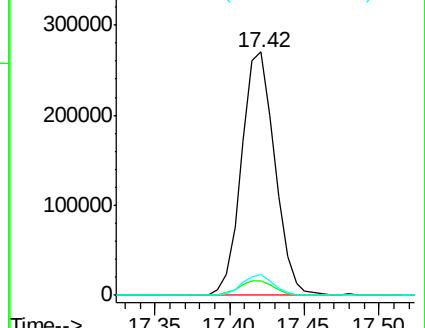

#75

Chrysene-d12

Concen: 20.000 ng

RT: 21.69 min Scan# 3132

Delta R.T. -0.00 min

Lab File: BG035605.D

Acq: 12 Jul 2018 21:49


Tgt Ion:240 Resp: 473152

Ion Ratio Lower Upper

240 100

120 5.6 6.8 10.2#



236 25.5 20.9 31.3

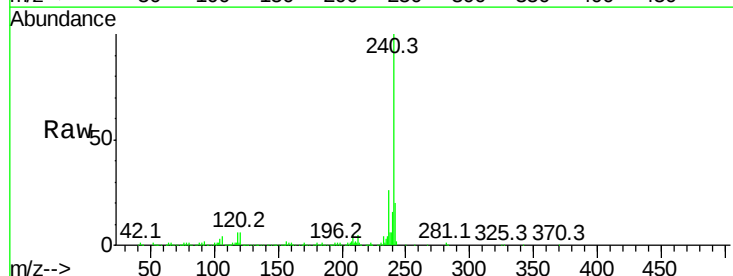


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

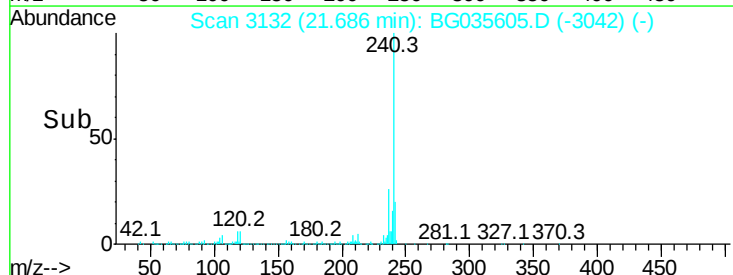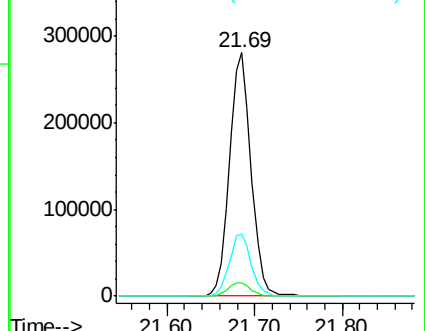

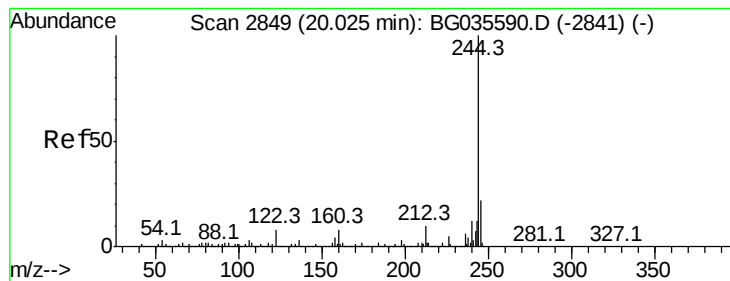

#78

Terphenyl-d14

Concen: 79.225 ng

RT: 20.02 min Scan# 2849

Delta R.T. -0.00 min

Lab File: BG035605.D

Acq: 12 Jul 2018 21:49

Instrument :

BNA_G

ClientSampleId :

PB110987BL


Tot Ion:244 Resp: 1700565

Ion Ratio Lower Upper

244 100

212 10.2 5.8 8.8#




122 7.5 7.0 10.4

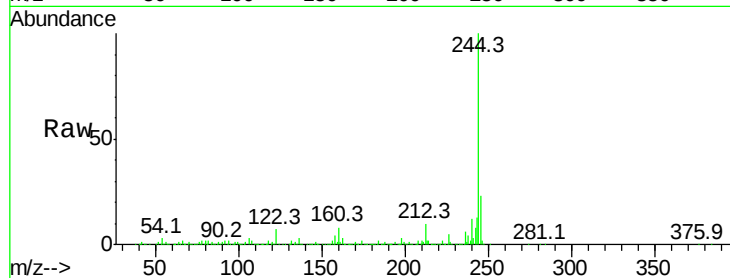

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

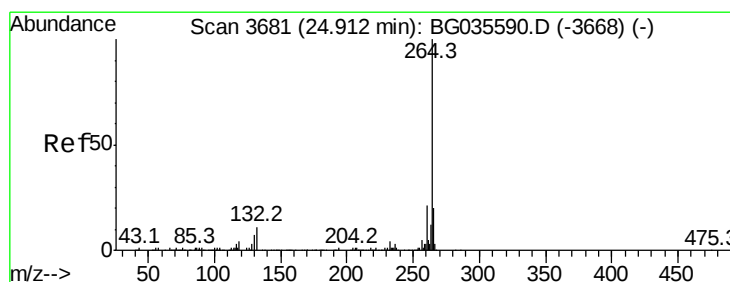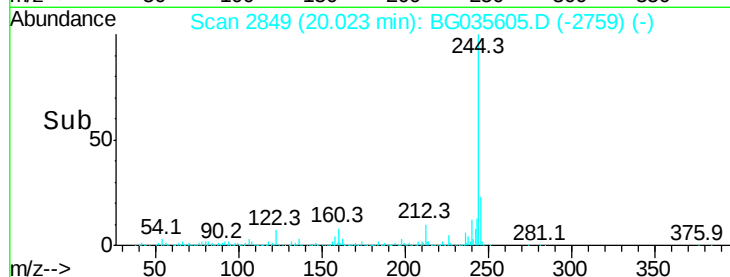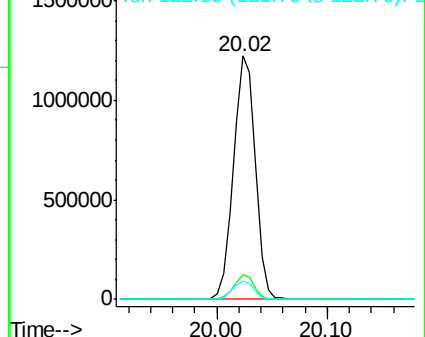

#86

Perylene-d12

Concen: 20.000 ng

RT: 24.91 min Scan# 3681

Delta R.T. -0.00 min

Lab File: BG035605.D

Acq: 12 Jul 2018 21:49


Tgt Ion:264 Resp: 432698

Ion Ratio Lower Upper

264 100

260 22.5 17.4 26.0

265 20.3 17.7 26.5

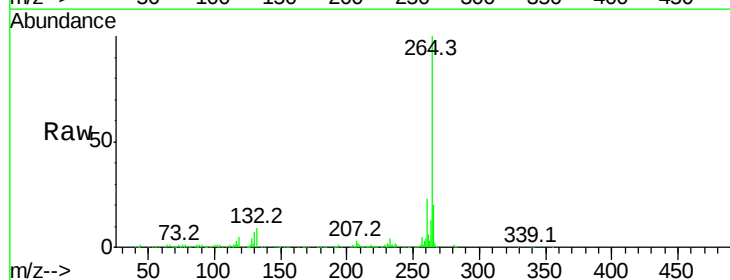

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

