


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071218\
 Data File : BG035586.D
 Acq On : 12 Jul 2018 9:26
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 31 12:30:06 2018

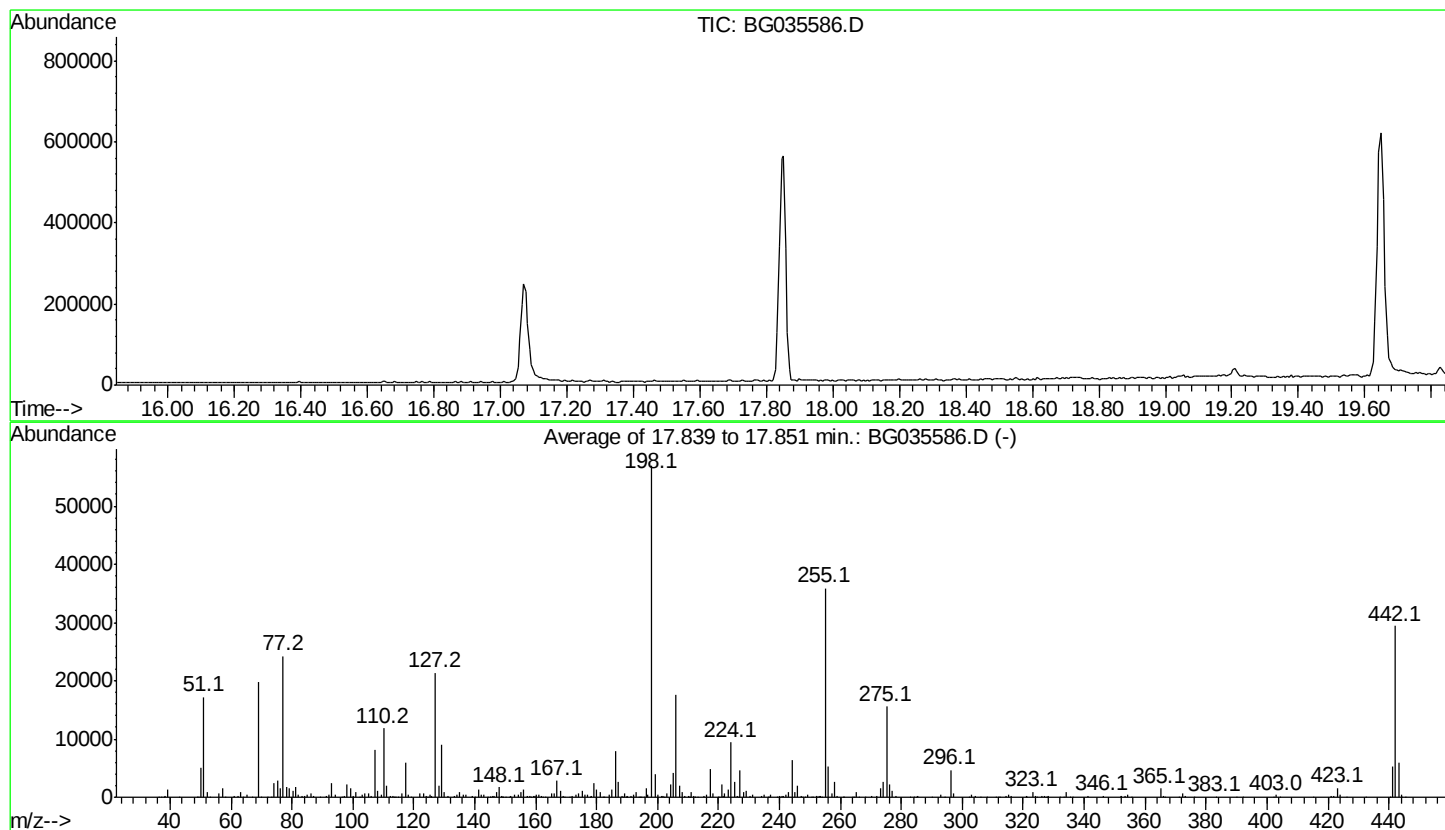

AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.1	17145	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	34.9	19878	PASS
70	69	0.00	2	0.6	112	PASS
127	198	10	80	37.5	21380	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	56938	PASS
199	198	5	9	6.9	3941	PASS
275	198	10	60	27.4	15596	PASS
365	198	1	100	2.6	1490	PASS
441	198	0.01	100	9.1	5183	PASS
442	198	50	100	51.6	29374	PASS
443	442	15	24	20.3	5953	PASS