


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG071218\
 Data File : BG035595.D
 Acq On : 12 Jul 2018 15:21
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 31 12:30:06 2018

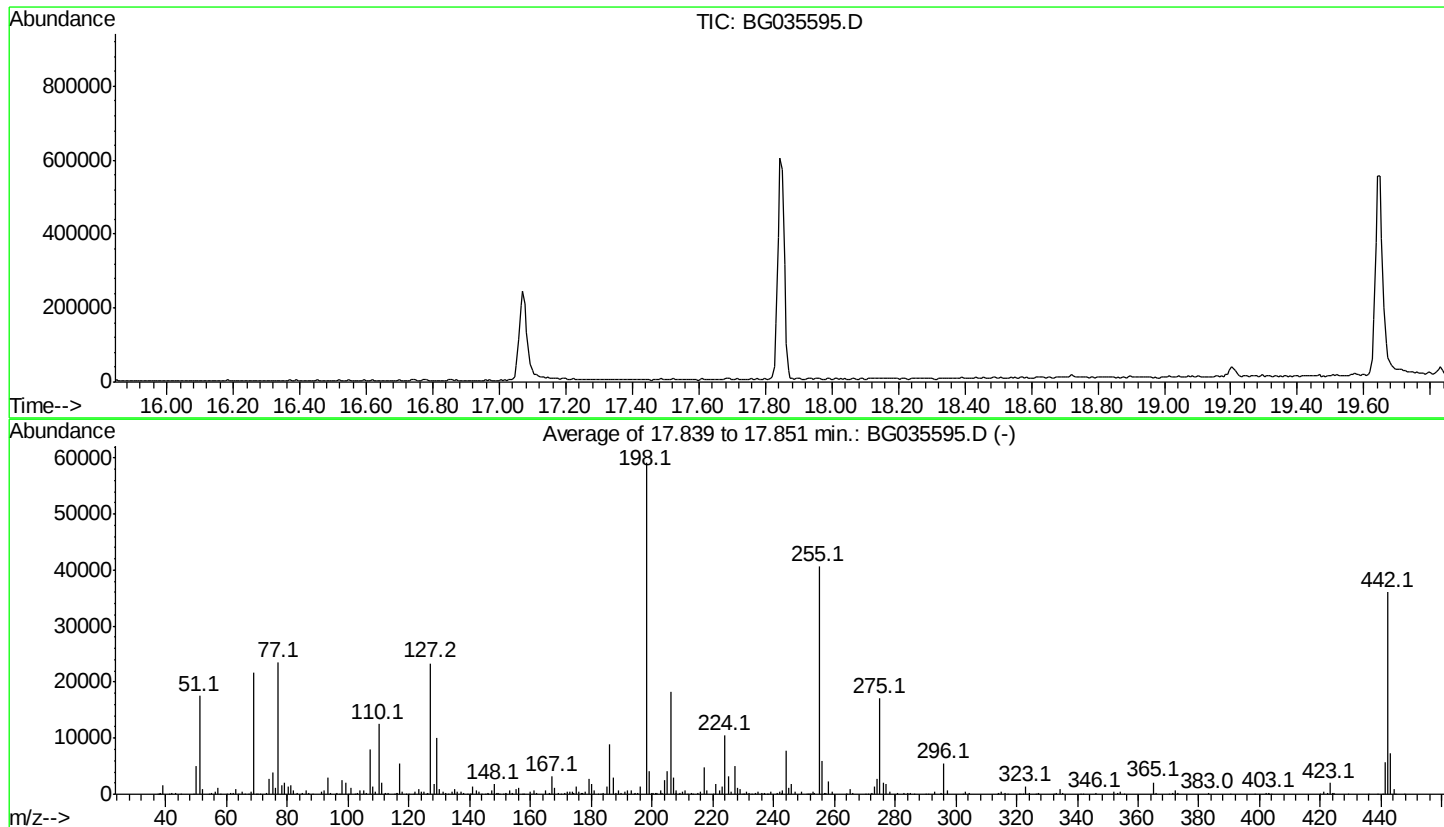

AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.7	17570	PASS
68	69	0.00	2	2.0	426	PASS
69	198	0.00	100	36.5	21599	PASS
70	69	0.00	2	0.4	78	PASS
127	198	10	80	39.5	23349	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	59162	PASS
199	198	5	9	7.0	4131	PASS
275	198	10	60	28.9	17088	PASS
365	198	1	100	3.6	2159	PASS
441	198	0.01	100	9.5	5623	PASS
442	198	50	100	60.9	36040	PASS
443	442	15	24	20.5	7379	PASS