
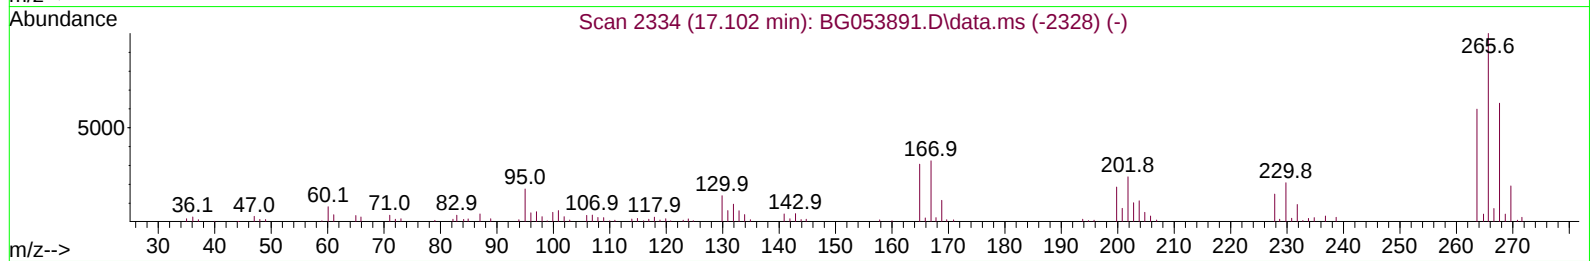
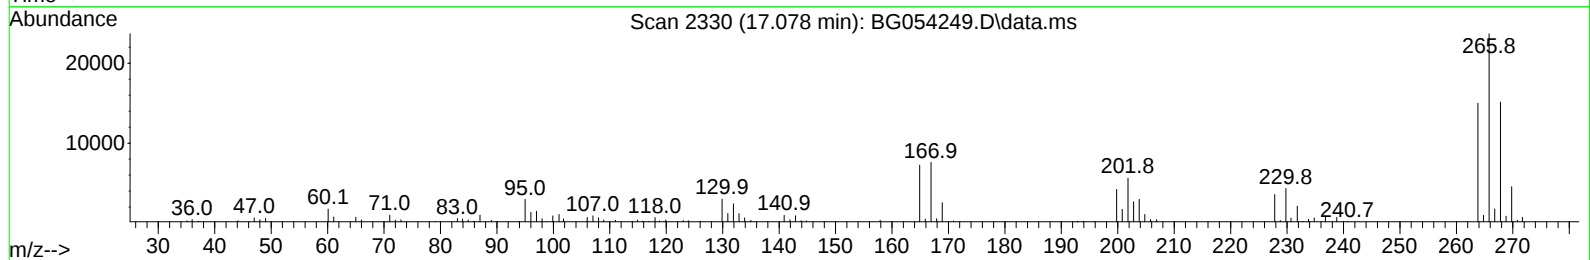


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071222\
Data File : BG054249.D
Acq On : 12 Jul 2022 10:00
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 12 11:32:36 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 12 11:27:58 2022
Response via : Initial Calibration

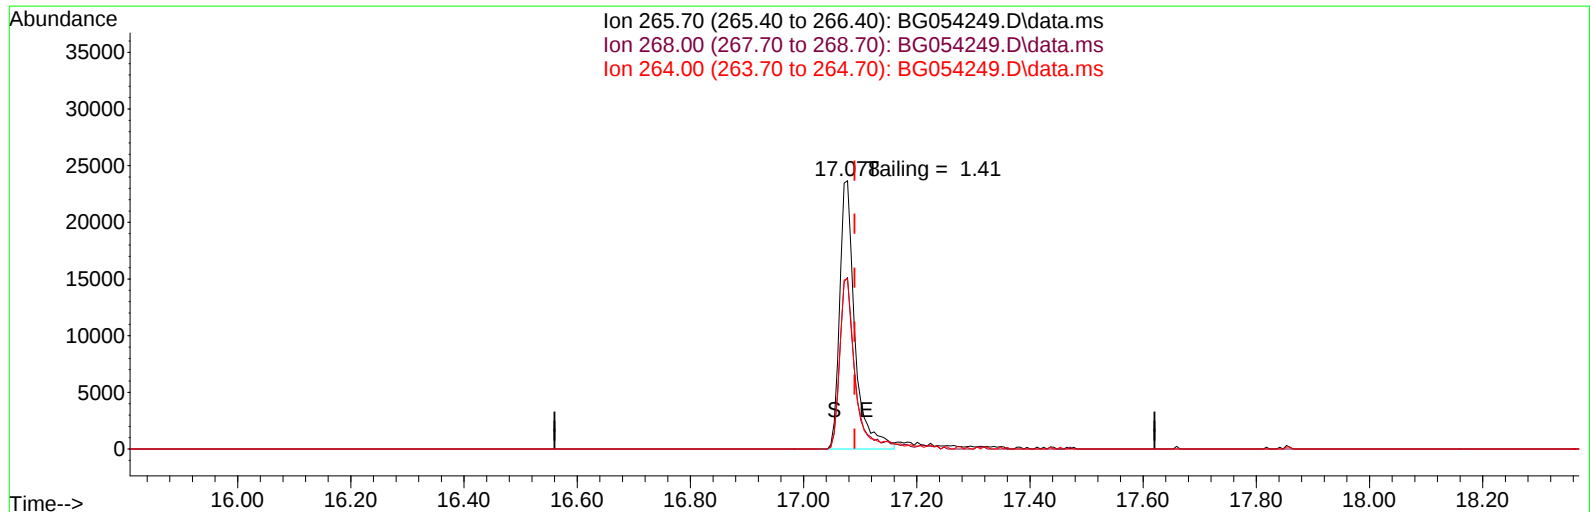

TIC: BG054249.D\data.ms

(70) Pentachlorophenol (C)




17.078min (-0.012) 32819.55 ng

response 44432

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	63.90
264.00	66.20	63.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071222\
Data File : BG054249.D
Acq On : 12 Jul 2022 10:00
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 12 11:32:36 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 12 11:27:58 2022
Response via : Initial Calibration

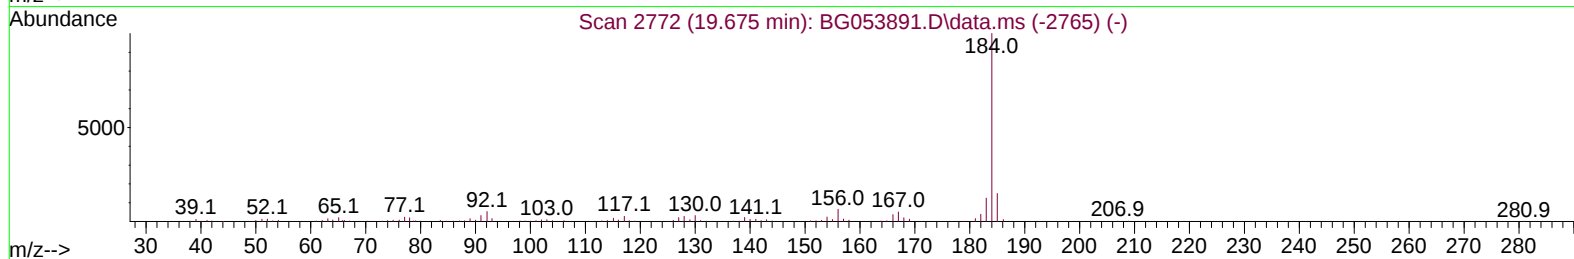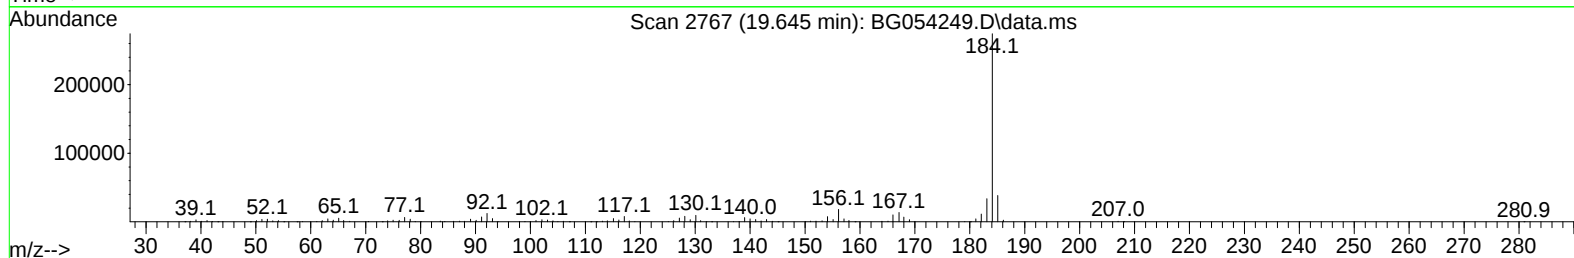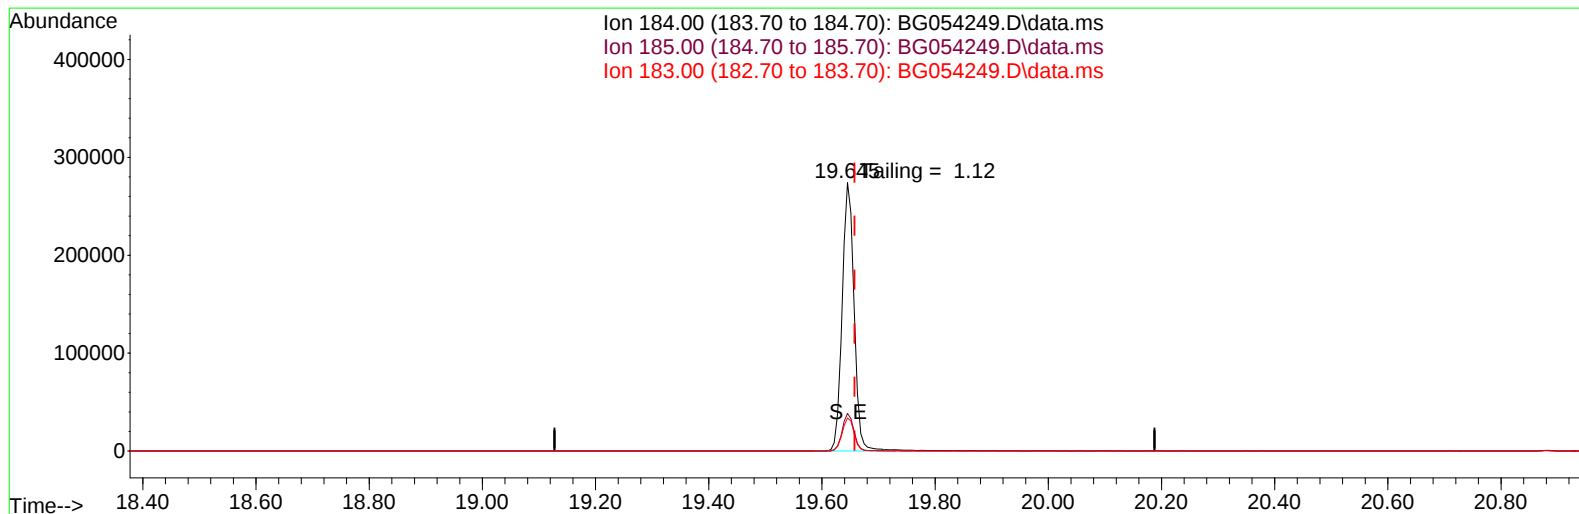

TIC: BG054249.D\data.ms

(77) Benzidine

19.645min (-0.012) 0.00 ng

response 402683

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.01
183.00	11.10	12.29
0.00	0.00	0.00