
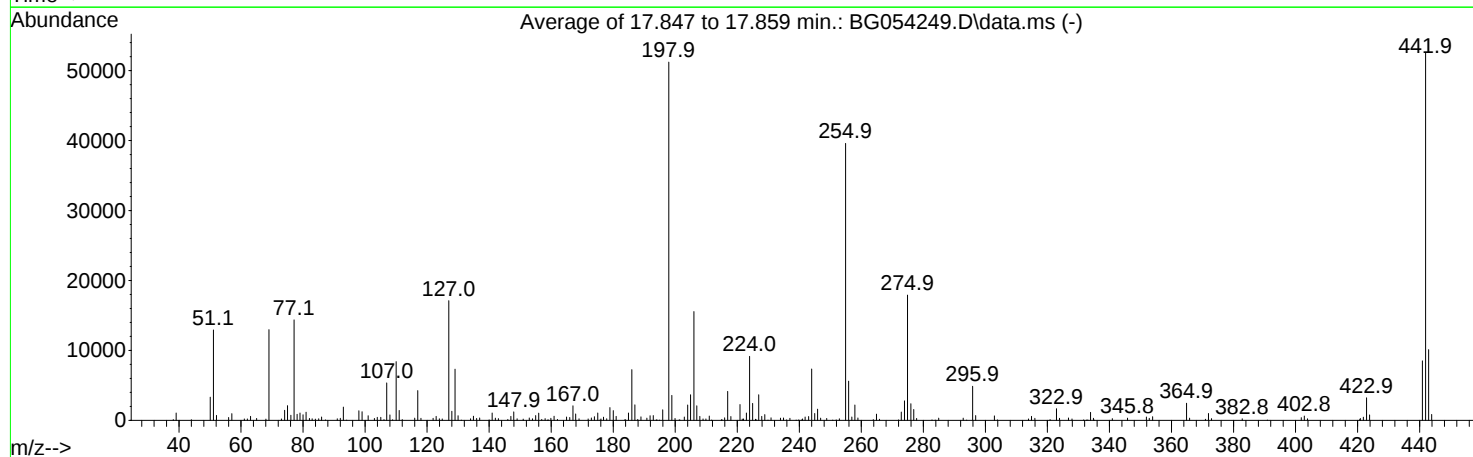


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071222\
 Data File : BG054249.D
 Acq On : 12 Jul 2022 10:00
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 12 15:49:20 2022

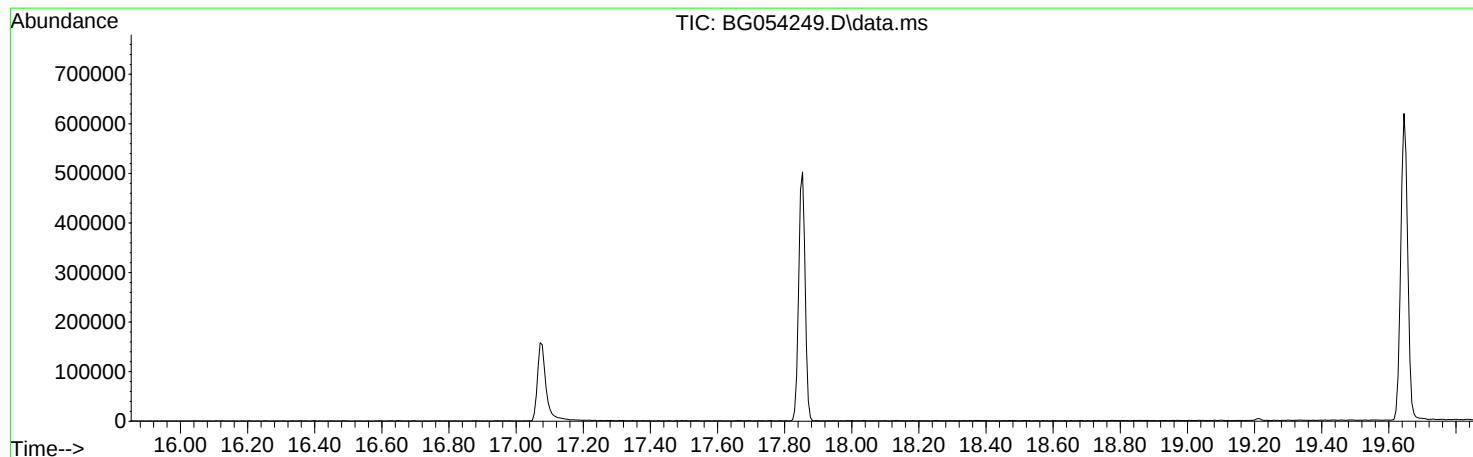

AutoFind: Scans 2461, 2462, 2463; Background Corrected with Scan 2454

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.2	12927	PASS
68	69	0.00	2	1.4	187	PASS
69	198	0.00	100	25.3	12976	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	33.4	17113	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	51219	PASS
199	198	5	9	7.0	3565	PASS
275	198	10	60	35.0	17916	PASS
365	198	1	100	4.8	2447	PASS
441	198	0.01	100	16.6	8510	PASS
442	442	50	100	100.0	52589	PASS
443	442	15	24	19.2	10106	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/12/2022	BNA_G	<u>BG054249.D</u>
Compound Name	Response	Retention Time
DDT	223621	20.87
DDD	654	20.43
DDE	0	19.93
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
654	224275	0.29

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071222\
Data File : BG054249.D
Acq On : 12 Jul 2022 10:00
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jul 12 11:32:36 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 12 11:27:58 2022
Response via : Initial Calibration

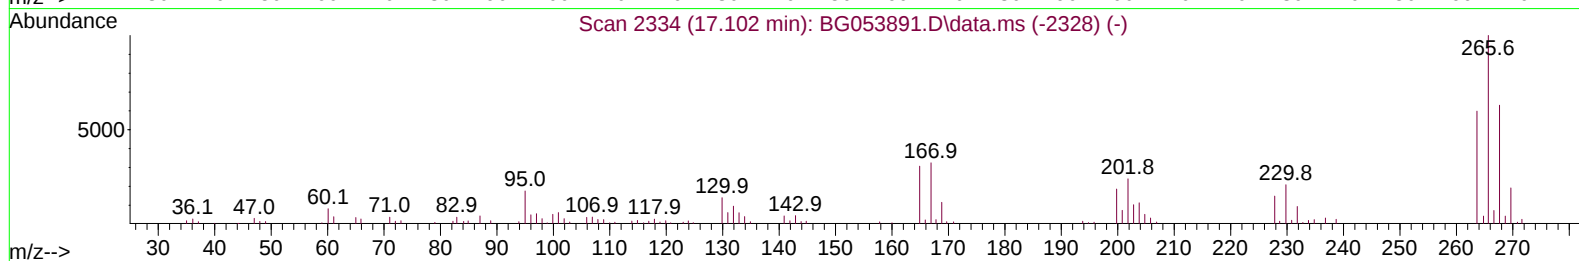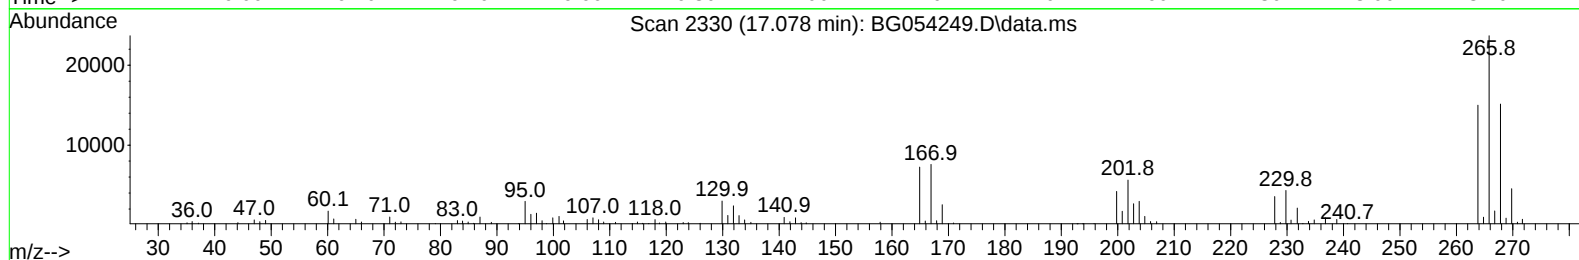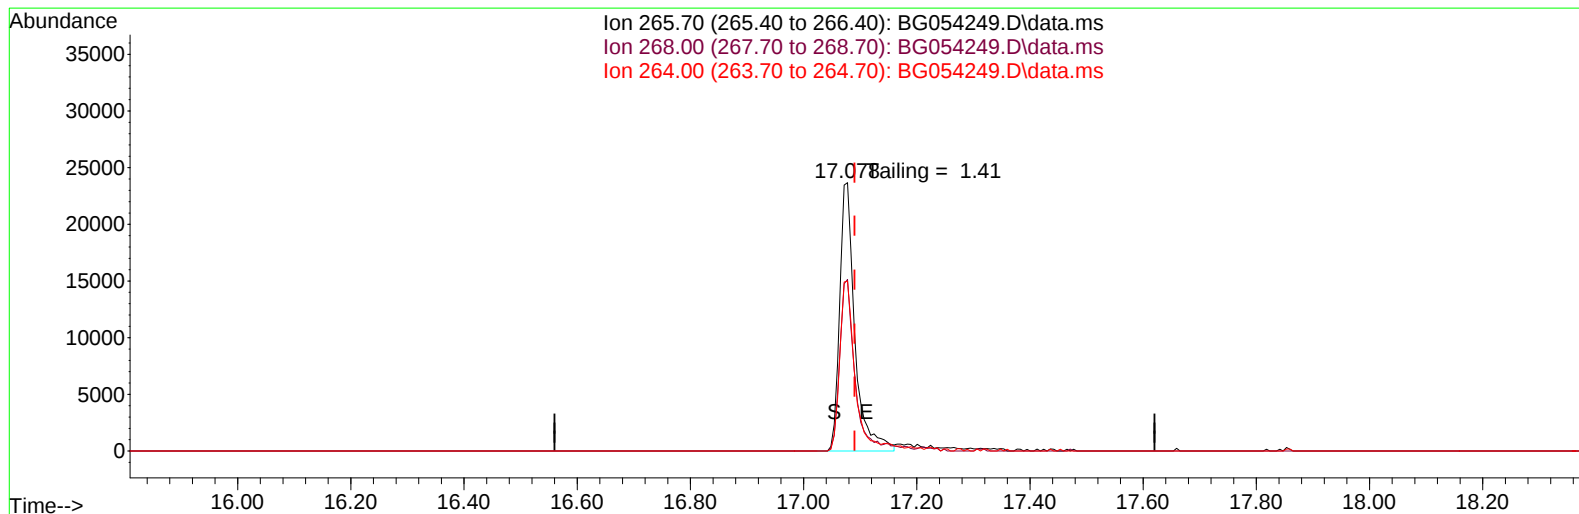

TIC: BG054249.D\data.ms

(70) Pentachlorophenol (C)

17.078min (-0.012) 32819.55 ng




response 44432

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	63.90
264.00	66.20	63.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071222\
Data File : BG054249.D
Acq On : 12 Jul 2022 10:00
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jul 12 11:32:36 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 12 11:27:58 2022
Response via : Initial Calibration

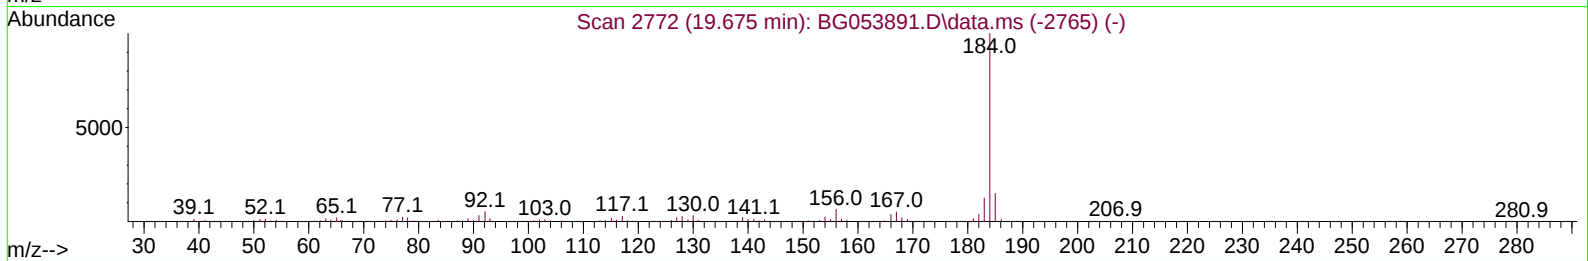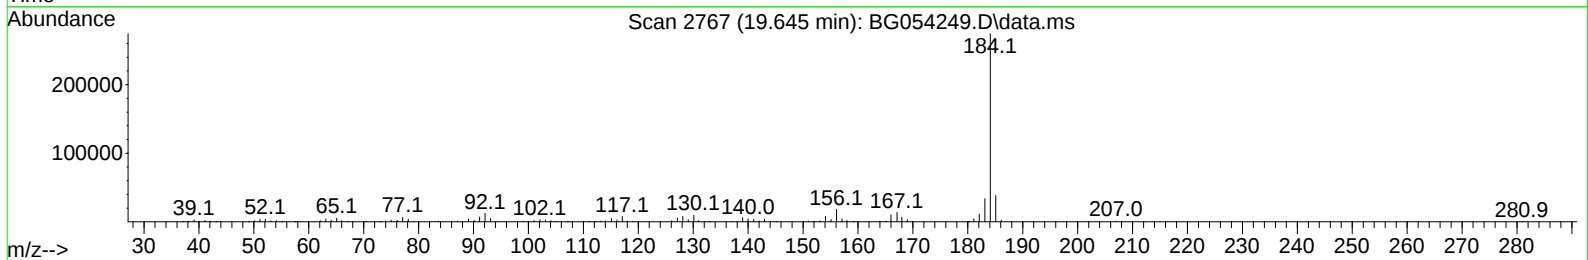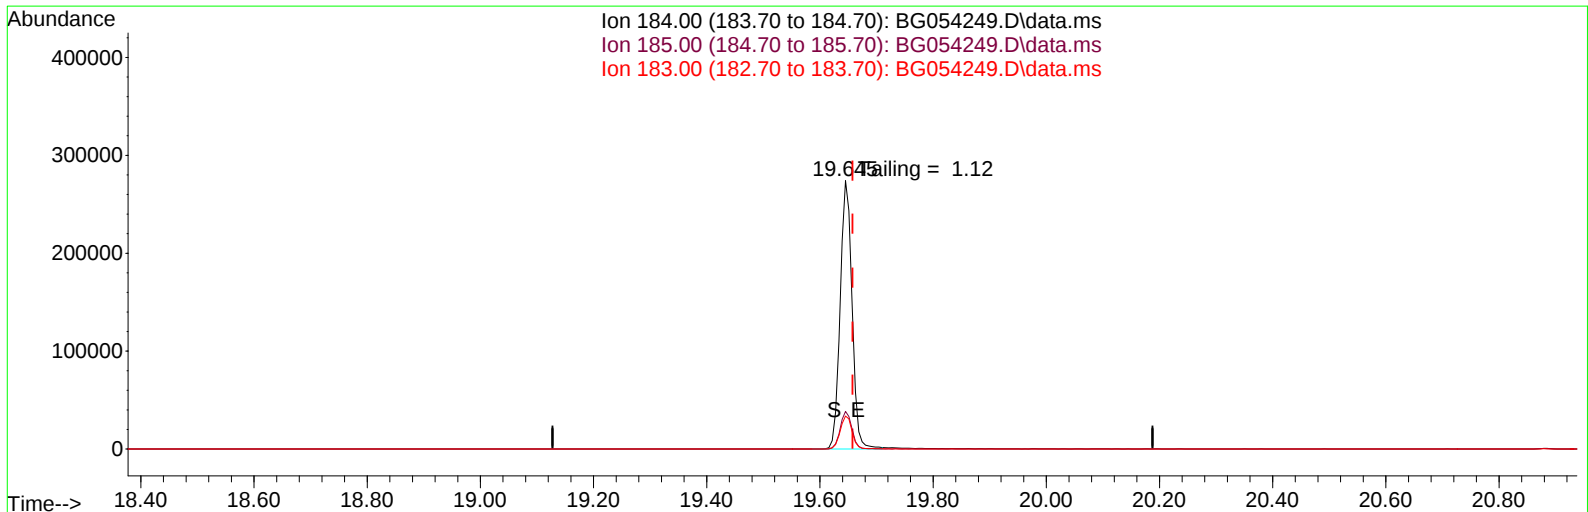

TIC: BG054249.D\data.ms

(77) Benzidine

19.645min (-0.012) 0.00 ng

response 402683

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.01
183.00	11.10	12.29
0.00	0.00	0.00