

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071224\
 Data File : BG062050.D
 Acq On : 12 Jul 2024 21:24
 Operator : MA/JU
 Sample : P3137-11
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 YDZE4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG062050.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.441	23	26	28	rBV2	9109	10707	0.47%	0.053%
2	3.635	57	59	61	rVB2	4587	3117	0.14%	0.015%
3	3.688	66	68	70	rBV2	4174	4333	0.19%	0.021%
4	3.782	81	84	86	rBV	5264	3709	0.16%	0.018%
5	3.858	93	97	104	rBV2	58115	93596	4.10%	0.464%
6	4.152	144	147	149	rVB3	3303	3374	0.15%	0.017%
7	4.205	152	156	160	rVB2	5755	7052	0.31%	0.035%
8	4.281	166	169	170	rBV	3908	3757	0.16%	0.019%
9	4.581	218	220	224	rBV2	2703	3096	0.14%	0.015%
10	4.687	235	238	241	rBV6	3009	4272	0.19%	0.021%
11	4.763	247	251	252	rBV3	2868	3085	0.14%	0.015%
12	5.121	310	312	321	rVB3	4090	6550	0.29%	0.032%
13	5.315	341	345	346	rBV2	4509	5364	0.24%	0.027%
14	5.351	349	351	355	rVB2	2990	3769	0.17%	0.019%
15	5.638	398	400	404	rVB	4379	4082	0.18%	0.020%
16	5.721	413	414	416	rBV	4717	3789	0.17%	0.019%
17	6.191	492	494	496	rBV	3075	2957	0.13%	0.015%
18	6.714	580	583	584	rBV	3285	3063	0.13%	0.015%
19	6.778	591	594	596	rBV	3094	3693	0.16%	0.018%
20	6.808	598	599	603	rVB2	3353	3335	0.15%	0.017%
21	7.013	628	634	635	rBV2	4254	6370	0.28%	0.032%
22	7.066	642	643	645	rBV	3117	3136	0.14%	0.016%
23	7.119	651	652	654	rBV2	3928	3366	0.15%	0.017%
24	7.195	659	665	675	rVB	72230	129614	5.68%	0.643%
25	7.366	687	694	703	rVB	165906	295159	12.93%	1.464%
26	7.571	722	729	738	rBV	220314	384932	16.87%	1.909%
27	7.736	755	757	762	rVB2	3015	3429	0.15%	0.017%
28	7.789	762	766	767	rVB3	3068	3485	0.15%	0.017%
29	8.041	801	809	817	rBV	212319	367892	16.12%	1.825%
30	8.130	820	824	826	rVB	3829	4285	0.19%	0.021%
31	8.177	826	832	834	rBV2	3430	4670	0.20%	0.023%
32	8.400	866	870	871	rBV	3980	3594	0.16%	0.018%
33	8.547	894	895	898	rBV	4010	4691	0.21%	0.023%
34	8.570	898	899	903	rVV2	4046	4127	0.18%	0.020%
35	8.623	905	908	911	rBV2	5152	6902	0.30%	0.034%
36	8.694	917	920	922	rBV	3664	4583	0.20%	0.023%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071224\
 Data File : BG062050.D
 Acq On : 12 Jul 2024 21:24
 Operator : MA/JU
 Sample : P3137-11
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 YDZE4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
 Title : SVOA CALIBRATION

37	8.747	922	929	938	rVB2	194355	337241	14.78%	1.673%
38	8.940	959	962	963	rBV2	3261	3098	0.14%	0.015%
39	9.205	1000	1007	1018	rBV	259556	477809	20.94%	2.370%
40	9.651	1078	1083	1084	rBV	2961	3438	0.15%	0.017%
41	9.927	1123	1130	1138	rBV2	256511	453026	19.85%	2.247%
42	10.468	1215	1222	1232	rBV	334729	596876	26.16%	2.960%
43	10.850	1281	1287	1294	rBV	294256	523383	22.94%	2.596%
44	10.985	1302	1310	1319	rBV2	267120	495927	21.73%	2.460%
45	11.103	1328	1330	1332	rVB	4571	3183	0.14%	0.016%
46	11.232	1349	1352	1357	rVB	4099	6742	0.30%	0.033%
47	11.449	1386	1389	1392	rVB	2702	3635	0.16%	0.018%
48	11.661	1415	1425	1432	rBV7	14611	36949	1.62%	0.183%
49	11.796	1445	1448	1451	rVB	3263	2954	0.13%	0.015%
50	12.131	1502	1505	1507	rVB	3814	4302	0.19%	0.021%
51	12.237	1518	1523	1525	rBV3	2907	3938	0.17%	0.020%
52	12.425	1554	1555	1559	rVB2	6078	6102	0.27%	0.030%
53	12.577	1578	1581	1583	rBV3	2594	2989	0.13%	0.015%
54	12.636	1589	1591	1593	rBV	3013	3403	0.15%	0.017%
55	12.977	1648	1649	1652	rBV	3712	2984	0.13%	0.015%
56	13.271	1696	1699	1703	rBV2	3751	6109	0.27%	0.030%
57	13.523	1739	1742	1744	rVB	2834	3071	0.13%	0.015%
58	13.547	1744	1746	1749	rBV	2905	3611	0.16%	0.018%
59	13.729	1774	1777	1780	rBV	3911	4029	0.18%	0.020%
60	13.782	1784	1786	1789	rBV2	3085	3695	0.16%	0.018%
61	13.846	1795	1797	1799	rVB	4935	4975	0.22%	0.025%
62	13.876	1799	1802	1803	rBV	4623	4569	0.20%	0.023%
63	14.070	1829	1835	1842	rBV	777808	1083779	47.49%	5.375%
64	14.140	1846	1847	1852	rBV2	3218	4068	0.18%	0.020%
65	14.369	1879	1886	1893	rBV2	700481	1108308	48.57%	5.497%
66	14.669	1930	1937	1945	rVB	530789	815440	35.73%	4.044%
67	14.781	1953	1956	1958	rVB2	3089	2957	0.13%	0.015%
68	14.875	1964	1972	1979	rBV3	103452	190213	8.34%	0.943%
69	15.662	2098	2106	2111	rBV	1025160	1507310	66.05%	7.475%
70	15.779	2119	2126	2132	rBV	497539	738152	32.35%	3.661%
71	16.003	2160	2164	2165	rBV2	5214	4366	0.19%	0.022%
72	16.285	2210	2212	2214	rBV3	4769	2986	0.13%	0.015%
73	16.402	2229	2232	2233	rBV2	3851	4499	0.20%	0.022%
74	16.608	2265	2267	2272	rVB2	4457	5278	0.23%	0.026%
75	16.808	2298	2301	2305	rBV2	3399	3830	0.17%	0.019%
76	17.002	2333	2334	2337	rBV	4586	3756	0.16%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071224\
 Data File : BG062050.D
 Acq On : 12 Jul 2024 21:24
 Operator : MA/JU
 Sample : P3137-11
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 YDZE4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
 Title : SVOA CALIBRATION

77	17.072	2343	2346	2347	rBV	5865	5364	0.24%	0.027%
78	17.131	2354	2356	2357	rBV2	5404	4488	0.20%	0.022%
79	17.254	2375	2377	2379	rBV3	4197	3432	0.15%	0.017%
80	17.319	2385	2388	2391	rVB4	5957	6226	0.27%	0.031%

81	17.413	2398	2404	2414	rVB	770612	1185940	51.97%	5.882%
82	17.513	2414	2421	2429	rBV	1230499	1867721	81.84%	9.263%
83	18.065	2511	2515	2519	rBV5	9028	12660	0.55%	0.063%
84	18.112	2521	2523	2524	rBV	5786	3035	0.13%	0.015%
85	18.153	2528	2530	2532	rBV3	4744	3328	0.15%	0.017%

86	18.235	2541	2544	2546	rBV4	4383	4576	0.20%	0.023%
87	18.277	2550	2551	2553	rBV2	6133	5651	0.25%	0.028%
88	18.512	2589	2591	2592	rBV2	4968	4298	0.19%	0.021%
89	18.641	2611	2613	2616	rBV4	7585	6931	0.30%	0.034%
90	18.905	2656	2658	2661	rBV2	7447	10726	0.47%	0.053%

91	19.363	2733	2736	2743	rVB7	31010	52528	2.30%	0.261%
92	19.410	2743	2744	2745	rBV	11211	7130	0.31%	0.035%
93	19.428	2745	2747	2750	rVB3	15147	16099	0.71%	0.080%
94	19.798	2804	2810	2816	rVB	1504707	2100832	92.06%	10.419%
95	21.673	3123	3129	3137	rVB	803817	1269510	55.63%	6.296%

96	24.663	3628	3638	3651	rVB2	833965	2282024	100.00%	11.318%
97	24.881	3667	3675	3687	rVB2	522641	1431133	62.71%	7.098%




Sum of corrected areas: 20163547

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071224\
Data File : BG062050.D
Acq On : 12 Jul 2024 21:24
Operator : MA/JU
Sample : P3137-11
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
YDZE4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

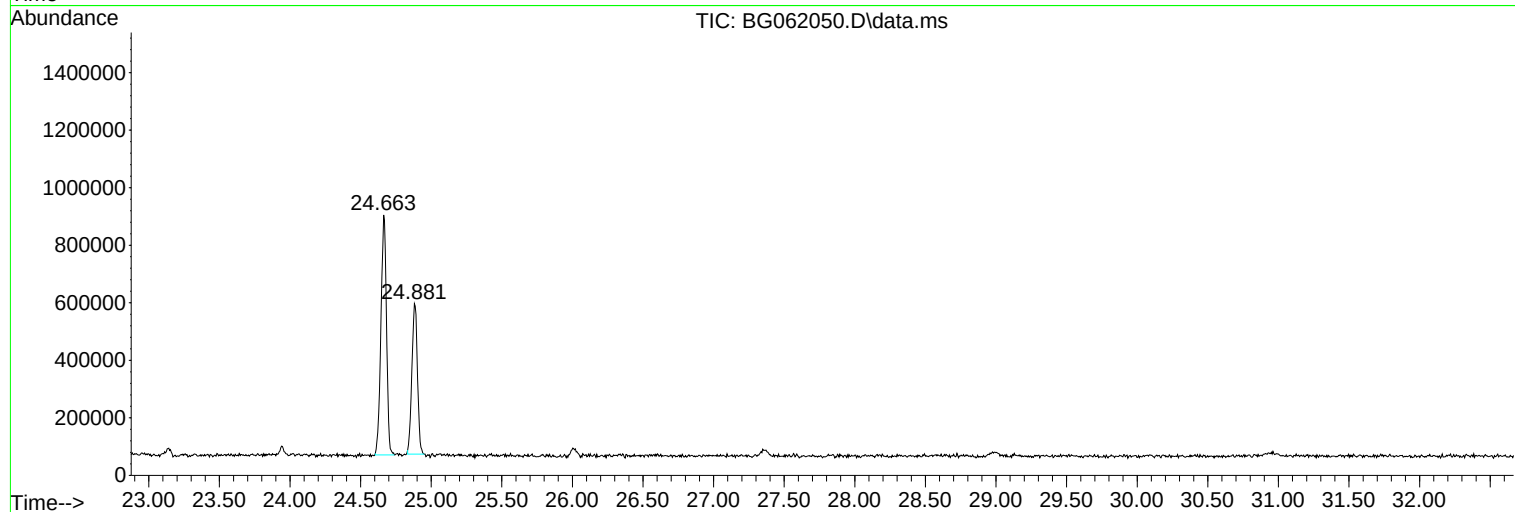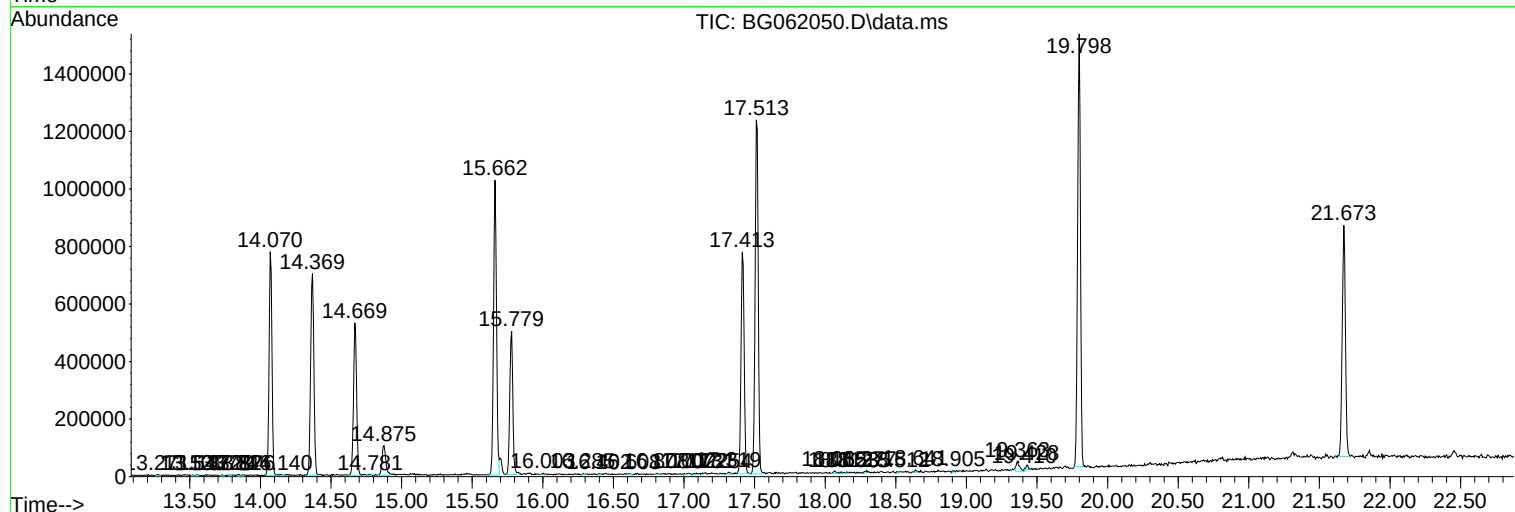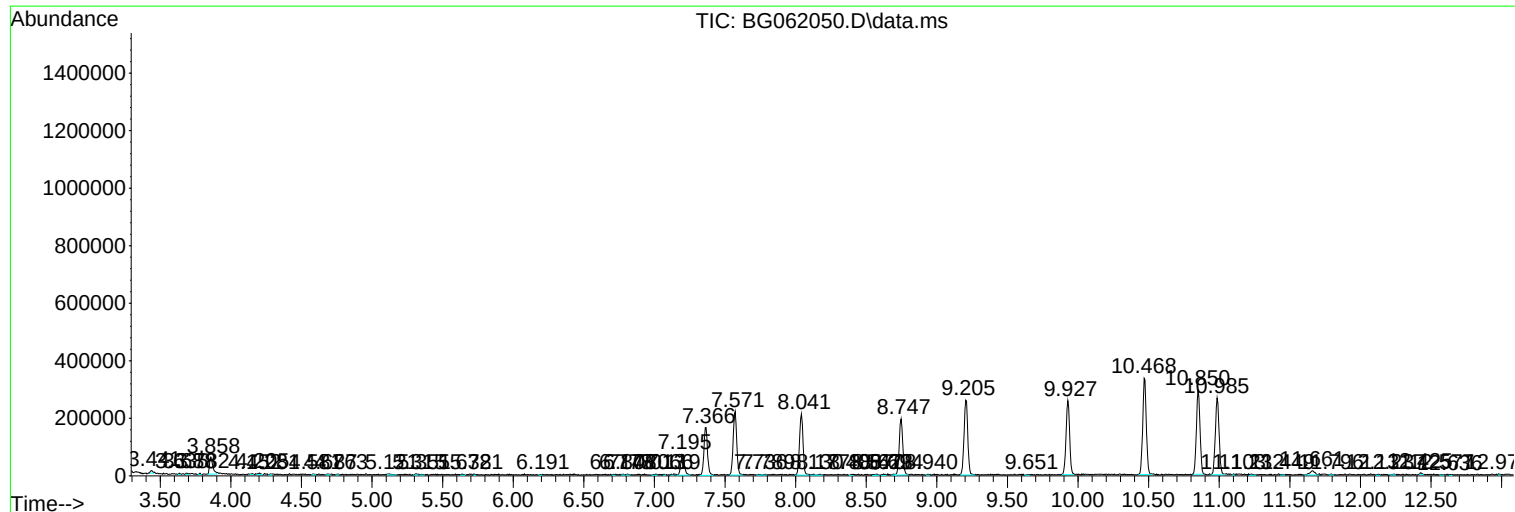

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071224\
Data File : BG062050.D
Acq On : 12 Jul 2024 21:24
Operator : MA/JU
Sample : P3137-11
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
YDZE4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071224\
Data File : BG062050.D
Acq On : 12 Jul 2024 21:24
Operator : MA/JU
Sample : P3137-11
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
YDZE4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc