

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071224\
 Data File : BG062061.D
 Acq On : 13 Jul 2024 5:35
 Operator : MA/JU
 Sample : PB161910BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK910

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG062061.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.434	21	25	29	rBV3	12209	17059	1.21%	0.129%
2	3.740	76	77	79	rVB2	4529	2669	0.19%	0.020%
3	3.857	94	97	110	rBV	156948	258778	18.29%	1.959%
4	4.521	208	210	213	rVB2	3294	3099	0.22%	0.023%
5	4.545	213	214	217	rBV2	2944	3176	0.22%	0.024%
6	4.650	227	232	235	rBV3	2658	3484	0.25%	0.026%
7	4.803	254	258	259	rVB3	2713	2758	0.19%	0.021%
8	4.968	283	286	289	rVB	3477	3715	0.26%	0.028%
9	4.997	289	291	294	rBV2	2331	2822	0.20%	0.021%
10	5.162	317	319	320	rVV2	3234	2523	0.18%	0.019%
11	5.173	320	321	325	rVB3	3433	2806	0.20%	0.021%
12	5.214	325	328	330	rBV2	2859	3629	0.26%	0.027%
13	5.491	373	375	376	rBV	2982	2418	0.17%	0.018%
14	5.614	391	396	399	rVB2	3856	6246	0.44%	0.047%
15	5.708	410	412	414	rVB	3441	2371	0.17%	0.018%
16	5.755	418	420	423	rVB2	3181	3288	0.23%	0.025%
17	6.002	459	462	463	rVB	3298	2550	0.18%	0.019%
18	6.125	481	483	487	rBV2	1968	2543	0.18%	0.019%
19	6.425	530	534	535	rBV	2991	3585	0.25%	0.027%
20	6.654	570	573	574	rBV	2430	2999	0.21%	0.023%
21	6.766	590	592	595	rVB	2669	2558	0.18%	0.019%
22	6.877	609	611	613	rBV	2624	2822	0.20%	0.021%
23	7.142	654	656	659	rBV	2573	4273	0.30%	0.032%
24	7.206	659	667	674	rVB2	220920	378923	26.78%	2.869%
25	7.365	685	694	702	rBV	105534	175261	12.39%	1.327%
26	7.500	713	717	720	rBV	2387	3796	0.27%	0.029%
27	7.571	722	729	735	rVV2	157568	268178	18.96%	2.030%
28	7.741	754	758	761	rVB	2224	2366	0.17%	0.018%
29	7.835	771	774	778	rVB	1969	2888	0.20%	0.022%
30	7.964	794	796	801	rBV2	2102	3544	0.25%	0.027%
31	8.041	801	809	815	rBV	103888	180216	12.74%	1.364%
32	8.446	876	878	883	rVB	1828	3244	0.23%	0.025%
33	8.481	883	884	891	rBV	2265	4204	0.30%	0.032%
34	8.751	924	930	941	rVB2	224840	377222	26.66%	2.856%
35	8.975	966	968	971	rBV	3684	3681	0.26%	0.028%
36	9.204	1000	1007	1015	rBV	164624	293056	20.71%	2.219%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071224\
 Data File : BG062061.D
 Acq On : 13 Jul 2024 5:35
 Operator : MA/JU
 Sample : PB161910BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK910

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
 Title : SVOA CALIBRATION

37	9.927	1124	1130	1137	rBV	158035	282553	19.97%	2.139%
38	10.009	1142	1144	1147	rBV	1751	2570	0.18%	0.019%
39	10.361	1201	1204	1206	rBV	2236	2618	0.19%	0.020%
40	10.473	1216	1223	1231	rBV	236497	413507	29.23%	3.130%
41	10.561	1235	1238	1240	rVV	2340	2553	0.18%	0.019%
42	10.673	1254	1257	1260	rBV	2241	3212	0.23%	0.024%
43	10.849	1278	1287	1295	rVB	159708	273936	19.36%	2.074%
44	10.984	1303	1310	1317	rBV	190279	343509	24.28%	2.600%
45	11.078	1322	1326	1329	rBV	2326	3721	0.26%	0.028%
46	11.507	1394	1399	1401	rBV	2074	2365	0.17%	0.018%
47	11.554	1403	1407	1410	rBV	1902	2900	0.20%	0.022%
48	12.441	1551	1558	1561	rBV4	4828	8270	0.58%	0.063%
49	12.576	1579	1581	1584	rBV	2838	2524	0.18%	0.019%
50	13.205	1684	1688	1691	rVV2	2248	3338	0.24%	0.025%
51	13.469	1731	1733	1734	rBV	3223	2548	0.18%	0.019%
52	14.075	1829	1836	1844	rBV	481533	682607	48.25%	5.168%
53	14.292	1870	1873	1876	rBV	2849	3152	0.22%	0.024%
54	14.368	1879	1886	1891	rVV	460575	711210	50.27%	5.384%
55	14.451	1899	1900	1904	rVB	2624	2492	0.18%	0.019%
56	14.668	1928	1937	1944	rBV	292123	450192	31.82%	3.408%
57	14.880	1967	1973	1982	rBV	247276	413348	29.22%	3.129%
58	15.068	2004	2005	2008	rBV	2984	2971	0.21%	0.022%
59	15.297	2042	2044	2047	rBV	2170	2823	0.20%	0.021%
60	15.420	2063	2065	2068	rVB	3373	2617	0.18%	0.020%
61	15.461	2068	2072	2075	rBV	3568	5079	0.36%	0.038%
62	15.661	2097	2106	2114	rBV	670976	972726	68.76%	7.364%
63	15.779	2120	2126	2132	rBV2	244024	364319	25.75%	2.758%
64	15.896	2144	2146	2150	rBV4	3822	4403	0.31%	0.033%
65	16.119	2183	2184	2186	rBV4	3862	2519	0.18%	0.019%
66	16.155	2188	2190	2194	rVV2	4384	4334	0.31%	0.033%
67	16.337	2219	2221	2223	rVB	2905	2703	0.19%	0.020%
68	16.360	2223	2225	2228	rVB2	4881	4359	0.31%	0.033%
69	16.431	2234	2237	2238	rBV2	2414	2760	0.20%	0.021%
70	16.595	2264	2265	2272	rBV2	2648	3440	0.24%	0.026%
71	16.695	2280	2282	2285	rVB	3521	2896	0.20%	0.022%
72	17.001	2332	2334	2337	rVB2	3545	3197	0.23%	0.024%
73	17.030	2337	2339	2341	rBV2	3663	2939	0.21%	0.022%
74	17.071	2344	2346	2347	rBV2	4287	3074	0.22%	0.023%
75	17.153	2359	2360	2364	rBV	1843	2835	0.20%	0.021%
76	17.212	2368	2370	2375	rVV	2169	3716	0.26%	0.028%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071224\
 Data File : BG062061.D
 Acq On : 13 Jul 2024 5:35
 Operator : MA/JU
 Sample : PB161910BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK910

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
 Title : SVOA CALIBRATION

77	17.412	2398	2404	2412	rVB	422172	651941	46.08%	4.935%
78	17.512	2415	2421	2430	rVV	753458	1155007	81.64%	8.744%
79	17.629	2439	2441	2444	rBV2	2584	3068	0.22%	0.023%
80	17.712	2453	2455	2457	rVB3	2861	2773	0.20%	0.021%
81	17.776	2465	2466	2469	rBV2	3478	3300	0.23%	0.025%
82	17.806	2469	2471	2472	rVV	4461	2849	0.20%	0.022%
83	17.847	2476	2478	2482	rVB	3138	3324	0.23%	0.025%
84	17.917	2484	2490	2494	rBV2	2876	6349	0.45%	0.048%
85	17.999	2500	2504	2505	rBV2	2878	2781	0.20%	0.021%
86	18.070	2514	2516	2517	rVB	6125	3215	0.23%	0.024%
87	18.135	2524	2527	2528	rBV2	4206	3686	0.26%	0.028%
88	18.170	2531	2533	2537	rBV4	3322	3866	0.27%	0.029%
89	18.564	2599	2600	2602	rBV2	4478	3183	0.22%	0.024%
90	18.587	2602	2604	2608	rVB3	4324	4730	0.33%	0.036%
91	18.628	2608	2611	2612	rBV2	3484	4196	0.30%	0.032%
92	18.787	2636	2638	2641	rBV3	3211	2697	0.19%	0.020%
93	18.846	2646	2648	2650	rBV4	3254	2432	0.17%	0.018%
94	19.186	2702	2706	2708	rBV4	4485	5853	0.41%	0.044%
95	19.310	2723	2727	2728	rBV4	3711	5800	0.41%	0.044%
96	19.363	2733	2736	2741	rVB4	11152	17056	1.21%	0.129%
97	19.797	2804	2810	2817	rVB	958234	1326046	93.73%	10.039%
98	21.672	3123	3129	3137	rBV	439835	707134	49.98%	5.353%
99	24.656	3629	3637	3649	rVB2	508081	1414718	100.00%	10.710%
100	24.880	3666	3675	3686	rVB	283147	827989	58.53%	6.268%




Sum of corrected areas: 13209578

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071224\
Data File : BG062061.D
Acq On : 13 Jul 2024 5:35
Operator : MA/JU
Sample : PB161910BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK910

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

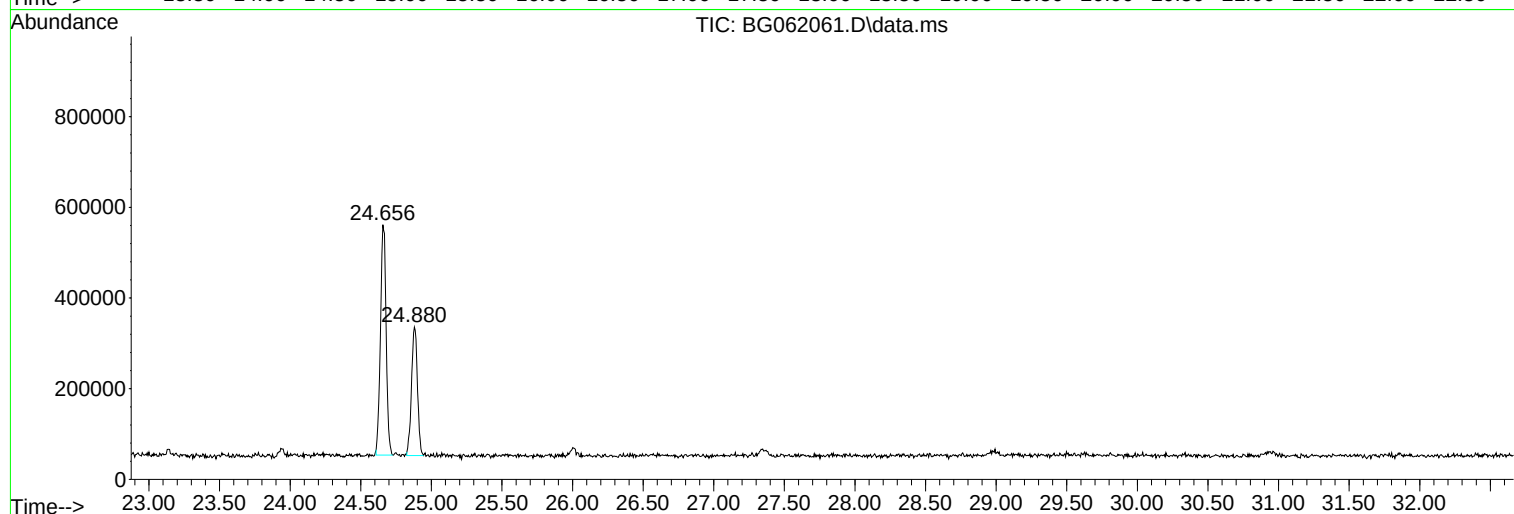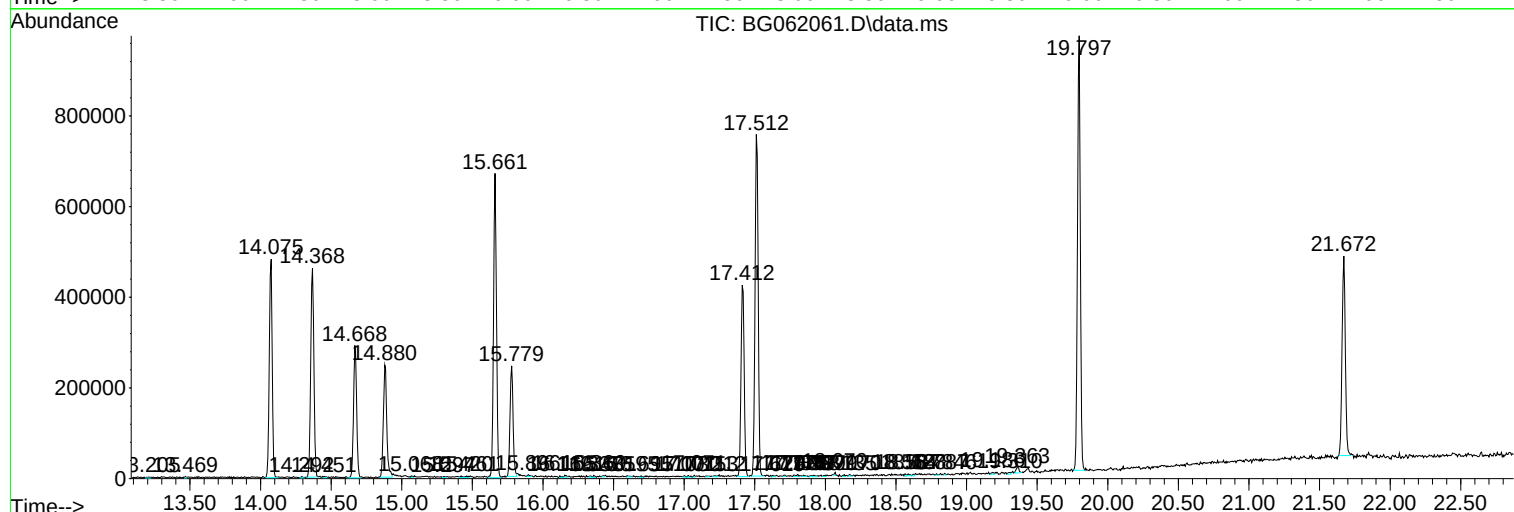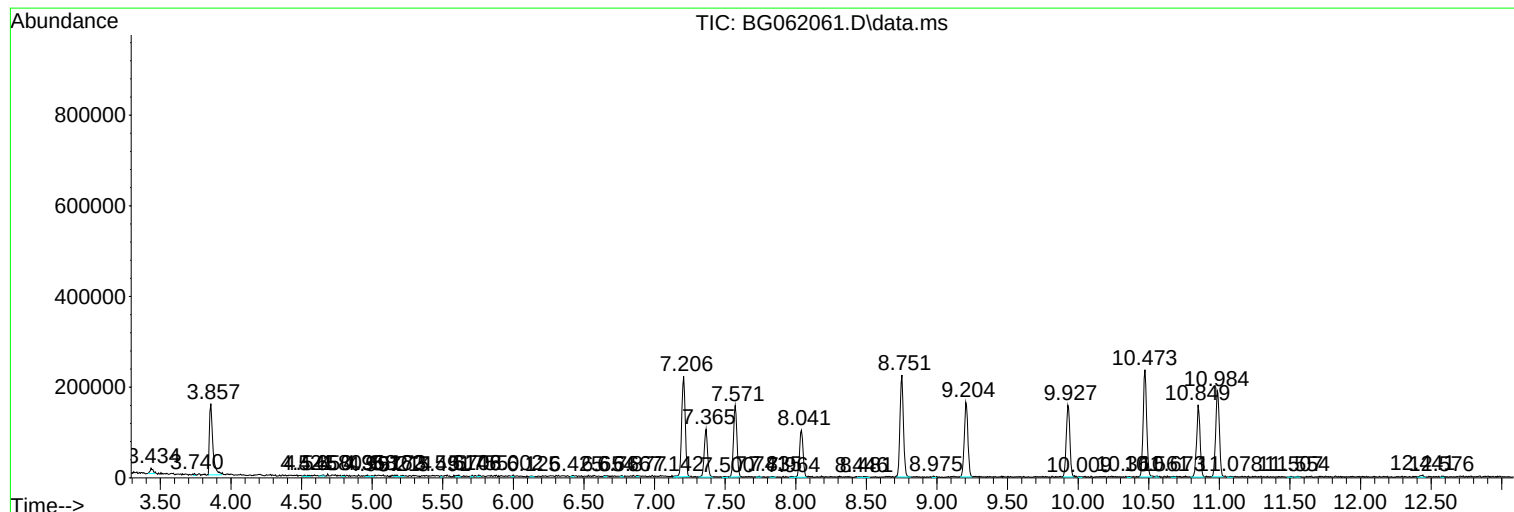

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071224\
Data File : BG062061.D
Acq On : 13 Jul 2024 5:35
Operator : MA/JU
Sample : PB161910BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK910

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071224\
Data File : BG062061.D
Acq On : 13 Jul 2024 5:35
Operator : MA/JU
Sample : PB161910BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK910

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc