

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071323\
 Data File : BG058236.D
 Acq On : 14 Jul 2023 18:29
 Operator : CG/JU
 Sample : 03418-03
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A46F4

Quant Time: Jul 15 01:16:59 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 13 14:01:20 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.906	152	58631	20.000	ng/ul	0.00
20) Naphthalene-d8	10.702	136	278788	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.539	164	201050	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.283	188	468213	20.000	ng/ul	0.00
79) Chrysene-d12	21.537	240	406210	20.000	ng/ul	0.00
88) Perylene-d12	24.680	264	506652	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.346	96	8409	5.022	ng/uL	0.00
4) Pyridine-d5	3.752	84	144047	28.338	ng/ul	0.00
7) Phenol-d5	7.071	99	208113	34.757	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.230	67	119582	33.140	ng/ul	0.00
11) 2-Chlorophenol-d4	7.436	132	142097	34.408	ng/ul	0.00
15) 4-Methylphenol-d8	8.611	113	158839	35.157	ng/ul	0.00
21) Nitrobenzene-d5	9.063	128	77223	33.985	ng/ul	0.00
24) 2-Nitrophenol-d4	9.786	143	88342	36.993	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.326	165	163484	35.686	ng/ul	0.00
31) 4-Chloroaniline-d4	10.843	131	217791	31.356	ng/ul	0.00
46) Dimethylphthalate-d6	13.946	166	519688	32.761	ng/ul	0.00
49) Acenaphthylene-d8	14.233	160	610847	35.288	ng/ul	0.00
54) 4-Nitrophenol-d4	14.745	143	83518	29.800	ng/ul	0.00
60) Fluorene-d10	15.532	176	470510	34.925	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.649	200	69702	27.416	ng/ul	0.00
73) Anthracene-d10	17.383	188	708376	32.605	ng/ul	0.00
81) Pyrene-d10	19.674	212	860929	33.652	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.463	264	902089	34.947	ng/ul	0.00


Target Compounds					Qvalue
17) N-Nitroso-di-n-propyla...	8.611	70	4307	1.075 ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071323\
Data File : BG058236.D
Acq On : 14 Jul 2023 18:29
Operator : CG/JU
Sample : 03418-03
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A46F4


Quant Time: Jul 15 01:16:59 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 13 14:01:20 2023
Response via : Initial Calibration

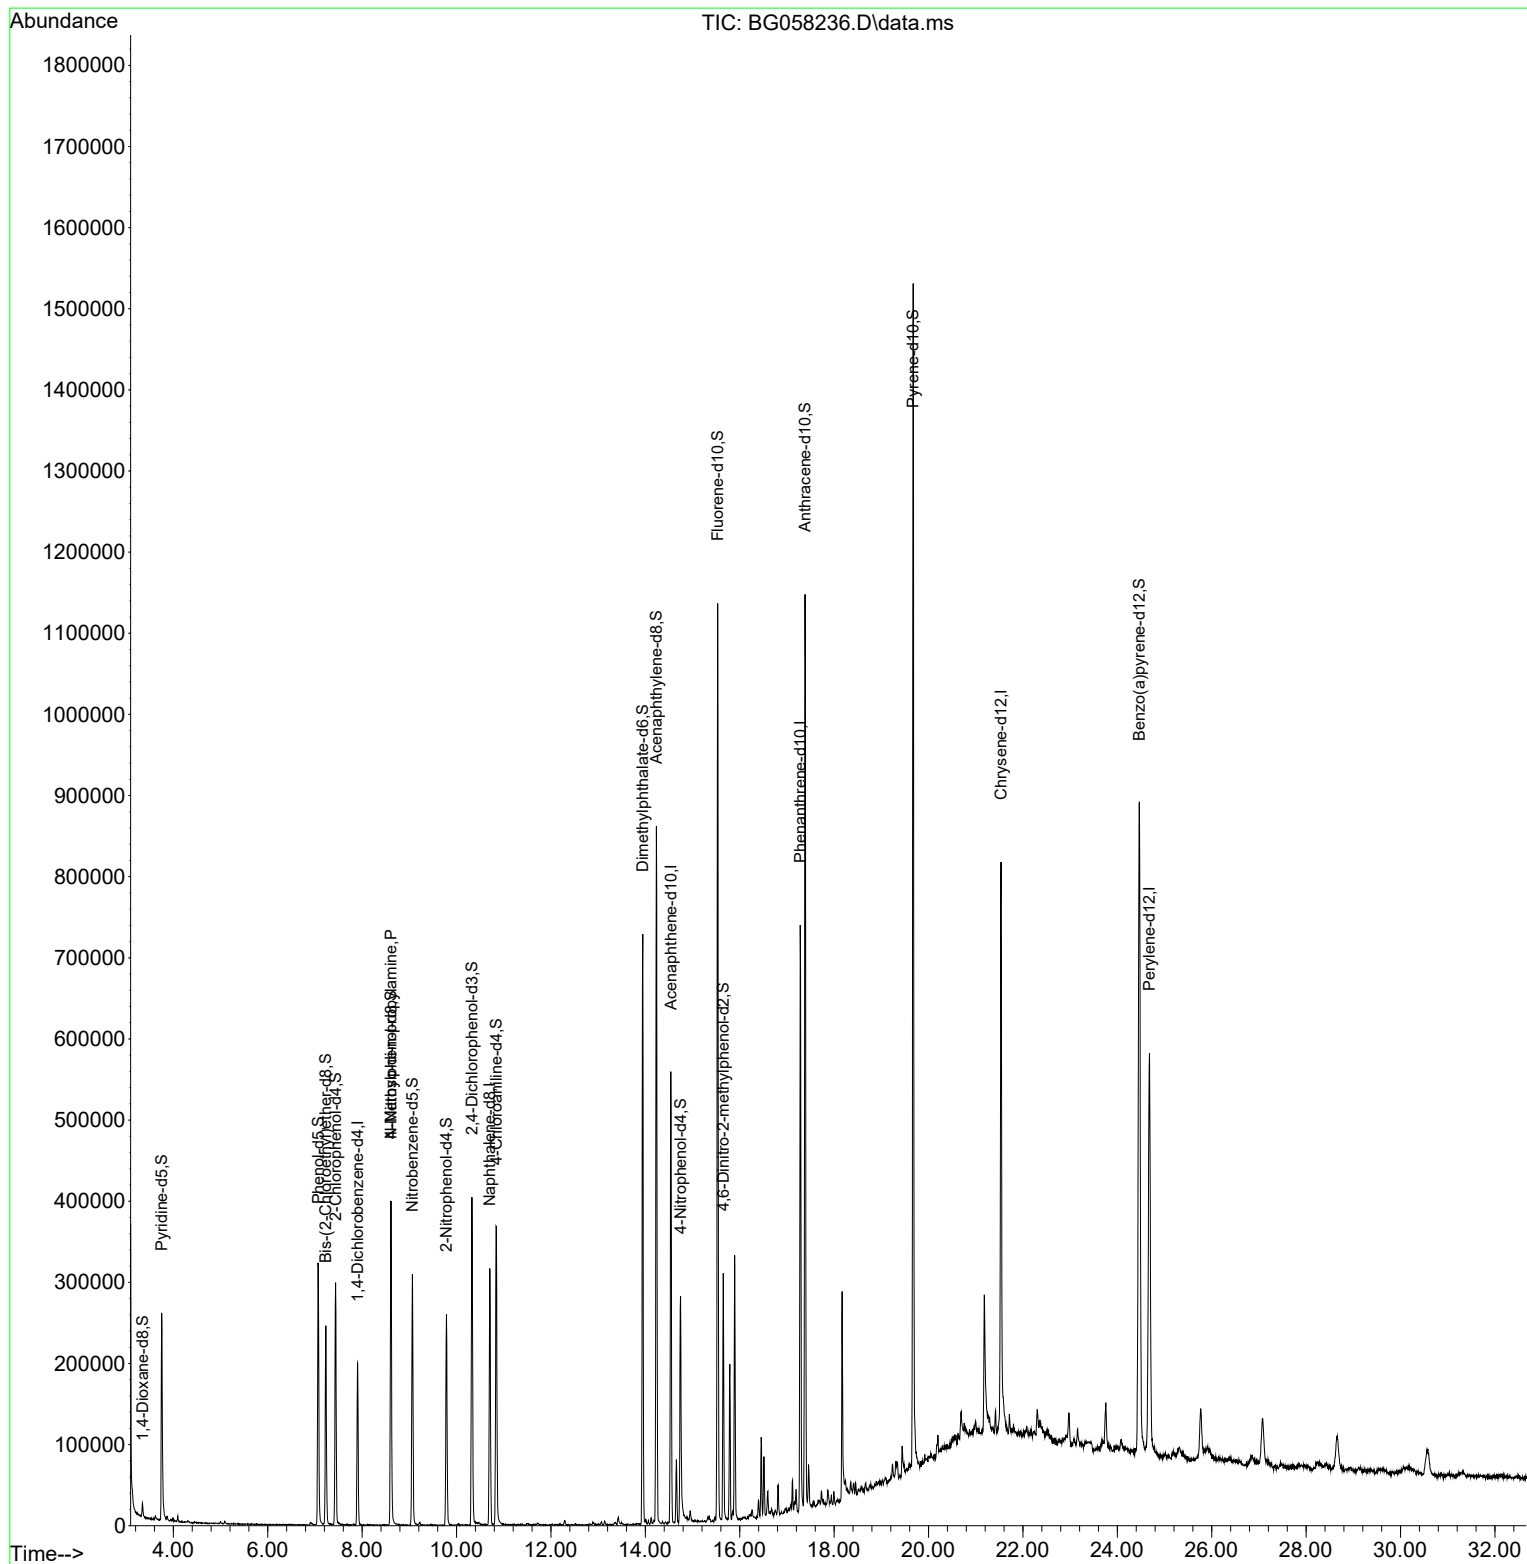

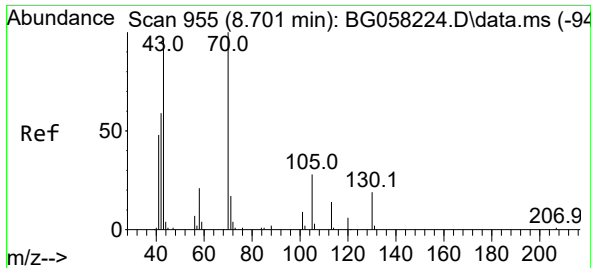

#17
 N-Nitroso-di-n-propylamine
 Concen: 1.075 ng/ul
 RT: 8.611 min Scan# 94
 Delta R.T. -0.094 min
 Lab File: BG058236.D
 Acq: 14 Jul 2023 18:29

Instrument :
 BNA_G
 ClientSampleId :
 A46F4

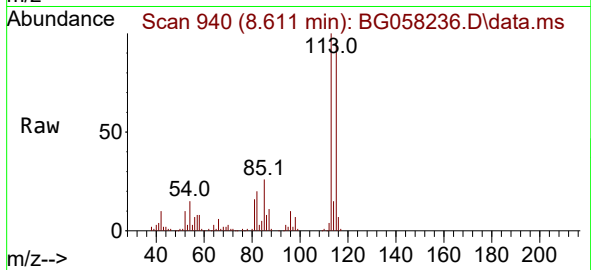

Tgt Ion: 70 Resp: 4307

Ion	Ratio	Lower	Upper
70	100		
42	362.5	48.0	72.0#
101	0.0	7.4	11.2#
130	0.0	13.4	20.0#

