

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071323\
 Data File : BG058257.D
 Acq On : 15 Jul 2023 11:10
 Operator : CG/JU
 Sample : 03437-10
 Misc :
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A46K7

Quant Time: Jul 15 22:36:13 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 13 14:01:20 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.900	152	59431	20.000	ng/ul	0.00
20) Naphthalene-d8	10.703	136	290377	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.539	164	209110	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.283	188	496848	20.000	ng/ul	0.00
79) Chrysene-d12	21.537	240	444342	20.000	ng/ul	0.00
88) Perylene-d12	24.674	264	541819	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.346	96	9920	5.845	ng/uL	0.00
4) Pyridine-d5	3.752	84	162383	31.515	ng/ul	0.00
7) Phenol-d5	7.066	99	237474	39.126	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.224	67	136786	37.398	ng/ul	0.00
11) 2-Chlorophenol-d4	7.430	132	160688	38.386	ng/ul	0.00
15) 4-Methylphenol-d8	8.605	113	171361	37.418	ng/ul	0.00
21) Nitrobenzene-d5	9.063	128	88269	37.296	ng/ul	0.00
24) 2-Nitrophenol-d4	9.786	143	102594	41.246	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.321	165	184922	38.754	ng/ul	0.00
31) 4-Chloroaniline-d4	10.838	131	250315	34.600	ng/ul	0.00
46) Dimethylphthalate-d6	13.940	166	593989	36.001	ng/ul	0.00
49) Acenaphthylene-d8	14.234	160	699060	38.827	ng/ul	0.00
54) 4-Nitrophenol-d4	14.745	143	93335	32.019	ng/ul	0.00
60) Fluorene-d10	15.532	176	540013	38.539	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.650	200	86856	32.194	ng/ul	0.00
73) Anthracene-d10	17.383	188	848862	36.819	ng/ul	0.00
81) Pyrene-d10	19.674	212	1013876	36.229	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.463	264	1078370	39.065	ng/ul	0.00


Target Compounds					Qvalue	
17) N-Nitroso-di-n-propyla...	8.611	70	4145	1.020	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071323\
Data File : BG058257.D
Acq On : 15 Jul 2023 11:10
Operator : CG/JU
Sample : 03437-10
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A46K7


Quant Time: Jul 15 22:36:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 13 14:01:20 2023
Response via : Initial Calibration

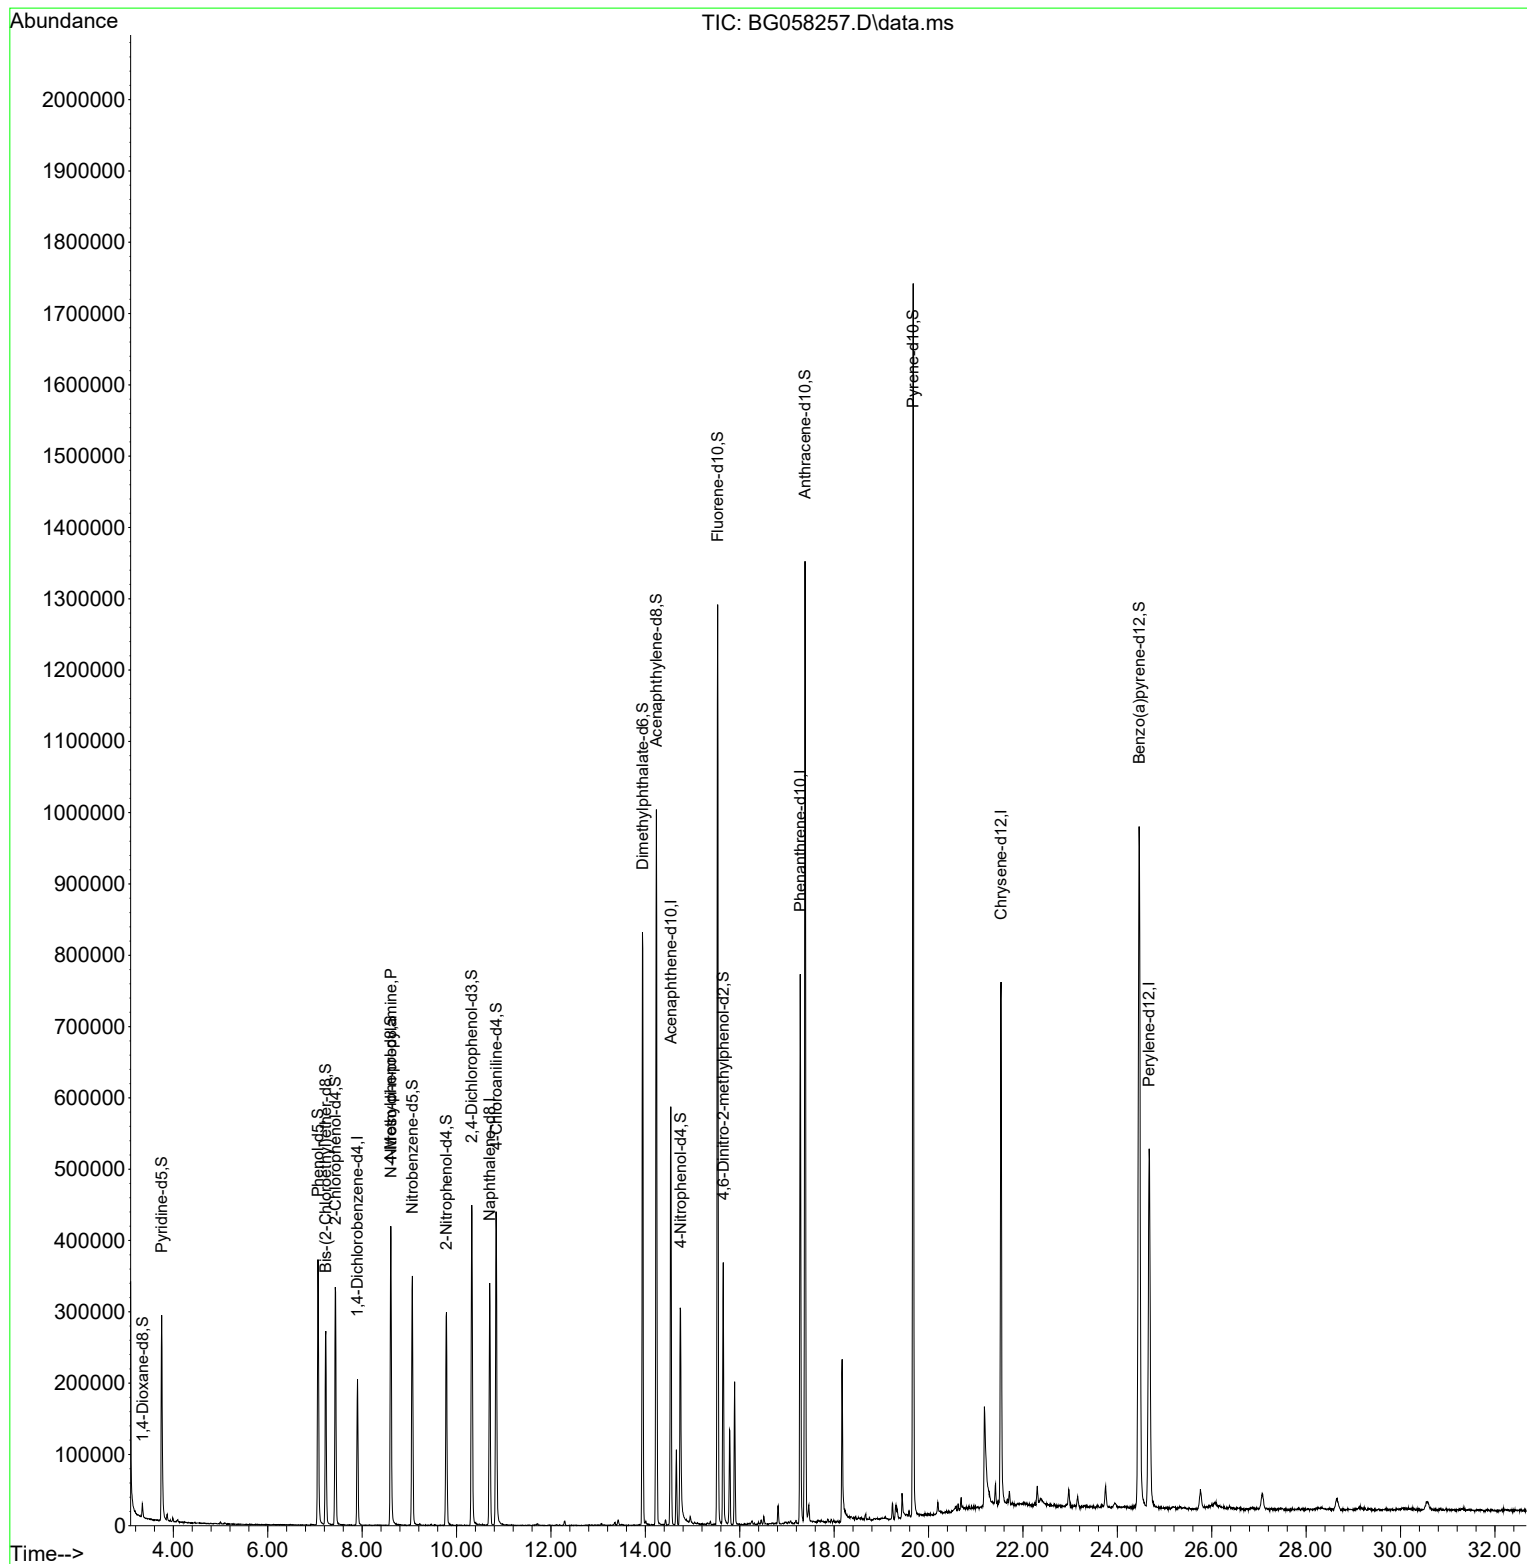

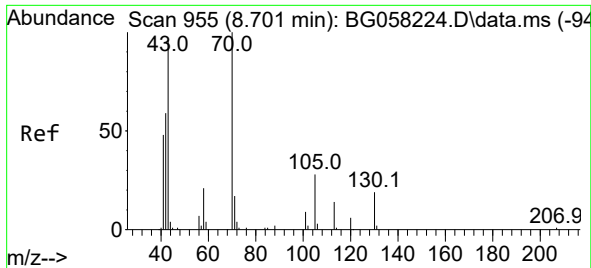

#17
 N-Nitroso-di-n-propylamine
 Concen: 1.020 ng/ul
 RT: 8.611 min Scan# 94
 Delta R.T. -0.094 min
 Lab File: BG058257.D
 Acq: 15 Jul 2023 11:10

Instrument :
 BNA_G
 ClientSampleId :
 A46K7

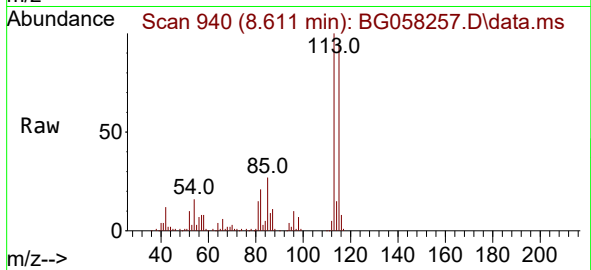

Tgt Ion:	70	Resp:	4145
Ion	Ratio	Lower	Upper
70	100		
42	468.3	48.0	72.0#
101	0.0	7.4	11.2#
130	0.0	13.4	20.0#

