

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071323\
 Data File : BG058269.D
 Acq On : 15 Jul 2023 20:54
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 81 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SSTD020519

Quant Time: Jul 15 22:38:23 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 13 14:01:20 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.900	152	50963	20.000	ng/u1	0.00
20) Naphthalene-d8	10.703	136	243254	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.539	164	174872	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.283	188	408541	20.000	ng/u1	0.00
79) Chrysene-d12	21.537	240	354742	20.000	ng/u1	0.00
88) Perylene-d12	24.674	264	446819	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.346	96	12906	8.868	ng/uL	0.00
4) Pyridine-d5	3.752	84	100263	22.692	ng/u1	0.00
7) Phenol-d5	7.066	99	116834	22.448	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.230	67	66334	21.149	ng/u1	0.00
11) 2-Chlorophenol-d4	7.436	132	80054	22.302	ng/u1	0.00
15) 4-Methylphenol-d8	8.611	113	87997	22.407	ng/u1	0.00
21) Nitrobenzene-d5	9.063	128	41252	20.807	ng/u1	0.00
24) 2-Nitrophenol-d4	9.786	143	46811	22.465	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.326	165	90579	22.660	ng/u1	0.00
31) 4-Chloroaniline-d4	10.838	131	123257	20.338	ng/u1	0.00
46) Dimethylphthalate-d6	13.940	166	266111	19.287	ng/u1	0.00
49) Acenaphthylene-d8	14.234	160	316041	20.990	ng/u1	0.00
54) 4-Nitrophenol-d4	14.745	143	41306	16.945	ng/u1	0.00
60) Fluorene-d10	15.532	176	242736	20.715	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.650	200	38858	17.516	ng/u1	0.00
73) Anthracene-d10	17.383	188	385354	20.327	ng/u1	0.00
81) Pyrene-d10	19.674	212	452314	20.245	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.457	264	467141	20.521	ng/u1	-0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.382	88	14052	7.815	ng/uL#	95
5) Pyridine	3.775	79	102455	22.631	ng/u1	99
6) Benzaldehyde	7.042	77	45478	26.165	ng/u1	94
8) Phenol	7.095	94	121148	22.938	ng/u1	98
10) Bis(2-Chloroethyl)ether	7.324	93	85504	20.967	ng/u1	97
12) 2-Chlorophenol	7.465	128	83911	22.464	ng/u1	96
13) 2-Methylphenol	8.341	108	92787	22.370	ng/u1	94
14) 2,2'-oxybis(1-Chloropr...	8.429	45	140414	22.368	ng/u1	98
16) Acetophenone	8.723	105	137466	21.098	ng/u1	100
17) N-Nitroso-di-n-propyla...	8.699	70	72572	20.835	ng/u1	97
18) 4-Methylphenol	8.670	108	102919	22.947	ng/u1	96
19) Hexachloroethane	8.981	117	32743	22.865	ng/u1	95
22) Nitrobenzene	9.104	77	107384	20.864	ng/u1	96
23) Isophorone	9.621	82	214334	19.516	ng/u1	97
25) 2-Nitrophenol	9.815	139	49235	22.020	ng/u1	90
26) 2,4-Dimethylphenol	9.874	107	110363	21.950	ng/u1	95
27) Bis(2-Chloroethoxy)met...	10.109	93	121999	19.713	ng/u1	100
29) 2,4-Dichlorophenol	10.350	162	88333	22.728	ng/u1	94
30) Naphthalene	10.755	128	290920	21.281	ng/u1	98
32) 4-Chloroaniline	10.867	127	129947	20.970	ng/u1	100
33) Hexachlorobutadiene	11.032	225	60967	22.158	ng/u1	97
34) Caprolactam	11.613	113	29555	18.915	ng/u1	90
35) 4-Chloro-3-methylphenol	11.989	107	106566	22.321	ng/u1	99
36) 2-Methylnaphthalene	12.365	142	193728	21.023	ng/u1	96


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071323\
 Data File : BG058269.D
 Acq On : 15 Jul 2023 20:54
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 81 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SSTD020519

Quant Time: Jul 15 22:38:23 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 13 14:01:20 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.583	142	198062	21.433	ng/ul	99
39) 1,2,4,5-Tetrachloroben...	12.730	216	115870	21.743	ng/ul	99
40) Hexachlorocyclopentadiene	12.706	237	53535	15.949	ng/ul	96
41) 2,4,6-Trichlorophenol	12.970	196	80063	22.167	ng/ul	100
42) 2,4,5-Trichlorophenol	13.047	196	84918	21.739	ng/ul	96
43) 1,1'-Biphenyl	13.370	154	264722	21.006	ng/ul	99
44) 2-Chloronaphthalene	13.417	162	213570	21.116	ng/ul	99
45) 2-Nitroaniline	13.617	65	75393	21.440	ng/ul	97
47) Dimethylphthalate	13.987	163	270015	19.479	ng/ul	99
48) 2,6-Dinitrotoluene	14.116	165	58489	20.556	ng/ul	99
50) Acenaphthylene	14.263	152	343241	21.111	ng/ul	100
51) 3-Nitroaniline	14.445	138	46774	19.452	ng/ul	100
52) Acenaphthene	14.604	153	233275	20.909	ng/ul	97
53) 2,4-Dinitrophenol	14.657	184	24283	16.370	ng/ul	99
55) 4-Nitrophenol	14.757	109	31003	17.168	ng/ul	84
56) Dibenzofuran	14.939	168	331472	20.900	ng/ul	100
57) 2,4-Dinitrotoluene	14.903	165	83596	20.736	ng/ul	98
58) 2,3,4,6-Tetrachlorophenol	15.162	232	74618	20.984	ng/ul#	98
59) Diethylphthalate	15.350	149	276816	19.133	ng/ul	99
61) Fluorene	15.585	166	268968	20.669	ng/ul	100
62) 4-Chlorophenyl-phenyle...	15.573	204	143987	20.912	ng/ul	98
63) 4-Nitroaniline	15.609	138	30441	14.132	ng/ul	94
66) 4,6-Dinitro-2-methylph...	15.667	198	39526	17.423	ng/ul	99
67) N-Nitrosodiphenylamine	15.791	169	225450	20.736	ng/ul	98
68) 4-Bromophenyl-phenylether	16.472	248	96376	21.491	ng/ul	99
69) Hexachlorobenzene	16.590	284	110471	22.002	ng/ul	98
70) Atrazine	16.737	200	89455	20.120	ng/ul	96
71) Pentachlorophenol	16.936	266	55382	18.373	ng/ul	97
72) Phenanthrene	17.324	178	426937	20.544	ng/ul	99
74) Anthracene	17.418	178	433417	20.610	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.341	216	122264	22.565	ng/uL	98
76) Pentachlorobenzene	14.856	250	128923	22.279	ng/uL	97
77) Carbazole	17.688	167	394000	20.716	ng/ul	98
78) Di-n-butylphthalate	18.241	149	487515	20.122	ng/ul	100
80) Fluoranthene	19.339	202	517098	19.974	ng/ul	98
82) Pyrene	19.698	202	521805	20.024	ng/ul	98
83) Butylbenzylphthalate	20.585	149	219376	20.760	ng/ul	100
84) 3,3'-Dichlorobenzidine	21.437	252	189276	22.040	ng/ul	100
85) Benzo(a)anthracene	21.519	228	530071	20.811	ng/ul	100
86) Bis(2-ethylhexyl)phtha...	21.419	149	319514	21.100	ng/ul	99
87) Chrysene	21.578	228	503305	21.079	ng/ul	99
89) Di-n-octyl phthalate	22.594	149	565384	20.594	ng/ul	100
90) Benzo(b)fluoranthene	23.676	252	566539	20.478	ng/ul	99
91) Benzo(k)fluoranthene	23.740	252	551046	20.321	ng/ul	99
93) Benzo(a)pyrene	24.528	252	496277	20.267	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	28.253	276	641034	19.714	ng/ul	98
95) Dibenzo(a,h)anthracene	28.305	278	543737	20.278	ng/ul	99
96) Benzo(g,h,i)perylene	29.375	276	492632	18.548	ng/ul	99





(#) = qualifier out of range (m) = manual integration (+) = signals summed



#2
1,4-Dioxane
Concen: 7.815 ng/uL
RT: 3.382 min Scan# 50
Delta R.T. 0.000 min
Lab File: BG058269.D
Acq: 15 Jul 2023 20:54




Instrument :
BNA_G
ClientSampleId :
SSTD020519


Tgt Ion: 88 Resp: 14052
Ion Ratio Lower Upper
88 100
43 32.9 20.6 30.8#
58 83.9 65.5 98.3

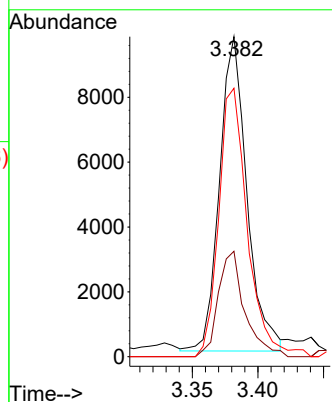

#5
Pyridine
Concen: 22.631 ng/uL
RT: 3.775 min Scan# 117
Delta R.T. 0.000 min
Lab File: BG058269.D
Acq: 15 Jul 2023 20:54

Tgt Ion: 79 Resp: 102455
Ion Ratio Lower Upper
79 100
52 86.1 68.6 102.8
51 37.2 29.4 44.0









#6
Benzaldehyde
Concen: 26.165 ng/ul
RT: 7.042 min Scan# 61
Delta R.T. 0.000 min
Lab File: BG058269.D
Acq: 15 Jul 2023 20:54




Instrument :
BNA_G
ClientSampleId :
SSTD020519


Tgt Ion: 77 Resp: 45478
Ion Ratio Lower Upper
77 100
105 99.9 74.7 112.1
106 90.4 75.9 113.9

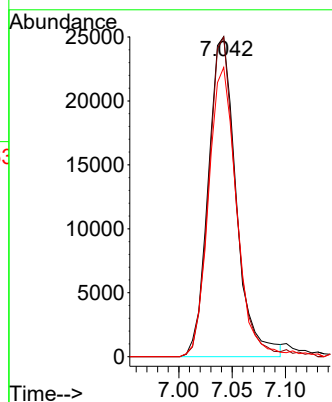

#8
Phenol
Concen: 22.938 ng/ul
RT: 7.095 min Scan# 682
Delta R.T. 0.000 min
Lab File: BG058269.D
Acq: 15 Jul 2023 20:54

Tgt Ion: 94 Resp: 121148
Ion Ratio Lower Upper
94 100
65 28.2 22.2 33.4
66 37.4 28.6 43.0



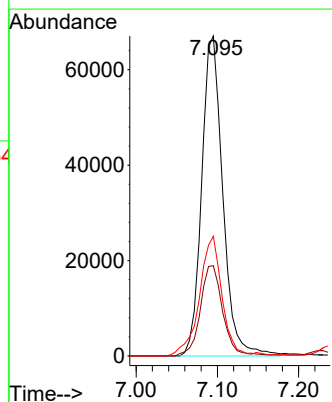
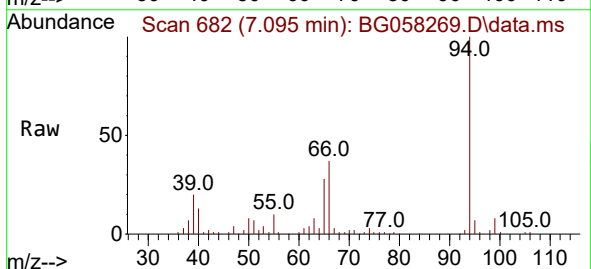




#10
Bis(2-Chloroethyl)ether
Concen: 20.967 ng/ul
RT: 7.324 min Scan# 720
Delta R.T. 0.000 min
Lab File: BG058269.D
Acq: 15 Jul 2023 20:54




Instrument :
BNA_G
ClientSampleId :
SSTD020519


Tgt Ion: 93 Resp: 85504
Ion Ratio Lower Upper
93 100
63 84.5 69.4 104.0
95 31.0 27.0 40.6



#12
2-Chlorophenol
Concen: 22.464 ng/ul
RT: 7.465 min Scan# 745
Delta R.T. 0.000 min
Lab File: BG058269.D
Acq: 15 Jul 2023 20:54

Tgt Ion: 128 Resp: 83911
Ion Ratio Lower Upper
128 100
64 57.4 44.3 66.5
130 30.3 27.3 40.9









#13
2-Methylphenol
Concen: 22.370 ng/ul
RT: 8.341 min Scan# 894
Delta R.T. -0.006 min
Lab File: BG058269.D
Acq: 15 Jul 2023 20:54




Instrument :
BNA_G
ClientSampleId :
SSTD020519


Tgt Ion:108 Resp: 92787
Ion Ratio Lower Upper
108 100
107 87.5 75.0 112.4



#14
2,2'-oxybis(1-Chloropropane)
Concen: 22.368 ng/ul
RT: 8.429 min Scan# 909
Delta R.T. 0.006 min
Lab File: BG058269.D
Acq: 15 Jul 2023 20:54

Tgt Ion: 45 Resp: 140414
Ion Ratio Lower Upper
45 100
77 12.5 9.4 14.2
79 9.9 8.3 12.5



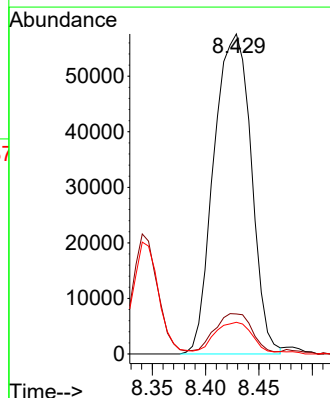





#16
Acetophenone
Concen: 21.098 ng/ul
RT: 8.723 min Scan# 91
Delta R.T. 0.000 min
Lab File: BG058269.D
Acq: 15 Jul 2023 20:54




Instrument :
BNA_G
ClientSampleId :
SSTD020519


Tgt Ion:105 Resp: 137466
Ion Ratio Lower Upper
105 100
77 76.6 61.2 91.8
51 29.0 23.5 35.3



#17
N-Nitroso-di-n-propylamine
Concen: 20.835 ng/ul
RT: 8.699 min Scan# 955
Delta R.T. -0.006 min
Lab File: BG058269.D
Acq: 15 Jul 2023 20:54

Tgt Ion: 70 Resp: 72572
Ion Ratio Lower Upper
70 100
42 57.6 48.0 72.0
101 9.9 7.4 11.2
130 18.2 13.4 20.0









#18
4-Methylphenol
Concen: 22.947 ng/ul
RT: 8.670 min Scan# 91
Delta R.T. -0.006 min
Lab File: BG058269.D
Acq: 15 Jul 2023 20:54




Instrument :
BNA_G
ClientSampleId :
SSTD020519


Tgt Ion:108 Resp: 102919
Ion Ratio Lower Upper
108 100
107 109.9 91.1 136.7



#19
Hexachloroethane
Concen: 22.865 ng/ul
RT: 8.981 min Scan# 1003
Delta R.T. 0.000 min
Lab File: BG058269.D
Acq: 15 Jul 2023 20:54

Tgt Ion:117 Resp: 32743
Ion Ratio Lower Upper
117 100
201 112.4 94.0 141.0
199 68.9 59.8 89.6


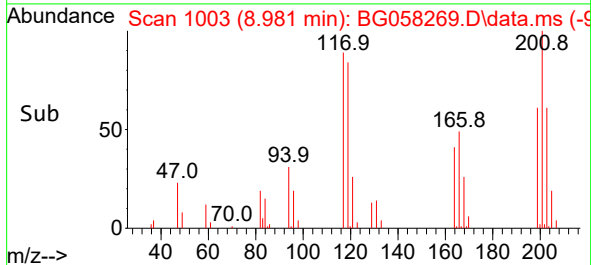






#22
Nitrobenzene
Concen: 20.864 ng/ul
RT: 9.104 min Scan# 1104
Delta R.T. 0.000 min
Lab File: BG058269.D
Acq: 15 Jul 2023 20:54




Instrument :
BNA_G
ClientSampleId :
SSTD020519


Tgt Ion: 77 Resp: 107384
Ion Ratio Lower Upper
77 100
123 44.0 33.3 49.9
65 14.8 10.4 15.6



#23
Isophorone
Concen: 19.516 ng/ul
RT: 9.621 min Scan# 1112
Delta R.T. -0.006 min
Lab File: BG058269.D
Acq: 15 Jul 2023 20:54

Tgt Ion: 82 Resp: 214334
Ion Ratio Lower Upper
82 100
95 6.5 4.8 7.2
138 15.5 11.4 17.0




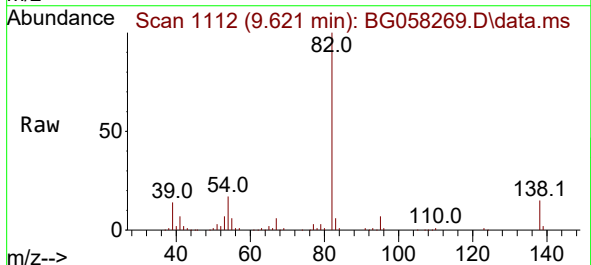




#25
2-Nitrophenol
Concen: 22.020 ng/ul
RT: 9.815 min Scan# 1145
Delta R.T. -0.006 min
Lab File: BG058269.D
Acq: 15 Jul 2023 20:54




Instrument :
BNA_G
ClientSampleId :
SSTD020519


Tgt Ion:139 Resp: 49235
Ion Ratio Lower Upper
139 100
65 62.8 42.6 64.0
109 27.6 20.7 31.1



#26
2,4-Dimethylphenol
Concen: 21.950 ng/ul
RT: 9.874 min Scan# 1155
Delta R.T. -0.006 min
Lab File: BG058269.D
Acq: 15 Jul 2023 20:54

Tgt Ion:107 Resp: 110363
Ion Ratio Lower Upper
107 100
121 46.7 40.6 60.8
122 79.8 67.1 100.7









#27
 Bis(2-Chloroethoxy)methane
 Concen: 19.713 ng/ul
 RT: 10.109 min Scan# 1195
 Delta R.T. 0.000 min
 Lab File: BG058269.D
 Acq: 15 Jul 2023 20:54




Instrument :
 BNA_G
 ClientSampleId :
 SSTD020519


Tgt Ion: 93 Resp: 121999
 Ion Ratio Lower Upper
 93 100
 95 33.0 26.4 39.6
 123 10.3 7.9 11.9

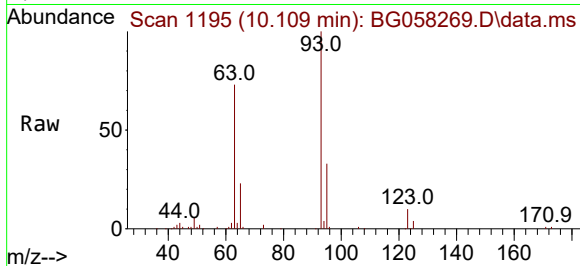

#29
 2,4-Dichlorophenol
 Concen: 22.728 ng/ul
 RT: 10.350 min Scan# 1236
 Delta R.T. -0.006 min
 Lab File: BG058269.D
 Acq: 15 Jul 2023 20:54

Tgt Ion:162 Resp: 88333
 Ion Ratio Lower Upper
 162 100
 164 69.1 51.1 76.7
 98 38.1 27.9 41.9




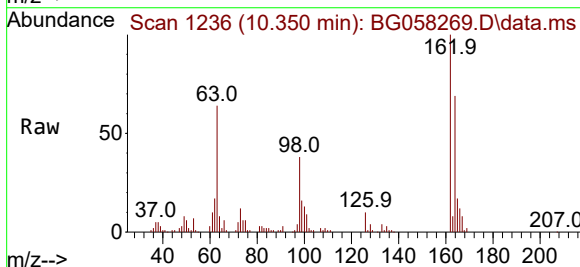




#30
Naphthalene
Concen: 21.281 ng/ul
RT: 10.755 min Scan# 11
Delta R.T. 0.000 min
Lab File: BG058269.D
Acq: 15 Jul 2023 20:54




Instrument :
BNA_G
ClientSampleId :
SSTD020519


Tgt Ion:128 Resp: 290920
Ion Ratio Lower Upper
128 100
129 10.7 8.6 12.8
127 13.8 10.2 15.2



#32
4-Chloroaniline
Concen: 20.970 ng/ul
RT: 10.867 min Scan# 1324
Delta R.T. 0.000 min
Lab File: BG058269.D
Acq: 15 Jul 2023 20:54

Tgt Ion:127 Resp: 129947
Ion Ratio Lower Upper
127 100
129 32.5 26.0 39.0

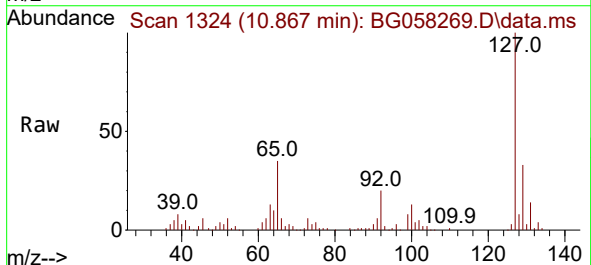



#33

Hexachlorobutadiene

Concen: 22.158 ng/ul

RT: 11.032 min Scan# 11

Delta R.T. -0.005 min

Lab File: BG058269.D

Acq: 15 Jul 2023 20:54

Instrument :

BNA_G

ClientSampleId :

SSTD020519





Tgt Ion:225 Resp: 60967

Ion Ratio Lower Upper

225 100

223 63.9 53.2 79.8

227 66.7 51.4 77.2

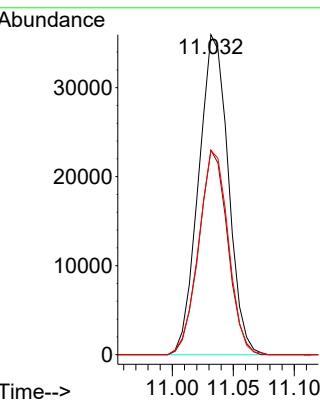

#34

Caprolactam

Concen: 18.915 ng/ul

RT: 11.613 min Scan# 1451

Delta R.T. -0.005 min

Lab File: BG058269.D

Acq: 15 Jul 2023 20:54




Tgt Ion:113 Resp: 29555


Ion Ratio Lower Upper

113 100

55 241.2 183.4 275.2

56 170.7 123.0 184.6



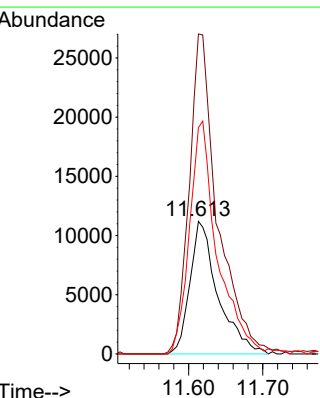





#35
4-Chloro-3-methylphenol
Concen: 22.321 ng/ul
RT: 11.989 min Scan# 11
Delta R.T. -0.006 min
Lab File: BG058269.D
Acq: 15 Jul 2023 20:54




Instrument :
BNA_G
ClientSampleId :
SSTD020519


Tgt Ion:107 Resp: 106566
Ion Ratio Lower Upper
107 100
144 24.0 19.0 28.4
142 71.8 58.4 87.6

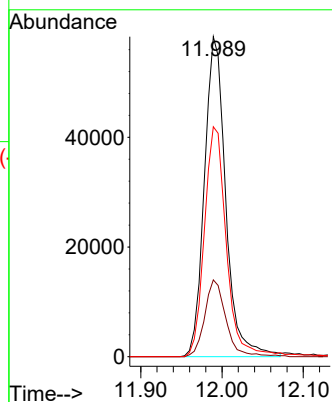

#36
2-Methylnaphthalene
Concen: 21.023 ng/ul
RT: 12.365 min Scan# 1579
Delta R.T. 0.000 min
Lab File: BG058269.D
Acq: 15 Jul 2023 20:54

Tgt Ion:142 Resp: 193728
Ion Ratio Lower Upper
142 100
141 90.8 69.4 104.2





#37

1-Methylnaphthalene

Concen: 21.433 ng/ul

RT: 12.583 min Scan# 1

Delta R.T. -0.006 min

Lab File: BG058269.D

Acq: 15 Jul 2023 20:54

Instrument :

BNA_G

ClientSampleId :

SSTD020519





Tgt Ion:142 Resp: 198062

Ion Ratio Lower Upper

142 100

141 93.5 73.8 110.8

116 3.9 3.0 4.4

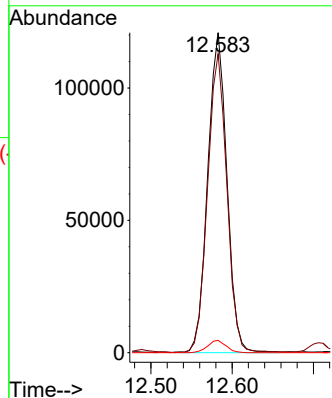

#39

1,2,4,5-Tetrachlorobenzene

Concen: 21.743 ng/ul

RT: 12.730 min Scan# 1641

Delta R.T. -0.006 min

Lab File: BG058269.D

Acq: 15 Jul 2023 20:54

Tgt Ion:216 Resp: 115870




Ion Ratio Lower Upper


216 100

214 81.4 64.1 96.1

179 19.5 16.0 24.0

108 15.3 12.1 18.1



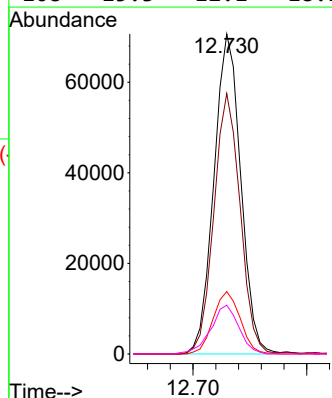





#40
Hexachlorocyclopentadiene
Concen: 15.949 ng/ul
RT: 12.706 min Scan# 1637
Delta R.T. -0.006 min
Lab File: BG058269.D
Acq: 15 Jul 2023 20:54




Instrument :
BNA_G
ClientSampleId :
SSTD020519


Tgt Ion:237 Resp: 53535
Ion Ratio Lower Upper
237 100
235 64.5 49.2 73.8
272 15.6 10.4 15.6



#41
2,4,6-Trichlorophenol
Concen: 22.167 ng/ul
RT: 12.970 min Scan# 1682
Delta R.T. -0.005 min
Lab File: BG058269.D
Acq: 15 Jul 2023 20:54

Tgt Ion:196 Resp: 80063
Ion Ratio Lower Upper
196 100
198 92.2 73.5 110.3
200 31.0 24.8 37.2




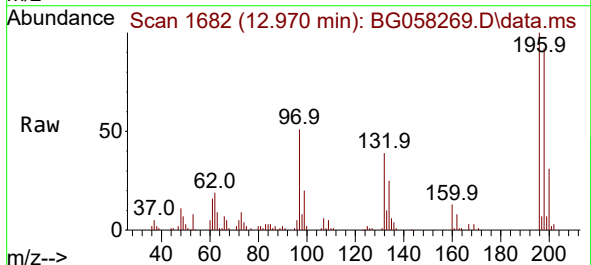




#42
2,4,5-Trichlorophenol
Concen: 21.739 ng/ul
RT: 13.047 min Scan# 1
Delta R.T. 0.000 min
Lab File: BG058269.D
Acq: 15 Jul 2023 20:54




Instrument :
BNA_G
ClientSampleId :
SSTD020519


Tgt Ion:196 Resp: 84918
Ion Ratio Lower Upper
196 100
198 92.7 77.2 115.8
200 30.9 23.8 35.6



#43
1,1'-Biphenyl
Concen: 21.006 ng/ul
RT: 13.370 min Scan# 1750
Delta R.T. -0.006 min
Lab File: BG058269.D
Acq: 15 Jul 2023 20:54

Tgt Ion:154 Resp: 264722
Ion Ratio Lower Upper
154 100
153 41.3 32.6 49.0
76 14.9 11.6 17.4









#44
2-Chloronaphthalene
Concen: 21.116 ng/ul
RT: 13.417 min Scan# 1758
Delta R.T. 0.000 min
Lab File: BG058269.D
Acq: 15 Jul 2023 20:54




Instrument :
BNA_G
ClientSampleId :
SSTD020519


Tgt Ion:162 Resp: 213570
Ion Ratio Lower Upper
162 100
164 35.0 27.7 41.5
127 38.4 30.9 46.3



#45
2-Nitroaniline
Concen: 21.440 ng/ul
RT: 13.617 min Scan# 1792
Delta R.T. -0.006 min
Lab File: BG058269.D
Acq: 15 Jul 2023 20:54

Tgt Ion: 65 Resp: 75393
Ion Ratio Lower Upper
65 100
92 62.4 53.2 79.8
138 90.3 71.1 106.7




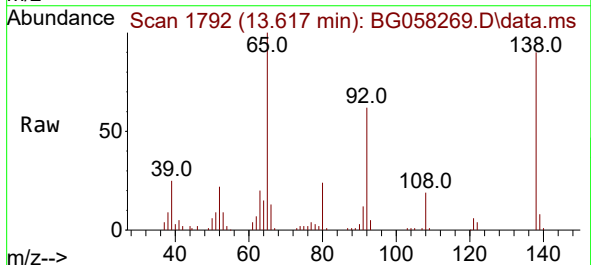




#47
Dimethylphthalate
Concen: 19.479 ng/ul
RT: 13.987 min Scan# 1855
Delta R.T. -0.006 min
Lab File: BG058269.D
Acq: 15 Jul 2023 20:54




Instrument :
BNA_G
ClientSampleId :
SSTD020519


Tgt Ion:163 Resp: 270015
Ion Ratio Lower Upper
163 100
194 3.4 3.0 4.4
164 10.3 8.6 12.8



#48
2,6-Dinitrotoluene
Concen: 20.556 ng/ul
RT: 14.116 min Scan# 1877
Delta R.T. 0.000 min
Lab File: BG058269.D
Acq: 15 Jul 2023 20:54

Tgt Ion:165 Resp: 58489
Ion Ratio Lower Upper
165 100
89 54.5 42.7 64.1
121 18.3 14.8 22.2


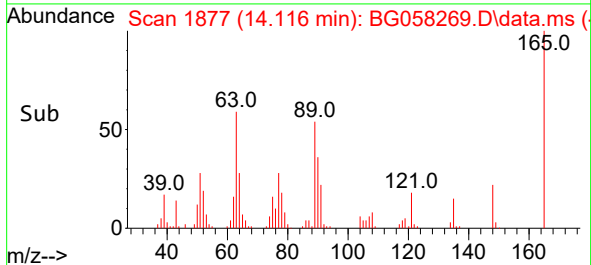






#50
Acenaphthylene
Concen: 21.111 ng/ul
RT: 14.263 min Scan# 1902
Delta R.T. 0.000 min
Lab File: BG058269.D
Acq: 15 Jul 2023 20:54




Instrument :
BNA_G
ClientSampleId :
SSTD020519


Tgt Ion:152 Resp: 343241
Ion Ratio Lower Upper
152 100
151 19.6 15.6 23.4
153 13.1 10.5 15.7



#51
3-Nitroaniline
Concen: 19.452 ng/ul
RT: 14.445 min Scan# 1933
Delta R.T. -0.006 min
Lab File: BG058269.D
Acq: 15 Jul 2023 20:54

Tgt Ion:138 Resp: 46774
Ion Ratio Lower Upper
138 100
108 11.4 8.2 12.2
92 125.1 100.2 150.4


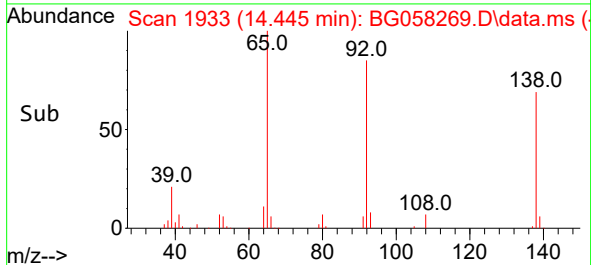






#52
Acenaphthene
Concen: 20.909 ng/ul
RT: 14.604 min Scan# 1960
Delta R.T. 0.000 min
Lab File: BG058269.D
Acq: 15 Jul 2023 20:54




Instrument :
BNA_G
ClientSampleId :
SSTD020519


Tgt Ion:153 Resp: 233275
Ion Ratio Lower Upper
153 100
152 49.1 36.5 54.7
154 90.4 70.5 105.7



#53
2,4-Dinitrophenol
Concen: 16.370 ng/ul
RT: 14.657 min Scan# 1969
Delta R.T. 0.000 min
Lab File: BG058269.D
Acq: 15 Jul 2023 20:54

Tgt Ion:184 Resp: 24283
Ion Ratio Lower Upper
184 100
63 64.3 51.1 76.7
154 53.0 43.3 64.9









#55
4-Nitrophenol
Concen: 17.168 ng/ul
RT: 14.757 min Scan# 1986
Delta R.T. -0.006 min
Lab File: BG058269.D
Acq: 15 Jul 2023 20:54




Instrument :
BNA_G
ClientSampleId :
SSTD020519


Tgt Ion:109 Resp: 31003
Ion Ratio Lower Upper
109 100
139 130.3 119.0 178.4
65 146.1 135.5 203.3

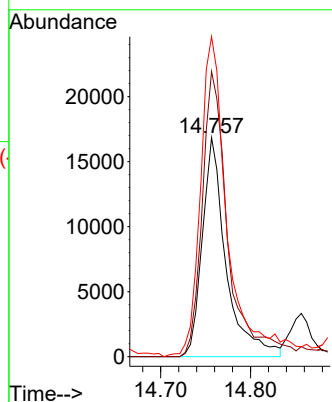

#56
Dibenzofuran
Concen: 20.900 ng/ul
RT: 14.939 min Scan# 2017
Delta R.T. 0.000 min
Lab File: BG058269.D
Acq: 15 Jul 2023 20:54

Tgt Ion:168 Resp: 331472
Ion Ratio Lower Upper
168 100
139 34.5 27.6 41.4

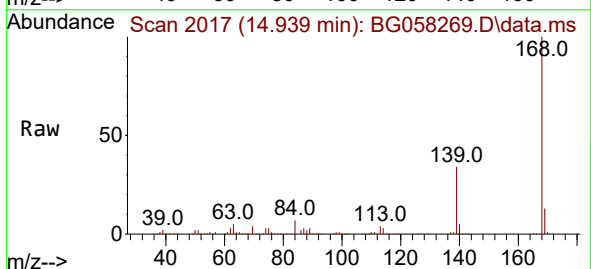



#57

2,4-Dinitrotoluene

Concen: 20.736 ng/ul

RT: 14.903 min Scan# 2011

Delta R.T. 0.000 min

Lab File: BG058269.D

Acq: 15 Jul 2023 20:54

Instrument :

BNA_G

ClientSampleId :

SSTD020519





Tgt Ion:165 Resp: 83596

Ion Ratio Lower Upper

165 100

63 46.0 35.8 53.8

182 2.3 1.6 2.4



#58

2,3,4,6-Tetrachlorophenol

Concen: 20.984 ng/ul

RT: 15.162 min Scan# 2055

Delta R.T. -0.005 min

Lab File: BG058269.D

Acq: 15 Jul 2023 20:54

Tgt Ion:232 Resp: 74618




Ion Ratio Lower Upper


232 100

131 39.3 30.5 45.7

130 2.4 1.4 2.0#

166 29.1 22.6 34.0



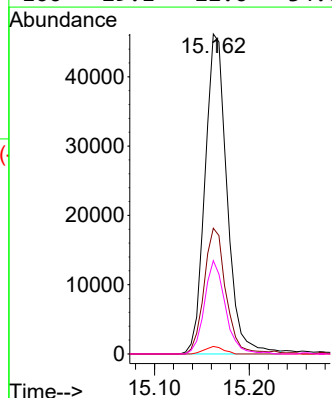





#59
Diethylphthalate
Concen: 19.133 ng/ul
RT: 15.350 min Scan# 2087
Delta R.T. -0.005 min
Lab File: BG058269.D
Acq: 15 Jul 2023 20:54




Instrument :
BNA_G
ClientSampleId :
SSTD020519


Tgt Ion:149 Resp: 276816
Ion Ratio Lower Upper
149 100
177 21.6 17.8 26.8
150 12.5 10.1 15.1



#61
Fluorene
Concen: 20.669 ng/ul
RT: 15.585 min Scan# 2127
Delta R.T. -0.006 min
Lab File: BG058269.D
Acq: 15 Jul 2023 20:54

Tgt Ion:166 Resp: 268968
Ion Ratio Lower Upper
166 100
165 98.7 79.1 118.7
167 12.6 10.7 16.1









#62
4-Chlorophenyl-phenylether
Concen: 20.912 ng/ul
RT: 15.573 min Scan# 2125
Delta R.T. -0.006 min
Lab File: BG058269.D
Acq: 15 Jul 2023 20:54




Instrument :
BNA_G
ClientSampleId :
SSTD020519


Tgt Ion:204 Resp: 143987
Ion Ratio Lower Upper
204 100
206 31.1 25.8 38.6
141 50.8 41.8 62.6



#63
4-Nitroaniline
Concen: 14.132 ng/ul
RT: 15.609 min Scan# 2131
Delta R.T. -0.006 min
Lab File: BG058269.D
Acq: 15 Jul 2023 20:54

Tgt Ion:138 Resp: 30441
Ion Ratio Lower Upper
138 100
92 58.2 43.8 65.8
108 79.9 58.8 88.2









#66
 4,6-Dinitro-2-methylphenol
 Concen: 17.423 ng/ul
 RT: 15.667 min Scan# 2141
 Delta R.T. 0.000 min
 Lab File: BG058269.D
 Acq: 15 Jul 2023 20:54




Instrument :
 BNA_G
 ClientSampleId :
 SSTD020519


Tgt Ion:198 Resp: 39526
 Ion Ratio Lower Upper
 198 100
 182 3.5 3.1 4.7
 77 22.6 17.9 26.9



#67
 N-Nitrosodiphenylamine
 Concen: 20.736 ng/ul
 RT: 15.791 min Scan# 2162
 Delta R.T. -0.006 min
 Lab File: BG058269.D
 Acq: 15 Jul 2023 20:54

Tgt Ion:169 Resp: 225450
 Ion Ratio Lower Upper
 169 100
 168 70.4 54.2 81.2
 167 38.6 30.8 46.2









#68
4-Bromophenyl-phenylether
Concen: 21.491 ng/ul
RT: 16.472 min Scan# 21
Delta R.T. 0.000 min
Lab File: BG058269.D
Acq: 15 Jul 2023 20:54




Instrument :
BNA_G
ClientSampleId :
SSTD020519


Tgt Ion:248 Resp: 96376
Ion Ratio Lower Upper
248 100
250 99.3 78.3 117.5
141 60.5 49.1 73.7



#69
Hexachlorobenzene
Concen: 22.002 ng/ul
RT: 16.590 min Scan# 2298
Delta R.T. -0.006 min
Lab File: BG058269.D
Acq: 15 Jul 2023 20:54

Tgt Ion:284 Resp: 110471
Ion Ratio Lower Upper
284 100
142 26.4 21.9 32.9
249 32.1 25.0 37.6









#70
 Atrazine
 Concen: 20.120 ng/ul
 RT: 16.737 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: BG058269.D
 Acq: 15 Jul 2023 20:54




Instrument :
 BNA_G
 ClientSampleId :
 SST020519


Tgt Ion:200 Resp: 89455
 Ion Ratio Lower Upper
 200 100
 173 26.4 20.0 30.0
 215 47.8 35.8 53.8

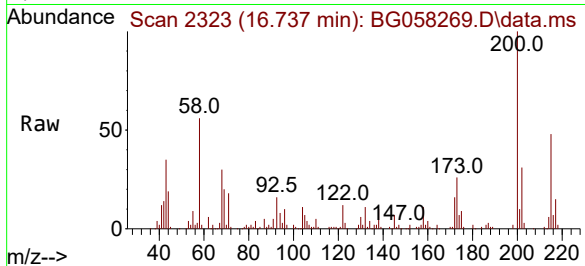

#71
 Pentachlorophenol
 Concen: 18.373 ng/ul
 RT: 16.936 min Scan# 2357
 Delta R.T. -0.006 min
 Lab File: BG058269.D
 Acq: 15 Jul 2023 20:54

Tgt Ion:266 Resp: 55382
 Ion Ratio Lower Upper
 266 100
 264 65.0 51.5 77.3
 268 65.9 49.0 73.4




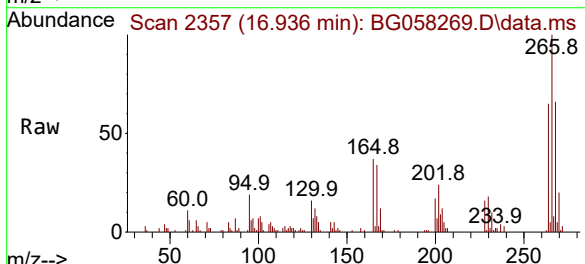




#72
Phenanthrene
Concen: 20.544 ng/ul
RT: 17.324 min Scan# 2424
Delta R.T. -0.006 min
Lab File: BG058269.D
Acq: 15 Jul 2023 20:54




Instrument :
BNA_G
ClientSampleId :
SSTD020519


Tgt Ion:178 Resp: 426937
Ion Ratio Lower Upper
178 100
179 15.8 12.8 19.2
176 19.9 15.7 23.5

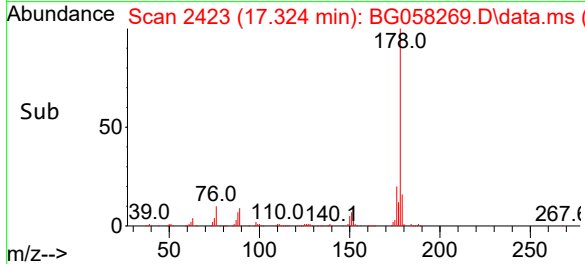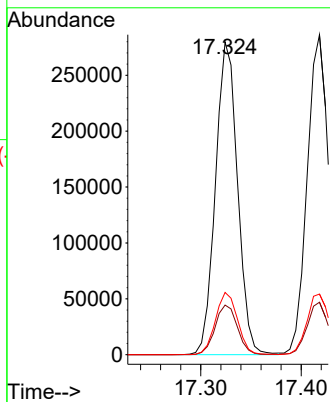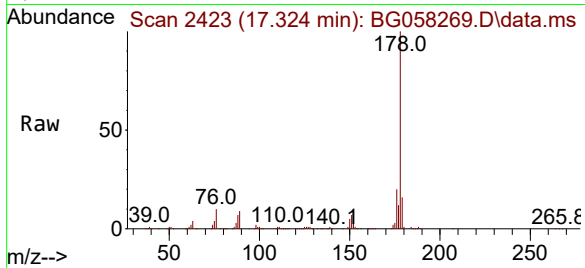

#74
Anthracene
Concen: 20.610 ng/ul
RT: 17.418 min Scan# 2439
Delta R.T. -0.006 min
Lab File: BG058269.D
Acq: 15 Jul 2023 20:54

Tgt Ion:178 Resp: 433417
Ion Ratio Lower Upper
178 100
179 16.4 12.6 18.8
176 18.9 15.4 23.2


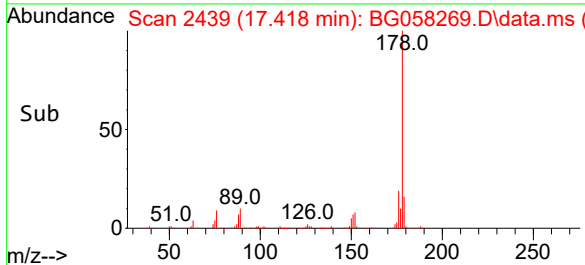

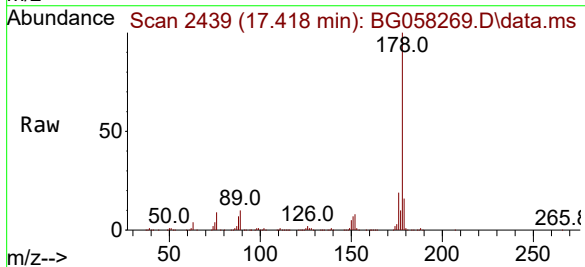




#75
1,2,3,4-Tetrachlorobenzene
Concen: 22.565 ng/uL
RT: 13.341 min Scan# 1745
Delta R.T. 0.000 min
Lab File: BG058269.D
Acq: 15 Jul 2023 20:54




Instrument :
BNA_G
ClientSampleId :
SSTD020519


Tgt Ion:216 Resp: 122264
Ion Ratio Lower Upper
216 100
214 78.6 64.8 97.2
218 48.0 39.1 58.7



#76
Pentachlorobenzene
Concen: 22.279 ng/uL
RT: 14.856 min Scan# 2003
Delta R.T. -0.006 min
Lab File: BG058269.D
Acq: 15 Jul 2023 20:54

Tgt Ion:250 Resp: 128923
Ion Ratio Lower Upper
250 100
248 62.7 52.8 79.2
252 64.6 52.4 78.6







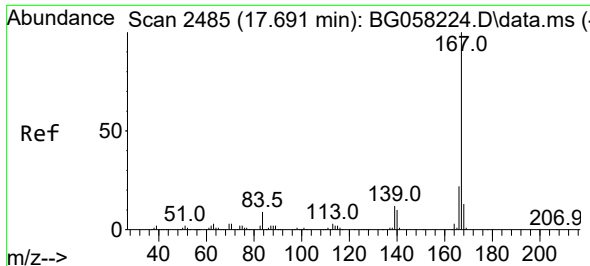

#77
 Carbazole
 Concen: 20.716 ng/ul
 RT: 17.688 min Scan# 2485
 Delta R.T. -0.006 min
 Lab File: BG058269.D
 Acq: 15 Jul 2023 20:54




Instrument :
 BNA_G
 ClientSampleId :
 SST020519


Tgt Ion:167 Resp: 394000
 Ion Ratio Lower Upper
 167 100
 166 23.3 17.5 26.3
 139 12.0 9.5 14.3

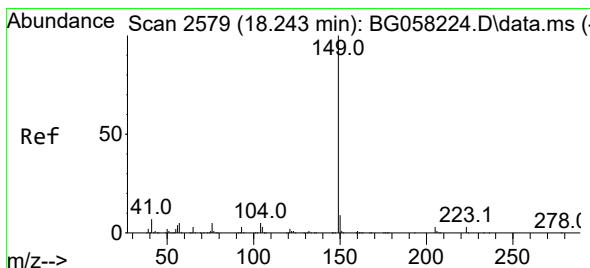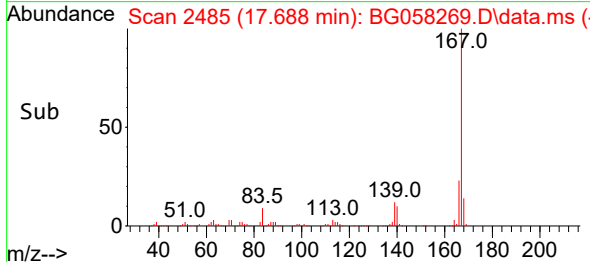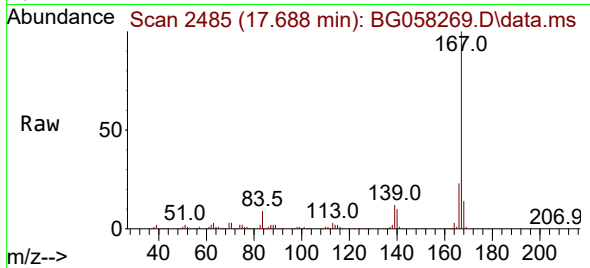

#78
 Di-n-butylphthalate
 Concen: 20.122 ng/ul
 RT: 18.241 min Scan# 2579
 Delta R.T. -0.006 min
 Lab File: BG058269.D
 Acq: 15 Jul 2023 20:54

Tgt Ion:149 Resp: 487515
 Ion Ratio Lower Upper
 149 100
 150 9.2 7.4 11.2
 104 4.8 3.9 5.9

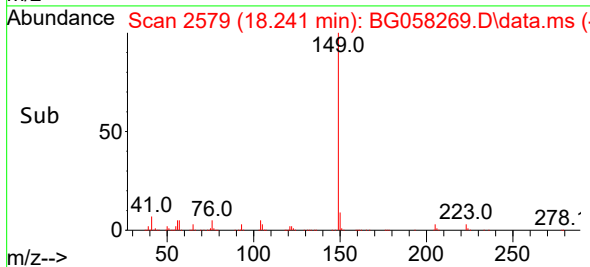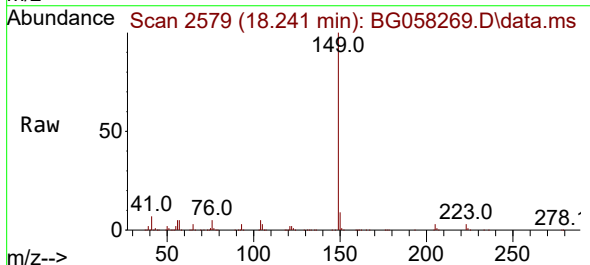



#80

Fluoranthene

Concen: 19.974 ng/ul

RT: 19.339 min Scan# 21

Delta R.T. -0.006 min

Lab File: BG058269.D

Acq: 15 Jul 2023 20:54

Instrument :

BNA_G

ClientSampleId :

SSTD020519





Tgt Ion:202 Resp: 517098

Ion Ratio Lower Upper

202 100

101 10.7 9.1 13.7

100 8.4 7.1 10.7



#82

Pyrene

Concen: 20.024 ng/ul

RT: 19.698 min Scan# 2827

Delta R.T. -0.006 min

Lab File: BG058269.D

Acq: 15 Jul 2023 20:54




Tgt Ion:202 Resp: 521805


Ion Ratio Lower Upper

202 100

101 14.0 10.2 15.2

100 11.6 8.9 13.3


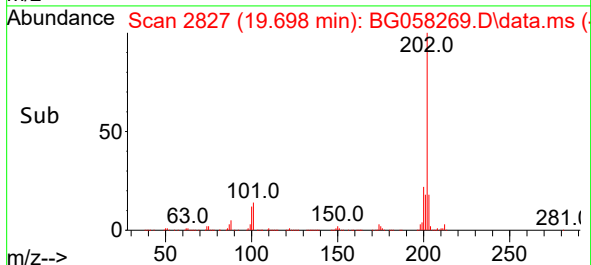






#83
Butylbenzylphthalate
Concen: 20.760 ng/ul
RT: 20.585 min Scan# 2978
Delta R.T. -0.006 min
Lab File: BG058269.D
Acq: 15 Jul 2023 20:54




Instrument :
BNA_G
ClientSampleId :
SSTD020519


Tgt Ion:149 Resp: 219376
Ion Ratio Lower Upper
149 100
91 70.7 56.5 84.7
206 21.8 17.4 26.0

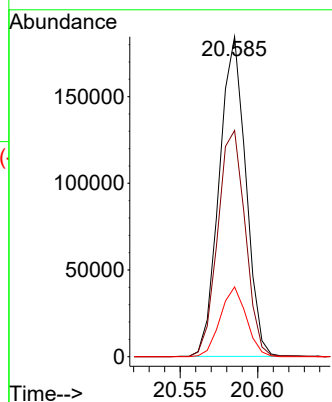

#84
3,3'-Dichlorobenzidine
Concen: 22.040 ng/ul
RT: 21.437 min Scan# 3123
Delta R.T. -0.006 min
Lab File: BG058269.D
Acq: 15 Jul 2023 20:54

Tgt Ion:252 Resp: 189276
Ion Ratio Lower Upper
252 100
254 63.4 50.7 76.1
126 9.0 6.6 10.0

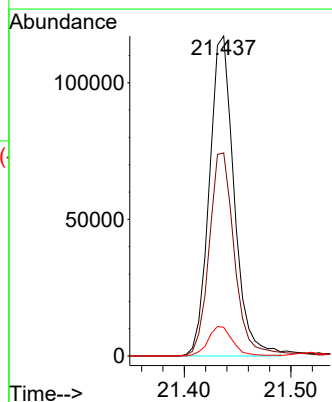



#85

Benzo(a)anthracene

Concen: 20.811 ng/ul

RT: 21.519 min Scan# 3137

Delta R.T. -0.006 min

Lab File: BG058269.D

Acq: 15 Jul 2023 20:54

Instrument :

BNA_G

ClientSampleId :

SSTD020519





Tgt Ion:228 Resp: 530071

Ion Ratio Lower Upper

228 100

229 20.3 16.0 24.0

226 27.5 22.0 33.0



#86

Bis(2-ethylhexyl)phthalate

Concen: 21.100 ng/ul

RT: 21.419 min Scan# 3120

Delta R.T. -0.006 min

Lab File: BG058269.D

Acq: 15 Jul 2023 20:54




Tgt Ion:149 Resp: 319514


Ion Ratio Lower Upper

149 100

167 26.6 20.9 31.3

279 3.9 3.1 4.7





#87

Chrysene

Concen: 21.079 ng/ul

RT: 21.578 min Scan# 31

Delta R.T. -0.011 min

Lab File: BG058269.D

Acq: 15 Jul 2023 20:54

Instrument :

BNA_G

ClientSampleId :

SSTD020519





Tgt Ion:228 Resp: 503305

Ion Ratio Lower Upper

228 100

226 31.0 24.4 36.6

229 20.2 15.5 23.3

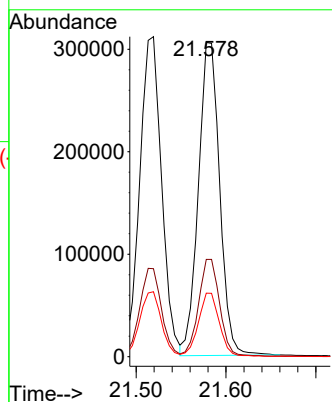

#89

Di-n-octyl phthalate

Concen: 20.594 ng/ul




RT: 22.594 min Scan# 3320


Delta R.T. -0.011 min

Lab File: BG058269.D

Acq: 15 Jul 2023 20:54

Tgt Ion:149 Resp: 565384









#90
Benzo(b)fluoranthene
Concen: 20.478 ng/ul
RT: 23.676 min Scan# 3505
Delta R.T. -0.011 min
Lab File: BG058269.D
Acq: 15 Jul 2023 20:54




Instrument :
BNA_G
ClientSampleId :
SSTD020519


Tgt Ion:252 Resp: 566539
Ion Ratio Lower Upper
252 100
253 22.3 18.1 27.1
125 9.1 7.5 11.3



#91
Benzo(k)fluoranthene
Concen: 20.321 ng/ul
RT: 23.740 min Scan# 3515
Delta R.T. -0.011 min
Lab File: BG058269.D
Acq: 15 Jul 2023 20:54

Tgt Ion:252 Resp: 551046
Ion Ratio Lower Upper
252 100
253 22.3 17.7 26.5
125 8.4 7.4 11.2




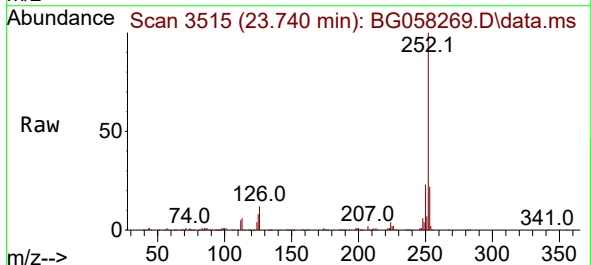




#93
Benzo(a)pyrene
Concen: 20.267 ng/ul
RT: 24.528 min Scan# 3649
Delta R.T. -0.011 min
Lab File: BG058269.D
Acq: 15 Jul 2023 20:54




Instrument :
BNA_G
ClientSampleId :
SSTD020519


Tgt Ion:252 Resp: 496277
Ion Ratio Lower Upper
252 100
253 21.7 17.8 26.6
125 9.9 8.3 12.5



#94
Indeno(1,2,3-cd)pyrene
Concen: 19.714 ng/ul
RT: 28.253 min Scan# 4283
Delta R.T. -0.017 min
Lab File: BG058269.D
Acq: 15 Jul 2023 20:54

Tgt Ion:276 Resp: 641034
Ion Ratio Lower Upper
276 100
138 18.0 14.0 21.0
277 25.9 19.4 29.2





#95

Dibenzo(a,h)anthracene

Concen: 20.278 ng/ul

RT: 28.305 min Scan# 41

Delta R.T. -0.017 min

Lab File: BG058269.D

Acq: 15 Jul 2023 20:54

Instrument :

BNA_G

ClientSampleId :

SSTD020519





Tgt Ion:278 Resp: 543737

Ion Ratio Lower Upper

278 100

139 13.3 11.3 16.9

279 23.9 18.9 28.3

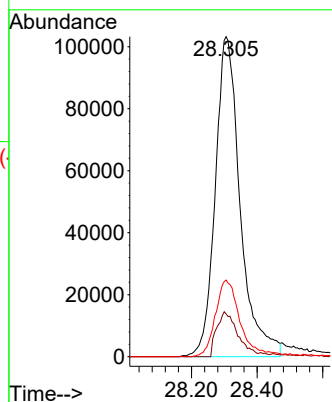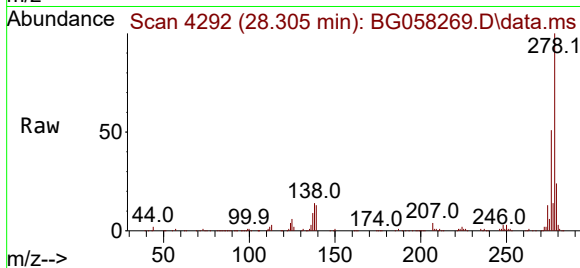

#96

Benzo(g,h,i)perylene

Concen: 18.548 ng/ul

RT: 29.375 min Scan# 4474

Delta R.T. -0.017 min

Lab File: BG058269.D

Acq: 15 Jul 2023 20:54

Tgt Ion:276 Resp: 492632

Ion Ratio Lower Upper

276 100

138 17.3 14.2 21.2

277 23.7 18.6 27.8

