

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071323\
Data File : BG058260.D
Acq On : 15 Jul 2023 13:15
Operator : CG/JU
Sample : 03437-17
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A46H1




Manual IntegrationsAPPROVED

Quant Time: Jul 15 22:36:36 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 13 14:01:20 2023
Response via : Initial Calibration

Reviewed By :Yogesh
Patel

07/17/2023
Supervised By :mohammad
ahmed

Ion 131.00 (130.70 to 131.70): BG058260.D\data.ms
Ion 133.00 (132.70 to 133.70): BG058260.D\data.ms
Ion 69.00 (68.70 to 69.70): BG058260.D\data.ms

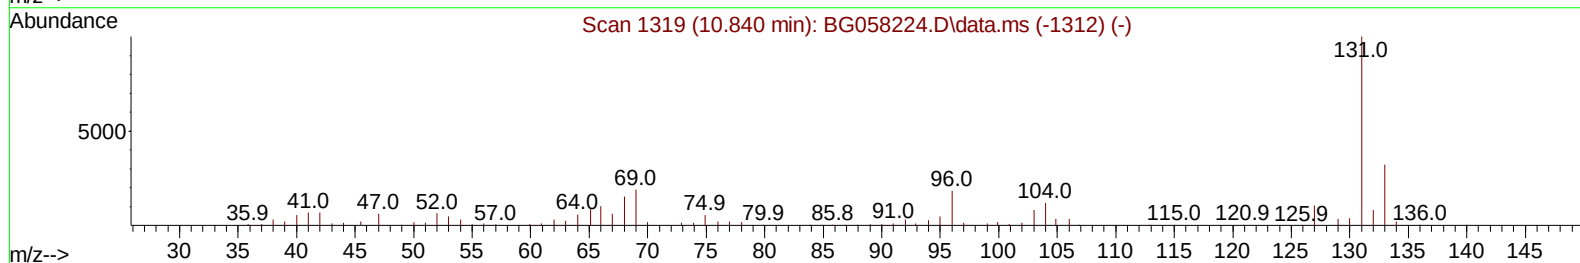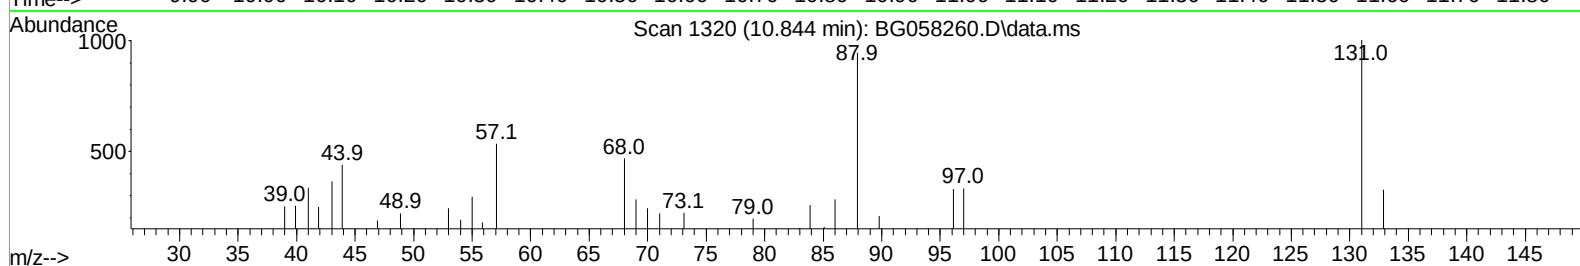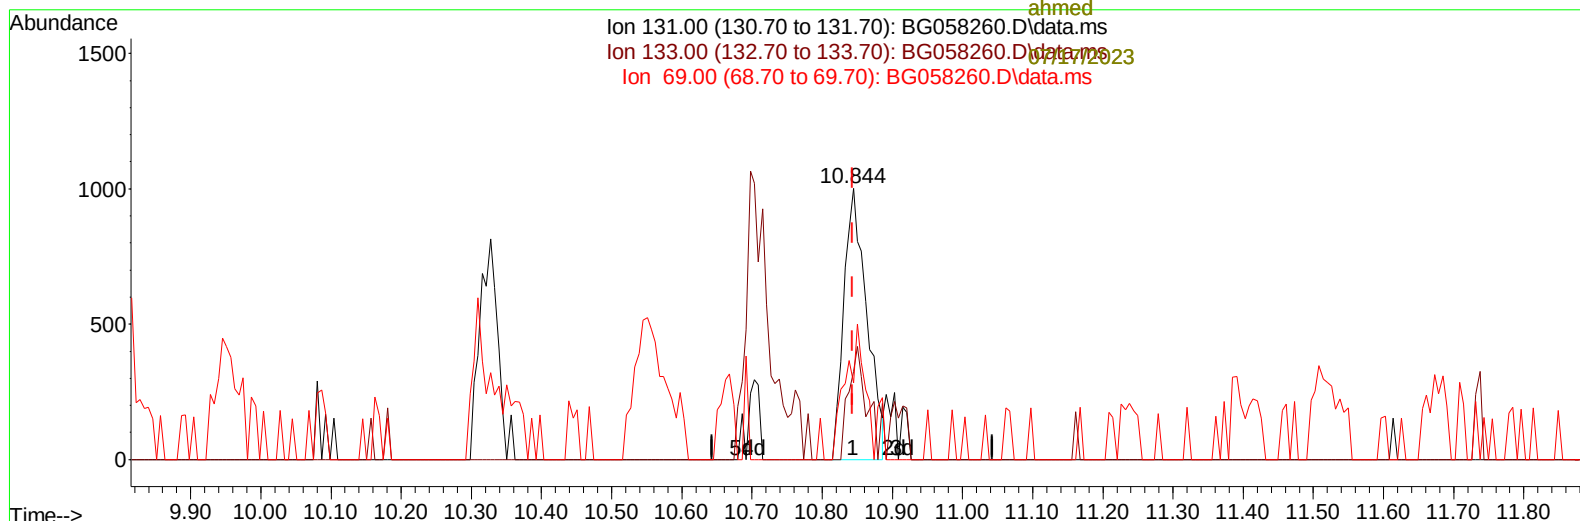

TIC: BG058260.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.844min (+ 0.001) 0.36 ng/ul

response 2272

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	31.10	32.50
69.00	18.00	28.22#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071323\
 Data File : BG058260.D
 Acq On : 15 Jul 2023 13:15
 Operator : CG/JU
 Sample : 03437-17
 Misc :
 ALS Vial : 70 Sample Multiplier: 1




Instrument :
 BNA_G
 ClientSampleId :
 A46H1

Manual IntegrationsAPPROVED

Quant Time: Jul 15 22:36:36 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 13 14:01:20 2023
 Response via : Initial Calibration

Reviewed By :Yogesh
 Patel

07/17/2023
 Supervised By :mohammad
 ahmed

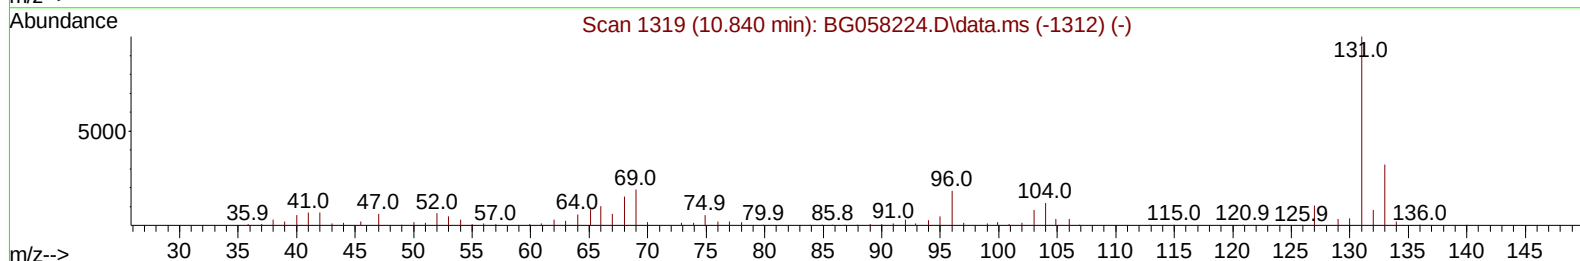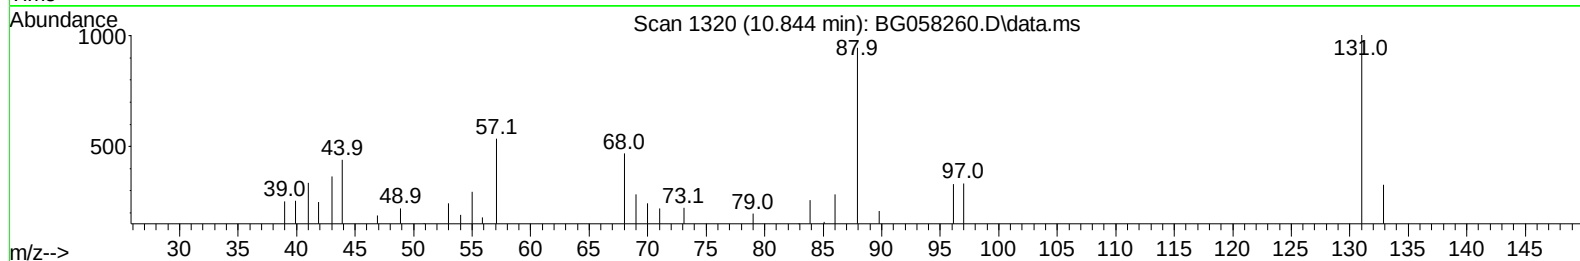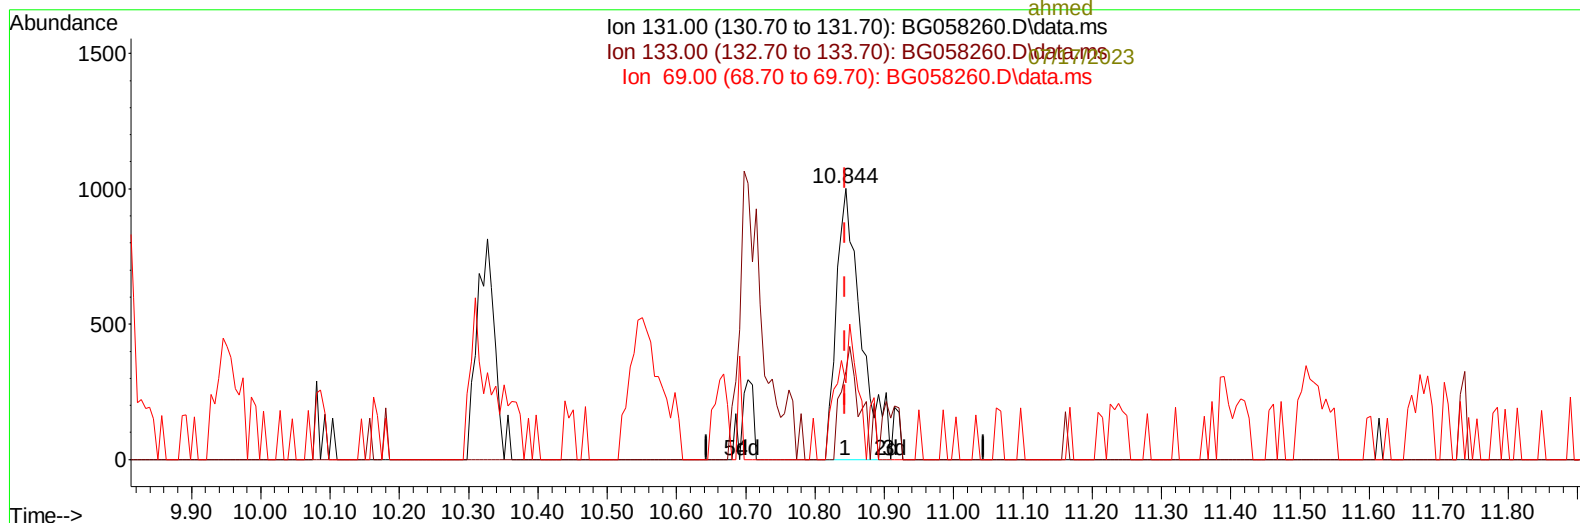

TIC: BG058260.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.844min (+ 0.001) 0.40 ng/ul m

response 2499

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	31.10	32.50
69.00	18.00	28.22#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071323\
 Data File : BG058260.D
 Acq On : 15 Jul 2023 13:15
 Operator : CG/JU
 Sample : 03437-17
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A46H1

Manual IntegrationsAPPROVED

Reviewed By :Yogesh
 Patel

07/17/2023
 Supervised By :mohammad
 ahmed

Quant Time: Jul 15 23:37:07 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 13 14:01:20 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----07/17/2023						
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.901	152	50655	20.000	ng/ul	0.00
20) Naphthalene-d8	10.703	136	250475	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.540	164	181927	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.284	188	428446	20.000	ng/ul	0.00
79) Chrysene-d12	21.538	240	372861	20.000	ng/ul	0.00
88) Perylene-d12	24.675	264	449062	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.347	96	2830	1.956	ng/uL	0.00
4) Pyridine-d5	3.758	84	7390	1.683	ng/ul	0.00
7) Phenol-d5	7.066	99	69297	13.396	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.225	67	44925	14.411	ng/ul	0.00
11) 2-Chlorophenol-d4	7.437	132	49042	13.745	ng/ul	0.00
15) 4-Methylphenol-d8	8.612	113	5173	1.325	ng/ul	0.00
21) Nitrobenzene-d5	9.064	128	28353	13.888	ng/ul	0.00
24) 2-Nitrophenol-d4	9.781	143	32132	14.976	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.327	165	49032	11.913	ng/ul	0.00
31) 4-Chloroaniline-d4	10.844	131	2499m	0.400	ng/ul	0.00
46) Dimethylphthalate-d6	13.941	166	212062	14.773	ng/ul	0.00
49) Acenaphthylene-d8	14.234	160	224522	14.334	ng/ul	0.00
54) 4-Nitrophenol-d4	14.746	143	28762	11.341	ng/ul	0.00
60) Fluorene-d10	15.527	176	196701	16.136	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.650	200	26000	11.176	ng/ul	0.00
73) Anthracene-d10	17.384	188	182896	9.200	ng/ul	0.00
81) Pyrene-d10	19.669	212	305122	12.993	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.458	264	119665	5.230	ng/ul	-0.01
Target Compounds						
					Qvalue	
16) Acetophenone	8.723	105	23486	3.626	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.414	149	42365	2.662	ng/ul#	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071323\
Data File : BG058260.D
Acq On : 15 Jul 2023 13:15
Operator : CG/JU
Sample : 03437-17
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A46H1

Manual IntegrationsAPPROVED

Quant Time: Jul 15 23:37:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 13 14:01:20 2023
Response via : Initial Calibration

Reviewed By :Yogesh
Patel

07/17/2023
Supervised By :mohammad
ahmed

07/17/2023

