




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071323\
 Data File : BG058265.D
 Acq On : 15 Jul 2023 17:25
 Operator : CG/JU
 Sample : 03457-02
 Misc :
 ALS Vial : 76 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0C52

Manual IntegrationsAPPROVED

Quant Time: Jul 15 22:37:55 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 13 14:01:20 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/17/2023
 Supervised By :mohammad ahmed 07/17/2023

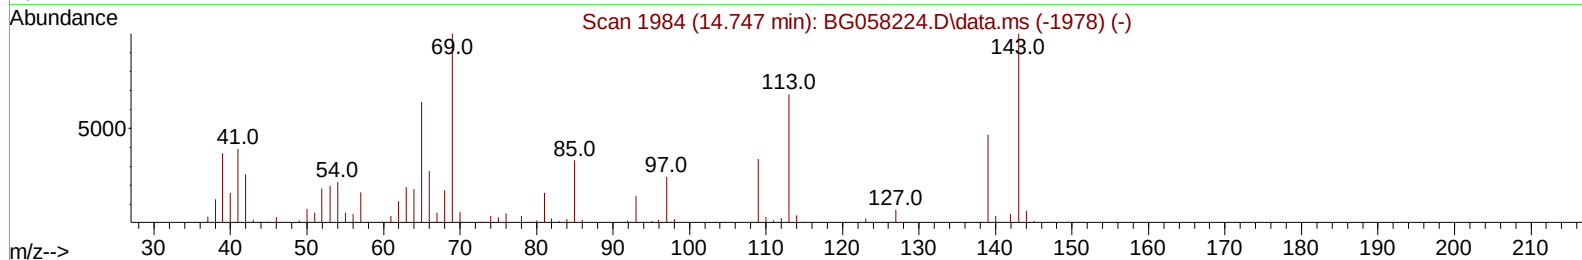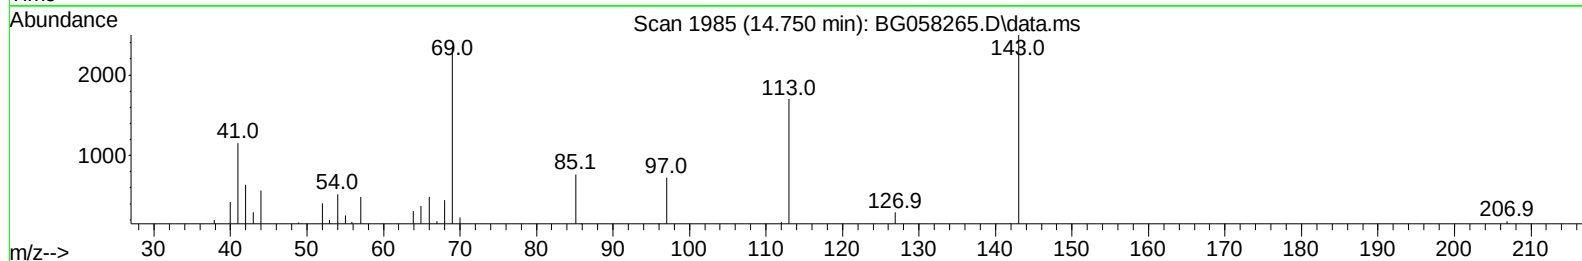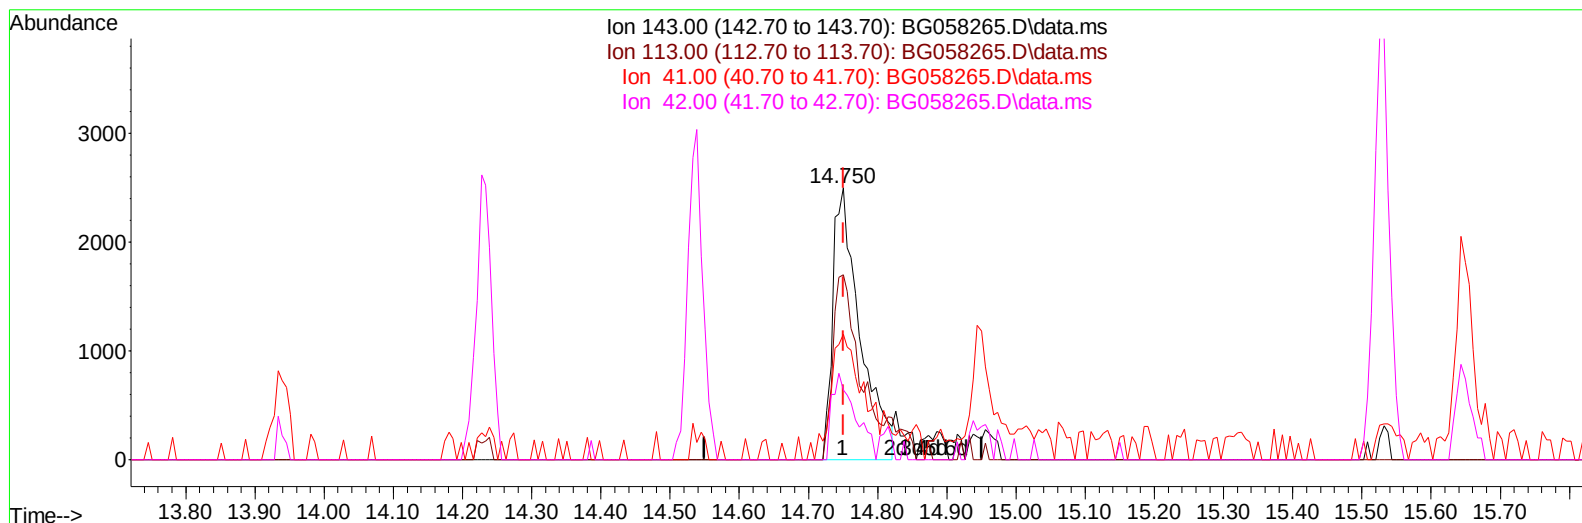

TIC: BG058265.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.750min (-0.000) 3.10 ng/ul

response 6805

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	66.40	68.08
41.00	40.50	46.18
42.00	27.50	25.47




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071323\
 Data File : BG058265.D
 Acq On : 15 Jul 2023 17:25
 Operator : CG/JU
 Sample : 03457-02
 Misc :
 ALS Vial : 76 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0C52

Manual IntegrationsAPPROVED

Quant Time: Jul 15 22:37:55 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 13 14:01:20 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/17/2023
 Supervised By :mohammad ahmed 07/17/2023

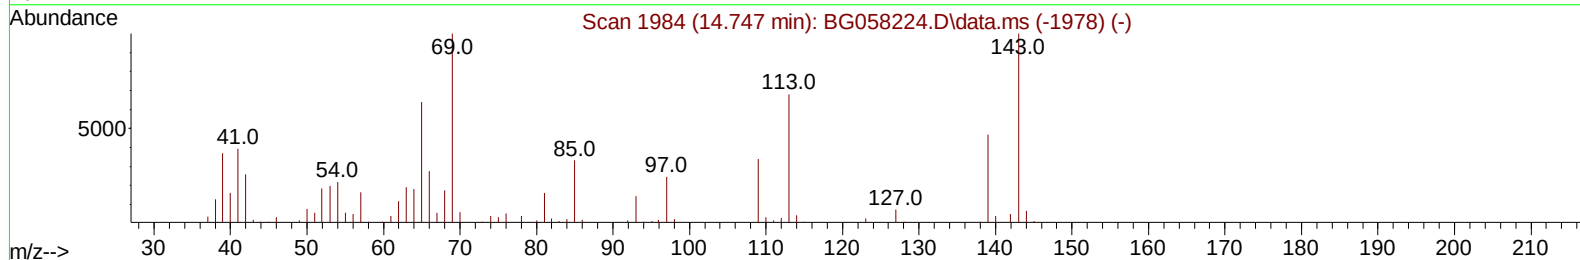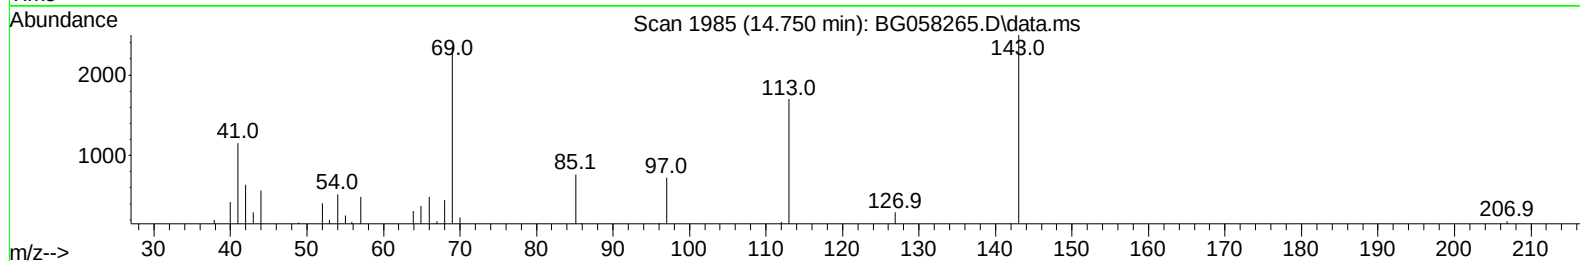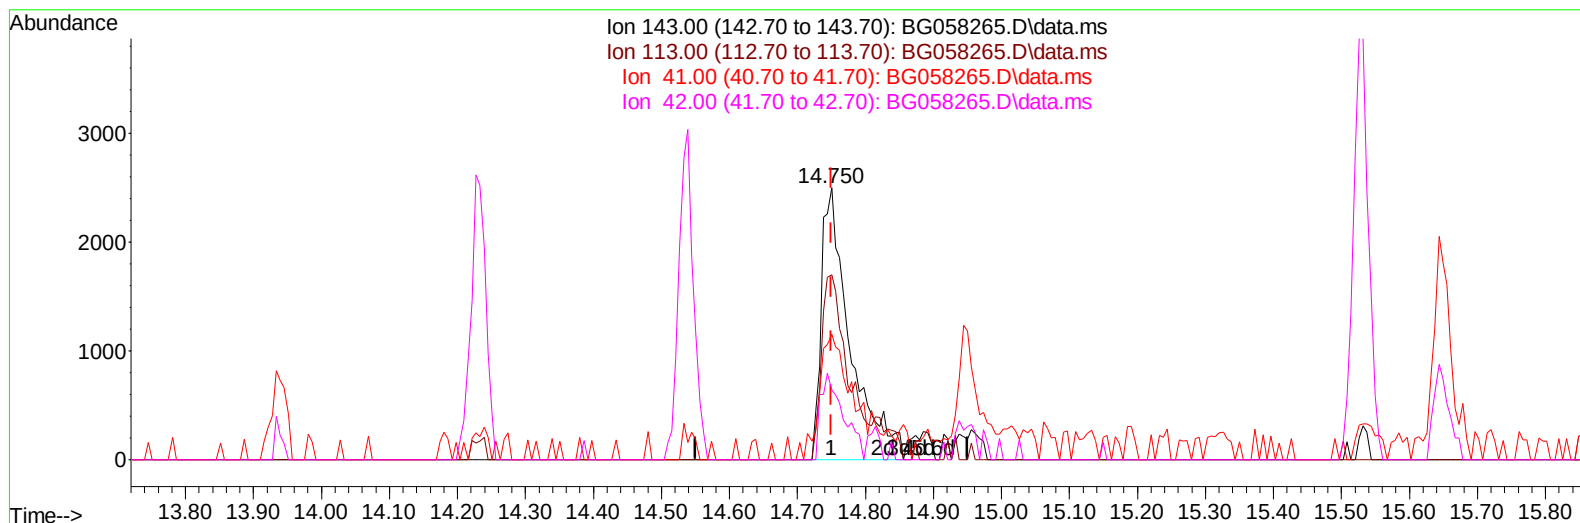

TIC: BG058265.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.750min (-0.000) 3.32 ng/ul m

response 7287

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	66.40	68.08
41.00	40.50	46.18
42.00	27.50	25.47

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071323\
 Data File : BG058265.D
 Acq On : 15 Jul 2023 17:25
 Operator : CG/JU
 Sample : 03457-02
 Misc :
 ALS Vial : 76 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0C52

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/17/2023
 Supervised By :mohammad ahmed 07/17/2023

Quant Time: Jul 15 23:51:11 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 13 14:01:20 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.899	152	42687	20.000	ng/ul	0.00
20) Naphthalene-d8	10.702	136	207845	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.539	164	157279	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.282	188	377242	20.000	ng/ul	0.00
79) Chrysene-d12	21.536	240	339925	20.000	ng/ul	0.00
88) Perylene-d12	24.674	264	414373	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.340	96	1895	1.554	ng/uL	0.00
4) Pyridine-d5	3.751	84	27154	7.337	ng/ul	0.00
7) Phenol-d5	7.065	99	20812	4.774	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.224	67	65052	24.762	ng/ul	0.00
11) 2-Chlorophenol-d4	7.435	132	59577	19.815	ng/ul	0.00
15) 4-Methylphenol-d8	8.604	113	41785	12.703	ng/ul	0.00
21) Nitrobenzene-d5	9.063	128	40161	23.707	ng/ul	0.00
24) 2-Nitrophenol-d4	9.785	143	42766	24.020	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.326	165	78980	23.124	ng/ul	0.00
31) 4-Chloroaniline-d4	10.837	131	108117	20.879	ng/ul	0.00
46) Dimethylphthalate-d6	13.939	166	293231	23.629	ng/ul	0.00
49) Acenaphthylene-d8	14.233	160	339349	25.060	ng/ul	0.00
54) 4-Nitrophenol-d4	14.750	143	7287m	3.324	ng/ul	0.00
60) Fluorene-d10	15.532	176	267806	25.411	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.649	200	34387	16.787	ng/ul	0.00
73) Anthracene-d10	17.382	188	452944	25.875	ng/ul	0.00
81) Pyrene-d10	19.668	212	542506	25.341	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.456	264	573077	27.145	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071323\
Data File : BG058265.D
Acq On : 15 Jul 2023 17:25
Operator : CG/JU
Sample : 03457-02
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0C52

Manual IntegrationsAPPROVED

Quant Time: Jul 15 23:51:11 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 13 14:01:20 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/17/2023
Supervised By :mohammad ahmed 07/17/2023

