

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071323\
 Data File : BG058225.D
 Acq On : 14 Jul 2023 10:50
 Operator : CG/JU
 Sample : PB153997BL
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK997

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG058225.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.348	40	44	51	rVB	23030	33554	1.25%	0.123%
2	3.753	108	113	133	rBV	326542	565752	21.03%	2.070%
3	4.088	166	170	175	rBV2	3696	5773	0.21%	0.021%
4	7.067	670	677	697	rBV	370127	665919	24.75%	2.437%
5	7.231	698	705	720	rVV	282781	492444	18.30%	1.802%
6	7.437	732	740	753	rVB	334711	609633	22.66%	2.231%
7	7.901	812	819	832	rVB	278420	483187	17.96%	1.768%
8	8.606	931	939	953	rBV	449441	814780	30.28%	2.981%
9	8.718	956	958	964	rVB3	1439	2823	0.10%	0.010%
10	9.065	1006	1017	1033	rBV	353229	650001	24.16%	2.378%
11	9.787	1131	1140	1150	rBV	292033	537334	19.97%	1.966%
12	10.328	1222	1232	1253	rBV	436745	827698	30.76%	3.029%
13	10.704	1286	1296	1306	rBV	437297	799005	29.70%	2.924%
14	10.839	1311	1319	1330	rBV	441161	841758	31.28%	3.080%
15	12.290	1561	1566	1575	rVB	6625	10600	0.39%	0.039%
16	13.430	1755	1760	1766	rVB3	6423	10054	0.37%	0.037%
17	13.947	1841	1848	1857	rBV	834697	1242020	46.16%	4.545%
18	14.235	1890	1897	1912	rBV	968420	1542749	57.34%	5.645%
19	14.541	1942	1949	1960	rBV	749764	1171604	43.54%	4.287%
20	14.746	1977	1984	2004	rBV	301989	605885	22.52%	2.217%
21	15.534	2111	2118	2130	rBV	1264379	1950738	72.50%	7.138%
22	15.651	2132	2138	2153	rVV	379869	589185	21.90%	2.156%
23	15.774	2156	2159	2163	rVB3	5976	7673	0.29%	0.028%
24	17.079	2376	2381	2384	rVB2	1712	2762	0.10%	0.010%
25	17.284	2409	2416	2426	rBV	919290	1472324	54.72%	5.387%
26	17.384	2426	2433	2443	rVV	1323379	2097204	77.94%	7.674%
27	19.235	2743	2748	2756	rVB	18312	27835	1.03%	0.102%
28	19.311	2756	2761	2766	rBV	15329	23234	0.86%	0.085%
29	19.588	2805	2808	2810	rBV3	4920	4899	0.18%	0.018%
30	19.676	2816	2823	2835	rBV	1657282	2444856	90.86%	8.946%
31	19.987	2873	2876	2879	rBV3	2058	2753	0.10%	0.010%
32	20.633	2983	2986	2989	rVB3	6439	5826	0.22%	0.021%
33	20.751	3004	3006	3009	rBV4	2129	2757	0.10%	0.010%
34	21.004	3046	3049	3052	rBV5	2836	4817	0.18%	0.018%
35	21.186	3077	3080	3083	rBV4	3786	5393	0.20%	0.020%
36	21.538	3133	3140	3152	rBV2	890073	1554247	57.76%	5.687%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071323\
Data File : BG058225.D
Acq On : 14 Jul 2023 10:50
Operator : CG/JU
Sample : PB153997BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK997

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Title : SVOA CALIBRATION

37	21.715	3168	3170	3175	rVB4	6096	8503	0.32%	0.031%
38	22.308	3266	3271	3276	rBV3	16104	29033	1.08%	0.106%
39	22.978	3380	3385	3394	rVB2	25079	48646	1.81%	0.178%
40	23.759	3512	3518	3526	rVB	36360	76661	2.85%	0.281%
41	24.300	3608	3610	3613	rBV3	3330	2874	0.11%	0.011%
42	24.470	3627	3639	3655	rBV2	947160	2690655	100.00%	9.845%
43	24.682	3664	3675	3695	rVB	638985	1875197	69.69%	6.861%
44	25.769	3852	3860	3872	rBV3	48378	147298	5.47%	0.539%
45	27.079	4075	4083	4098	rVB4	51356	185313	6.89%	0.678%
46	28.659	4343	4352	4370	rVB6	35153	153205	5.69%	0.561%
47	29.494	4492	4494	4497	rBV4	2858	3117	0.12%	0.011%




Sum of corrected areas: 27329578

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071323\
Data File : BG058225.D
Acq On : 14 Jul 2023 10:50
Operator : CG/JU
Sample : PB153997BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK997

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

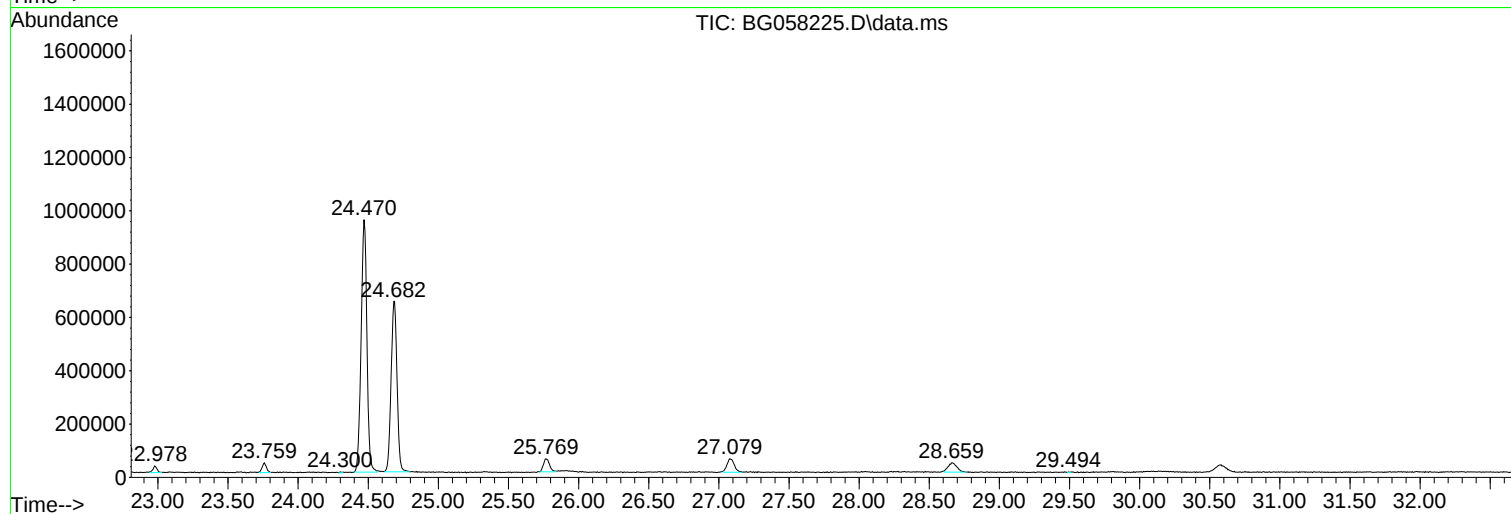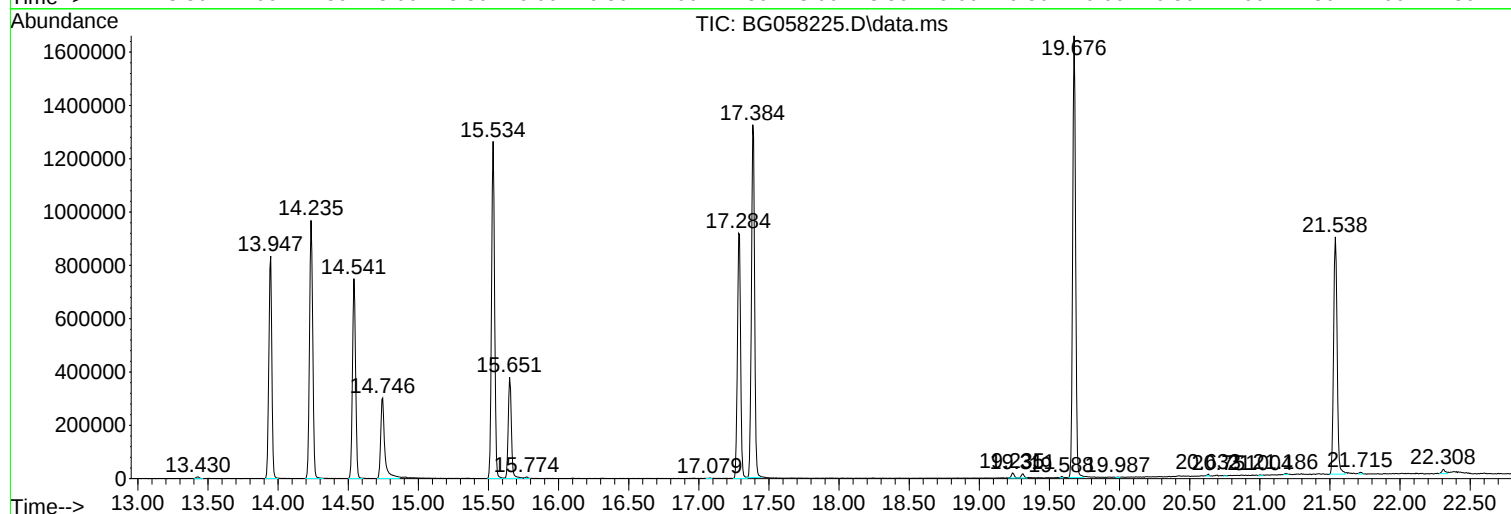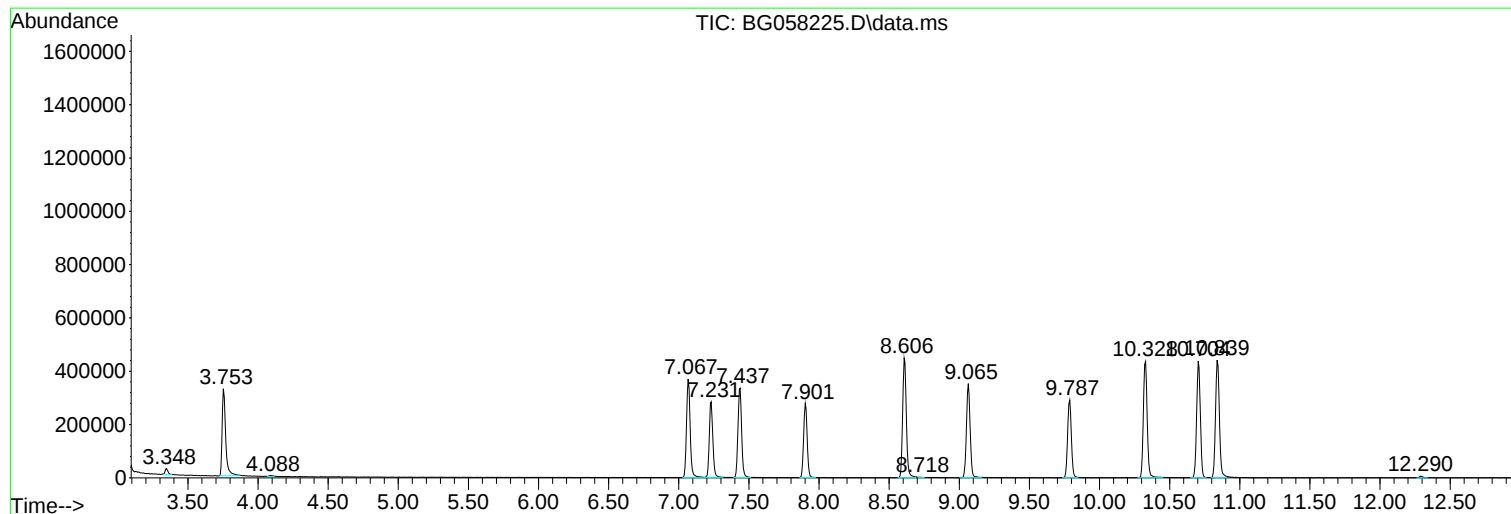

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071323\
Data File : BG058225.D
Acq On : 14 Jul 2023 10:50
Operator : CG/JU
Sample : PB153997BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK997

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071323\
Data File : BG058225.D
Acq On : 14 Jul 2023 10:50
Operator : CG/JU
Sample : PB153997BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK997

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------