

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071323\
 Data File : BG058270.D
 Acq On : 15 Jul 2023 21:36
 Operator : CG/JU
 Sample : PB153869BL
 Misc :
 ALS Vial : 82 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK869

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG058270.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.346	40	44	52	rVB	15886	26572	1.49%	0.154%
2	3.752	108	113	130	rBV	212540	370154	20.76%	2.145%
3	4.093	167	171	173	rVV4	2209	2896	0.16%	0.017%
4	7.066	670	677	692	rBV	232617	400826	22.48%	2.322%
5	7.230	697	705	723	rBV	167268	295336	16.56%	1.711%
6	7.430	732	739	748	rBV	217502	382439	21.44%	2.216%
7	7.900	811	819	826	rBV	167983	284118	15.93%	1.646%
8	8.605	932	939	955	rBV2	283796	517700	29.03%	3.000%
9	9.063	1009	1017	1029	rBV	221674	396608	22.24%	2.298%
10	9.780	1131	1139	1150	rBV	176647	327726	18.38%	1.899%
11	10.321	1224	1231	1249	rBV	277322	528448	29.63%	3.062%
12	10.703	1287	1296	1306	rBV	271137	489280	27.44%	2.835%
13	10.838	1312	1319	1333	rBV	296034	553123	31.02%	3.205%
14	12.289	1561	1566	1573	rVB	3338	5762	0.32%	0.033%
15	13.423	1755	1759	1765	rVB2	4696	7060	0.40%	0.041%
16	13.940	1840	1847	1856	rBV	559705	814006	45.64%	4.716%
17	14.234	1889	1897	1909	rBV	624804	1005720	56.39%	5.827%
18	14.539	1941	1949	1962	rBV	465450	729926	40.93%	4.229%
19	14.739	1977	1983	2007	rBV	148072	345826	19.39%	2.004%
20	15.532	2108	2118	2127	rBV	819242	1272897	71.38%	7.375%
21	15.650	2132	2138	2153	rVV	168884	275787	15.46%	1.598%
22	15.767	2153	2158	2162	rVB3	3842	5792	0.32%	0.034%
23	17.072	2376	2380	2385	rVB2	1529	2312	0.13%	0.013%
24	17.283	2409	2416	2425	rBV	611009	912401	51.16%	5.286%
25	17.383	2425	2433	2450	rVB	902130	1394915	78.22%	8.082%
26	19.234	2744	2748	2754	rBV3	12389	16938	0.95%	0.098%
27	19.310	2756	2761	2764	rBV2	8429	12830	0.72%	0.074%
28	19.580	2805	2807	2812	rVV2	4351	5252	0.29%	0.030%
29	19.668	2816	2822	2836	rBV	1091669	1646534	92.33%	9.540%
30	20.139	2896	2902	2904	rBV5	1667	2691	0.15%	0.016%
31	20.374	2938	2942	2943	rBV2	1716	1818	0.10%	0.011%
32	20.620	2982	2984	2988	rVV4	4636	4485	0.25%	0.026%
33	20.938	3035	3038	3039	rBV2	1829	2174	0.12%	0.013%
34	21.155	3072	3075	3077	rBV3	2648	3832	0.21%	0.022%
35	21.531	3133	3139	3154	rBV2	576693	970987	54.45%	5.626%
36	22.301	3268	3270	3275	rVB5	8662	11720	0.66%	0.068%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071323\
 Data File : BG058270.D
 Acq On : 15 Jul 2023 21:36
 Operator : CG/JU
 Sample : PB153869BL
 Misc :
 ALS Vial : 82 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK869

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Title : SVOA CALIBRATION

37	22.788	3351	3353	3356	rBV4	2504	2505	0.14%	0.015%
38	22.970	3381	3384	3392	rVB4	13527	23132	1.30%	0.134%
39	23.746	3511	3516	3526	rVB4	20562	46558	2.61%	0.270%
40	24.457	3626	3637	3657	rBV2	612941	1783383	100.00%	10.333%
41	24.674	3663	3674	3694	rVB	391489	1121651	62.89%	6.499%
42	25.003	3728	3730	3732	rBV3	2401	2117	0.12%	0.012%
43	25.750	3851	3857	3868	rBV4	27011	81312	4.56%	0.471%
44	27.072	4073	4082	4092	rVB5	26320	87998	4.93%	0.510%
45	27.965	4232	4234	4235	rBV2	2586	2088	0.12%	0.012%
46	28.646	4340	4350	4351	rBV8	16359	37580	2.11%	0.218%
47	28.911	4393	4395	4398	rVB3	2539	1863	0.10%	0.011%
48	29.974	4574	4576	4578	rBV3	2962	2255	0.13%	0.013%
49	30.379	4643	4645	4647	rBV3	2883	2693	0.15%	0.016%
50	30.556	4665	4675	4676	rBV6	13563	32173	1.80%	0.186%
51	31.989	4915	4919	4921	rBV4	4315	5004	0.28%	0.029%




Sum of corrected areas: 17259203

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071323\
Data File : BG058270.D
Acq On : 15 Jul 2023 21:36
Operator : CG/JU
Sample : PB153869BL
Misc :
ALS Vial : 82 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK869

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

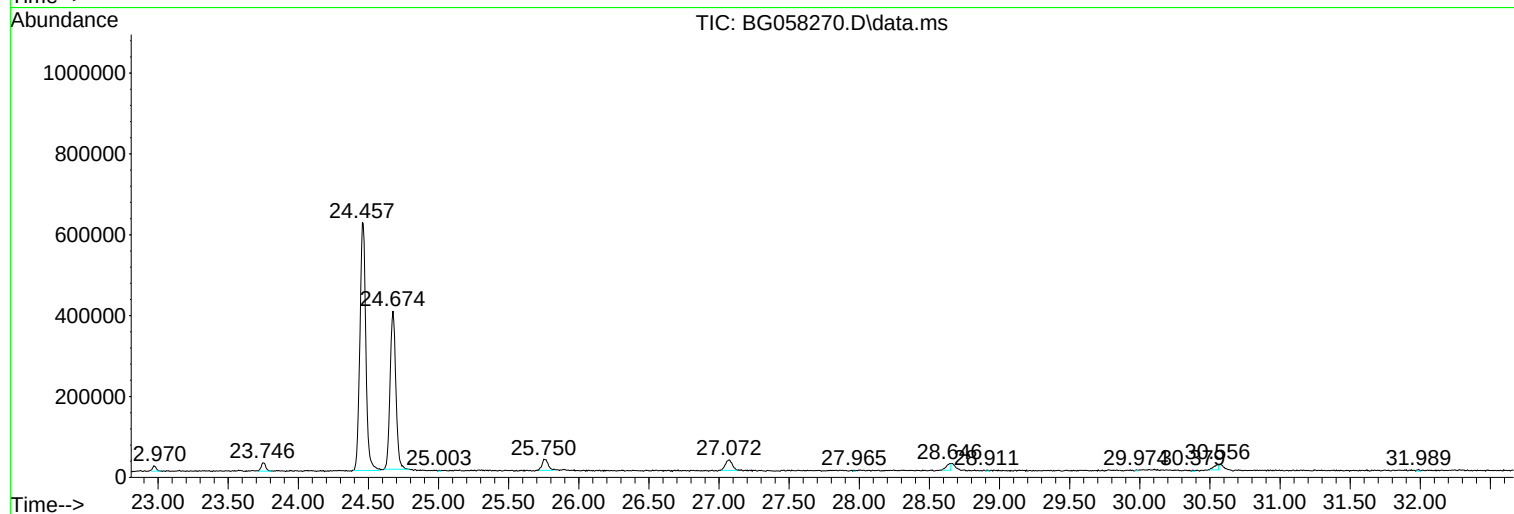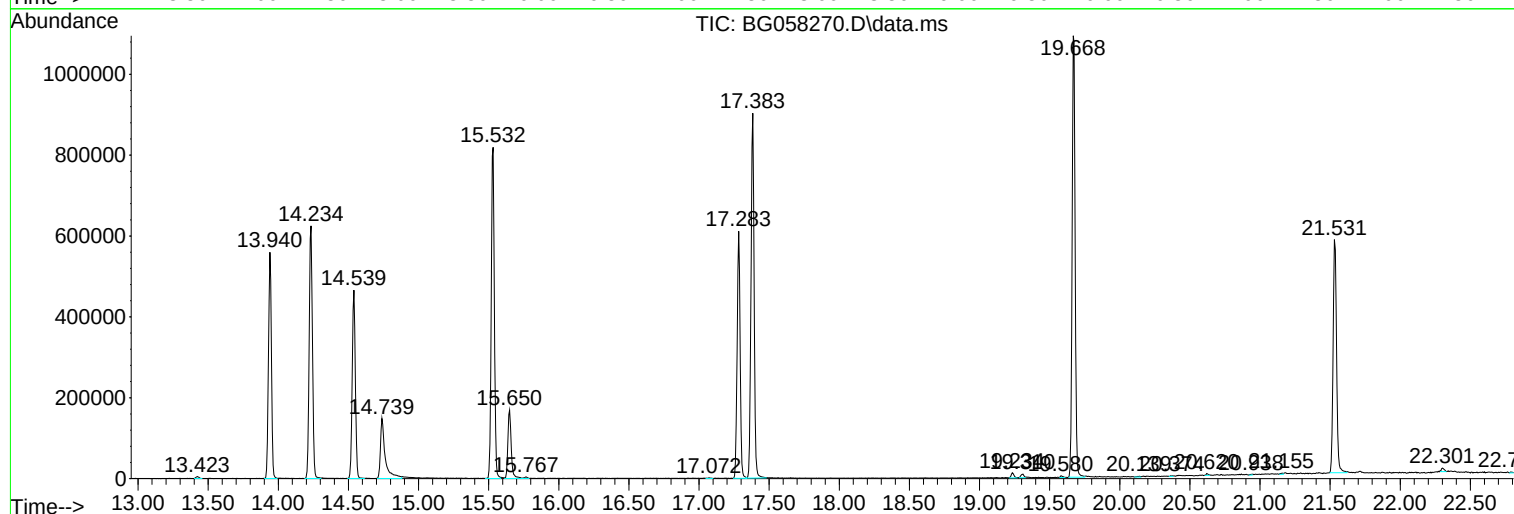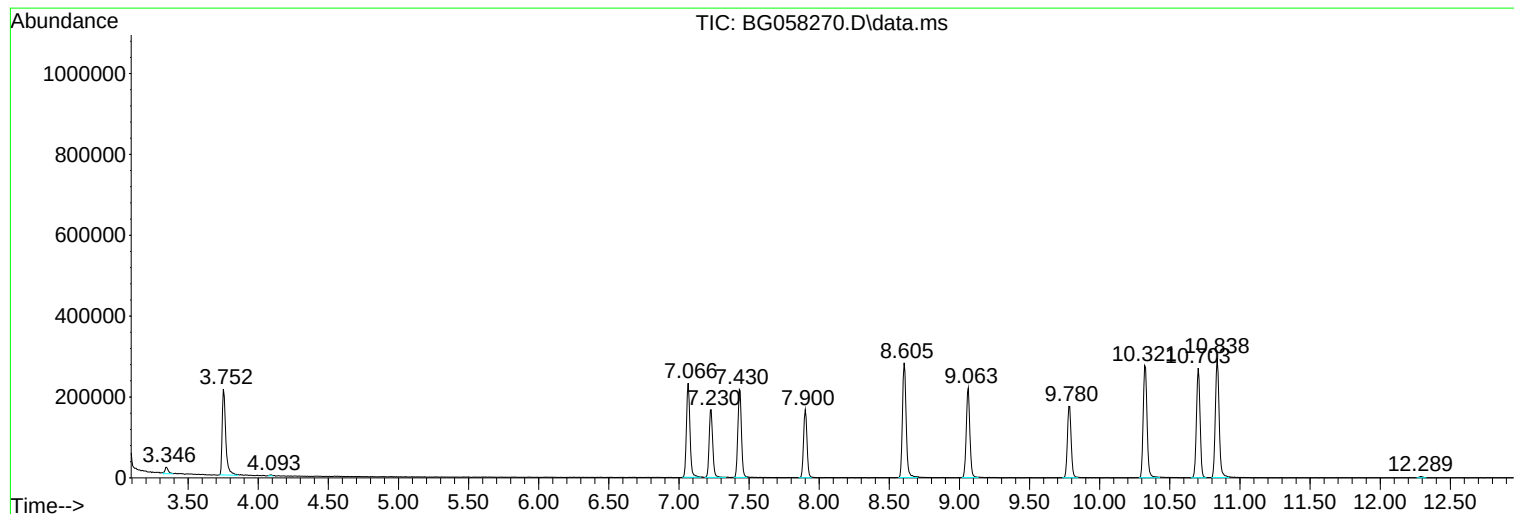

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071323\
Data File : BG058270.D
Acq On : 15 Jul 2023 21:36
Operator : CG/JU
Sample : PB153869BL
Misc :
ALS Vial : 82 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK869

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071323\
Data File : BG058270.D
Acq On : 15 Jul 2023 21:36
Operator : CG/JU
Sample : PB153869BL
Misc :
ALS Vial : 82 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK869

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc