




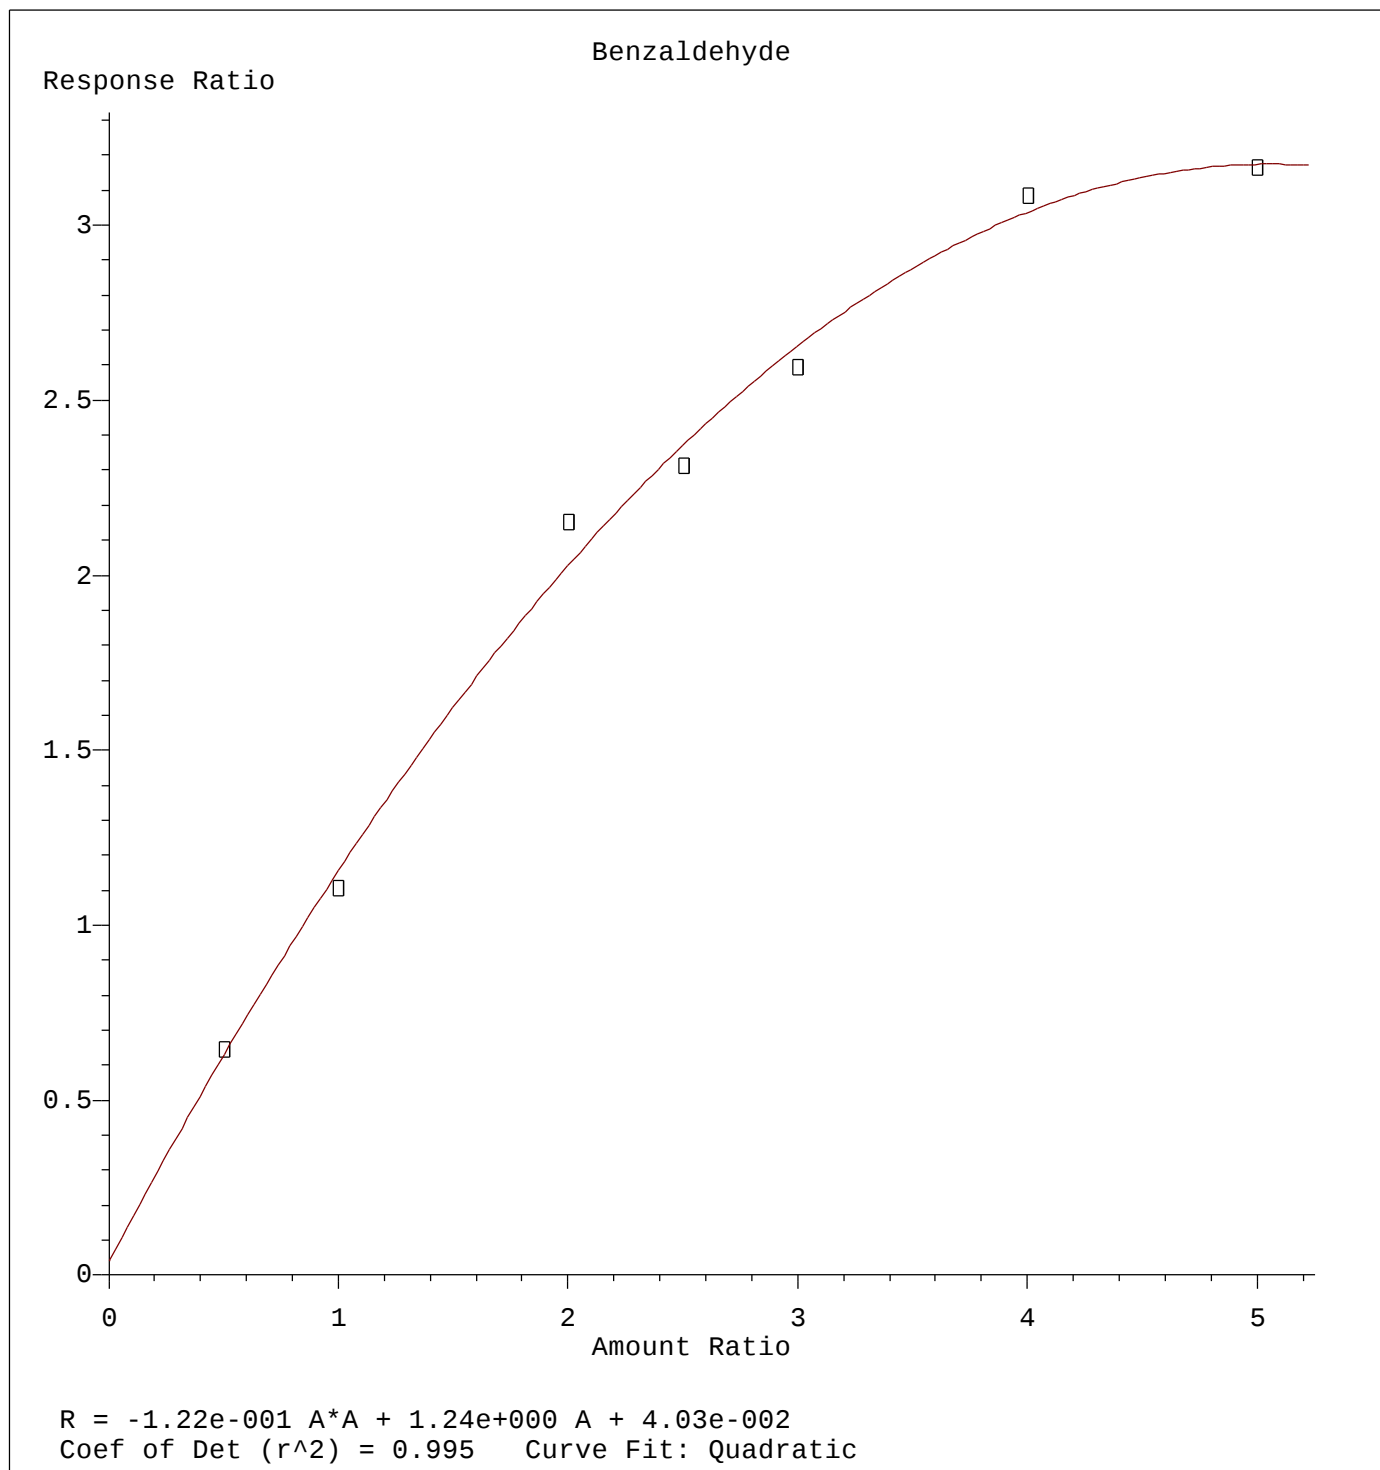

Method Name: Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071519.M
Calibration Table Last Updated: Mon Jul 15 16:16:21 2019

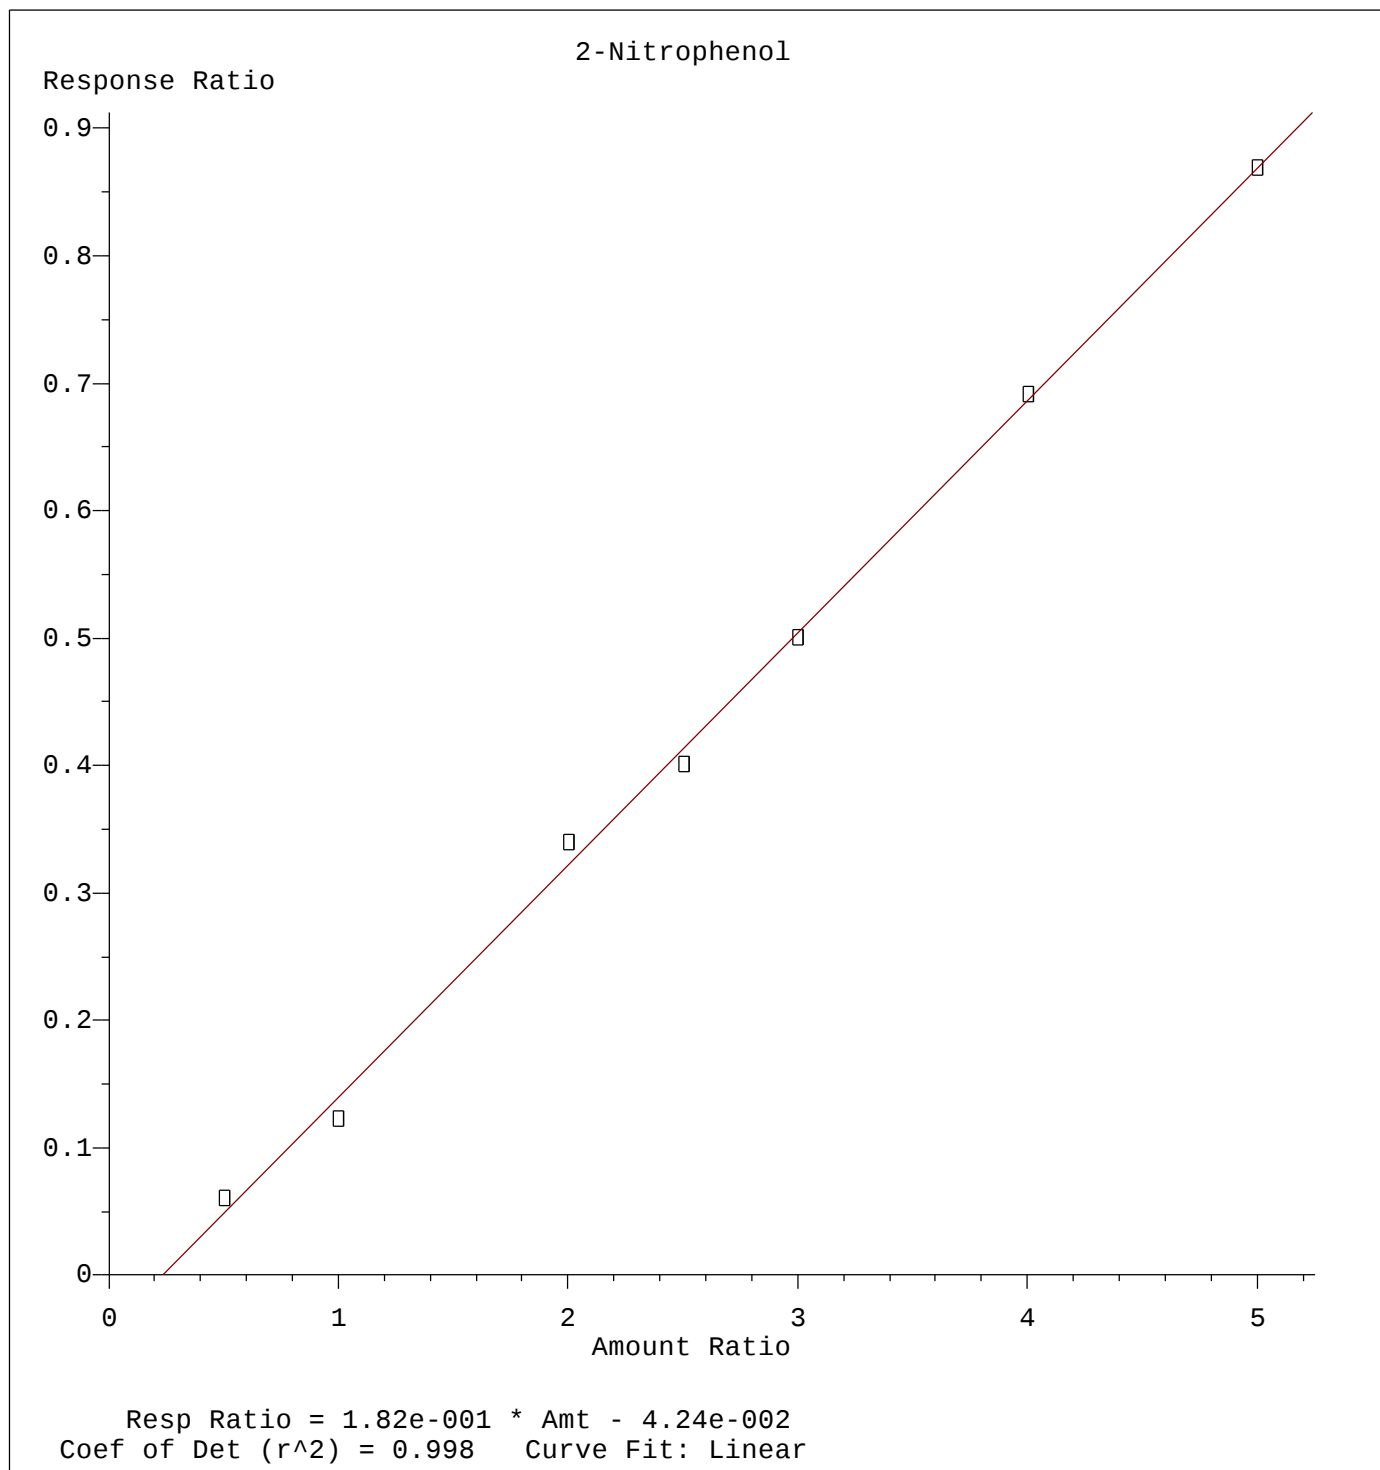


Method Name: Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071519.M
Calibration Table Last Updated: Mon Jul 15 16:16:21 2019

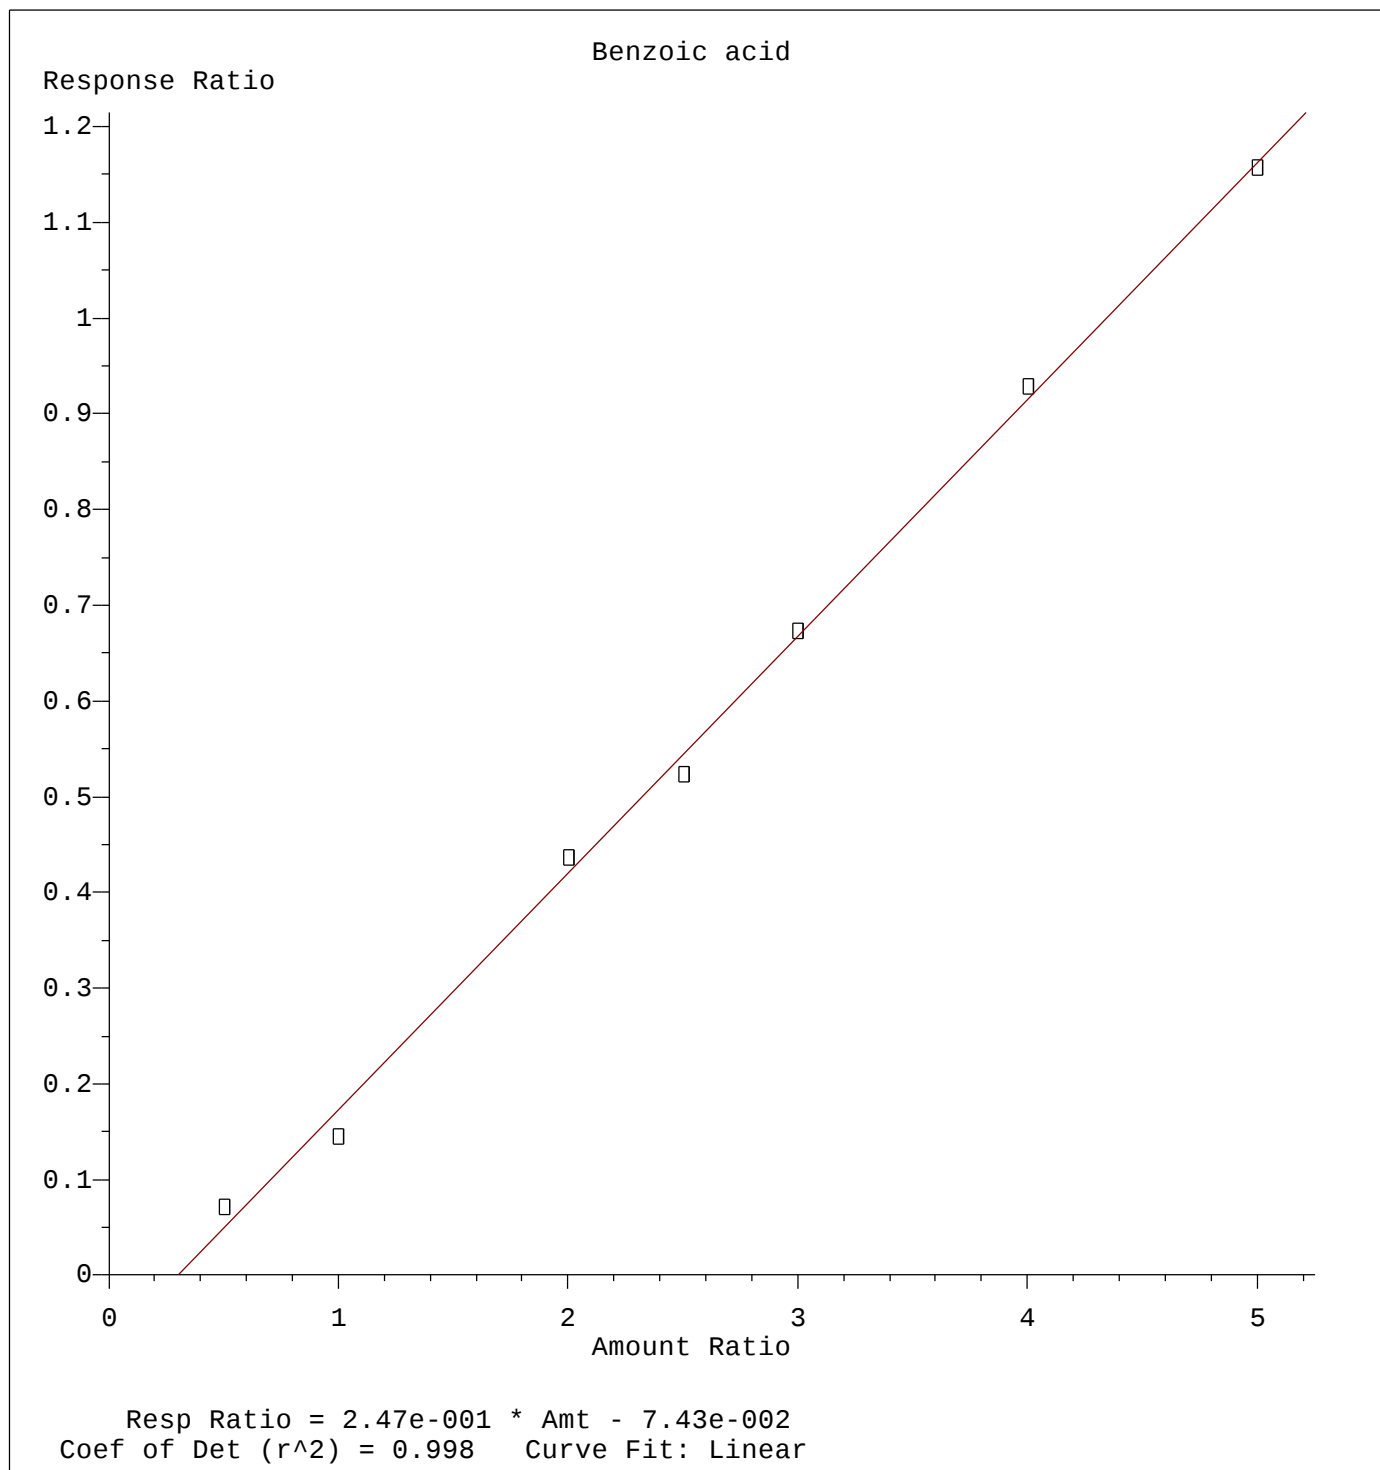

Method Name: Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071519.M
Calibration Table Last Updated: Mon Jul 15 16:16:21 2019

2,4-Dinitrophenol


Response Ratio

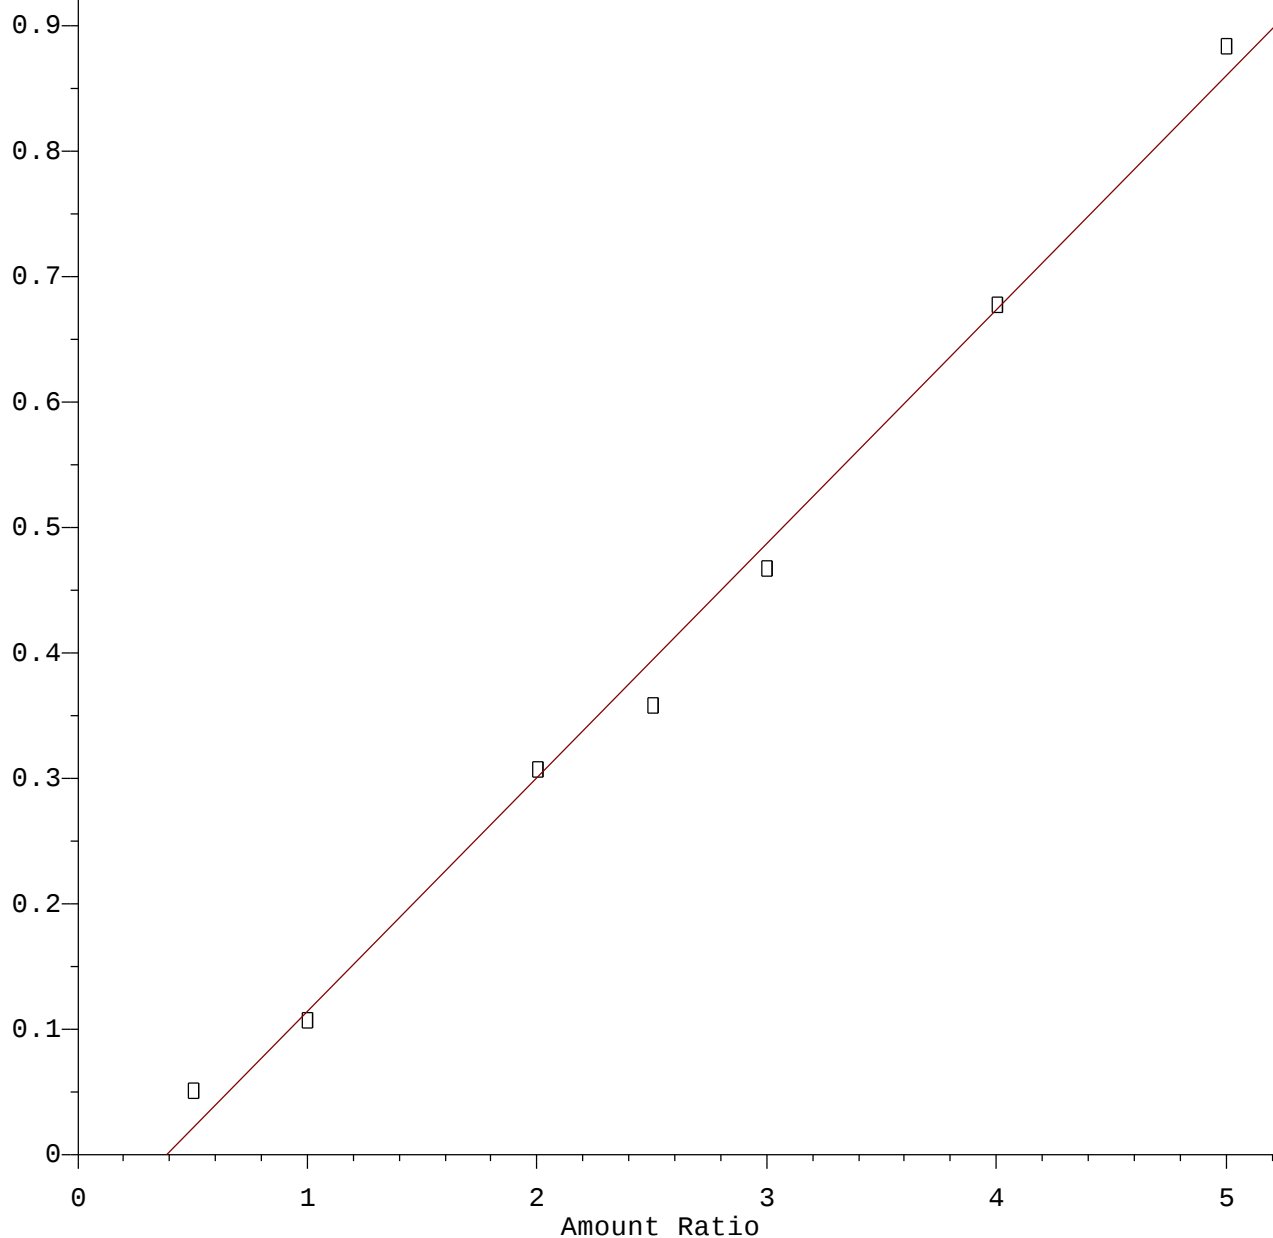

Resp Ratio = $1.86 \times 10^{-1} \times \text{Amt} - 7.20 \times 10^{-2}$
Coef of Det (r^2) = 0.994 Curve Fit: Linear


Method Name: Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071519.M
Calibration Table Last Updated: Mon Jul 15 16:16:21 2019

4,6-Dinitro-2-methylphenol

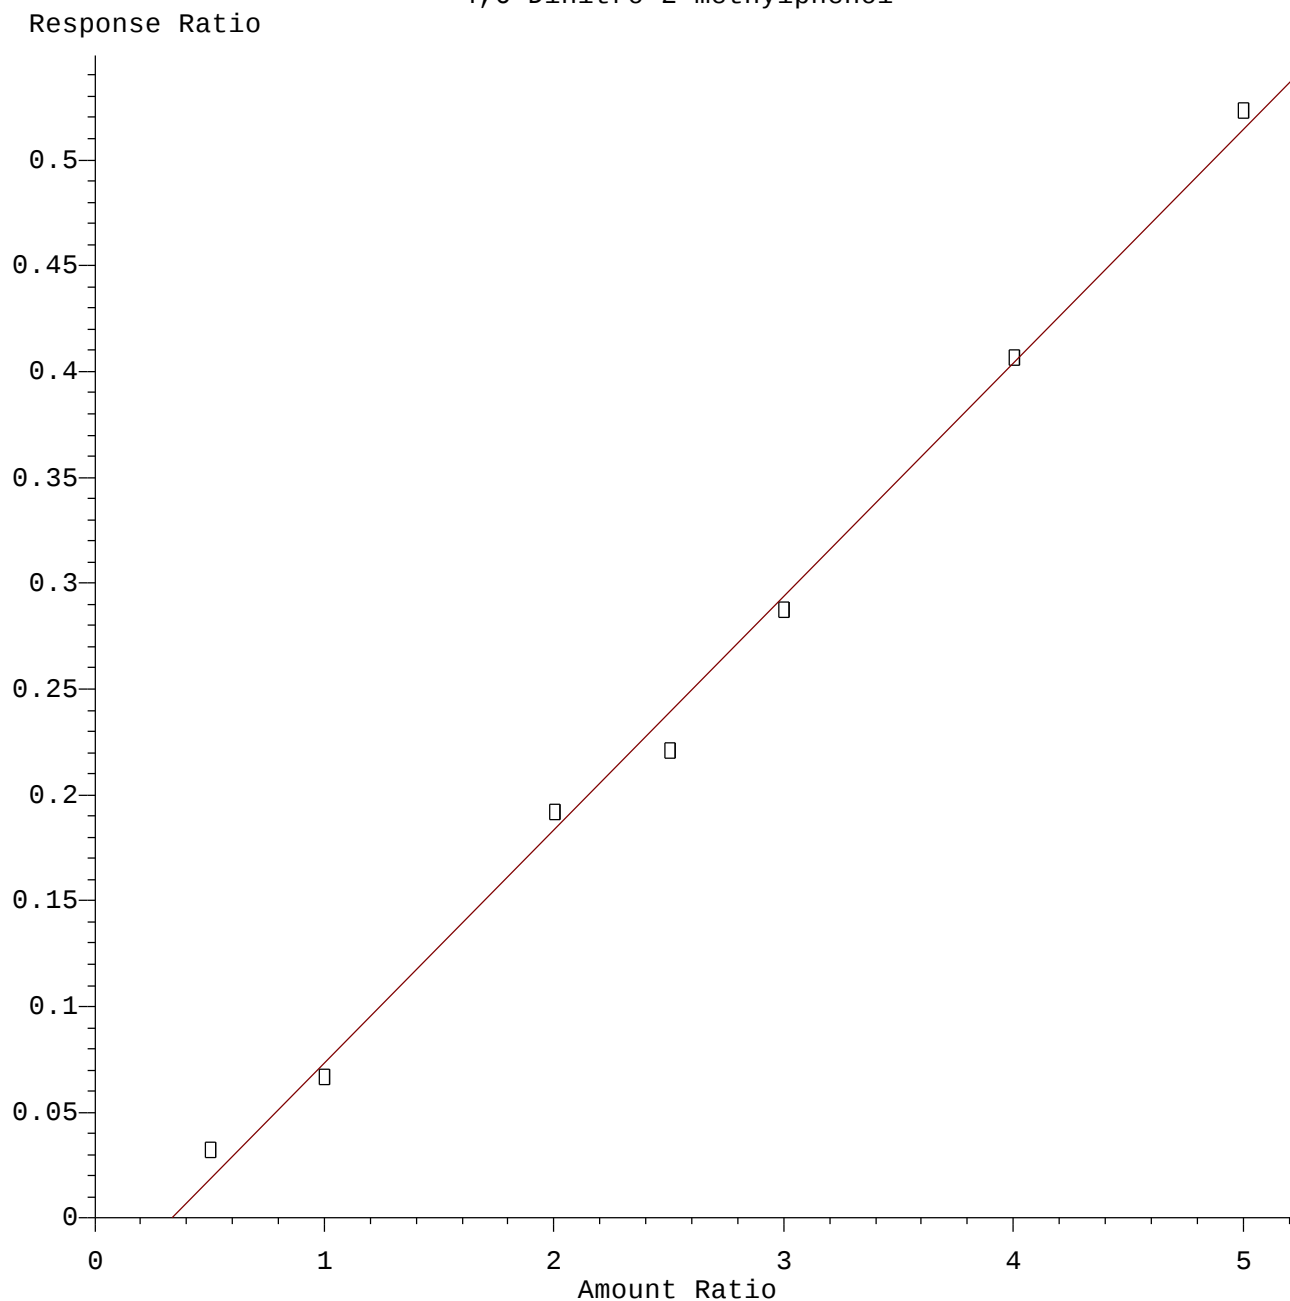

Resp Ratio = $1.10 \times 10^{-1} \times \text{Amt} - 3.68 \times 10^{-2}$
Coef of Det (r^2) = 0.996 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071519.M
Calibration Table Last Updated: Mon Jul 15 16:16:21 2019

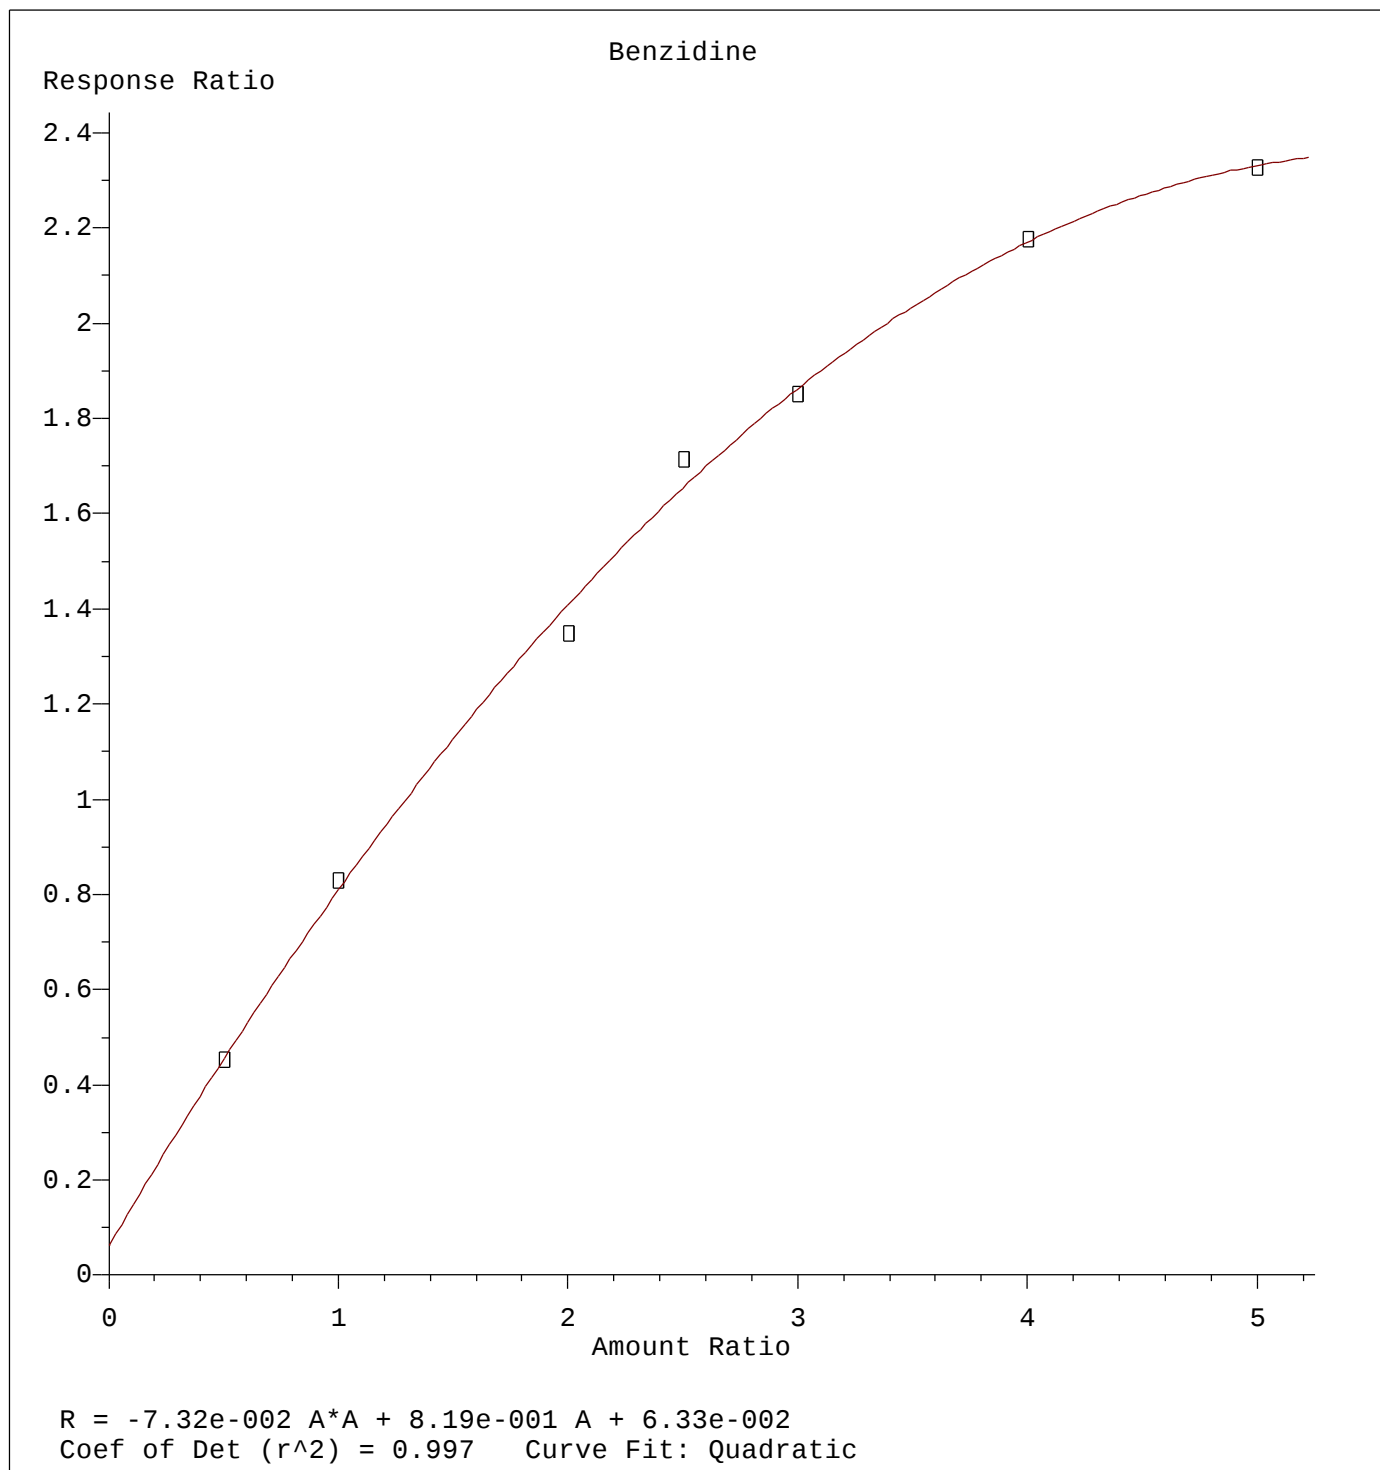

Method Name: Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071519.M
Calibration Table Last Updated: Mon Jul 15 16:16:21 2019