
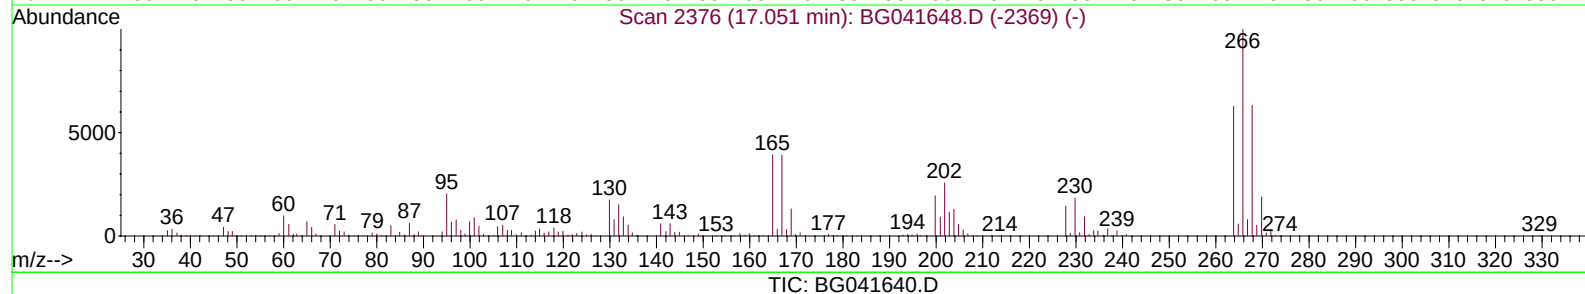
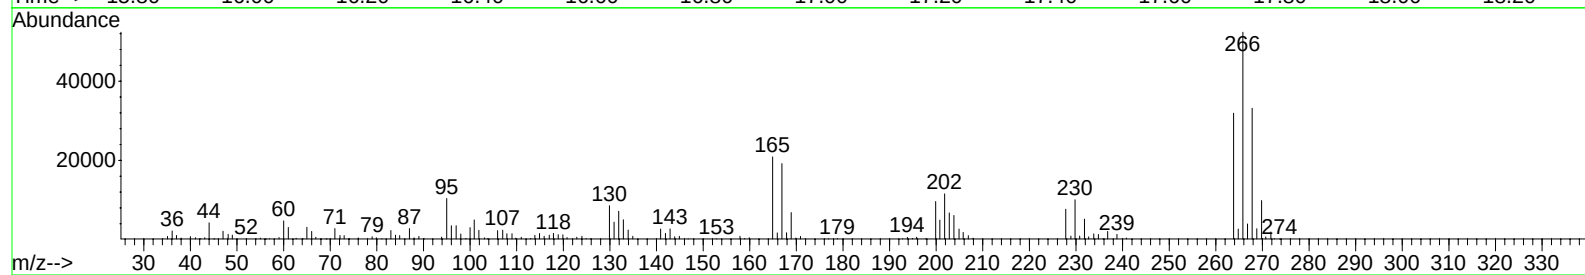


```
Data Path   : Z:\svoasrv\HPCHEM1\BNA G\Data\BG071519\  
Data File   : BG041640.D  
Acq On      : 15 Jul 2019    7:53  
Operator    : HP/JU  
Sample      : DFTPP  
Misc        :  
ALS Vial    : 1      Sample Multiplier: 1
```

Quant Time: Jul 15 16:44:09 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 15 16:16:21 2019
Response via : Initial Calibration

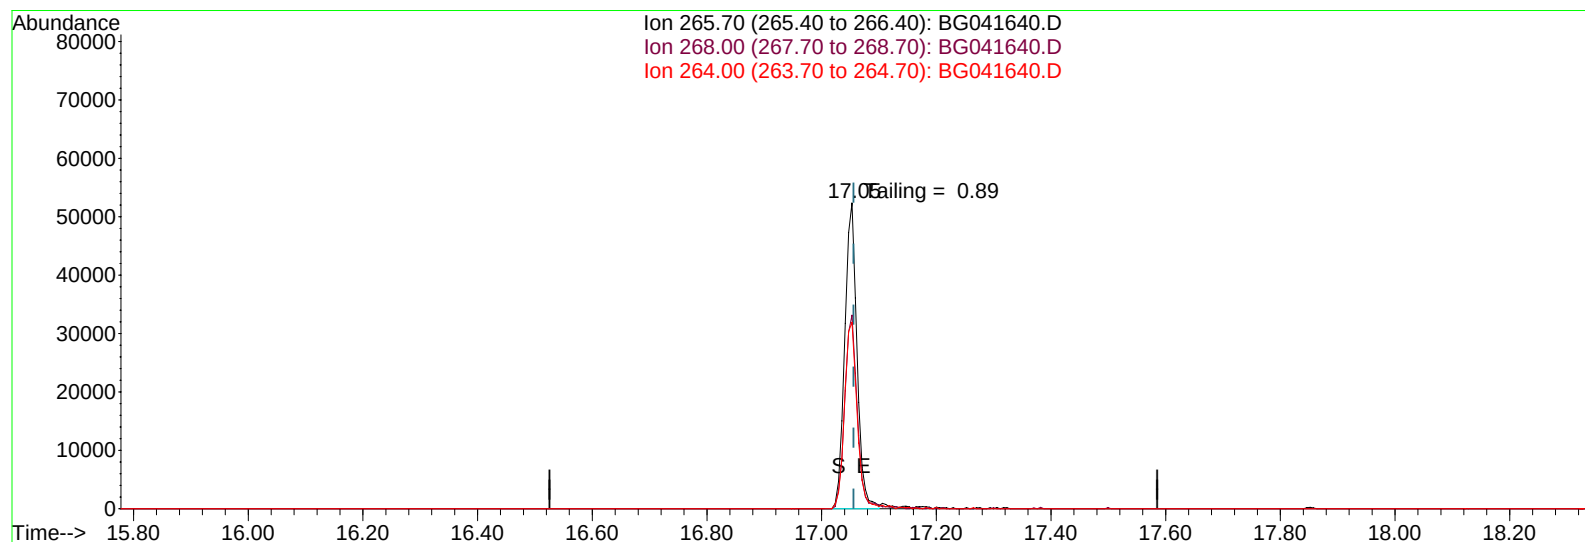

(70) Pentachlorophenol (C)




17.053min (-0.003) 189001.49ng

response 77878

Ion	Exp%	Act%
265.70	100	100
268.00	66.10	63.32
264.00	64.30	60.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG071519\
Data File : BG041640.D
Acq On : 15 Jul 2019 7:53
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 15 16:44:09 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 15 16:16:21 2019
Response via : Initial Calibration

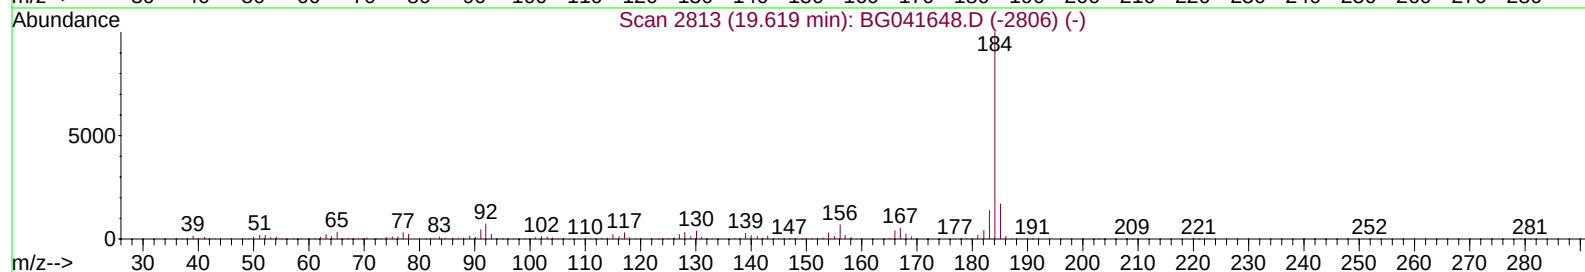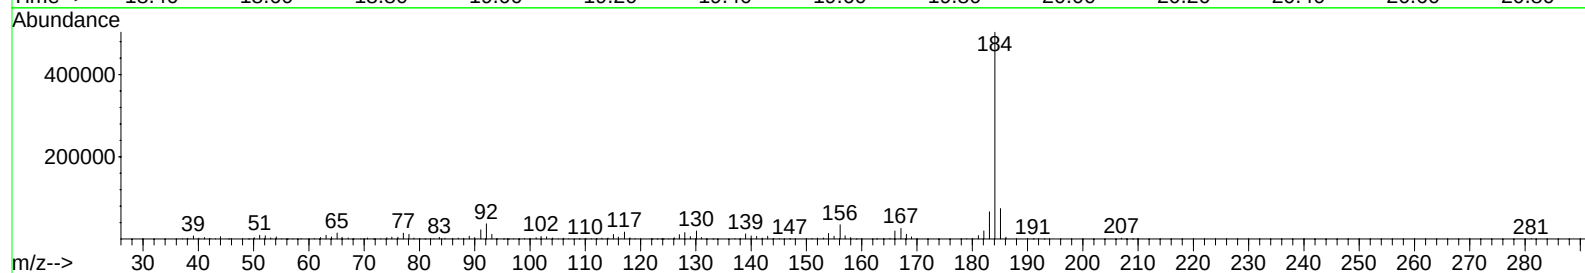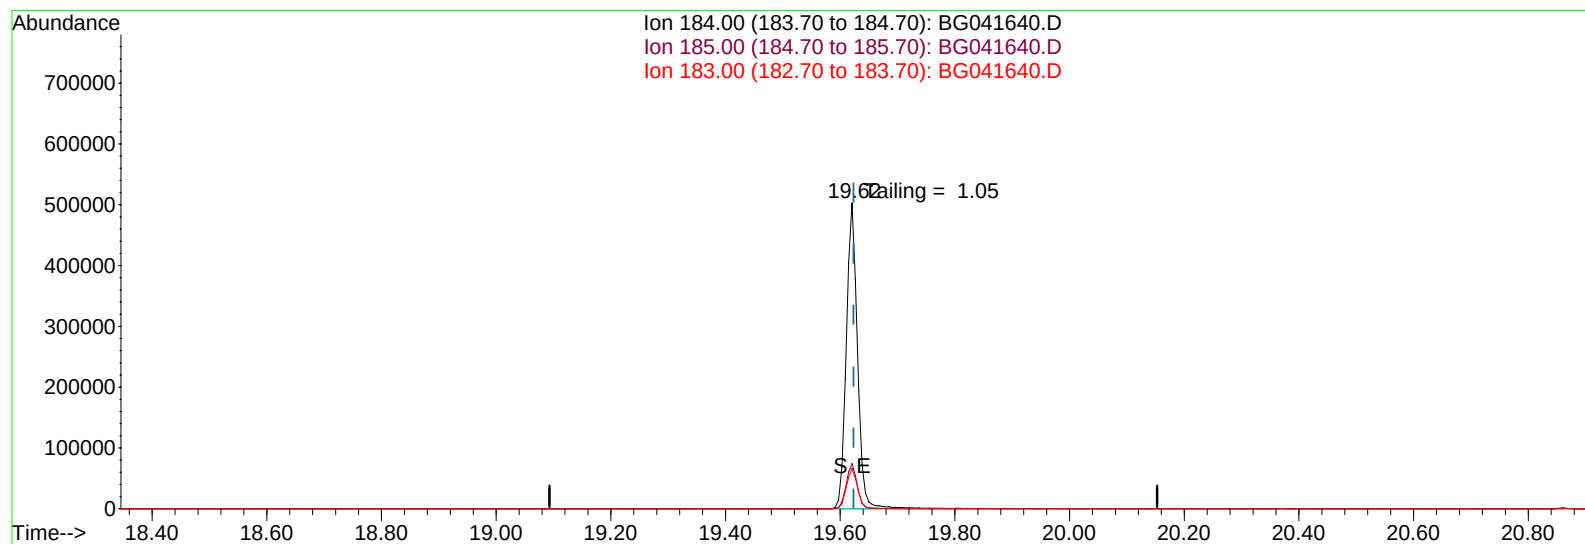

TIC: BG041640.D

(77) Benzidine

19.621min (-0.003) 0.00ng

response 680976

Ion	Exp%	Act%
184.00	100	100
185.00	16.20	14.74
183.00	14.70	13.19
0.00	0.00	0.00