


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG071519\
 Data File : BG041640.D
 Acq On : 15 Jul 2019 7:53
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 15 16:16:21 2019

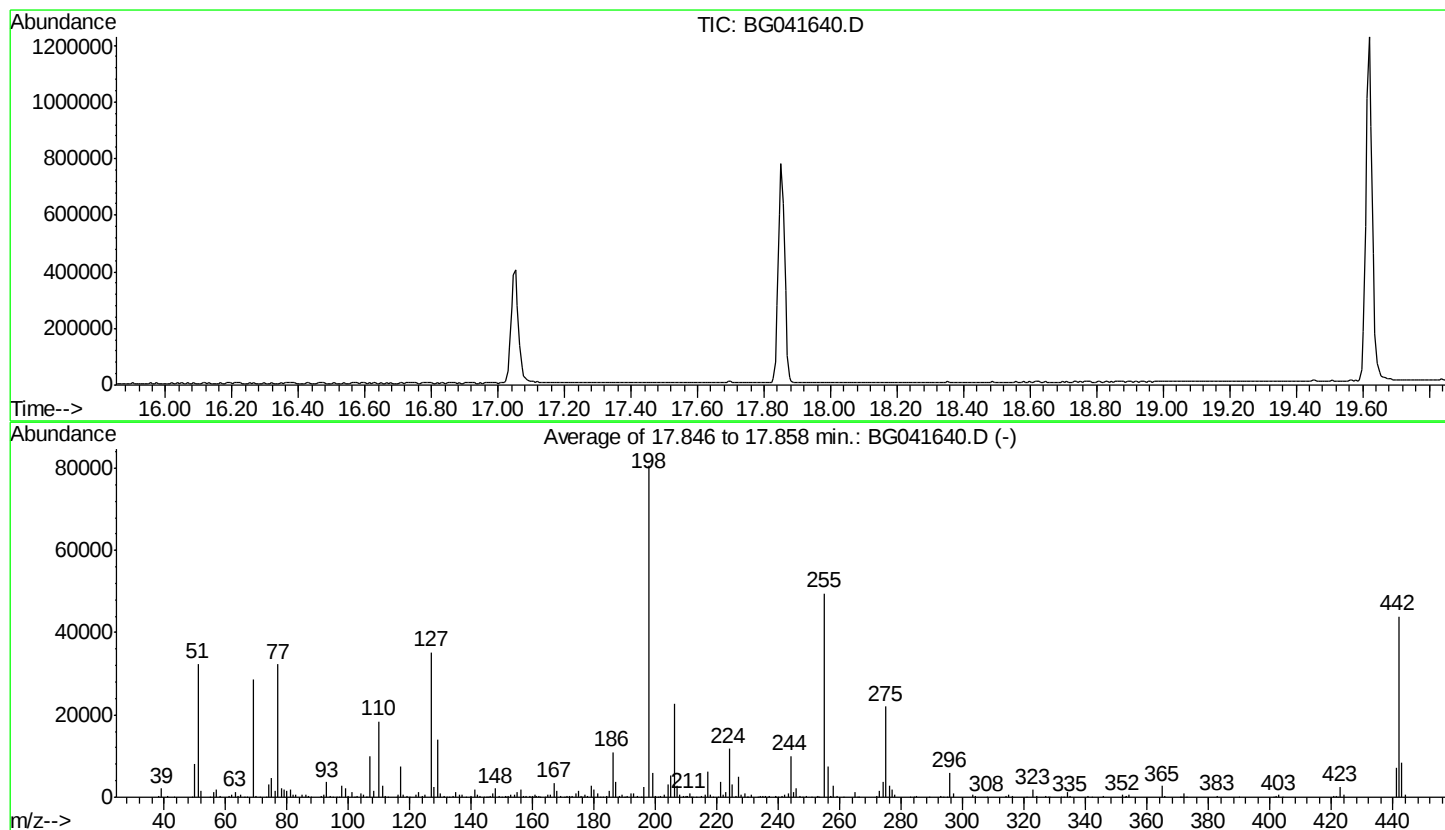

AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2505

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.3	32464	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.4	28554	PASS
70	69	0.00	2	0.7	196	PASS
127	198	10	80	43.7	35234	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	80610	PASS
199	198	5	9	7.2	5781	PASS
275	198	10	60	27.2	21962	PASS
365	198	1	100	3.5	2795	PASS
441	198	0.01	100	8.9	7208	PASS
442	198	50	100	54.6	43994	PASS
443	442	15	24	19.1	8397	PASS